

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121222\
 Data File : PL079687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2022 17:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 20:42:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.565	47519540	59583151	21.035	21.889
28)	SA Decachlor...	8.765	7.630	41983223	51164536	21.617	21.779
Target Compounds							
2)	A alpha-BHC	0.000	3.039	0	430511	N.D.	0.100 #
3)	MA gamma-BHC...	4.139f	0.000	14718	0	0.005	N.D. #
4)	MA Heptachlor	4.683	3.675f	172727	319412	0.052	0.083 #
5)	MB Aldrin	0.000	3.988f	0	749043	N.D.	0.202 #
6)	B beta-BHC	0.000	3.675	0	319412	N.D.	0.211 #
8)	B Heptachlo...	5.464	4.478	864748	398870	0.303	0.118 #
14)	MA Endrin	0.000	5.388f	0	280043	N.D.	0.093 #
15)	B Endosulfa...	0.000	5.632f	0	297779	N.D.	0.106 #
22)	Mirex	7.889	0.000	75900	0	0.040	N.D. #
23)	Chlordane-1	0.000	3.532	0	228481	N.D.	2.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121222\
Data File : PL079687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2022 17:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 20:42:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

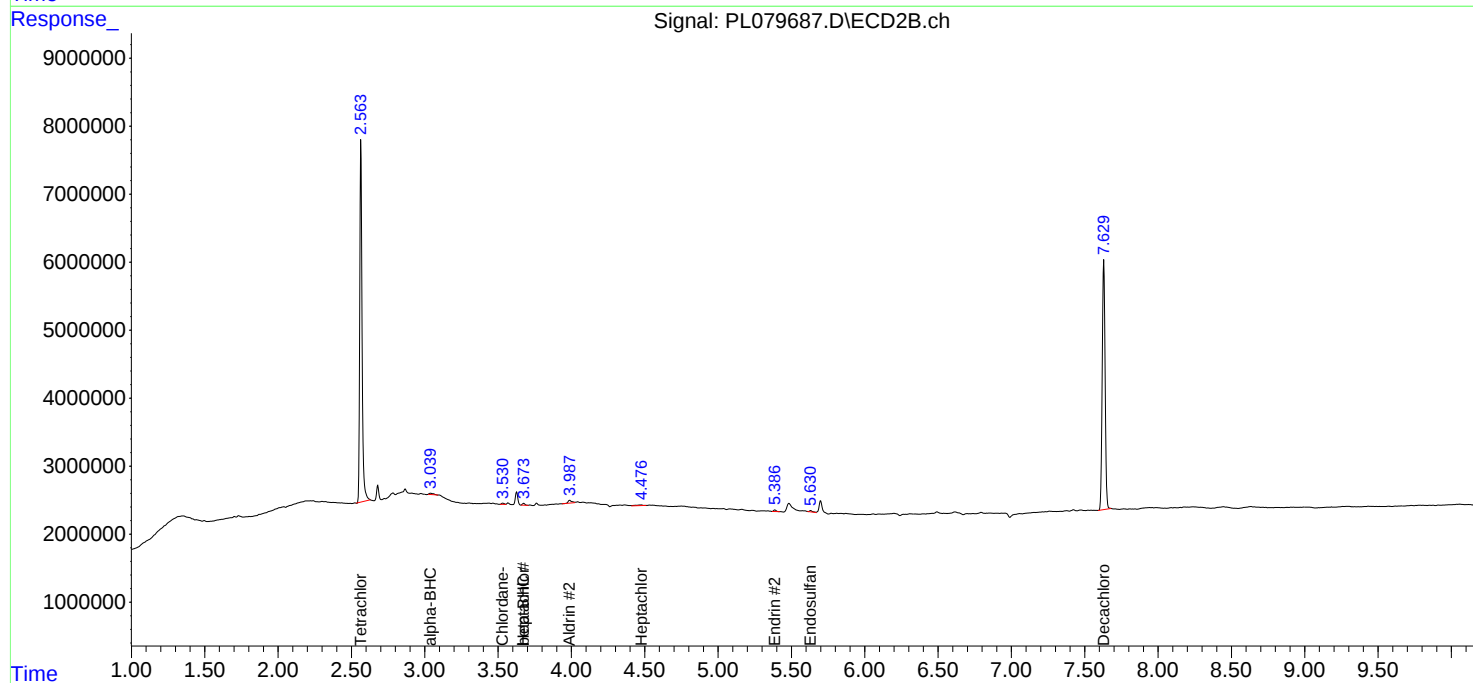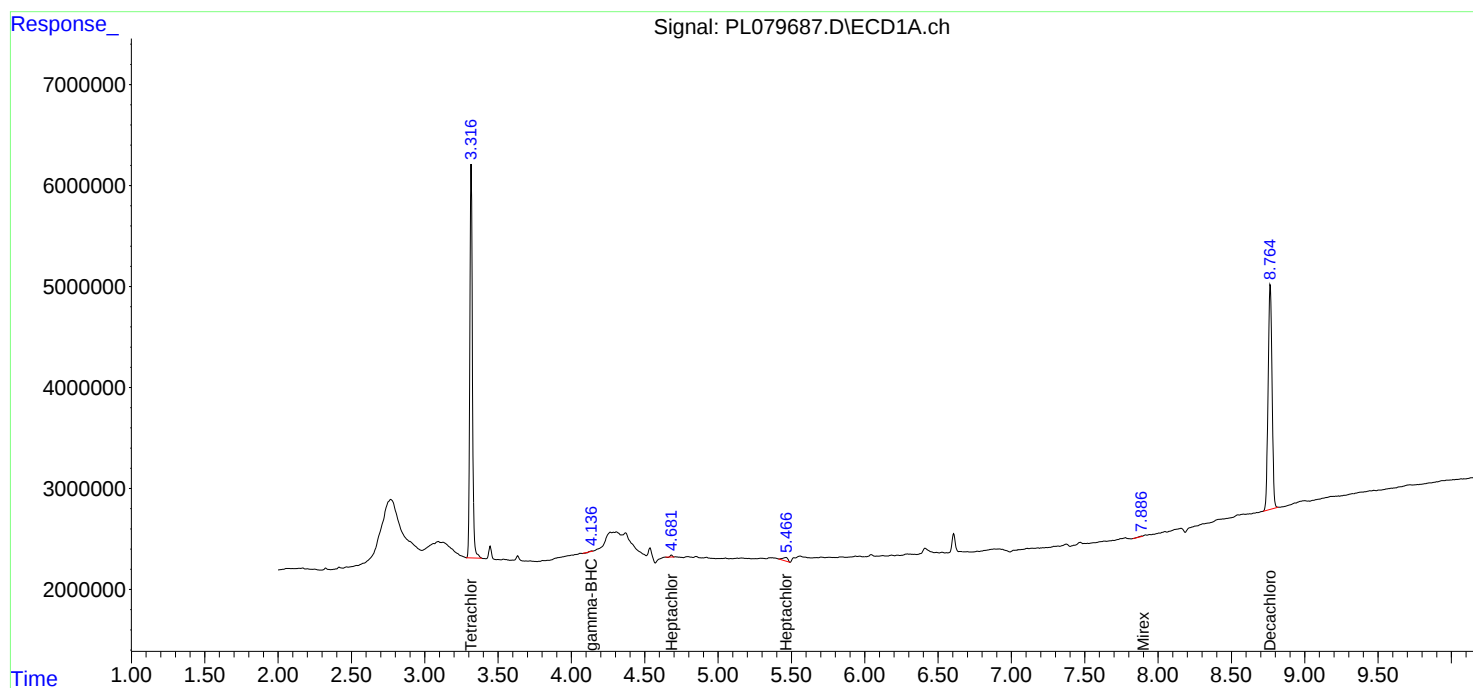


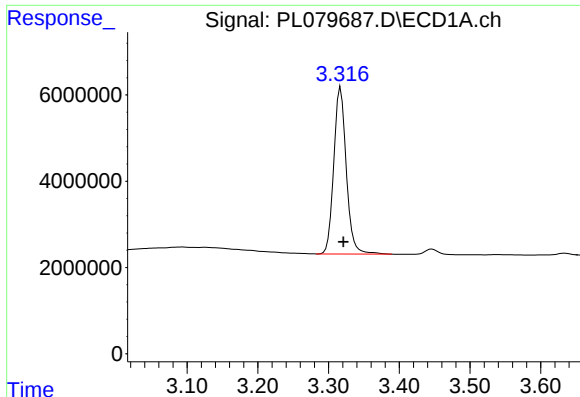

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.004 min
Response: 47519540
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

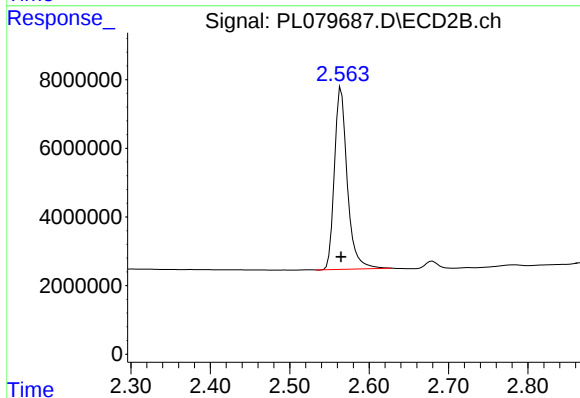


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 59583151
Conc: 21.89 ng/ml

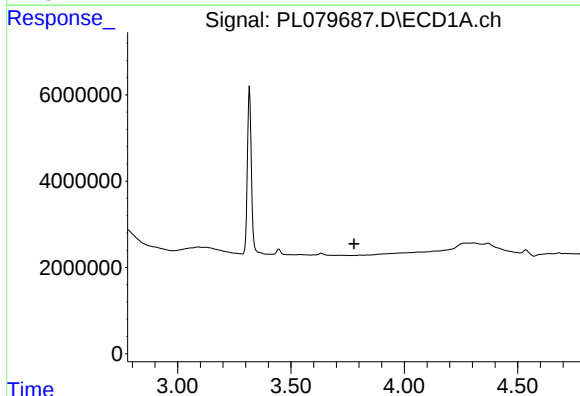


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.778 min
Response: 0
Conc: N.D.

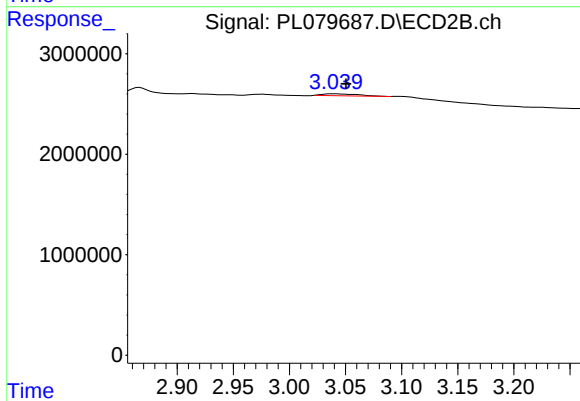

#2 alpha-BHC


R.T.: 3.039 min
Delta R.T.: -0.011 min
Response: 430511
Conc: 0.10 ng/ml

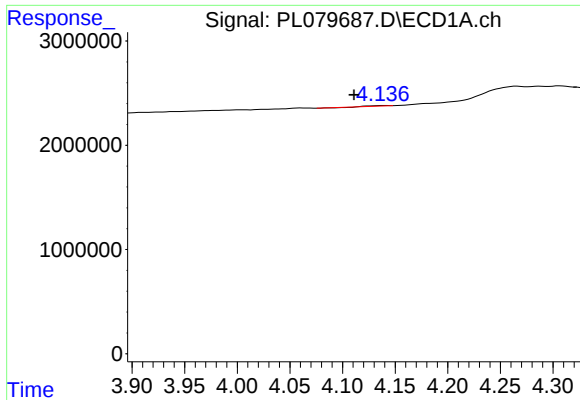

#3 gamma-BHC (Lindane)


R.T.: 4.139 min
Delta R.T.: 0.028 min
Response: 14718
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

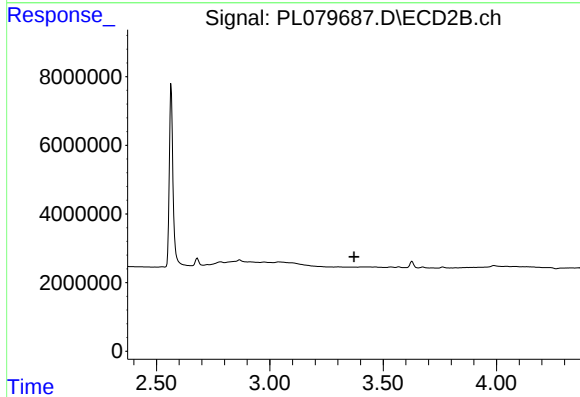


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.371 min
Response: 0
Conc: N.D.

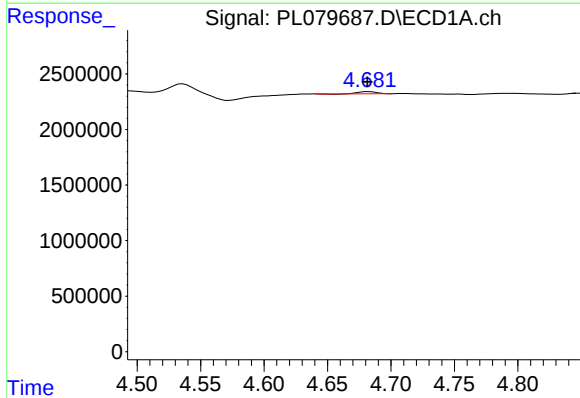


#4 Heptachlor

R.T.: 4.683 min
Delta R.T.: 0.001 min
Response: 172727
Conc: 0.05 ng/ml

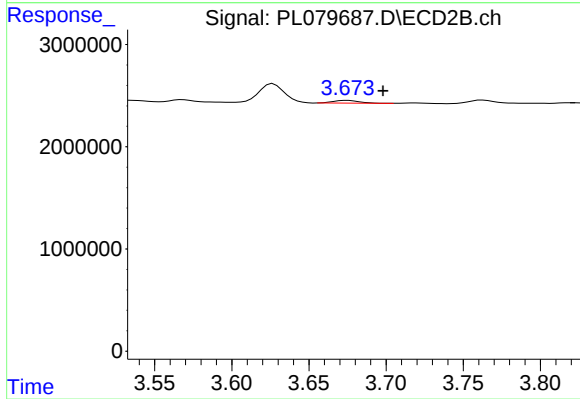

#4 Heptachlor


R.T.: 3.675 min
Delta R.T.: -0.023 min
Response: 319412
Conc: 0.08 ng/ml

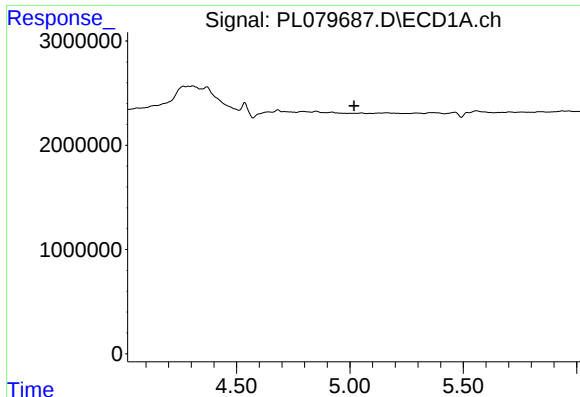

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

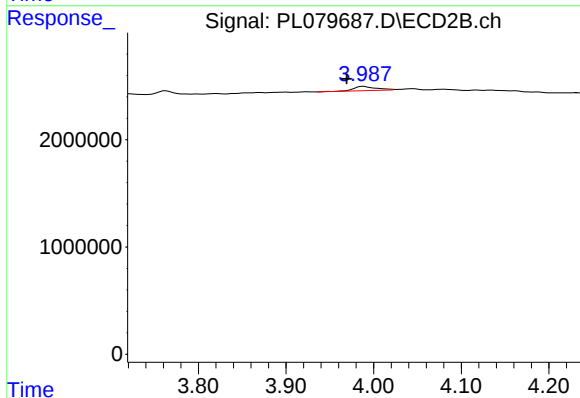


#5 Aldrin

R.T.: 3.988 min
Delta R.T.: 0.019 min
Response: 749043
Conc: 0.20 ng/ml

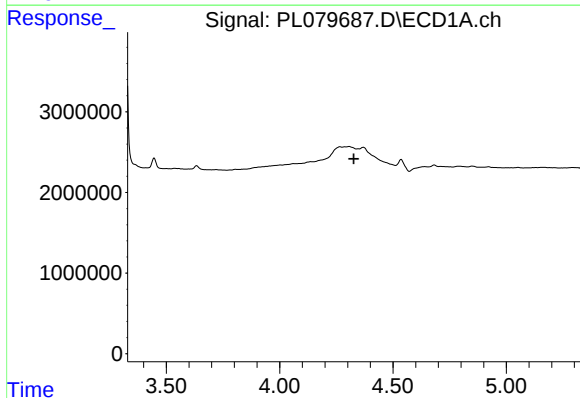


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.327 min
Response: 0
Conc: N.D.

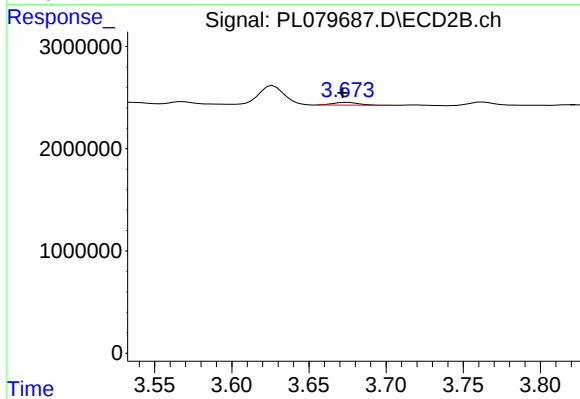

#6 beta-BHC


R.T.: 3.675 min
Delta R.T.: 0.003 min
Response: 319412
Conc: 0.21 ng/ml

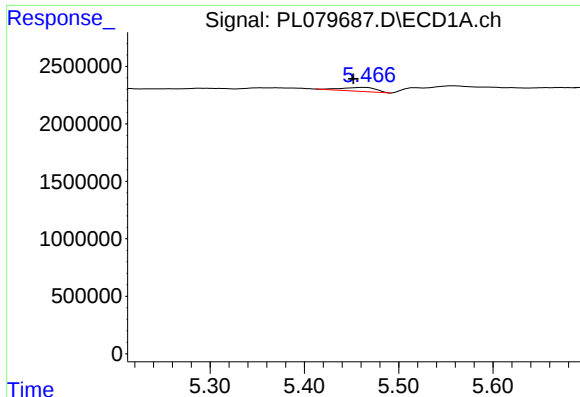

#8 Heptachlor epoxide


R.T.: 5.464 min
Delta R.T.: 0.012 min
Response: 864748
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

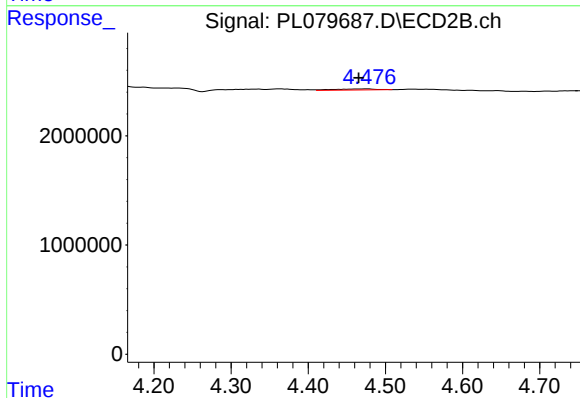


#8 Heptachlor epoxide

R.T.: 4.478 min
Delta R.T.: 0.012 min
Response: 398870
Conc: 0.12 ng/ml

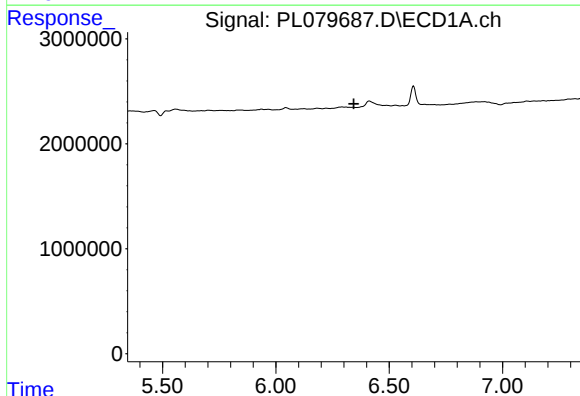


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

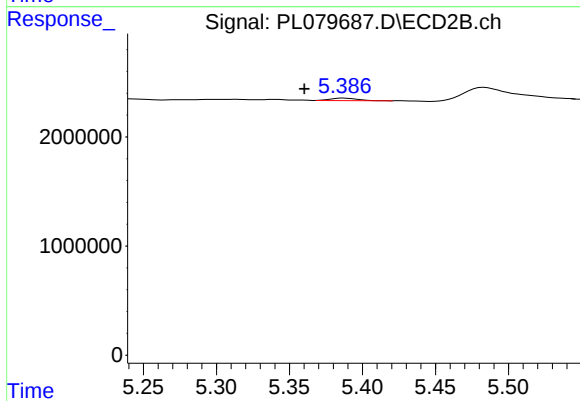

#14 Endrin


R.T.: 5.388 min
Delta R.T.: 0.027 min
Response: 280043
Conc: 0.09 ng/ml

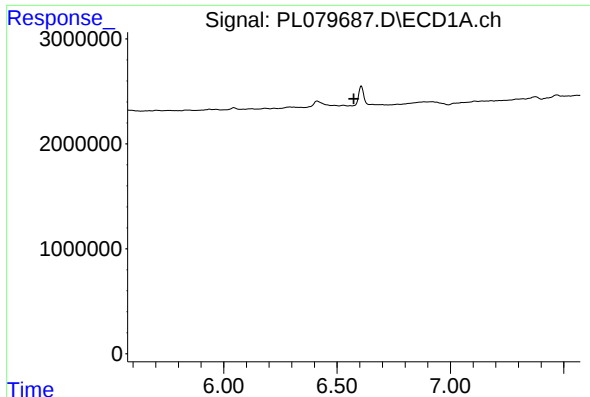

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

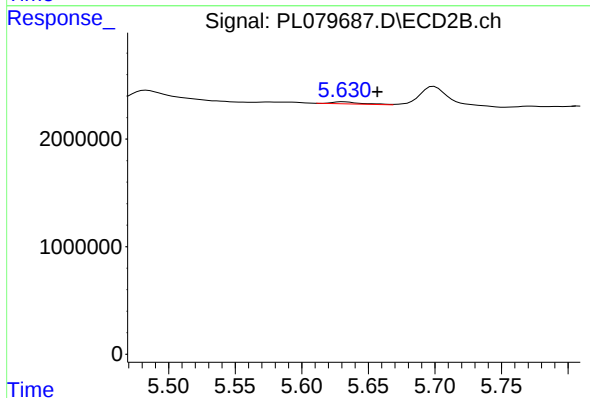


#15 Endosulfan II

R.T.: 5.632 min
Delta R.T.: -0.025 min
Response: 297779
Conc: 0.11 ng/ml

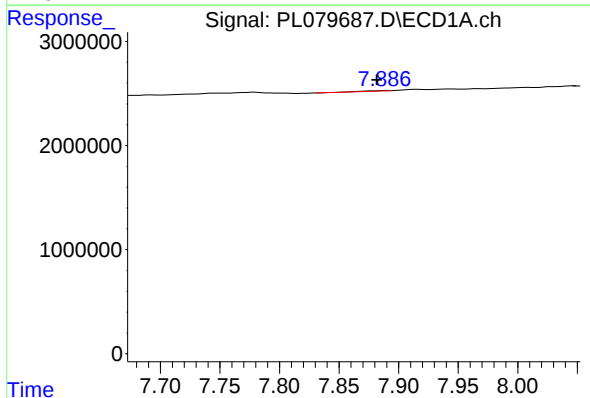


#22 Mirex

R.T.: 7.889 min
Delta R.T.: 0.008 min
Response: 75900
Conc: 0.04 ng/ml

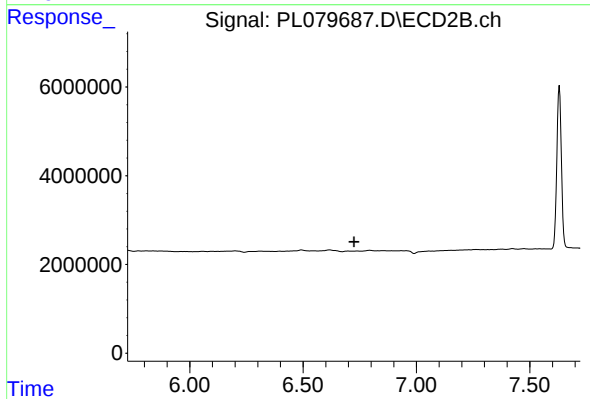

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.725 min
Response: 0
Conc: N.D.

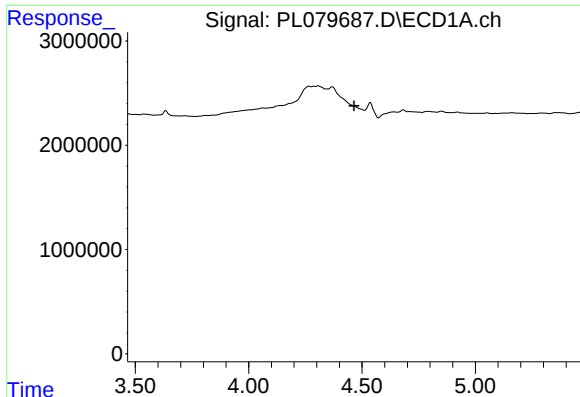

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

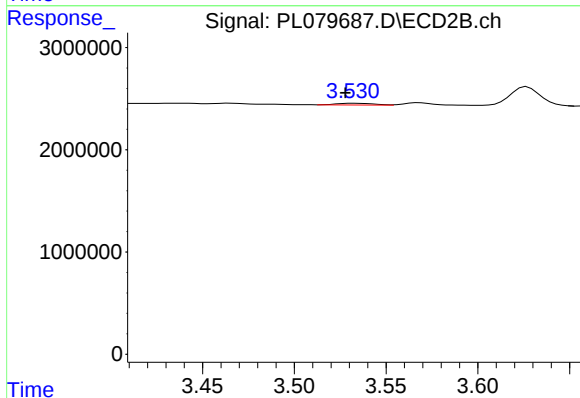


#23 Chlordane-1

R.T.: 3.532 min
Delta R.T.: 0.005 min
Response: 228481
Conc: 2.15 ng/ml

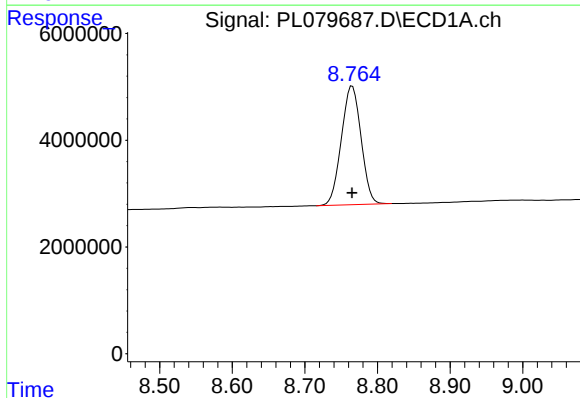

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 41983223
Conc: 21.62 ng/ml

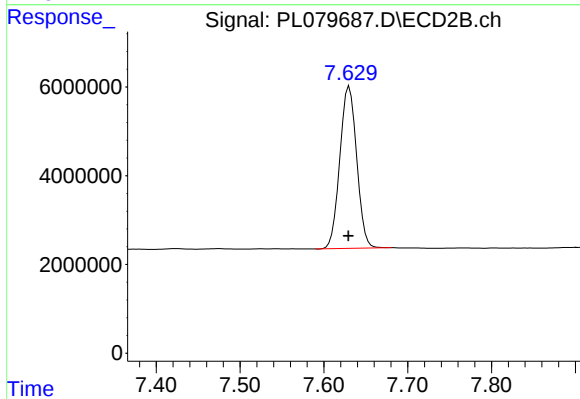

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.001 min
Response: 51164536
Conc: 21.78 ng/ml