

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2022 14:50
 Operator : AR\AJ
 Sample : N5964-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-518-COMP-04

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/13/2022
 Supervised By : Ankita Jodhani 12/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 20:30:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.565	26226334	31580520	11.610m	11.602
28)	SA Decachlor...	8.765	7.630	28016220	32672468	14.426	13.907

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121222\
Data File : PL079676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2022 14:50
Operator : AR\AJ
Sample : N5964-07
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-518-COMP-04


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/13/2022
Supervised By : Ankita Jodhani 12/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 20:30:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

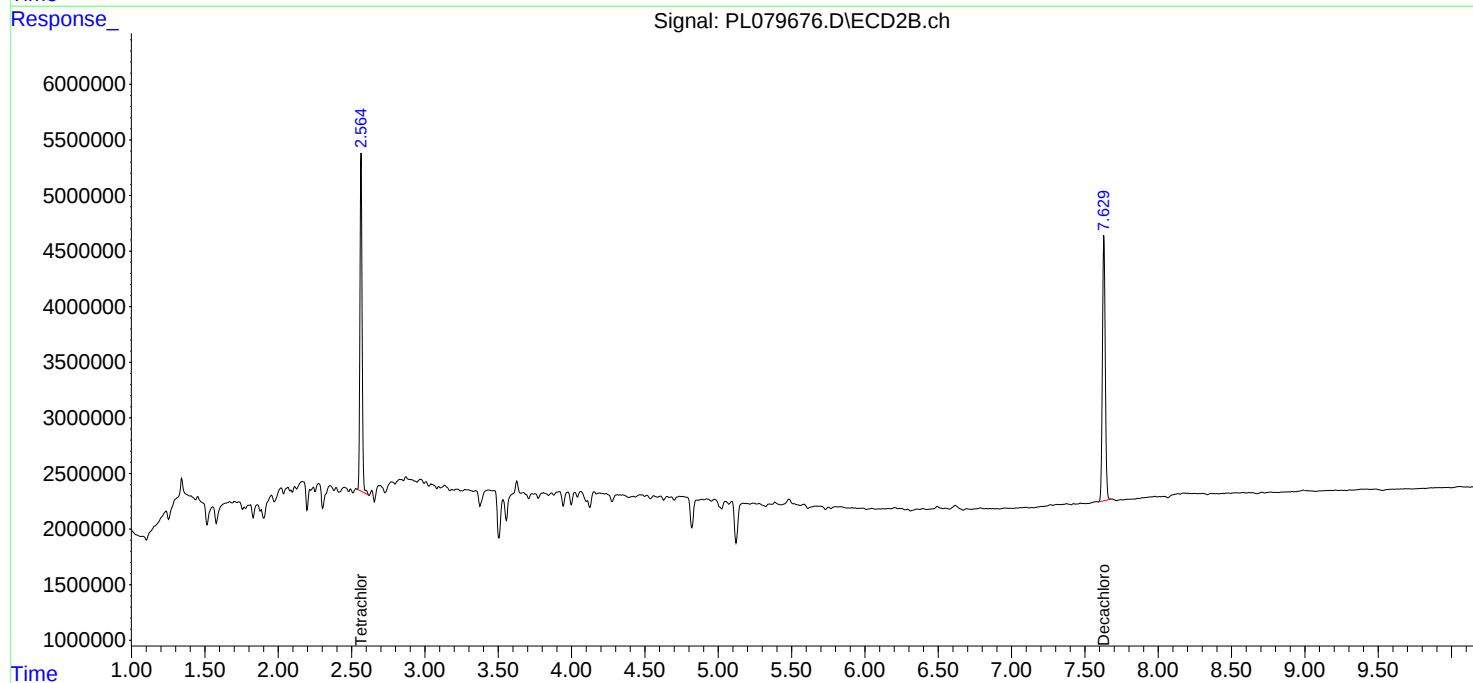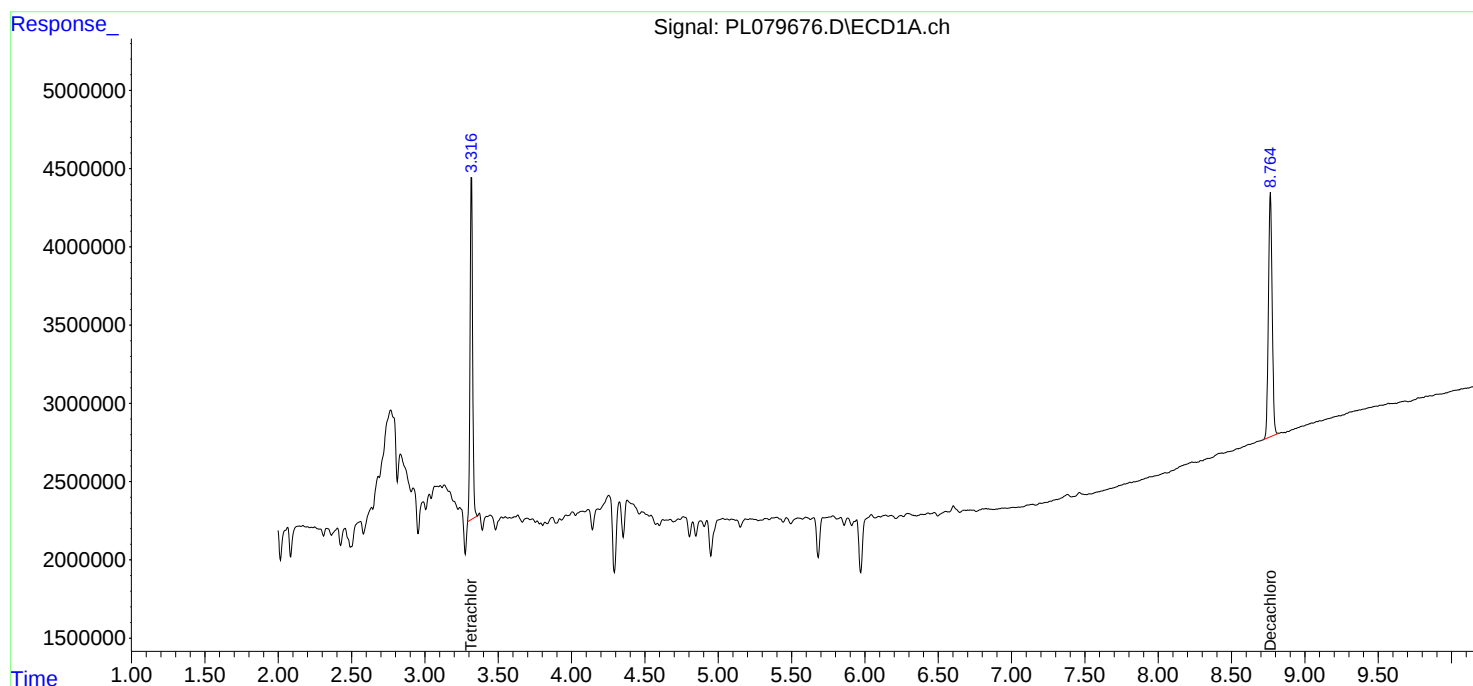

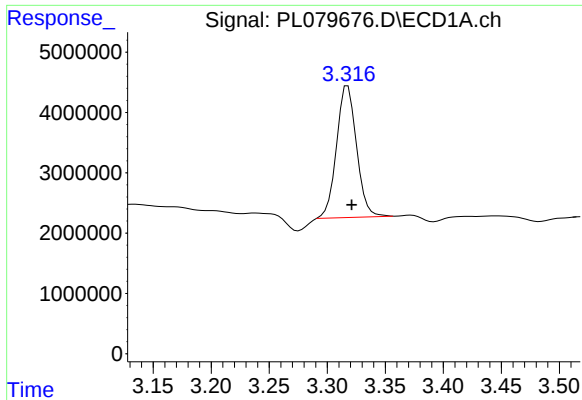


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.005 min
Response: 26226334
Conc: 11.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-518-COMP-04


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/13/2022
Supervised By :Ankita Jodhani 12/13/2022

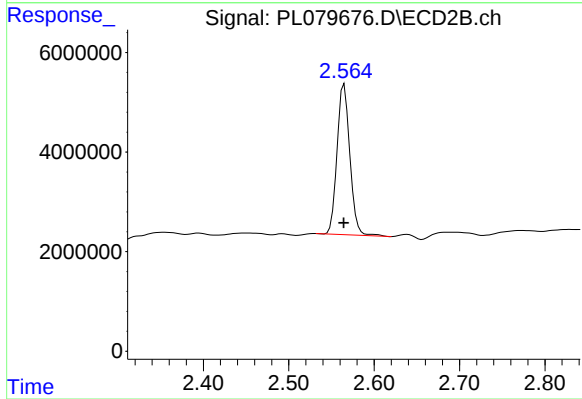


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 31580520
Conc: 11.60 ng/ml

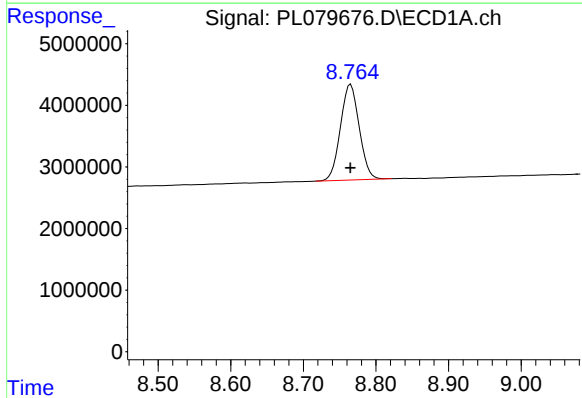

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 28016220
Conc: 14.43 ng/ml

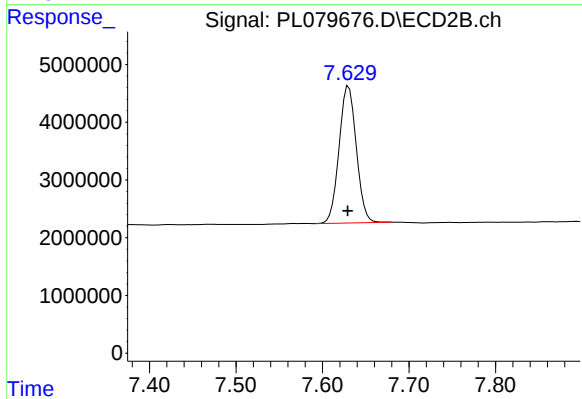

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.001 min
Response: 32672468
Conc: 13.91 ng/ml