

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
 Data File : PL087086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 12:52
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 15:55:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 15:50:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	2.702	66265923	18066023	18.162	18.292
28)	SA Decachlor...	9.048	7.901	55135924	19109058	18.216	18.655
Target Compounds							
9)	A Endosulfan I	6.007	5.045	35754915	12980256	8.862	10.678
10)	B gamma-Chl...	5.878	4.927	39669060	13280063	9.246	10.851
12)	B 4,4'-DDE	6.143	5.190	59766530	19265977	18.258	18.534
13)	MA Dieldrin	6.287	5.313	73140968	21461830	17.947	18.444
19)	B Endosulfa...	7.111	6.294	60745116	17751832	18.478	19.000
20)	A Methoxychlor	7.478	6.589	140.0E6	49873454	95.751	91.473
21)	B Endrin ke...	7.599	6.800	60316333	19273927	18.591	17.933



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
Data File : PL087086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 12:52
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 15:55:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 15:50:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

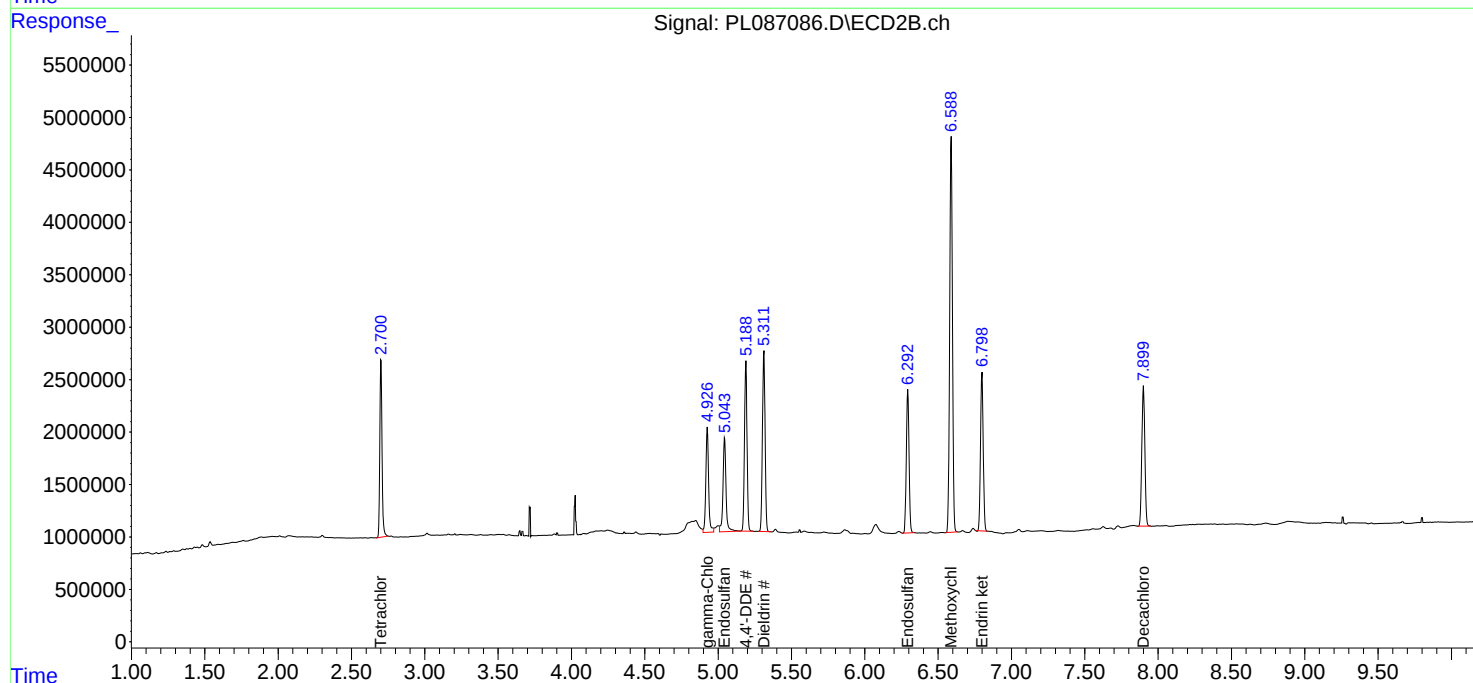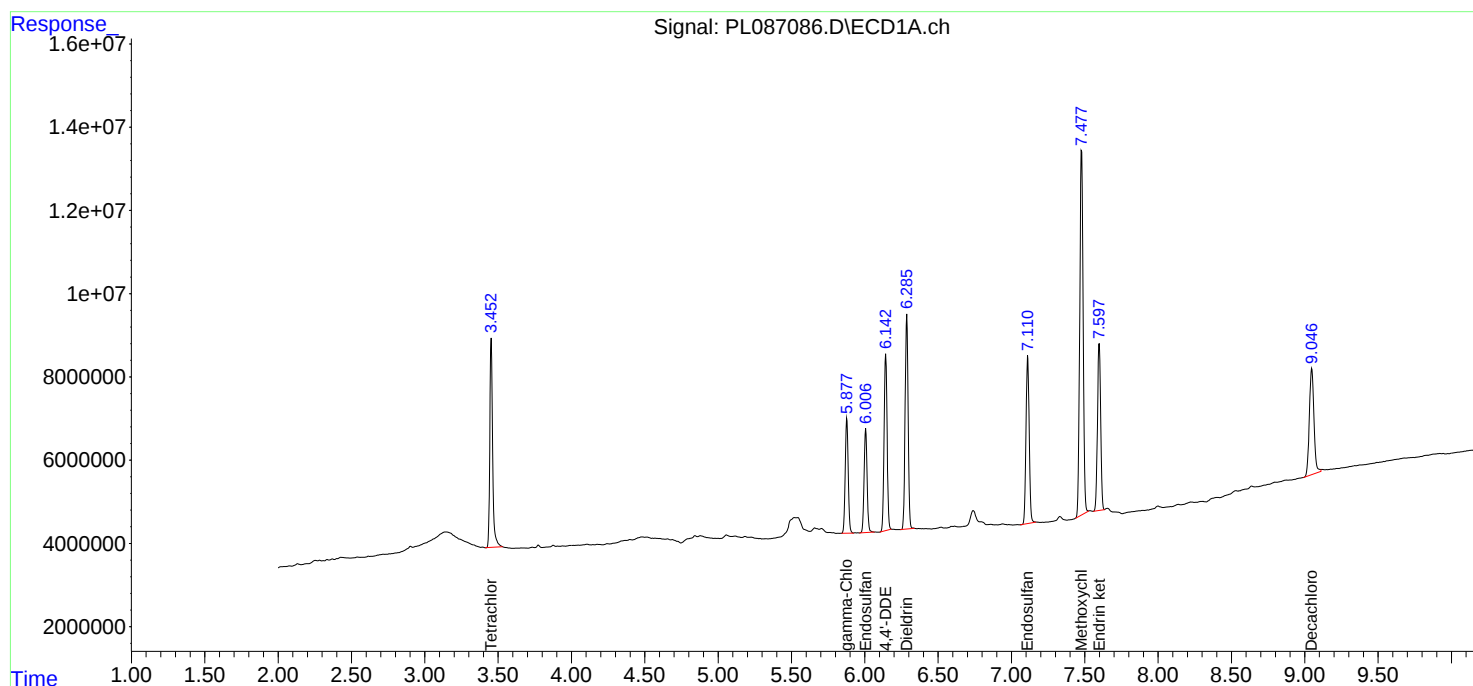


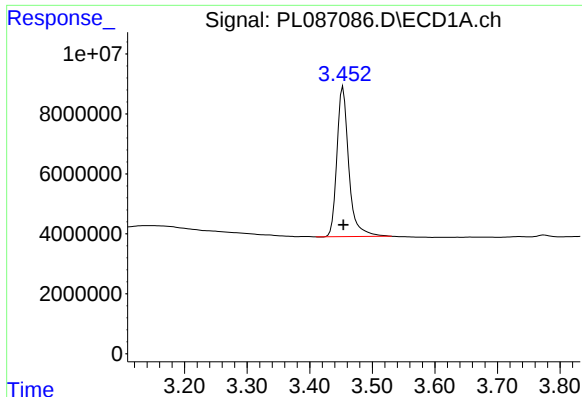

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 66265923
Conc: 18.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

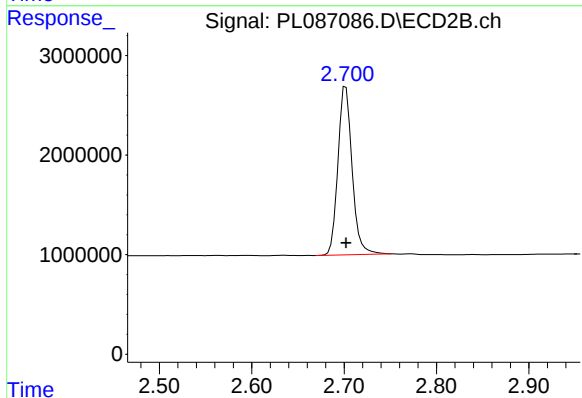


#1 Tetrachloro-m-xylene

R.T.: 2.702 min
Delta R.T.: 0.000 min
Response: 18066023
Conc: 18.29 ng/ml

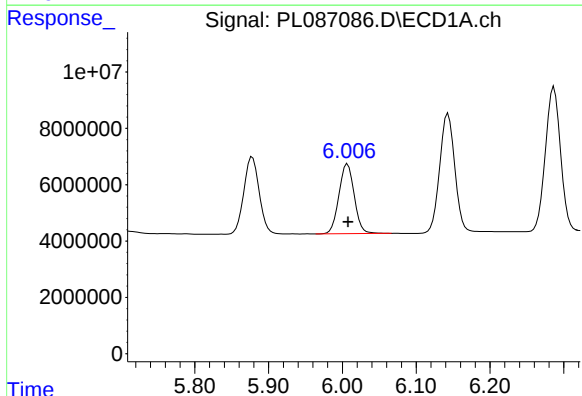


#9 Endosulfan I

R.T.: 6.007 min
Delta R.T.: 0.000 min
Response: 35754915
Conc: 8.86 ng/ml

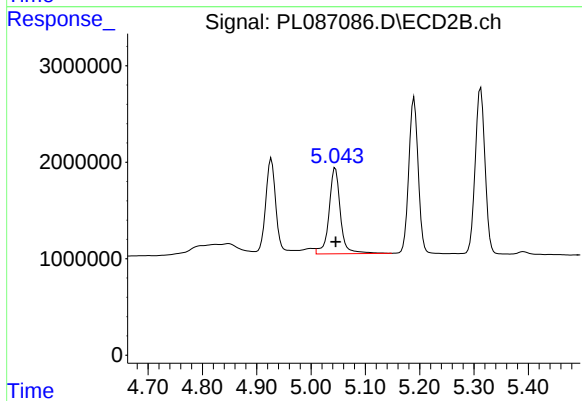

#9 Endosulfan I


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 12980256
Conc: 10.68 ng/ml

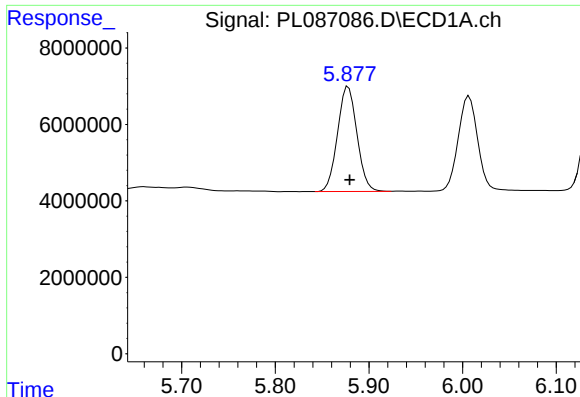

#10 gamma-Chlordane


R.T.: 5.878 min
Delta R.T.: -0.002 min
Response: 39669060
Conc: 9.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

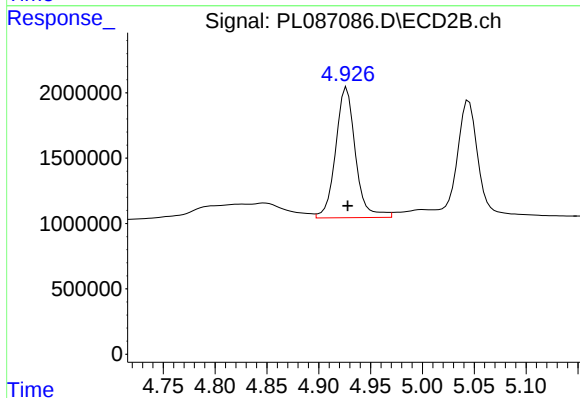


#10 gamma-Chlordane

R.T.: 4.927 min
Delta R.T.: -0.001 min
Response: 13280063
Conc: 10.85 ng/ml

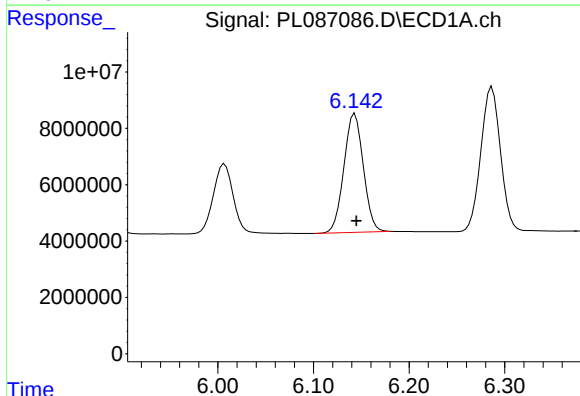


#12 4,4'-DDE

R.T.: 6.143 min
Delta R.T.: -0.002 min
Response: 59766530
Conc: 18.26 ng/ml

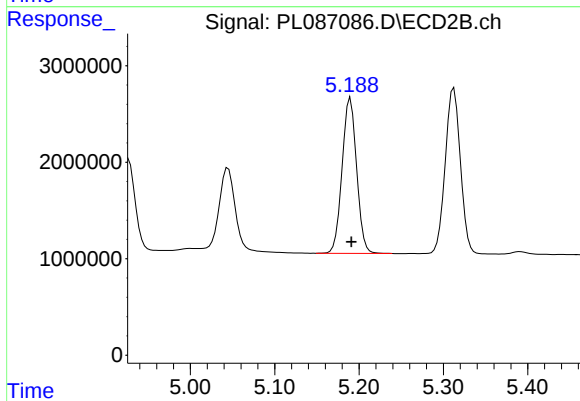

#12 4,4'-DDE


R.T.: 5.190 min
Delta R.T.: 0.000 min
Response: 19265977
Conc: 18.53 ng/ml

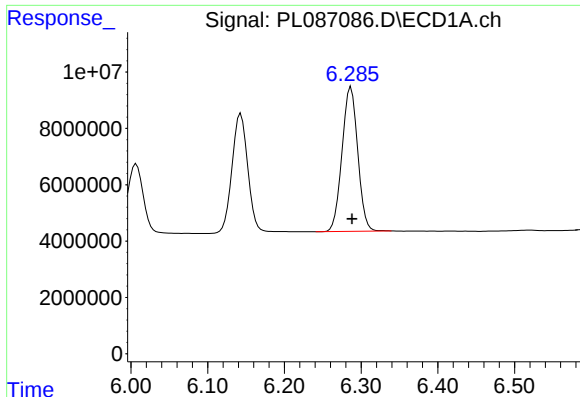

#13 Dieldrin


R.T.: 6.287 min
Delta R.T.: -0.001 min
Response: 73140968
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

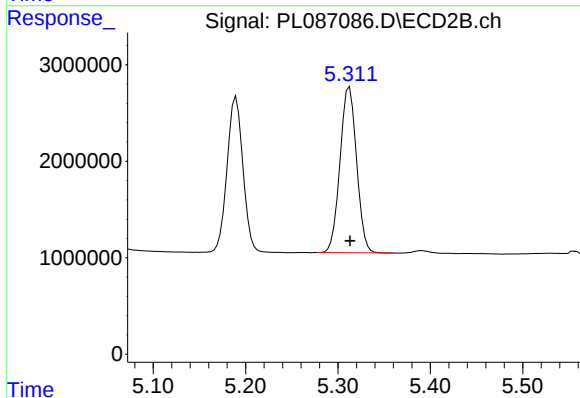


#13 Dieldrin

R.T.: 5.313 min
Delta R.T.: 0.000 min
Response: 21461830
Conc: 18.44 ng/ml

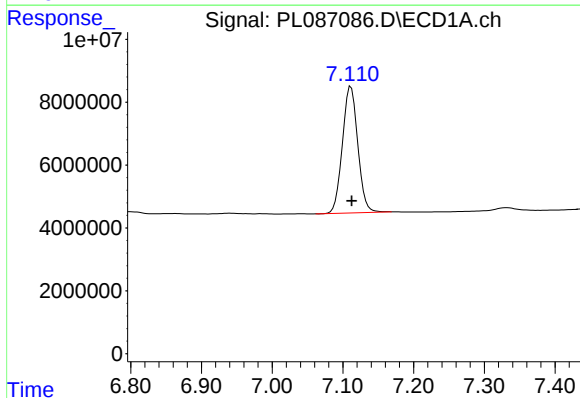


#19 Endosulfan Sulfate

R.T.: 7.111 min
Delta R.T.: 0.000 min
Response: 60745116
Conc: 18.48 ng/ml

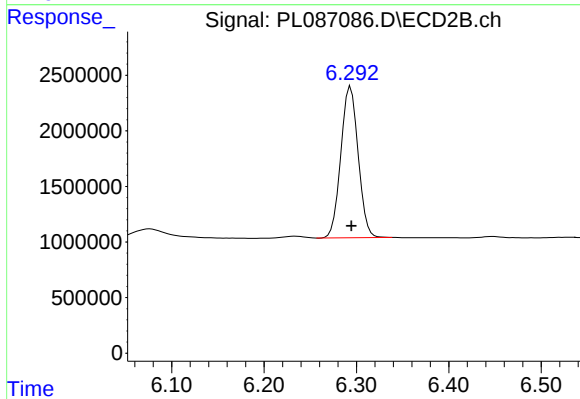

#19 Endosulfan Sulfate


R.T.: 6.294 min
Delta R.T.: 0.000 min
Response: 17751832
Conc: 19.00 ng/ml

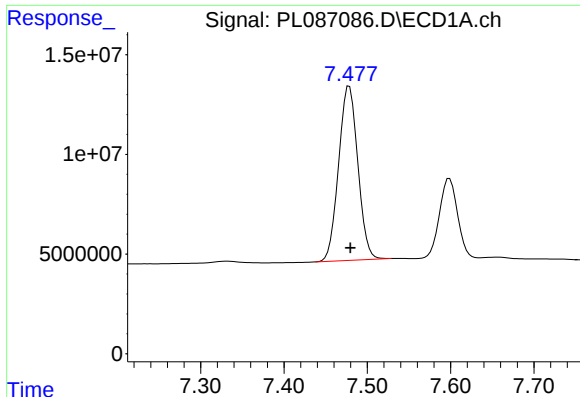

#20 Methoxychlor


R.T.: 7.478 min
Delta R.T.: -0.001 min
Response: 140027628
Conc: 95.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

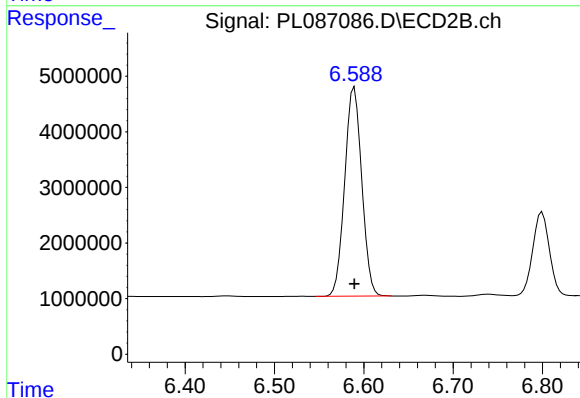


#20 Methoxychlor

R.T.: 6.589 min
Delta R.T.: 0.000 min
Response: 49873454
Conc: 91.47 ng/ml

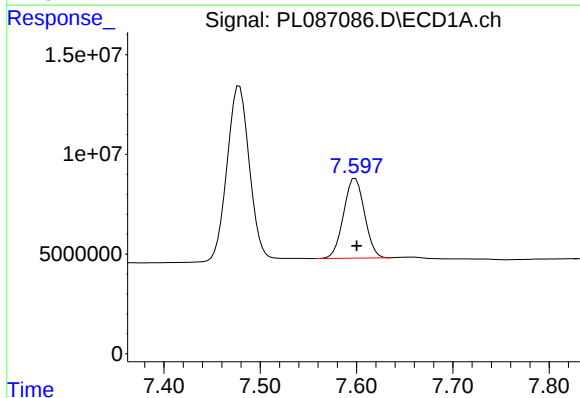


#21 Endrin ketone

R.T.: 7.599 min
Delta R.T.: -0.002 min
Response: 60316333
Conc: 18.59 ng/ml

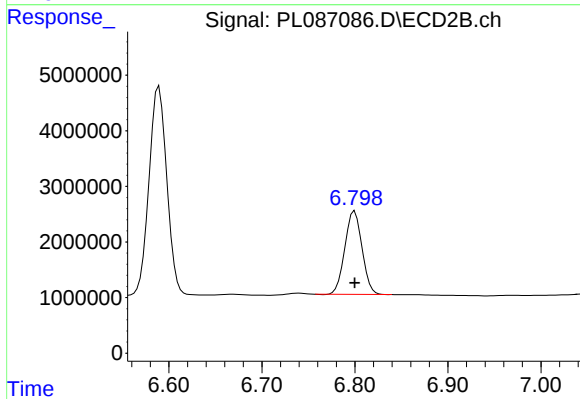

#21 Endrin ketone


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 19273927
Conc: 17.93 ng/ml

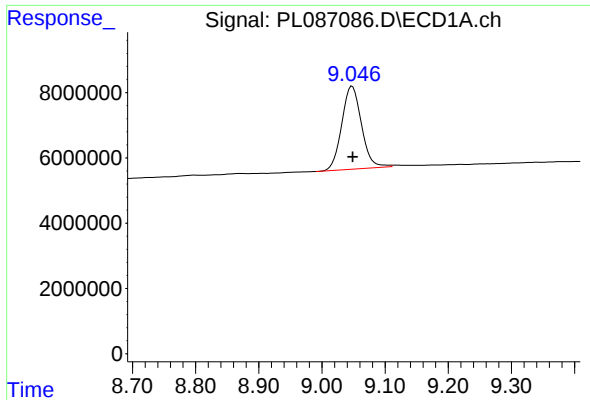

#28 Decachlorobiphenyl

R.T.: 9.048 min
Delta R.T.: 0.000 min
Response: 55135924
Conc: 18.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

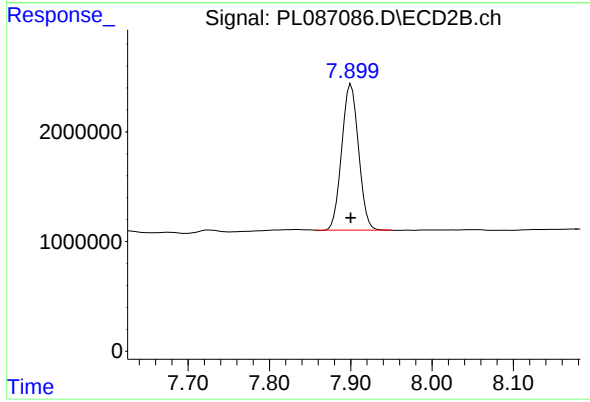

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 19109058
Conc: 18.65 ng/ml