

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
 Data File : PL087093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 14:29
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 15:43:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 15:39:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	2.701	253.9E6	87795556	74.420	74.162
28)	SA Decachlor...	9.048	7.900	202.6E6	70476029	74.122	74.394
Target Compounds							
23)	Chlordane-1	4.626	3.709	111.5E6	25123021	743.543	739.269
24)	Chlordane-2	5.163	4.292	113.9E6	30563971	743.659	736.983
25)	Chlordane-3	5.880	4.927	464.1E6	93768724	745.281	811.369
26)	Chlordane-4	5.964	4.991	568.0E6	97342997	744.304	737.903
27)	Chlordane-5	6.820	5.665	86897939	24391736	743.480	769.838



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
Data File : PL087093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 14:29
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 15:43:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 15:39:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

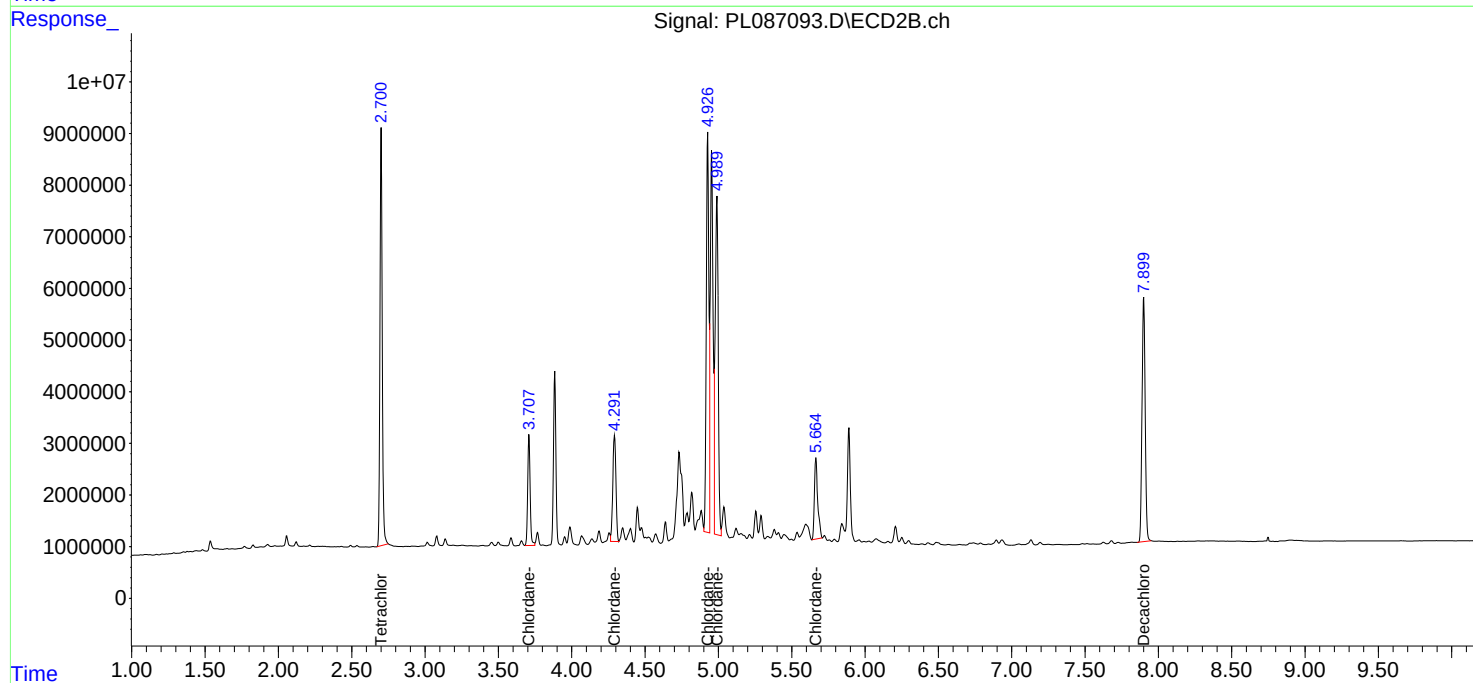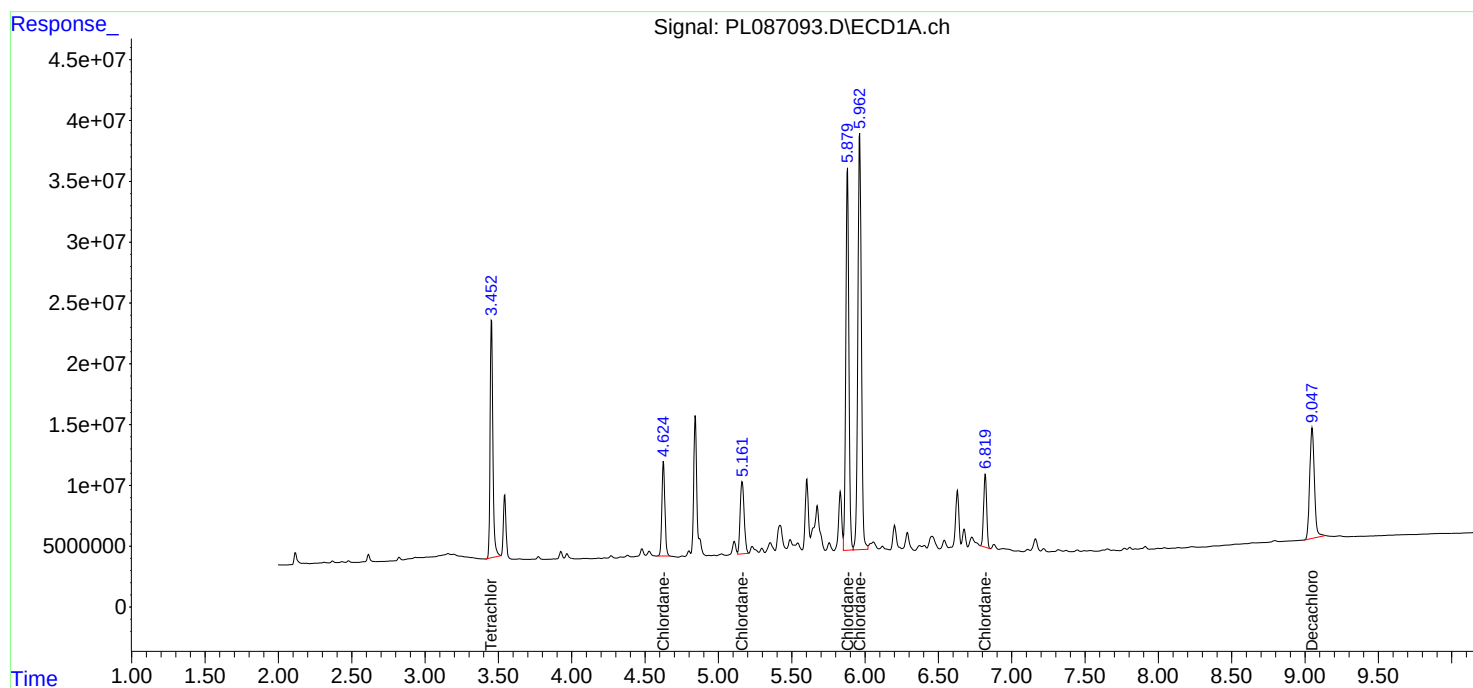


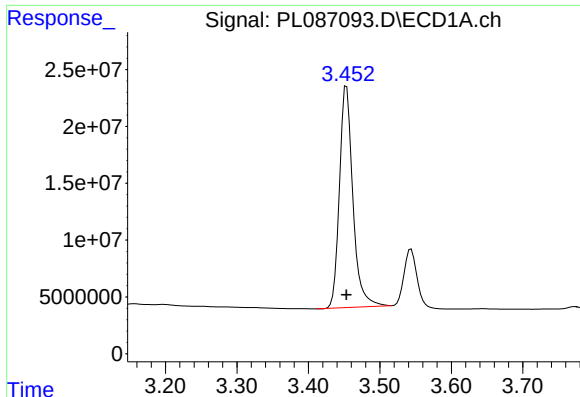

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 253856451
Conc: 74.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

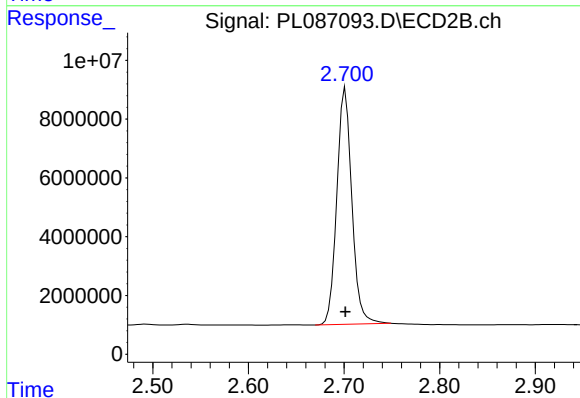


#1 Tetrachloro-m-xylene

R.T.: 2.701 min
Delta R.T.: 0.000 min
Response: 87795556
Conc: 74.16 ng/ml

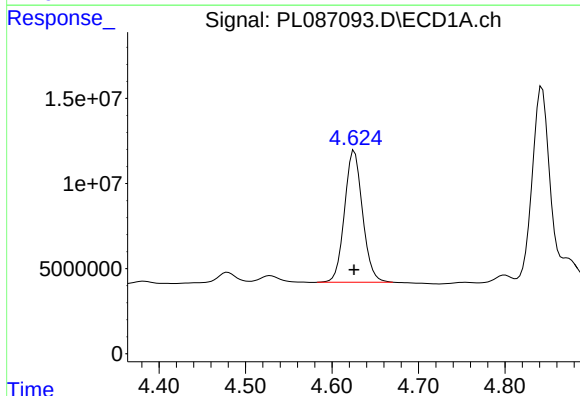


#23 Chlordane-1

R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 111459641
Conc: 743.54 ng/ml

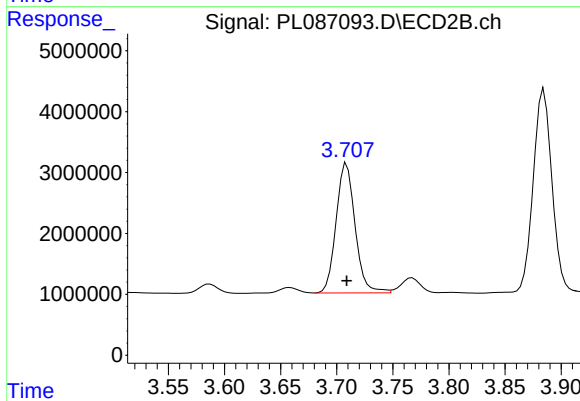

#23 Chlordane-1


R.T.: 3.709 min
Delta R.T.: 0.000 min
Response: 25123021
Conc: 739.27 ng/ml

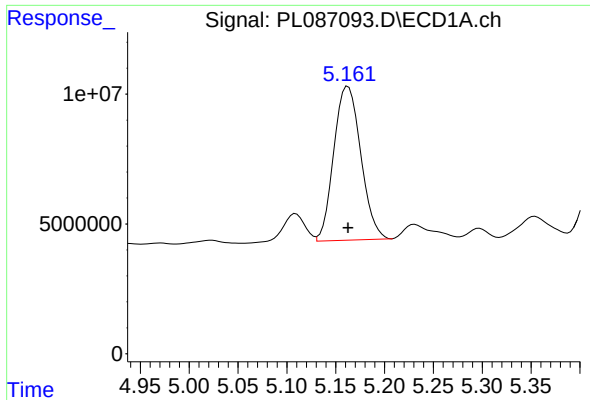

#24 Chlordane-2


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 113933550
Conc: 743.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

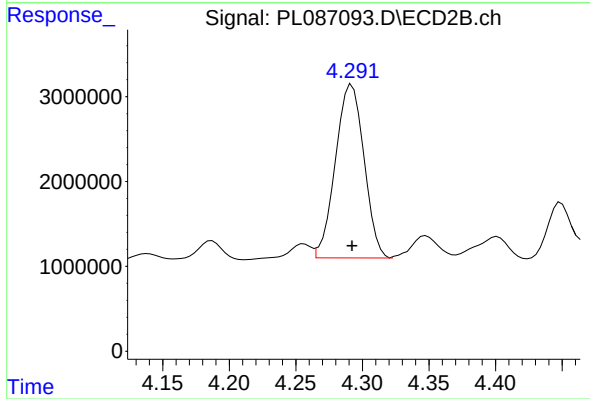


#24 Chlordane-2

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 30563971
Conc: 736.98 ng/ml

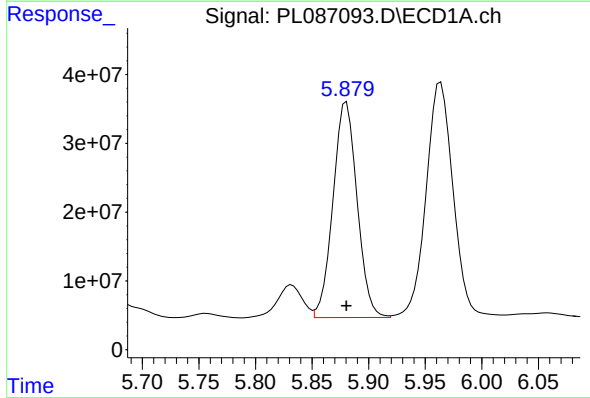


#25 Chlordane-3

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 464060294
Conc: 745.28 ng/ml

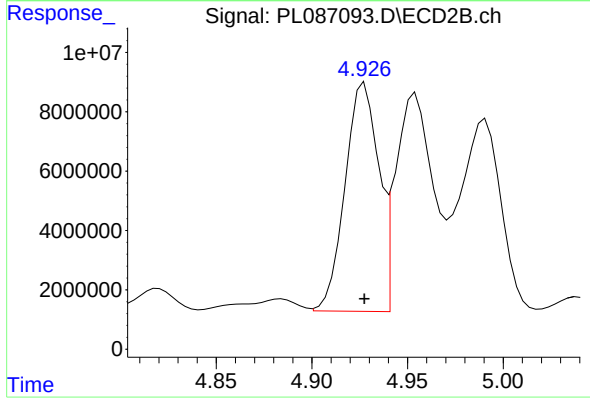

#25 Chlordane-3


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 93768724
Conc: 811.37 ng/ml

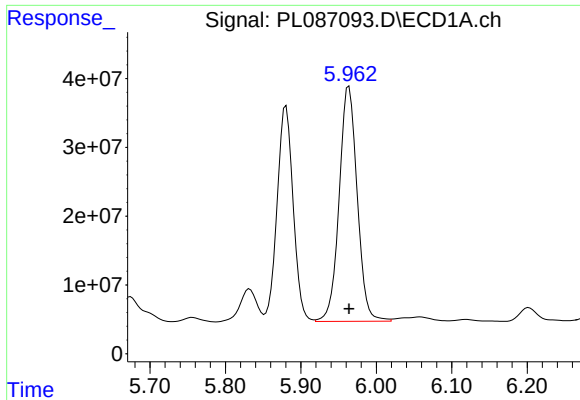

#26 Chlordane-4


R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 567969755
Conc: 744.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

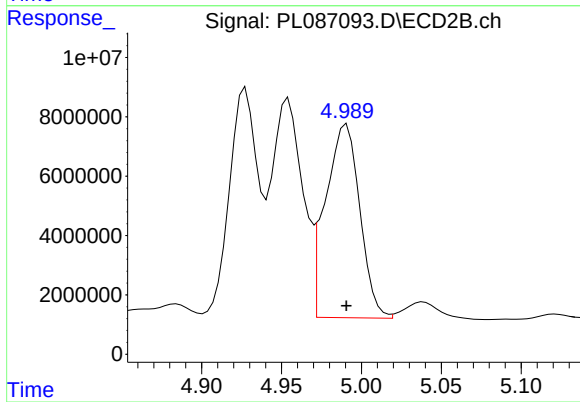


#26 Chlordane-4

R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 97342997
Conc: 737.90 ng/ml

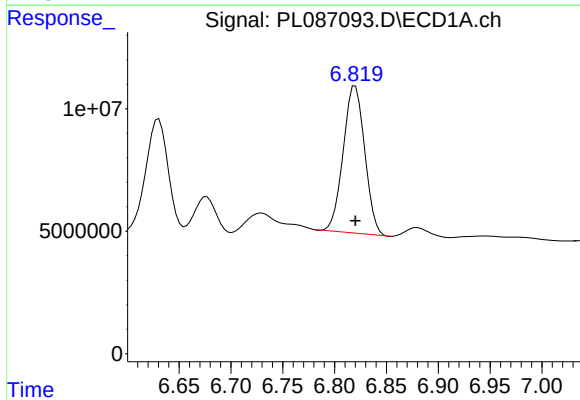


#27 Chlordane-5

R.T.: 6.820 min
Delta R.T.: 0.000 min
Response: 86897939
Conc: 743.48 ng/ml

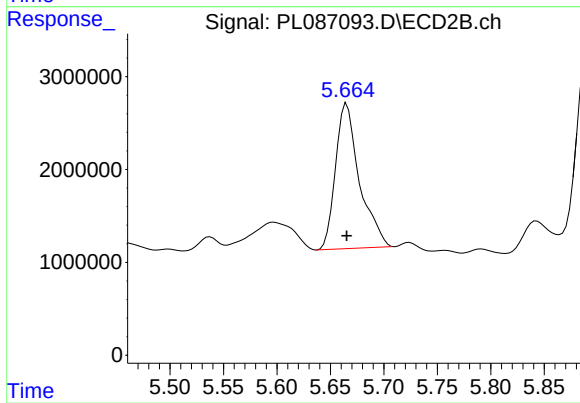

#27 Chlordane-5

R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 24391736
Conc: 769.84 ng/ml

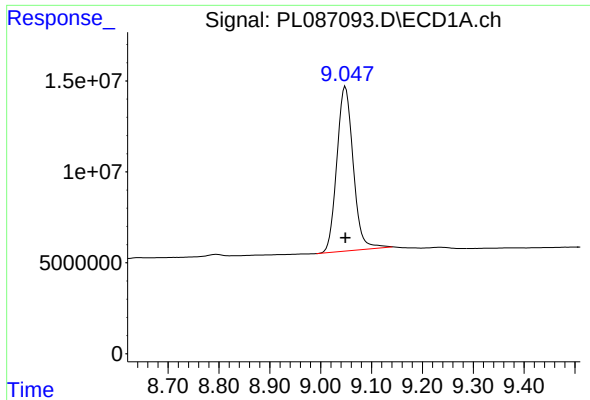

#28 Decachlorobiphenyl


R.T.: 9.048 min

Delta R.T.: 0.000 min

Response: 202590280

Conc: 74.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

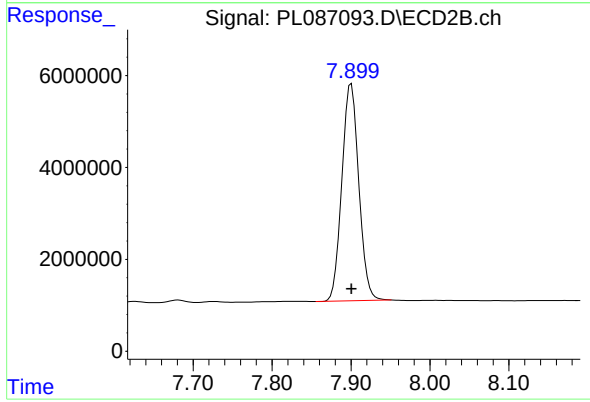

#28 Decachlorobiphenyl

R.T.: 7.900 min

Delta R.T.: 0.000 min

Response: 70476029

Conc: 74.39 ng/ml