

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
 Data File : PL087095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 14:57
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 15:46:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 15:39:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	2.701	85609847	28749185	25.073	24.460
28)	SA Decachlor...	9.049	7.900	70223796	25713734	25.516	26.574
Target Compounds							
23)	Chlordane-1	4.625	3.709	37582633	8293726	250.534	245.511
24)	Chlordane-2	5.162	4.292	40745929	10771022	261.778	257.219
25)	Chlordane-3	5.880	4.927	143.2E6	30791177	234.724	262.125
26)	Chlordane-4	5.964	4.990	179.9E6	32145455	239.209	245.228
27)	Chlordane-5	6.819	5.665	28701829	8144887	246.660	255.261



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
Data File : PL087095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 14:57
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 15:46:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 15:39:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

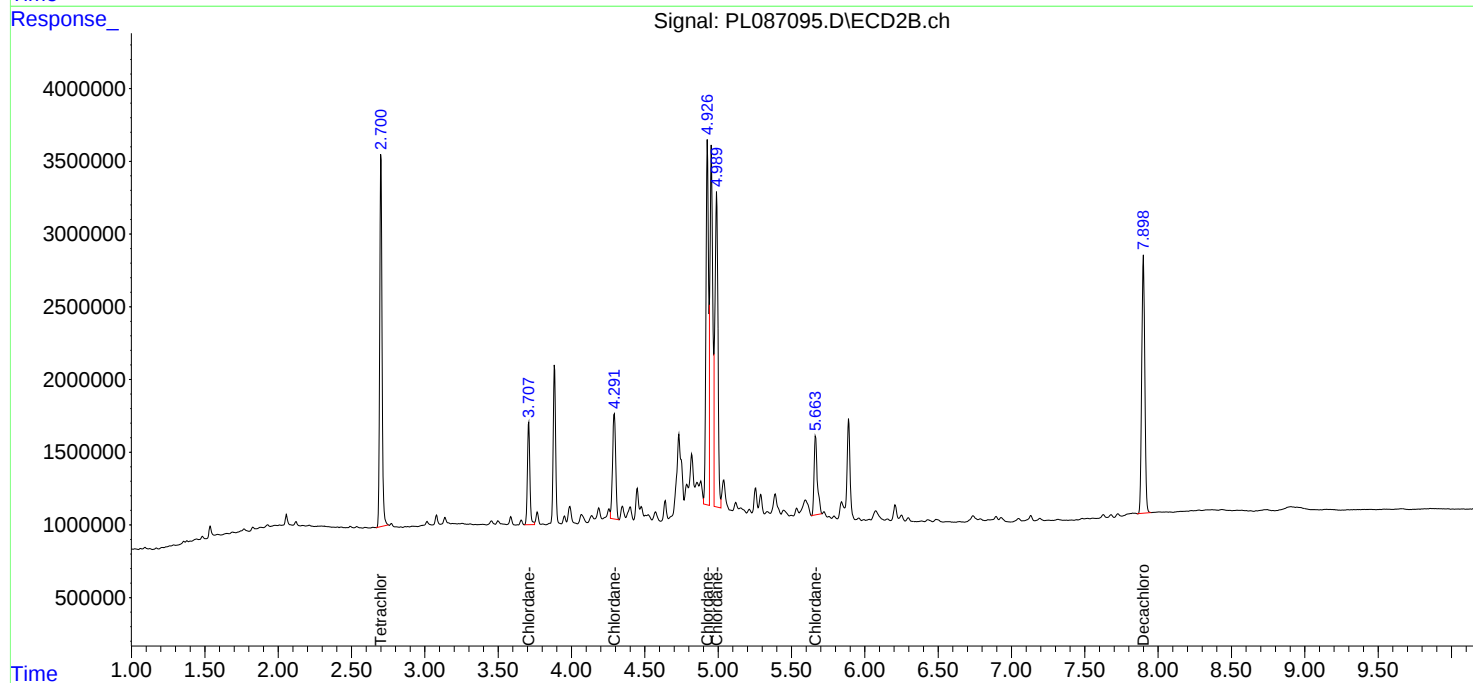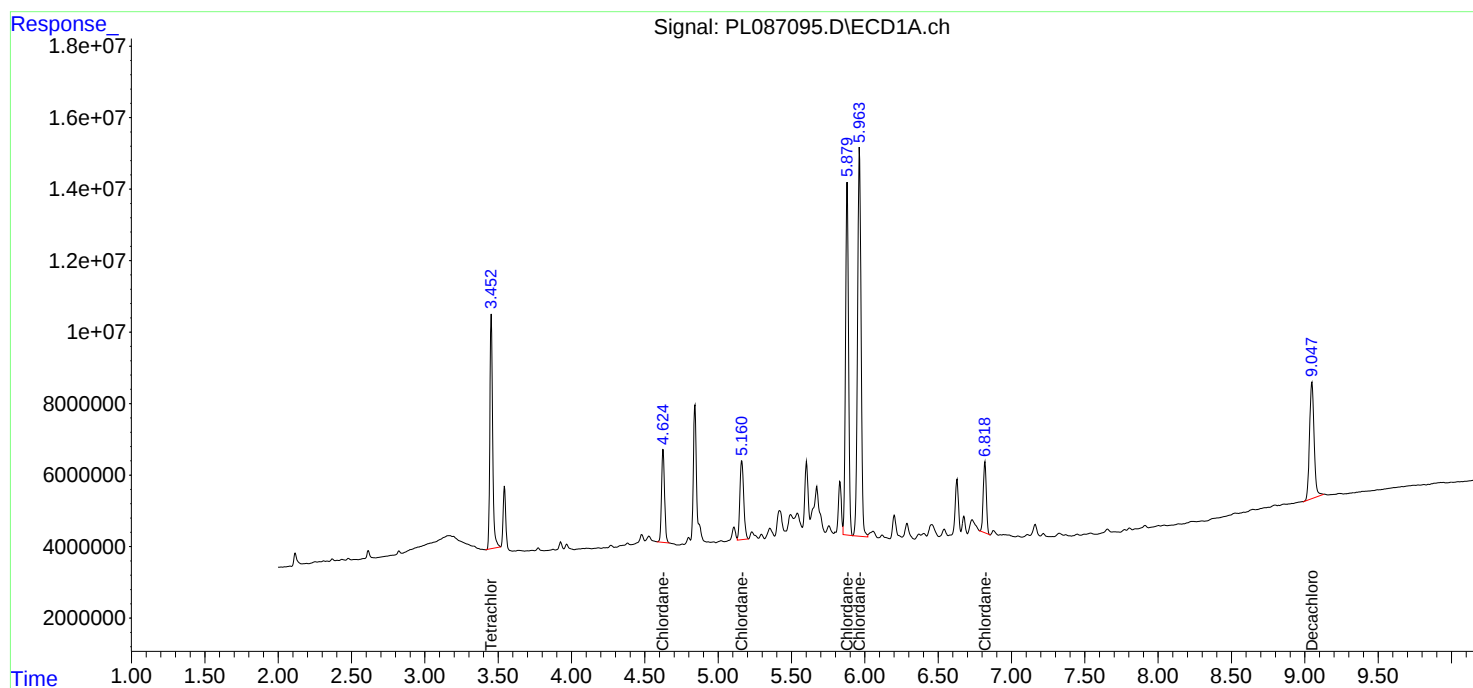


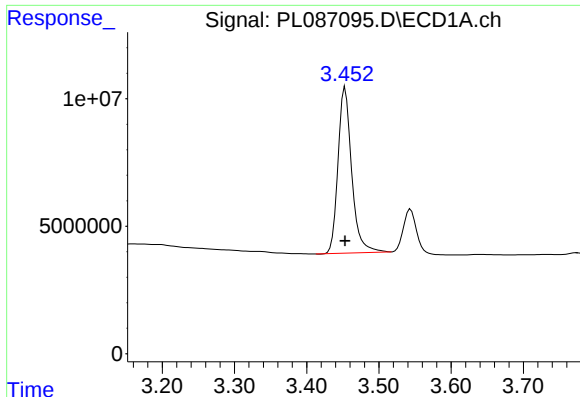

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 85609847
Conc: 25.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

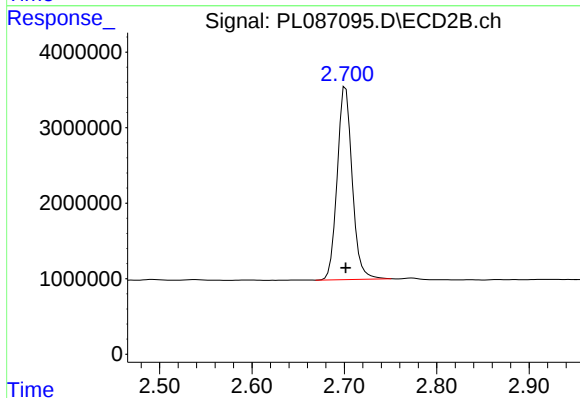


#1 Tetrachloro-m-xylene

R.T.: 2.701 min
Delta R.T.: 0.000 min
Response: 28749185
Conc: 24.46 ng/ml

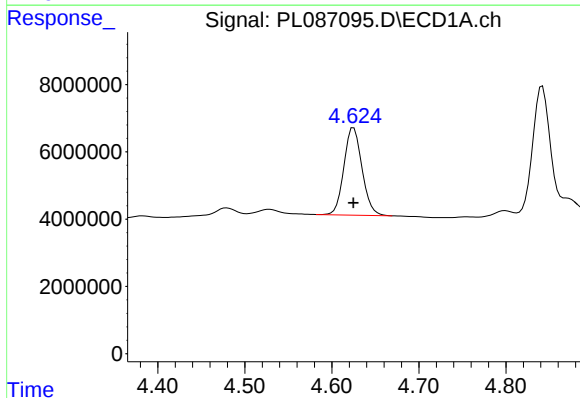


#23 Chlordane-1

R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 37582633
Conc: 250.53 ng/ml

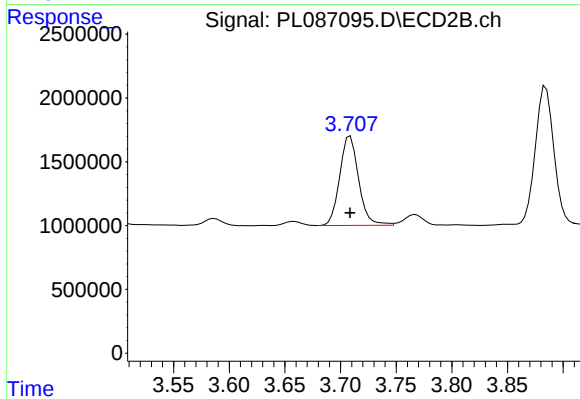

#23 Chlordane-1


R.T.: 3.709 min
Delta R.T.: 0.000 min
Response: 8293726
Conc: 245.51 ng/ml

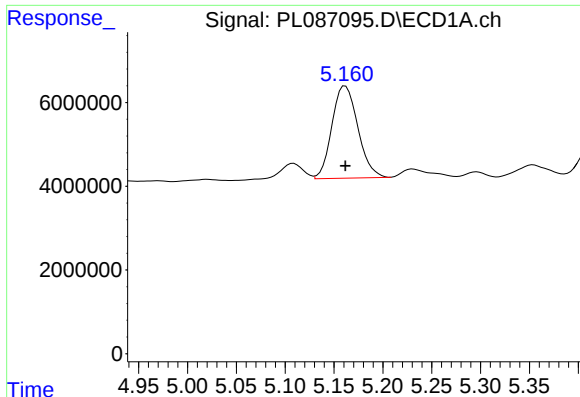

#24 Chlordane-2


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 40745929
Conc: 261.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

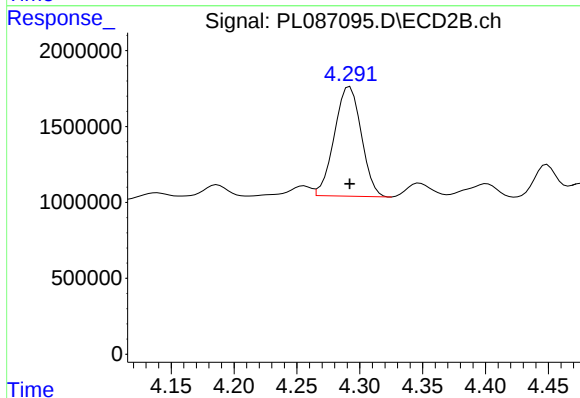


#24 Chlordane-2

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 10771022
Conc: 257.22 ng/ml

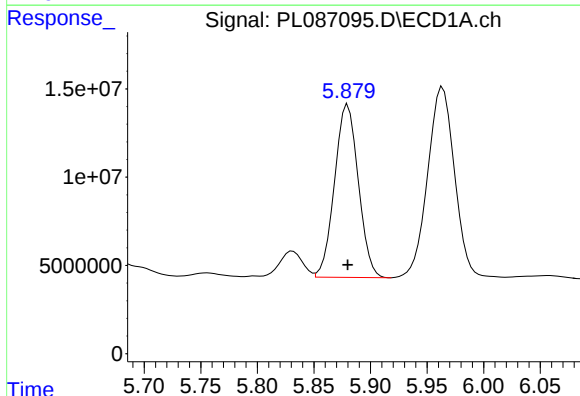


#25 Chlordane-3

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 143237213
Conc: 234.72 ng/ml

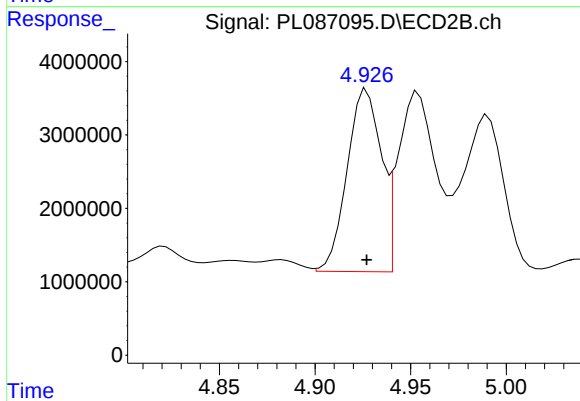

#25 Chlordane-3


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 30791177
Conc: 262.12 ng/ml

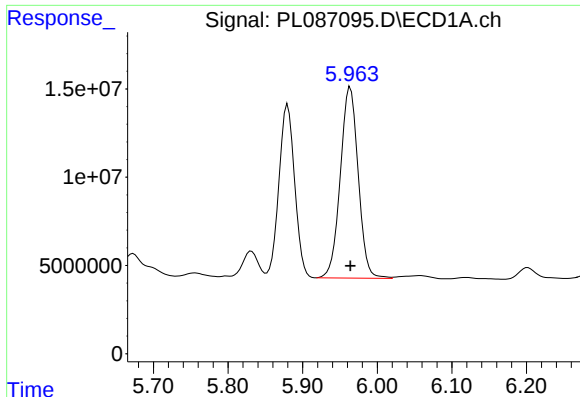

#26 Chlordane-4


R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 179948706
Conc: 239.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

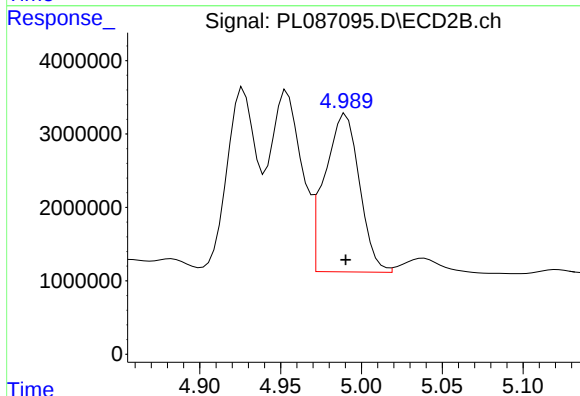


#26 Chlordane-4

R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 32145455
Conc: 245.23 ng/ml

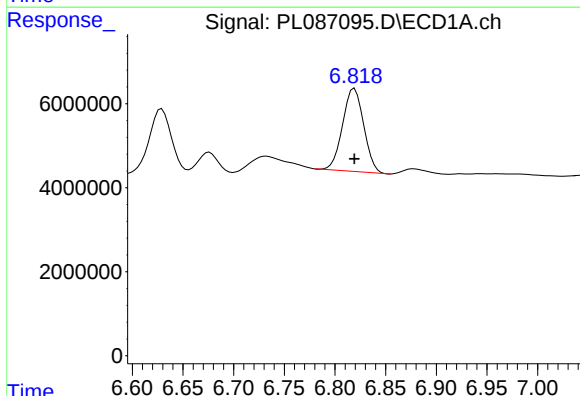


#27 Chlordane-5

R.T.: 6.819 min
Delta R.T.: 0.000 min
Response: 28701829
Conc: 246.66 ng/ml

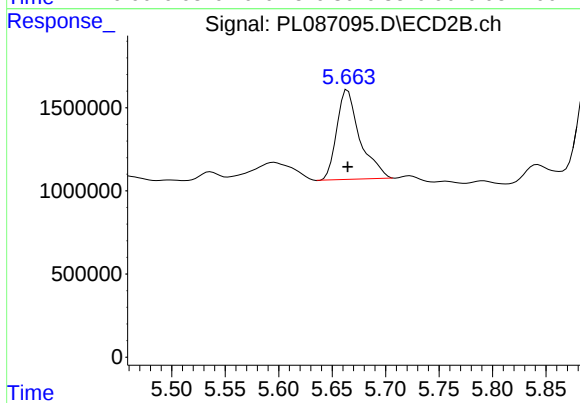

#27 Chlordane-5


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 8144887
Conc: 255.26 ng/ml

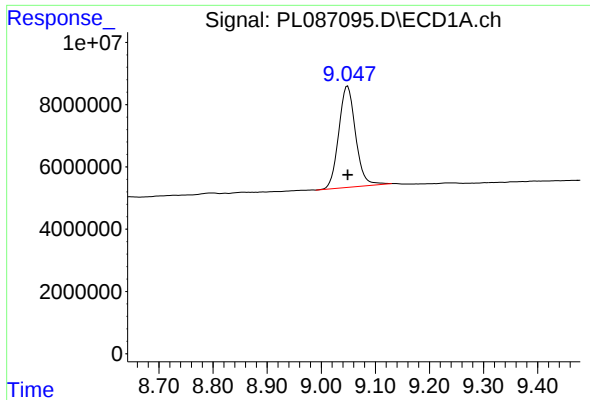

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 70223796
Conc: 25.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

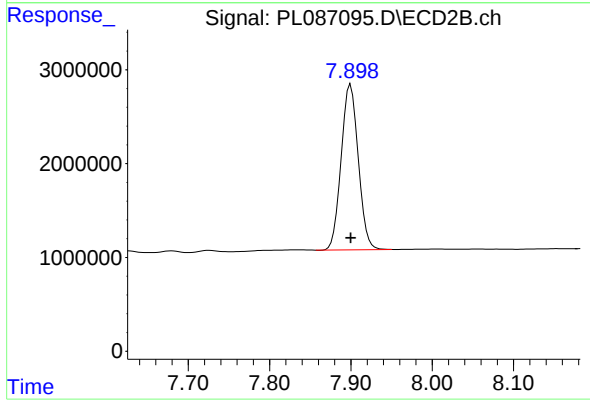

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 25713734
Conc: 26.57 ng/ml