

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
 Data File : PL087096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 15:11
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 15:48:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 15:39:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	2.701	17434296	5673938	5.084	4.861
28)	SA Decachlor...	9.049	7.900	14895848	5565972	5.325	5.584
Target Compounds							
23)	Chlordane-1	4.625	3.708	7214841	1698076	48.465	50.213
24)	Chlordane-2	5.161	4.292	8579435	2263064	54.014	53.183
25)	Chlordane-3	5.880	4.927	29791799	6500461	49.052	54.181
26)	Chlordane-4	5.963	4.990	37877958	7075319	50.281	53.131
27)	Chlordane-5	6.818	5.665	5880192	1588707	50.426	49.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121223\
Data File : PL087096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 15:11
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 15:48:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 15:39:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

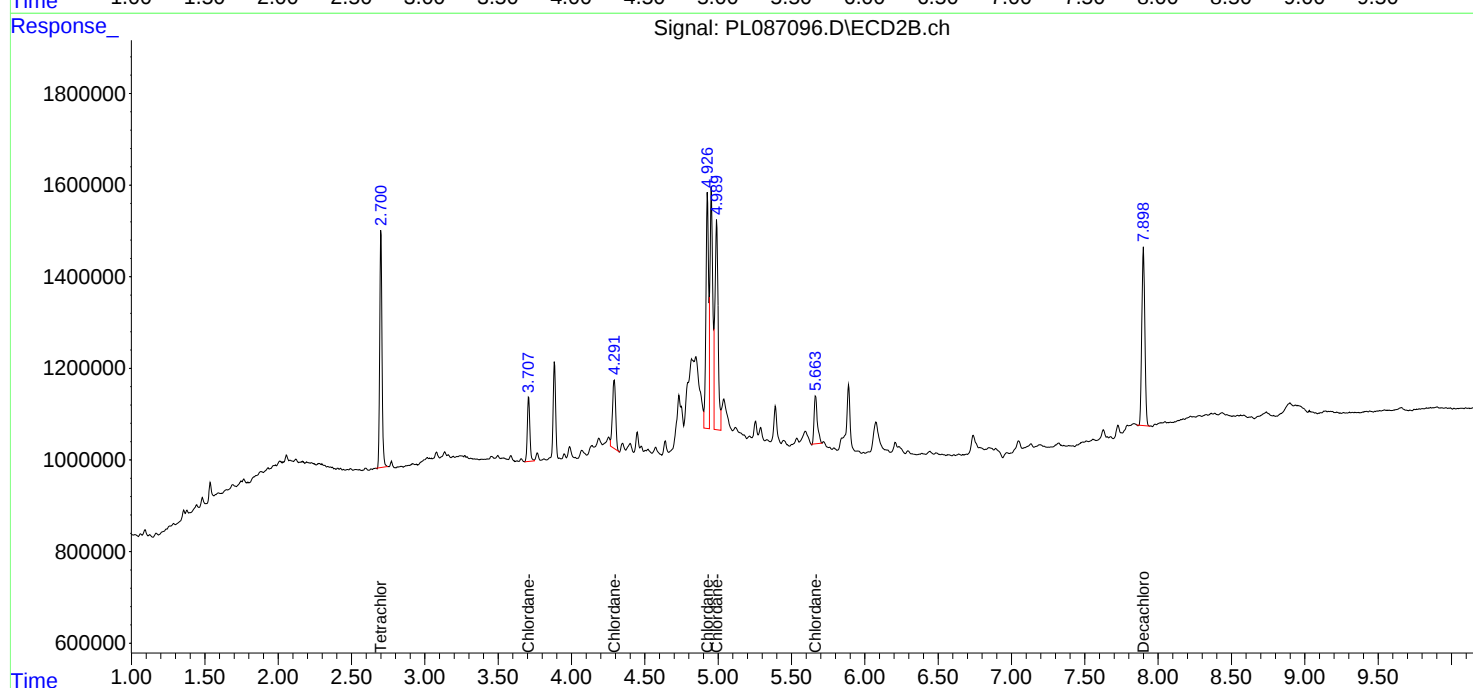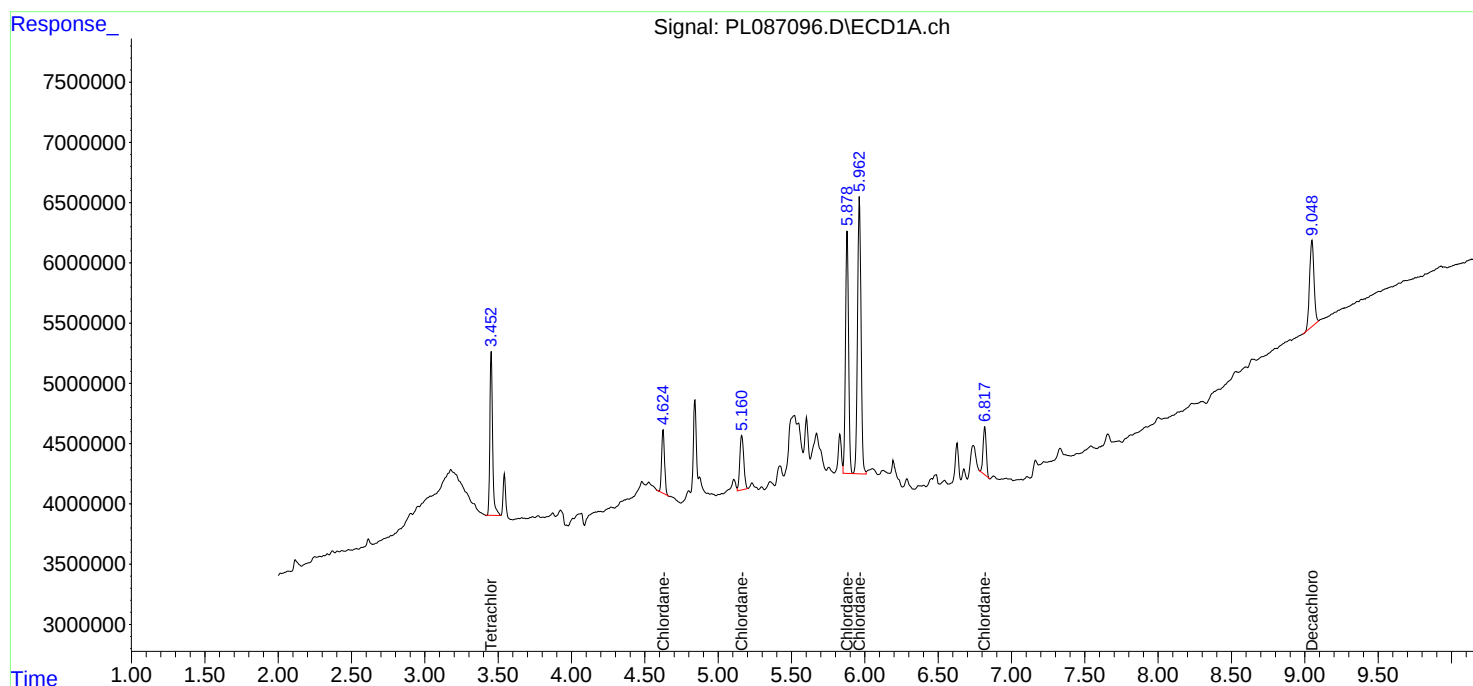


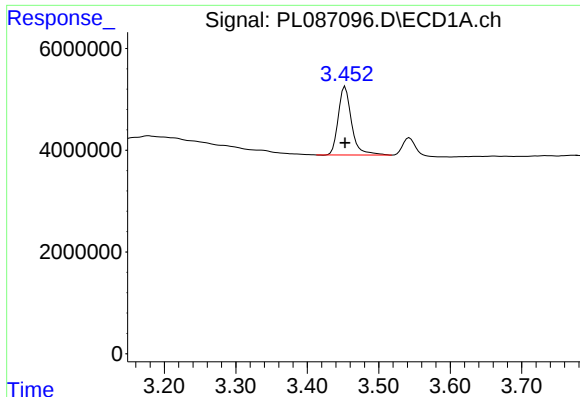

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 17434296
Conc: 5.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

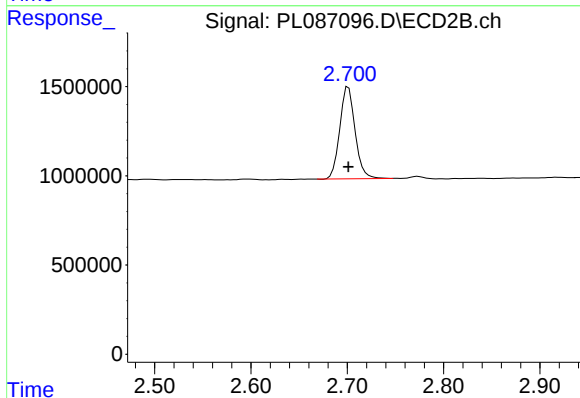


#1 Tetrachloro-m-xylene

R.T.: 2.701 min
Delta R.T.: 0.000 min
Response: 5673938
Conc: 4.86 ng/ml

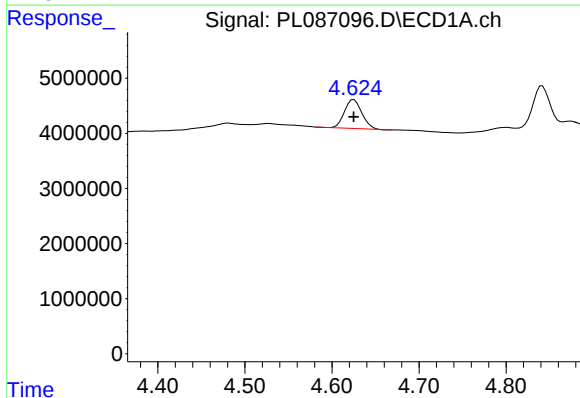


#23 Chlordane-1

R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 7214841
Conc: 48.46 ng/ml

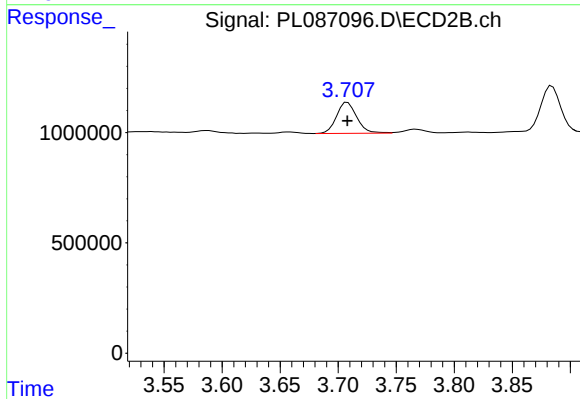

#23 Chlordane-1


R.T.: 3.708 min
Delta R.T.: 0.000 min
Response: 1698076
Conc: 50.21 ng/ml

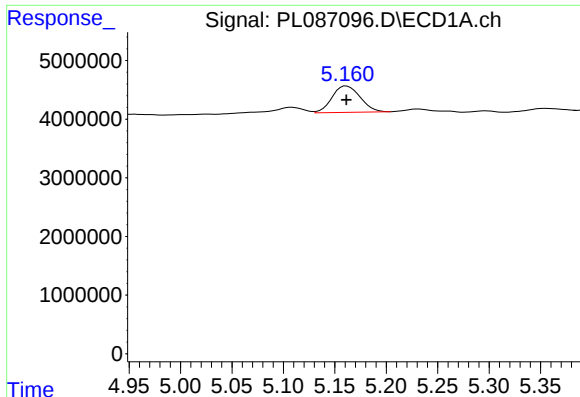

#24 Chlordane-2


R.T.: 5.161 min
Delta R.T.: 0.000 min
Response: 8579435
Conc: 54.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

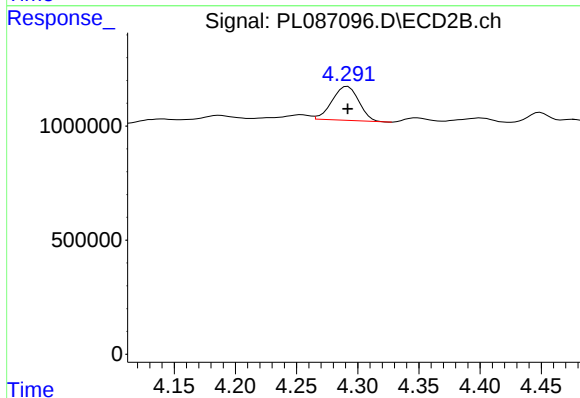


#24 Chlordane-2

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 2263064
Conc: 53.18 ng/ml

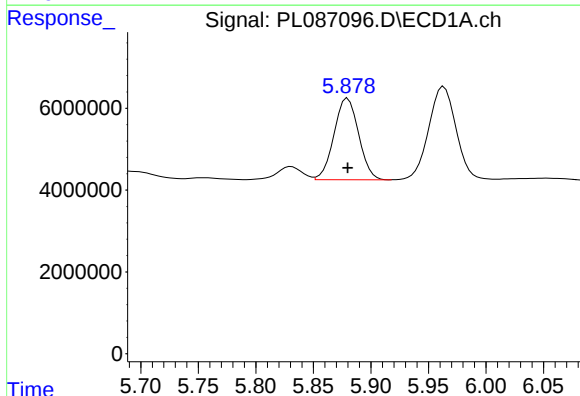


#25 Chlordane-3

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 29791799
Conc: 49.05 ng/ml

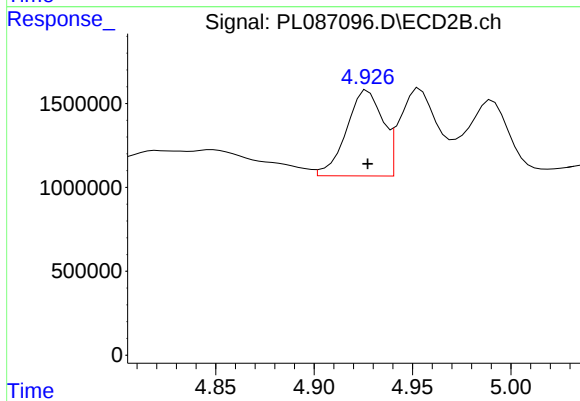

#25 Chlordane-3


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 6500461
Conc: 54.18 ng/ml

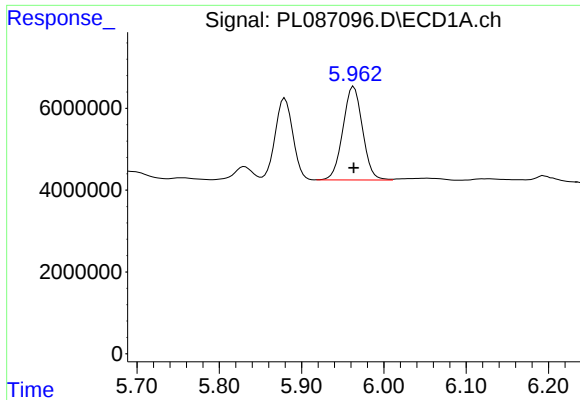

#26 Chlordane-4


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 37877958
Conc: 50.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

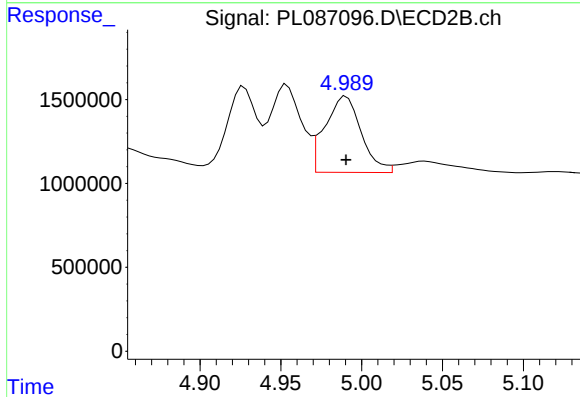


#26 Chlordane-4

R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 7075319
Conc: 53.13 ng/ml

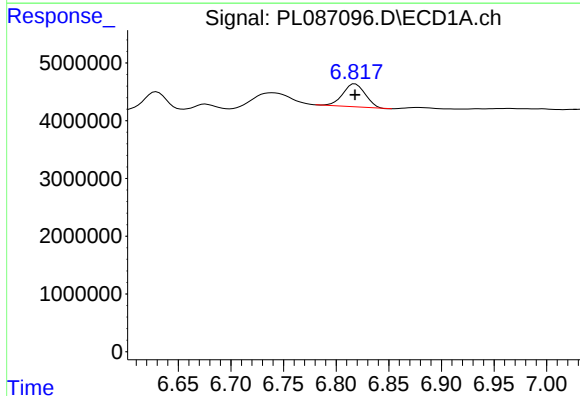


#27 Chlordane-5

R.T.: 6.818 min
Delta R.T.: 0.000 min
Response: 5880192
Conc: 50.43 ng/ml

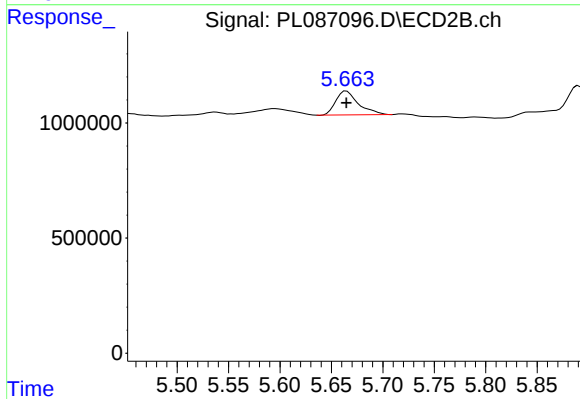

#27 Chlordane-5


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 1588707
Conc: 49.83 ng/ml

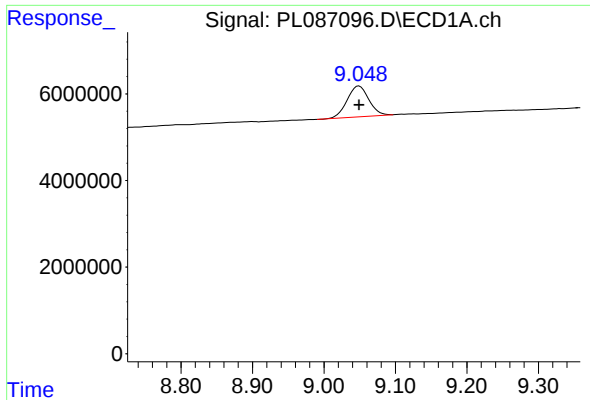

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 14895848
Conc: 5.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

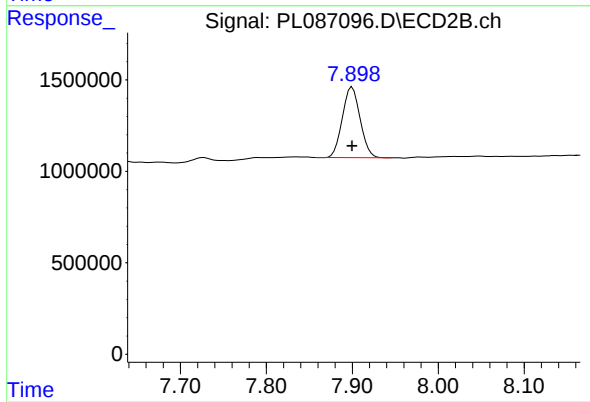

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 5565972
Conc: 5.58 ng/ml