

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121318\
 Data File : PL043110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2018 21:34
 Operator : AJ\SJ
 Sample : J6362-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 00:31:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.098	57316124	30915340	9.346	10.431
28)	SA Decachlor...	8.197	9.224	67086331	26414289	10.274	10.126
Target Compounds							
6)	B beta-BHC	4.395f	0.000	2876337	0	0.780	N.D. #
7)	B delta-BHC	0.000	5.157	0	4418829	N.D.	1.028 #
8)	B Heptachlo...	0.000	5.990	0	3019545	N.D.	0.796 #
14)	MA Endrin	6.060f	0.000	2005493	0	0.279	N.D. #
16)	A 4,4'-DDD	6.197f	6.953	1696800	2422788	0.299	0.826 #
17)	MA 4,4'-DDT	6.367	0.000	1916054	0	0.322	N.D. #
18)	B Endrin al...	6.409f	0.000	822769	0	0.149	N.D. #
19)	B Endosulfa...	6.652	0.000	2323666	0	0.347	N.D. #
21)	B Endrin ke...	0.000	7.819f	0	913575	N.D.	0.299 #
23)	Chlordane-1	4.395	5.157	2876337	4418829	10.704	31.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121318\
Data File : PL043110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2018 21:34
Operator : AJ\SJ
Sample : J6362-04
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
P-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 00:31:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

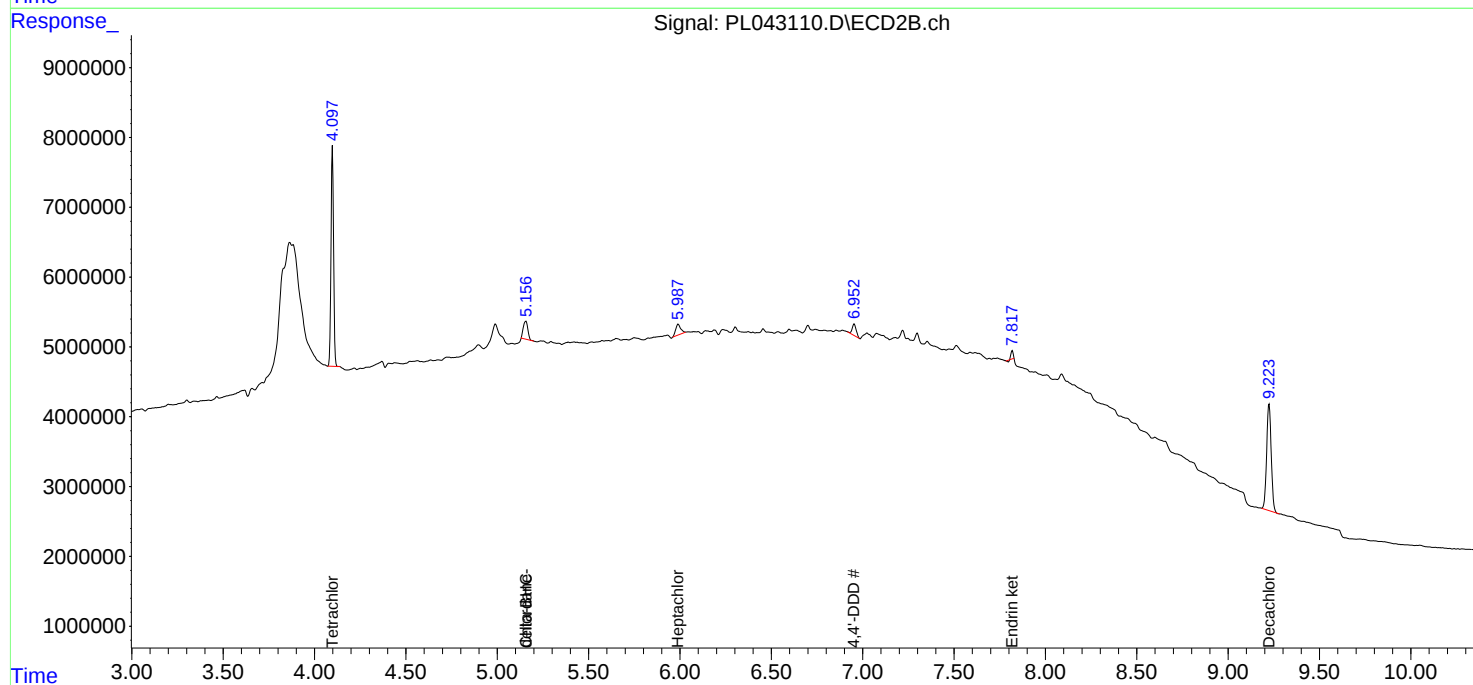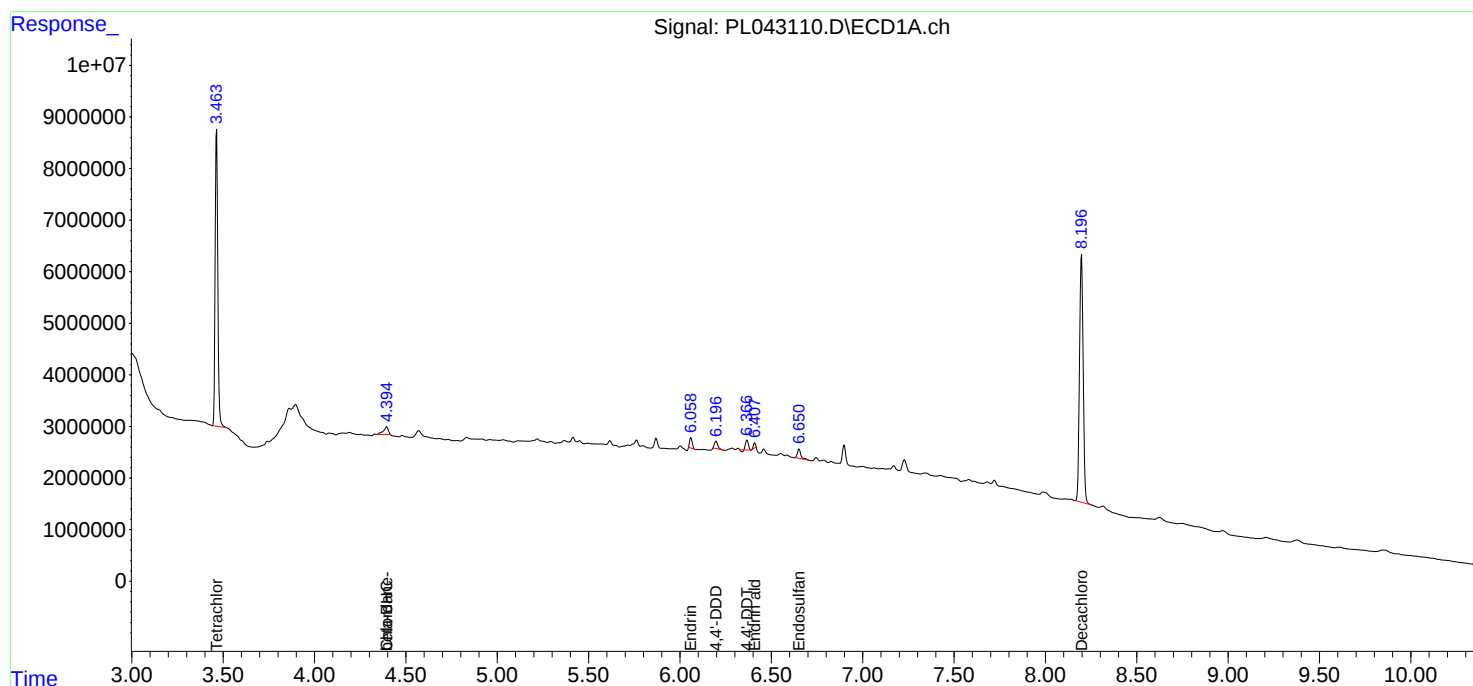


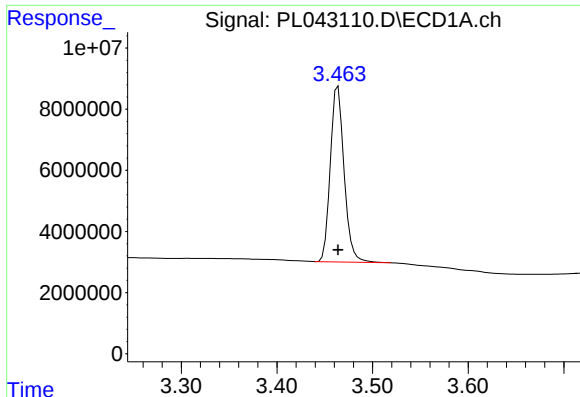

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 57316124
Conc: 9.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-4

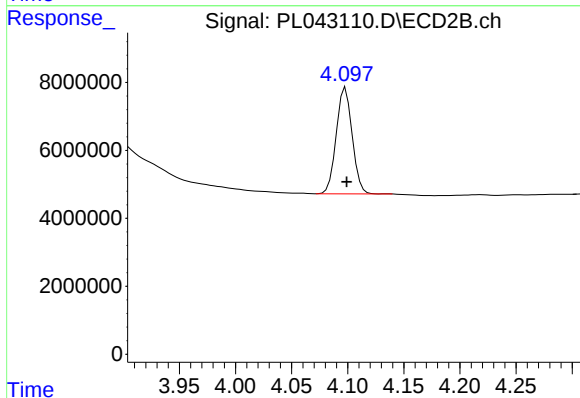


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 30915340
Conc: 10.43 ng/ml

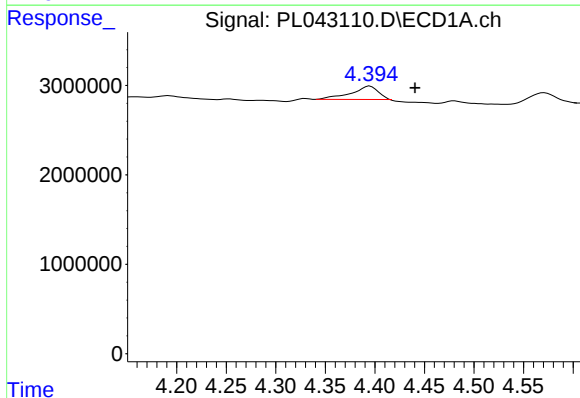


#6 beta-BHC

R.T.: 4.395 min
Delta R.T.: -0.046 min
Response: 2876337
Conc: 0.78 ng/ml

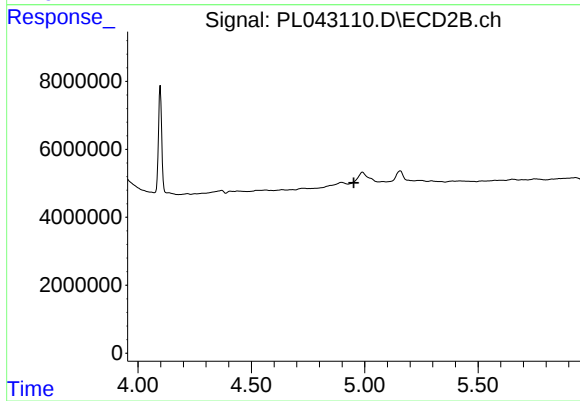

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

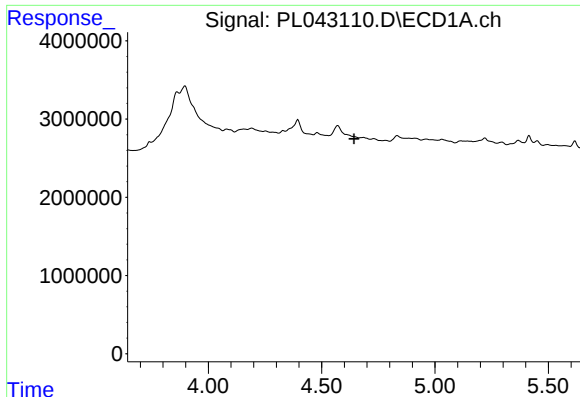

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
P-4

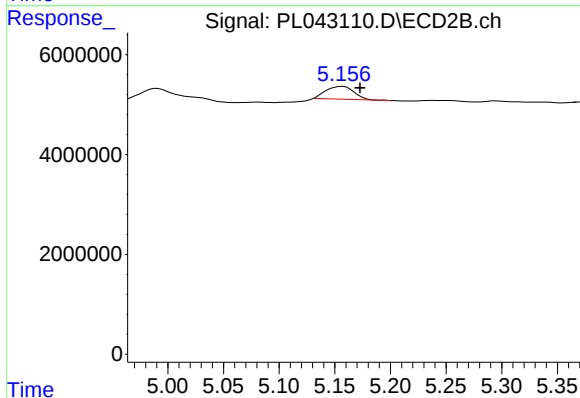


#7 delta-BHC

R.T.: 5.157 min
Delta R.T.: -0.016 min
Response: 4418829
Conc: 1.03 ng/ml

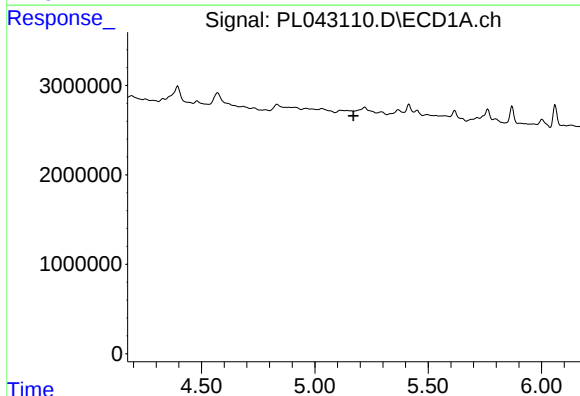


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

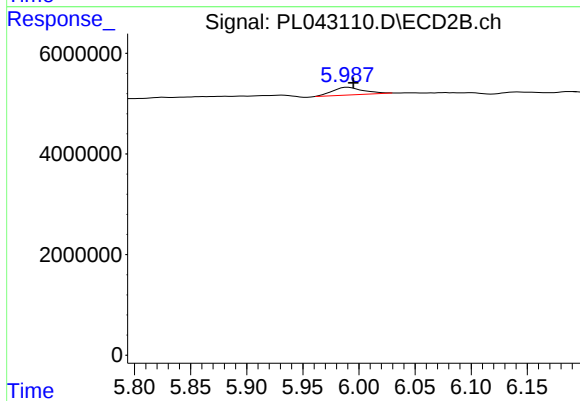

#8 Heptachlor epoxide


R.T.: 5.990 min
Delta R.T.: -0.005 min
Response: 3019545
Conc: 0.80 ng/ml

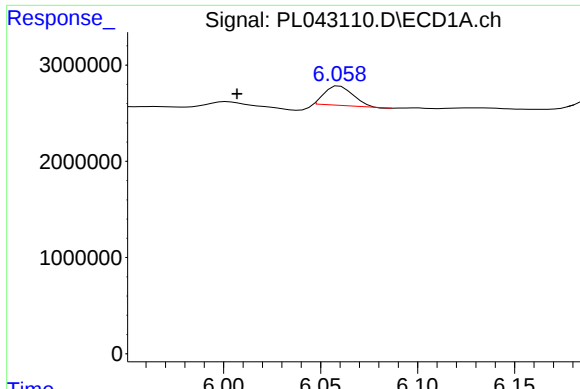

#14 Endrin


R.T.: 6.060 min
Delta R.T.: 0.053 min
Response: 2005493
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-4

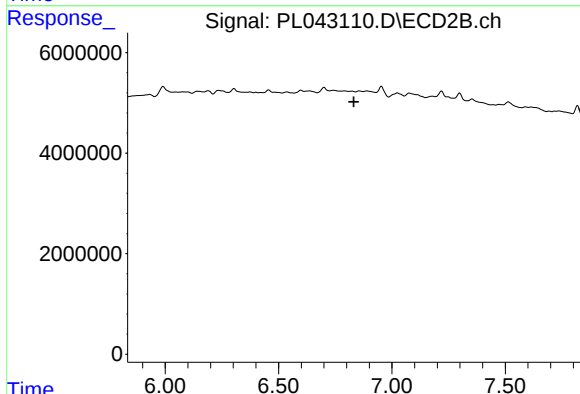


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

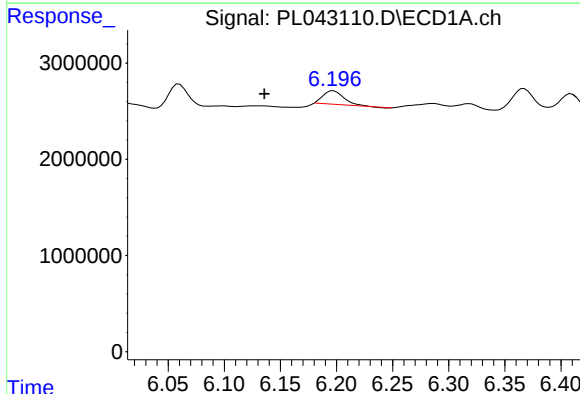


#16 4,4'-DDD

R.T.: 6.197 min
Delta R.T.: 0.062 min
Response: 1696800
Conc: 0.30 ng/ml

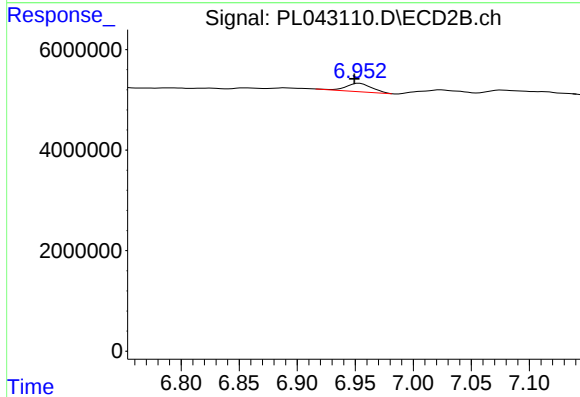

#16 4,4'-DDD


R.T.: 6.953 min
Delta R.T.: 0.004 min
Response: 2422788
Conc: 0.83 ng/ml

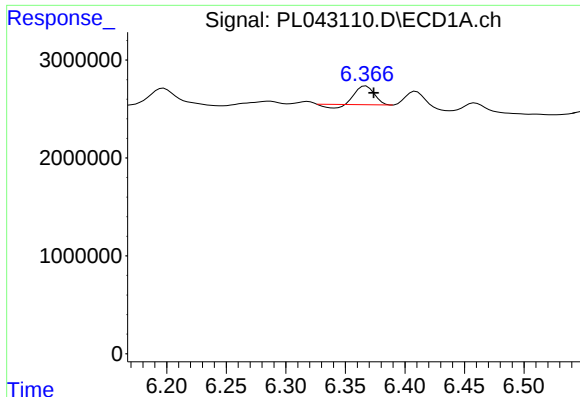

#17 4,4'-DDT


R.T.: 6.367 min
Delta R.T.: -0.007 min
Response: 1916054
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-4

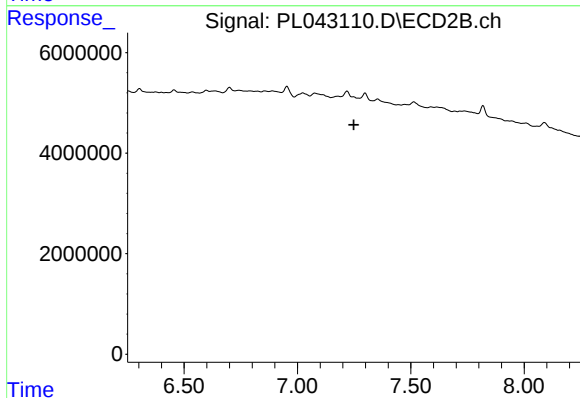


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

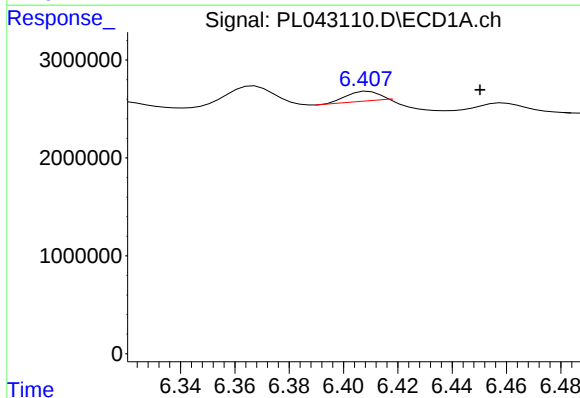


#18 Endrin aldehyde

R.T.: 6.409 min
Delta R.T.: -0.041 min
Response: 822769
Conc: 0.15 ng/ml

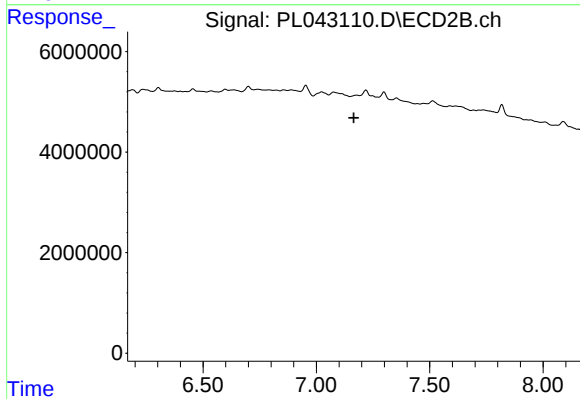

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.165 min
Response: 0
Conc: N.D.

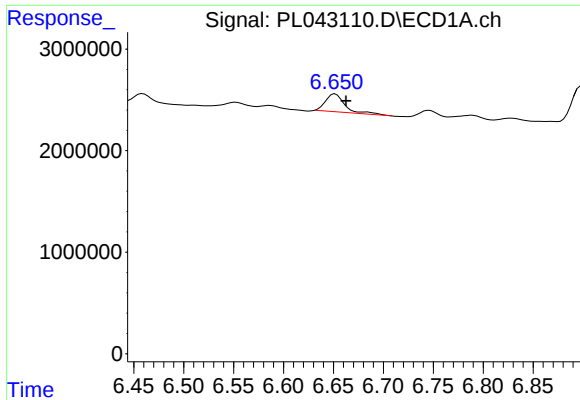

#19 Endosulfan Sulfate


R.T.: 6.652 min
Delta R.T.: -0.011 min
Response: 2323666
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-4

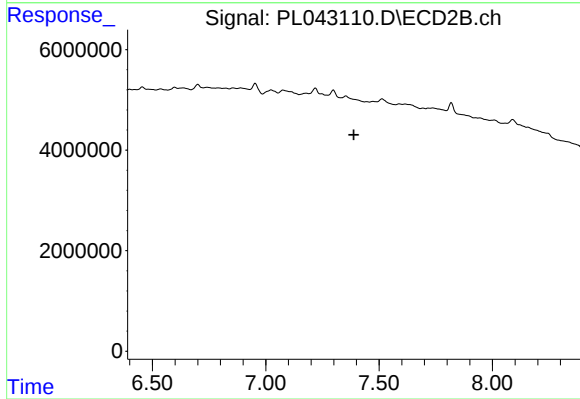


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

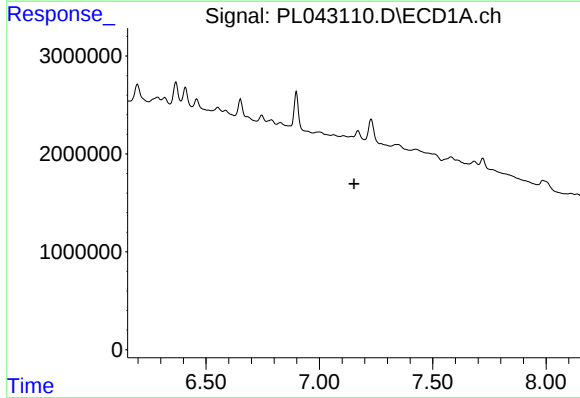


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

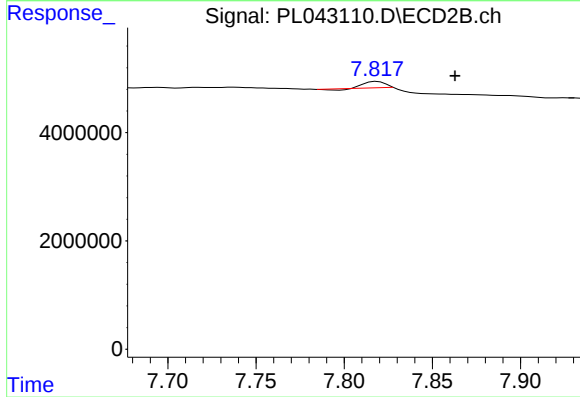

#21 Endrin ketone


R.T.: 7.819 min
Delta R.T.: -0.044 min
Response: 913575
Conc: 0.30 ng/ml

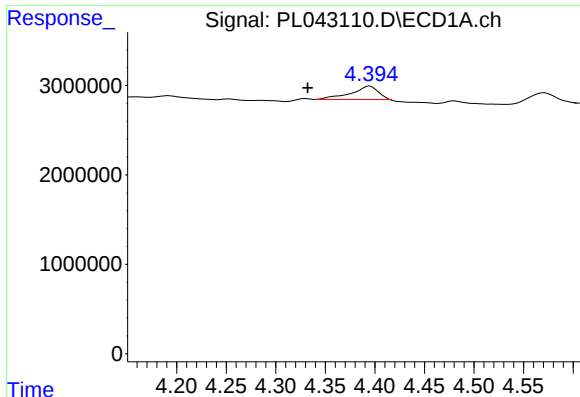

#23 Chlordane-1


R.T.: 4.395 min
Delta R.T.: 0.063 min
Response: 2876337
Conc: 10.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-4

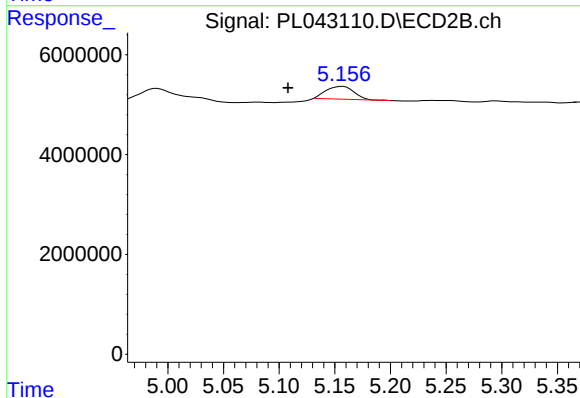


#23 Chlordane-1

R.T.: 5.157 min
Delta R.T.: 0.049 min
Response: 4418829
Conc: 31.27 ng/ml

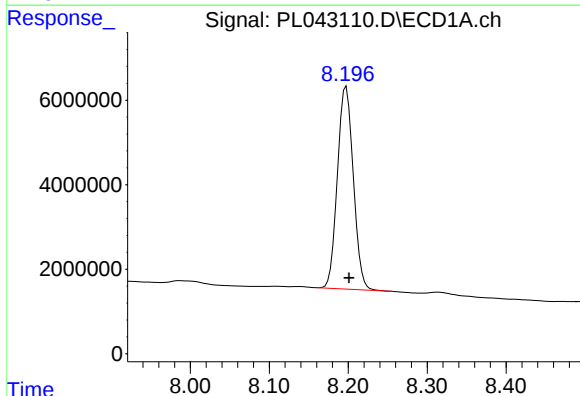

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 67086331
Conc: 10.27 ng/ml

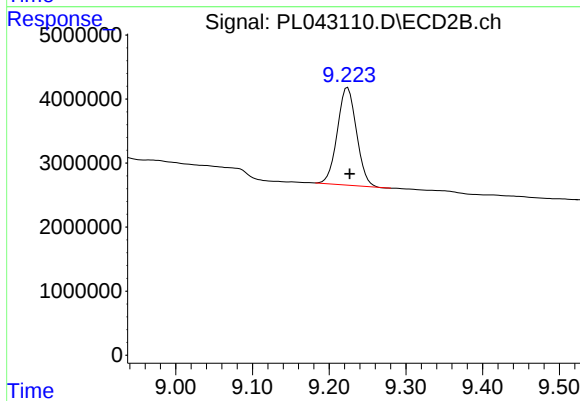

#28 Decachlorobiphenyl

R.T.: 9.224 min
Delta R.T.: -0.003 min
Response: 26414289
Conc: 10.13 ng/ml