

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121319\
 Data File : PL054971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2019 09:27
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 02:22:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.048	267.6E6	60985061	23.004	23.899
28)	SA Decachlor...	8.315	9.146	200.5E6	50712450	20.936	21.153
Target Compounds							
2)	A alpha-BHC	3.976	0.000	10782939	0	0.568	N.D. #
23)	Chlordane-1	4.444f	0.000	2777890	0	7.039	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121319\
Data File : PL054971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2019 09:27
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 02:22:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

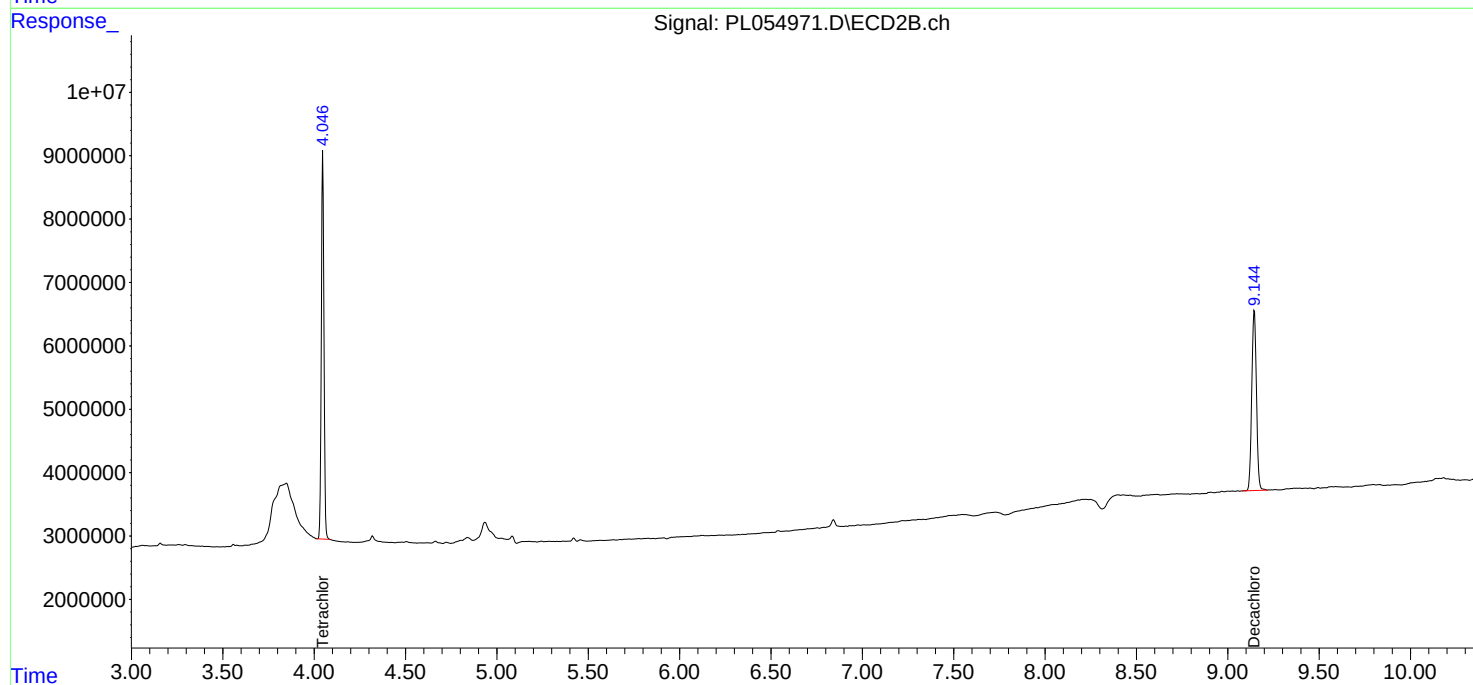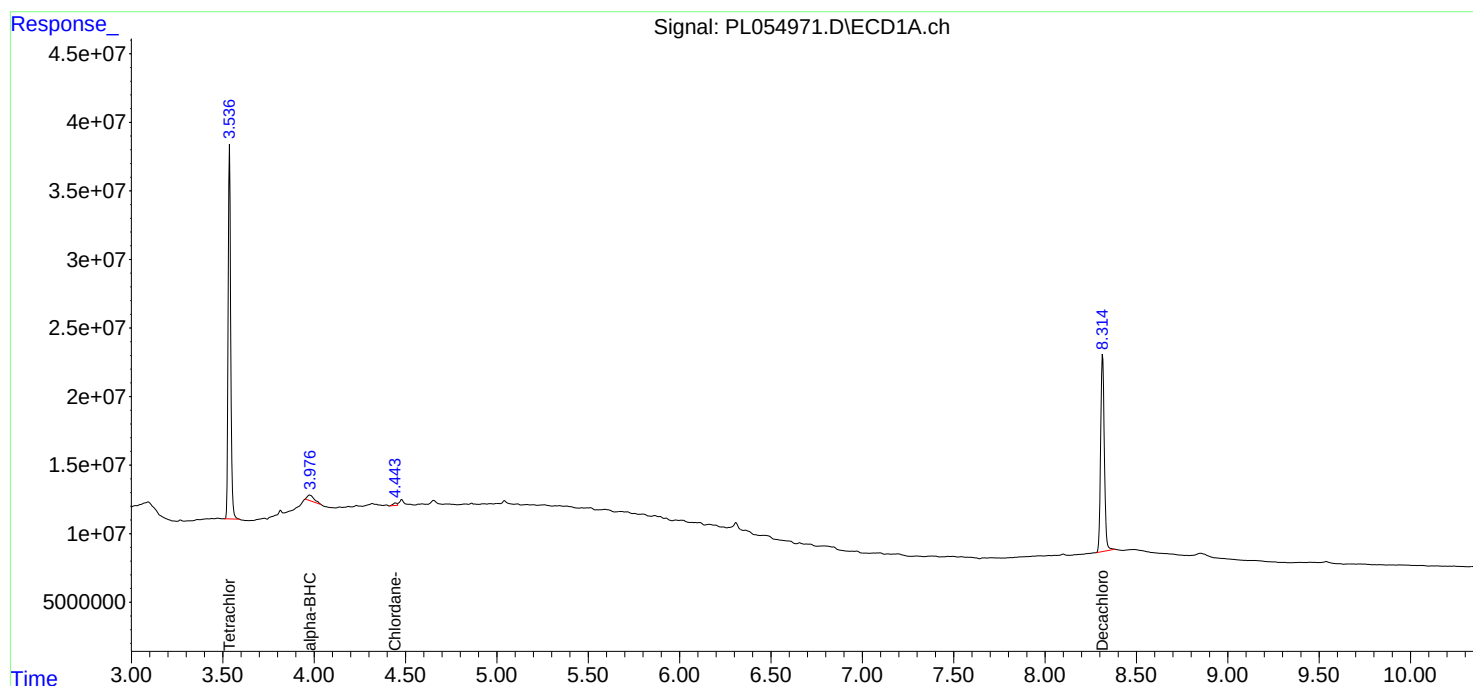


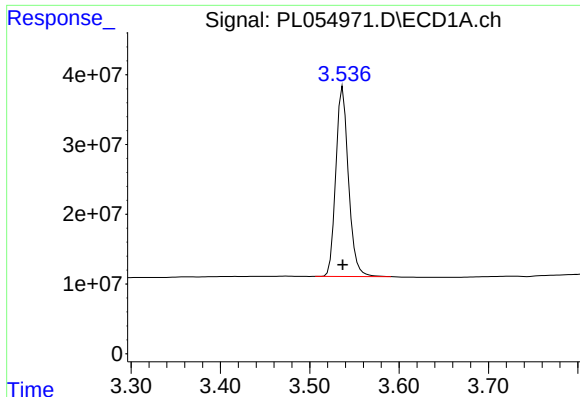

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 267631020
Conc: 23.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

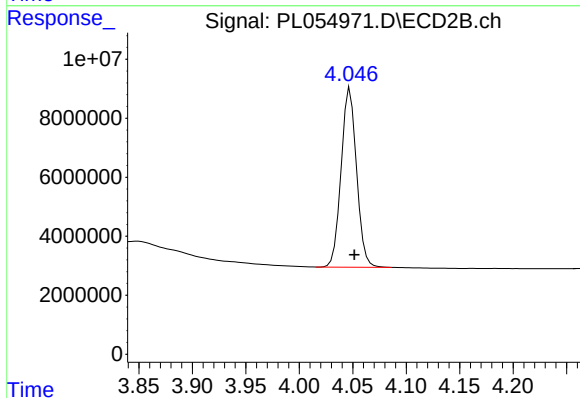


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.004 min
Response: 60985061
Conc: 23.90 ng/ml

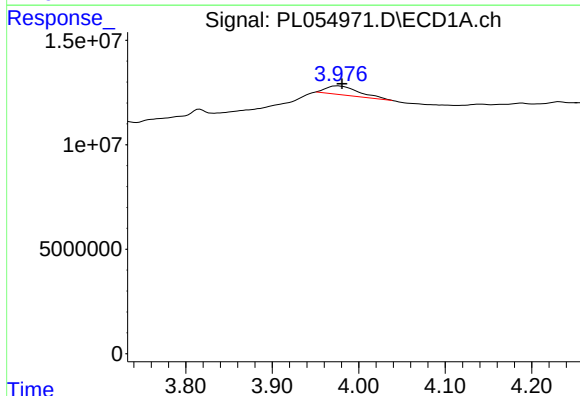


#2 alpha-BHC

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 10782939
Conc: 0.57 ng/ml

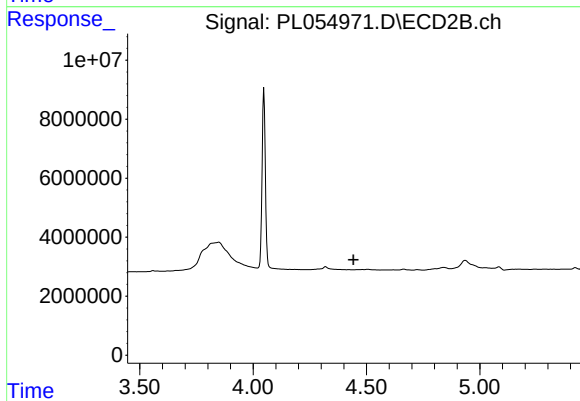

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.443 min
Response: 0
Conc: N.D.

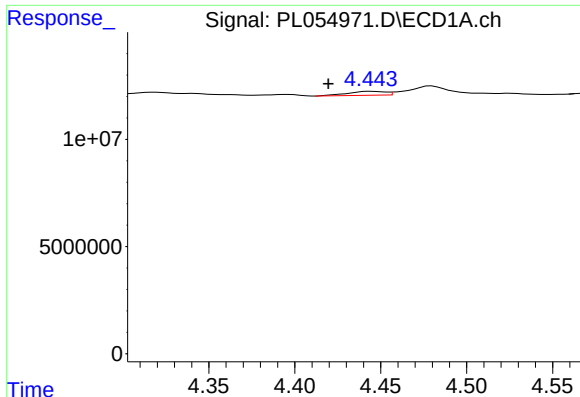

#23 Chlordane-1


R.T.: 4.444 min
Delta R.T.: 0.025 min
Response: 2777890
Conc: 7.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

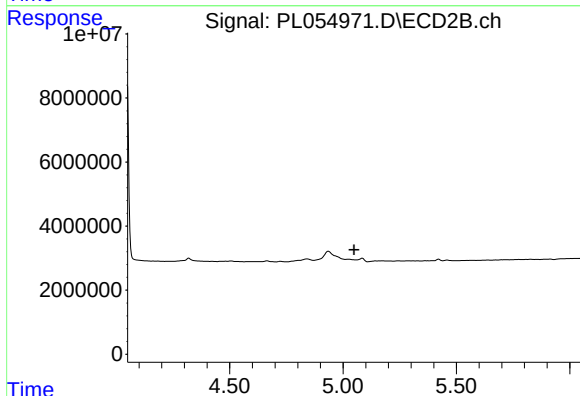


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

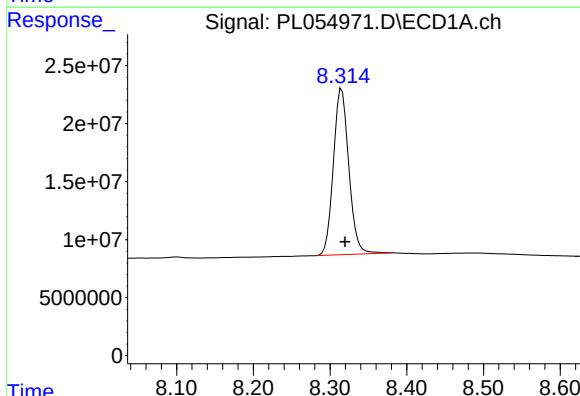

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.004 min
Response: 200485364
Conc: 20.94 ng/ml

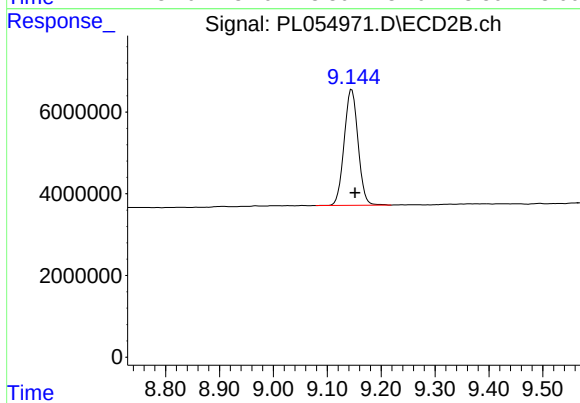

#28 Decachlorobiphenyl

R.T.: 9.146 min
Delta R.T.: -0.006 min
Response: 50712450
Conc: 21.15 ng/ml