

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 10:53
 Operator : DD\AJ
 Sample : L5016-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-06-121020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:25:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	7201417	12325823	4.232	3.933
28)	SA Decachlor...	8.125	8.989	7632634	9930470	3.790	3.943
Target Compounds							
6)	B beta-BHC	0.000	4.798	0	26531036	N.D.	13.356 #
7)	B delta-BHC	0.000	5.004	0	6214876	N.D.	1.536 #
8)	B Heptachlo...	0.000	5.826	0	8508859	N.D.	2.349 #
19)	B Endosulfa...	6.598	0.000	8433306	0	4.918	N.D. #
23)	Chlordane-1	0.000	4.927	0	6874863	N.D.	59.918 #
24)	Chlordane-2	4.773	0.000	13550820	0	215.802	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 10:53
Operator : DD\AJ
Sample : L5016-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-06-121020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:25:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

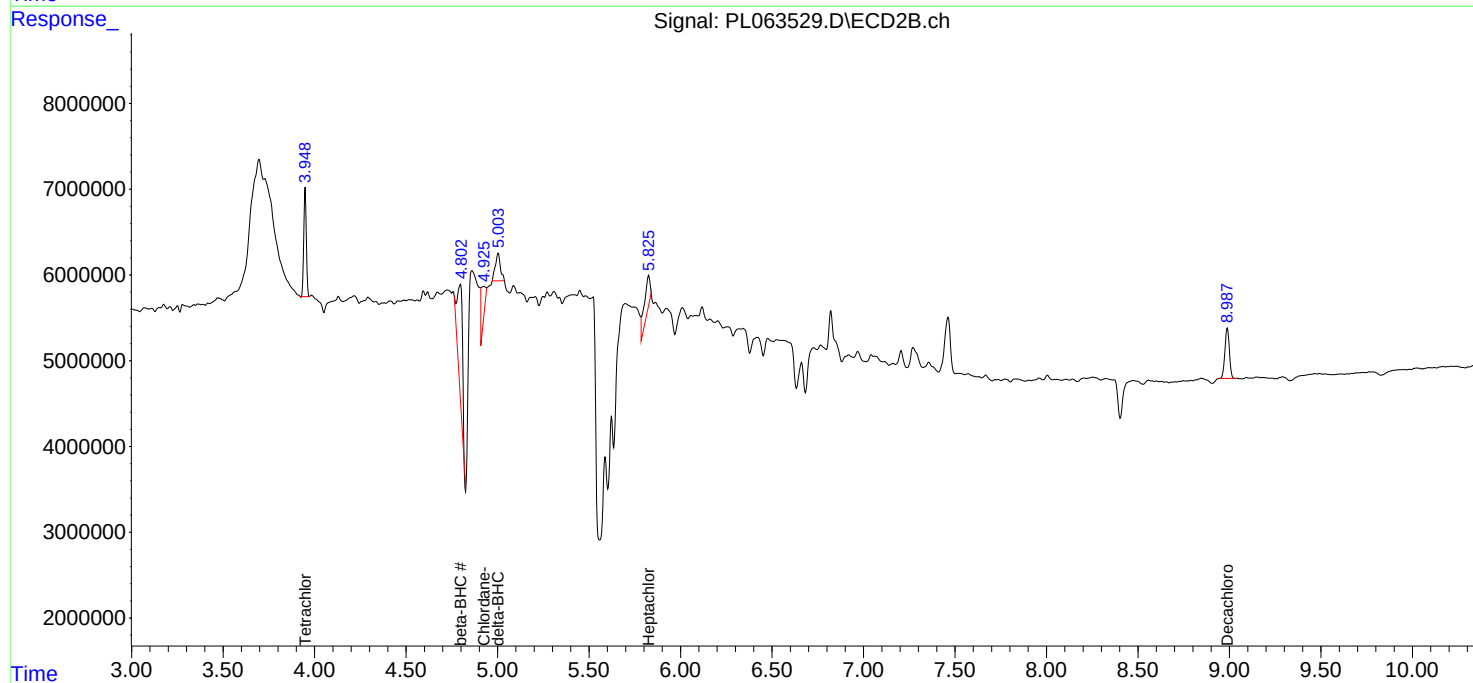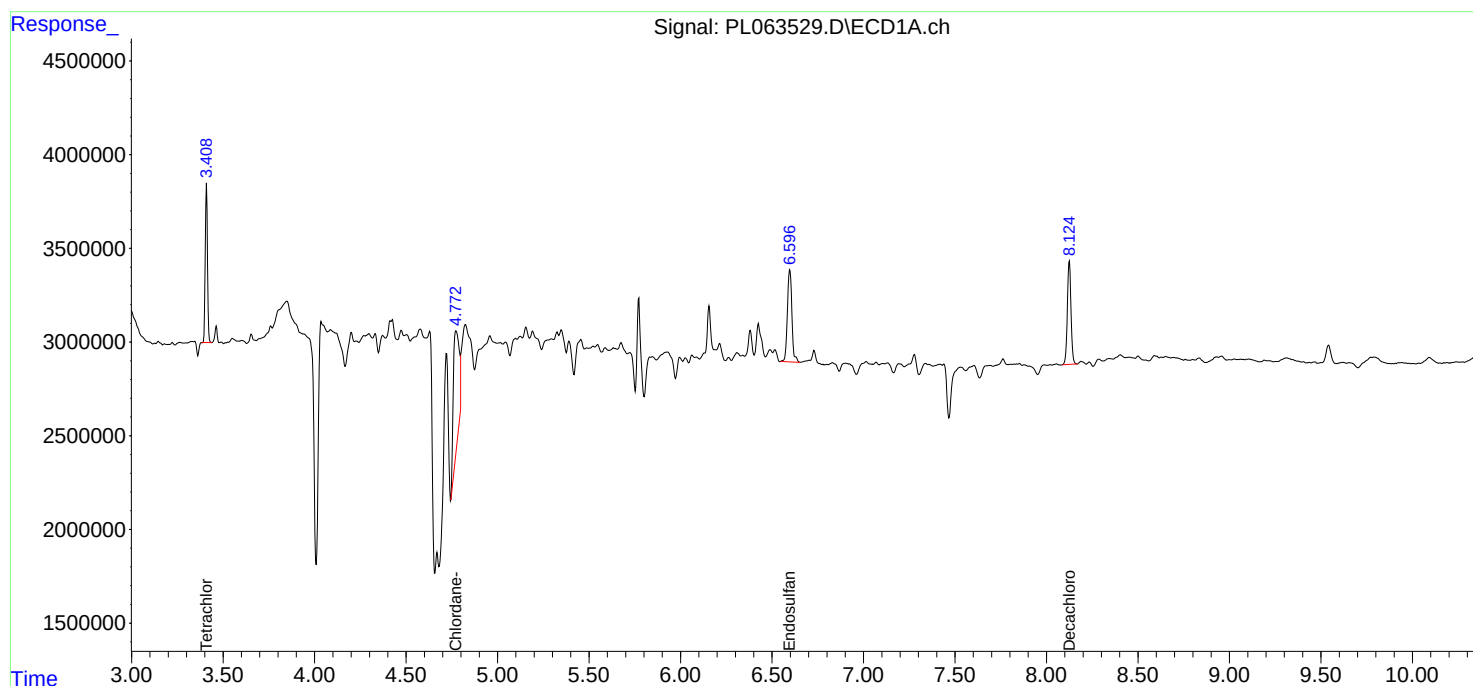


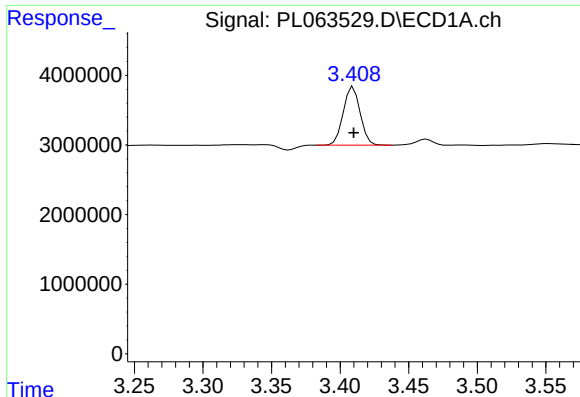

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 7201417
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-121020

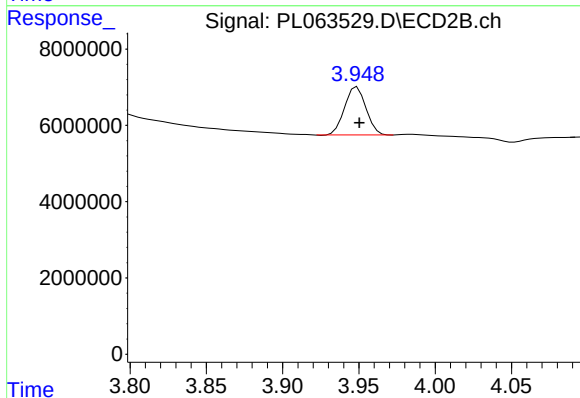


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 12325823
Conc: 3.93 ng/ml

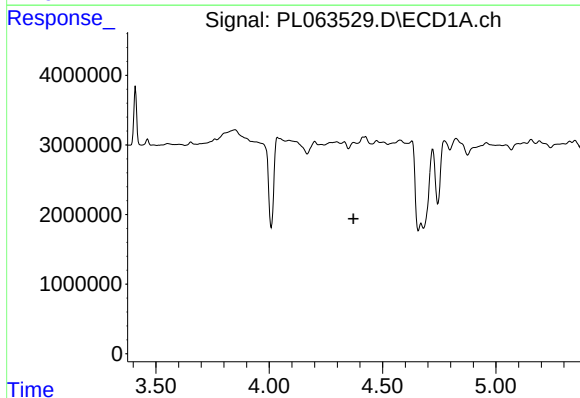


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

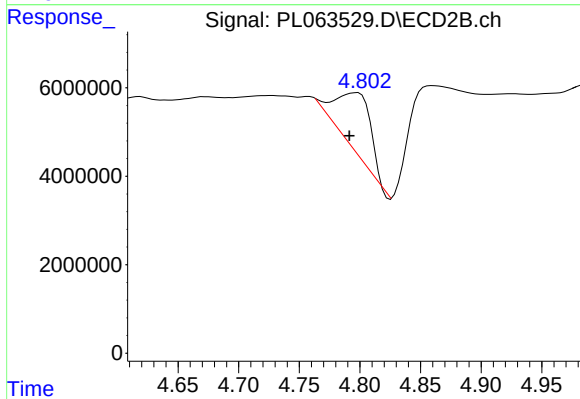

#6 beta-BHC


R.T.: 4.798 min
Delta R.T.: 0.007 min
Response: 26531036
Conc: 13.36 ng/ml

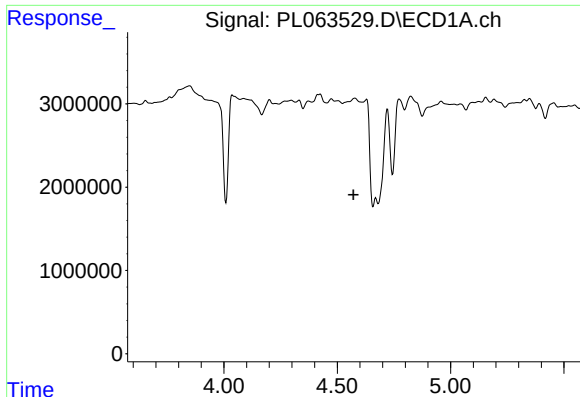

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-06-121020

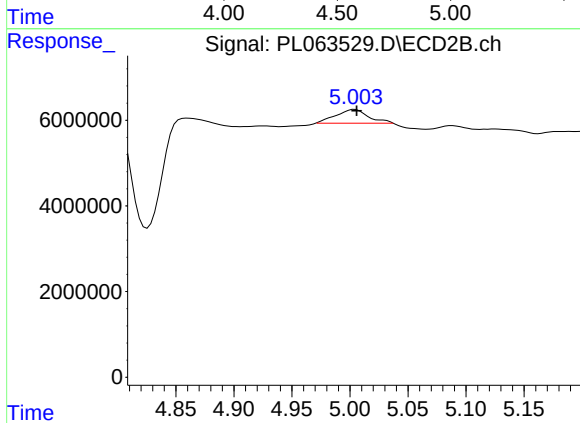


#7 delta-BHC

R.T.: 5.004 min
Delta R.T.: -0.001 min
Response: 6214876
Conc: 1.54 ng/ml

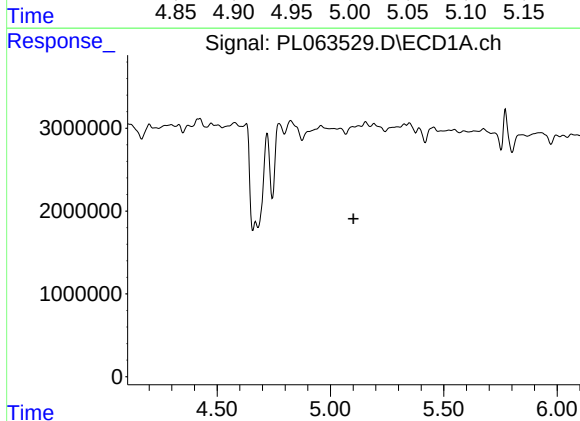


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

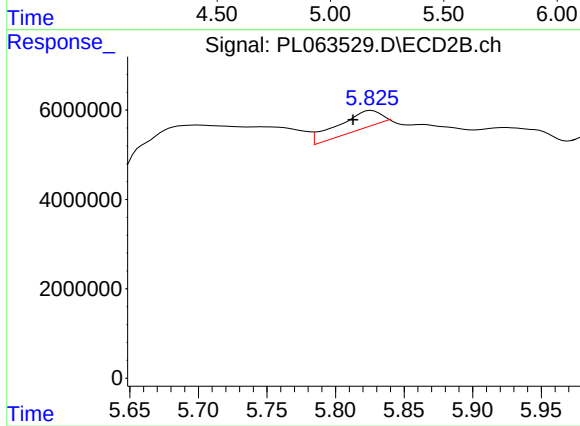

#8 Heptachlor epoxide


R.T.: 5.826 min
Delta R.T.: 0.014 min
Response: 8508859
Conc: 2.35 ng/ml

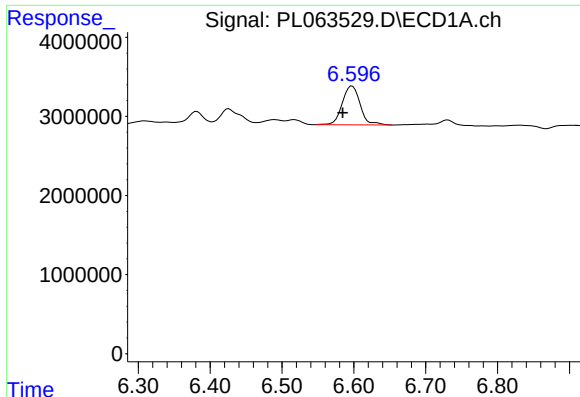

#19 Endosulfan Sulfate


R.T.: 6.598 min
Delta R.T.: 0.013 min
Response: 8433306
Conc: 4.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-121020

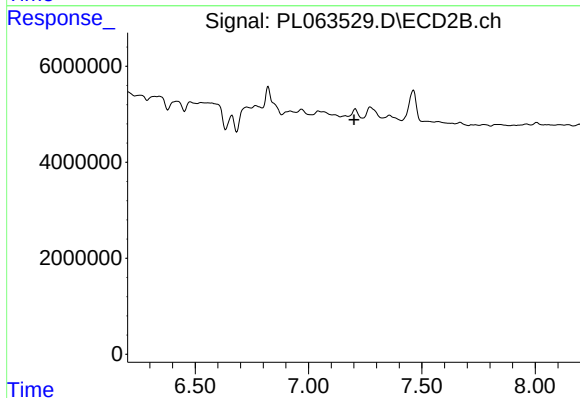


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

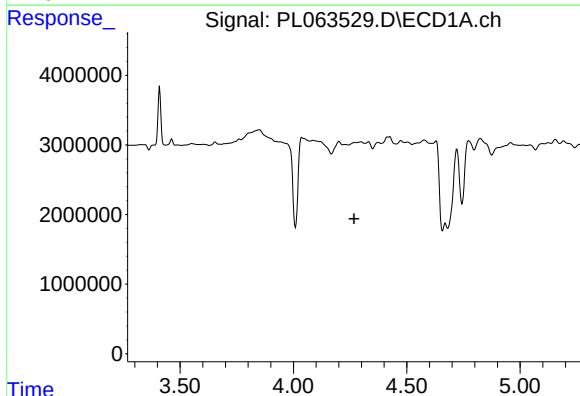


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.267 min
Response: 0
Conc: N.D.

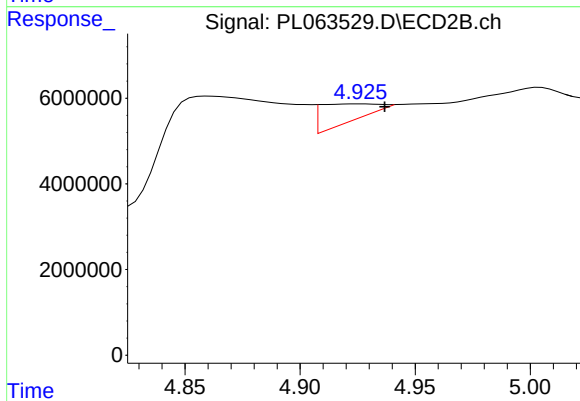

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: -0.010 min
Response: 6874863
Conc: 59.92 ng/ml

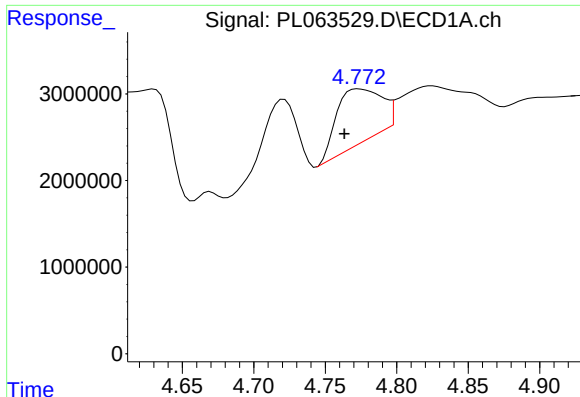

#24 Chlordane-2


R.T.: 4.773 min
Delta R.T.: 0.010 min
Response: 13550820
Conc: 215.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-121020

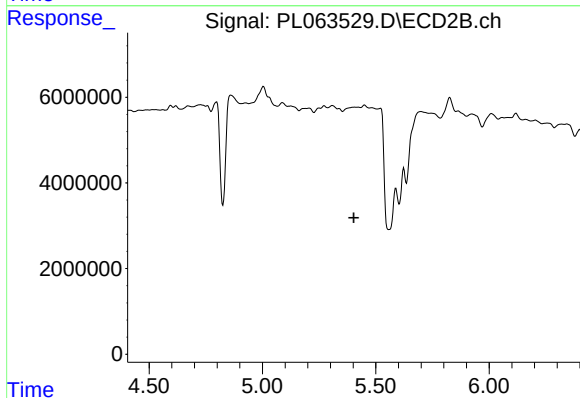


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

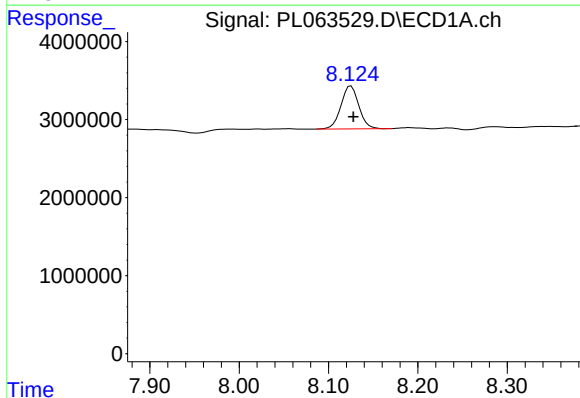

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 7632634
Conc: 3.79 ng/ml

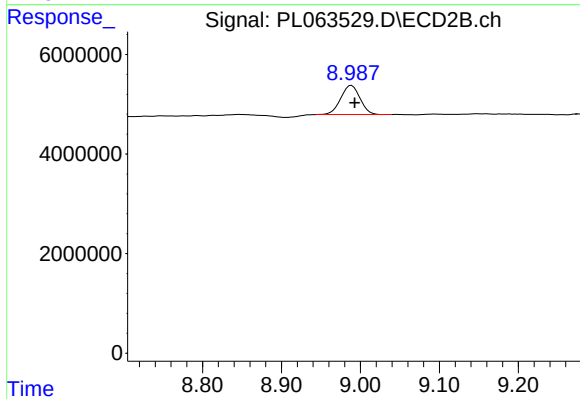

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 9930470
Conc: 3.94 ng/ml