

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 12:48
 Operator : DD\AJ
 Sample : L5033-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:27:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	36487277	68221823	21.442	21.767
28)	SA Decachlor...	8.124	8.989	33634288	46639704	16.701	18.520
Target Compounds							
7)	B delta-BHC	0.000	5.001	0	5664880	N.D.	1.400 #
8)	B Heptachlo...	0.000	5.825	0	4953938	N.D.	1.368 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 12:48
Operator : DD\AJ
Sample : L5033-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-47

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:27:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

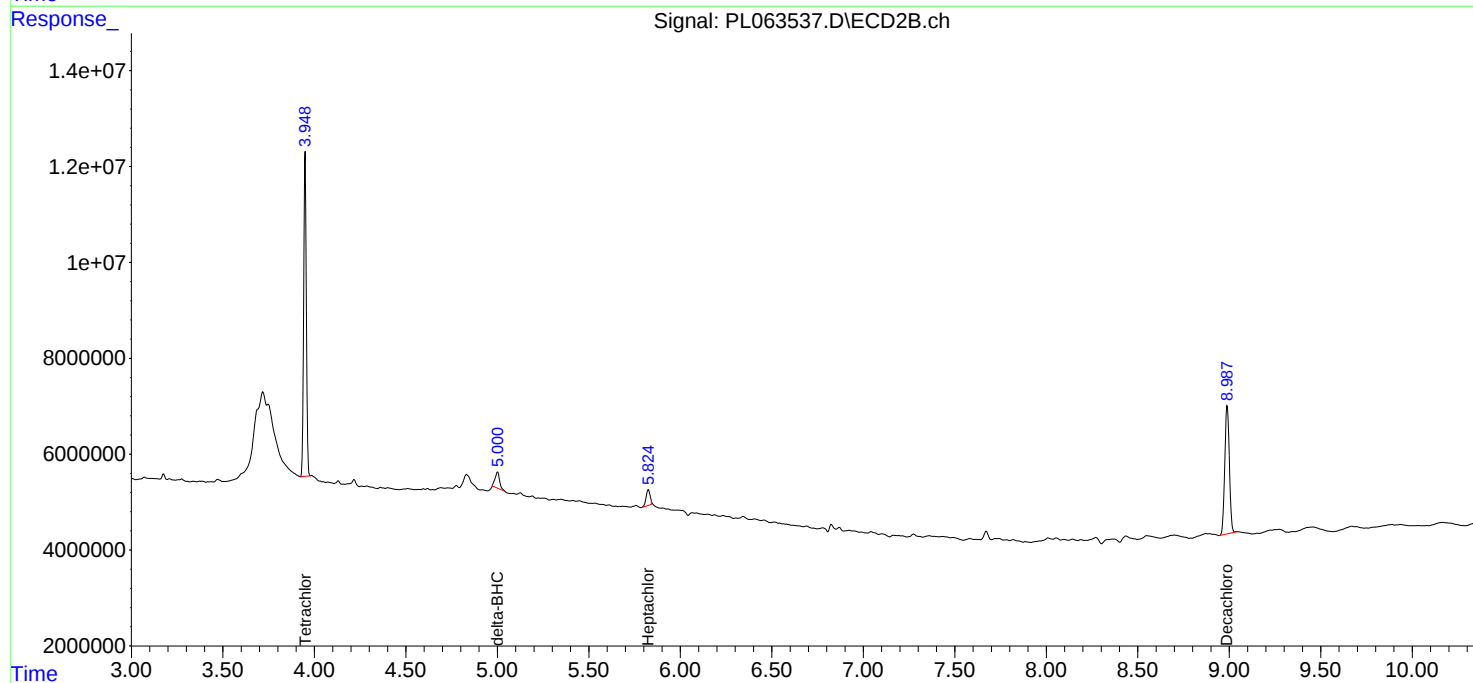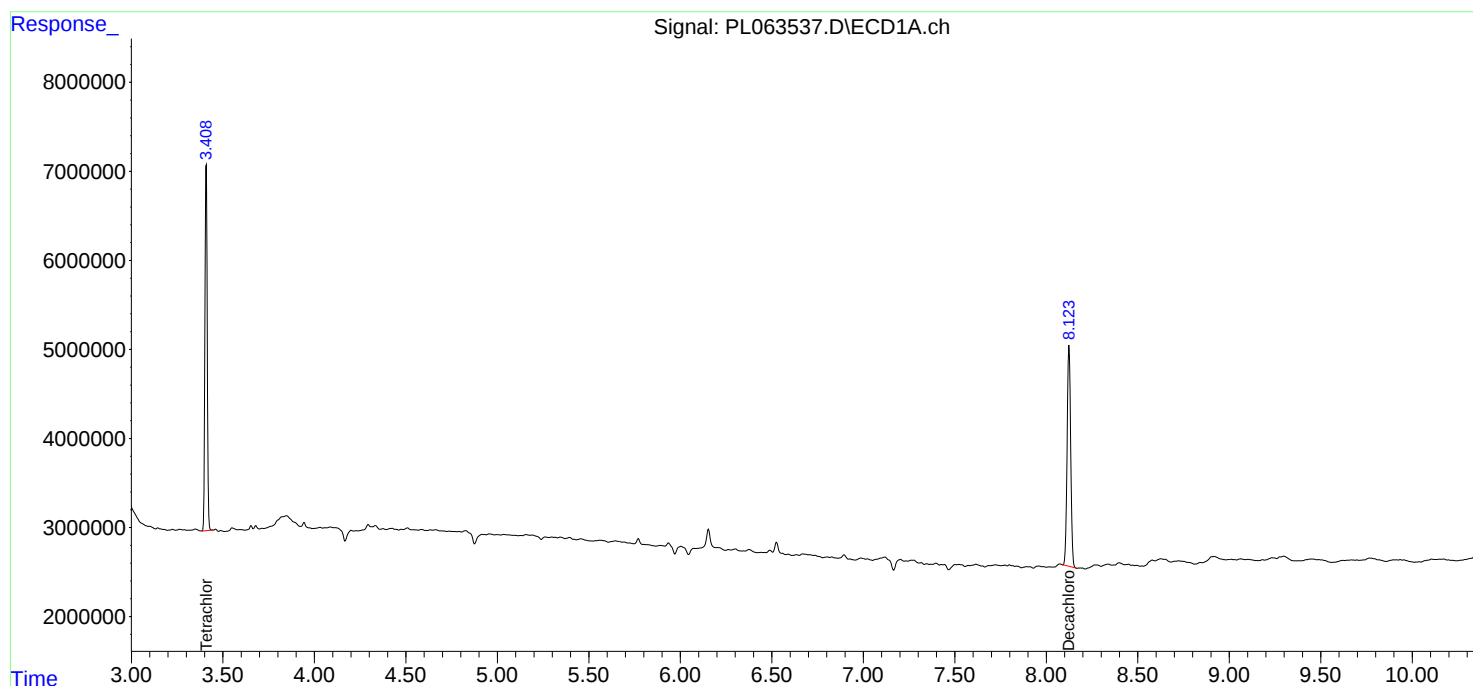


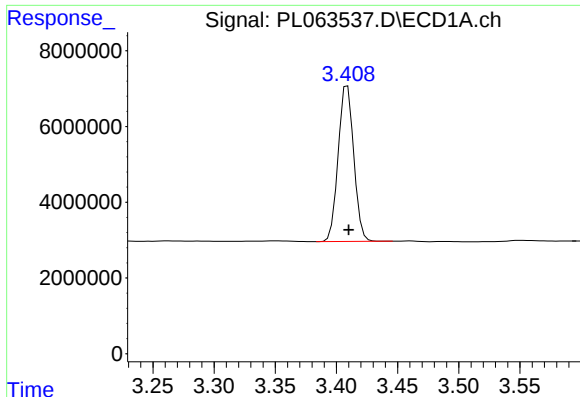

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 36487277
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-47

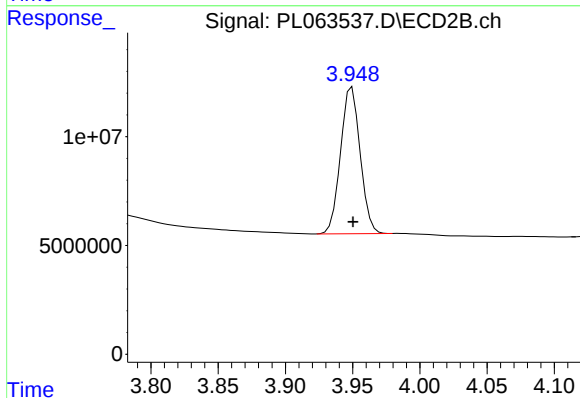


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 68221823
Conc: 21.77 ng/ml

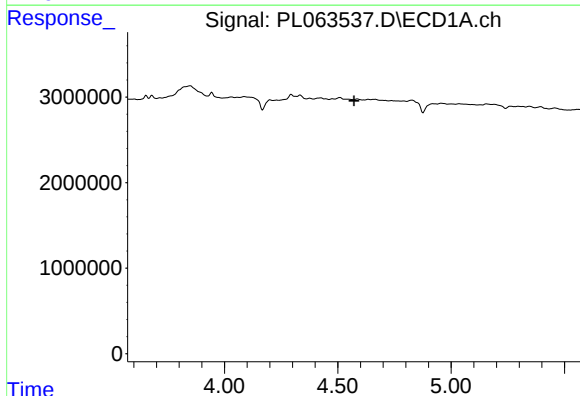


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

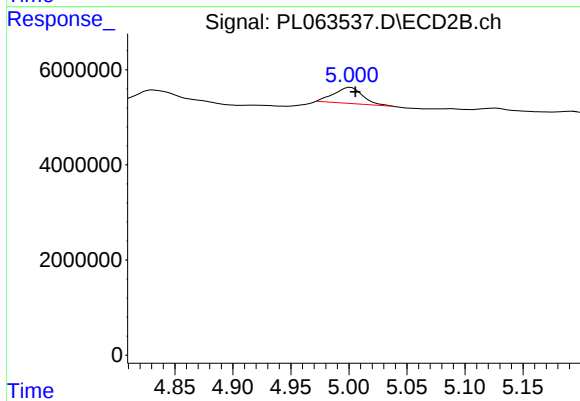

#7 delta-BHC


R.T.: 5.001 min
Delta R.T.: -0.004 min
Response: 5664880
Conc: 1.40 ng/ml

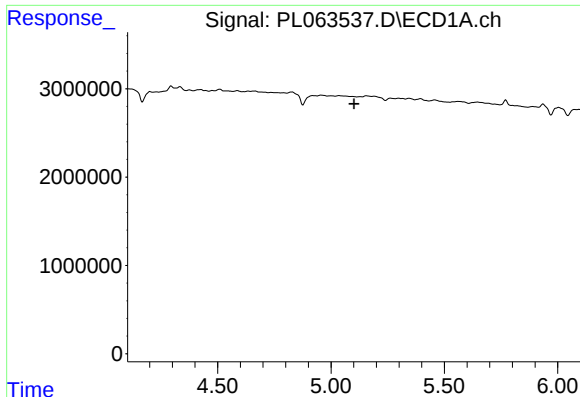

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-47

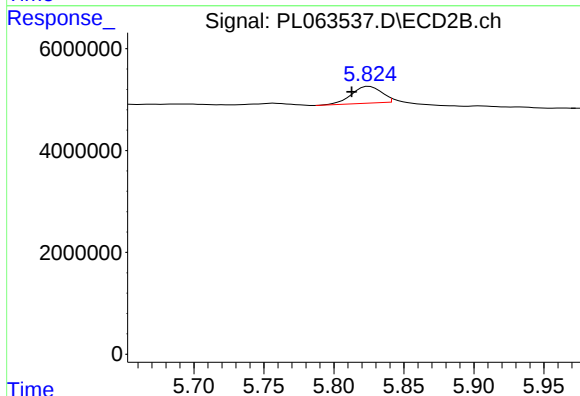


#8 Heptachlor epoxide

R.T.: 5.825 min
Delta R.T.: 0.013 min
Response: 4953938
Conc: 1.37 ng/ml

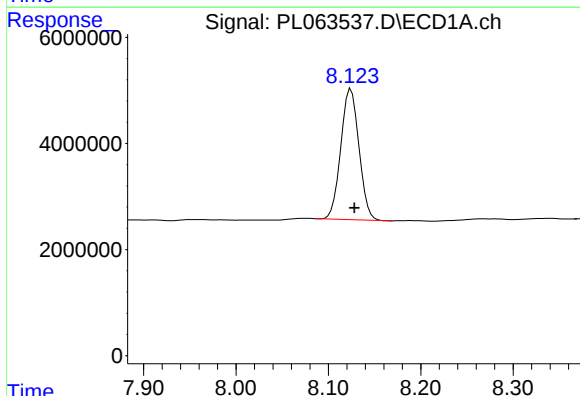

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 33634288
Conc: 16.70 ng/ml

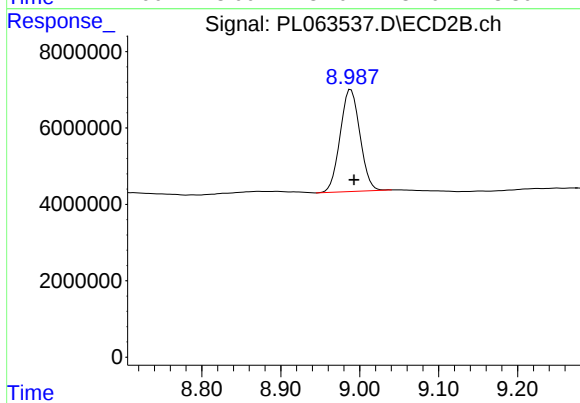

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 46639704
Conc: 18.52 ng/ml