

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 18:18
 Operator : DD\AJ
 Sample : L5066-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:33:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	18031215	28379238	10.596	9.055
28)	SA Decachlor...	8.125	8.990	15273940	19456351	7.584	7.726
Target Compounds							
2)	A alpha-BHC	0.000	4.357f	0	4062615	N.D.	0.858 #
6)	B beta-BHC	0.000	4.813f	0	289385	N.D.	0.146 #
7)	B delta-BHC	0.000	5.004	0	4847847	N.D.	1.198 #
8)	B Heptachlo...	0.000	5.826	0	4035753	N.D.	1.114 #
23)	Chlordane-1	4.266	0.000	3361321	0	61.487	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 18:18
Operator : DD\AJ
Sample : L5066-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:33:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

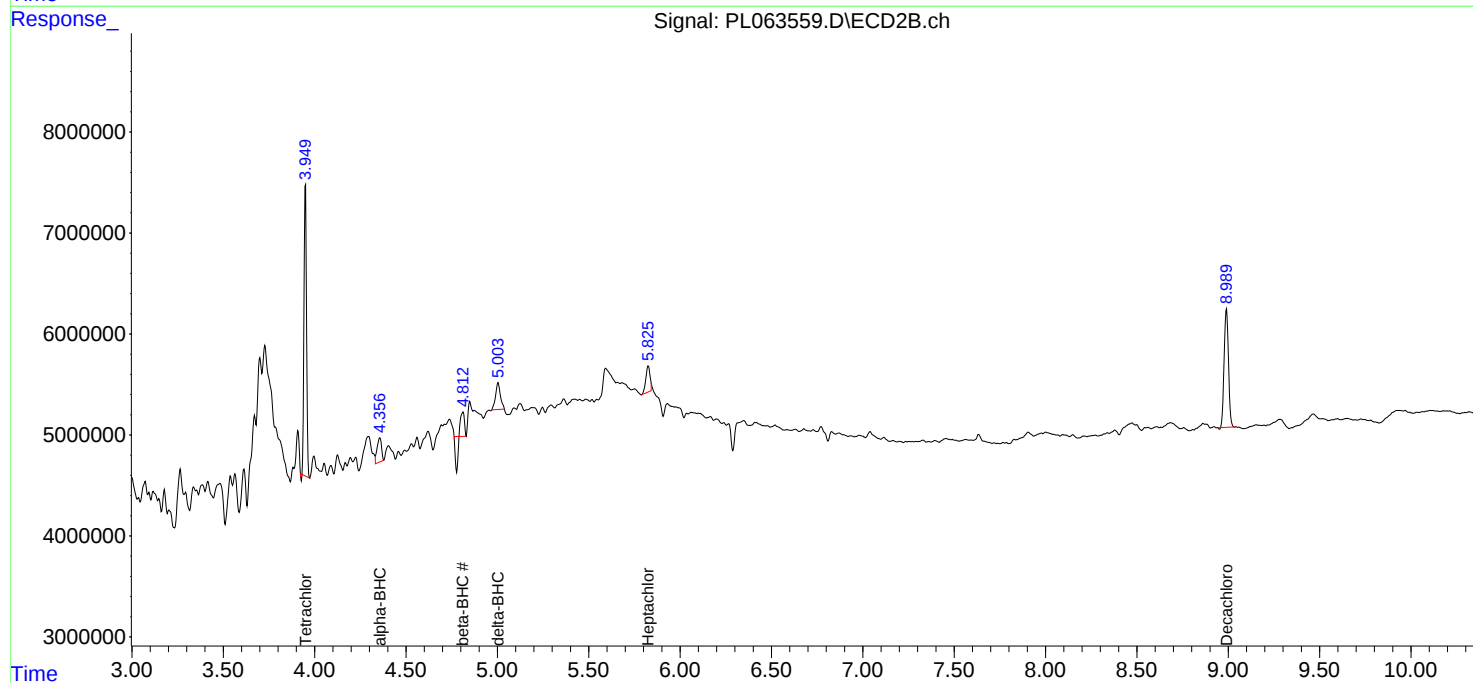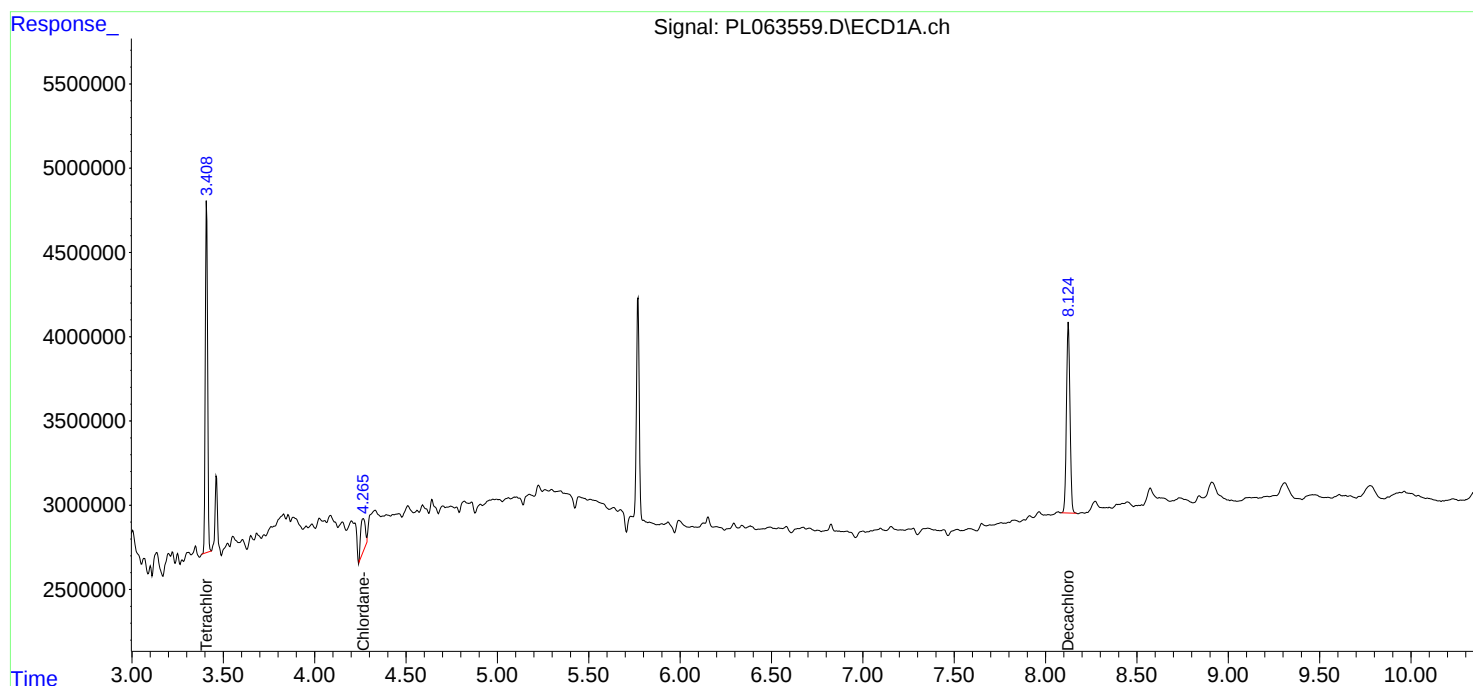


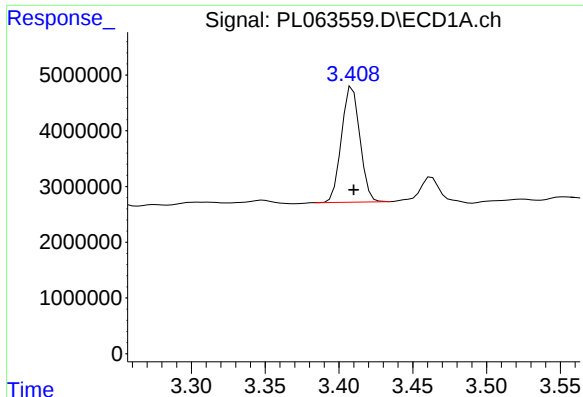

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 18031215
Conc: 10.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

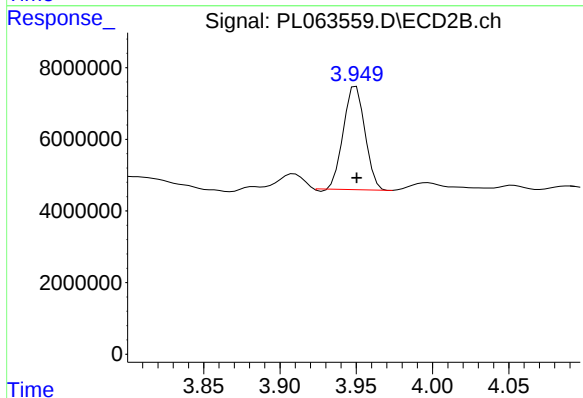


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 28379238
Conc: 9.05 ng/ml

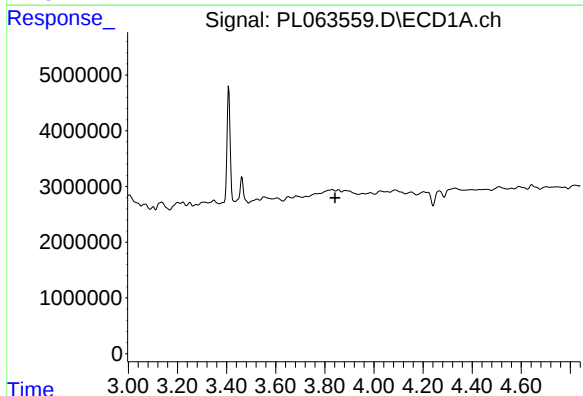


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.842 min
Response: 0
Conc: N.D.

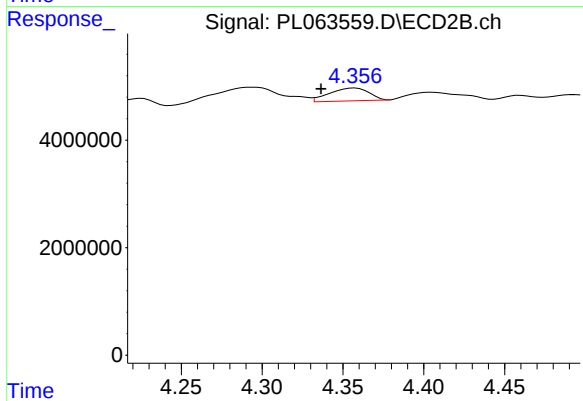

#2 alpha-BHC


R.T.: 4.357 min
Delta R.T.: 0.021 min
Response: 4062615
Conc: 0.86 ng/ml

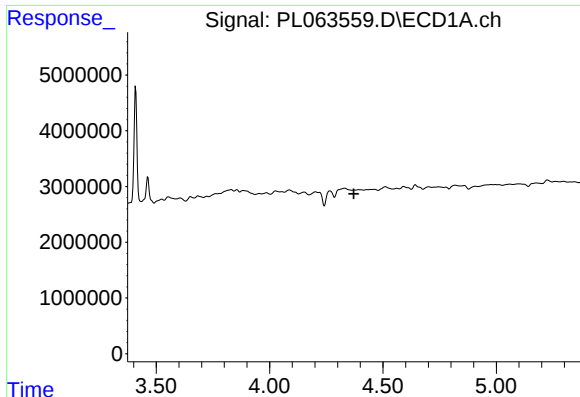

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

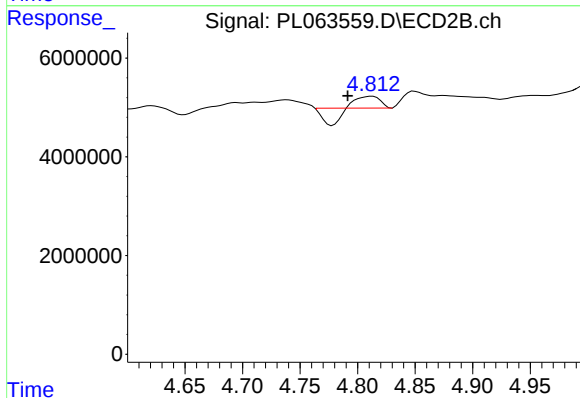


#6 beta-BHC

R.T.: 4.813 min
Delta R.T.: 0.021 min
Response: 289385
Conc: 0.15 ng/ml

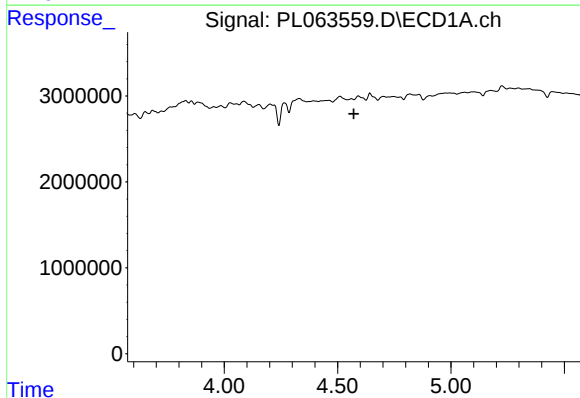


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

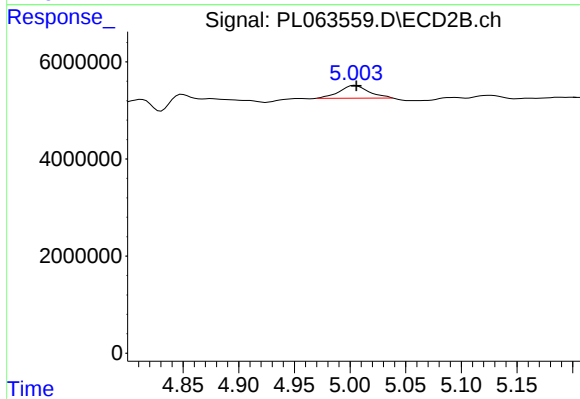

#7 delta-BHC


R.T.: 5.004 min
Delta R.T.: -0.001 min
Response: 4847847
Conc: 1.20 ng/ml

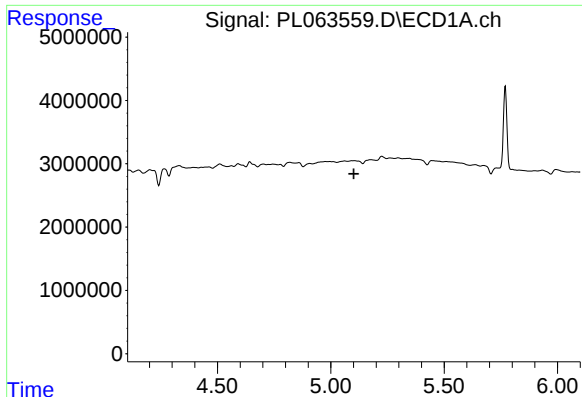

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

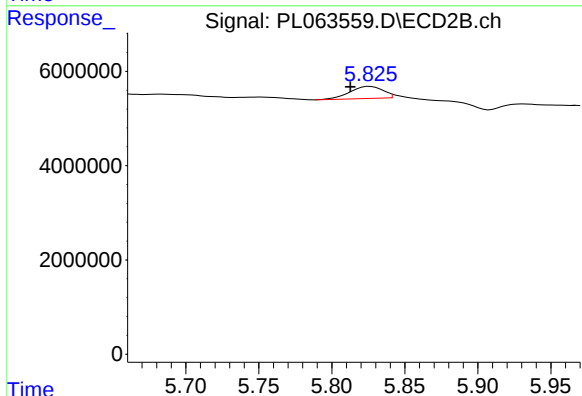


#8 Heptachlor epoxide

R.T.: 5.826 min
Delta R.T.: 0.014 min
Response: 4035753
Conc: 1.11 ng/ml

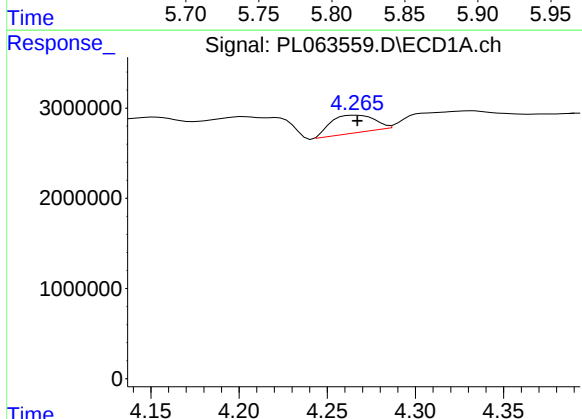


#23 Chlordane-1

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 3361321
Conc: 61.49 ng/ml

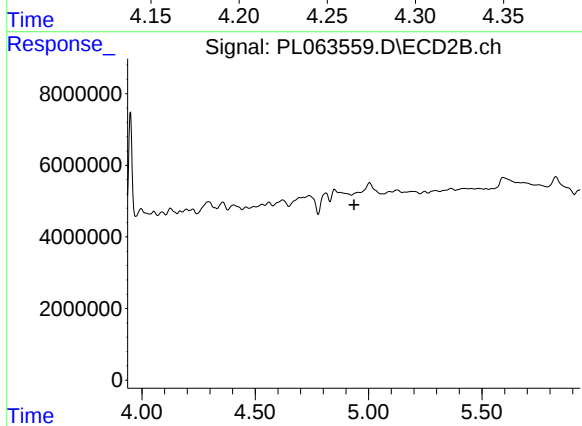

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.937 min
Response: 0
Conc: N.D.

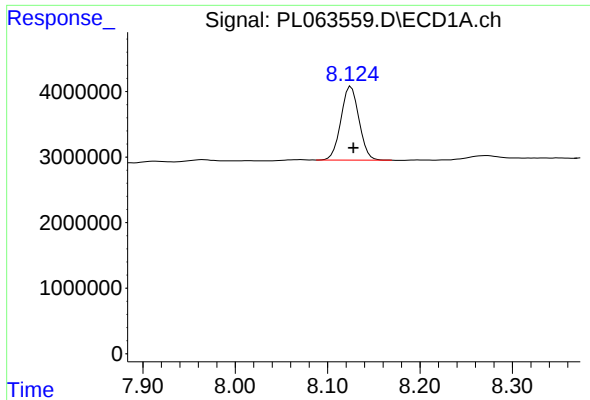

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 15273940
Conc: 7.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

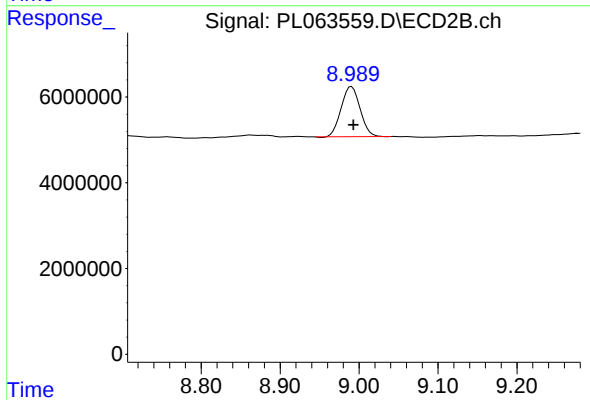

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 19456351
Conc: 7.73 ng/ml