

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 18:46
 Operator : DD\AJ
 Sample : L5066-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:33:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	17118658	31371824	10.060	10.010
28)	SA Decachlor...	8.126	8.991	14172298	19091393	7.037	7.581
Target Compounds							
4)	MA Heptachlor	0.000	5.146f	0	2551286	N.D.	0.621 #
5)	MB Aldrin	0.000	5.404f	0	5835948	N.D.	1.508 #
8)	B Heptachlo...	0.000	5.827	0	1706336	N.D.	0.471 #
10)	B gamma-Chl...	5.349f	6.046	4821062	4584479	2.592	1.292 #
11)	B alpha-Chl...	5.384	6.120	5268877	14546532	2.834	4.104 #
23)	Chlordane-1	4.267	4.936	2328281	3606045	42.590	31.429 #
24)	Chlordane-2	0.000	5.404	0	5835948	N.D.	46.242 #
25)	Chlordane-3	5.349f	6.046	4821062	4584479	27.826	9.949 #
26)	Chlordane-4	5.384	6.120	5268877	14546532	36.021	26.532 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 18:46
Operator : DD\AJ
Sample : L5066-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:33:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

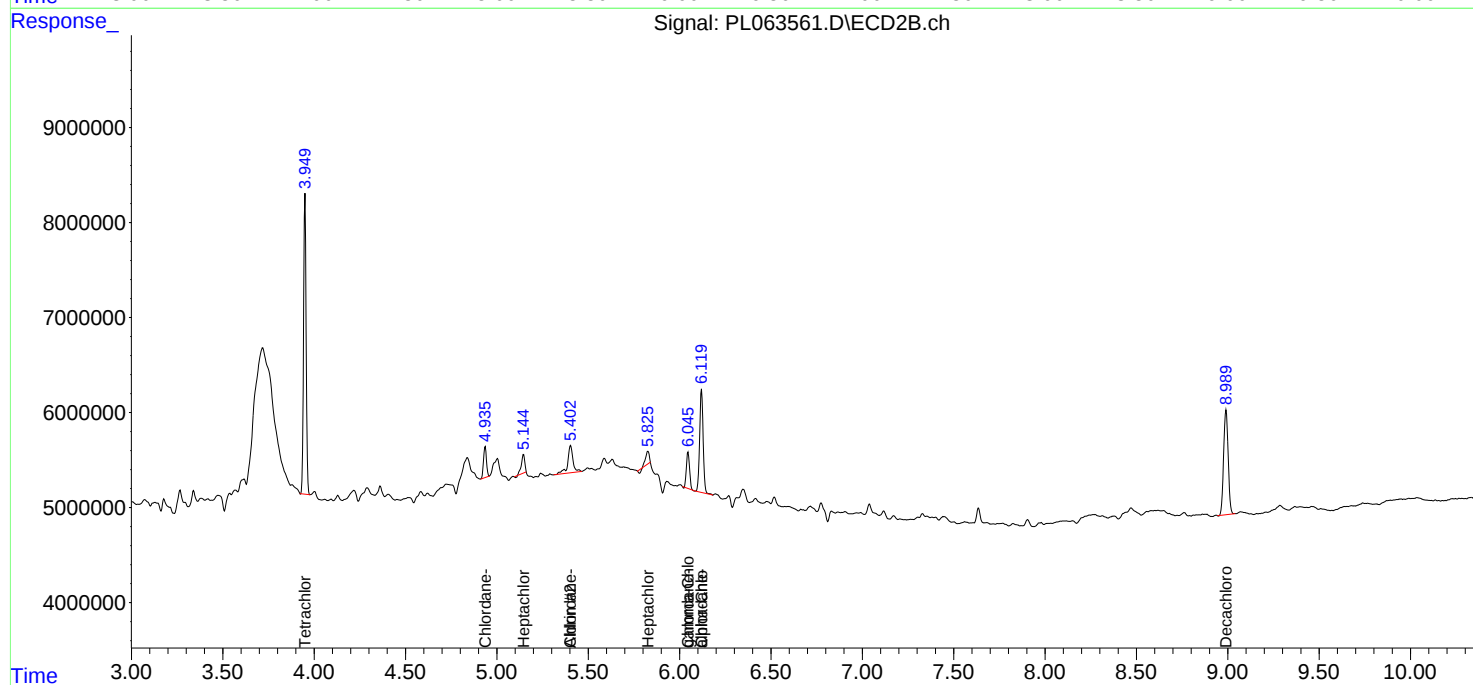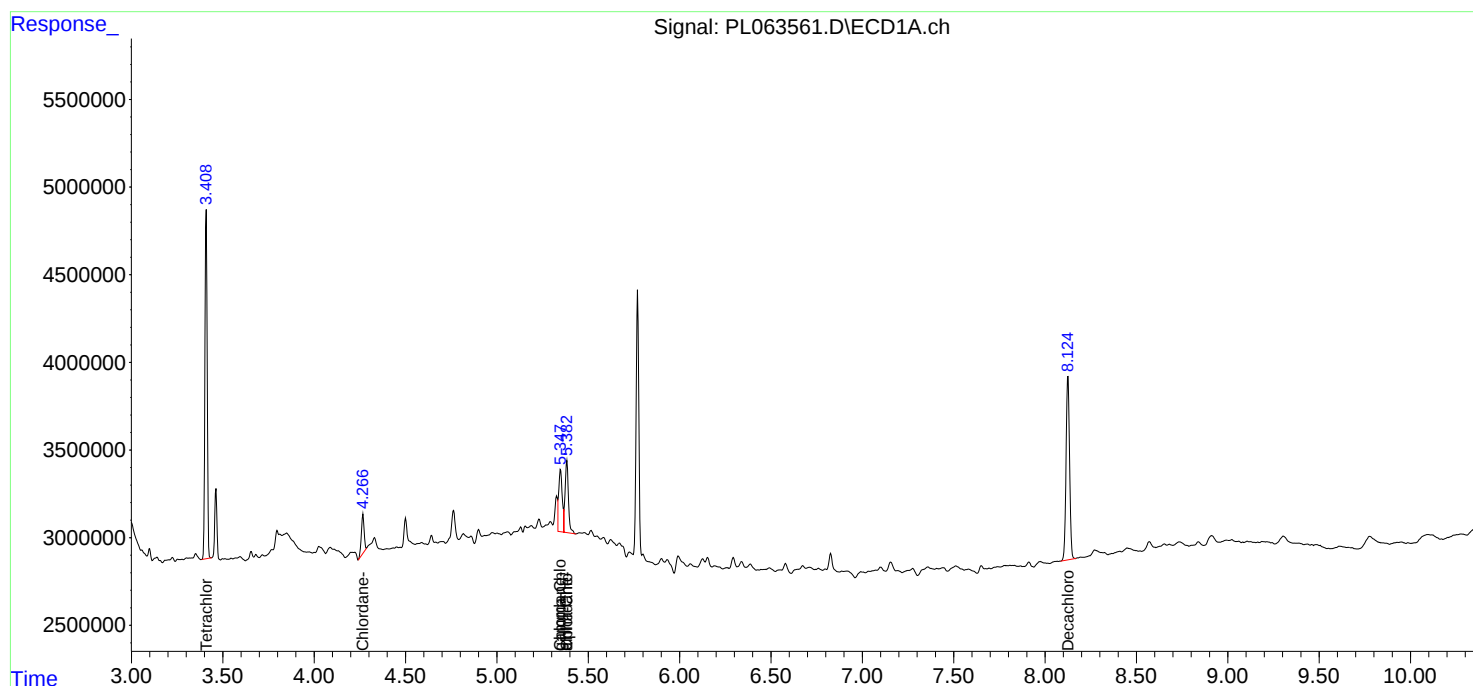


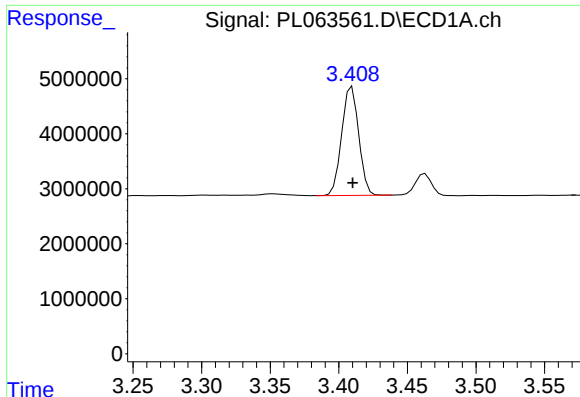

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 17118658
Conc: 10.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

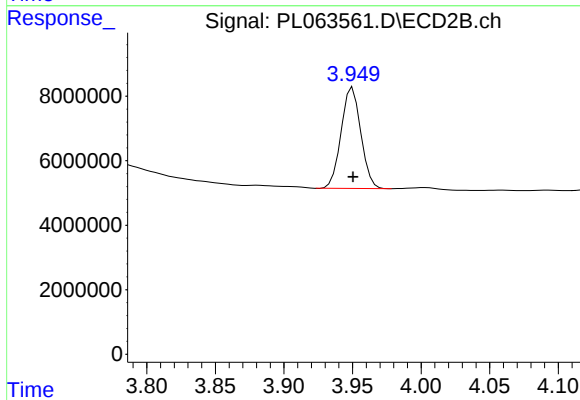


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 31371824
Conc: 10.01 ng/ml

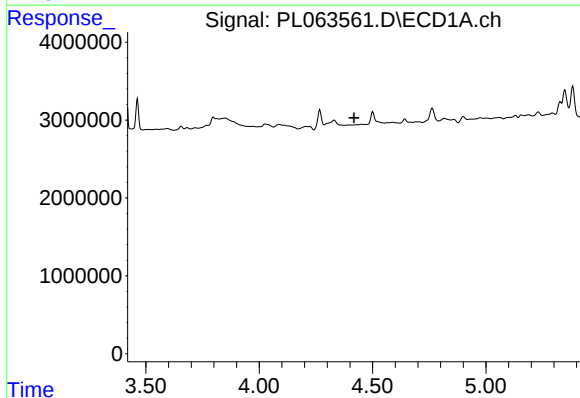


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

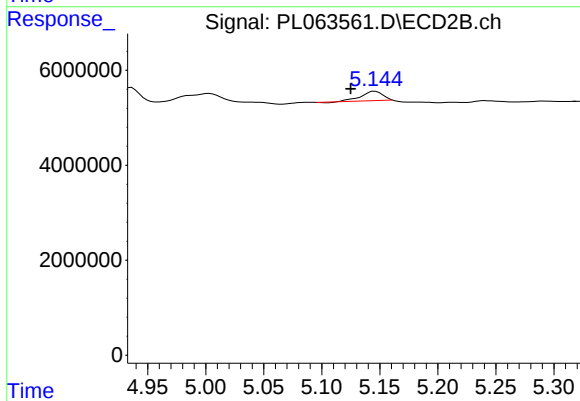

#4 Heptachlor


R.T.: 5.146 min
Delta R.T.: 0.021 min
Response: 2551286
Conc: 0.62 ng/ml

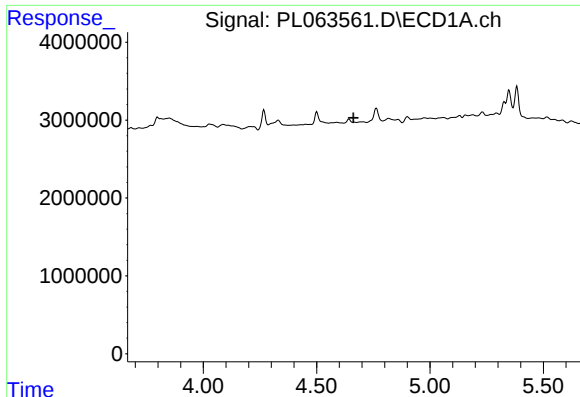

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

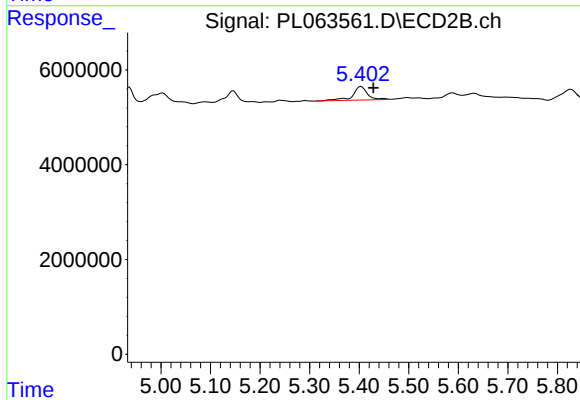


#5 Aldrin

R.T.: 5.404 min
Delta R.T.: -0.025 min
Response: 5835948
Conc: 1.51 ng/ml

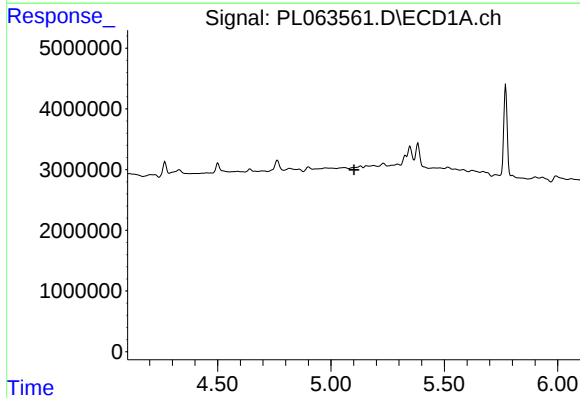


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

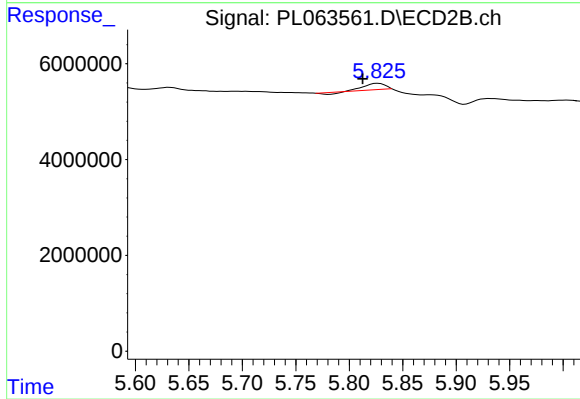

#8 Heptachlor epoxide


R.T.: 5.827 min
Delta R.T.: 0.014 min
Response: 1706336
Conc: 0.47 ng/ml

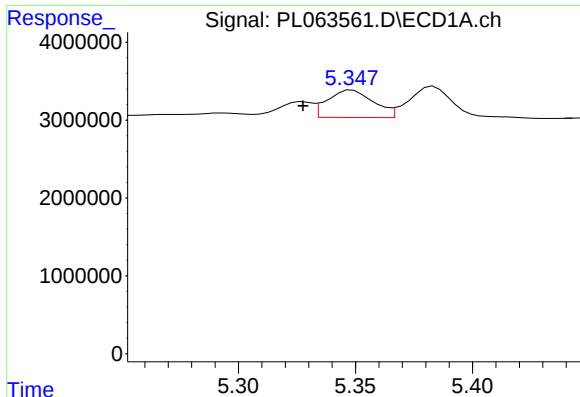

#10 gamma-Chlordane


R.T.: 5.349 min
Delta R.T.: 0.021 min
Response: 4821062
Conc: 2.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

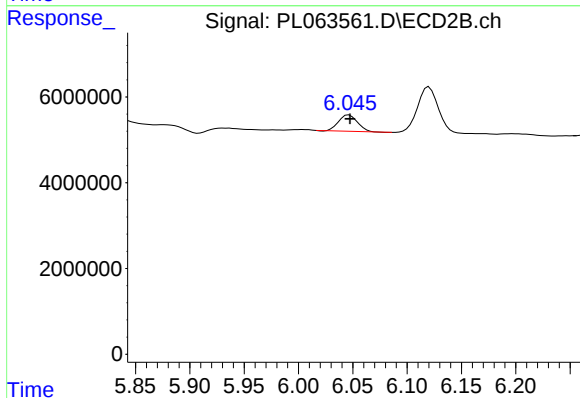


#10 gamma-Chlordane

R.T.: 6.046 min
Delta R.T.: -0.001 min
Response: 4584479
Conc: 1.29 ng/ml

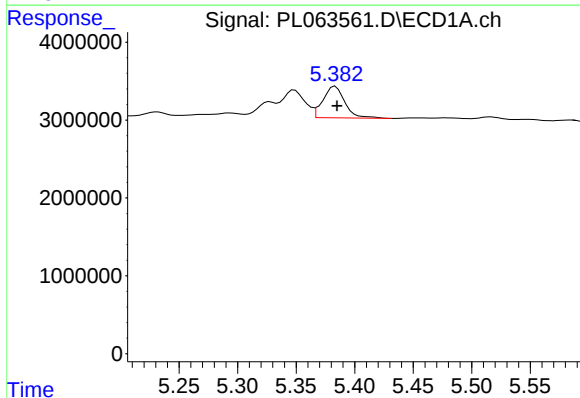


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.001 min
Response: 5268877
Conc: 2.83 ng/ml

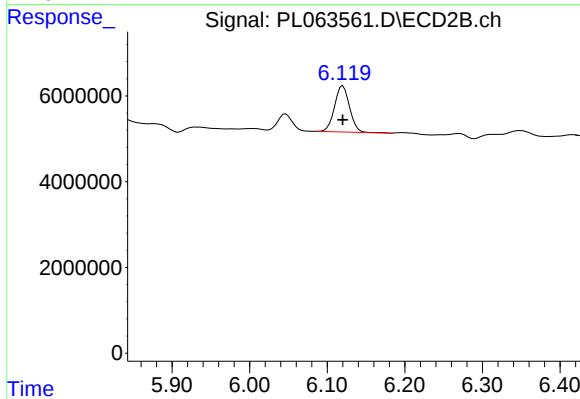

#11 alpha-Chlordane


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 14546532
Conc: 4.10 ng/ml

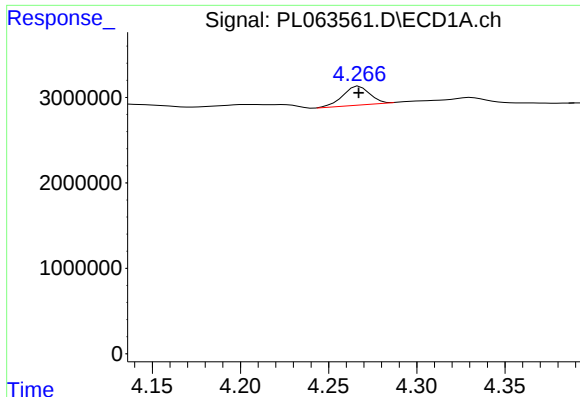

#23 Chlordane-1


R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 2328281
Conc: 42.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

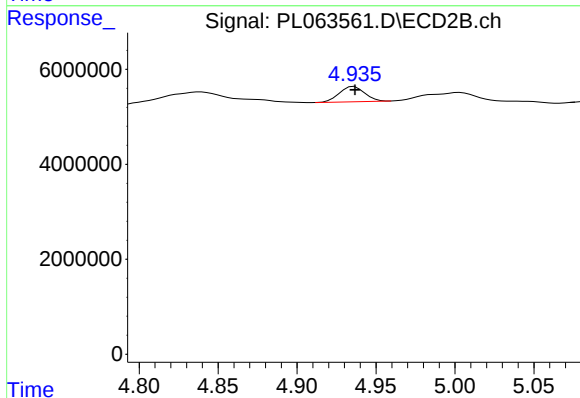


#23 Chlordane-1

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 3606045
Conc: 31.43 ng/ml

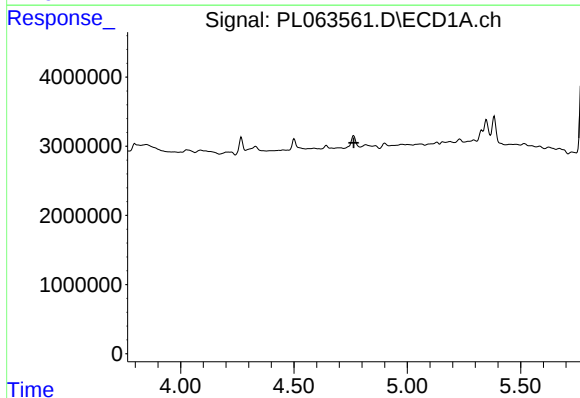


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

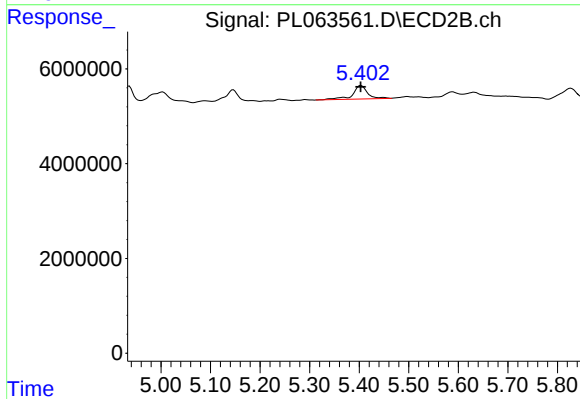

#24 Chlordane-2


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 5835948
Conc: 46.24 ng/ml

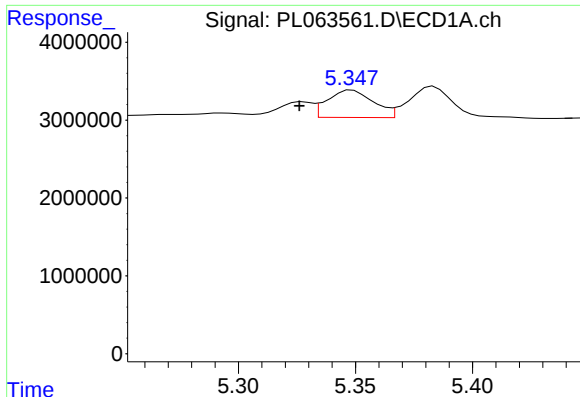

#25 Chlordane-3


R.T.: 5.349 min
Delta R.T.: 0.023 min
Response: 4821062
Conc: 27.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

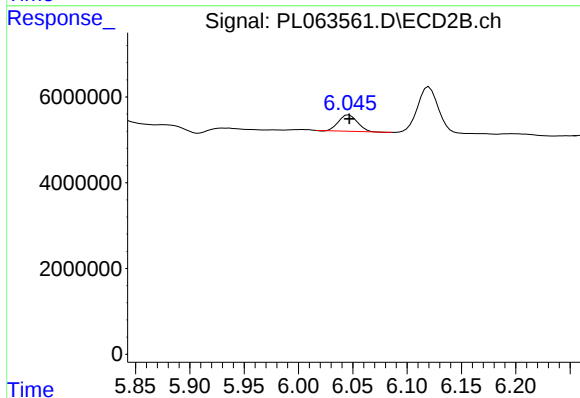


#25 Chlordane-3

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 4584479
Conc: 9.95 ng/ml

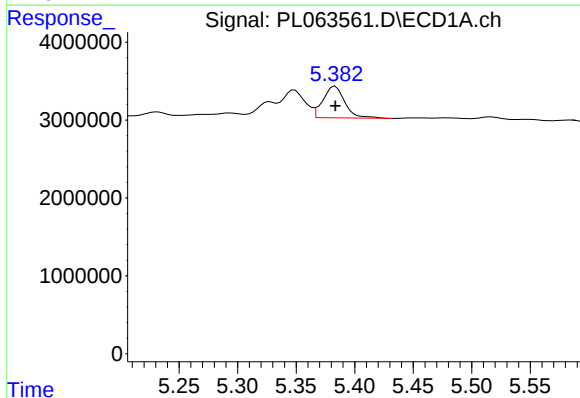


#26 Chlordane-4

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 5268877
Conc: 36.02 ng/ml

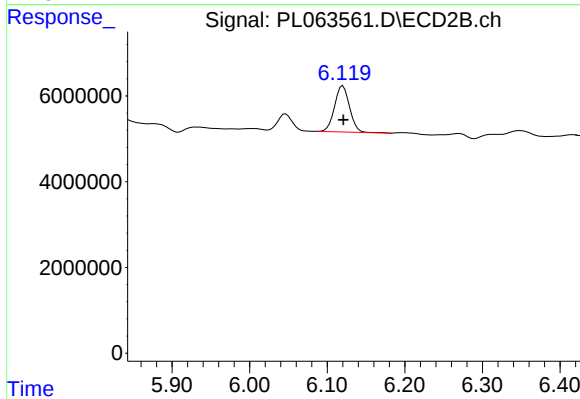

#26 Chlordane-4


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 14546532
Conc: 26.53 ng/ml

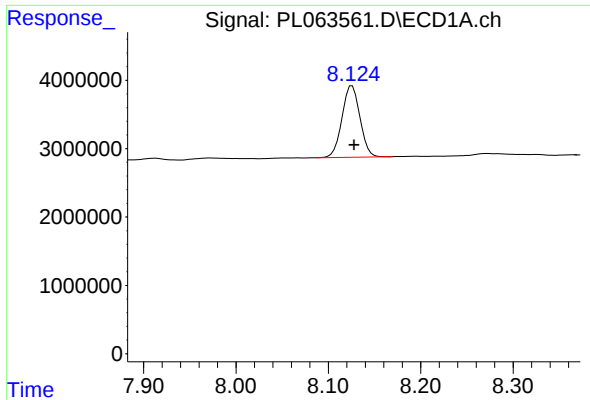

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.002 min
Response: 14172298
Conc: 7.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

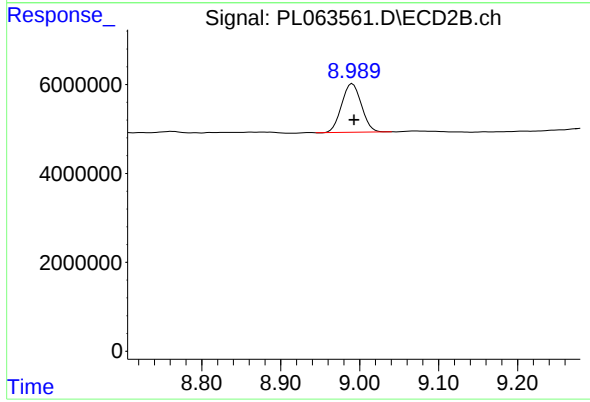

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: -0.002 min
Response: 19091393
Conc: 7.58 ng/ml