

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 19:29
 Operator : DD\AJ
 Sample : L5043-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KENS-SS1-121020-0-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:34:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	37251906	69388051	21.891	22.139
28)	SA Decachlor...	8.125	8.990	33685360	44842750	16.727	17.807
Target Compounds							
7)	B delta-BHC	0.000	5.006	0	3377868	N.D.	0.835 #
8)	B Heptachlo...	0.000	5.828f	0	2289464	N.D.	0.632 #
10)	B gamma-Chl...	5.346f	0.000	10411179	0	5.597	N.D. #
15)	B Endosulfa...	0.000	6.873f	0	11546210	N.D.	3.625 #
17)	MA 4,4'-DDT	0.000	7.041f	0	11422420	N.D.	4.467 #
18)	B Endrin al...	0.000	6.949f	0	46575878	N.D.	18.252 #
25)	Chlordane-3	5.346f	0.000	10411179	0	60.091	N.D. #
27)	Chlordane-5	0.000	6.949f	0	46575878	N.D.	513.225 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 19:29
Operator : DD\AJ
Sample : L5043-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:34:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

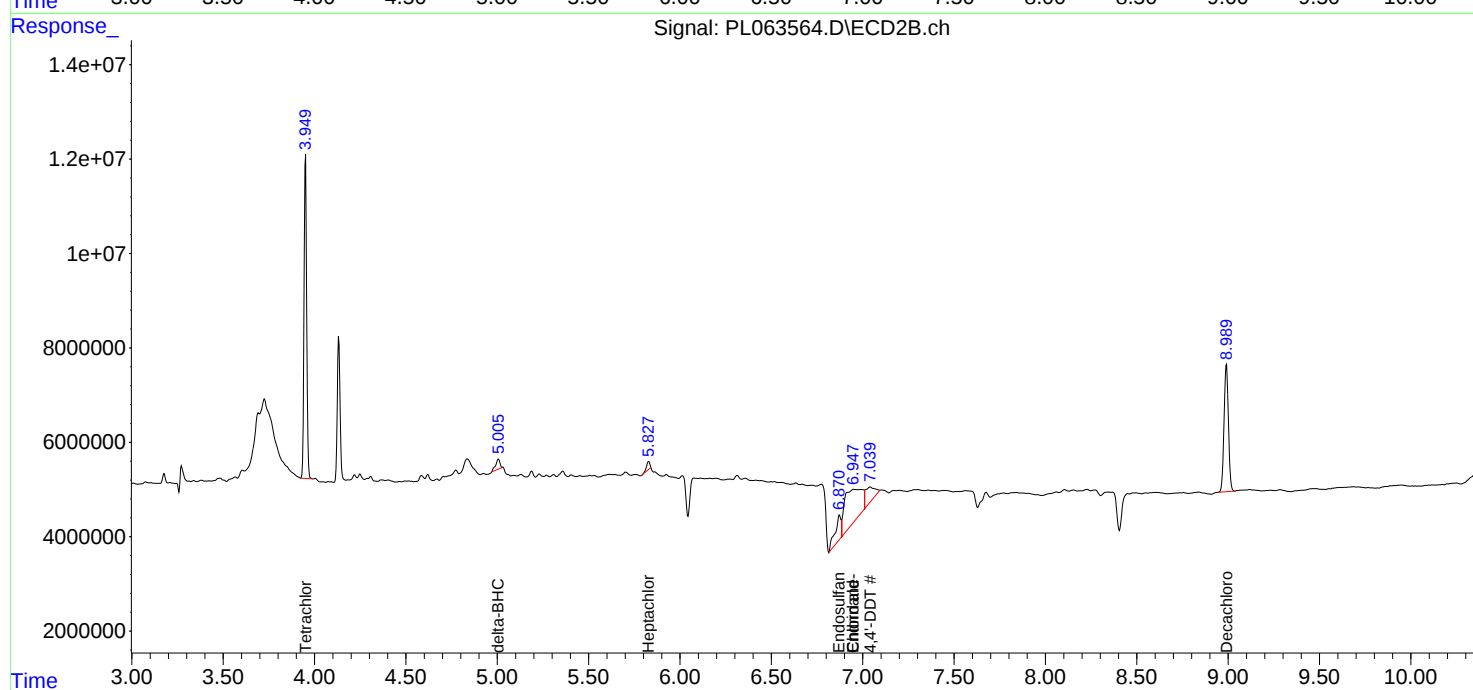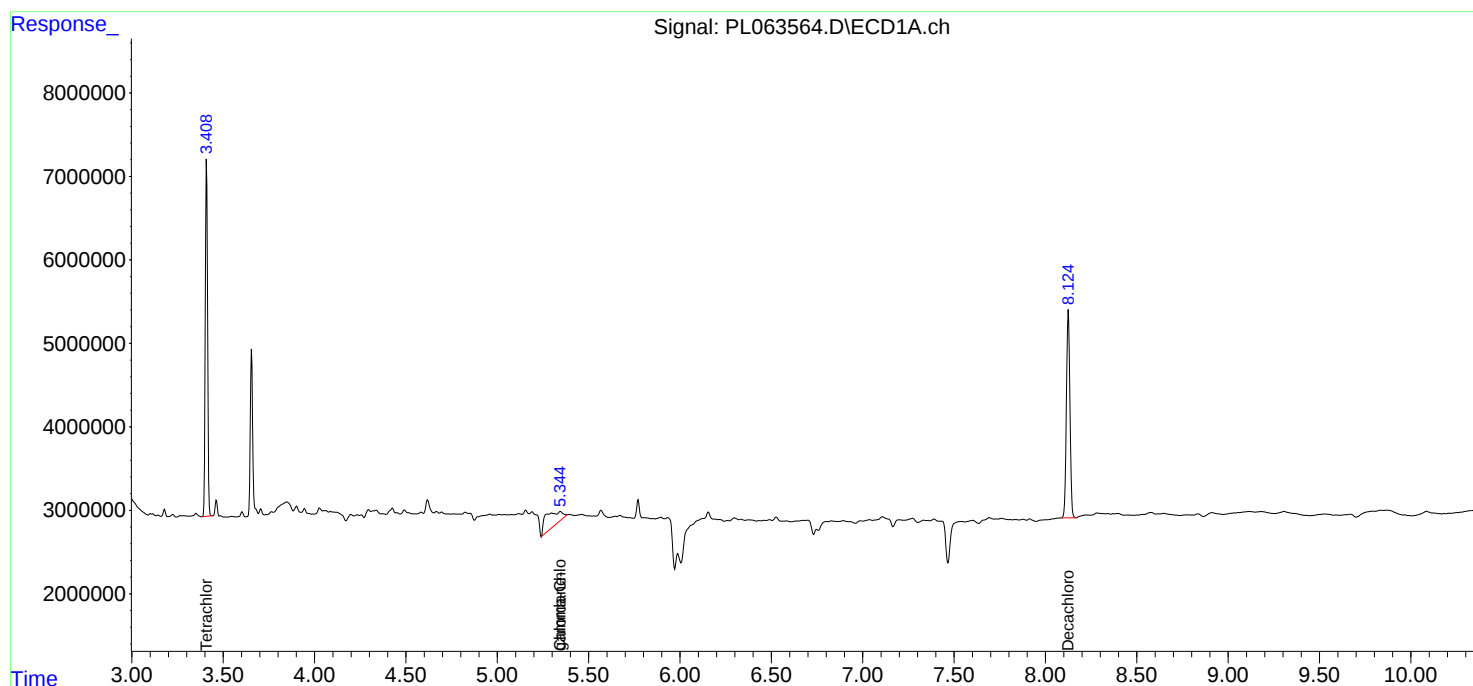


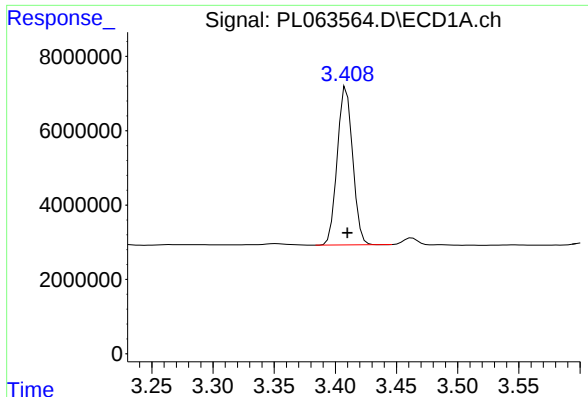

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 37251906
Conc: 21.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

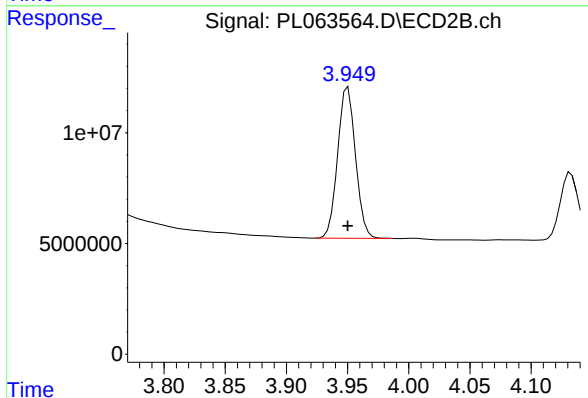


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 69388051
Conc: 22.14 ng/ml

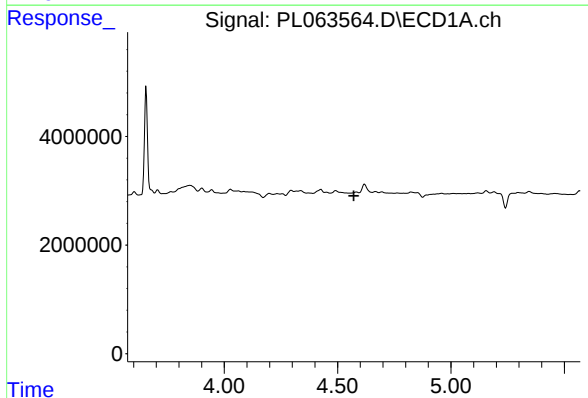


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

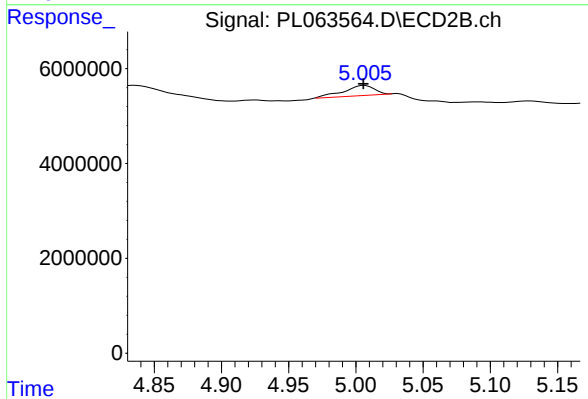

#7 delta-BHC


R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 3377868
Conc: 0.83 ng/ml

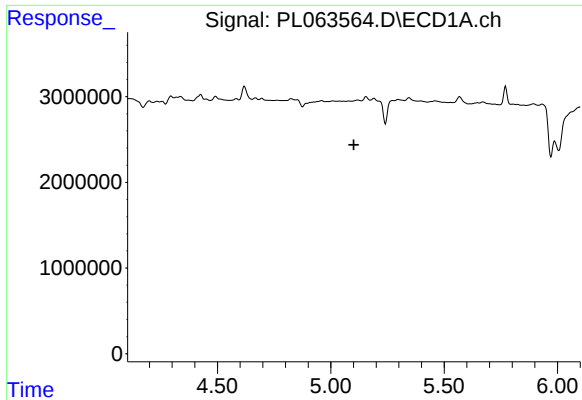

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

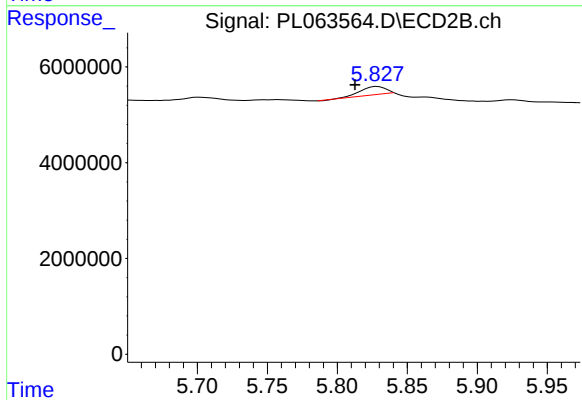


#8 Heptachlor epoxide

R.T.: 5.828 min
Delta R.T.: 0.016 min
Response: 2289464
Conc: 0.63 ng/ml

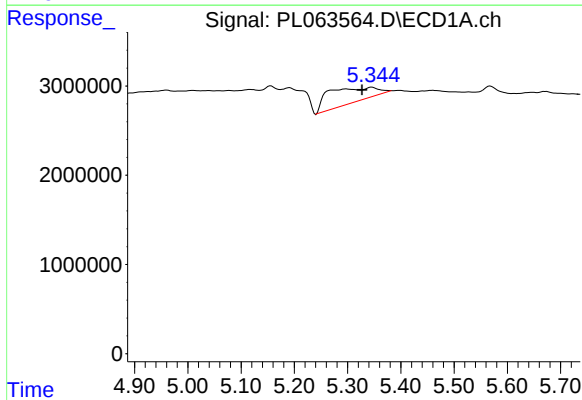


#10 gamma-Chlordane

R.T.: 5.346 min
Delta R.T.: 0.018 min
Response: 10411179
Conc: 5.60 ng/ml

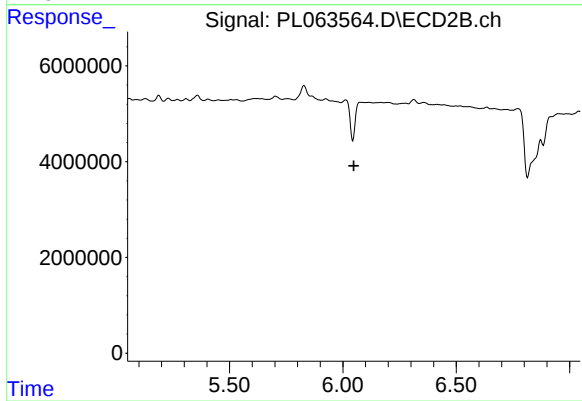

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.048 min
Response: 0
Conc: N.D.

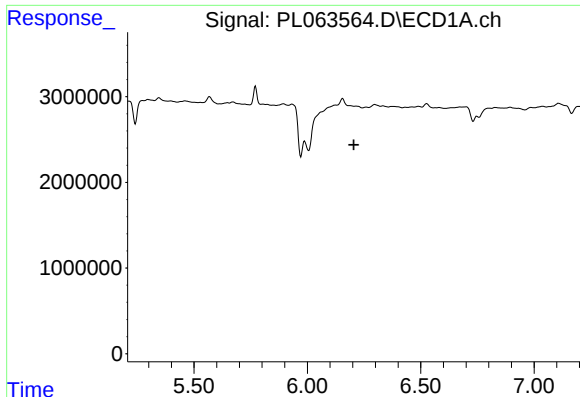

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

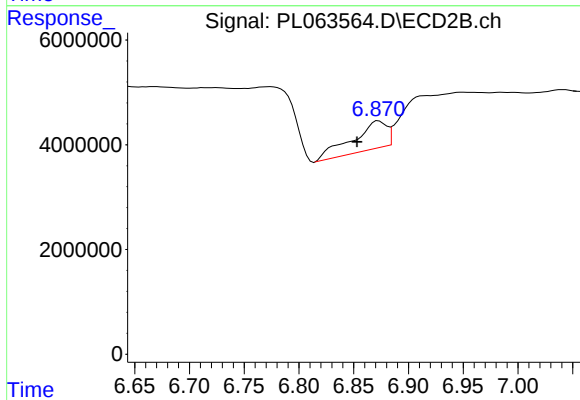


#15 Endosulfan II

R.T.: 6.873 min
Delta R.T.: 0.020 min
Response: 11546210
Conc: 3.63 ng/ml

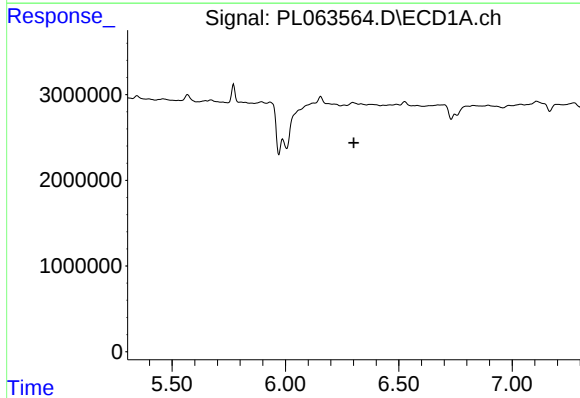


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.301 min
Response: 0
Conc: N.D.

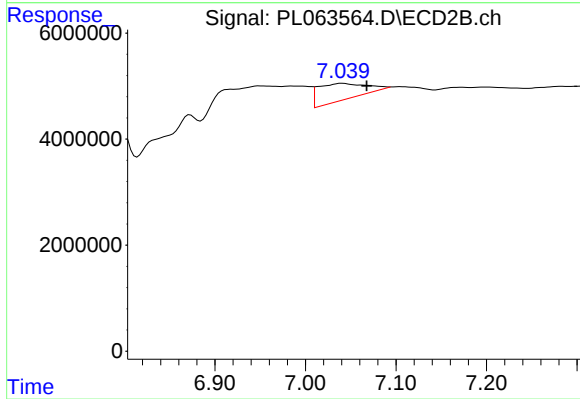

#17 4,4'-DDT


R.T.: 7.041 min
Delta R.T.: -0.027 min
Response: 11422420
Conc: 4.47 ng/ml

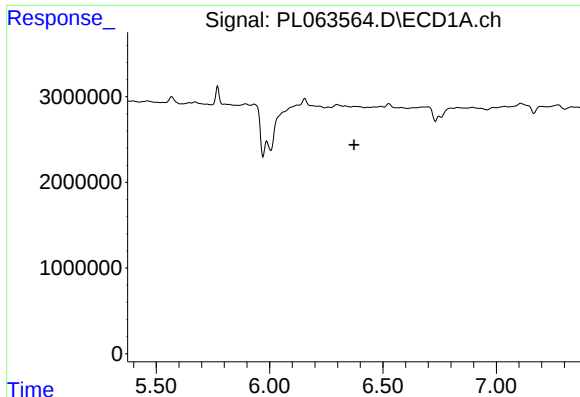

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

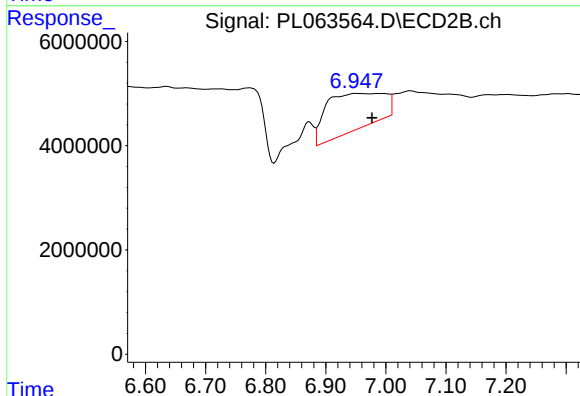


#18 Endrin aldehyde

R.T.: 6.949 min
Delta R.T.: -0.028 min
Response: 46575878
Conc: 18.25 ng/ml

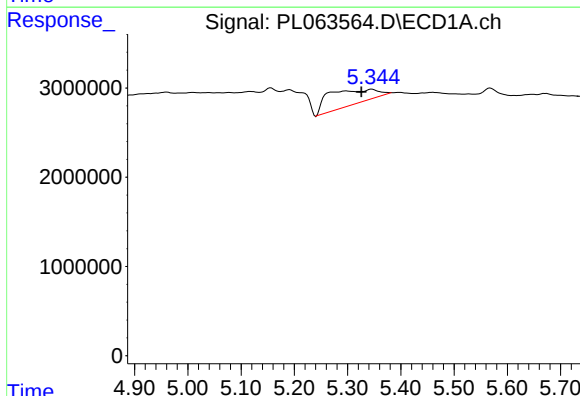


#25 Chlordane-3

R.T.: 5.346 min
Delta R.T.: 0.019 min
Response: 10411179
Conc: 60.09 ng/ml

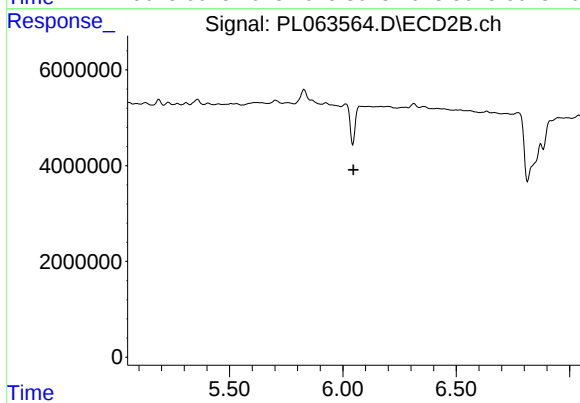

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.047 min
Response: 0
Conc: N.D.

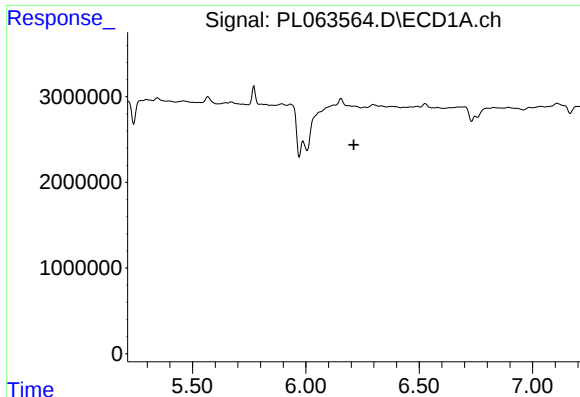

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS1-121020-0-7

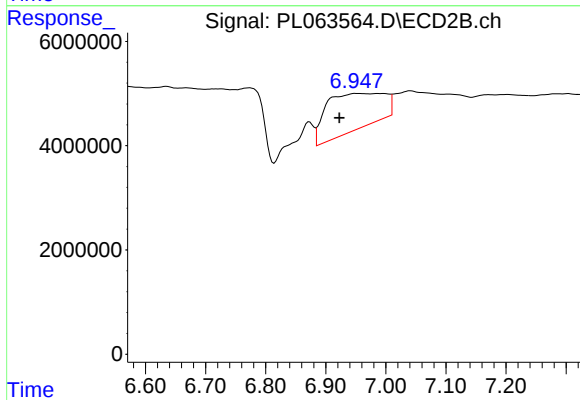


#27 Chlordane-5

R.T.: 6.949 min
Delta R.T.: 0.027 min
Response: 46575878
Conc: 513.23 ng/ml

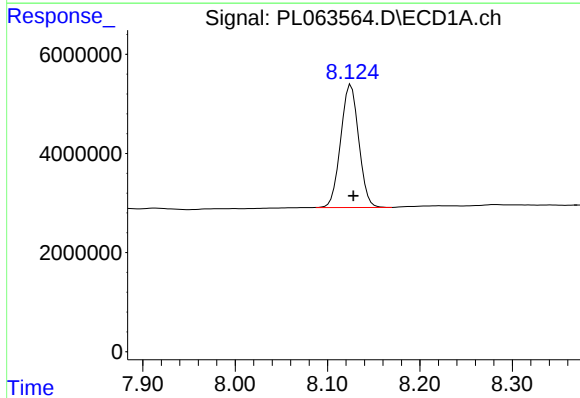

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 33685360
Conc: 16.73 ng/ml

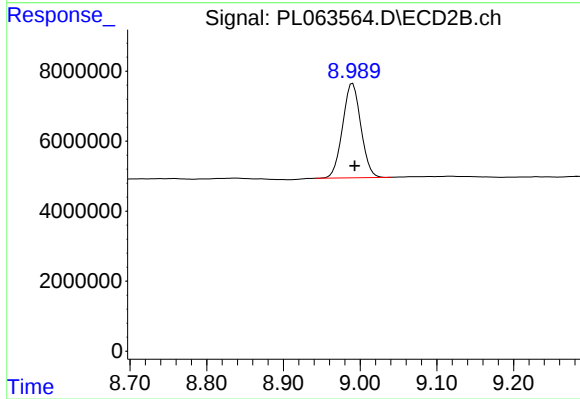

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: -0.003 min
Response: 44842750
Conc: 17.81 ng/ml