

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
 Data File : PL063536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2020 12:34
 Operator : DD\AJ
 Sample : L5015-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-121020

Manual Integrations
 APPROVED

Ankita
 12/14/2020 4:23:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.949	25135150	43225119	14.771	13.792
28)	SA Decachlor...	8.124	8.989	26312077	36321443	13.066	14.423
Target Compounds							
12)	B 4,4'-DDE	5.548	6.275	6615536	14563169	3.895	4.158
17)	MA 4,4'-DDT	6.296	7.065	2986268	6306238	2.176m	2.466

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121320\
Data File : PL063536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2020 12:34
Operator : DD\AJ
Sample : L5015-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:23:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

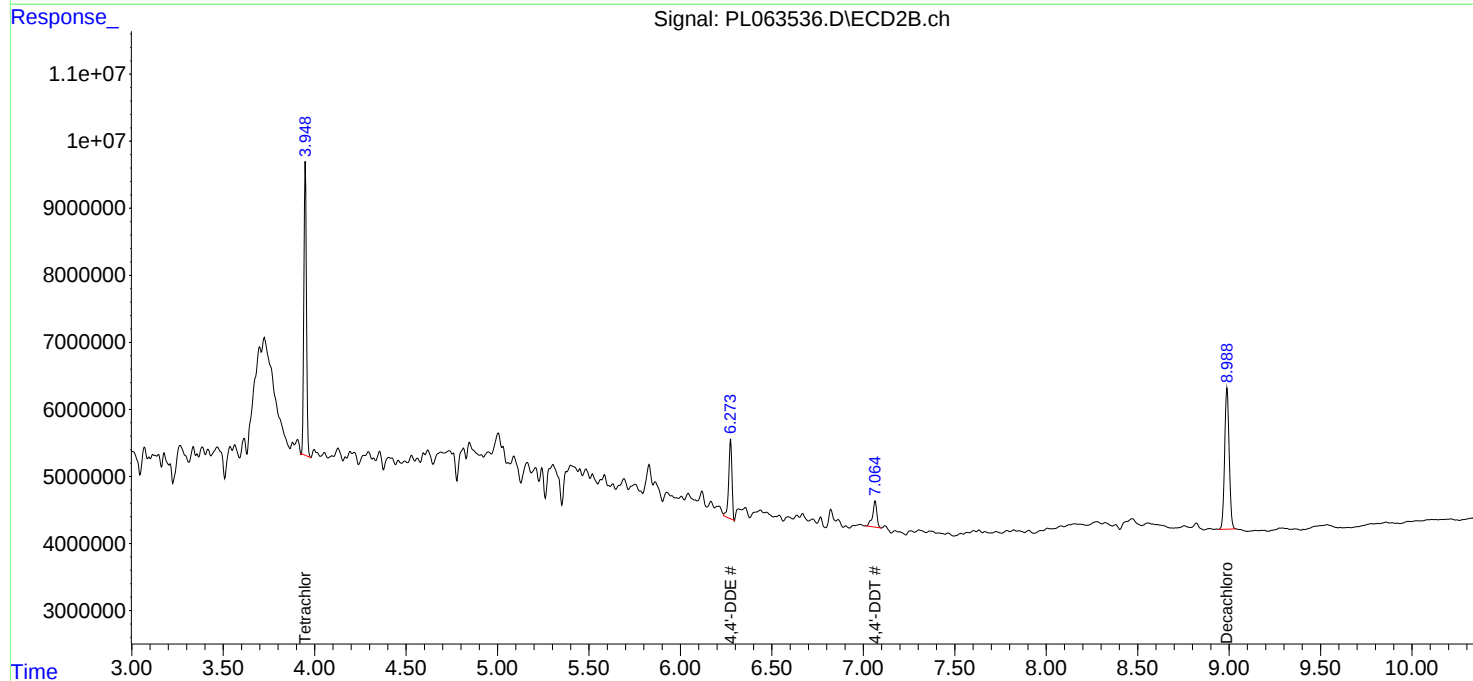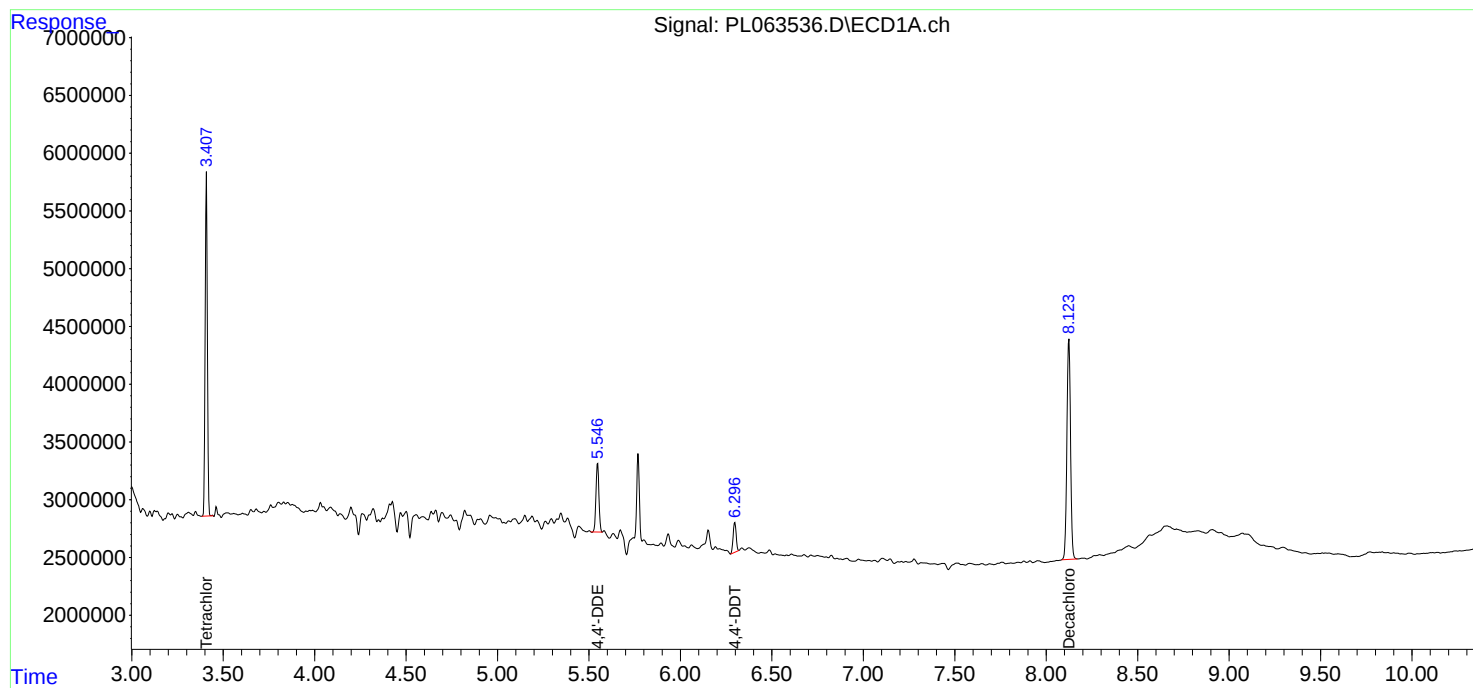

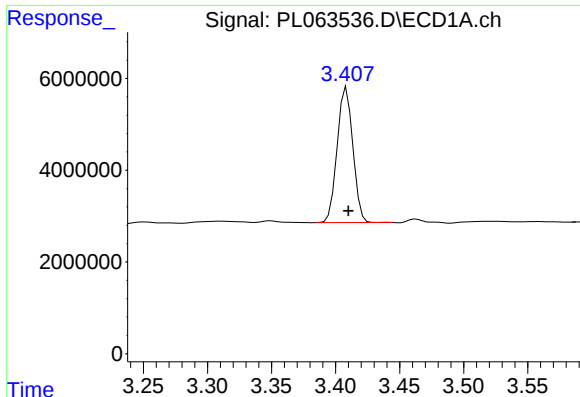


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: -0.001 min
Response: 25135150
Conc: 14.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:23:06 PM

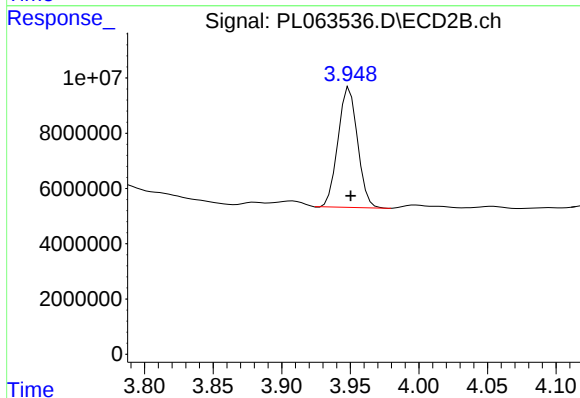


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 43225119
Conc: 13.79 ng/ml

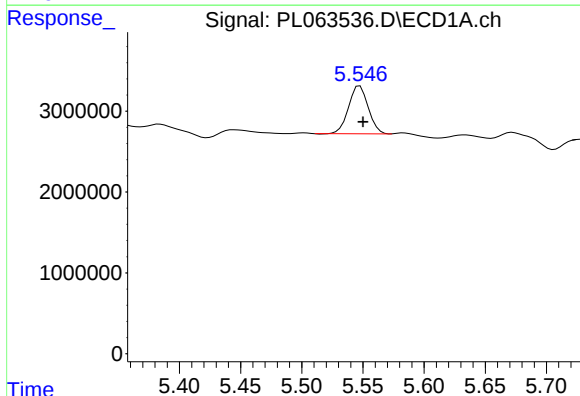


#12 4,4'-DDE

R.T.: 5.548 min
Delta R.T.: -0.003 min
Response: 6615536
Conc: 3.90 ng/ml

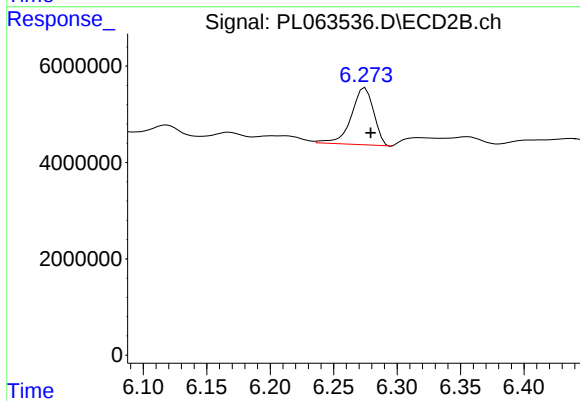

#12 4,4'-DDE

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 14563169
Conc: 4.16 ng/ml

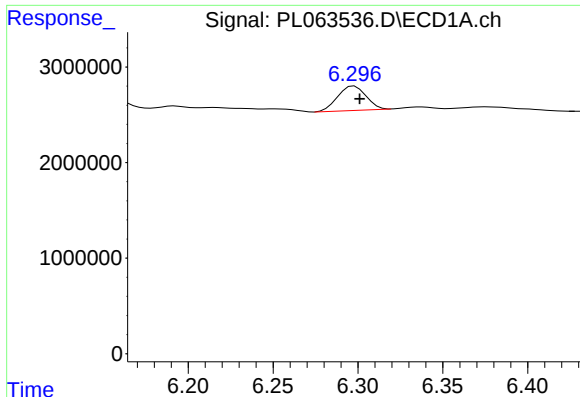


#17 4,4'-DDT

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 2986268
Conc: 2.18 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:23:06 PM

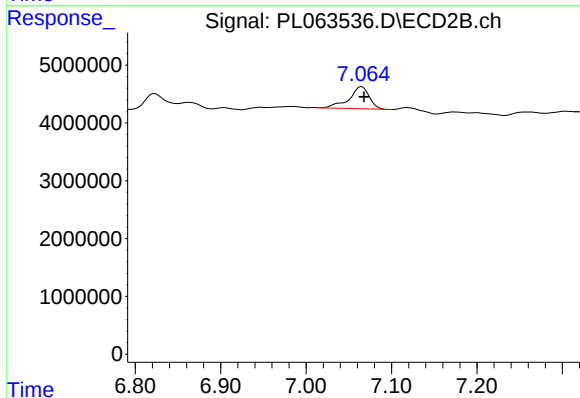


#17 4,4'-DDT

R.T.: 7.065 min
Delta R.T.: -0.002 min
Response: 6306238
Conc: 2.47 ng/ml

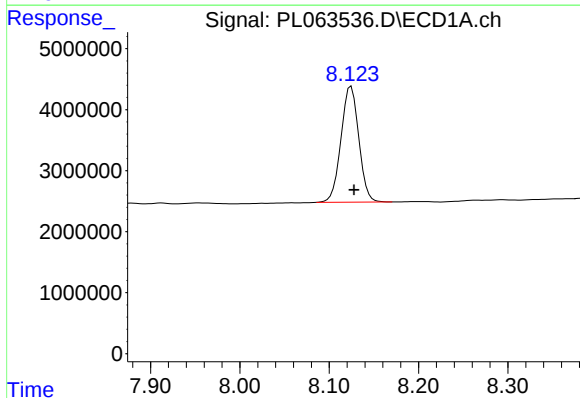

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 26312077
Conc: 13.07 ng/ml

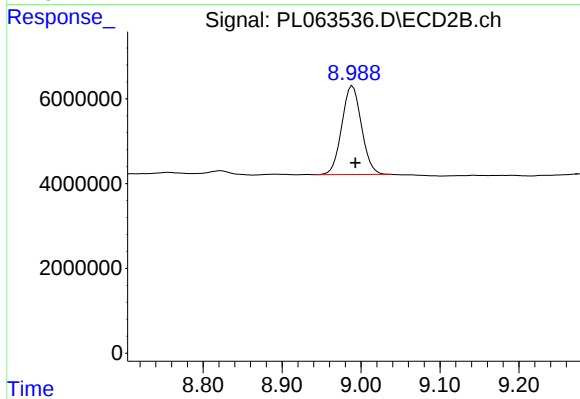

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 36321443
Conc: 14.42 ng/ml