

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2022 08:48
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 20:40:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	8.764	0.000	97125	0	0.050	N.D. #
Target Compounds							
8)	B Heptachlo...	5.465	4.449f	3902058	1214870	1.367	0.360 #
9)	A Endosulfan I	5.839	0.000	41090	0	0.015	N.D. #
11)	B alpha-Chl...	0.000	4.752f	0	1611791	N.D.	0.481 #
13)	MA Dieldrin	0.000	5.092	0	3432562	N.D.	1.018 #
14)	MA Endrin	0.000	5.390f	0	1952950	N.D.	0.646 #
15)	B Endosulfa...	0.000	5.684f	0	35164	N.D.	0.013 #
17)	MA 4,4'-DDT	6.825f	0.000	57328	0	0.025	N.D. #
19)	B Endosulfa...	0.000	6.078f	0	197736	N.D.	0.070 #
20)	A Methoxychlor	7.305f	0.000	36484	0	0.030	N.D. #
22)	Mirex	7.907f	0.000	129034	0	0.068	N.D. #
24)	Chlordane-2	0.000	4.099	0	17777079	N.D.	151.834 #
26)	Chlordane-4	0.000	4.752f	0	1611791	N.D.	4.448 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2022 08:48
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 20:40:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

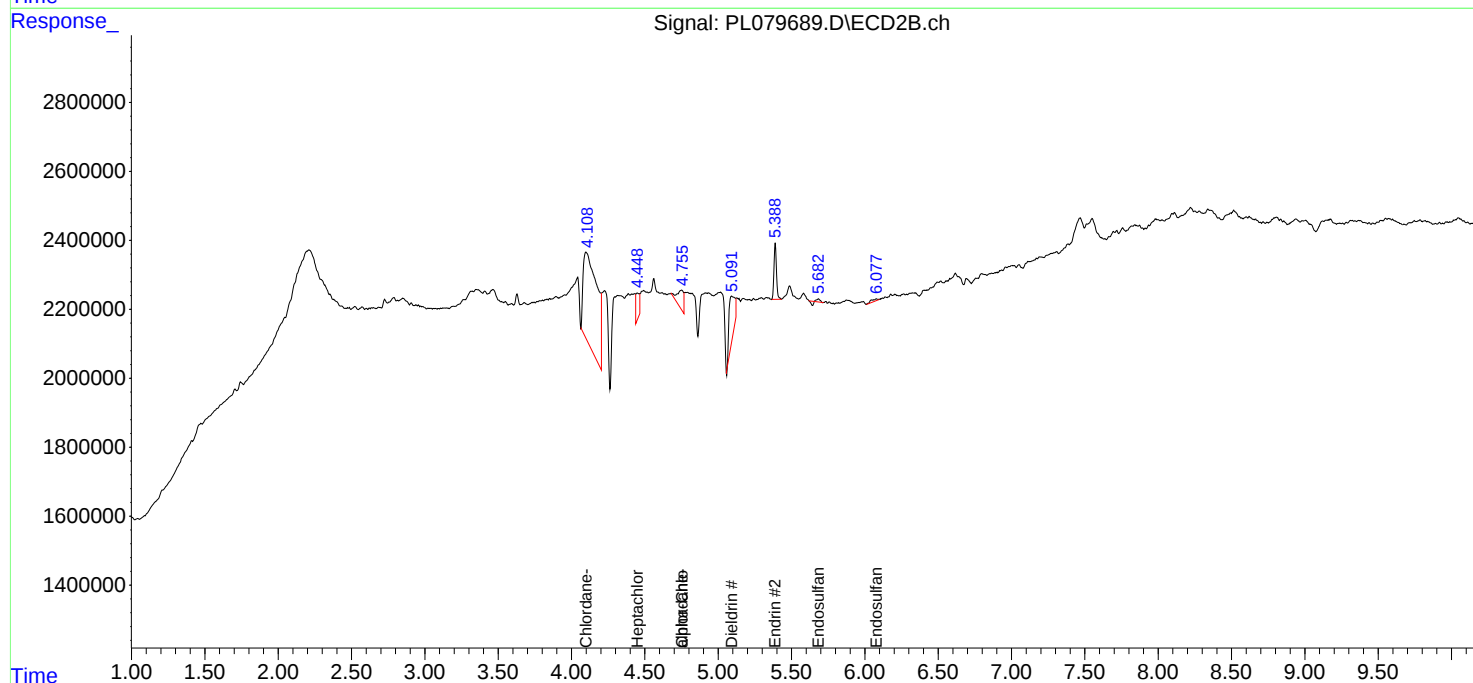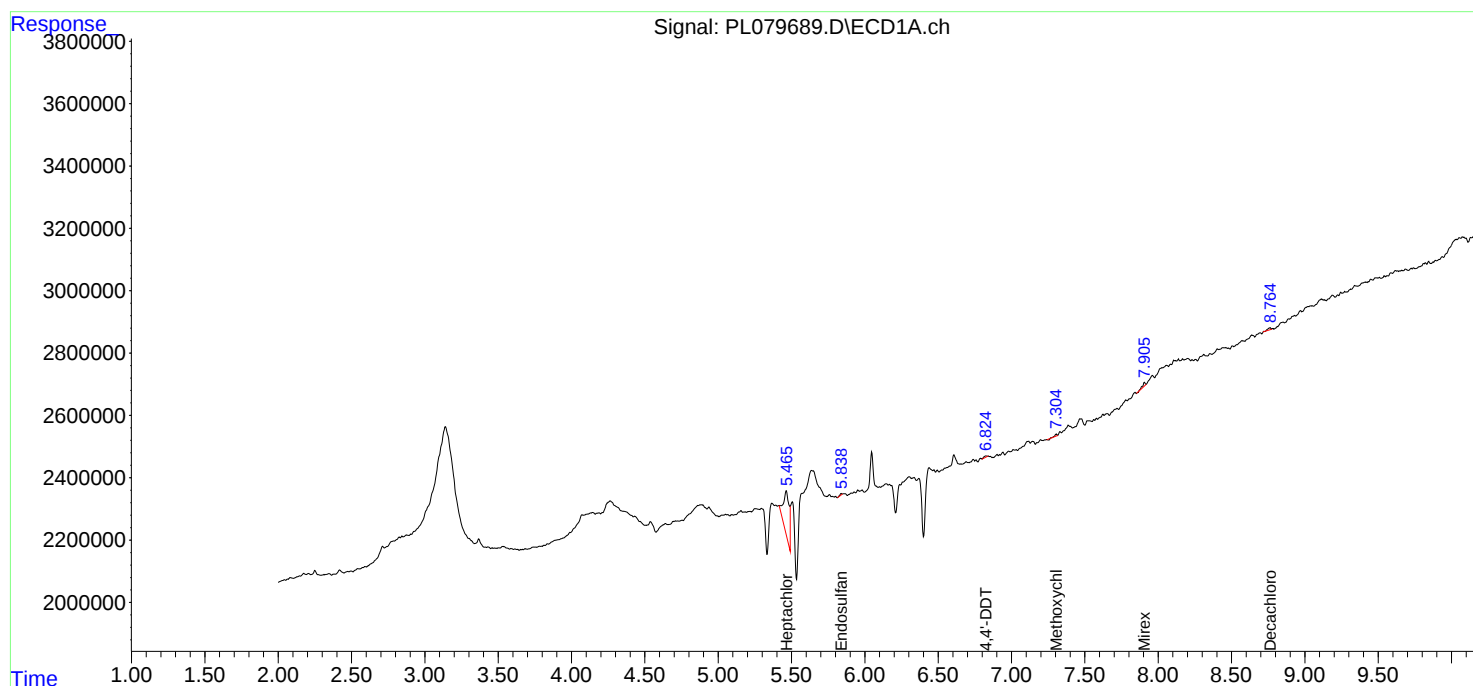


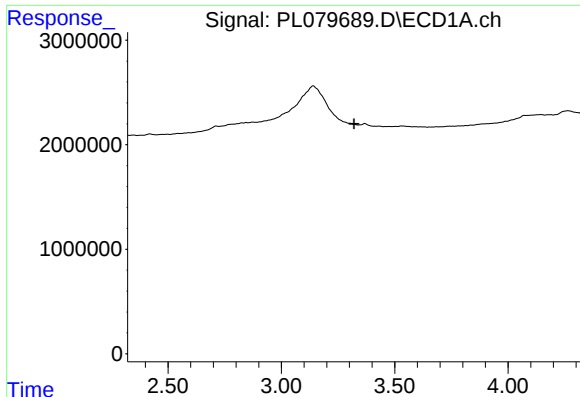

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

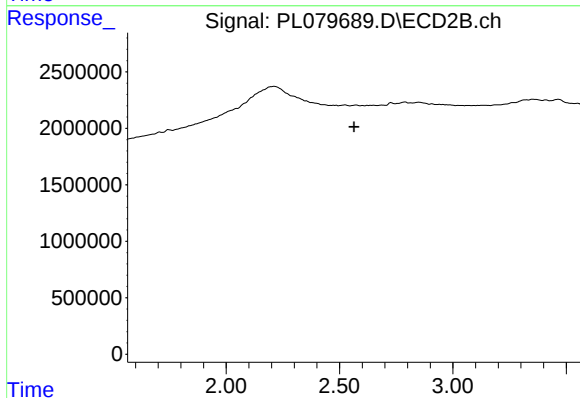


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.564 min
Response: 0
Conc: N.D.

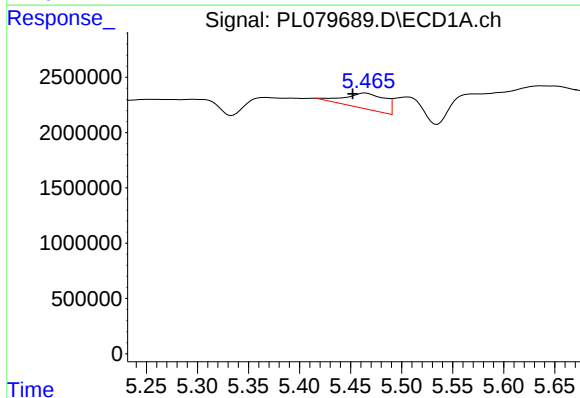


#8 Heptachlor epoxide

R.T.: 5.465 min
Delta R.T.: 0.013 min
Response: 3902058
Conc: 1.37 ng/ml

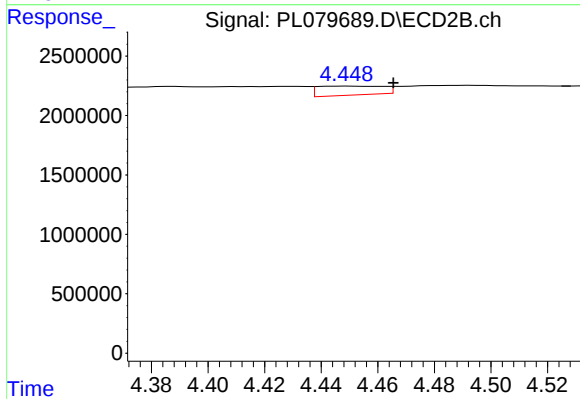

#8 Heptachlor epoxide


R.T.: 4.449 min
Delta R.T.: -0.016 min
Response: 1214870
Conc: 0.36 ng/ml

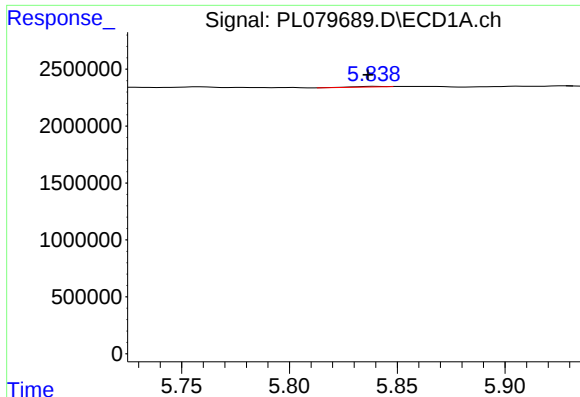

#9 Endosulfan I


R.T.: 5.839 min
Delta R.T.: 0.003 min
Response: 41090
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

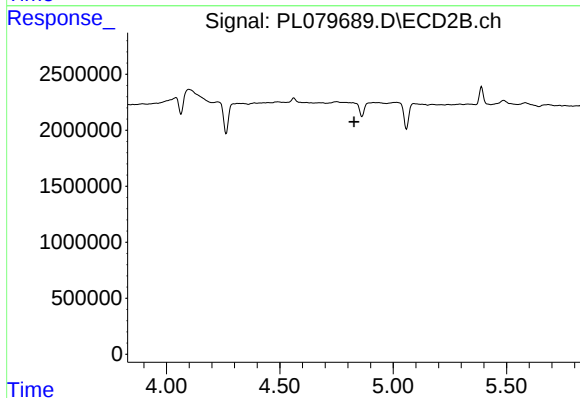


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

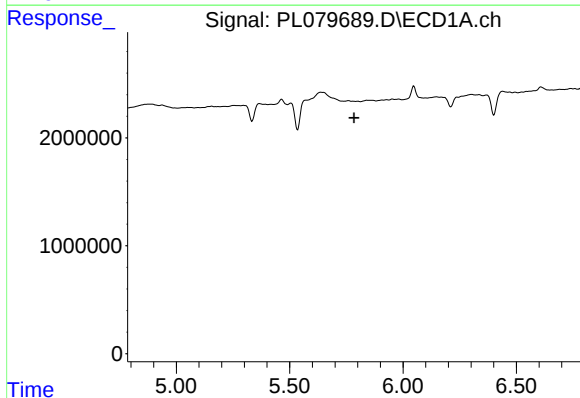


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.784 min
Response: 0
Conc: N.D.

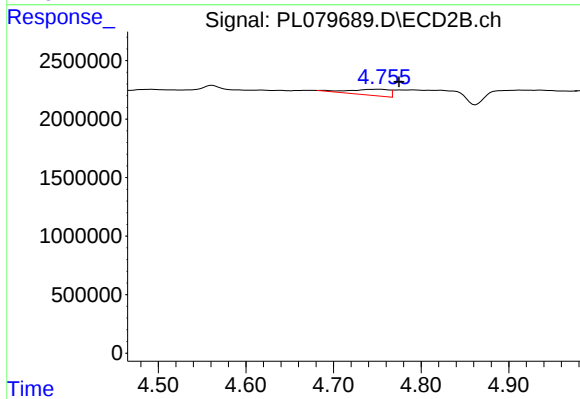

#11 alpha-Chlordane


R.T.: 4.752 min
Delta R.T.: -0.023 min
Response: 1611791
Conc: 0.48 ng/ml

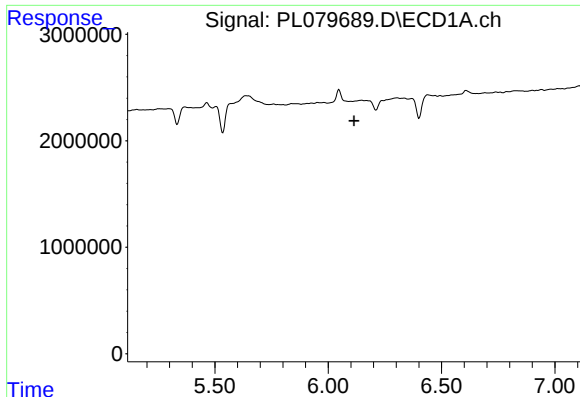

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

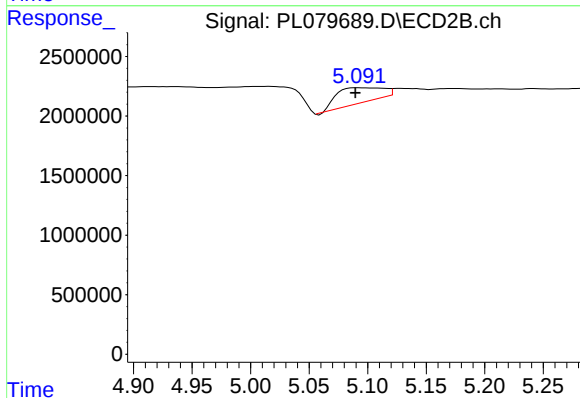


#13 Dieldrin

R.T.: 5.092 min
Delta R.T.: 0.002 min
Response: 3432562
Conc: 1.02 ng/ml

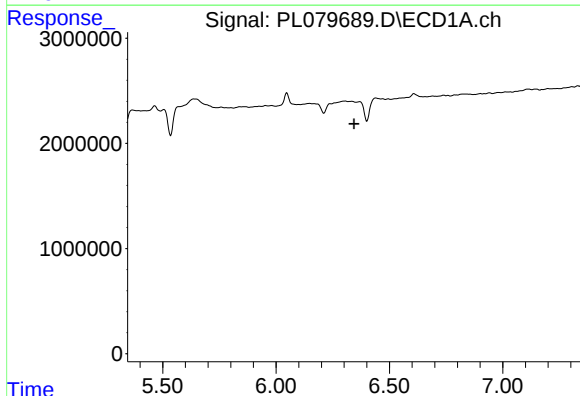


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

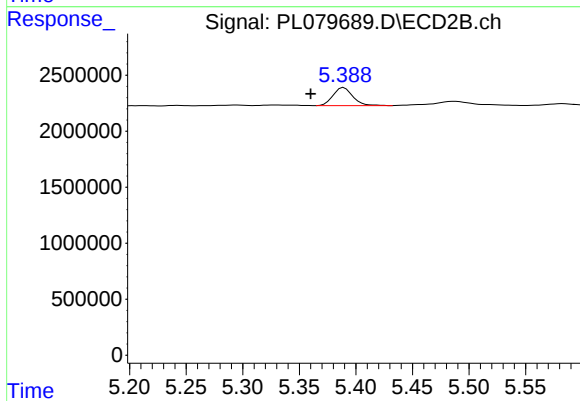

#14 Endrin


R.T.: 5.390 min
Delta R.T.: 0.029 min
Response: 1952950
Conc: 0.65 ng/ml

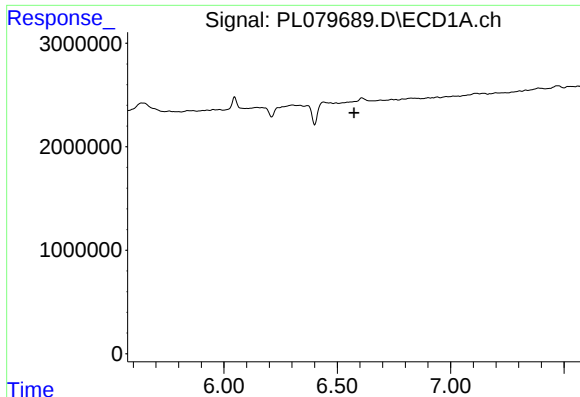

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

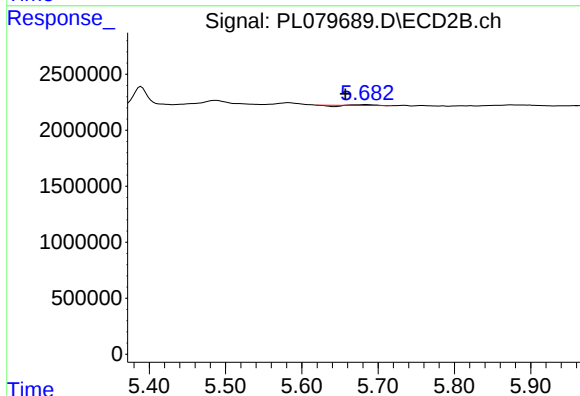


#15 Endosulfan II

R.T.: 5.684 min
Delta R.T.: 0.027 min
Response: 35164
Conc: 0.01 ng/ml

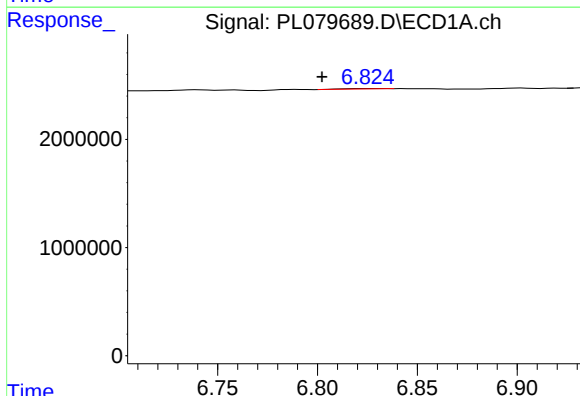


#17 4,4'-DDT

R.T.: 6.825 min
Delta R.T.: 0.023 min
Response: 57328
Conc: 0.03 ng/ml

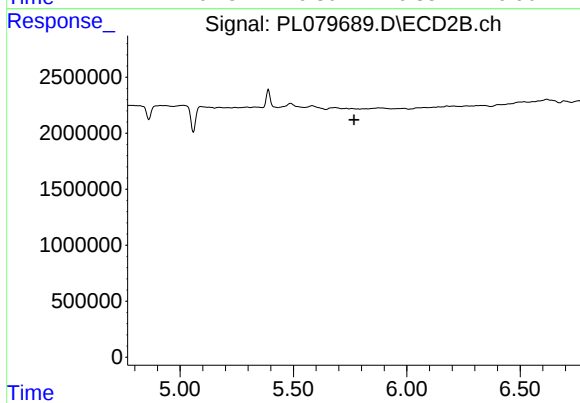

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 5.767 min
Response: 0
Conc: N.D.

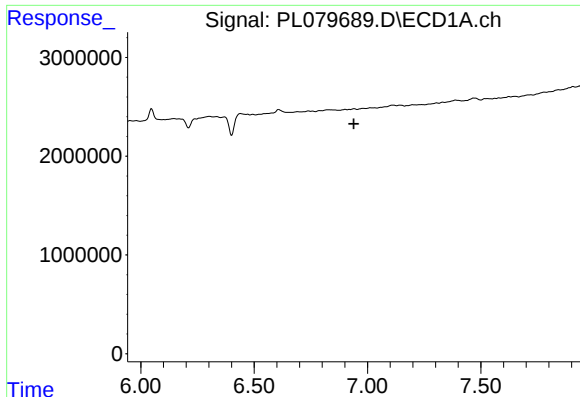

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

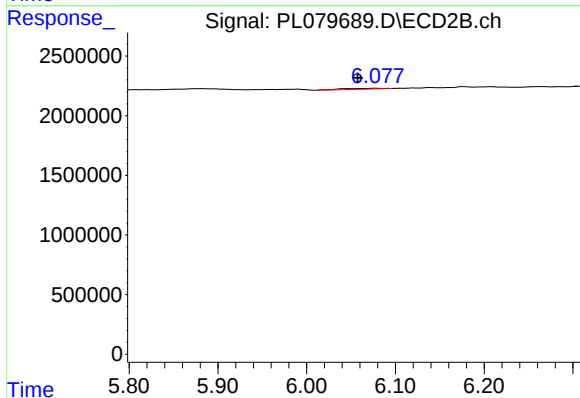


#19 Endosulfan Sulfate

R.T.: 6.078 min
Delta R.T.: 0.021 min
Response: 197736
Conc: 0.07 ng/ml

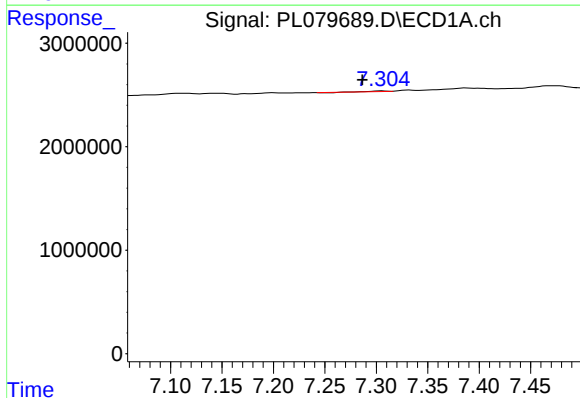


#20 Methoxychlor

R.T.: 7.305 min
Delta R.T.: 0.019 min
Response: 36484
Conc: 0.03 ng/ml

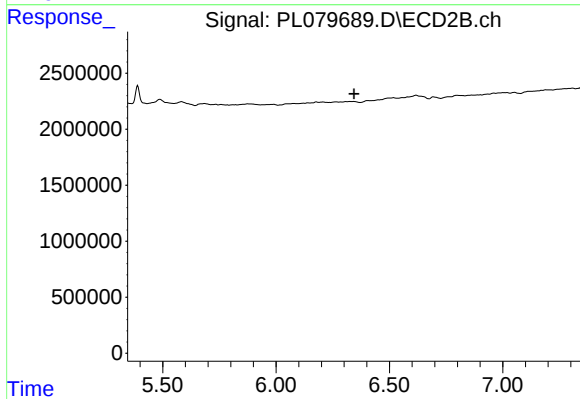

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

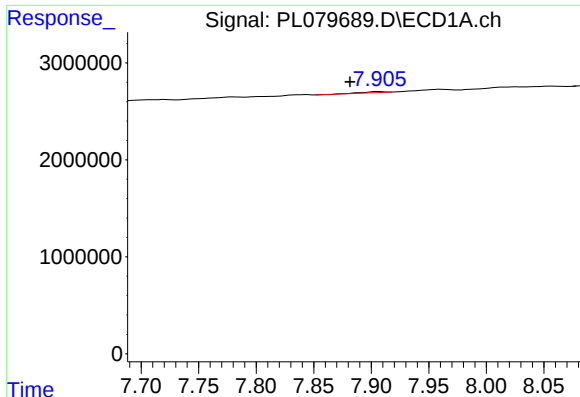

#22 Mirex


R.T.: 7.907 min
Delta R.T.: 0.025 min
Response: 129034
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

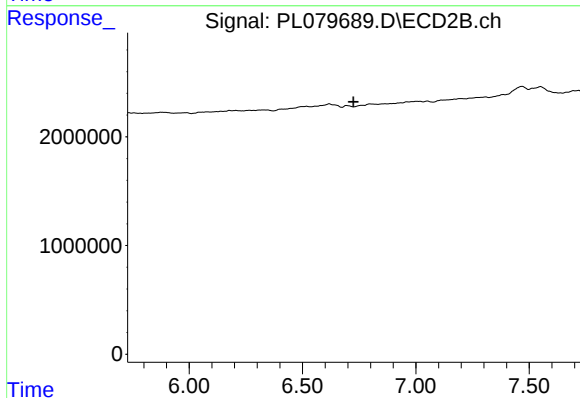


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 6.725 min
Response: 0
Conc: N.D.

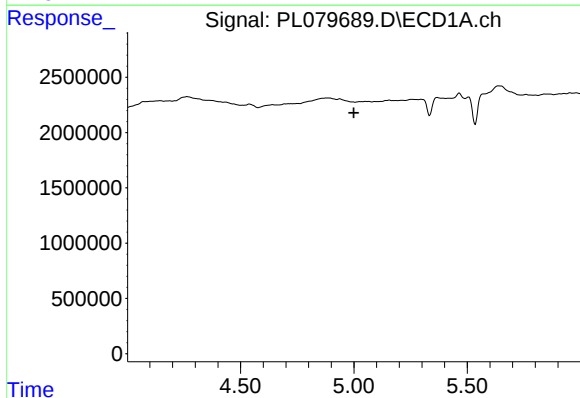


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.999 min
Response: 0
Conc: N.D.

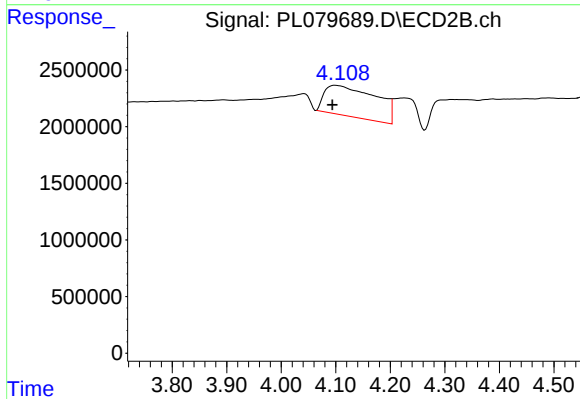

#24 Chlordane-2


R.T.: 4.099 min
Delta R.T.: 0.005 min
Response: 17777079
Conc: 151.83 ng/ml

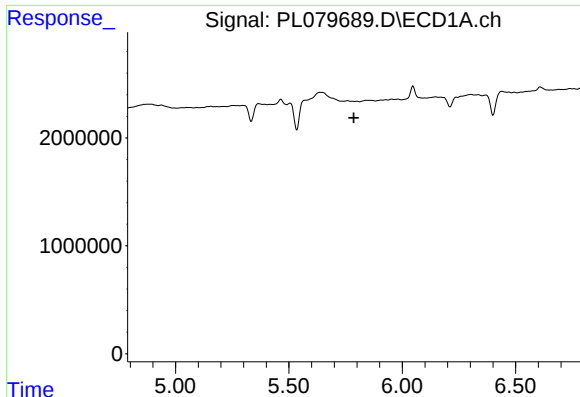

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

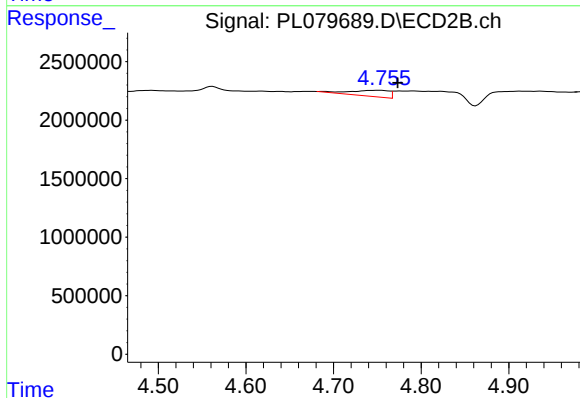


#26 Chlordane-4

R.T.: 4.752 min
Delta R.T.: -0.022 min
Response: 1611791
Conc: 4.45 ng/ml

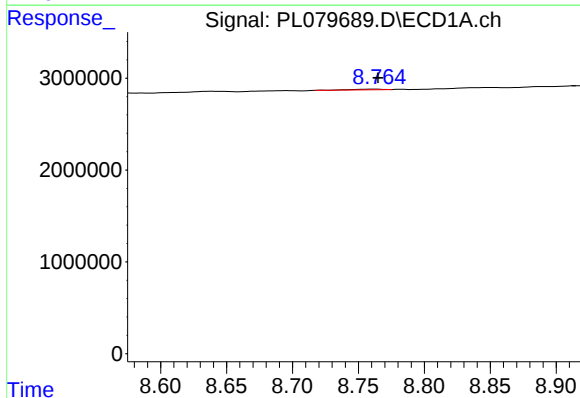

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.001 min
Response: 97125
Conc: 0.05 ng/ml

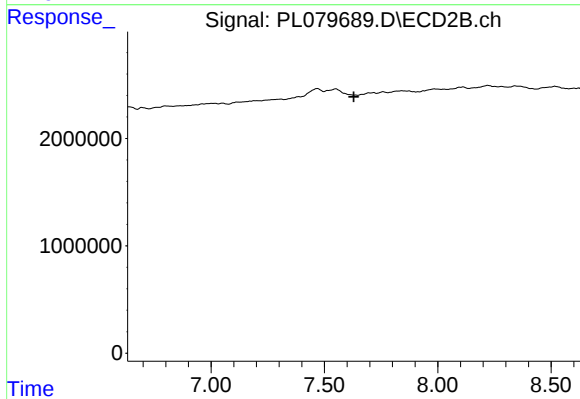

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.629 min
Response: 0
Conc: N.D.