

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121323\
 Data File : PL087142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 17:46
 Operator : AR\AJ
 Sample : 05791-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MW-1B-U-DD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/14/2023
 Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 23:35:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 17:22:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	2.704	64698492	18213058	17.732m	18.441m
2)	SA Decachlor...	9.051	7.902	41048949	12866355	13.562	12.560

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121323\
Data File : PL087142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2023 17:46
Operator : AR\AJ
Sample : 05791-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MW-1B-U-DD


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/14/2023
Supervised By : Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 23:35:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 17:22:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

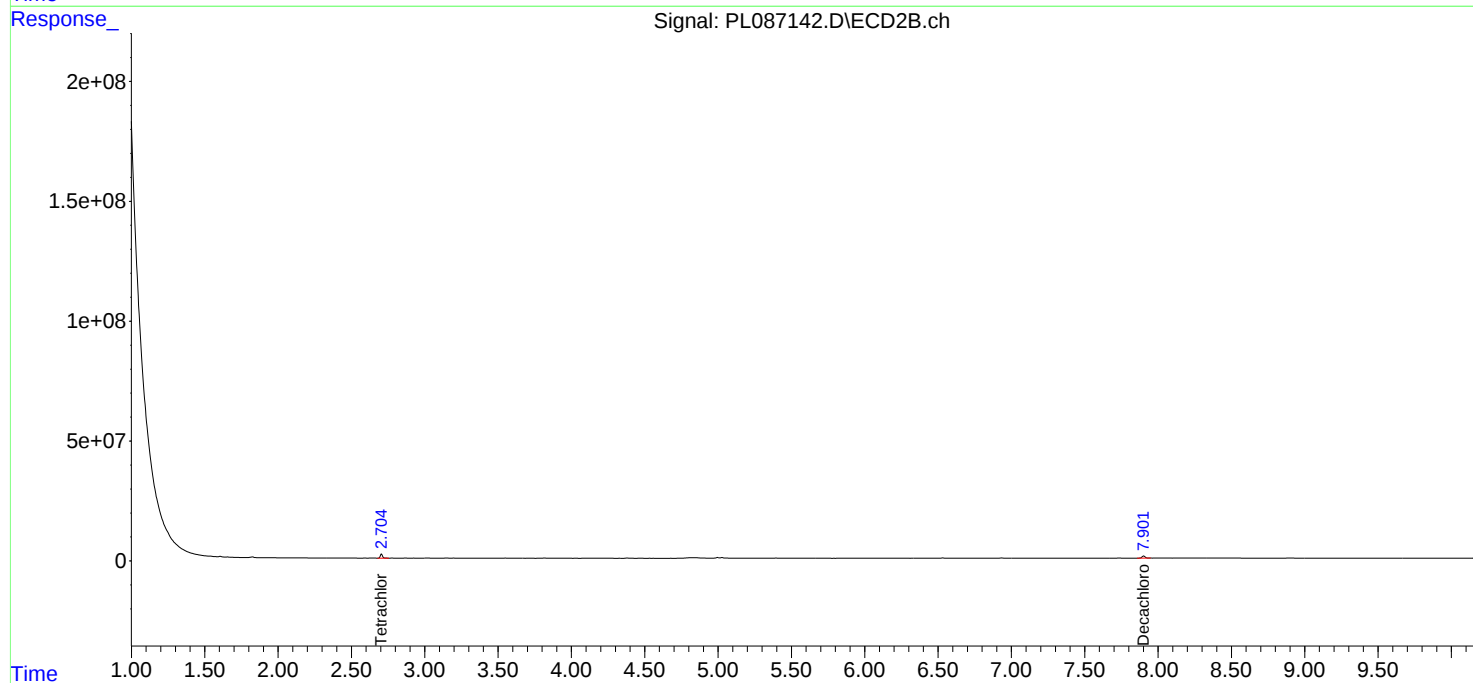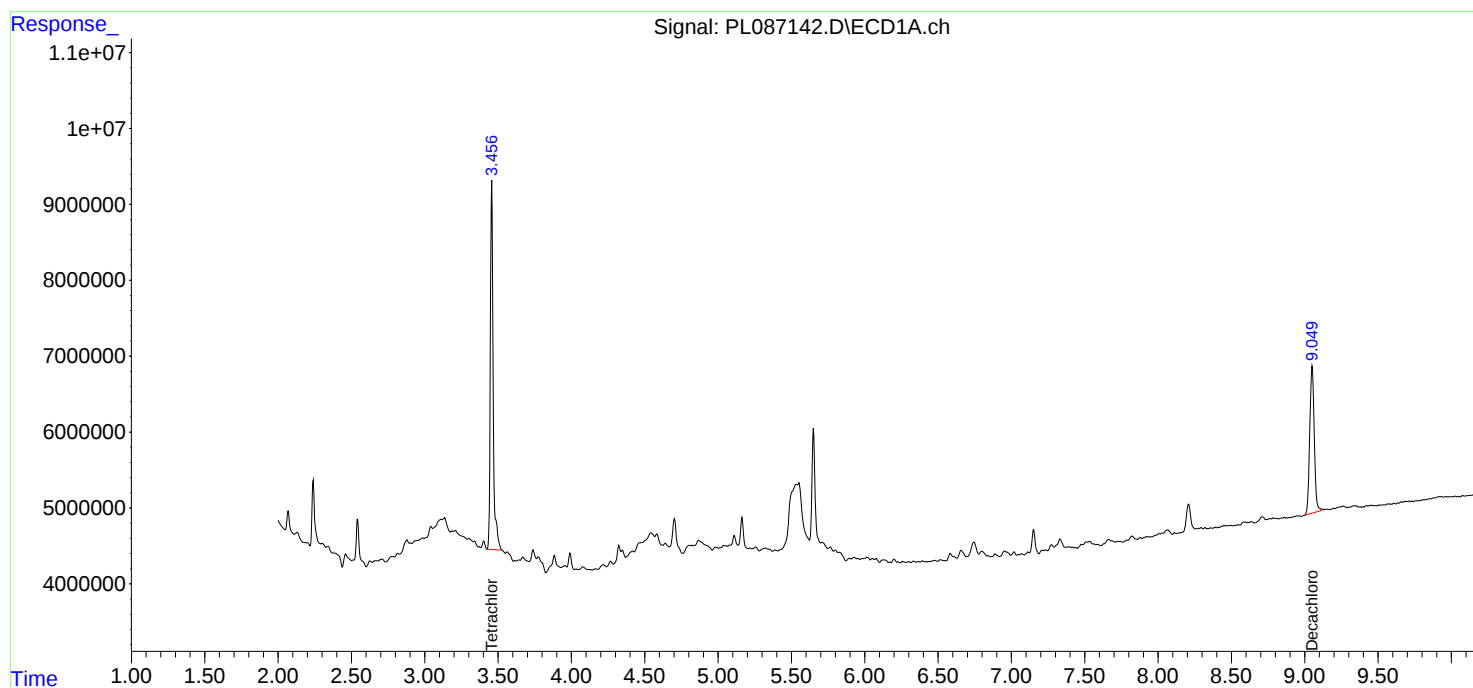

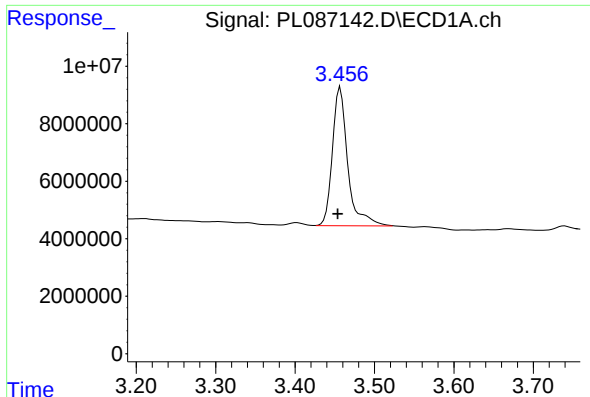


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.002 min
Response: 64698492
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
MW-1B-U-DD


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

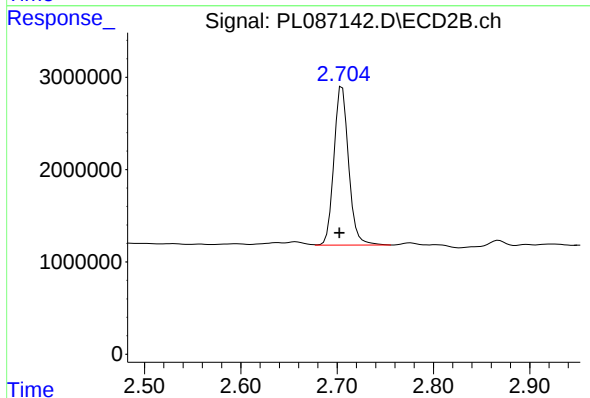


#1 Tetrachloro-m-xylene

R.T.: 2.704 min
Delta R.T.: 0.002 min
Response: 18213058
Conc: 18.44 ng/ml m

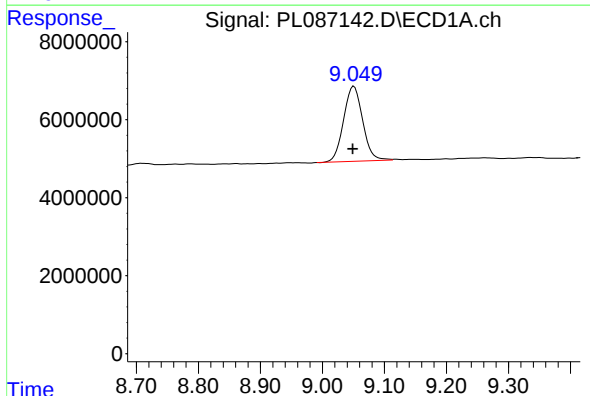

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: 0.002 min
Response: 41048949
Conc: 13.56 ng/ml

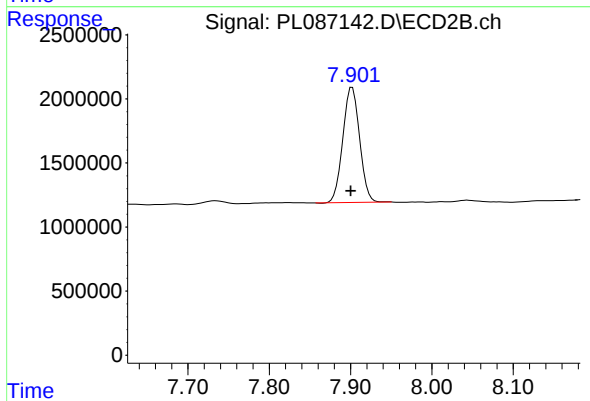

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.002 min
Response: 12866355
Conc: 12.56 ng/ml