

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121323\
 Data File : PL087145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 18:27
 Operator : AR\AJ
 Sample : 05791-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MW-1B-EE-NN

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/14/2023
 Supervised By : Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 23:35:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 12 17:22:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.455	2.704	56640609	17841647	15.524m	18.065m
28) SA Decachlor...	9.050	7.900	29472975	9018389	9.737	8.804

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121323\
Data File : PL087145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2023 18:27
Operator : AR\AJ
Sample : 05791-11
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MW-1B-EE-NN


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/14/2023
Supervised By : Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 23:35:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121223.M
Quant Title : GC Extractables
QLast Update : Tue Dec 12 17:22:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

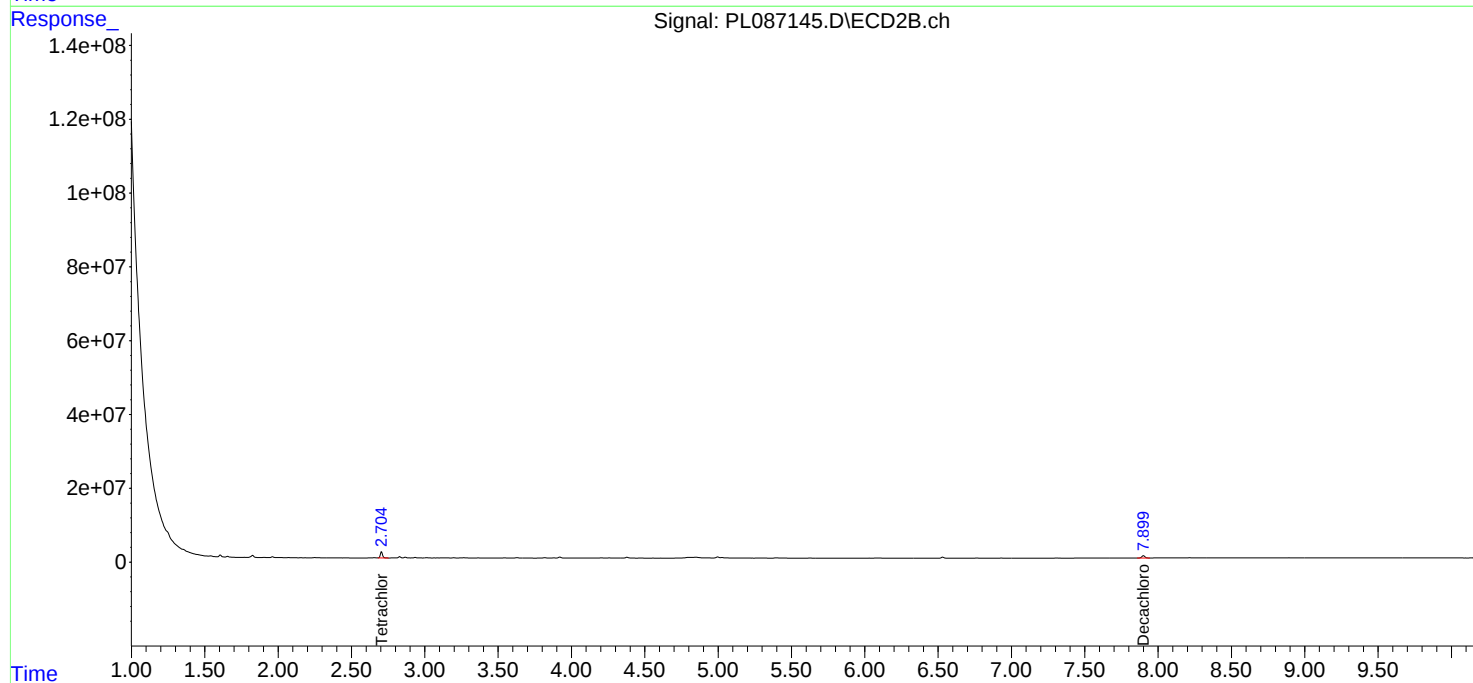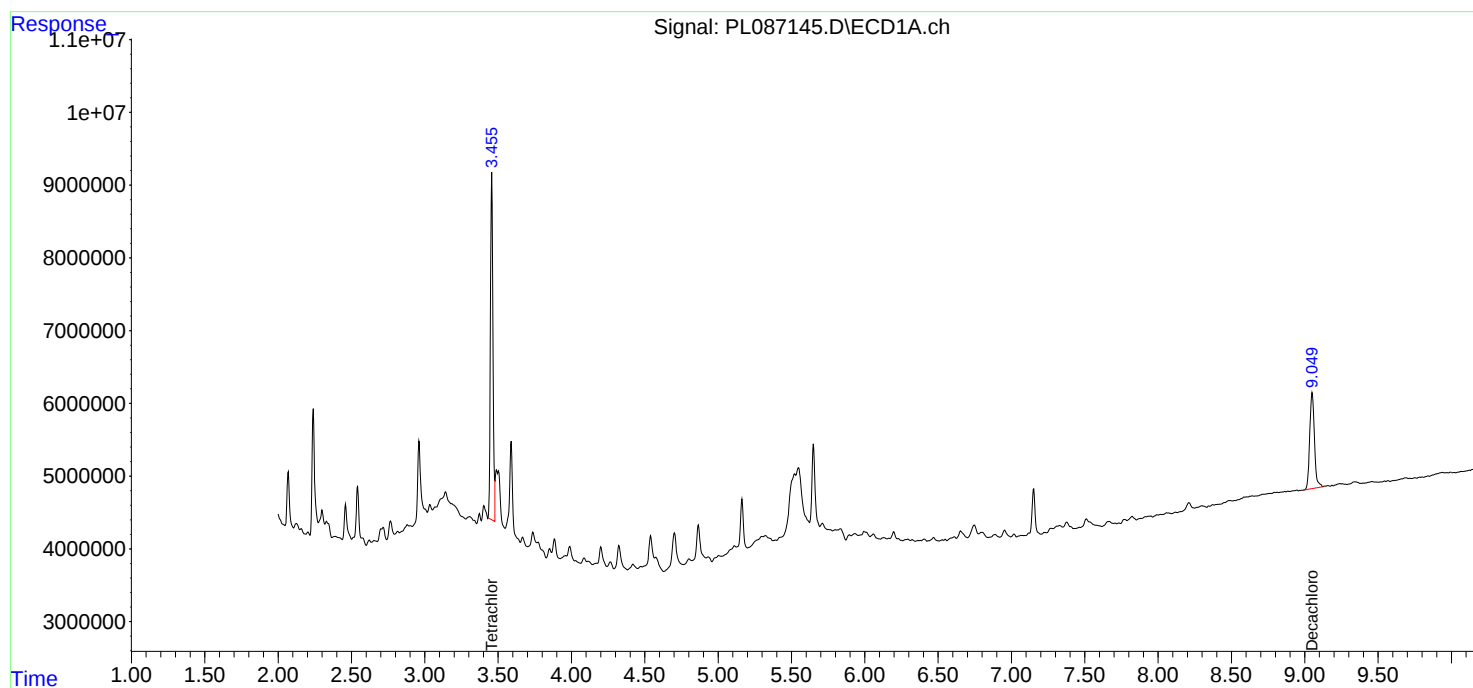

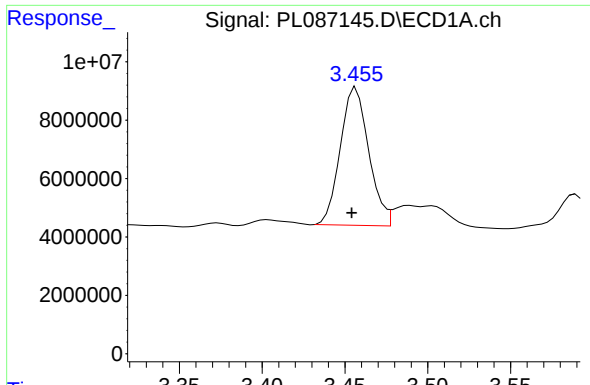


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.001 min
Response: 56640609
Conc: 15.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
MW-1B-EE-NN


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

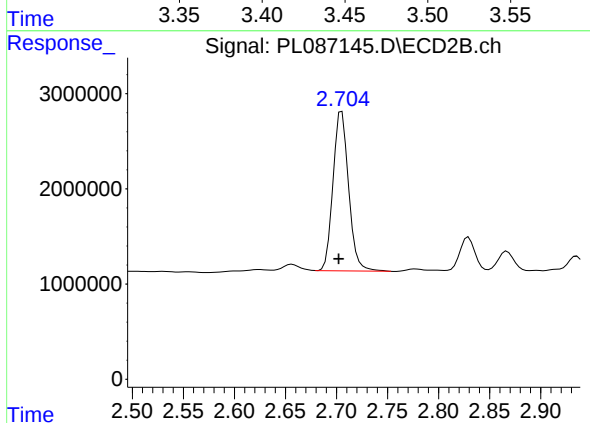


#1 Tetrachloro-m-xylene

R.T.: 2.704 min
Delta R.T.: 0.002 min
Response: 17841647
Conc: 18.06 ng/ml m

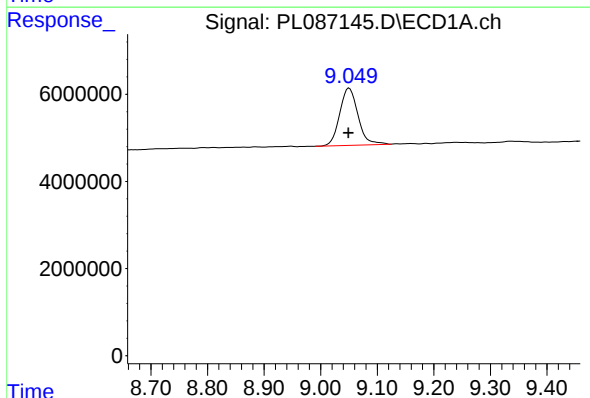

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: 0.002 min
Response: 29472975
Conc: 9.74 ng/ml

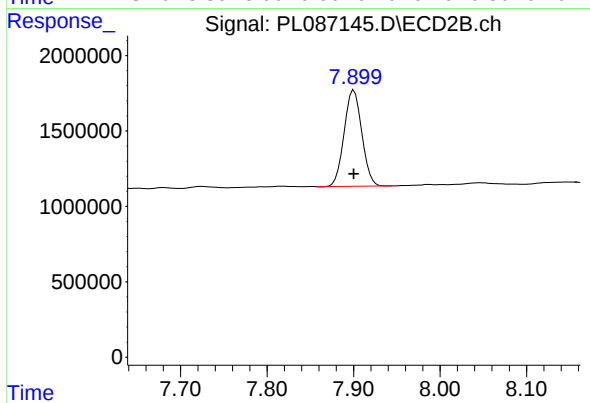

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 9018389
Conc: 8.80 ng/ml