

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
 Data File : PL043135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 10:49
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 22:21:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.098	146.4E6	72702021	23.865	24.529
28)	SA Decachlor...	8.200	9.223	149.0E6	59198004	22.821	22.694
Target Compounds							
2)	A alpha-BHC	3.896	0.000	4125966	0	0.436	N.D. #
6)	B beta-BHC	4.398f	0.000	5226079	0	1.417	N.D. #
7)	B delta-BHC	0.000	5.144f	0	3289591	N.D.	0.765 #
8)	B Heptachlo...	0.000	5.998	0	1612410	N.D.	0.425 #
20)	A Methoxychlor	6.885f	0.000	4031828	0	1.202	N.D. #
23)	Chlordane-1	4.362	5.144	915032	3289591	3.405	23.275 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
Data File : PL043135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 10:49
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 22:21:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

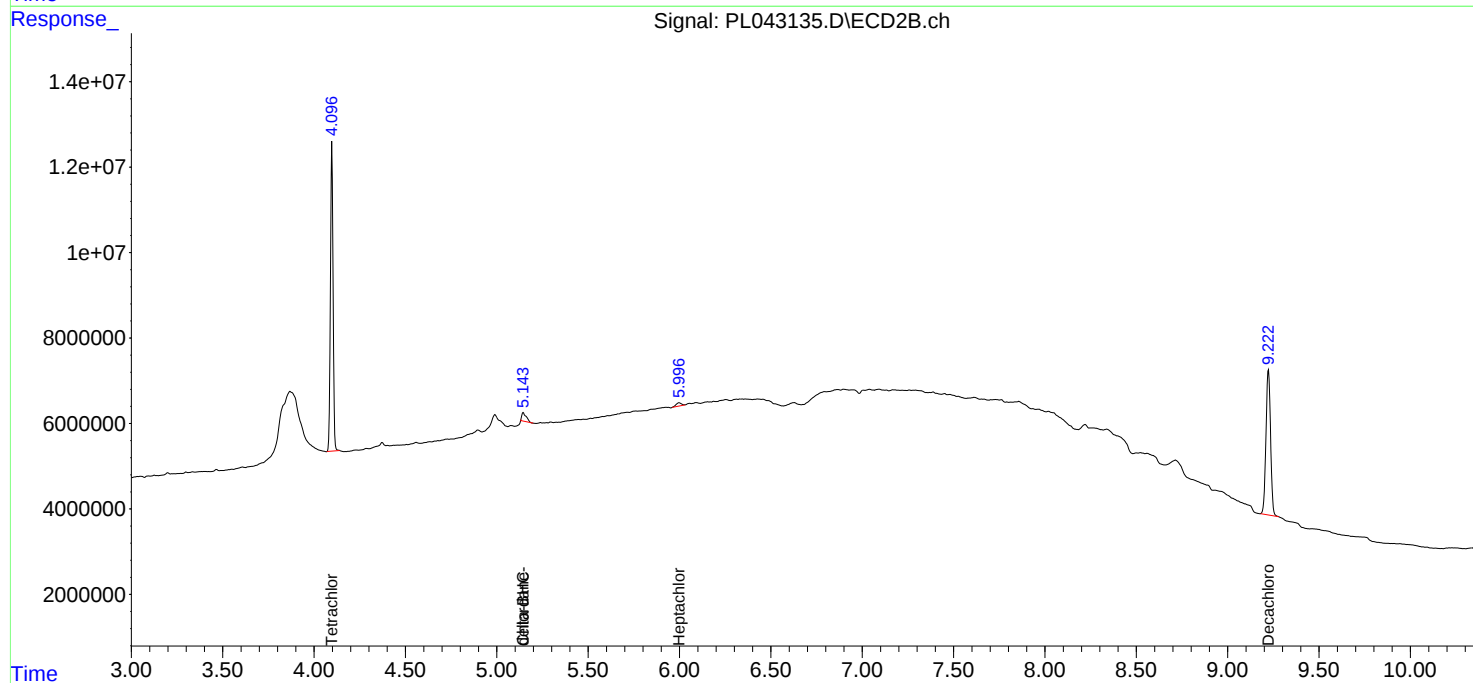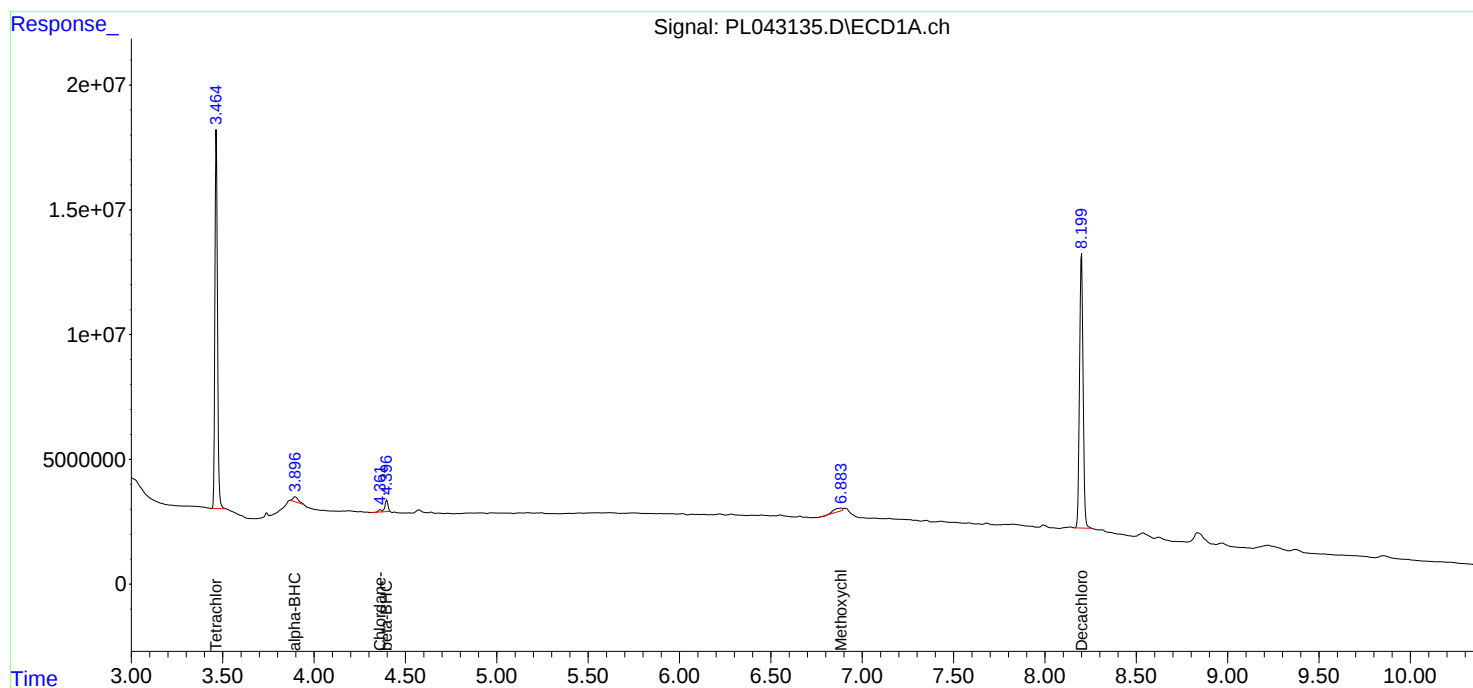


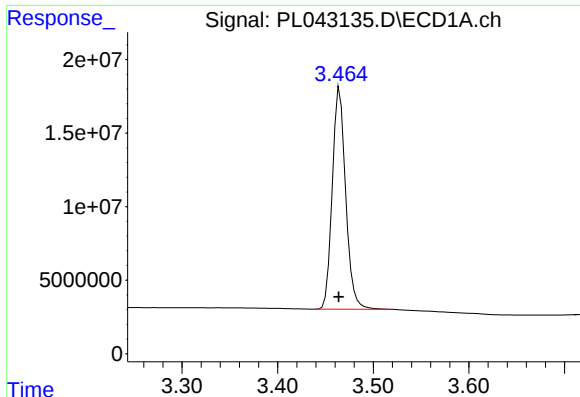

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 146363725
Conc: 23.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

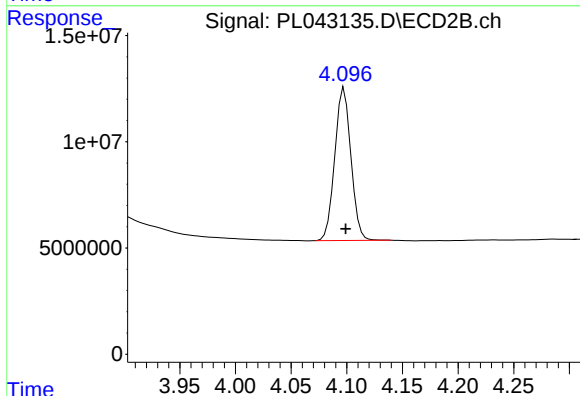


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.001 min
Response: 72702021
Conc: 24.53 ng/ml

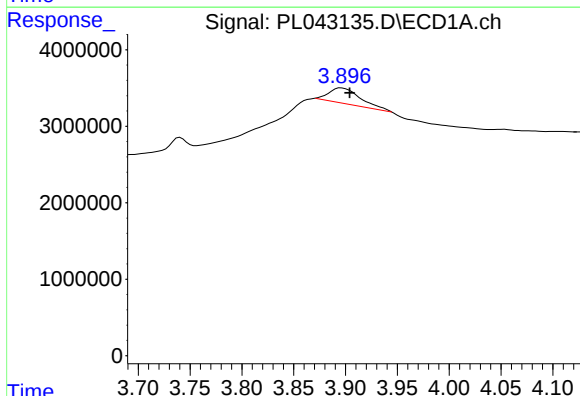


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: -0.008 min
Response: 4125966
Conc: 0.44 ng/ml

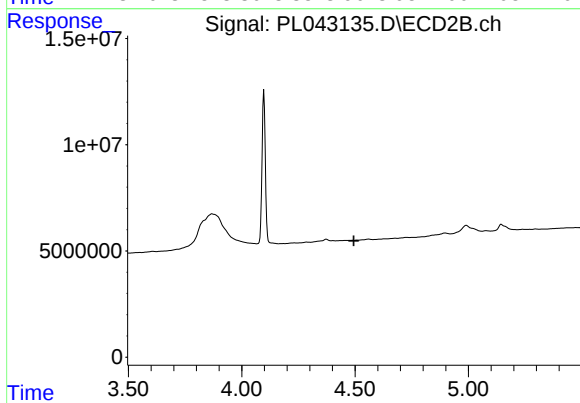

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

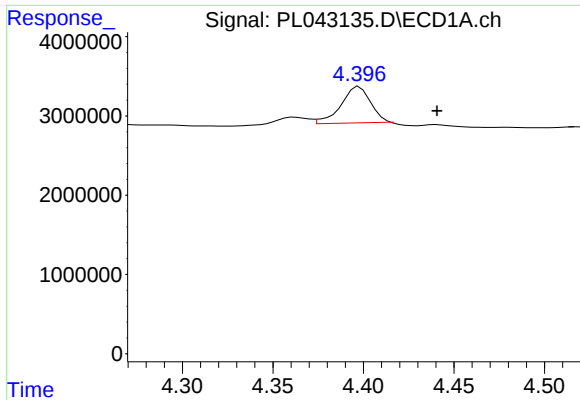

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 5226079
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

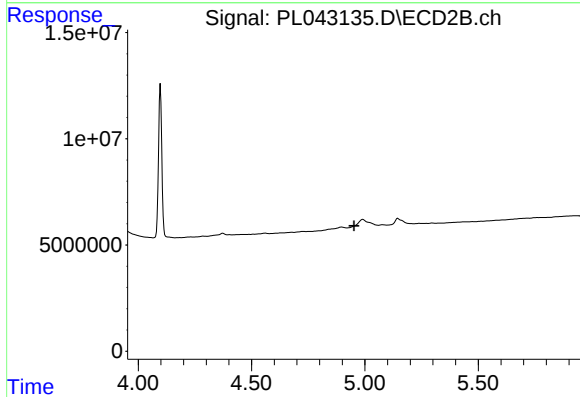


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

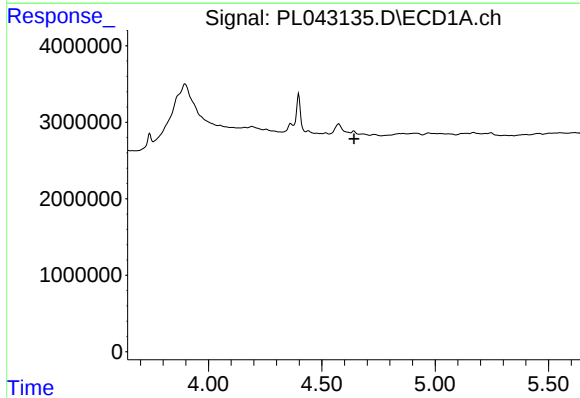


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

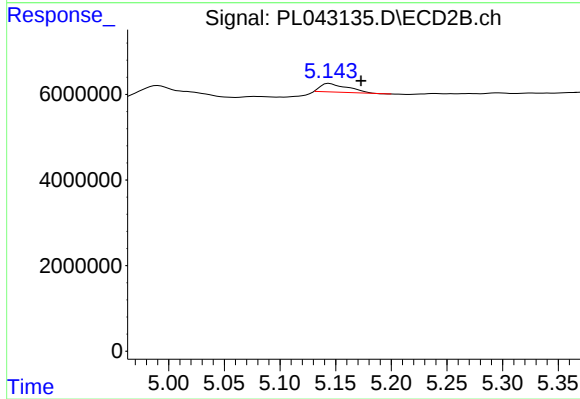

#7 delta-BHC


R.T.: 5.144 min
Delta R.T.: -0.028 min
Response: 3289591
Conc: 0.77 ng/ml

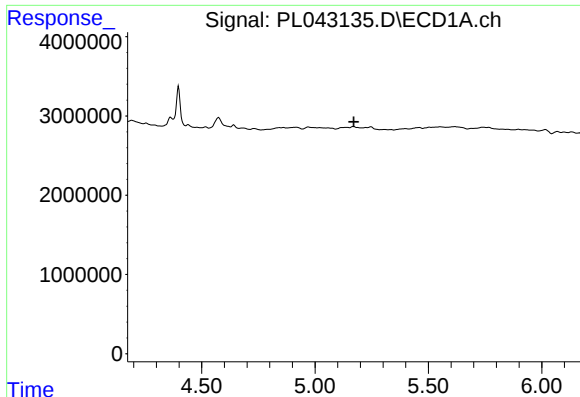

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

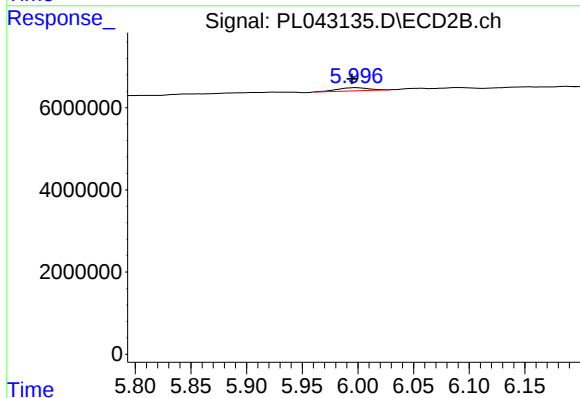


#8 Heptachlor epoxide

R.T.: 5.998 min
Delta R.T.: 0.003 min
Response: 1612410
Conc: 0.43 ng/ml

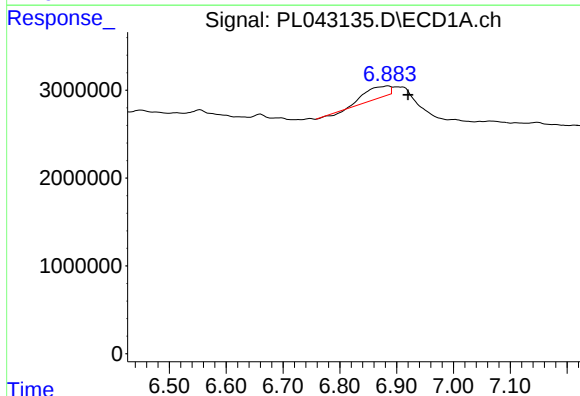


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: -0.035 min
Response: 4031828
Conc: 1.20 ng/ml

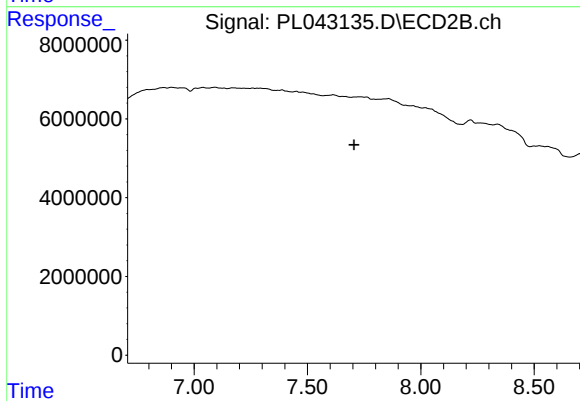

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.705 min
Response: 0
Conc: N.D.

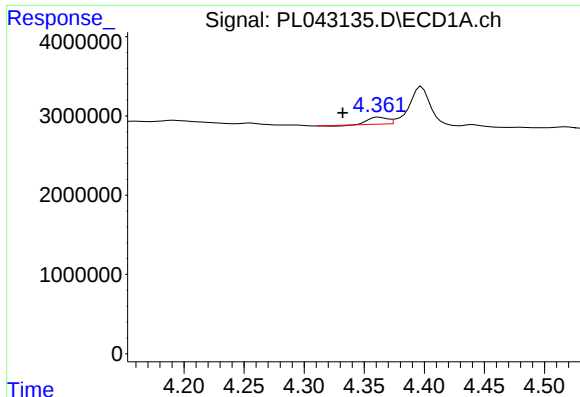

#23 Chlordane-1


R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 915032
Conc: 3.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

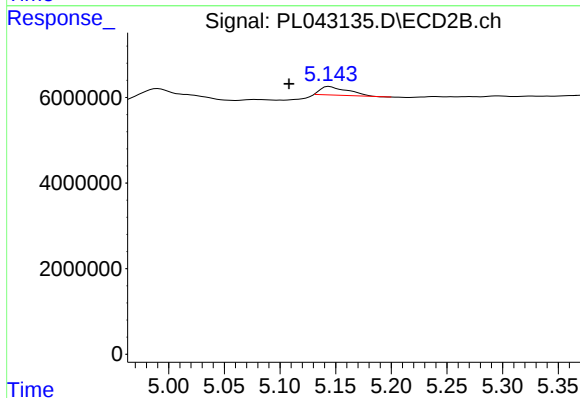


#23 Chlordane-1

R.T.: 5.144 min
Delta R.T.: 0.036 min
Response: 3289591
Conc: 23.28 ng/ml

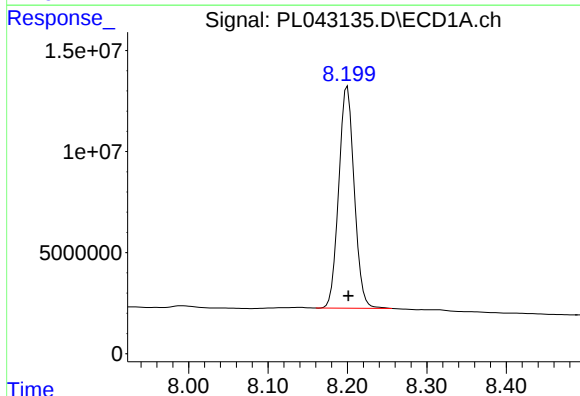

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.001 min
Response: 149023781
Conc: 22.82 ng/ml

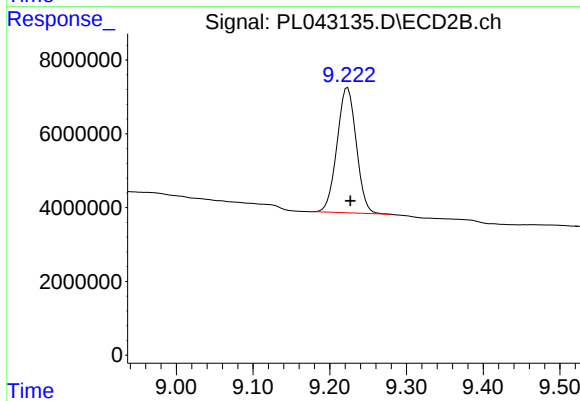

#28 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 59198004
Conc: 22.69 ng/ml