

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
 Data File : PL043139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 12:26
 Operator : AJ\SJ
 Sample : J6376-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 22:21:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.097	109.5E6	56116887	17.859	18.933
28)	SA Decachlor...	8.200	9.224	132.2E6	51761115	20.249	19.843
Target Compounds							
6)	B beta-BHC	4.399f	0.000	2167599	0	0.588	N.D. #
7)	B delta-BHC	0.000	5.153	0	4511783	N.D.	1.050 #
8)	B Heptachlo...	0.000	5.986	0	26694290	N.D.	7.040 #
10)	B gamma-Chl...	0.000	6.183f	0	2770534	N.D.	0.754 #
14)	MA Endrin	6.019	0.000	4030485	0	0.560	N.D. #
16)	A 4,4'-DDD	6.069f	0.000	1534024	0	0.270	N.D. #
17)	MA 4,4'-DDT	0.000	7.302f	0	2148019	N.D.	0.731 #
23)	Chlordane-1	4.399	5.153	2167599	4511783	8.067	31.923 #
25)	Chlordane-3	0.000	6.183	0	2770534	N.D.	5.642 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
Data File : PL043139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 12:26
Operator : AJ\SJ
Sample : J6376-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 22:21:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

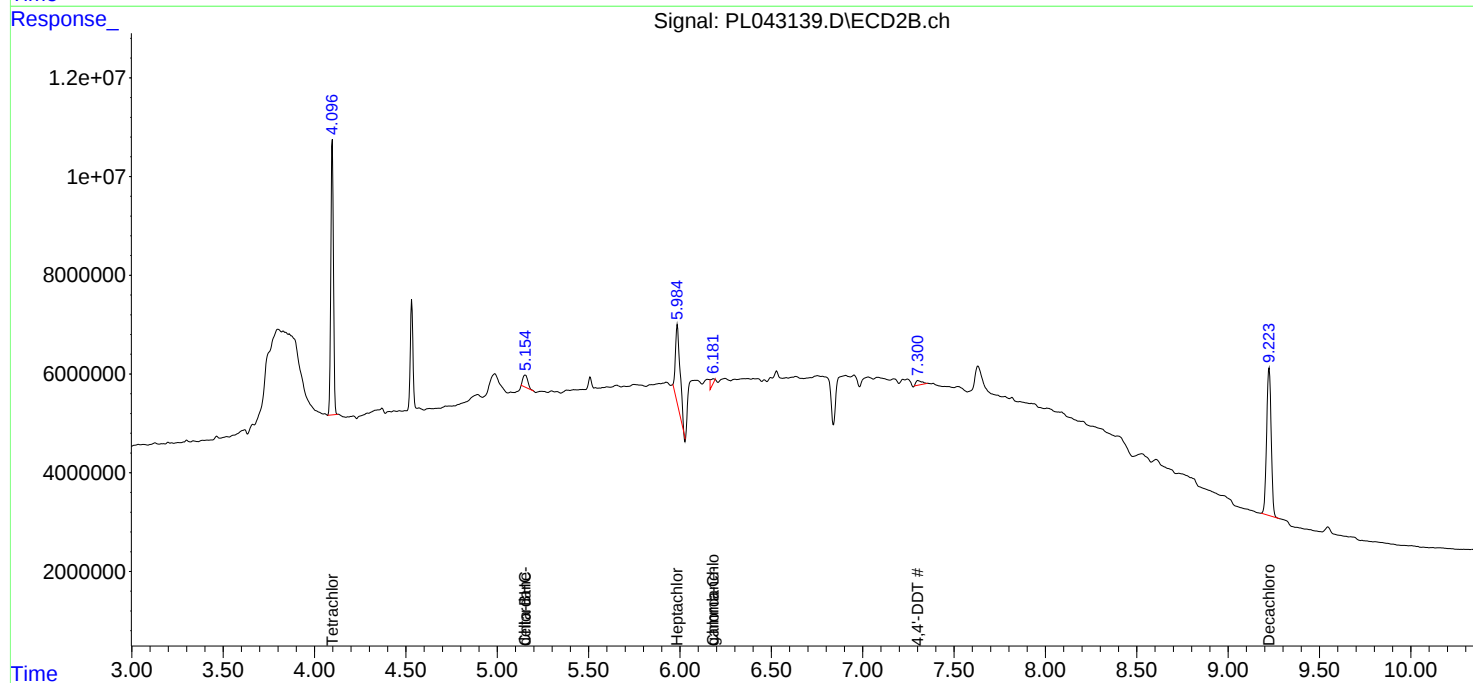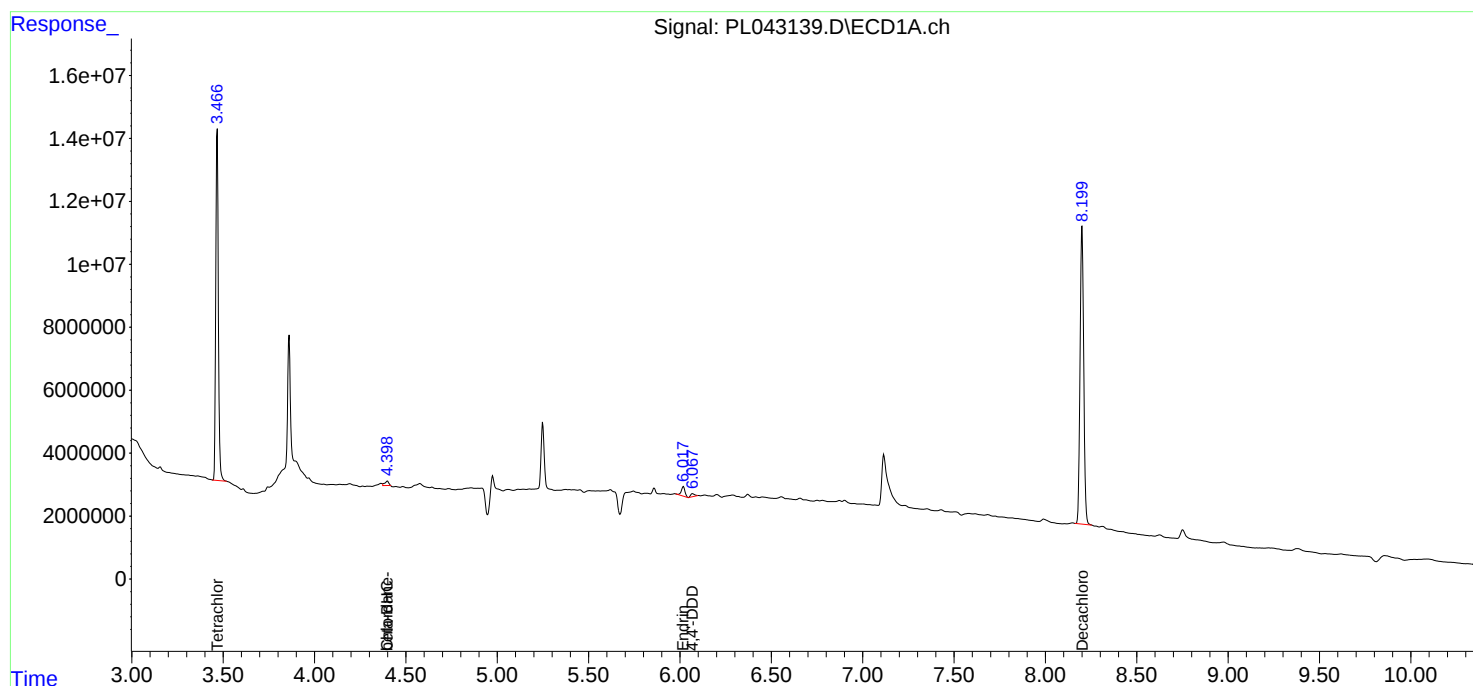


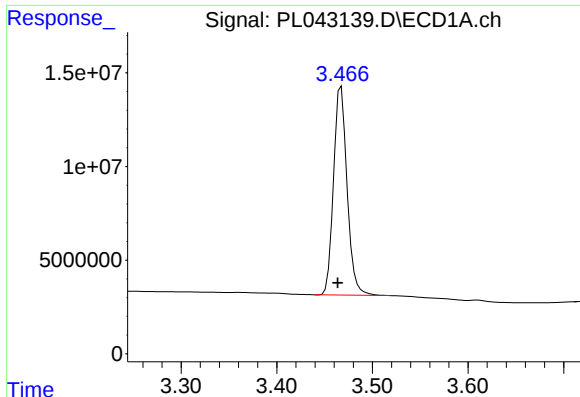

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.003 min
Response: 109526077
Conc: 17.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

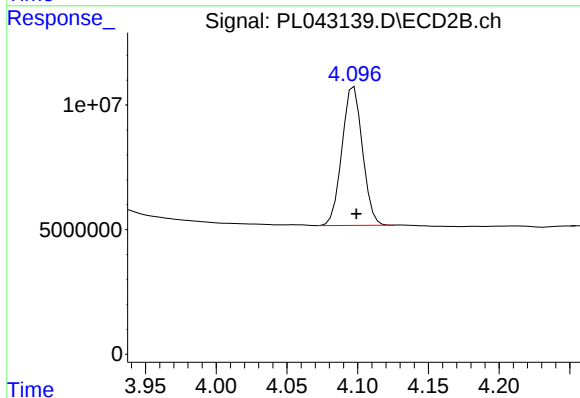


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.002 min
Response: 56116887
Conc: 18.93 ng/ml

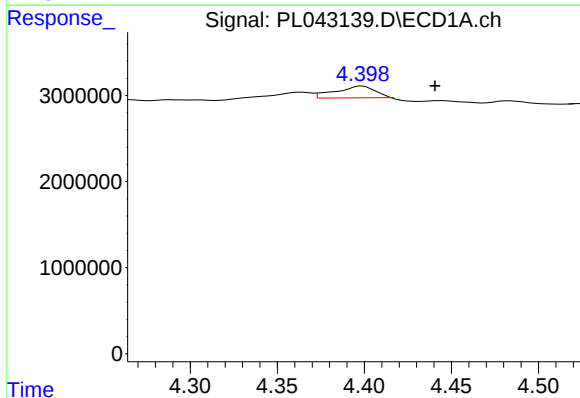


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 2167599
Conc: 0.59 ng/ml

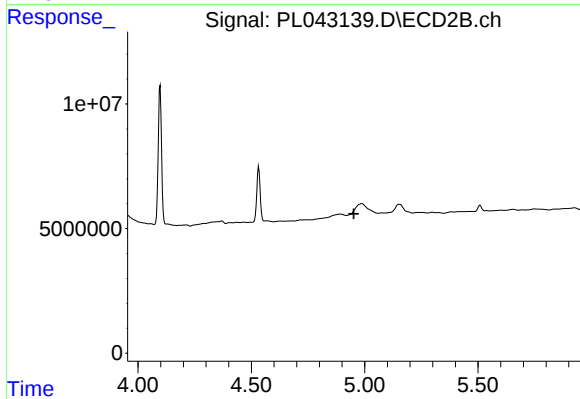

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

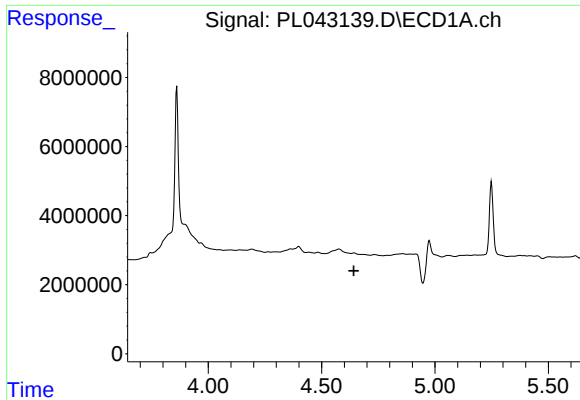

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

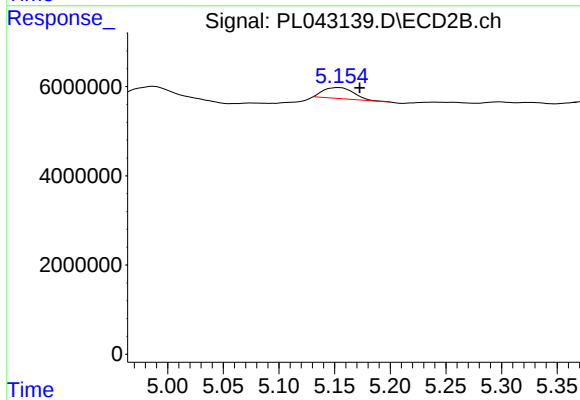


#7 delta-BHC

R.T.: 5.153 min
Delta R.T.: -0.019 min
Response: 4511783
Conc: 1.05 ng/ml

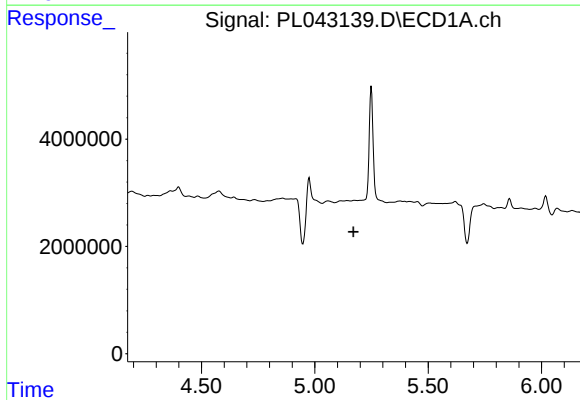


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

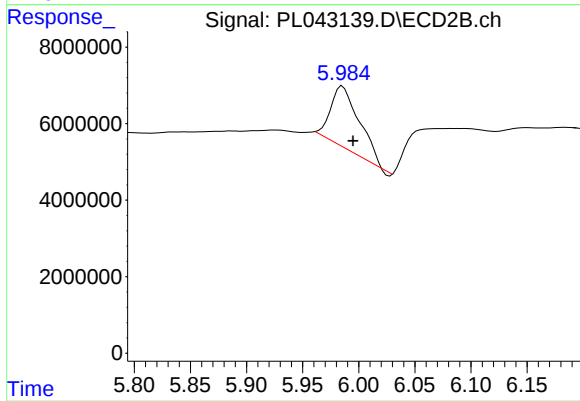

#8 Heptachlor epoxide


R.T.: 5.986 min
Delta R.T.: -0.009 min
Response: 26694290
Conc: 7.04 ng/ml

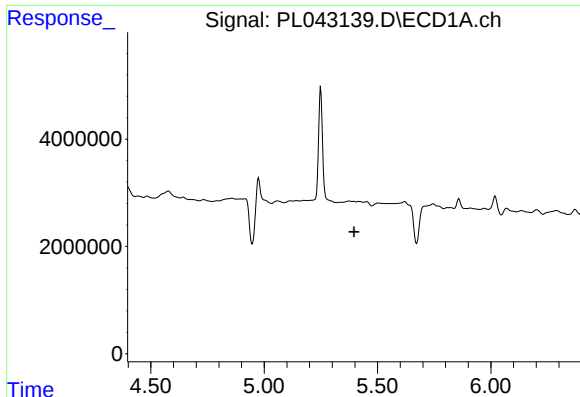

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

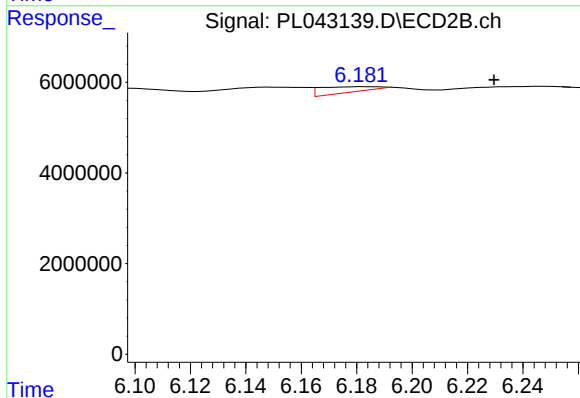


#10 gamma-Chlordane

R.T.: 6.183 min
Delta R.T.: -0.046 min
Response: 2770534
Conc: 0.75 ng/ml

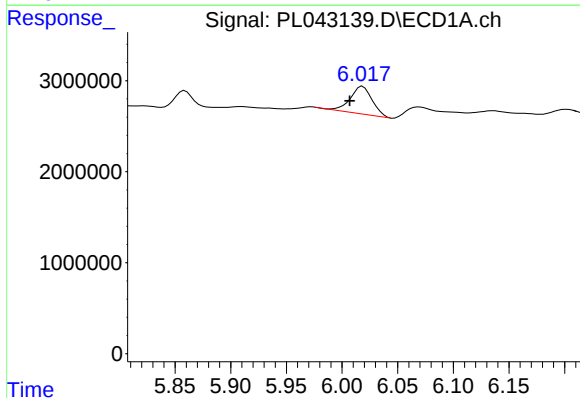


#14 Endrin

R.T.: 6.019 min
Delta R.T.: 0.012 min
Response: 4030485
Conc: 0.56 ng/ml

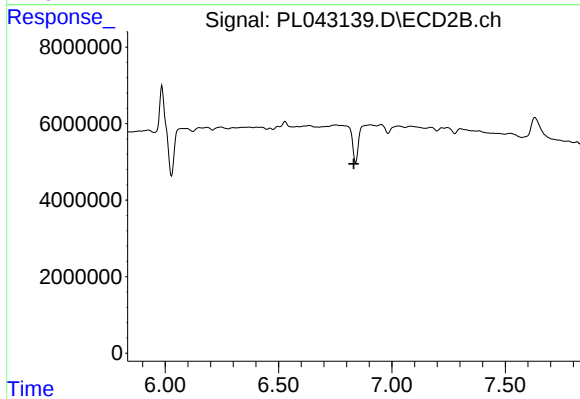

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.832 min
Response: 0
Conc: N.D.

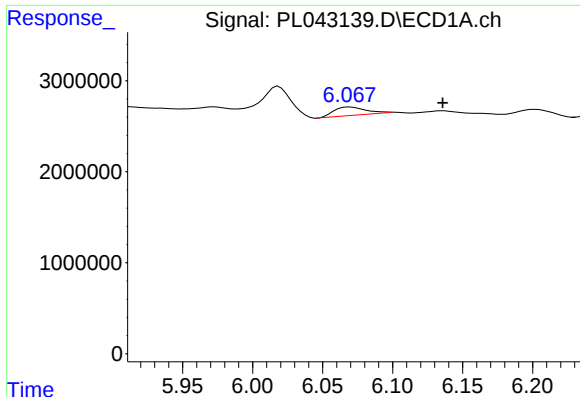

#16 4,4'-DDD


R.T.: 6.069 min
Delta R.T.: -0.067 min
Response: 1534024
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

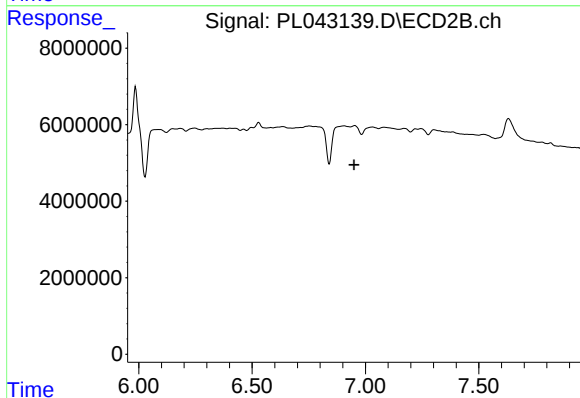


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

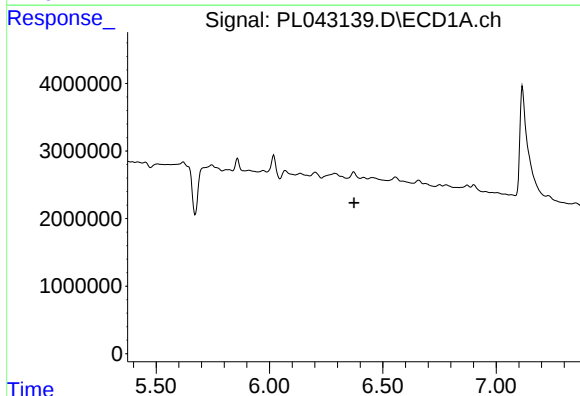


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.374 min
Response: 0
Conc: N.D.

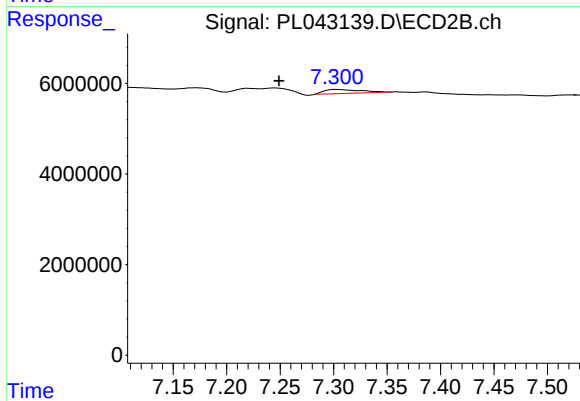

#17 4,4'-DDT


R.T.: 7.302 min
Delta R.T.: 0.053 min
Response: 2148019
Conc: 0.73 ng/ml

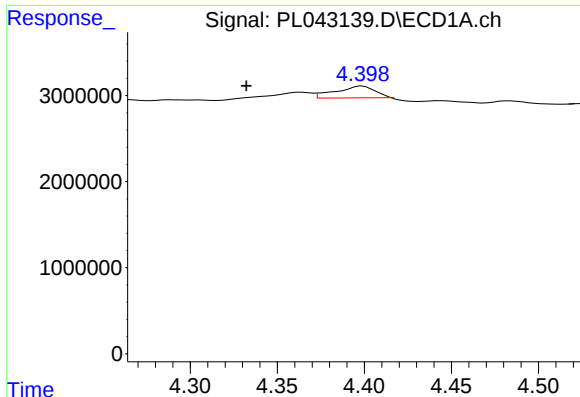

#23 Chlordane-1


R.T.: 4.399 min
Delta R.T.: 0.067 min
Response: 2167599
Conc: 8.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

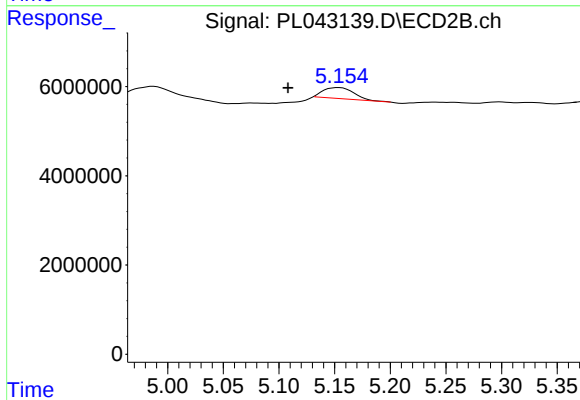


#23 Chlordane-1

R.T.: 5.153 min
Delta R.T.: 0.045 min
Response: 4511783
Conc: 31.92 ng/ml

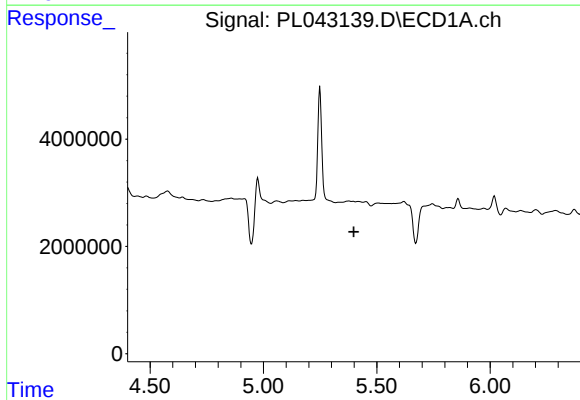


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

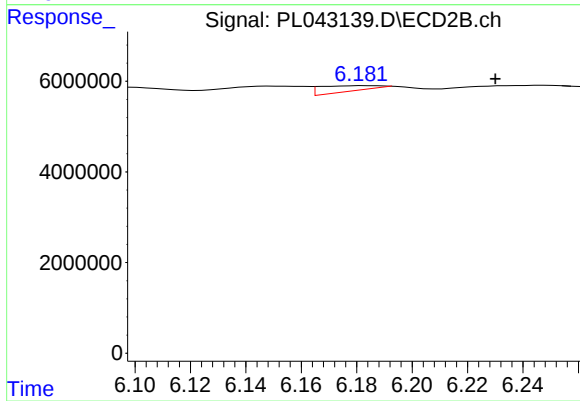

#25 Chlordane-3


R.T.: 6.183 min
Delta R.T.: -0.047 min
Response: 2770534
Conc: 5.64 ng/ml

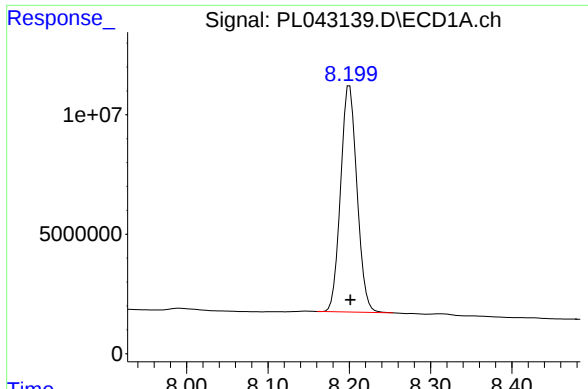

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: 0.000 min
Response: 132224142
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

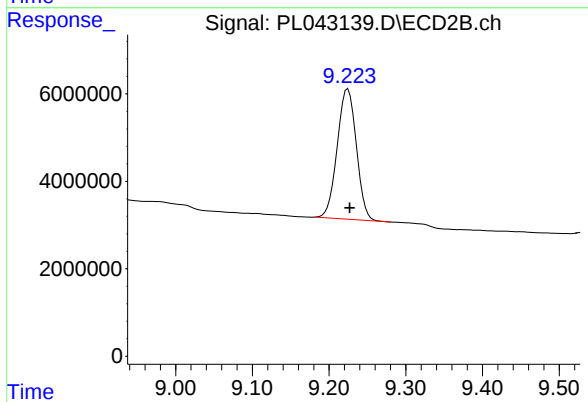

#28 Decachlorobiphenyl

R.T.: 9.224 min
Delta R.T.: -0.002 min
Response: 51761115
Conc: 19.84 ng/ml