

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
 Data File : PL043144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 15:22
 Operator : AJ\SJ
 Sample : PB115698BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 22:23:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.097	117.2E6	58872275	19.110	19.863
28)	SA Decachlor...	8.208	9.227	130.7E6	52482749	20.013	20.120
Target Compounds							
2)	A alpha-BHC	3.864f	0.000	2012992	0	0.213	N.D. #
6)	B beta-BHC	4.406f	0.000	1485088	0	0.403	N.D. #
7)	B delta-BHC	0.000	5.146f	0	3939388	N.D.	0.917 #
8)	B Heptachlo...	0.000	5.934f	0	5844910	N.D.	1.541 #
9)	A Endosulfan I	0.000	6.320	0	6203511	N.D.	1.827 #
11)	B alpha-Chl...	0.000	6.320	0	6203511	N.D.	1.725 #
14)	MA Endrin	0.000	6.860	0	540785	N.D.	0.173 #
23)	Chlordane-1	4.370	5.146	329250	3939388	1.225	27.873 #
26)	Chlordane-4	0.000	6.320	0	6203511	N.D.	10.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
Data File : PL043144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 15:22
Operator : AJ\SJ
Sample : PB115698BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 22:23:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

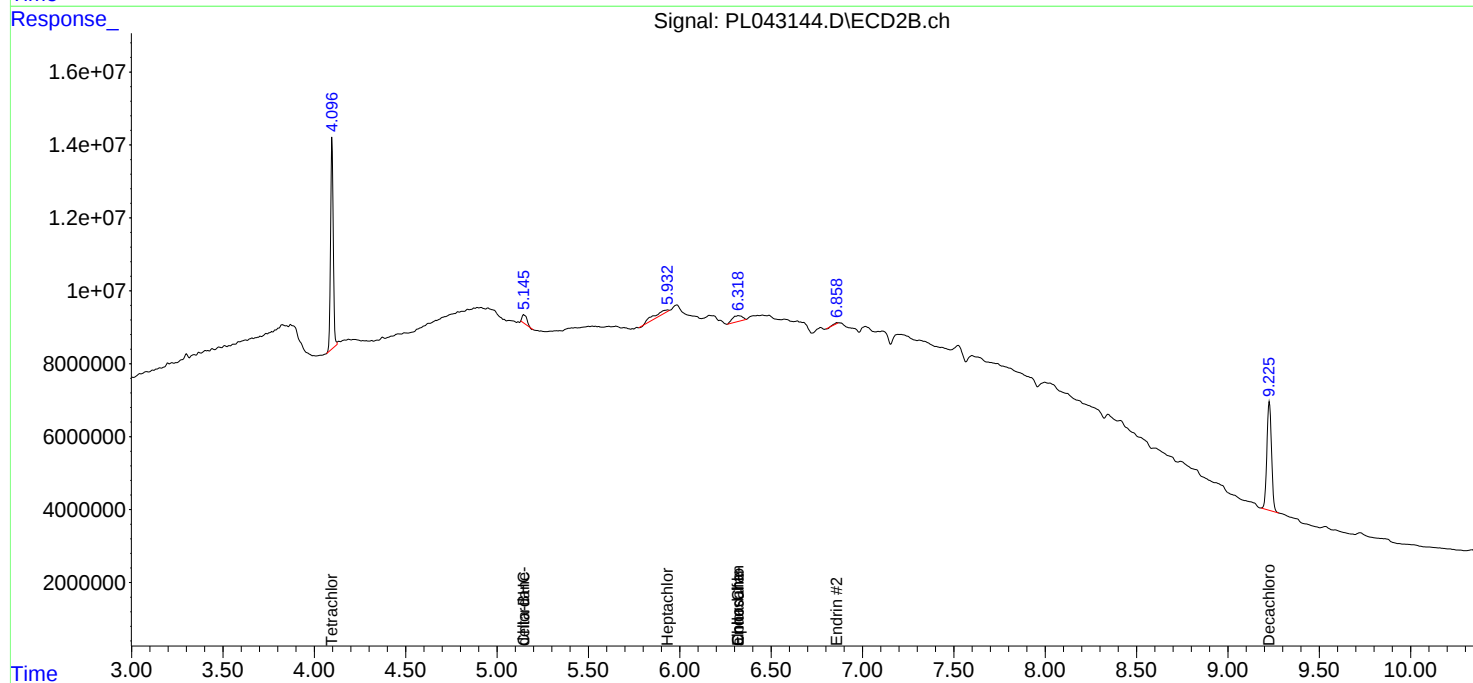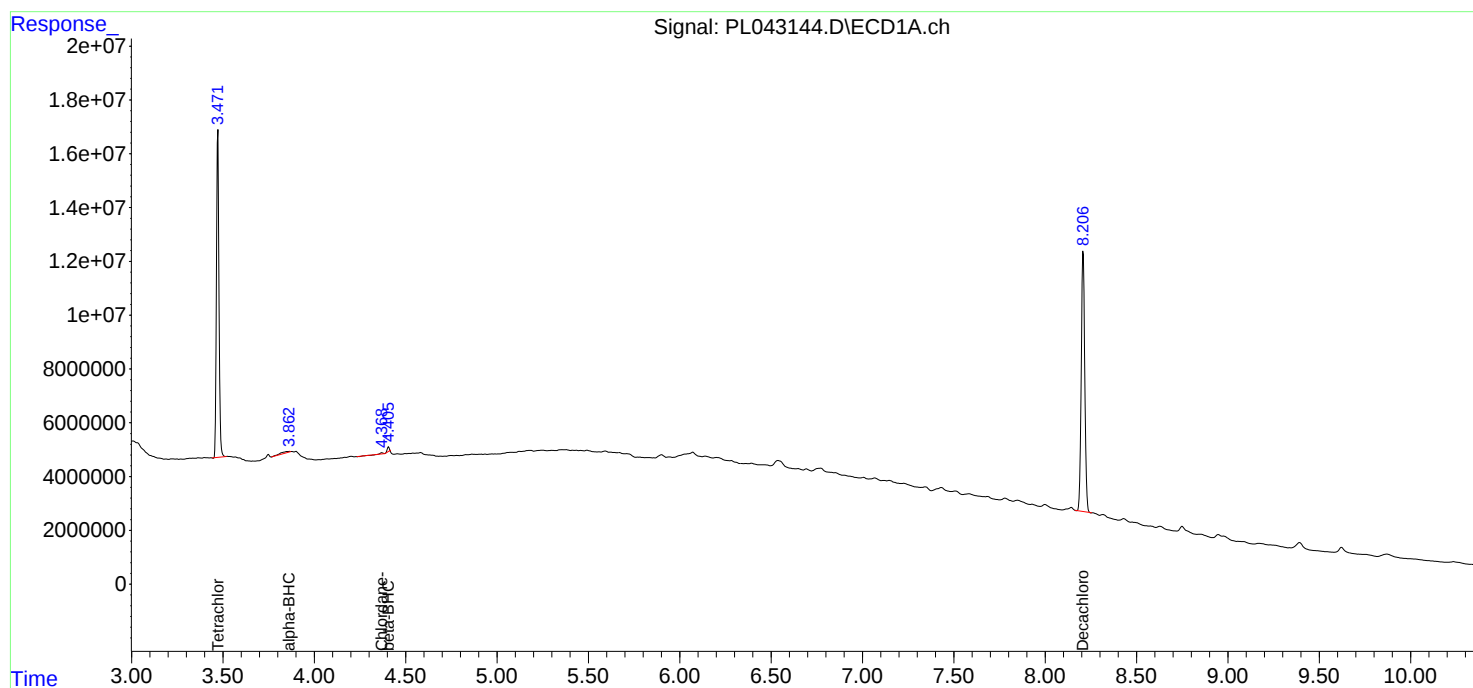


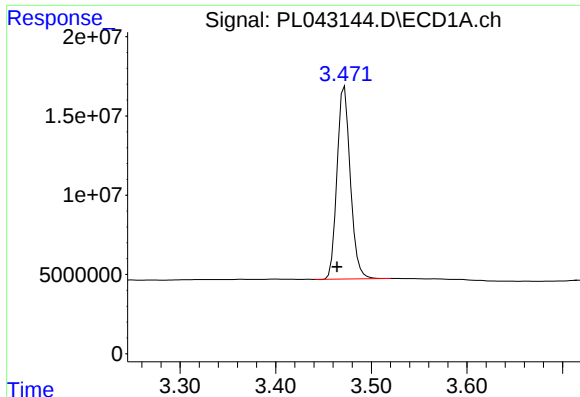

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: 0.008 min
Response: 117199404
Conc: 19.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

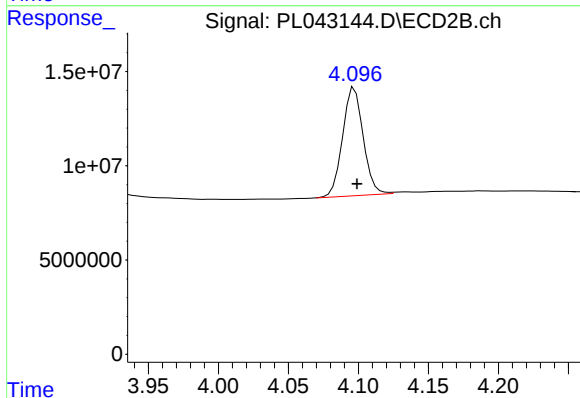


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.002 min
Response: 58872275
Conc: 19.86 ng/ml

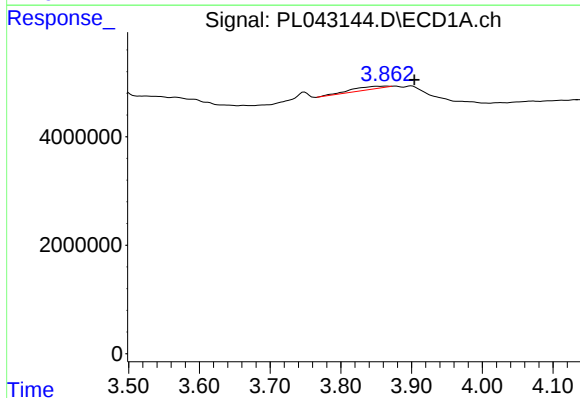


#2 alpha-BHC

R.T.: 3.864 min
Delta R.T.: -0.040 min
Response: 2012992
Conc: 0.21 ng/ml

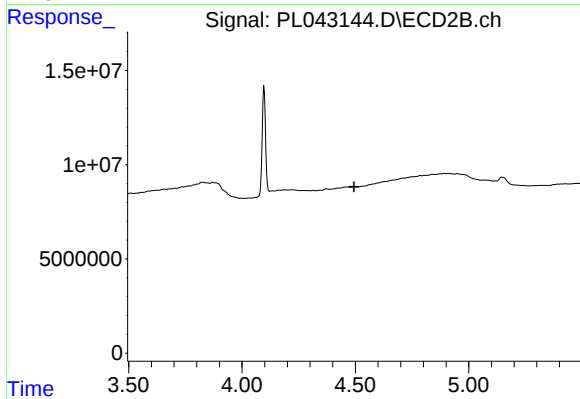

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

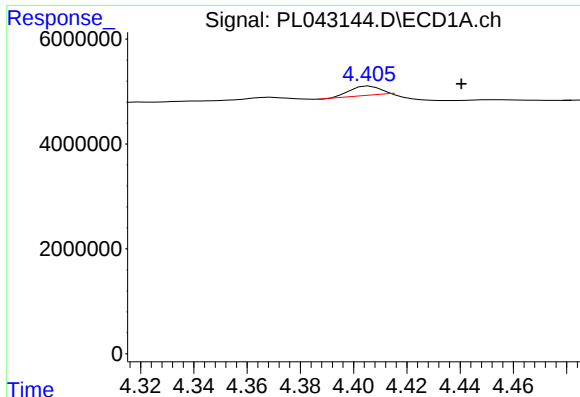

#6 beta-BHC


R.T.: 4.406 min
Delta R.T.: -0.034 min
Response: 1485088
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

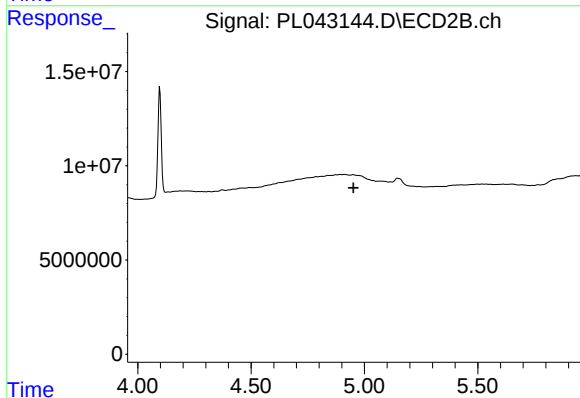


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

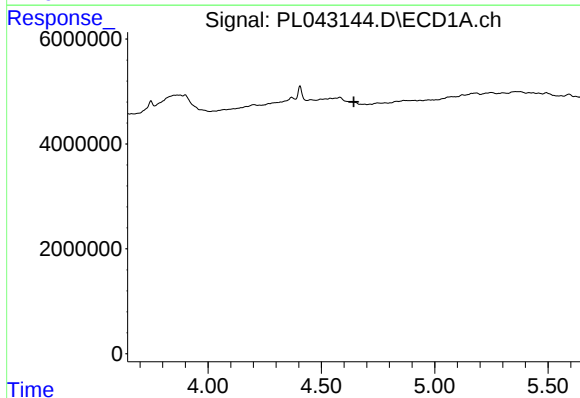


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

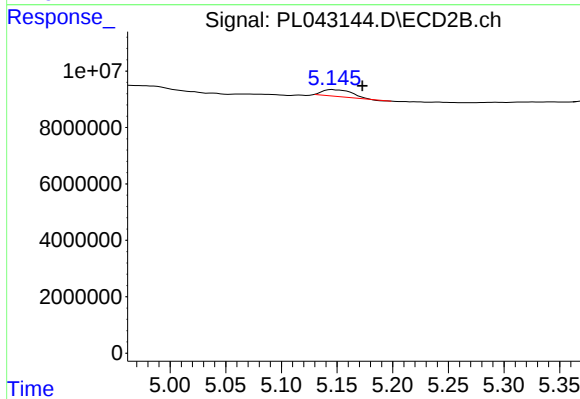

#7 delta-BHC


R.T.: 5.146 min
Delta R.T.: -0.027 min
Response: 3939388
Conc: 0.92 ng/ml

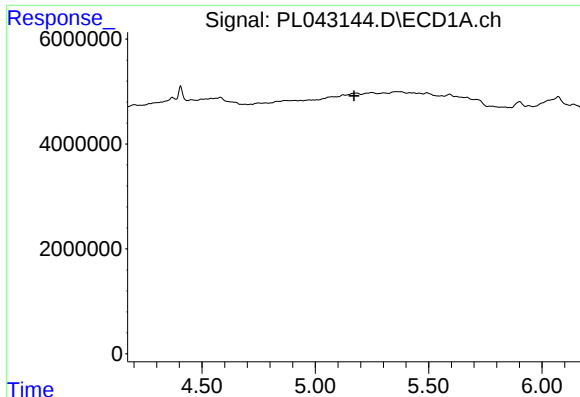

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

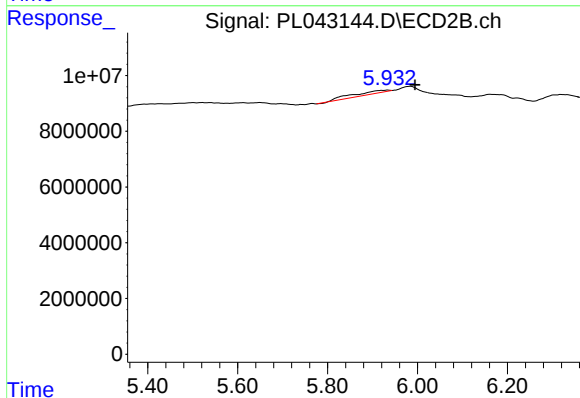


#8 Heptachlor epoxide

R.T.: 5.934 min
Delta R.T.: -0.061 min
Response: 5844910
Conc: 1.54 ng/ml

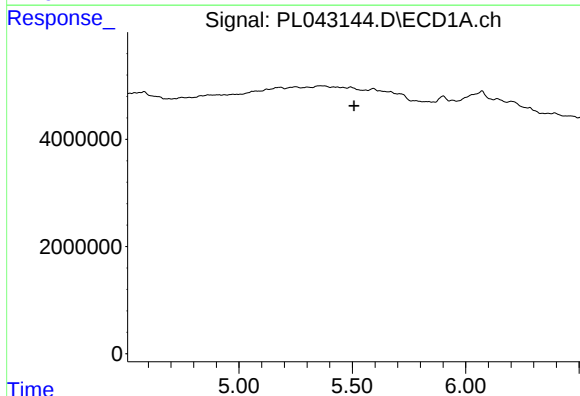


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

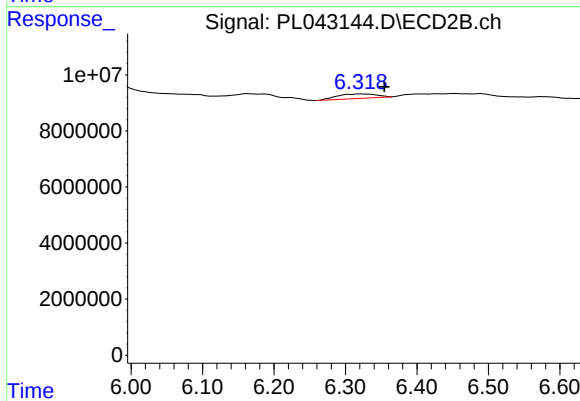

#9 Endosulfan I


R.T.: 6.320 min
Delta R.T.: -0.035 min
Response: 6203511
Conc: 1.83 ng/ml

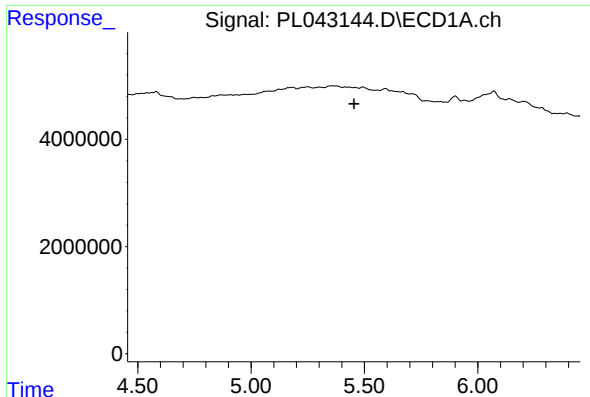

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

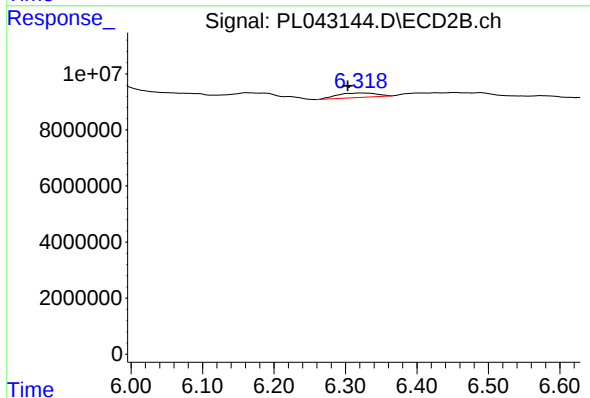


#11 alpha-Chlordane

R.T.: 6.320 min
Delta R.T.: 0.017 min
Response: 6203511
Conc: 1.72 ng/ml

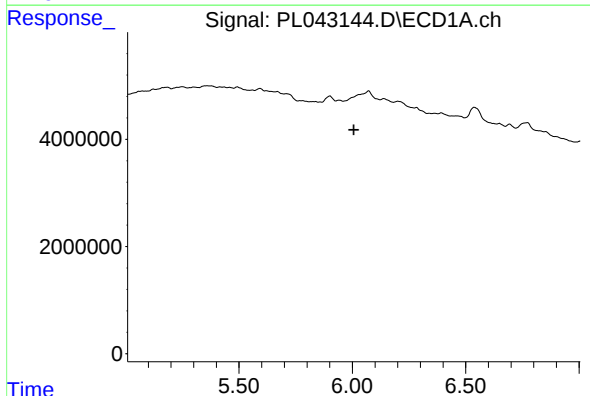


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.007 min
Response: 0
Conc: N.D.

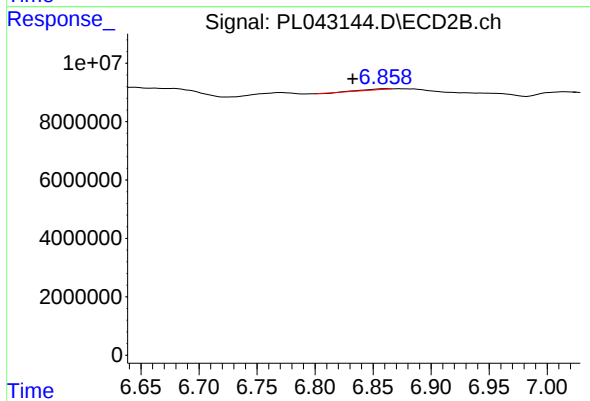

#14 Endrin


R.T.: 6.860 min
Delta R.T.: 0.027 min
Response: 540785
Conc: 0.17 ng/ml

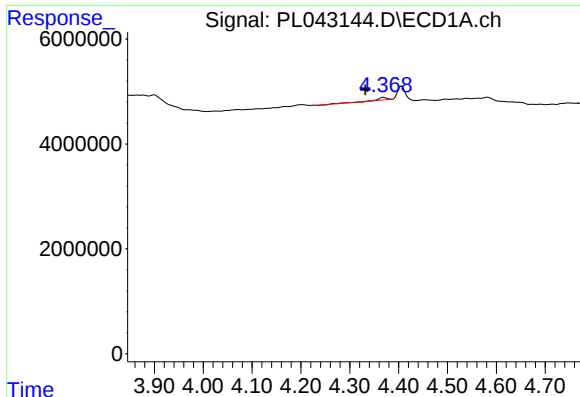

#23 Chlordane-1


R.T.: 4.370 min
Delta R.T.: 0.037 min
Response: 329250
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

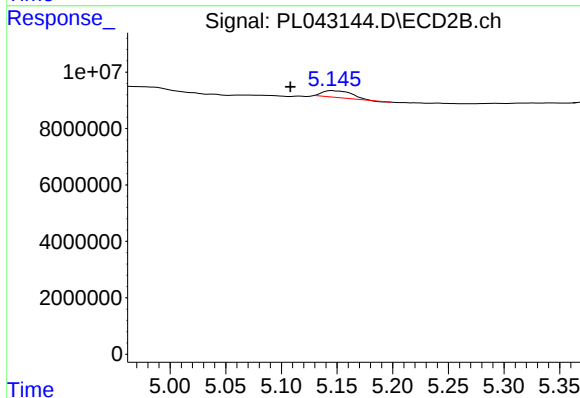


#23 Chlordane-1

R.T.: 5.146 min
Delta R.T.: 0.038 min
Response: 3939388
Conc: 27.87 ng/ml

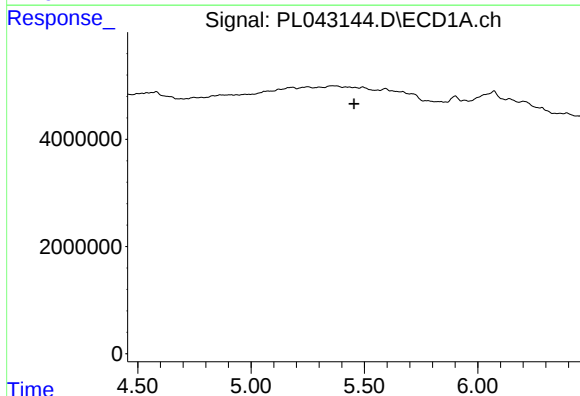


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

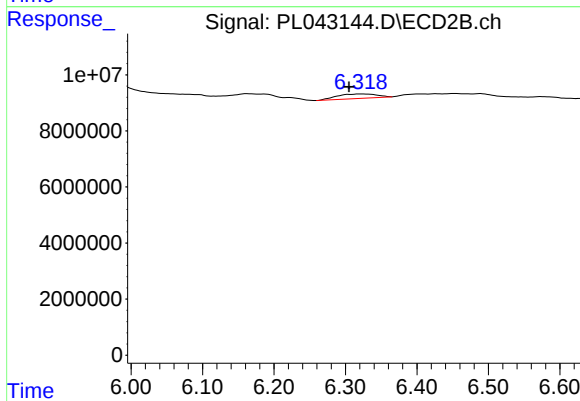

#26 Chlordane-4

R.T.: 6.320 min
Delta R.T.: 0.015 min
Response: 6203511
Conc: 10.87 ng/ml

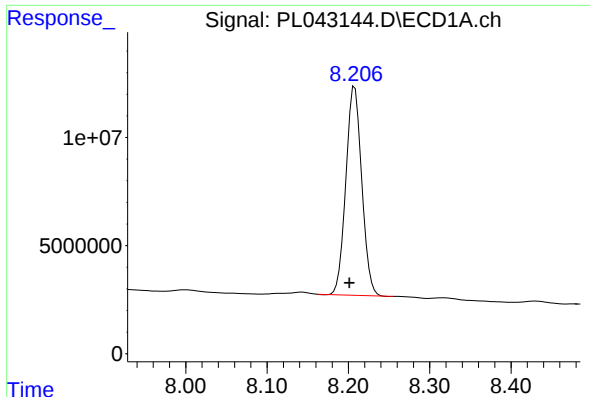

#28 Decachlorobiphenyl


R.T.: 8.208 min

Delta R.T.: 0.007 min

Response: 130681325

Conc: 20.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

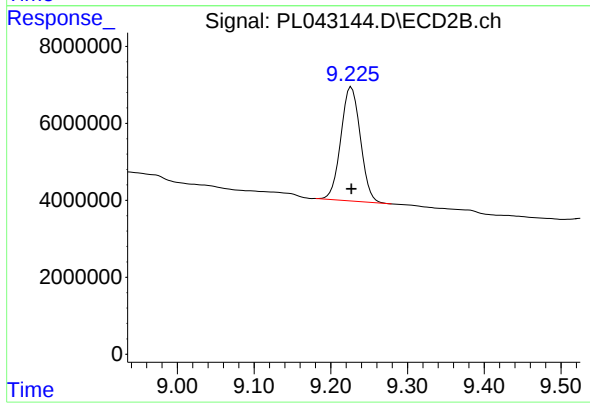

#28 Decachlorobiphenyl

R.T.: 9.227 min

Delta R.T.: 0.000 min

Response: 52482749

Conc: 20.12 ng/ml