

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
 Data File : PL043153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 17:29
 Operator : AJ\SJ
 Sample : J6373-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 22:25:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.098	132.9E6	67348137	21.663	22.723
28)	SA Decachlor...	8.197	9.223	134.4E6	54045598	20.575	20.719
Target Compounds							
2)	A alpha-BHC	3.857f	0.000	4343019	0	0.459	N.D. #
3)	MA gamma-BHC...	0.000	4.784	0	1319564	N.D.	0.315 #
6)	B beta-BHC	4.396f	0.000	13278696	0	3.600	N.D. #
7)	B delta-BHC	0.000	5.145f	0	7410699	N.D.	1.724 #
8)	B Heptachlo...	0.000	5.993	0	3694187	N.D.	0.974 #
9)	A Endosulfan I	0.000	6.338	0	1310231	N.D.	0.386 #
11)	B alpha-Chl...	0.000	6.338f	0	1310231	N.D.	0.364 #
23)	Chlordane-1	4.396	5.145	13278696	7410699	49.417	52.434
26)	Chlordane-4	0.000	6.338	0	1310231	N.D.	2.296 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
Data File : PL043153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 17:29
Operator : AJ\SJ
Sample : J6373-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 22:25:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

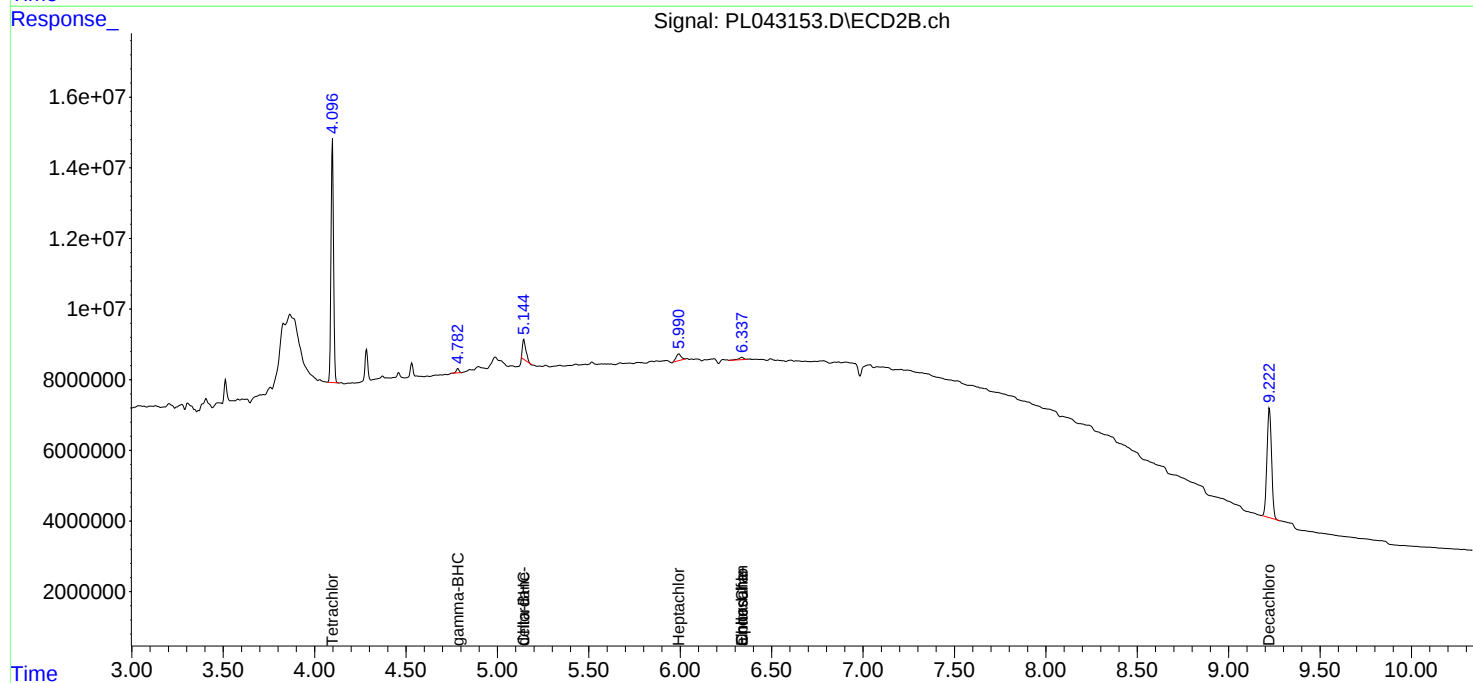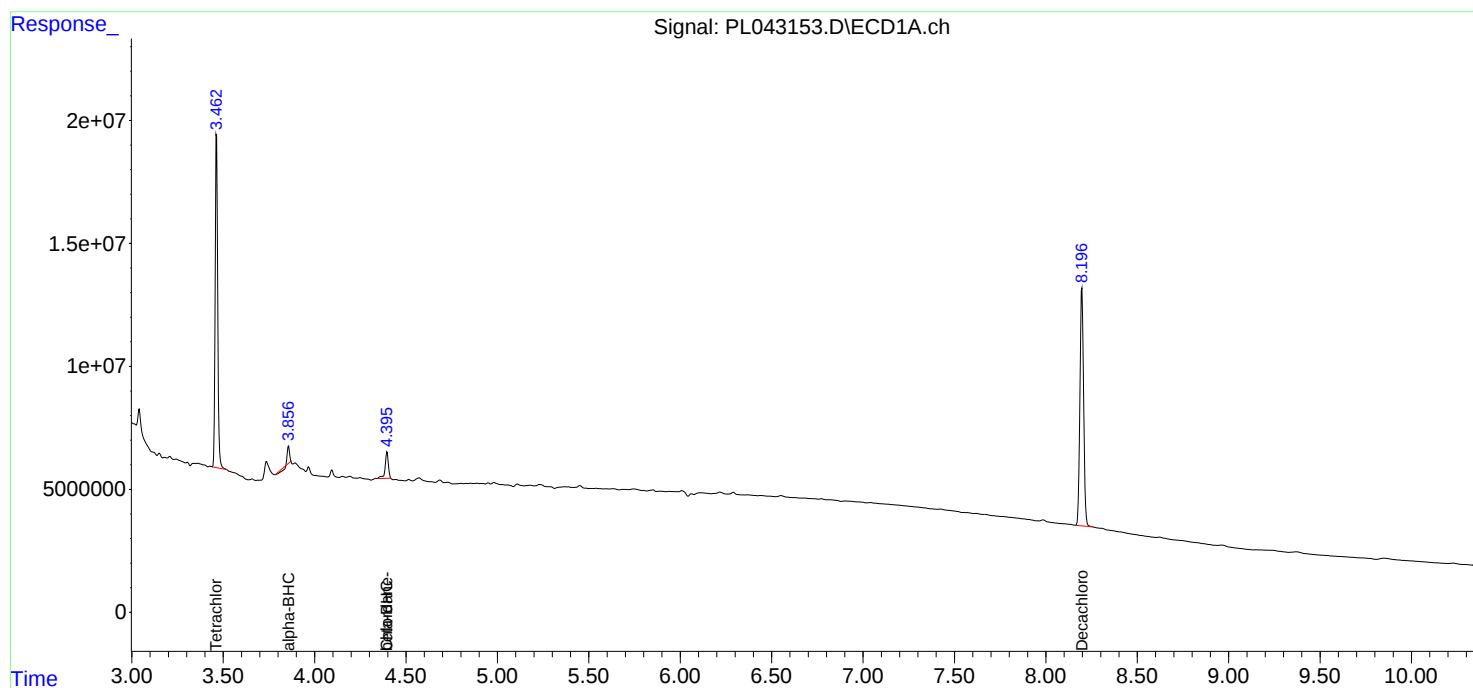


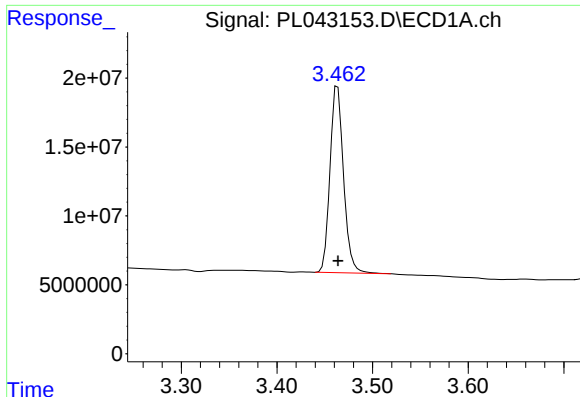

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 132859490
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

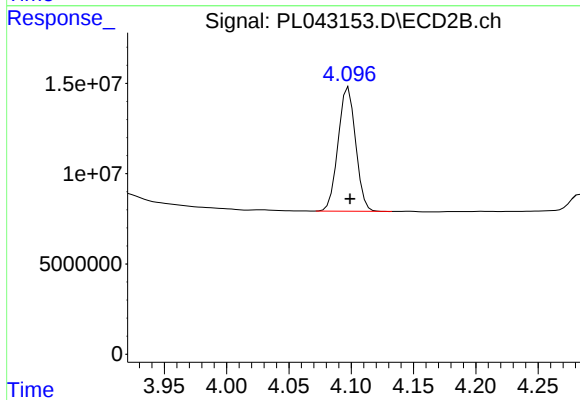


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.001 min
Response: 67348137
Conc: 22.72 ng/ml

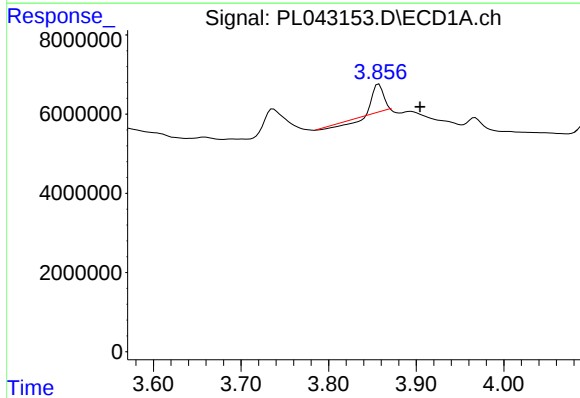


#2 alpha-BHC

R.T.: 3.857 min
Delta R.T.: -0.047 min
Response: 4343019
Conc: 0.46 ng/ml

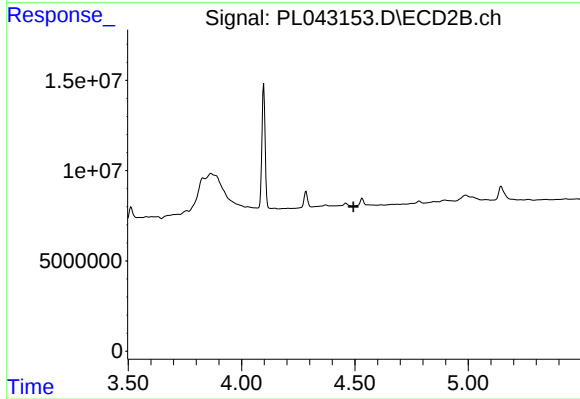

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

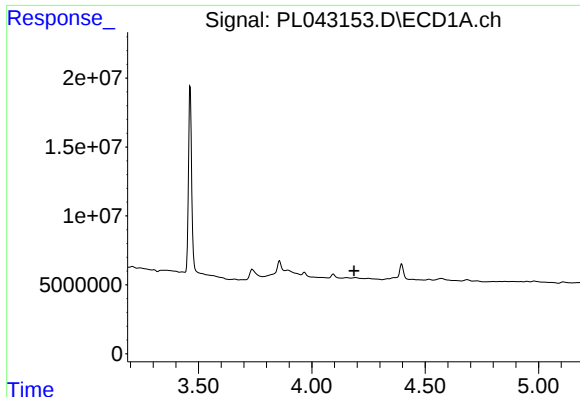

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

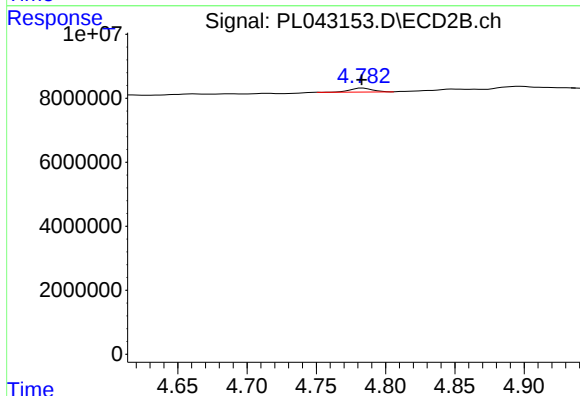


#3 gamma-BHC (Lindane)

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 1319564
Conc: 0.31 ng/ml

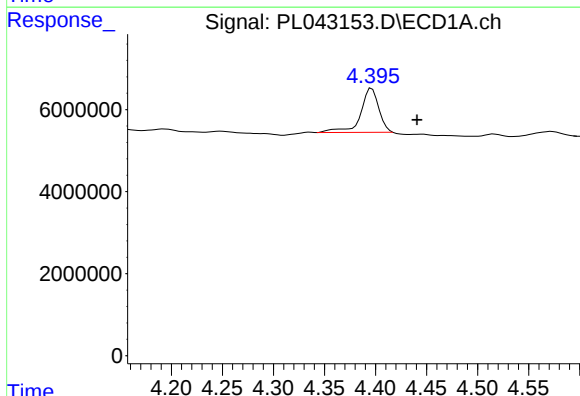


#6 beta-BHC

R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 13278696
Conc: 3.60 ng/ml

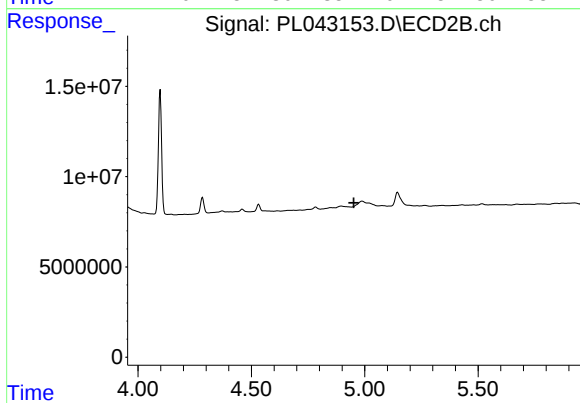

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

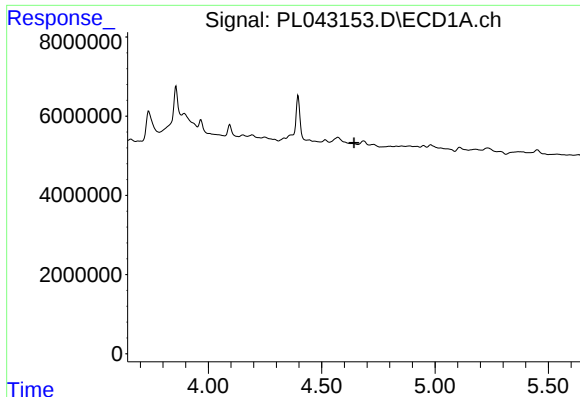

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

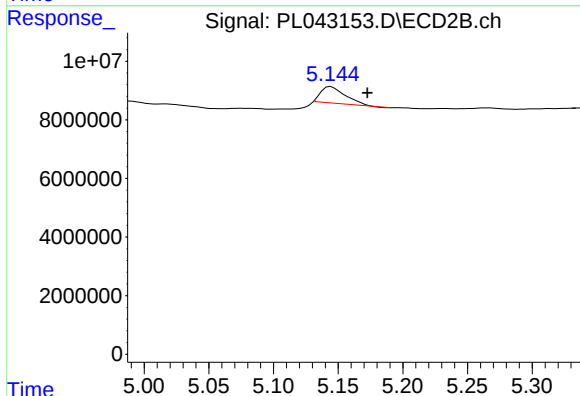


#7 delta-BHC

R.T.: 5.145 min
Delta R.T.: -0.028 min
Response: 7410699
Conc: 1.72 ng/ml

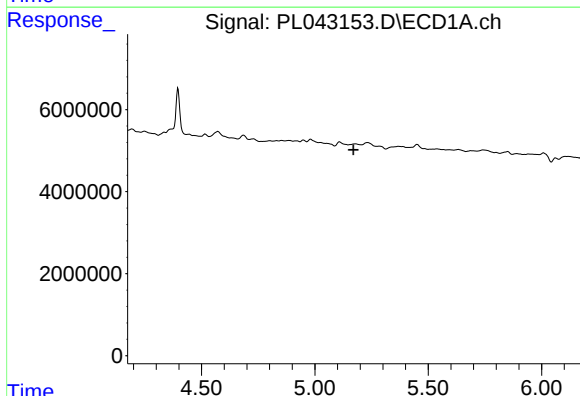


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

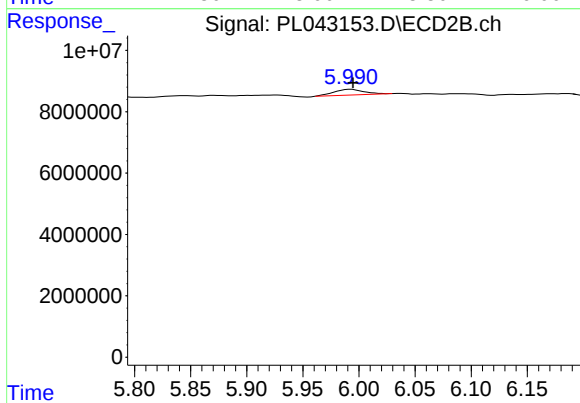

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 3694187
Conc: 0.97 ng/ml

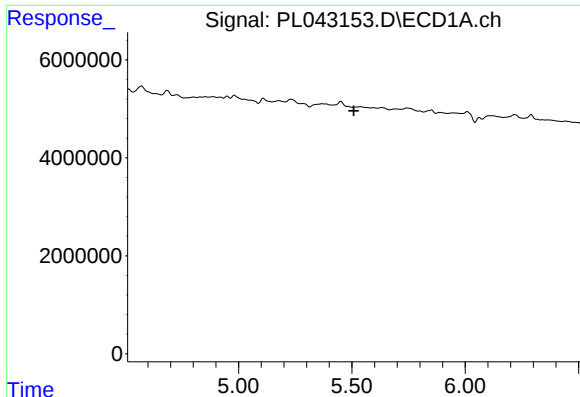

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

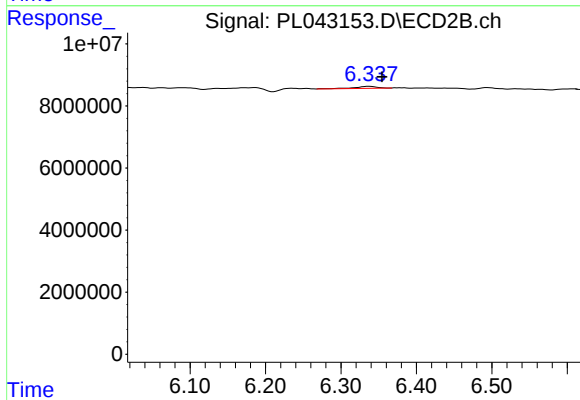


#9 Endosulfan I

R.T.: 6.338 min
Delta R.T.: -0.016 min
Response: 1310231
Conc: 0.39 ng/ml

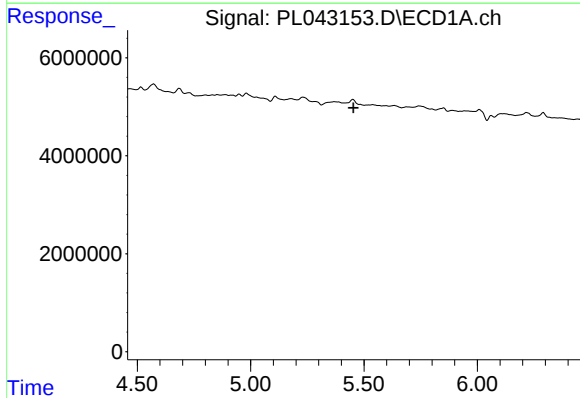


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

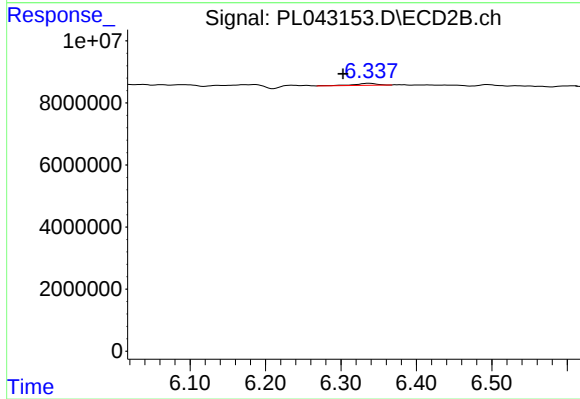

#11 alpha-Chlordane


R.T.: 6.338 min
Delta R.T.: 0.035 min
Response: 1310231
Conc: 0.36 ng/ml

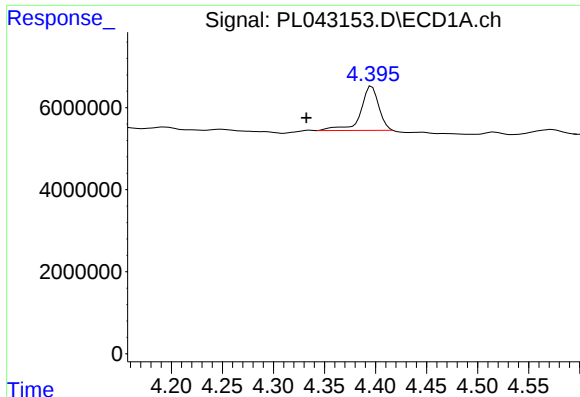

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.064 min
Response: 13278696
Conc: 49.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

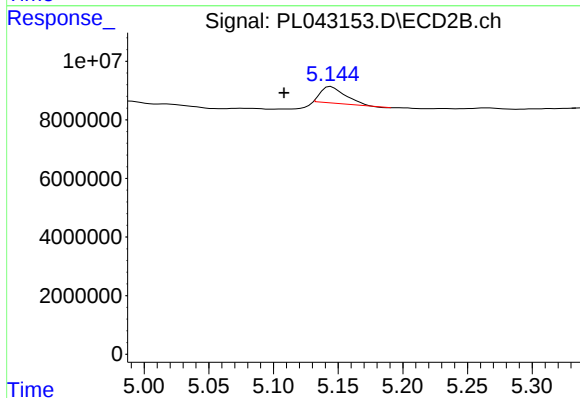


#23 Chlordane-1

R.T.: 5.145 min
Delta R.T.: 0.036 min
Response: 7410699
Conc: 52.43 ng/ml

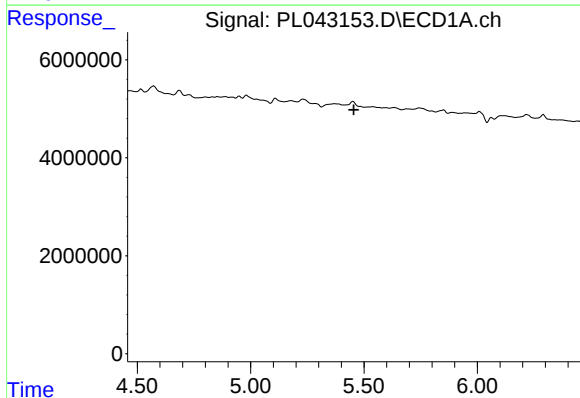


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

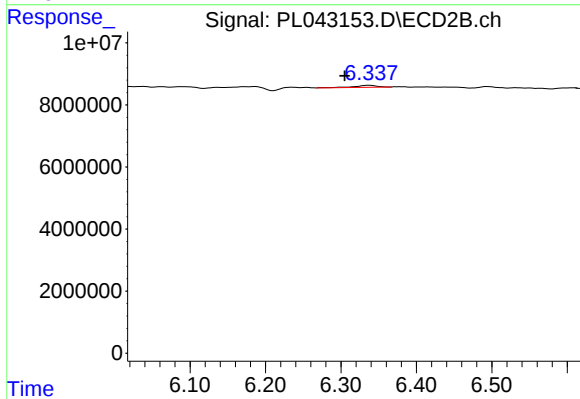

#26 Chlordane-4


R.T.: 6.338 min
Delta R.T.: 0.033 min
Response: 1310231
Conc: 2.30 ng/ml

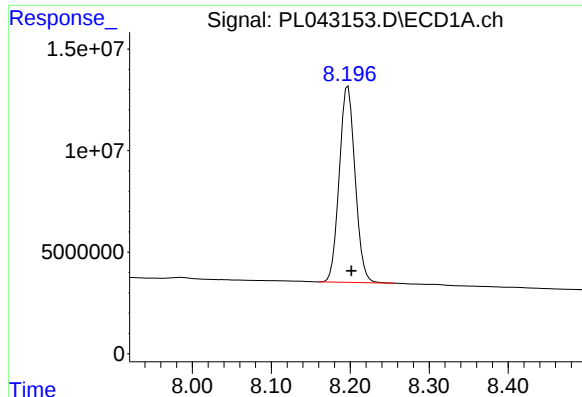

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 134354068
Conc: 20.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

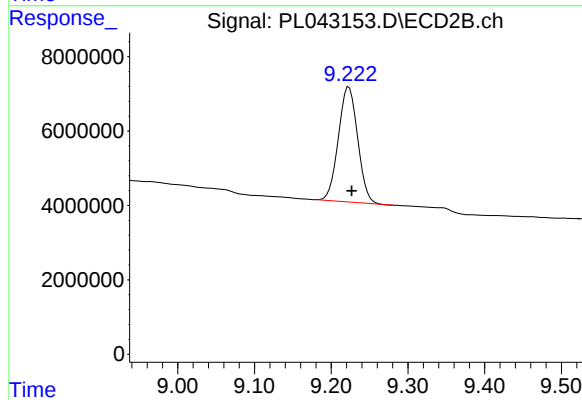

#28 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 54045598
Conc: 20.72 ng/ml