

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
 Data File : PL043156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 18:11
 Operator : AJ\SJ
 Sample : J6376-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 22:25:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.098	134.1E6	70368064	21.871	23.742
28)	SA Decachlor...	8.198	9.223	123.2E6	46886389	18.860	17.974
Target Compounds							
2)	A alpha-BHC	3.861f	0.000	151564	0	0.016	N.D. #
6)	B beta-BHC	4.396f	0.000	10051384	0	2.725	N.D. #
7)	B delta-BHC	0.000	5.145f	0	4353270	N.D.	1.013 #
8)	B Heptachlo...	0.000	5.992	0	2730355	N.D.	0.720 #
14)	MA Endrin	6.066f	0.000	620600	0	0.086	N.D. #
23)	Chlordane-1	4.362	5.145	1392569	4353270	5.183	30.802 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121418\
Data File : PL043156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 18:11
Operator : AJ\SJ
Sample : J6376-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 22:25:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

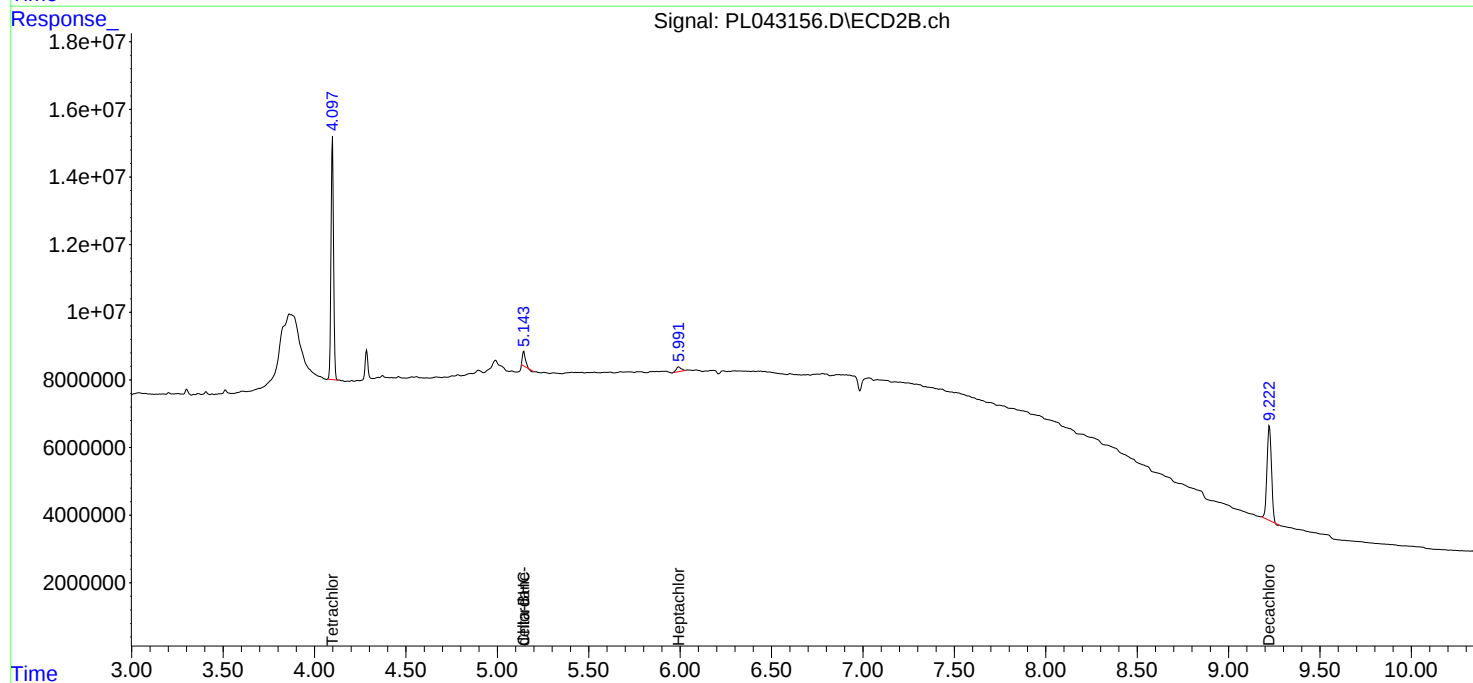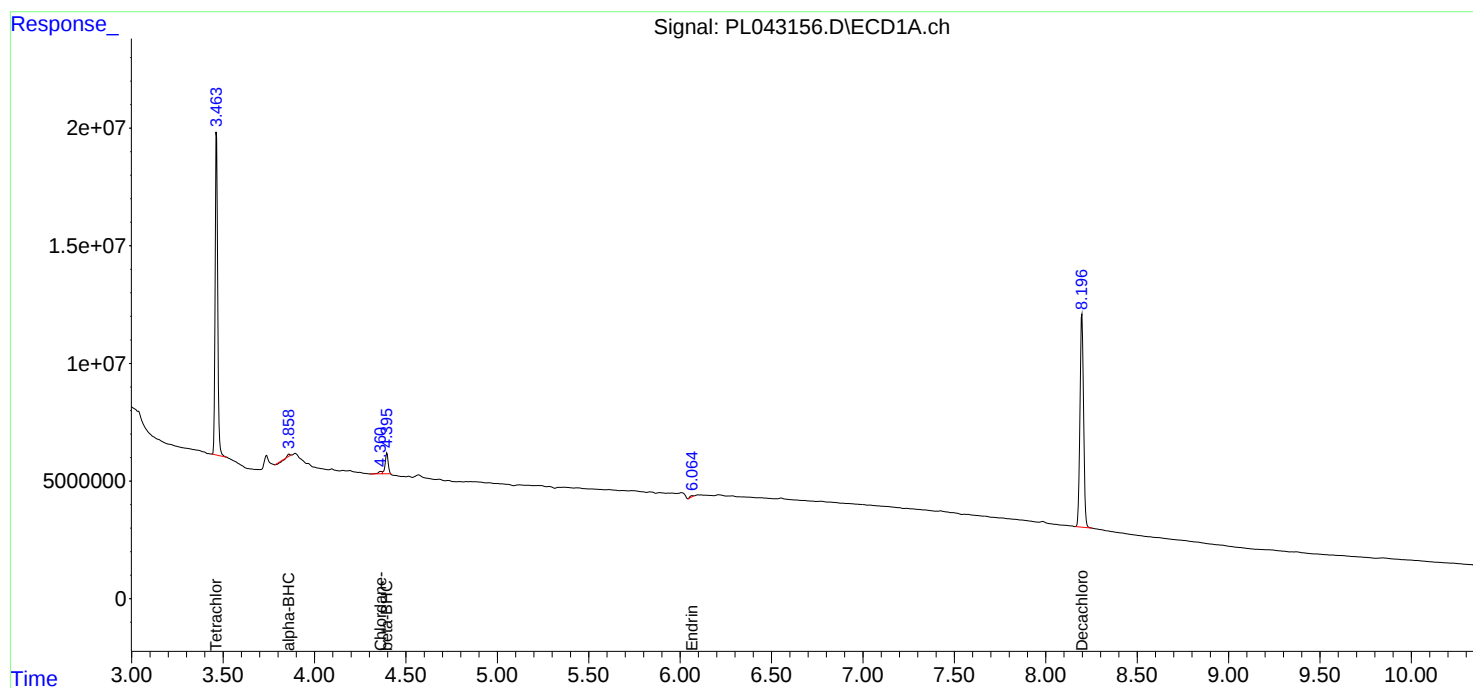


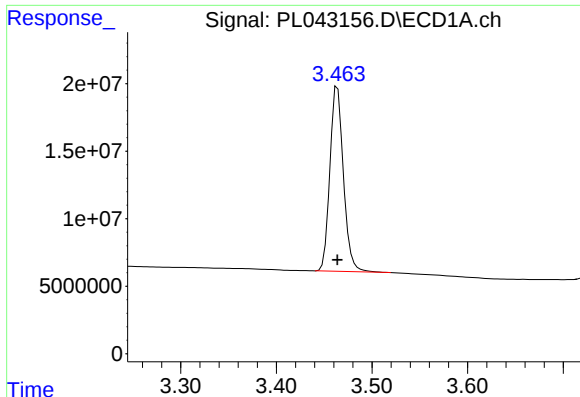

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 134134500
Conc: 21.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

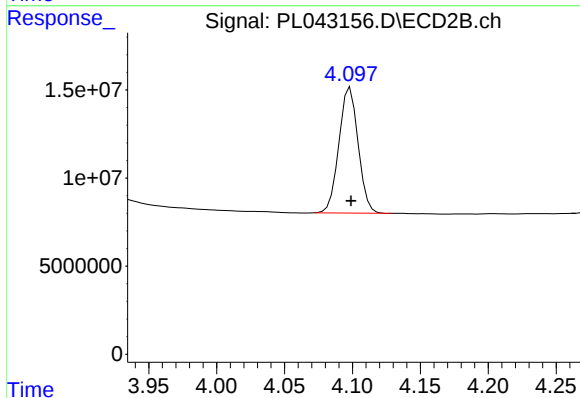


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 70368064
Conc: 23.74 ng/ml

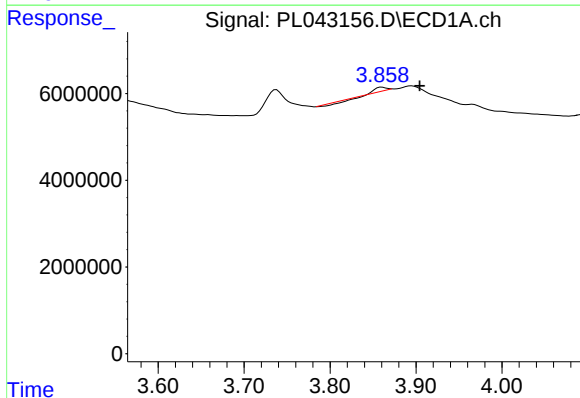


#2 alpha-BHC

R.T.: 3.861 min
Delta R.T.: -0.044 min
Response: 151564
Conc: 0.02 ng/ml

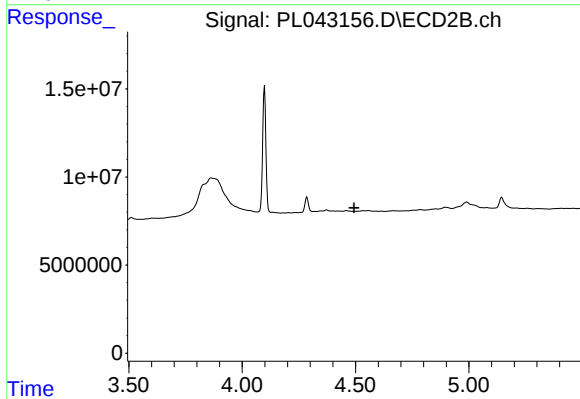

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

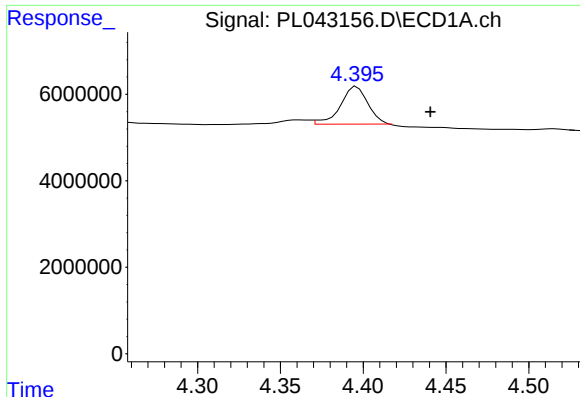

#6 beta-BHC


R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 10051384
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

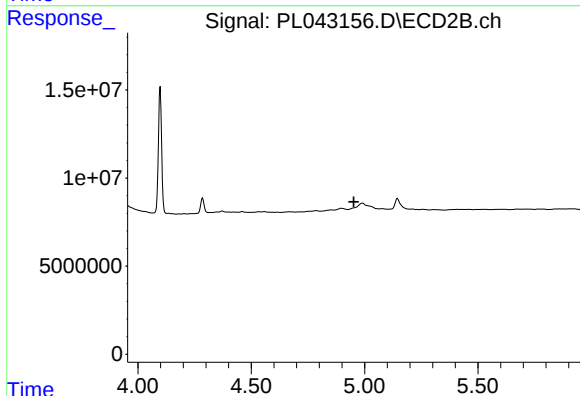


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

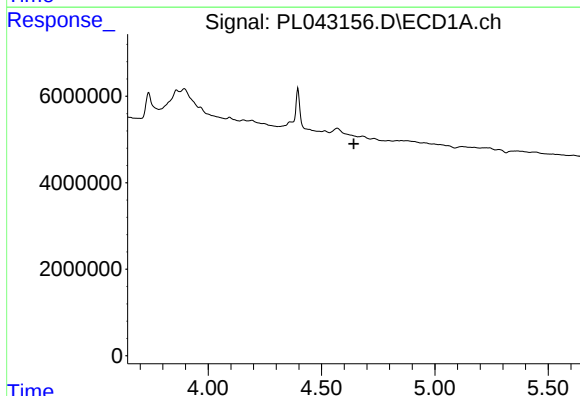


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.



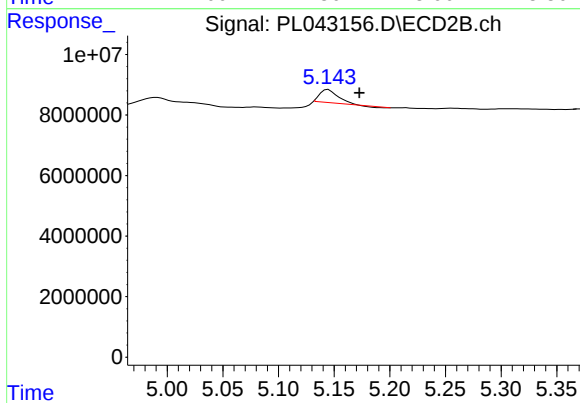



#7 delta-BHC

R.T.: 5.145 min
Delta R.T.: -0.028 min
Response: 4353270
Conc: 1.01 ng/ml

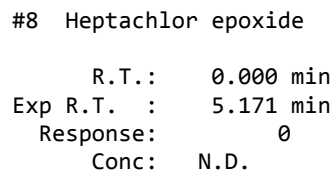

Instrument :
ECD_L
ClientSampleId :

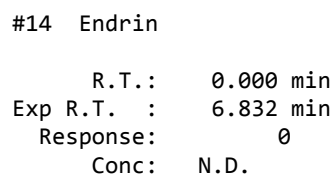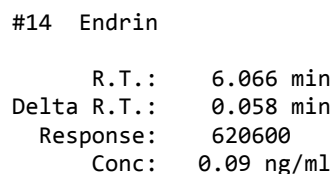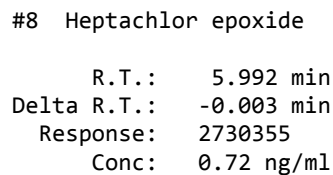


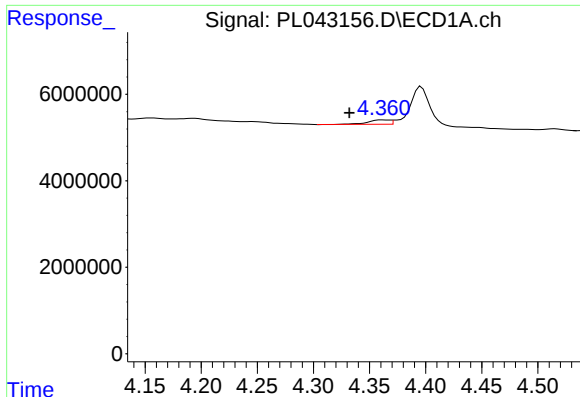

#23 Chlordane-1


R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 1392569
Conc: 5.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

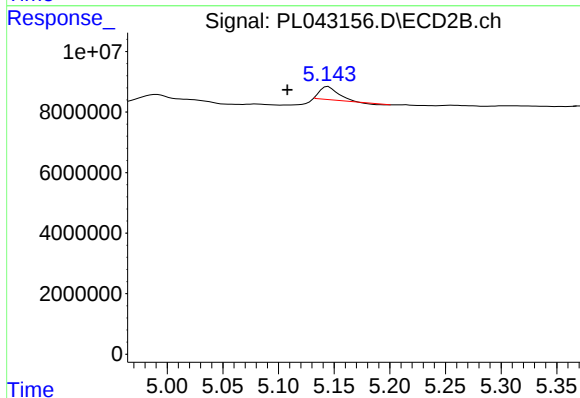


#23 Chlordane-1

R.T.: 5.145 min
Delta R.T.: 0.037 min
Response: 4353270
Conc: 30.80 ng/ml

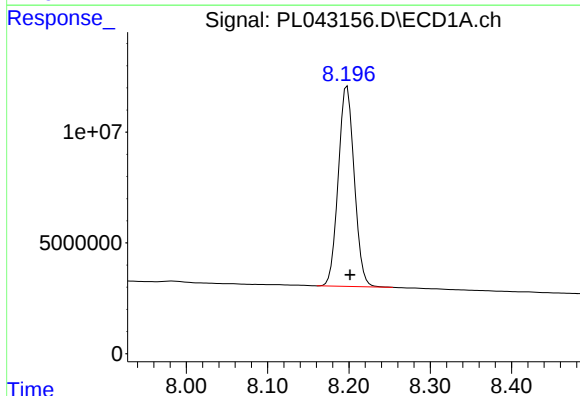

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 123153875
Conc: 18.86 ng/ml

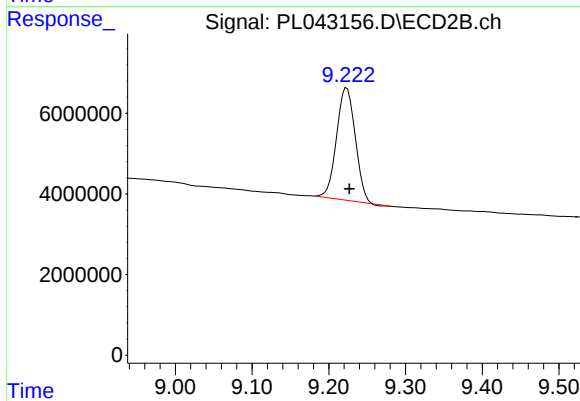

#28 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 46886389
Conc: 17.97 ng/ml