

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
 Data File : PL063598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2020 16:16
 Operator : DD\AJ
 Sample : L5043-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KENS-SS-121020-BD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:48:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	40235288	64616701	23.644	20.617
28)	SA Decachlor...	8.126	8.993	35862255	47858887	17.808	19.004
Target Compounds							
7)	B delta-BHC	0.000	5.006	0	7126933	N.D.	1.761 #
8)	B Heptachlo...	0.000	5.829f	0	1675927	N.D.	0.463 #
15)	B Endosulfa...	0.000	6.871f	0	29098076	N.D.	9.136 #
17)	MA 4,4'-DDT	0.000	7.072	0	4465597	N.D.	1.747 #
18)	B Endrin al...	0.000	6.956f	0	47373204	N.D.	18.564 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
Data File : PL063598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2020 16:16
Operator : DD\AJ
Sample : L5043-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KENS-SS-121020-BD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:48:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

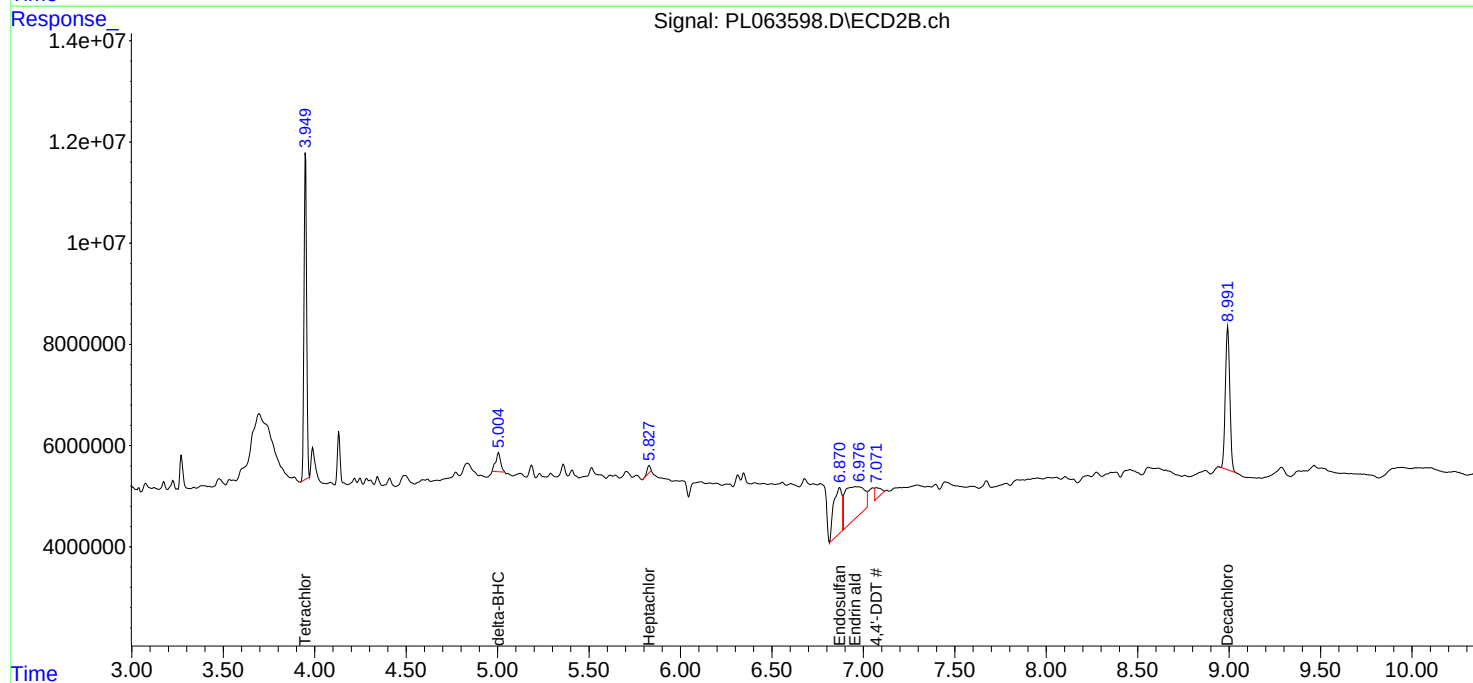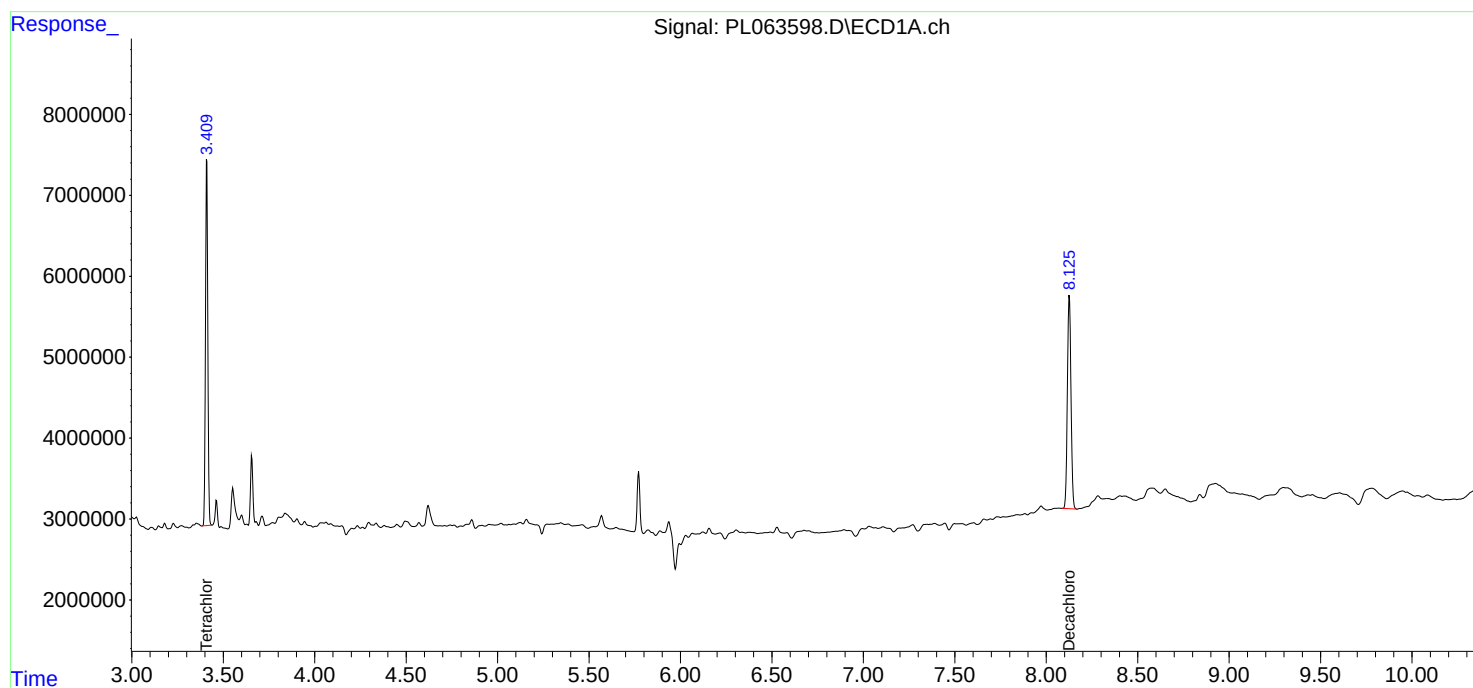


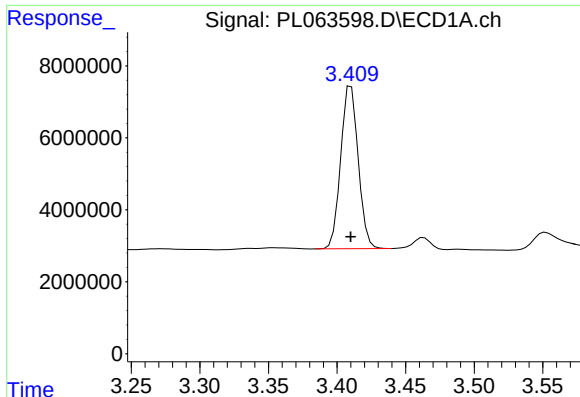

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 40235288
Conc: 23.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
KENS-SS-121020-BD

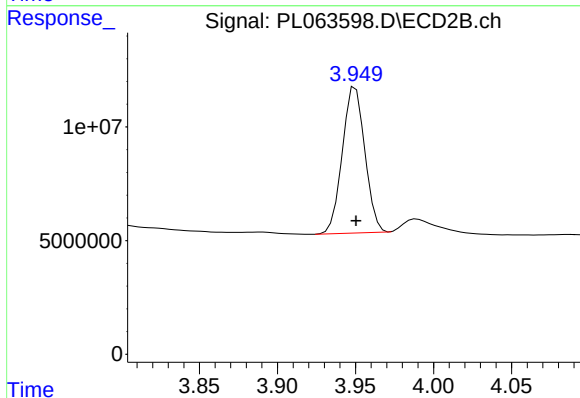


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 64616701
Conc: 20.62 ng/ml

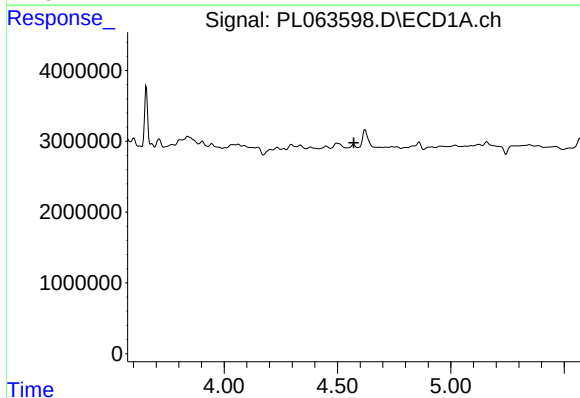


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

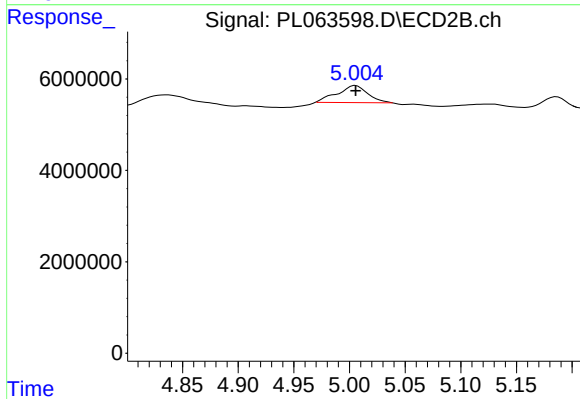

#7 delta-BHC


R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 7126933
Conc: 1.76 ng/ml

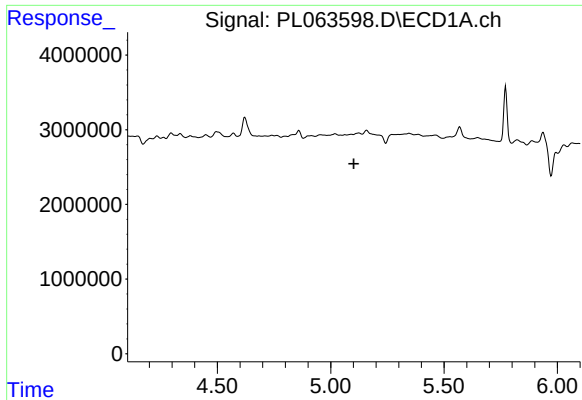

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS-121020-BD

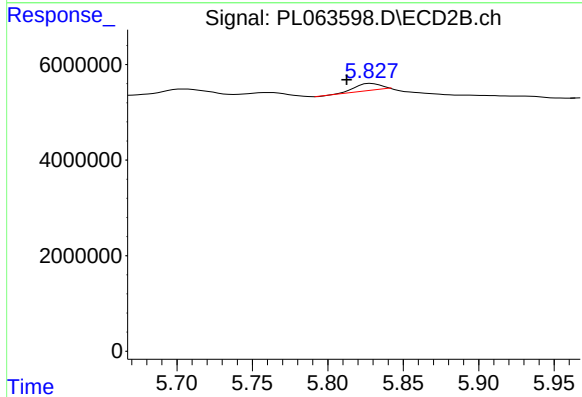


#8 Heptachlor epoxide

R.T.: 5.829 min
Delta R.T.: 0.016 min
Response: 1675927
Conc: 0.46 ng/ml

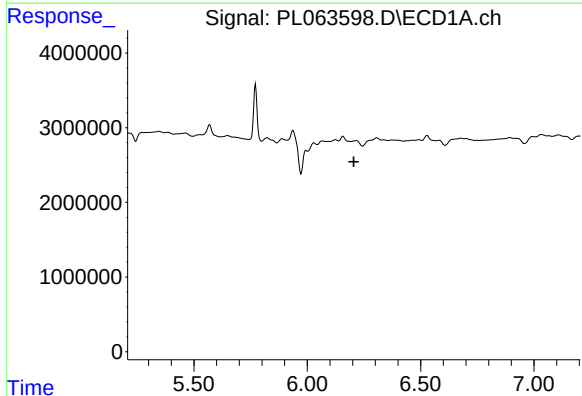


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

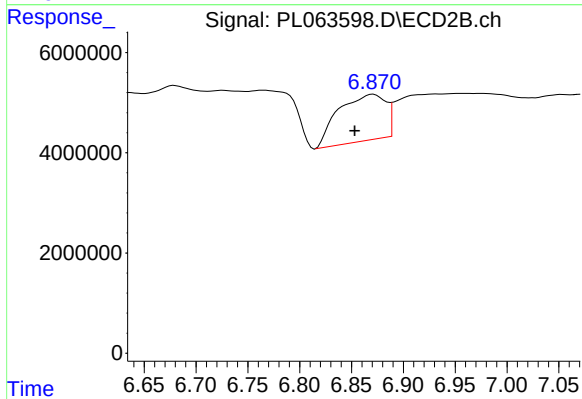

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.018 min
Response: 29098076
Conc: 9.14 ng/ml

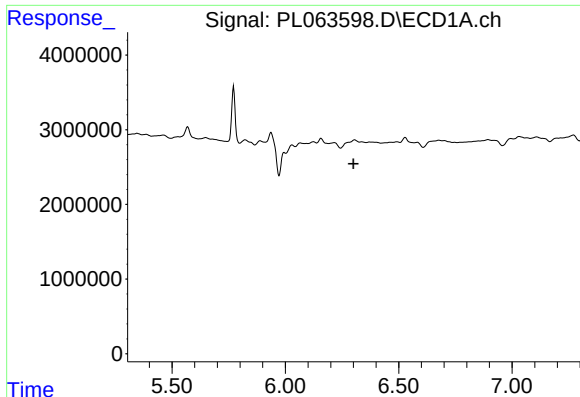

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-SS-121020-BD

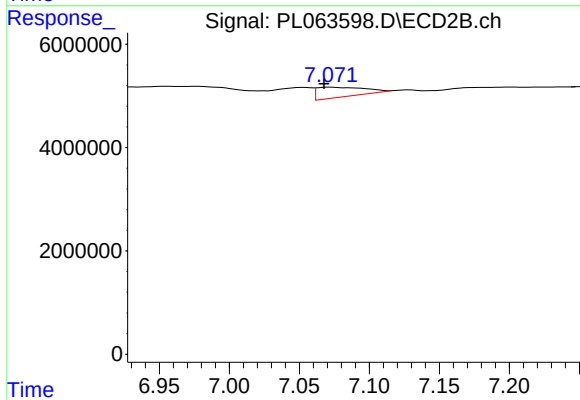


#17 4,4'-DDT

R.T.: 7.072 min
Delta R.T.: 0.005 min
Response: 4465597
Conc: 1.75 ng/ml

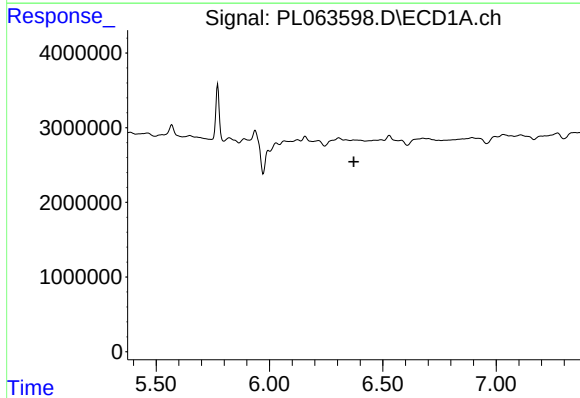


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

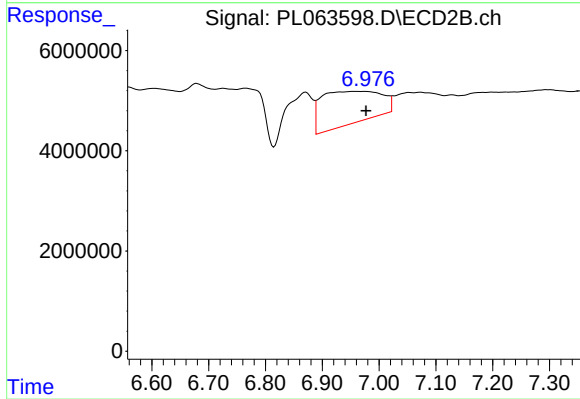

#18 Endrin aldehyde


R.T.: 6.956 min
Delta R.T.: -0.021 min
Response: 47373204
Conc: 18.56 ng/ml

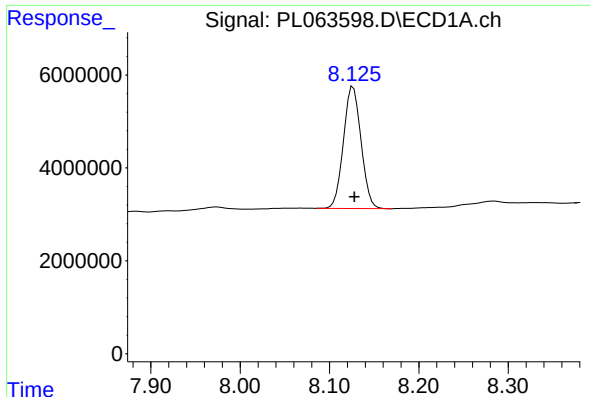

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.002 min
Response: 35862255
Conc: 17.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
KENS-SS-121020-BD

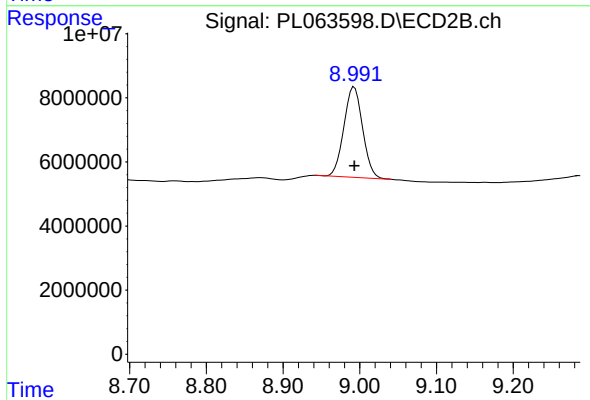

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 47858887
Conc: 19.00 ng/ml