

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
 Data File : PL063604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2020 20:26
 Operator : DD\AJ
 Sample : L5038-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:50:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.967f	35789136	59817419	21.031	19.086
28)	SA Decachlor...	8.127	9.008f	39614520	36313089	19.671	14.419 #
Target Compounds							
2)	A alpha-BHC	0.000	4.330	0	8611843	N.D.	1.819 #
7)	B delta-BHC	0.000	5.000	0	7761057	N.D.	1.918 #
8)	B Heptachlo...	0.000	5.836f	0	7992718	N.D.	2.207 #
9)	A Endosulfan I	0.000	6.196f	0	40105628	N.D.	12.016 #
11)	B alpha-Chl...	5.391	0.000	9445261	0	5.080	N.D. #
14)	MA Endrin	5.936	0.000	4488522	0	2.674	N.D. #
15)	B Endosulfa...	0.000	6.840	0	23927266	N.D.	7.512 #
18)	B Endrin al...	6.397f	6.983	5212606	9499541	3.401	3.723
26)	Chlordane-4	5.391	0.000	9445261	0	64.572	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
Data File : PL063604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2020 20:26
Operator : DD\AJ
Sample : L5038-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:50:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

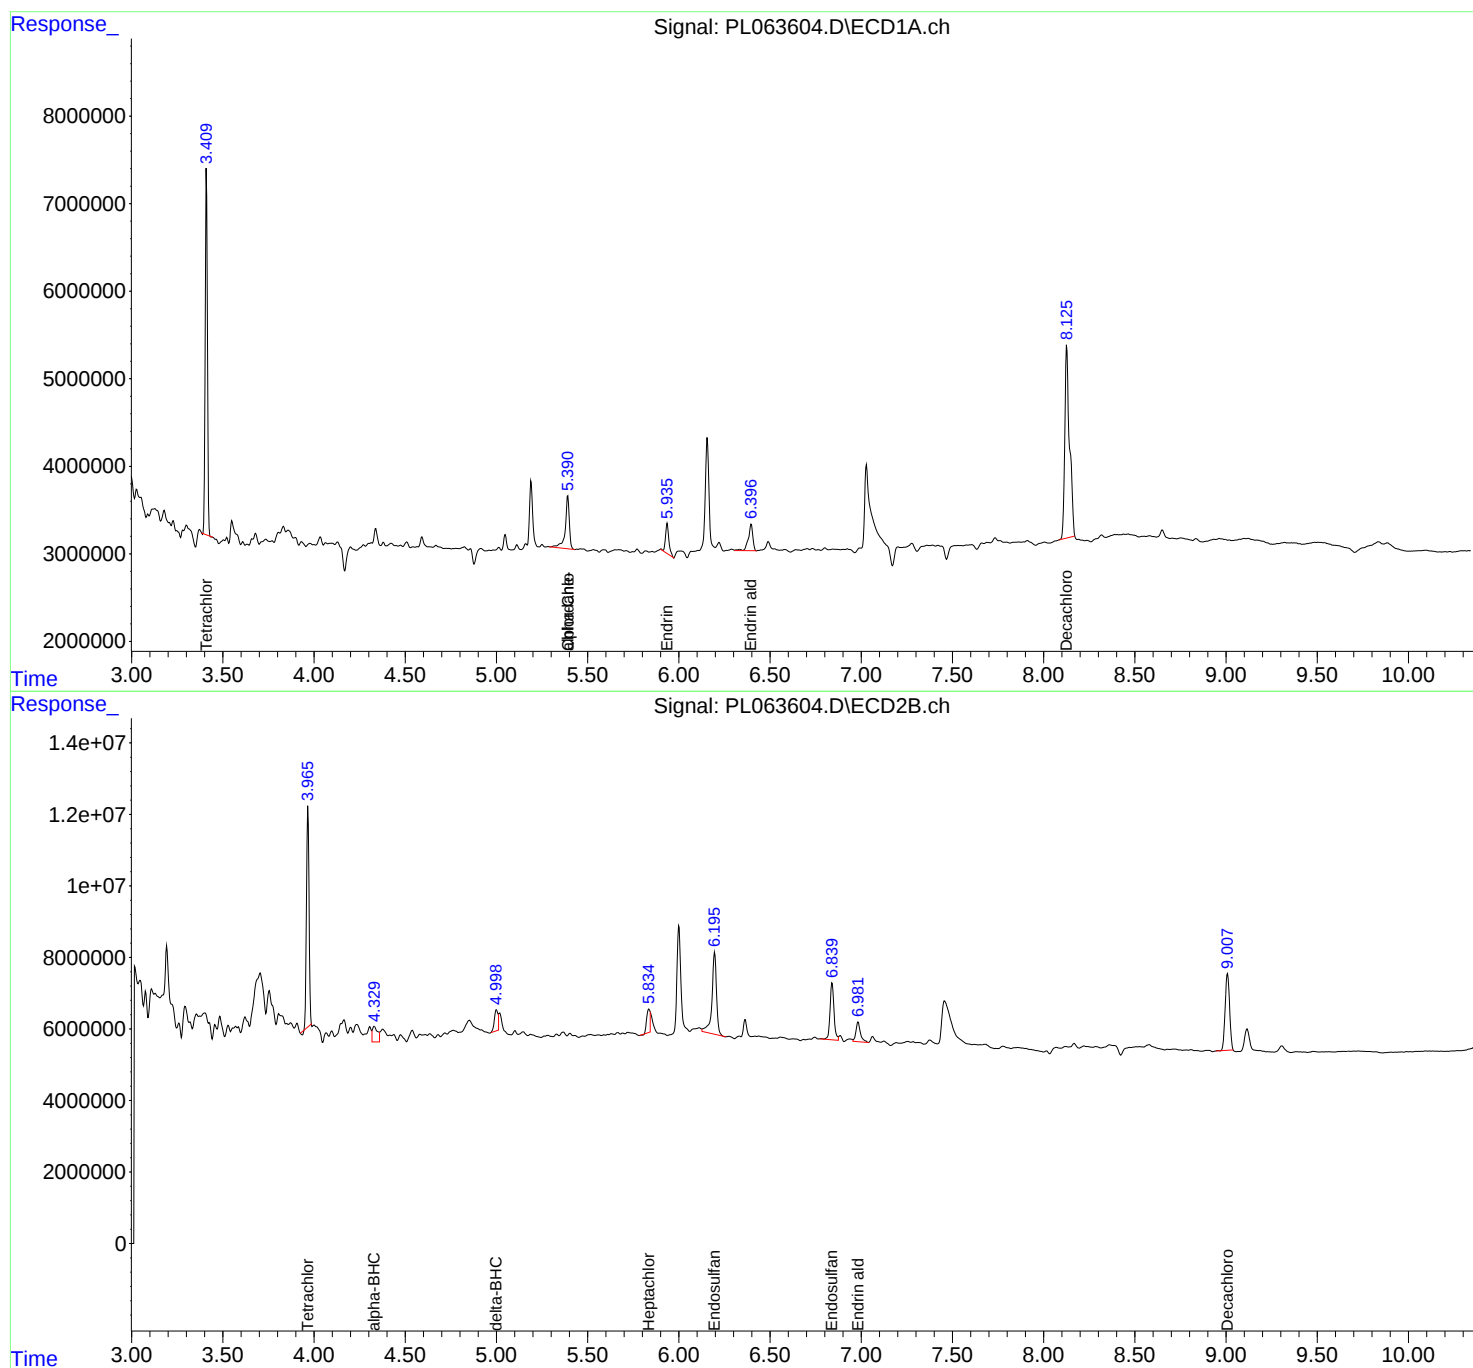


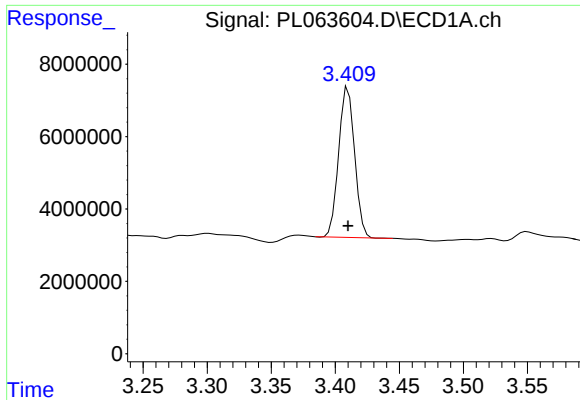

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 35789136
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

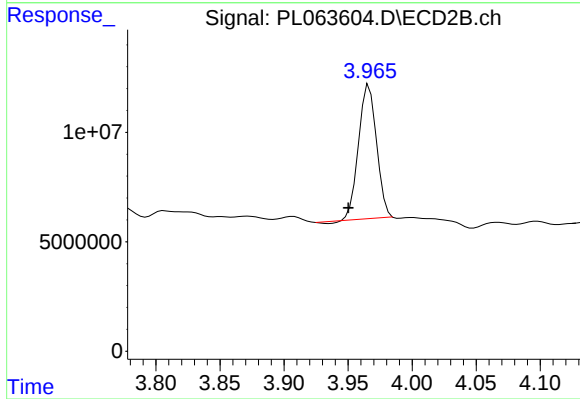


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.016 min
Response: 59817419
Conc: 19.09 ng/ml

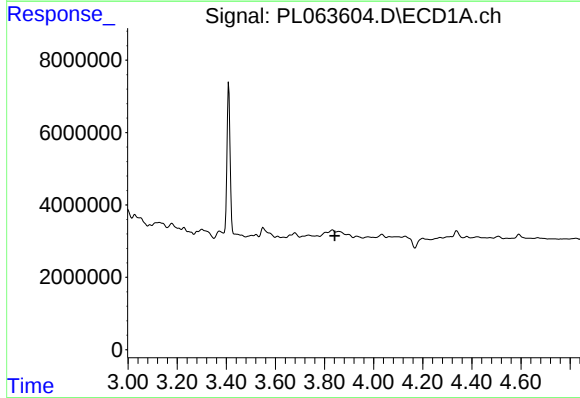


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.842 min
Response: 0
Conc: N.D.

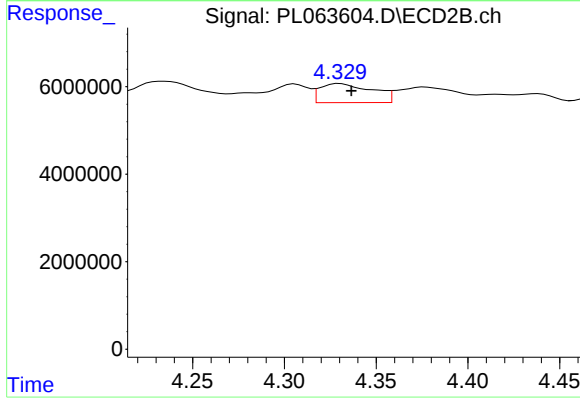

#2 alpha-BHC


R.T.: 4.330 min
Delta R.T.: -0.006 min
Response: 8611843
Conc: 1.82 ng/ml

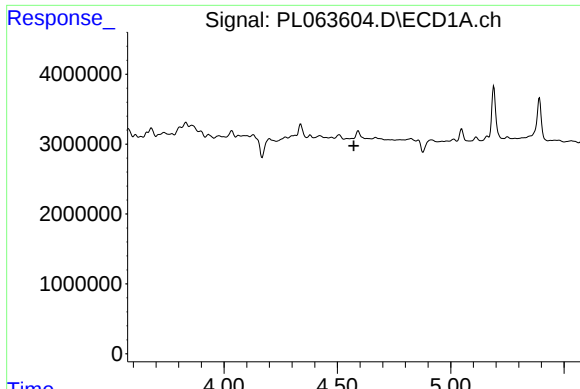

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

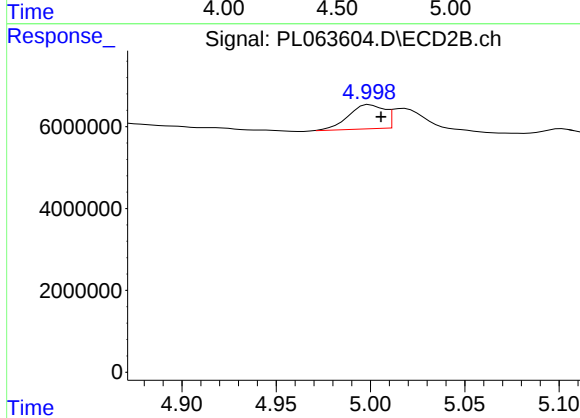


#7 delta-BHC

R.T.: 5.000 min
Delta R.T.: -0.006 min
Response: 7761057
Conc: 1.92 ng/ml

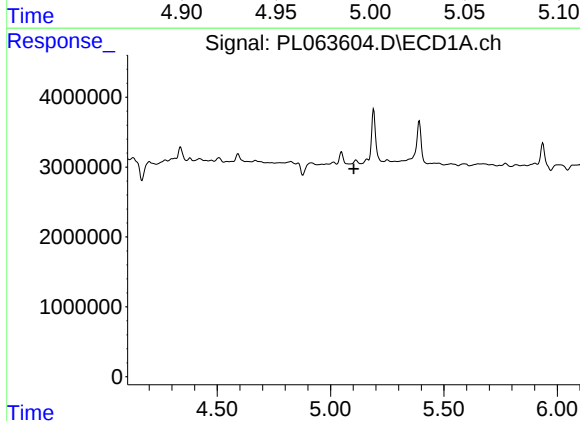


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

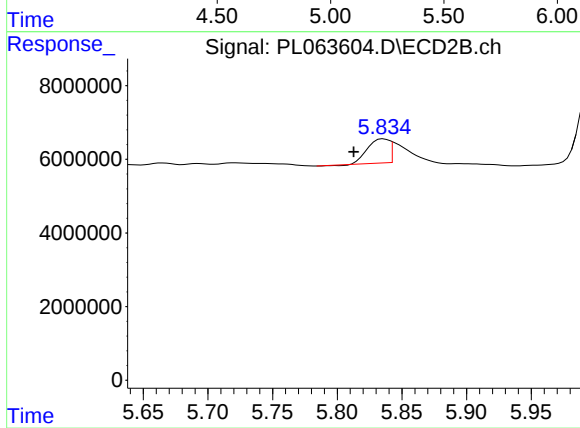

#8 Heptachlor epoxide


R.T.: 5.836 min
Delta R.T.: 0.023 min
Response: 7992718
Conc: 2.21 ng/ml

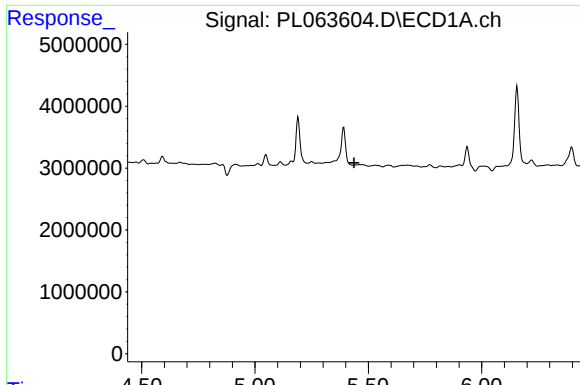

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

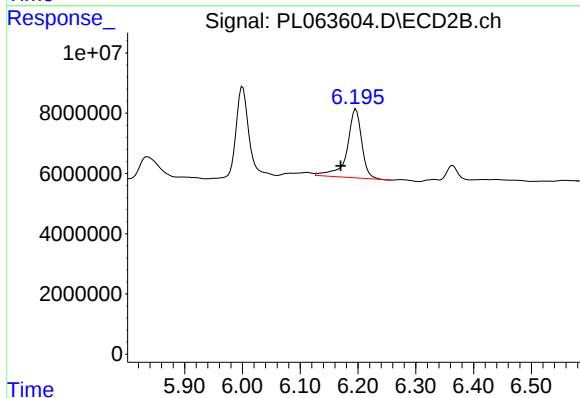


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.026 min
Response: 40105628
Conc: 12.02 ng/ml

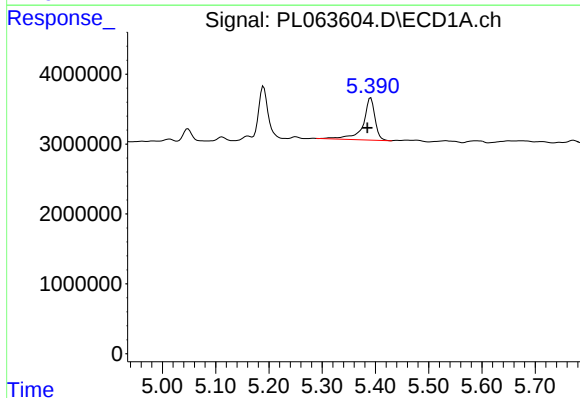


#11 alpha-Chlordane

R.T.: 5.391 min
Delta R.T.: 0.006 min
Response: 9445261
Conc: 5.08 ng/ml

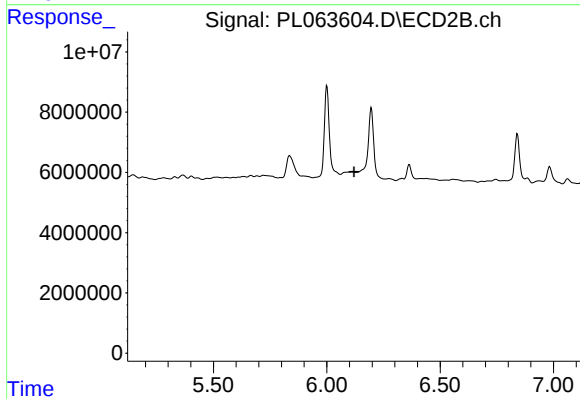

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.120 min
Response: 0
Conc: N.D.

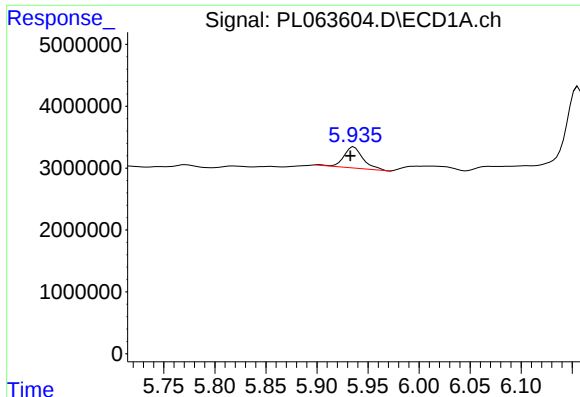

#14 Endrin


R.T.: 5.936 min
Delta R.T.: 0.003 min
Response: 4488522
Conc: 2.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

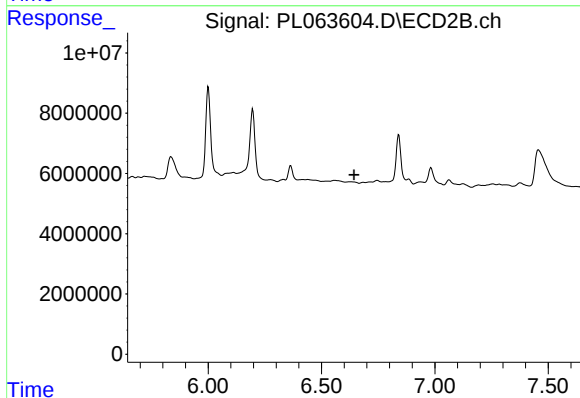


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

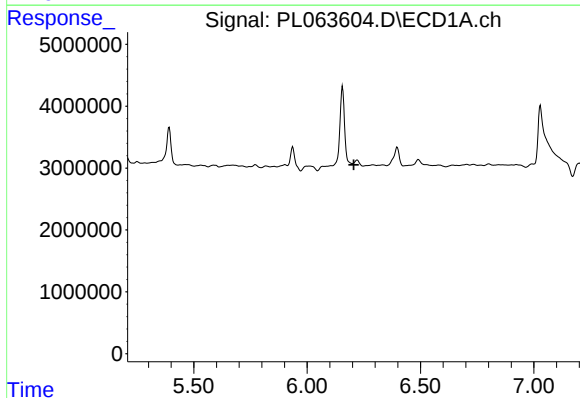


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

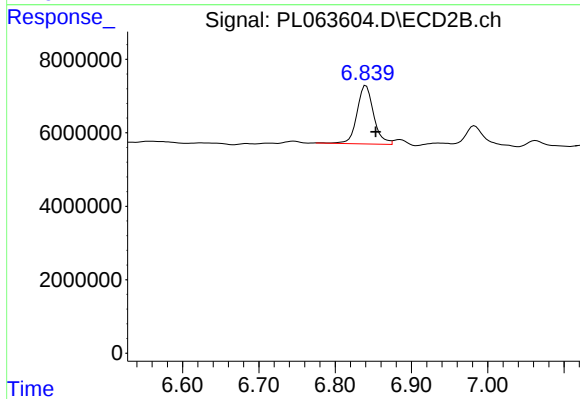

#15 Endosulfan II


R.T.: 6.840 min
Delta R.T.: -0.013 min
Response: 23927266
Conc: 7.51 ng/ml

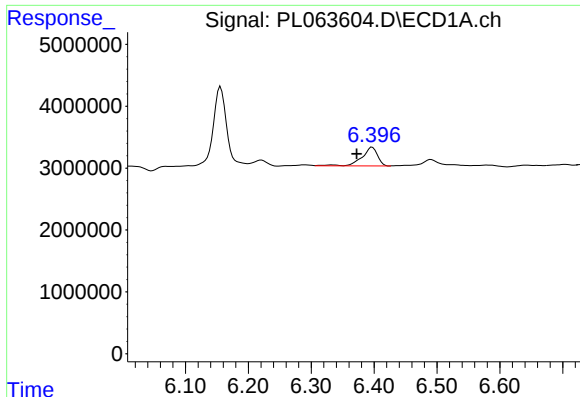

#18 Endrin aldehyde


R.T.: 6.397 min
Delta R.T.: 0.025 min
Response: 5212606
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

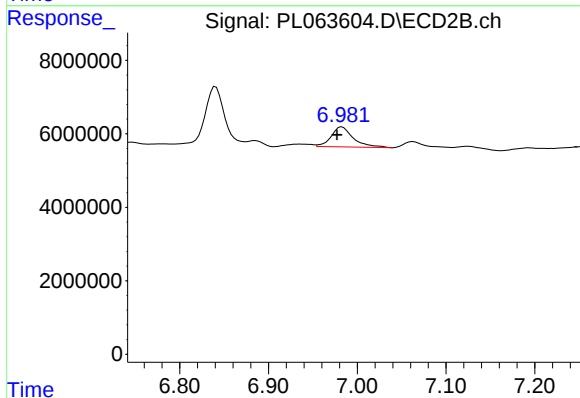


#18 Endrin aldehyde

R.T.: 6.983 min
Delta R.T.: 0.006 min
Response: 9499541
Conc: 3.72 ng/ml

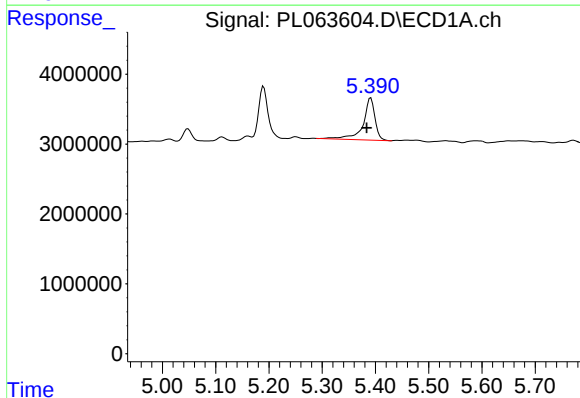


#26 Chlordane-4

R.T.: 5.391 min
Delta R.T.: 0.008 min
Response: 9445261
Conc: 64.57 ng/ml

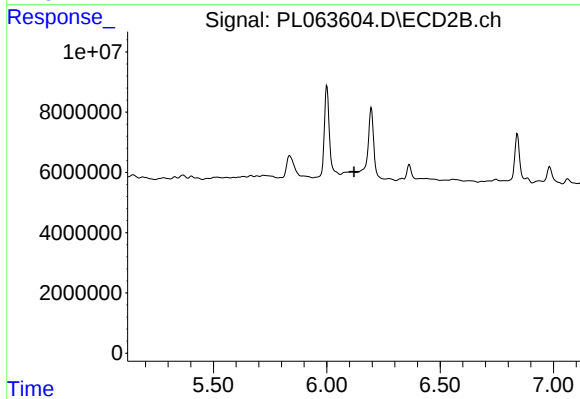

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

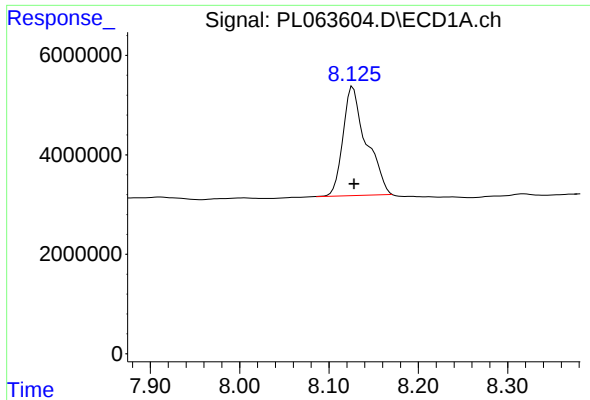

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: -0.001 min
Response: 39614520
Conc: 19.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

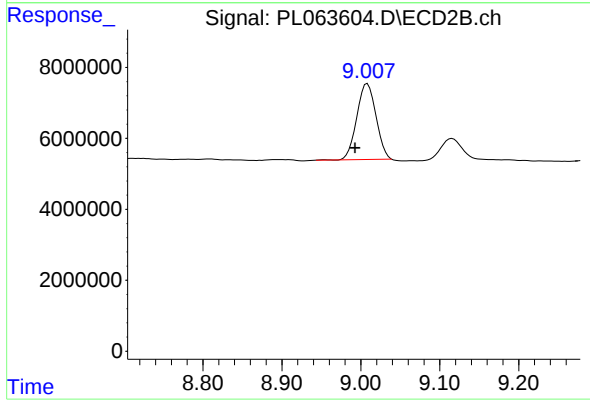

#28 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: 0.015 min
Response: 36313089
Conc: 14.42 ng/ml