

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
 Data File : PL063605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2020 20:41
 Operator : DD\AJ
 Sample : L5039-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JBD-WC-L-SB-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:50:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	33438050	57646204	19.650	18.393
28)	SA Decachlor...	8.127	8.991	30335999	31659942	15.064	12.572
Target Compounds							
2)	A alpha-BHC	0.000	4.313f	0	10259376	N.D.	2.167 #
7)	B delta-BHC	0.000	4.982f	0	5252014	N.D.	1.298 #
8)	B Heptachlo...	0.000	5.817	0	17997038	N.D.	4.969 #
9)	A Endosulfan I	0.000	6.179	0	34810235	N.D.	10.430 #
11)	B alpha-Chl...	5.391	0.000	6371943	0	3.427	N.D. #
14)	MA Endrin	5.937	0.000	4050241	0	2.413	N.D. #
15)	B Endosulfa...	0.000	6.823f	0	21052413	N.D.	6.610 #
18)	B Endrin al...	6.397f	6.966	4687922	9228343	3.058	3.616
26)	Chlordane-4	5.391	0.000	6371943	0	43.562	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121420\
Data File : PL063605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2020 20:41
Operator : DD\AJ
Sample : L5039-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:50:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

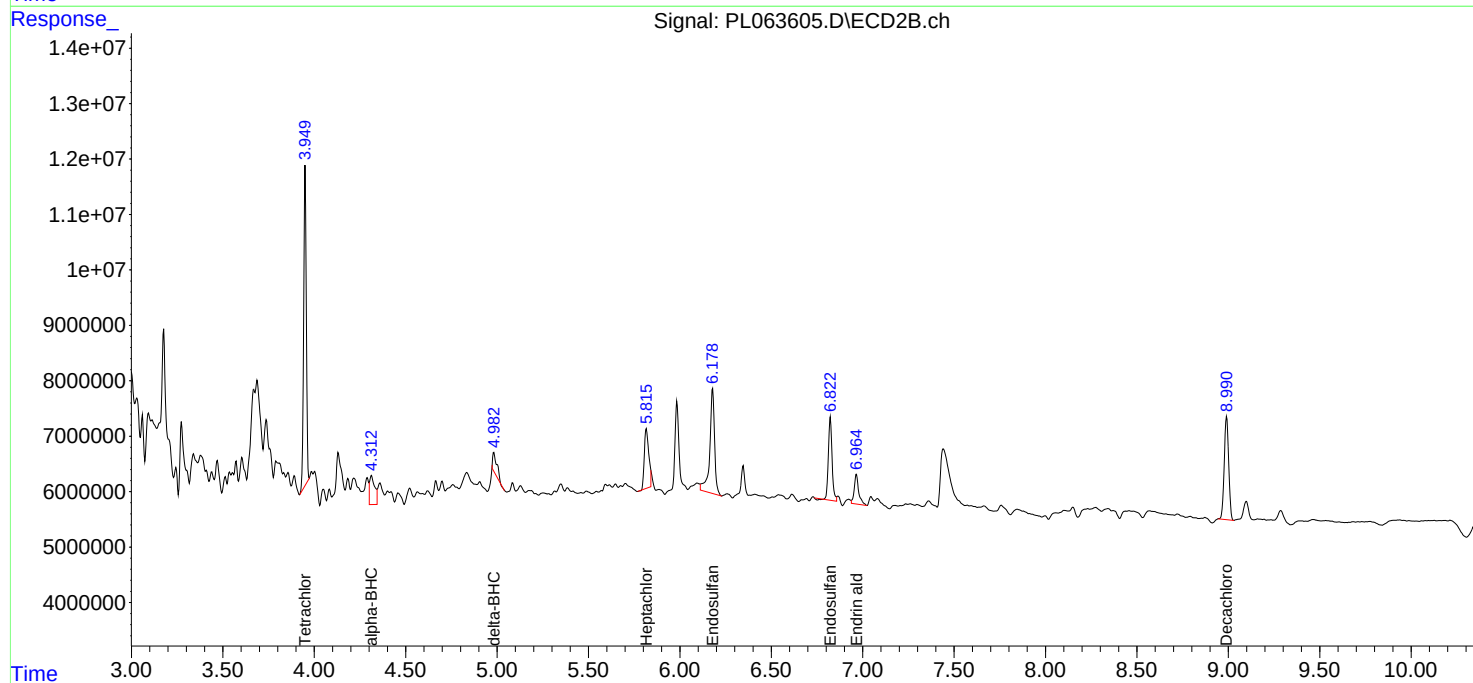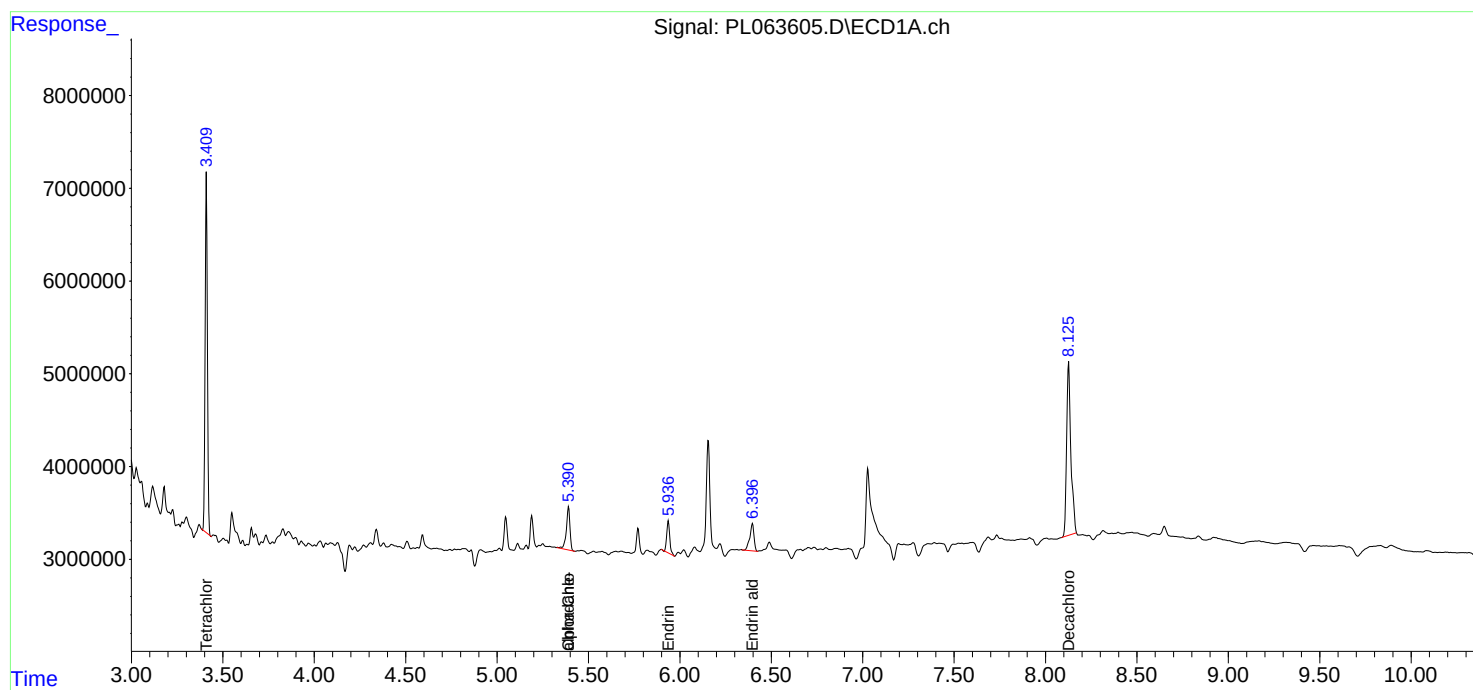


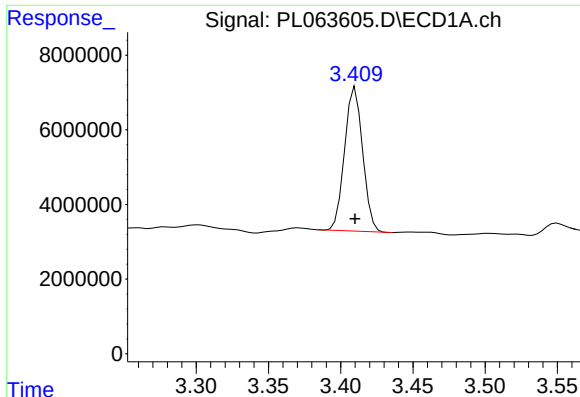

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 33438050
Conc: 19.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

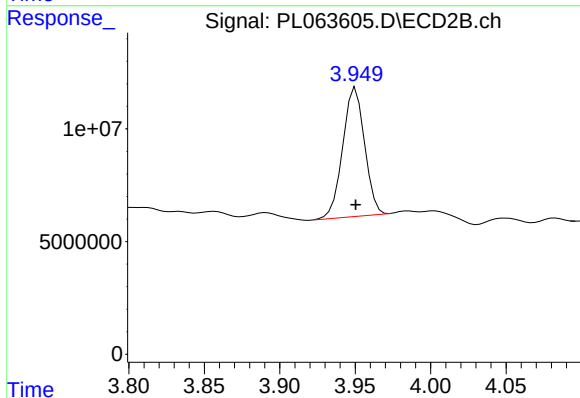


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 57646204
Conc: 18.39 ng/ml

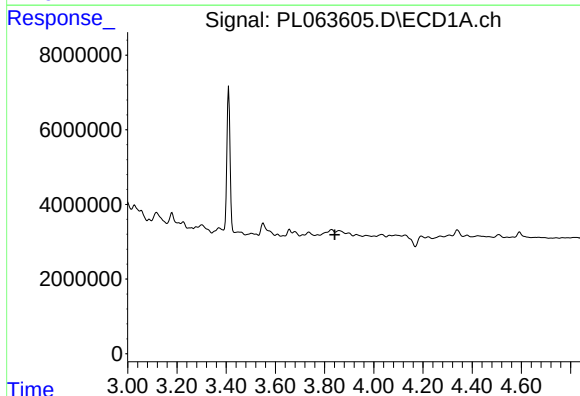


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.842 min
Response: 0
Conc: N.D.

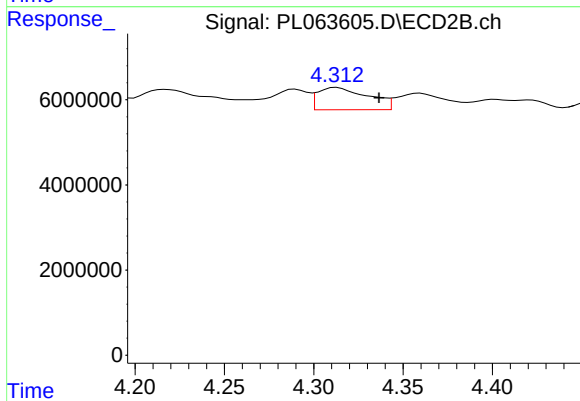

#2 alpha-BHC


R.T.: 4.313 min
Delta R.T.: -0.024 min
Response: 10259376
Conc: 2.17 ng/ml

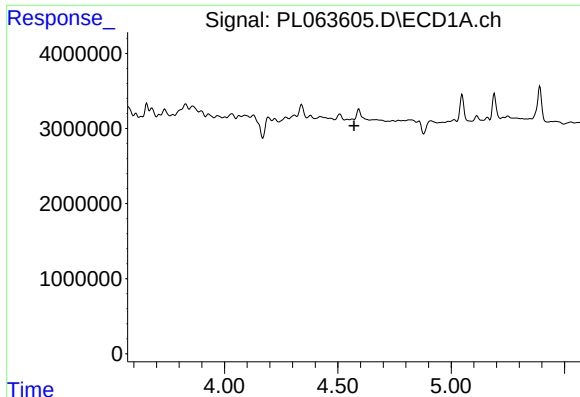

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

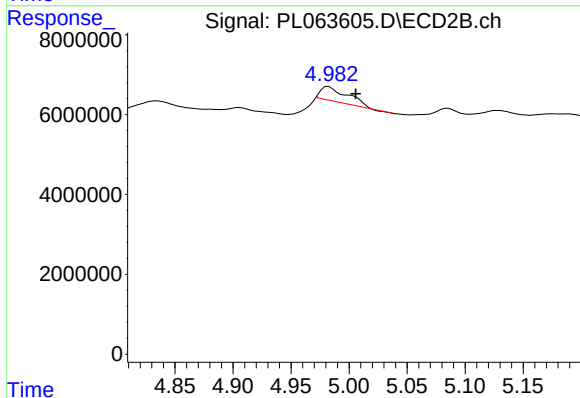


#7 delta-BHC

R.T.: 4.982 min
Delta R.T.: -0.023 min
Response: 5252014
Conc: 1.30 ng/ml

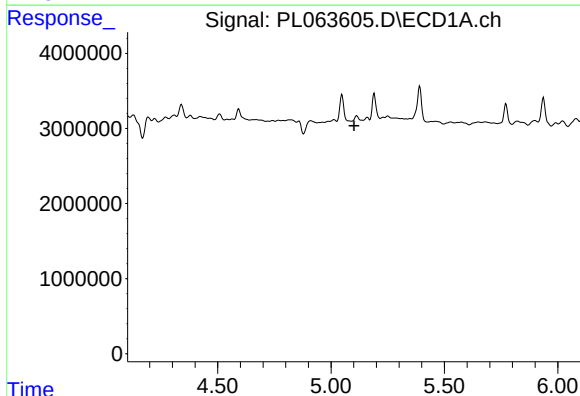


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

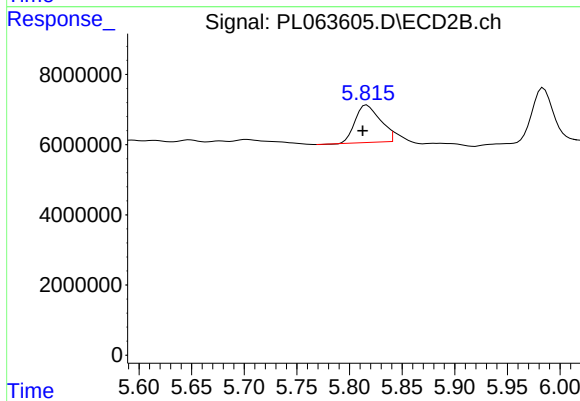

#8 Heptachlor epoxide


R.T.: 5.817 min
Delta R.T.: 0.004 min
Response: 17997038
Conc: 4.97 ng/ml

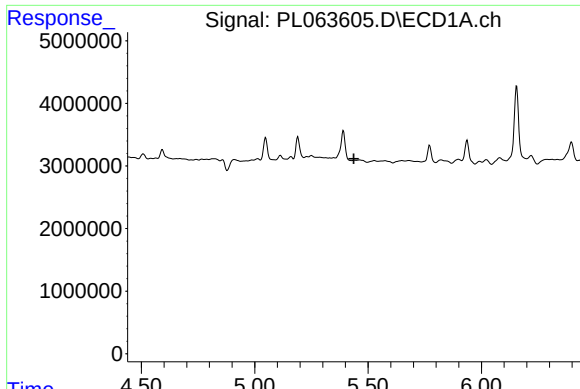

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

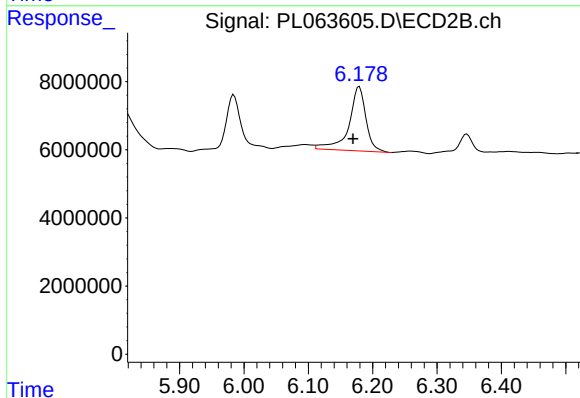


#9 Endosulfan I

R.T.: 6.179 min
Delta R.T.: 0.010 min
Response: 34810235
Conc: 10.43 ng/ml

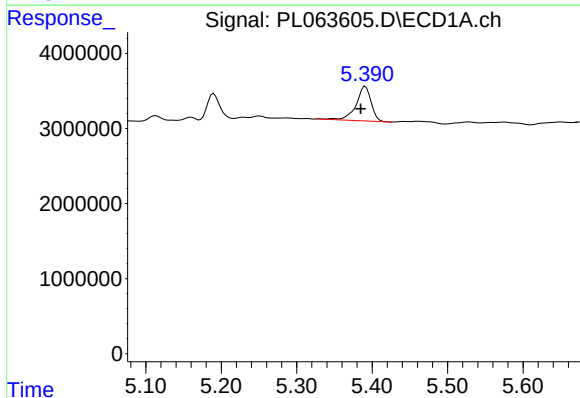


#11 alpha-Chlordane

R.T.: 5.391 min
Delta R.T.: 0.006 min
Response: 6371943
Conc: 3.43 ng/ml

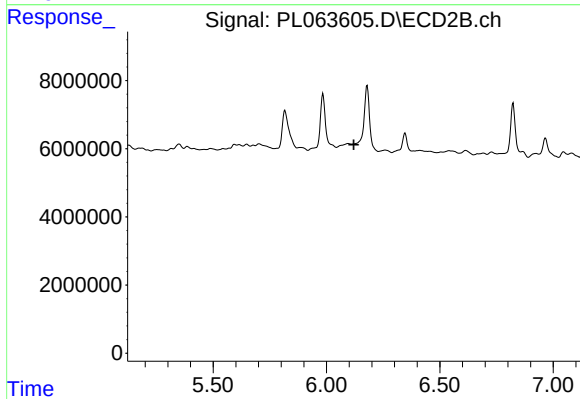

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.120 min
Response: 0
Conc: N.D.

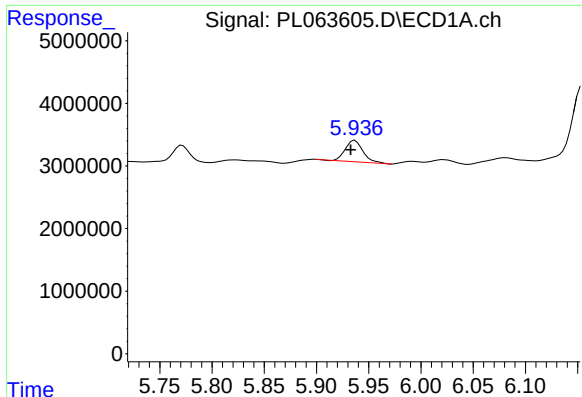

#14 Endrin


R.T.: 5.937 min
Delta R.T.: 0.004 min
Response: 4050241
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

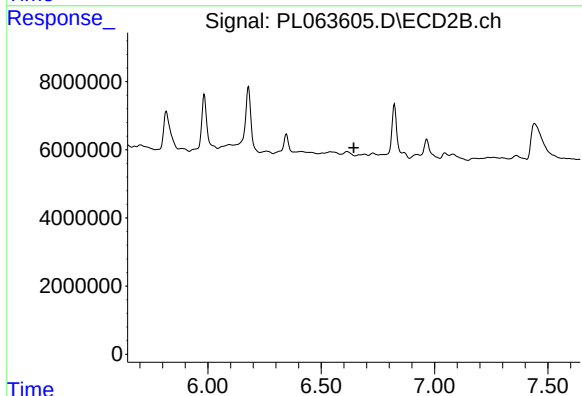


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

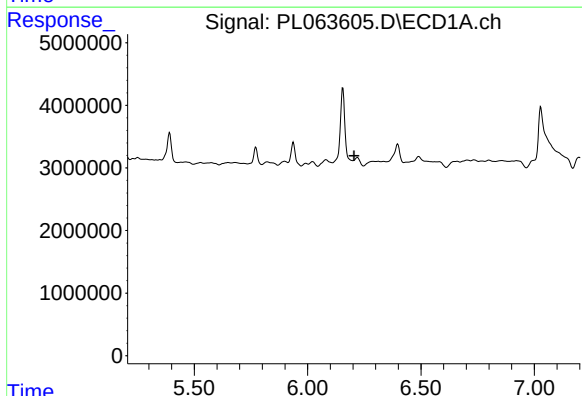


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

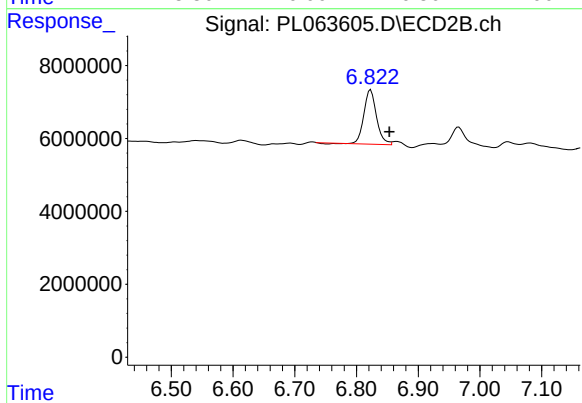

#15 Endosulfan II


R.T.: 6.823 min
Delta R.T.: -0.030 min
Response: 21052413
Conc: 6.61 ng/ml

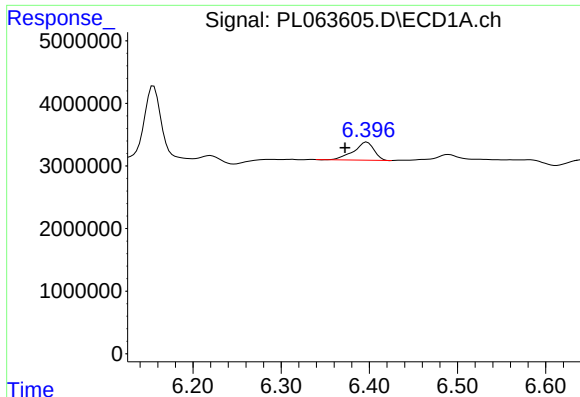

#18 Endrin aldehyde


R.T.: 6.397 min
Delta R.T.: 0.025 min
Response: 4687922
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

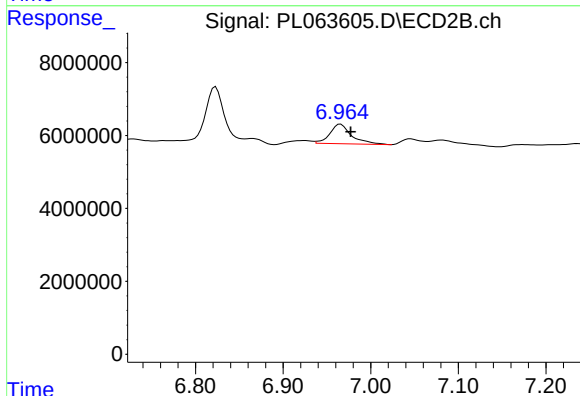


#18 Endrin aldehyde

R.T.: 6.966 min
Delta R.T.: -0.011 min
Response: 9228343
Conc: 3.62 ng/ml

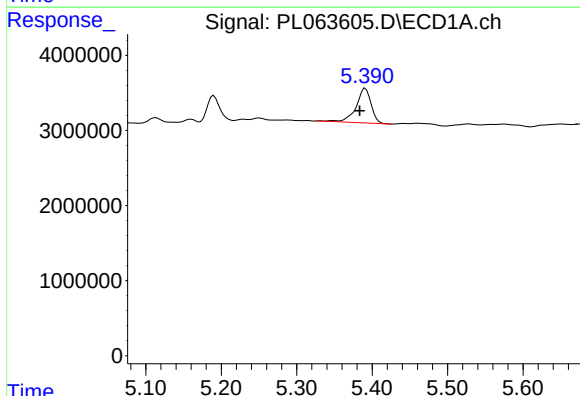


#26 Chlordane-4

R.T.: 5.391 min
Delta R.T.: 0.007 min
Response: 6371943
Conc: 43.56 ng/ml

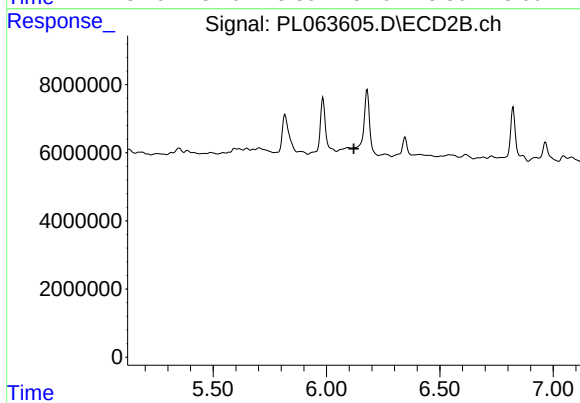

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.121 min
Response: 0
Conc: N.D.

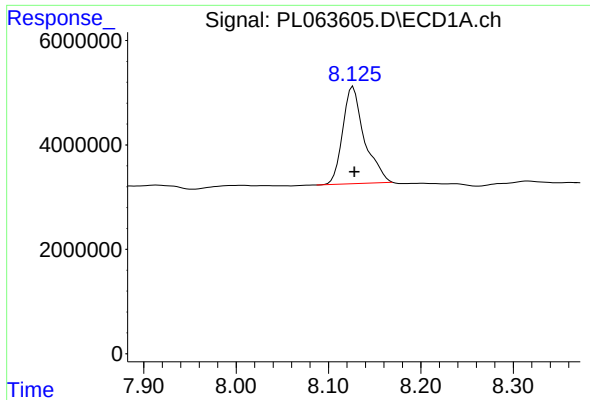

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: -0.001 min
Response: 30335999
Conc: 15.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
JBD-WC-L-SB-02

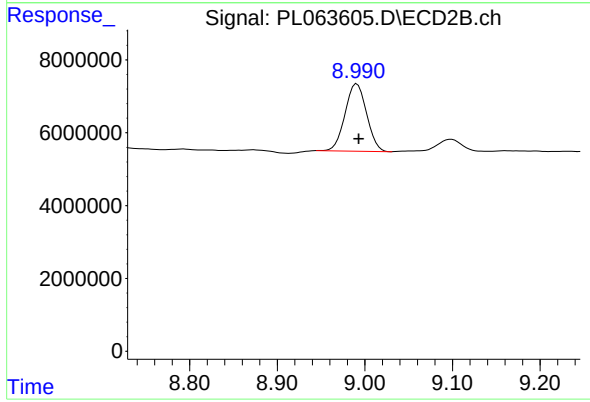

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: -0.002 min
Response: 31659942
Conc: 12.57 ng/ml