

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
 Data File : PL071402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 12:36
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 14:25:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:24:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.496	57399778	119.6E6	115.174	98.433
28)	SA Decachlor...	10.318	11.383	59922296	106.3E6	91.635	96.407
Target Compounds							
23)	Chlordane-1	5.885	6.877	16595348	45193366	984.241	983.204
24)	Chlordane-2	6.573	7.469	20595291	45960458	952.688	974.583
25)	Chlordane-3	7.273	8.225	58607677	177.0E6	1011.461	1011.067
26)	Chlordane-4	7.340	8.307	62318921	208.9E6	1003.934	994.897
27)	Chlordane-5	8.289	9.192	20974478	34359170	980.788	977.943



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
Data File : PL071402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 12:36
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 14:25:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:24:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

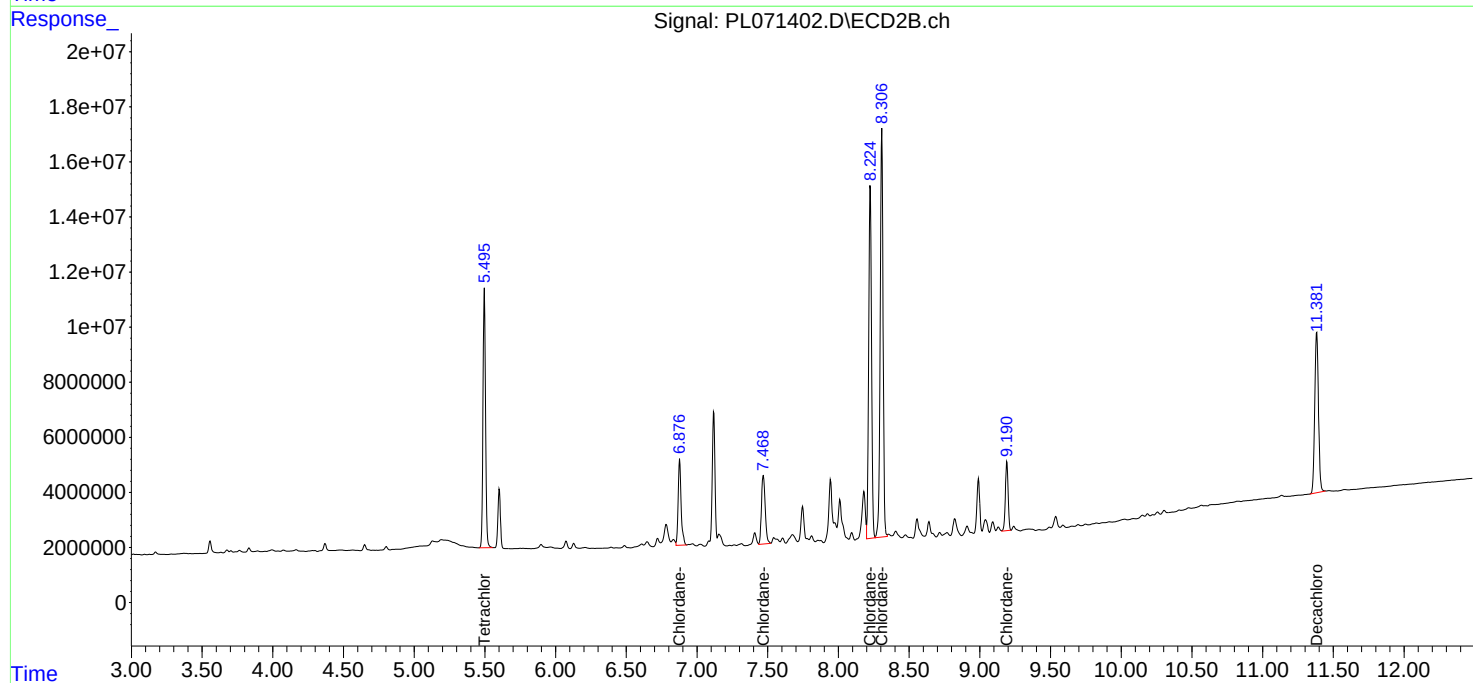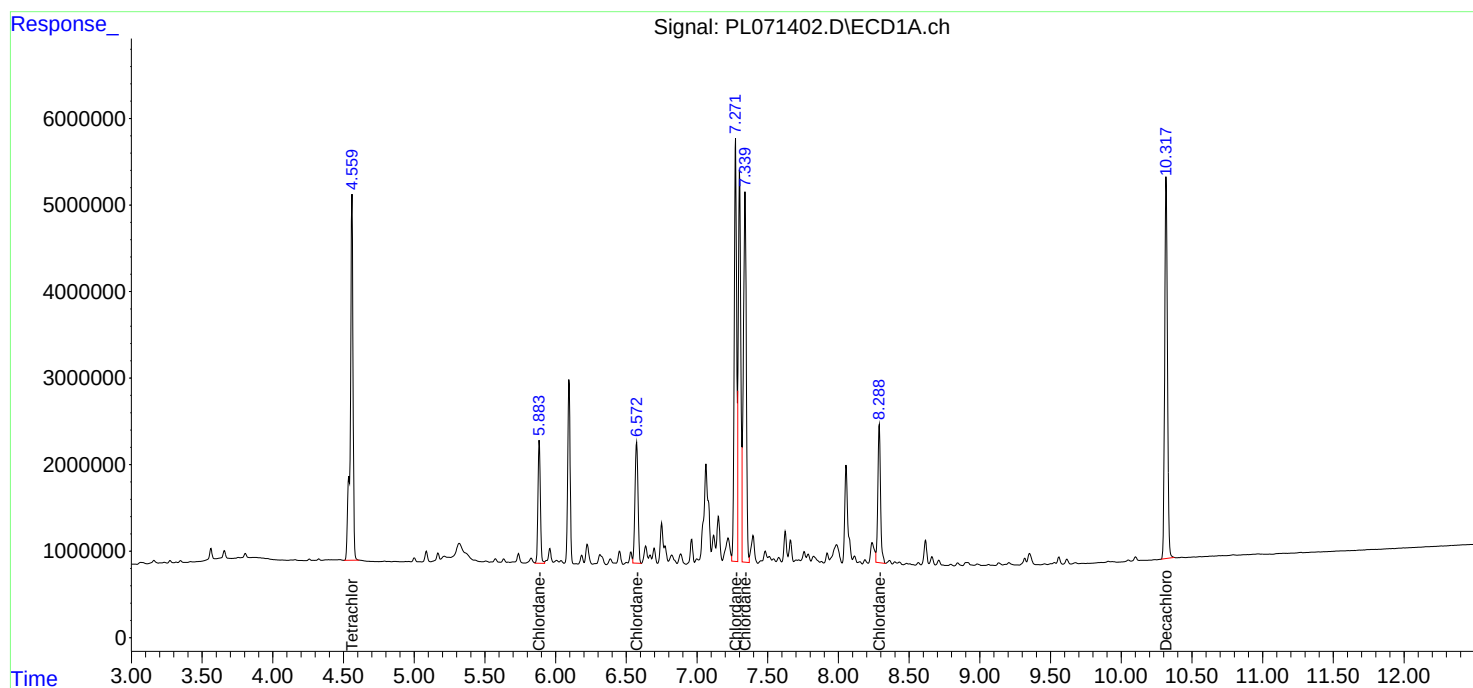


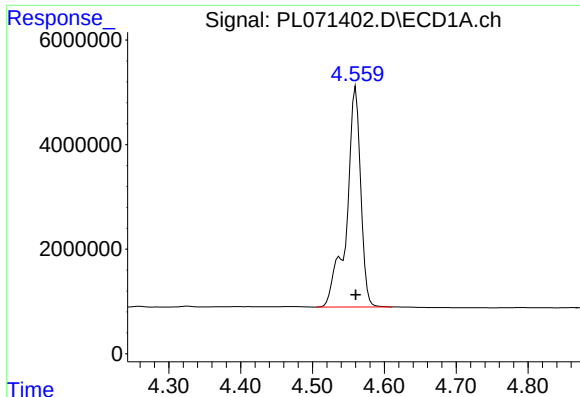

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 57399778
Conc: 115.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

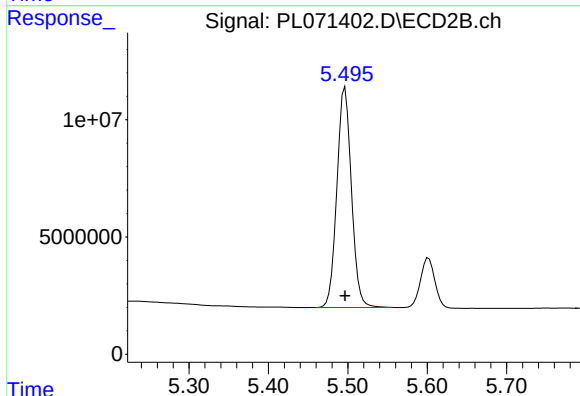


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 119586006
Conc: 98.43 ng/ml

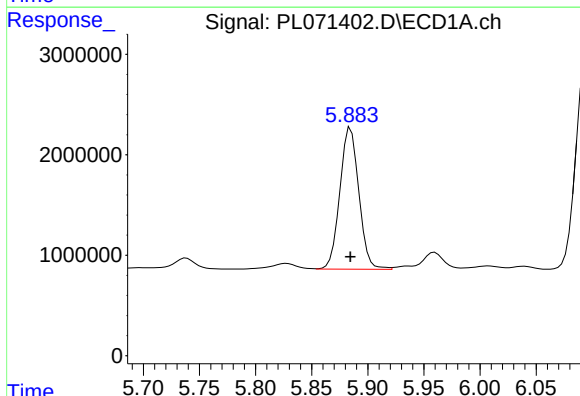


#23 Chlordane-1

R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 16595348
Conc: 984.24 ng/ml

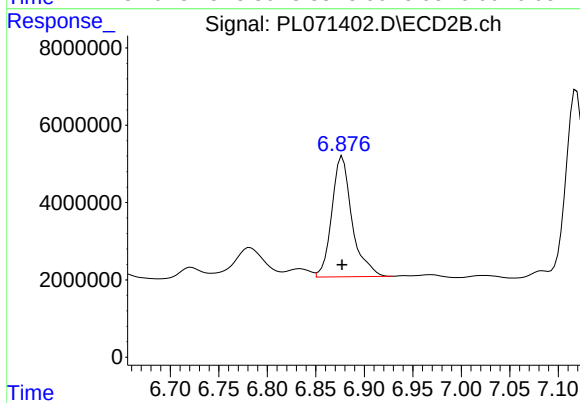

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 45193366
Conc: 983.20 ng/ml

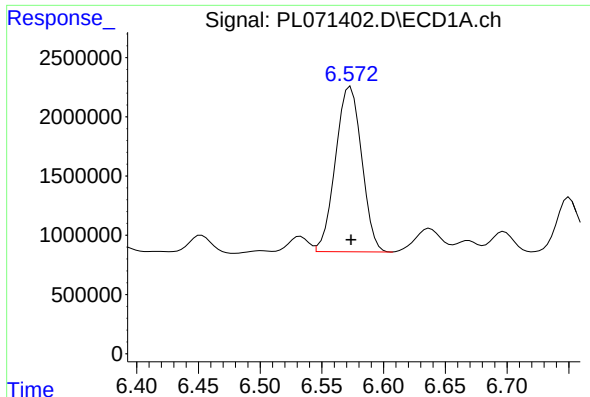

#24 Chlordane-2


R.T.: 6.573 min
Delta R.T.: 0.000 min
Response: 20595291
Conc: 952.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

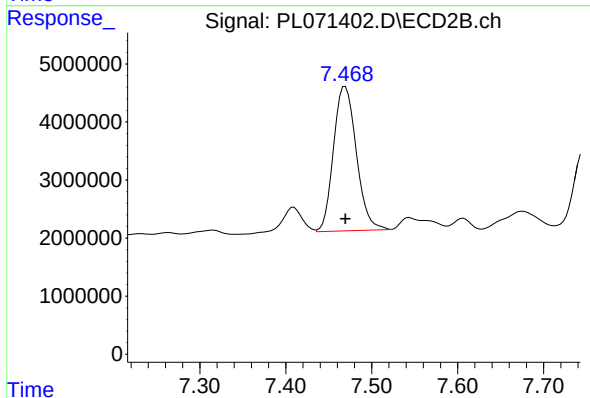


#24 Chlordane-2

R.T.: 7.469 min
Delta R.T.: 0.000 min
Response: 45960458
Conc: 974.58 ng/ml

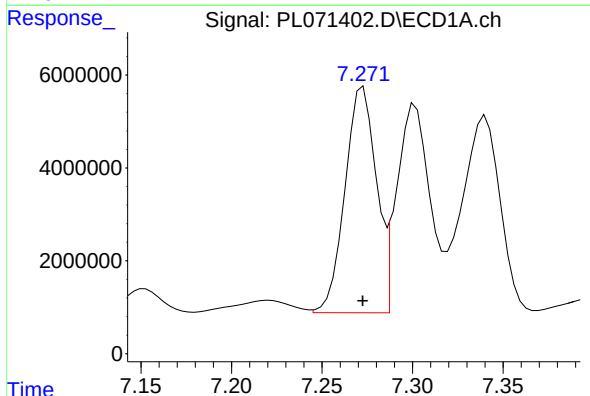


#25 Chlordane-3

R.T.: 7.273 min
Delta R.T.: 0.000 min
Response: 58607677
Conc: 1011.46 ng/ml

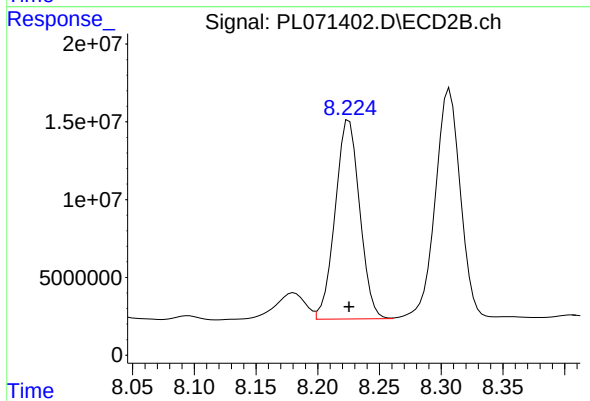

#25 Chlordane-3


R.T.: 8.225 min
Delta R.T.: 0.000 min
Response: 176993009
Conc: 1011.07 ng/ml

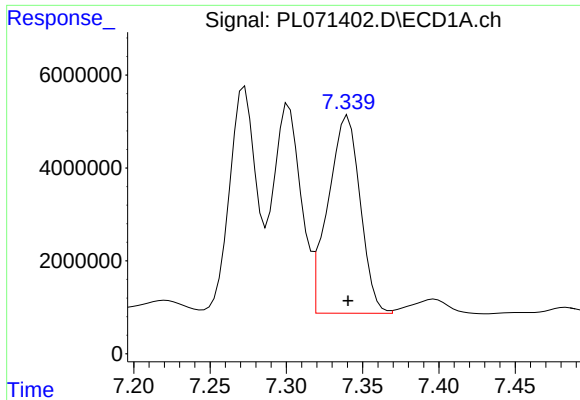

#26 Chlordane-4


R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 62318921
Conc: 1003.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

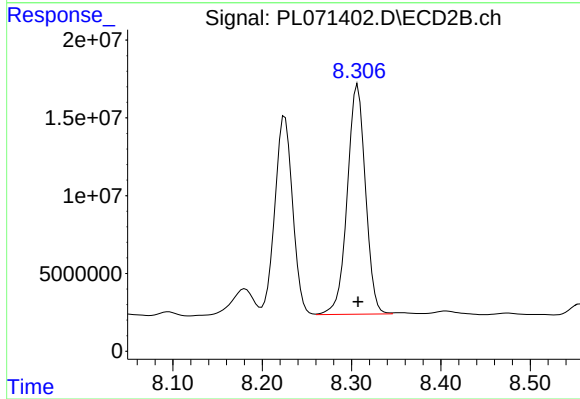


#26 Chlordane-4

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 208882436
Conc: 994.90 ng/ml

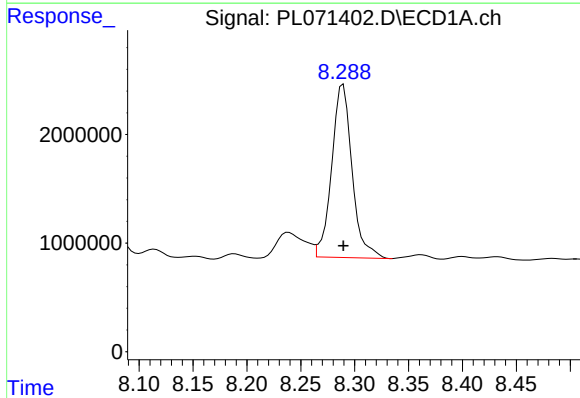


#27 Chlordane-5

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 20974478
Conc: 980.79 ng/ml

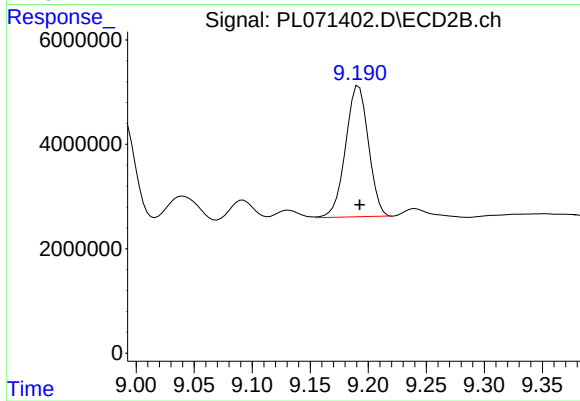

#27 Chlordane-5


R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 34359170
Conc: 977.94 ng/ml

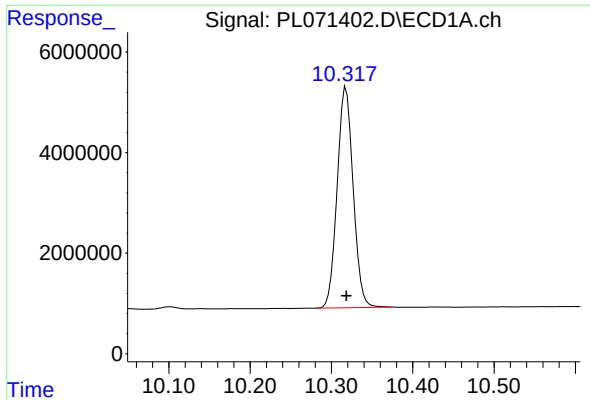

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 59922296
Conc: 91.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

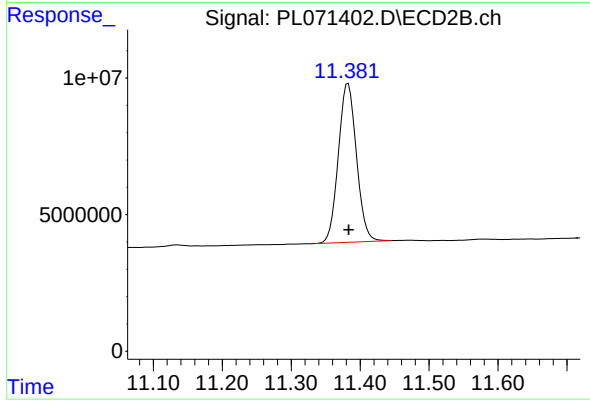

#28 Decachlorobiphenyl

R.T.: 11.383 min
Delta R.T.: 0.000 min
Response: 106295120
Conc: 96.41 ng/ml