

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
 Data File : PL071403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 12:53
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 14:25:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:24:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.497	36578553	88887049	73.396	73.164
28)	SA Decachlor...	10.318	11.384	45828539	79441798	70.082	72.051
Target Compounds							
23)	Chlordane-1	5.885	6.877	12325274	32968578	730.991	717.248
24)	Chlordane-2	6.573	7.469	15516625	33945029	717.761	719.798
25)	Chlordane-3	7.272	8.226	42917741	129.2E6	740.681	738.088
26)	Chlordane-4	7.340	8.307	45757970	153.2E6	737.143	729.486
27)	Chlordane-5	8.289	9.192	15805799	25472242	739.095	725.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
Data File : PL071403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 12:53
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 14:25:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:24:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

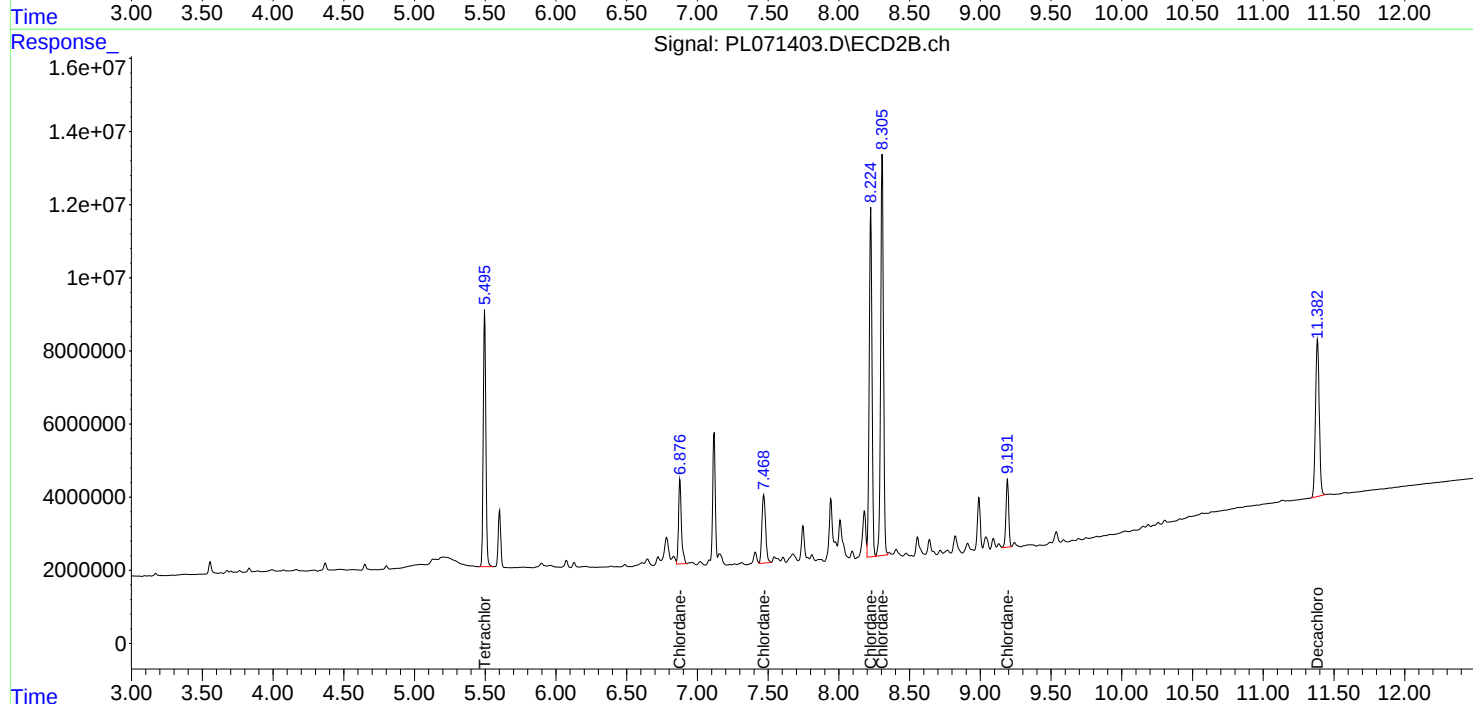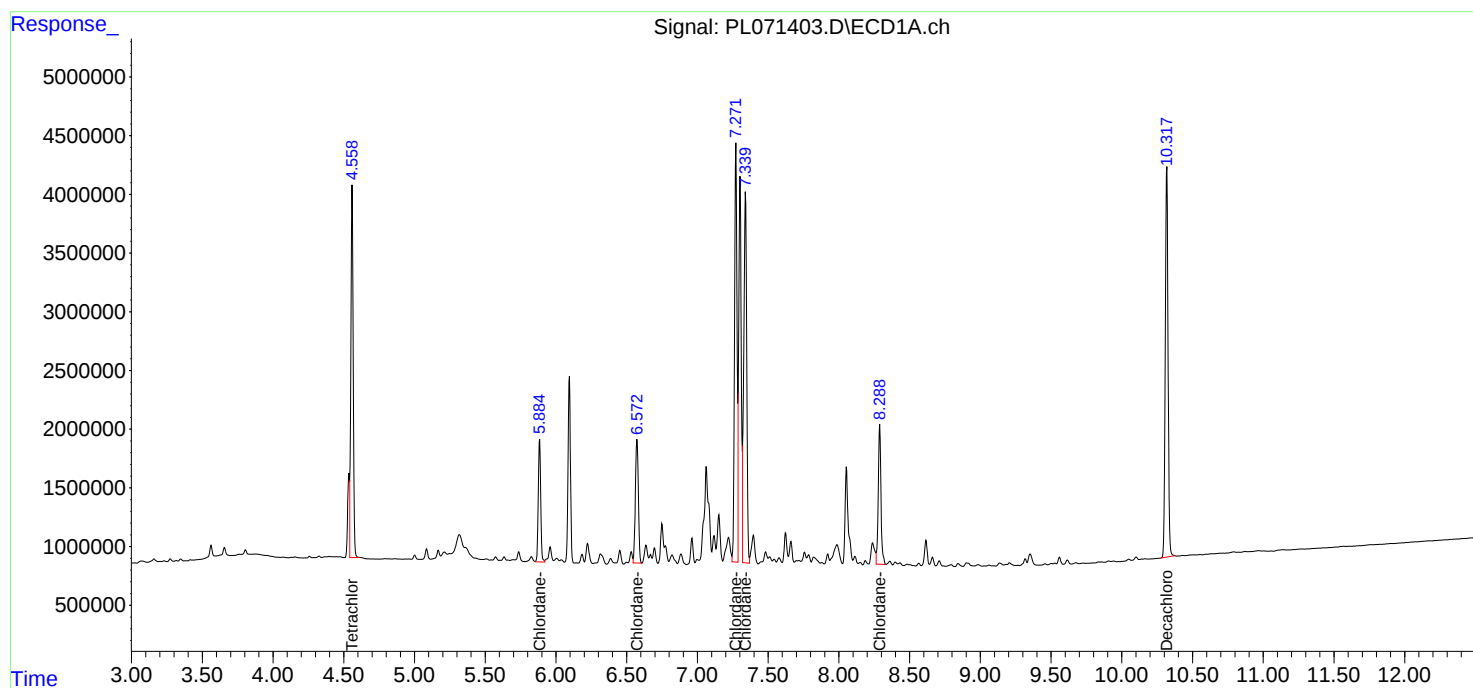


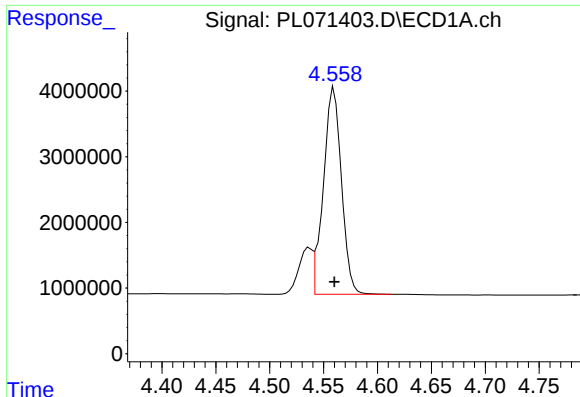

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 36578553
Conc: 73.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

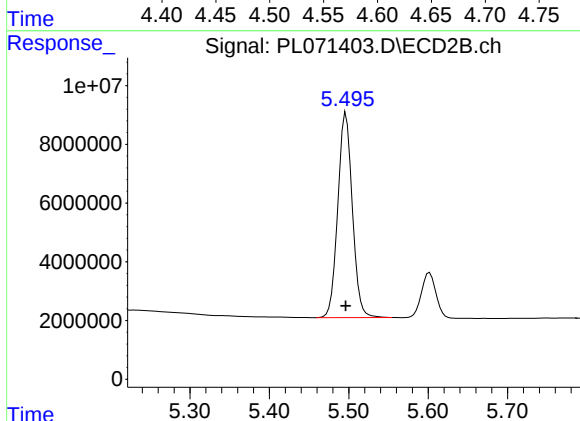


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 88887049
Conc: 73.16 ng/ml

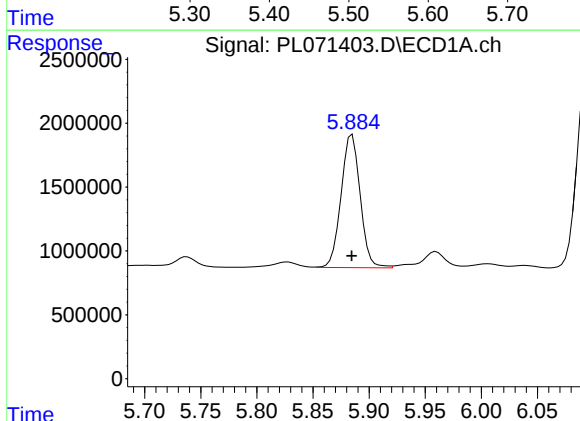


#23 Chlordane-1

R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 12325274
Conc: 730.99 ng/ml

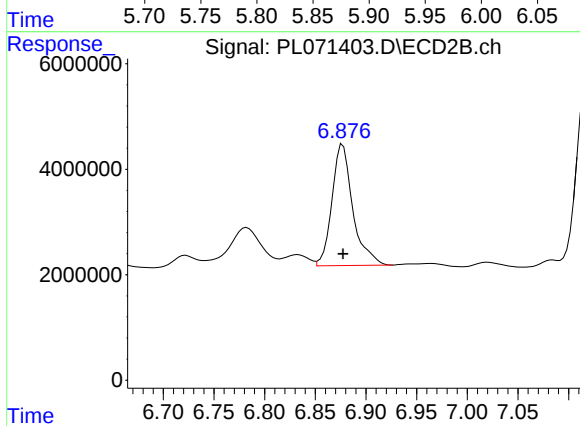

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 32968578
Conc: 717.25 ng/ml

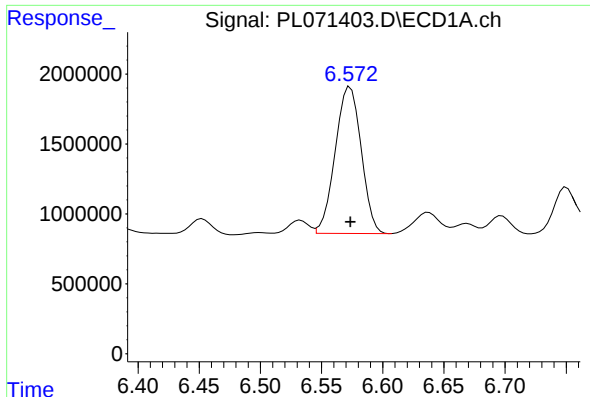

#24 Chlordane-2


R.T.: 6.573 min
Delta R.T.: 0.000 min
Response: 15516625
Conc: 717.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

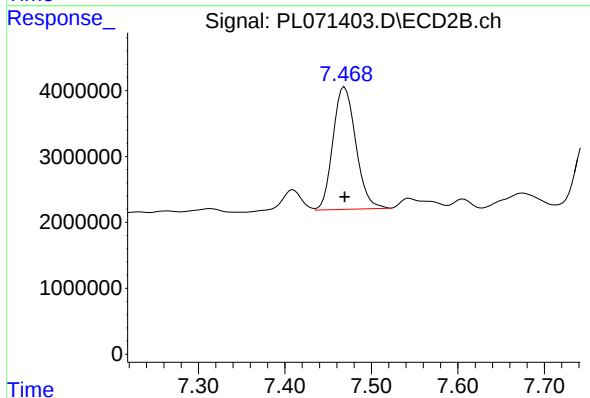


#24 Chlordane-2

R.T.: 7.469 min
Delta R.T.: 0.000 min
Response: 33945029
Conc: 719.80 ng/ml

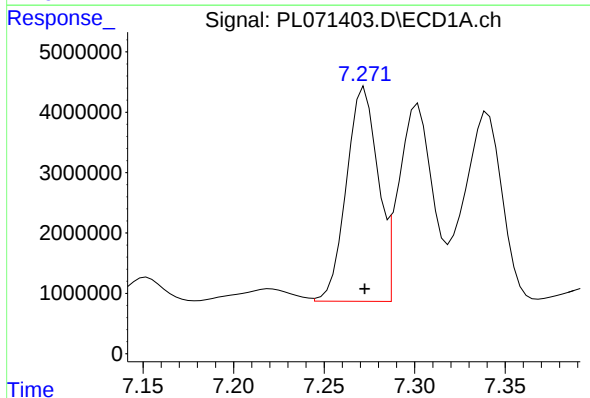


#25 Chlordane-3

R.T.: 7.272 min
Delta R.T.: 0.000 min
Response: 42917741
Conc: 740.68 ng/ml

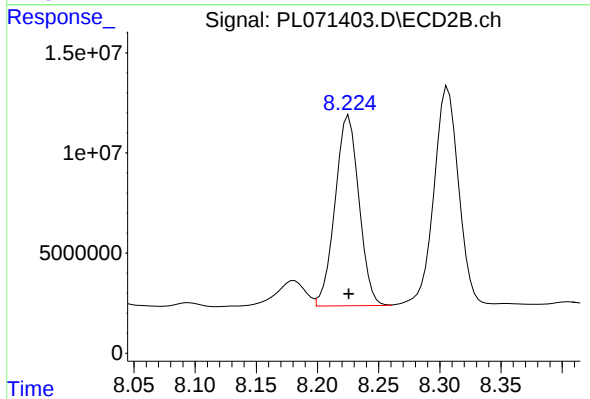

#25 Chlordane-3


R.T.: 8.226 min
Delta R.T.: 0.000 min
Response: 129206479
Conc: 738.09 ng/ml

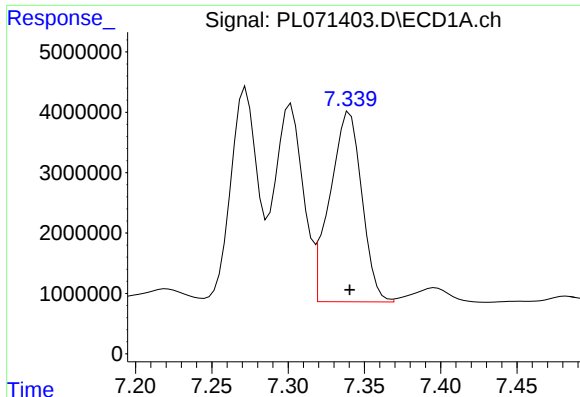

#26 Chlordane-4


R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 45757970
Conc: 737.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

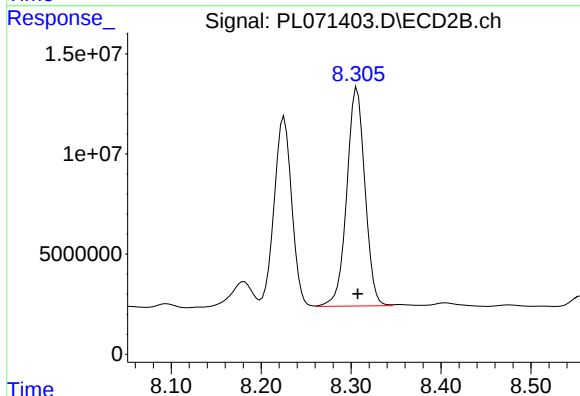


#26 Chlordane-4

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 153158413
Conc: 729.49 ng/ml

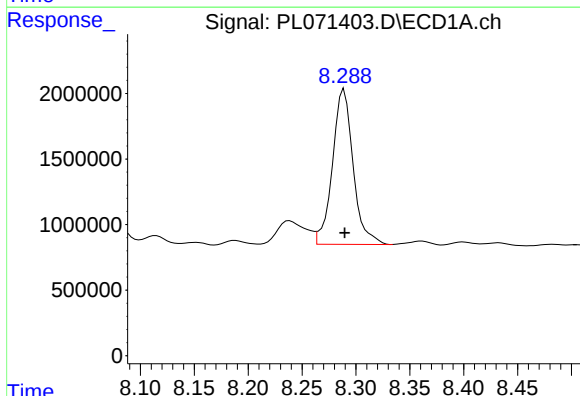


#27 Chlordane-5

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 15805799
Conc: 739.10 ng/ml

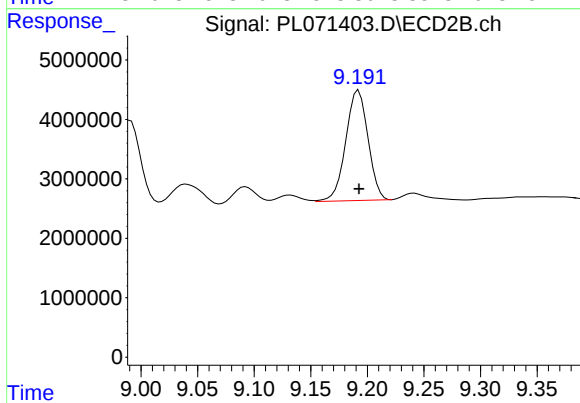

#27 Chlordane-5


R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 25472242
Conc: 725.00 ng/ml

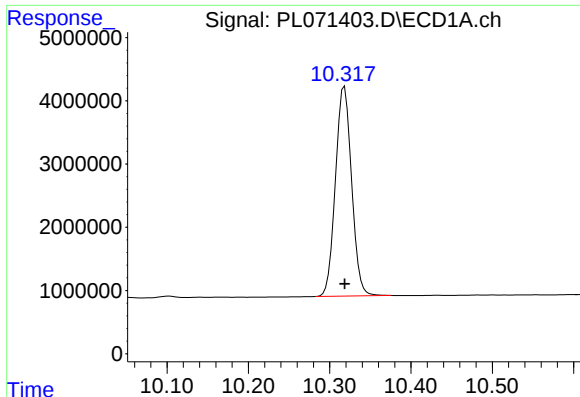

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 45828539
Conc: 70.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

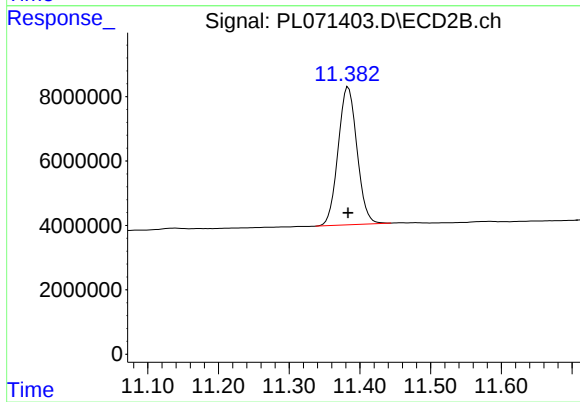

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: 0.000 min
Response: 79441798
Conc: 72.05 ng/ml