

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
 Data File : PL071434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 23:17
 Operator : AR\AJ
 Sample : M5064-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SASP2-121-1-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 03:11:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.496	9542987	24686478	20.133	20.722
28)	SA Decachlor...	10.317	11.383	13038020	21272898	19.624	19.580

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121421\
Data File : PL071434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 23:17
Operator : AR\AJ
Sample : M5064-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SASP2-121-1-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 03:11:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

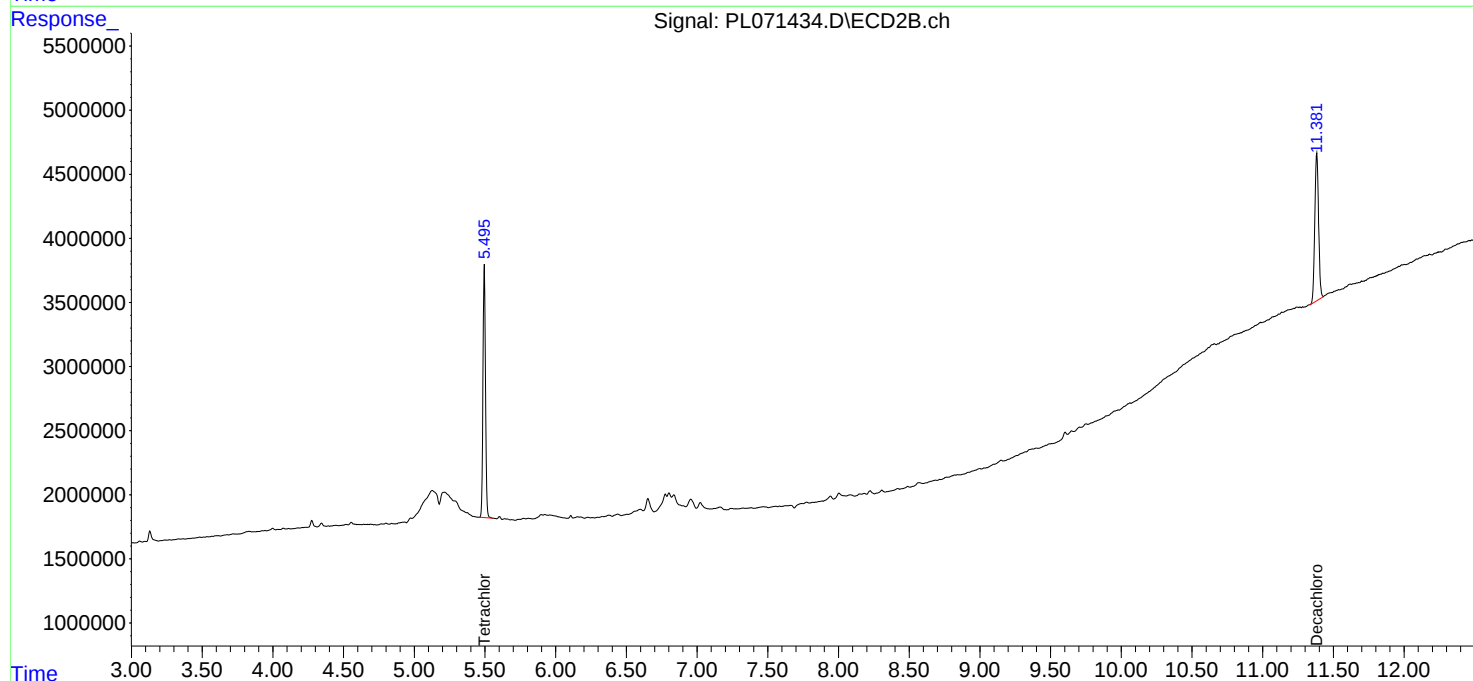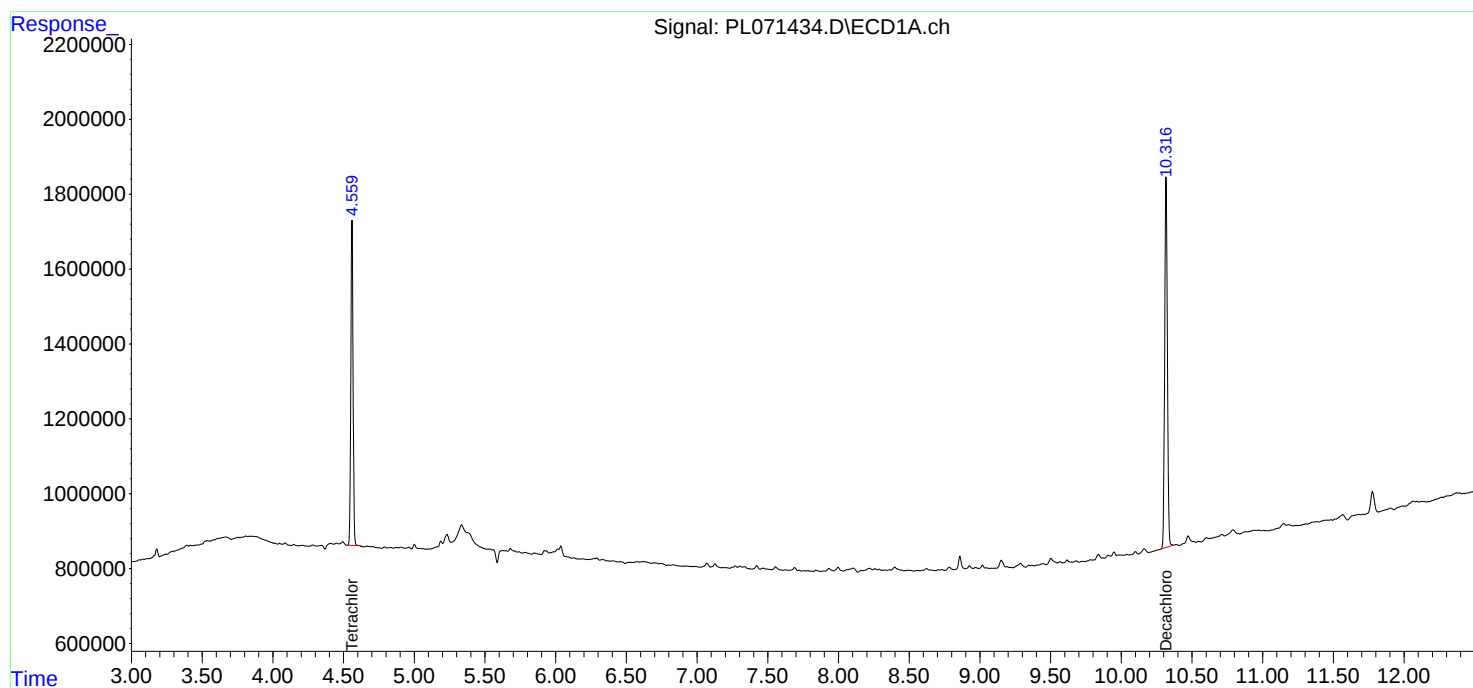


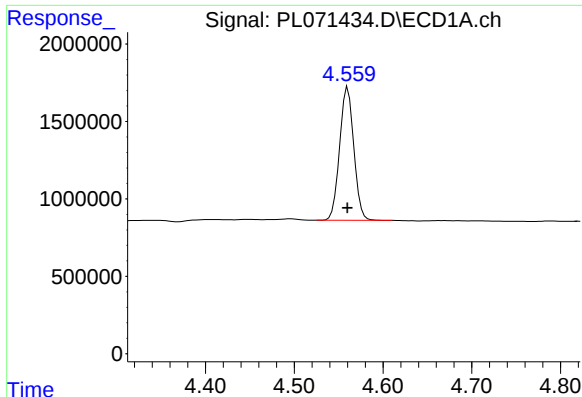

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 9542987
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
SASP2-121-1-(0-5)

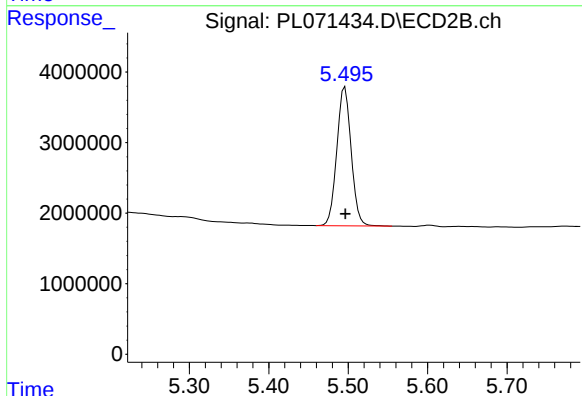


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 24686478
Conc: 20.72 ng/ml

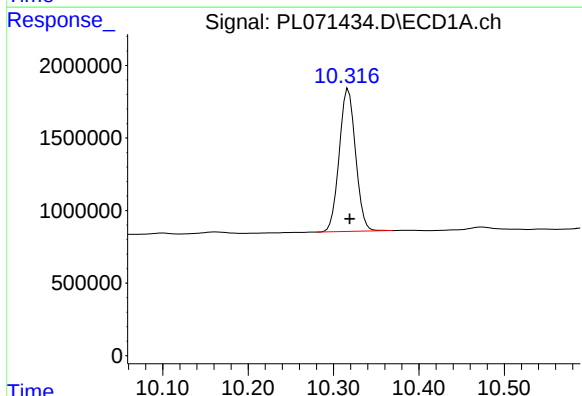

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.002 min
Response: 13038020
Conc: 19.62 ng/ml

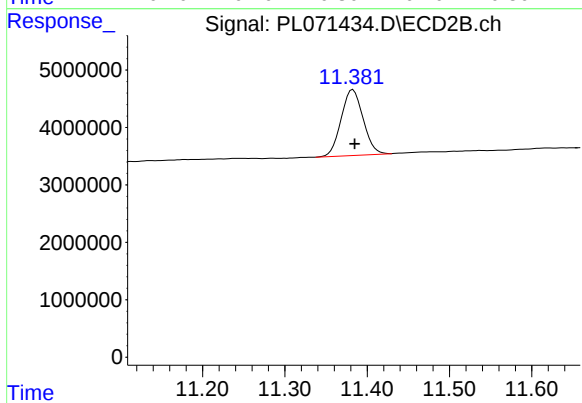

#28 Decachlorobiphenyl

R.T.: 11.383 min
Delta R.T.: -0.002 min
Response: 21272898
Conc: 19.58 ng/ml