

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 00:33
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:51:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:49:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	2.682	263.8E6	150.0E6	74.752	74.880
28)	SA Decachlor...	8.988	7.876	213.9E6	107.2E6	65.969	65.364
Target Compounds							
23)	Chlordane-1	4.596	3.687	115.5E6	45505566	734.565	738.283
24)	Chlordane-2	5.130	4.270	121.6E6	54602046	711.702	714.218
25)	Chlordane-3	5.845	4.905	516.2E6	166.3E6	730.939	735.964
26)	Chlordane-4	5.928	4.968	623.3E6	172.9E6	723.743	730.190
27)	Chlordane-5	6.781	5.642	98785387	46850287	712.387	714.548


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 00:33
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:51:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:49:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

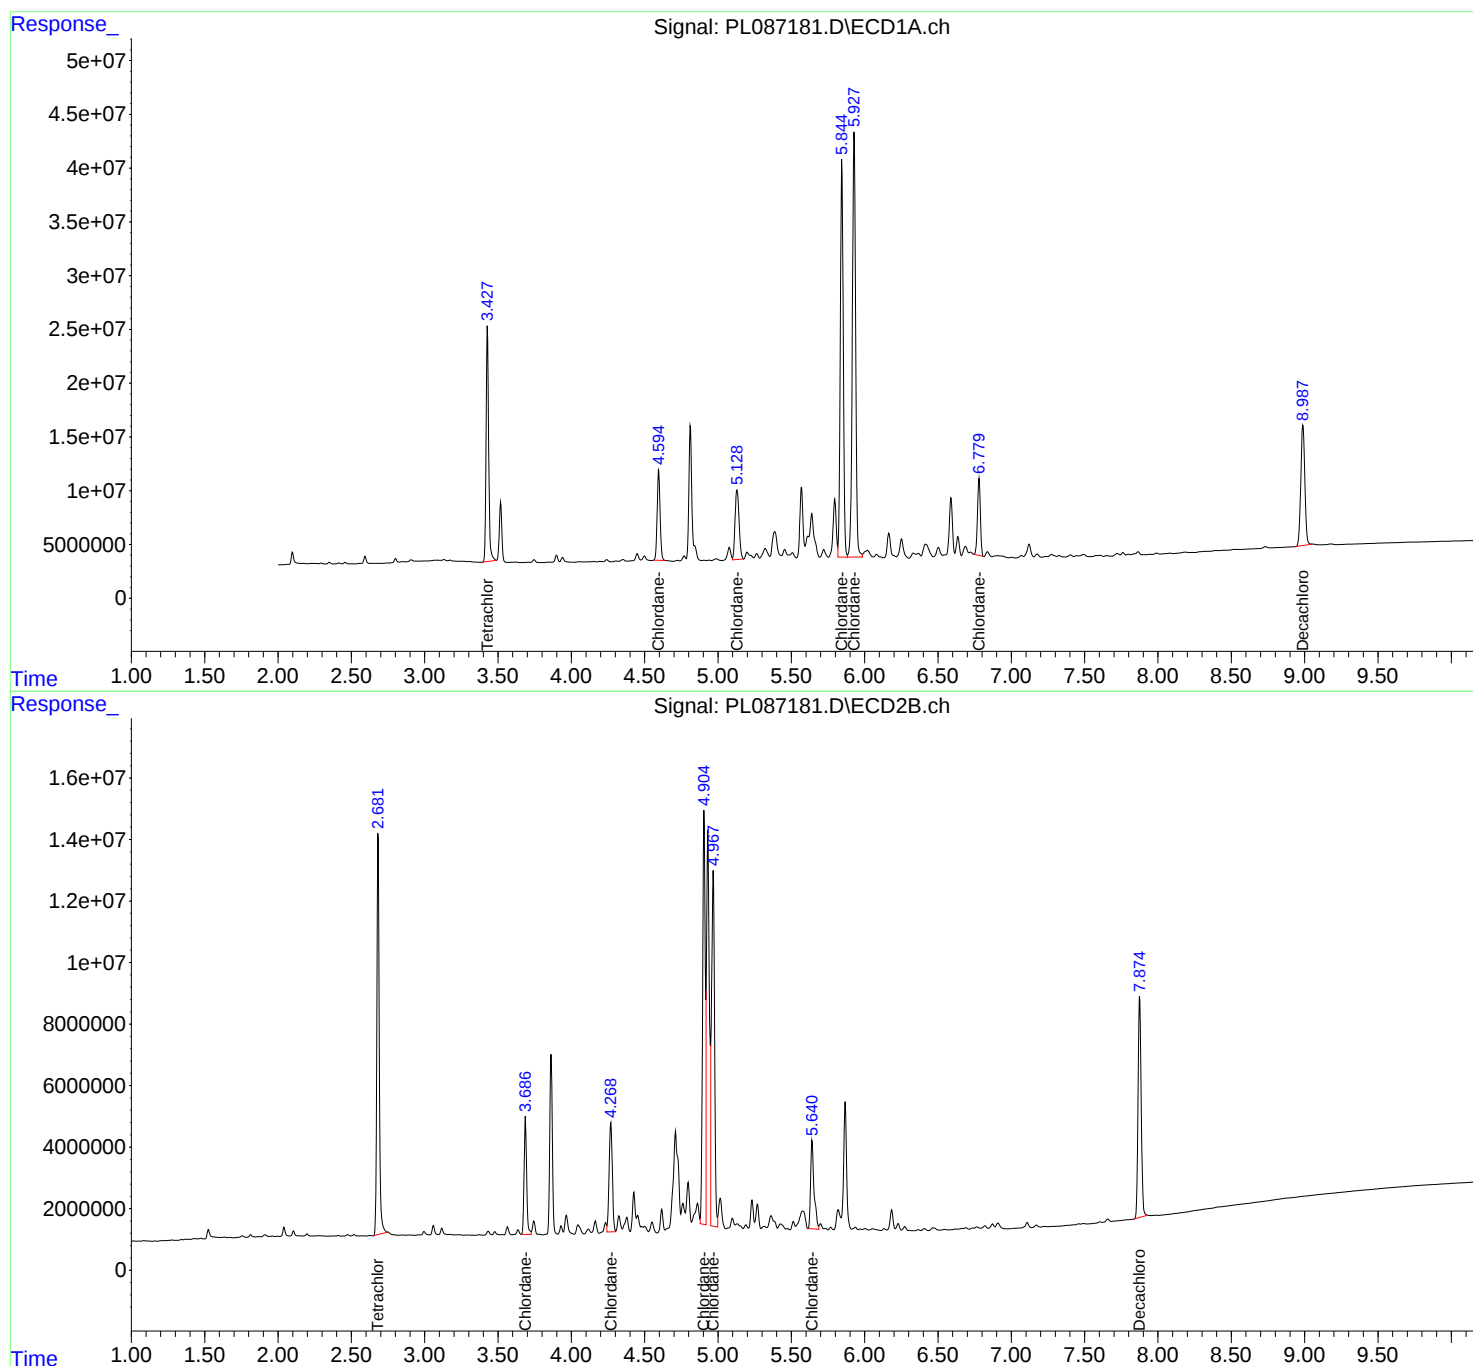


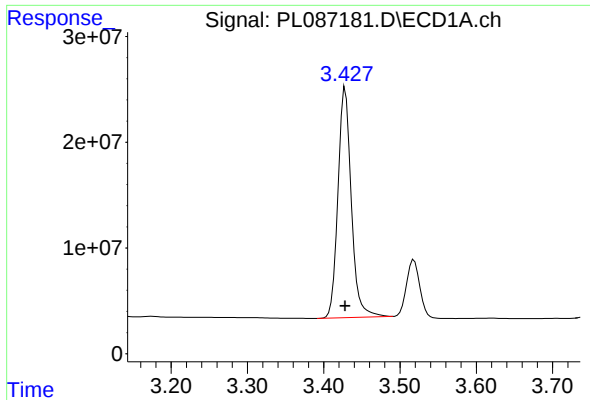

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 263765440
Conc: 74.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

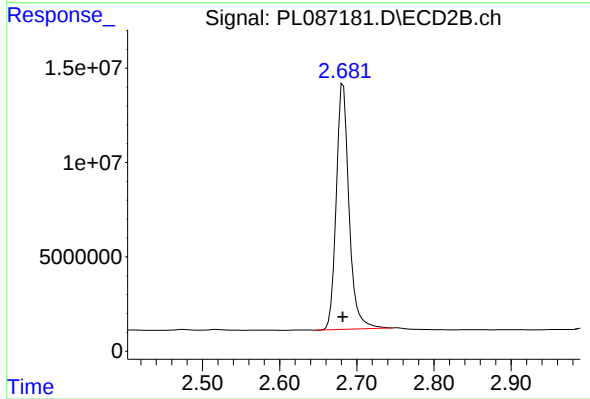


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 150049202
Conc: 74.88 ng/ml

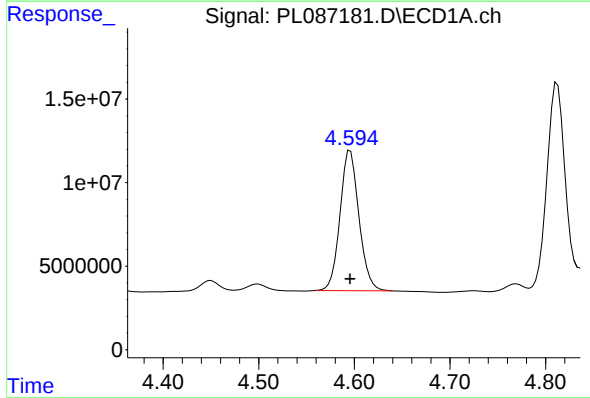


#23 Chlordane-1

R.T.: 4.596 min
Delta R.T.: 0.000 min
Response: 115519053
Conc: 734.56 ng/ml

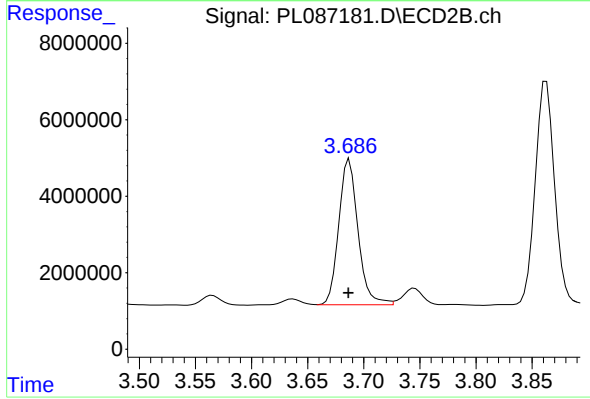

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.001 min
Response: 45505566
Conc: 738.28 ng/ml

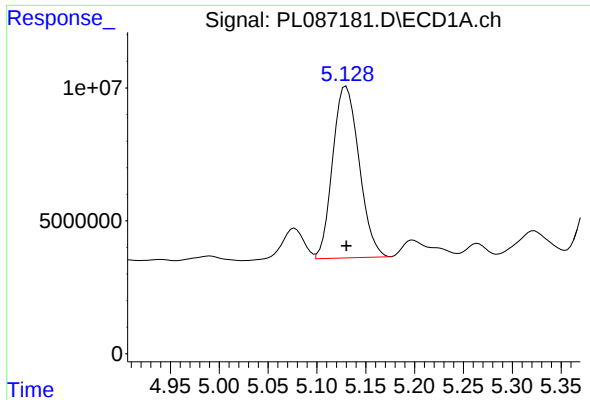

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 121623888
Conc: 711.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

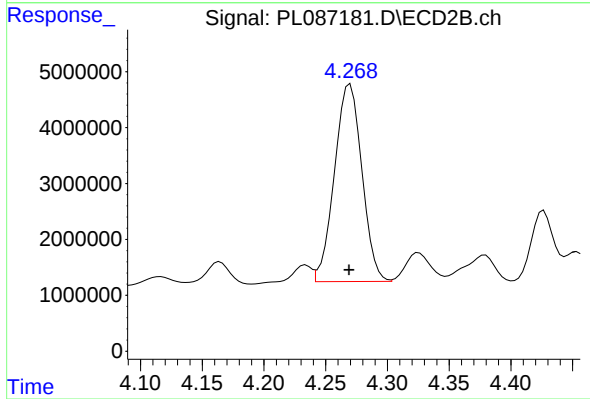


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 54602046
Conc: 714.22 ng/ml

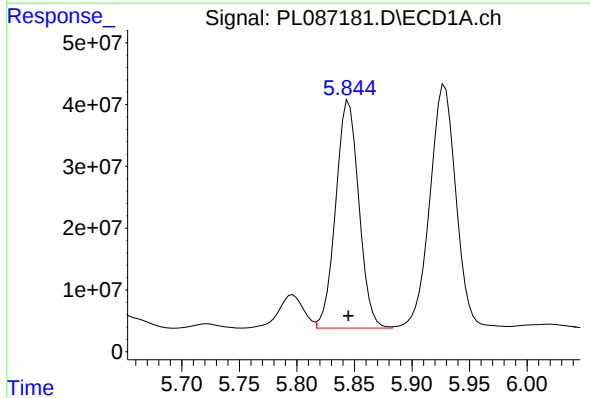


#25 Chlordane-3

R.T.: 5.845 min
Delta R.T.: 0.000 min
Response: 516157499
Conc: 730.94 ng/ml

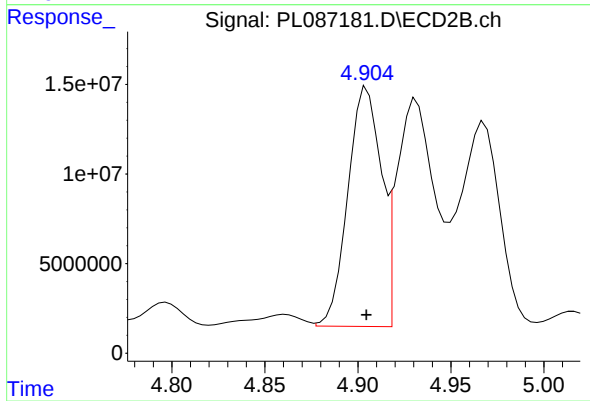

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 166265745
Conc: 735.96 ng/ml

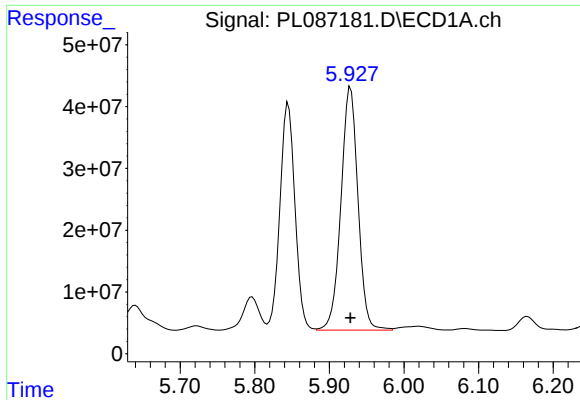

#26 Chlordane-4


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 623255915
Conc: 723.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

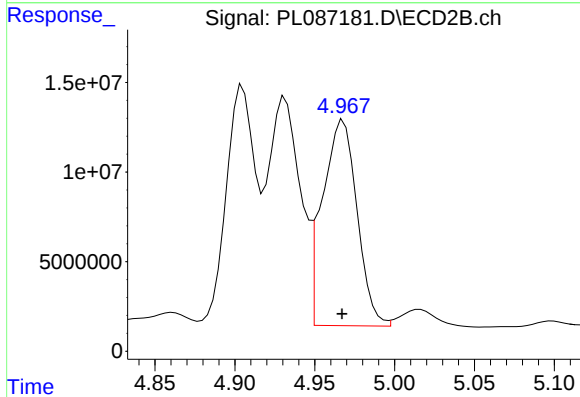


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 172853988
Conc: 730.19 ng/ml

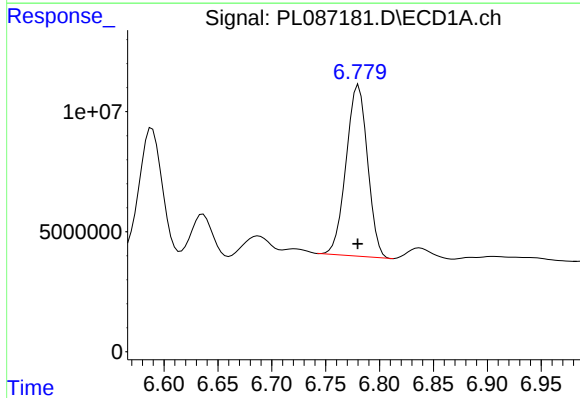


#27 Chlordane-5

R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 98785387
Conc: 712.39 ng/ml

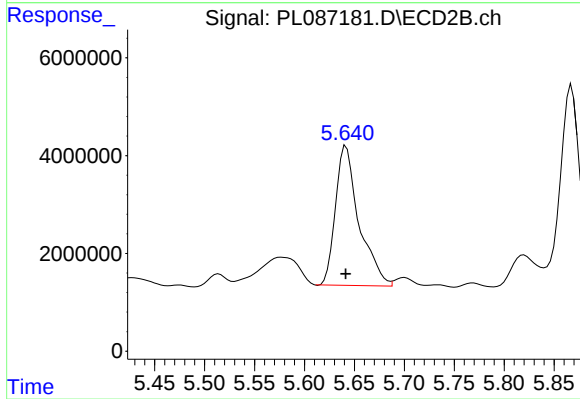

#27 Chlordane-5


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 46850287
Conc: 714.55 ng/ml

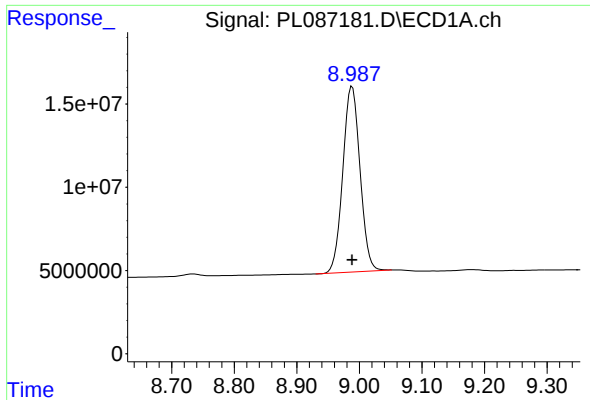

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 213863992
Conc: 65.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

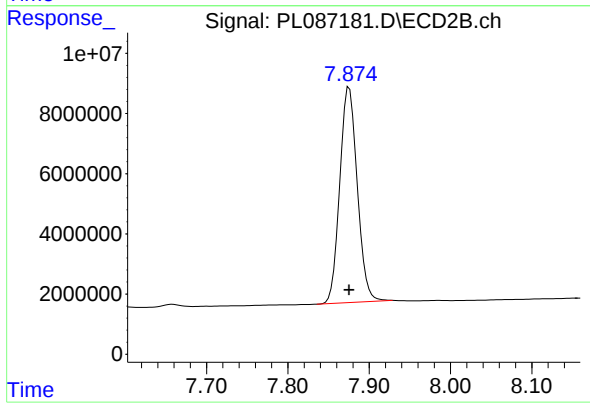

#28 Decachlorobiphenyl

R.T.: 7.876 min
Delta R.T.: 0.000 min
Response: 107200512
Conc: 65.36 ng/ml