

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 00:47
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:51:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:49:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	2.682	176.4E6	100.2E6	50.000	50.000
28)	SA Decachlor...	8.988	7.875	162.1E6	82003312	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.596	3.686	78630960	30818525	500.000	500.000
24)	Chlordane-2	5.130	4.269	85445839	38225082	500.000	500.000
25)	Chlordane-3	5.845	4.905	353.1E6	113.0E6	500.000	500.000
26)	Chlordane-4	5.928	4.967	430.6E6	118.4E6	500.000	500.000
27)	Chlordane-5	6.780	5.642	69334092	32783158	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 00:47
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:51:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:49:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

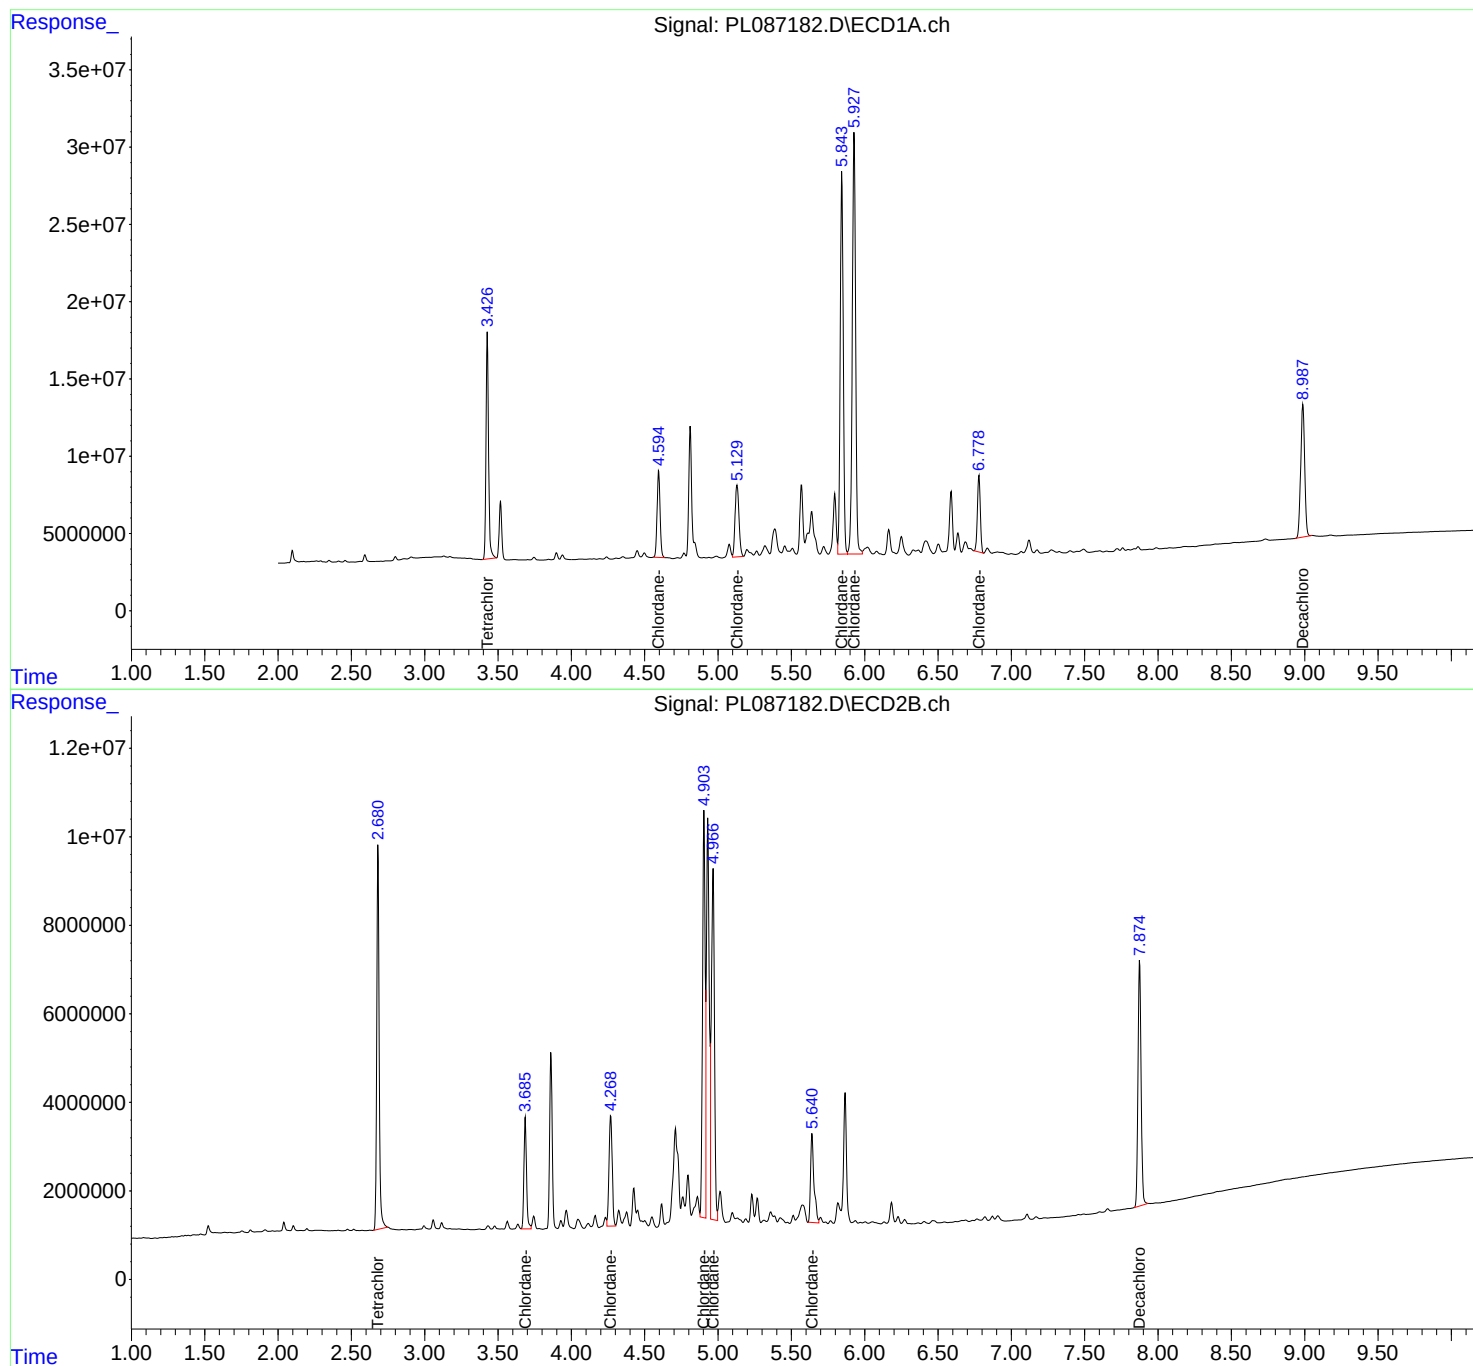


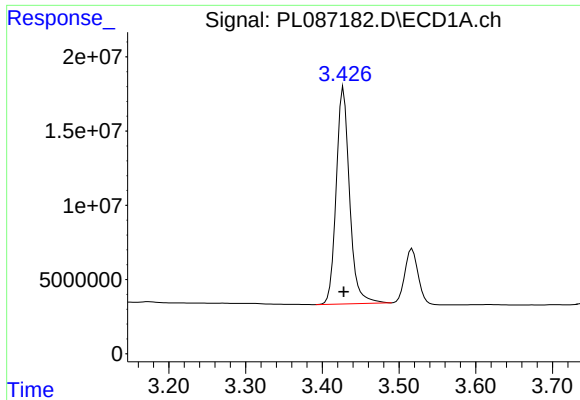

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 176428109
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

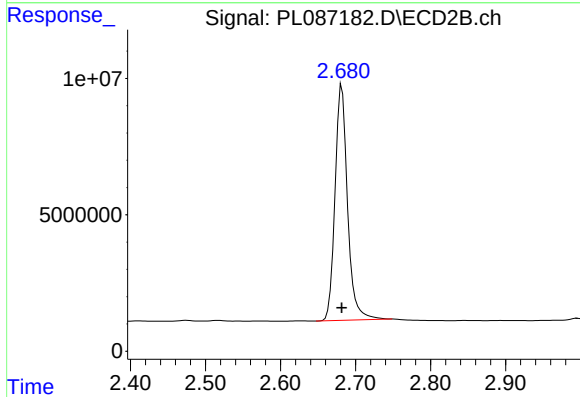


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 100193148
Conc: 50.00 ng/ml

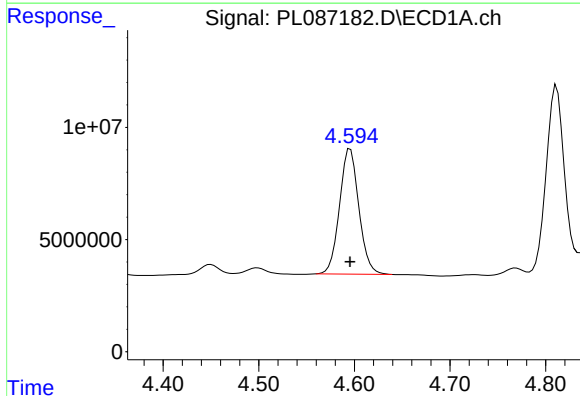


#23 Chlordane-1

R.T.: 4.596 min
Delta R.T.: 0.000 min
Response: 78630960
Conc: 500.00 ng/ml

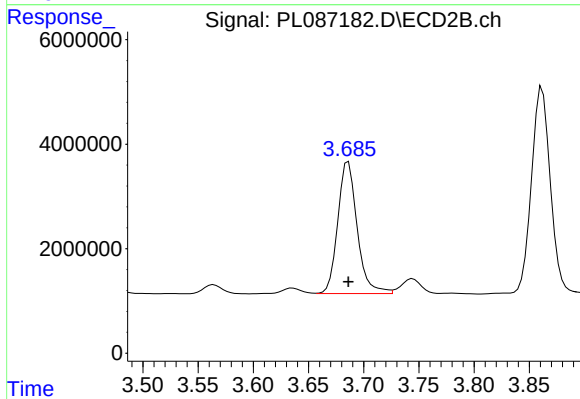

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 30818525
Conc: 500.00 ng/ml

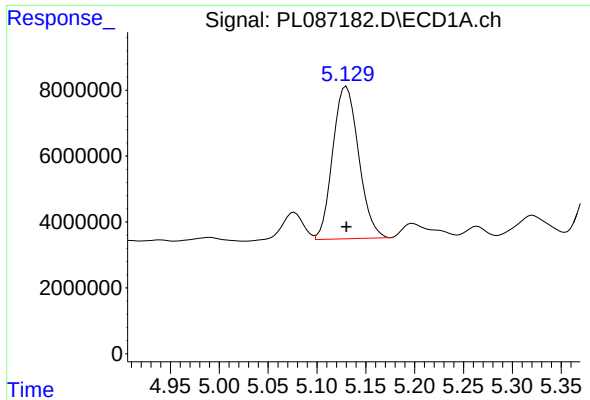

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 85445839
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

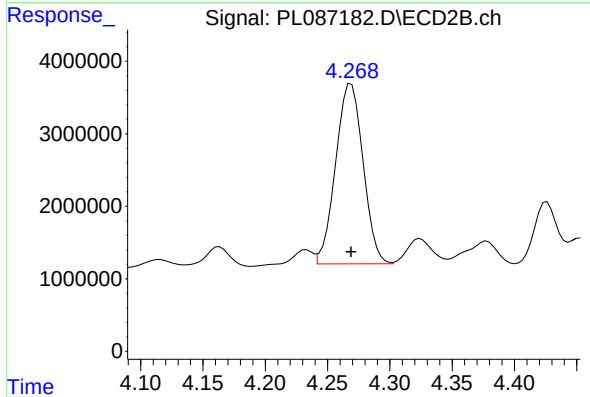


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 38225082
Conc: 500.00 ng/ml

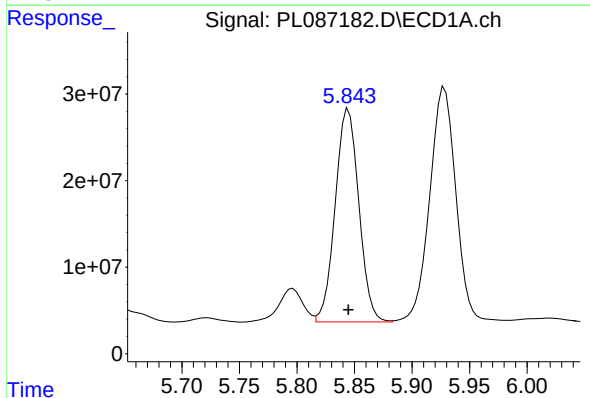


#25 Chlordane-3

R.T.: 5.845 min
Delta R.T.: 0.000 min
Response: 353078533
Conc: 500.00 ng/ml

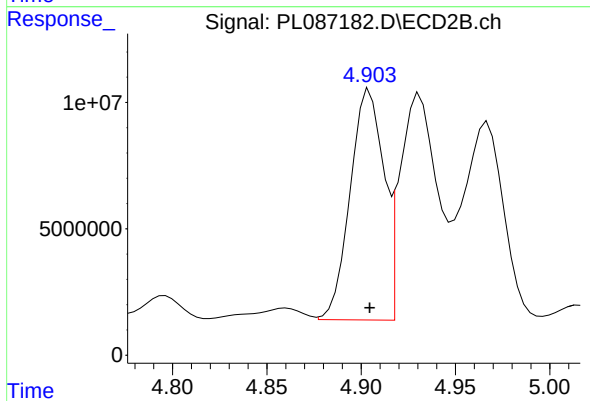

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 112957850
Conc: 500.00 ng/ml

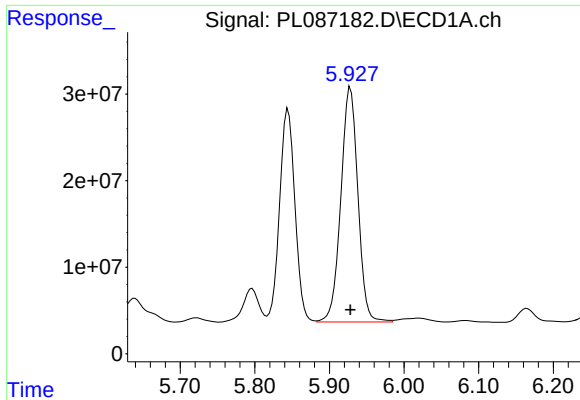

#26 Chlordane-4


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 430578069
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

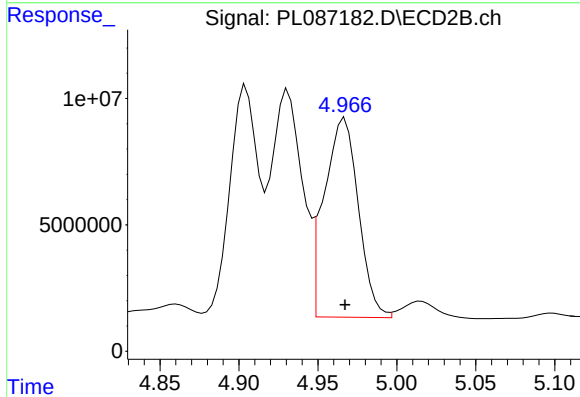


#26 Chlordane-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 118362332
Conc: 500.00 ng/ml

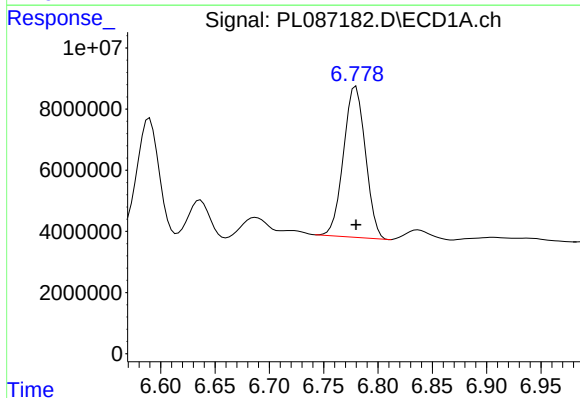


#27 Chlordane-5

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 69334092
Conc: 500.00 ng/ml

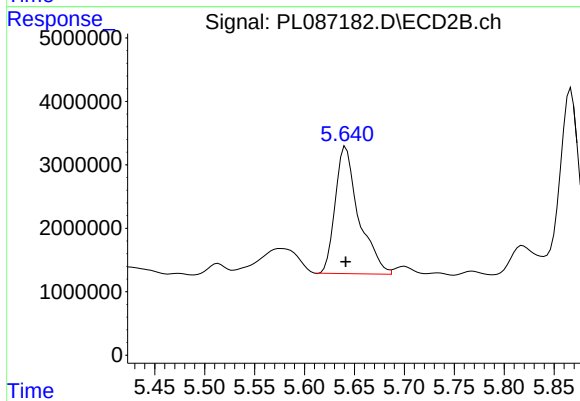

#27 Chlordane-5


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 32783158
Conc: 500.00 ng/ml

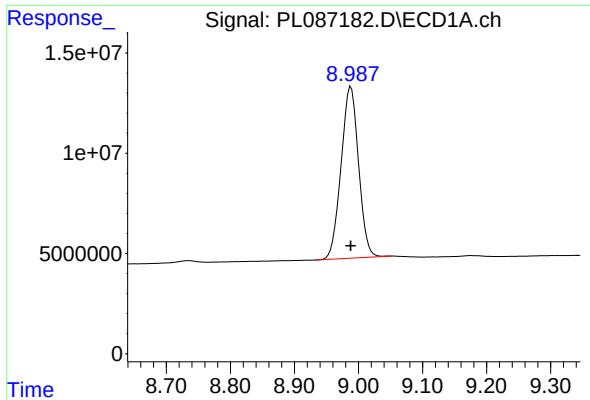

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 162095370
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

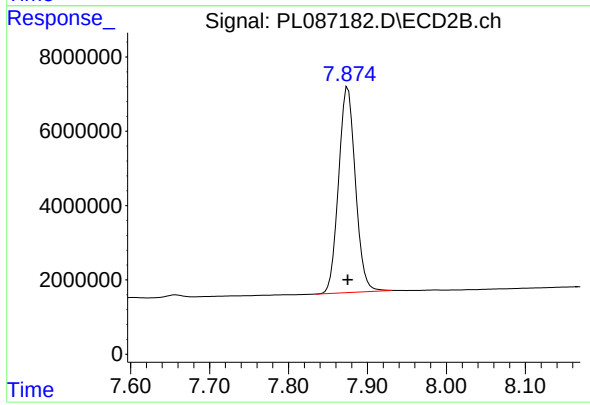

#28 Decachlorobiphenyl

R.T.: 7.875 min
Delta R.T.: 0.000 min
Response: 82003312
Conc: 50.00 ng/ml