

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 00:19
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:56:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:55:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	2.682	358.8E6	206.3E6	100.838	101.445
28)	SA Decachlor...	8.989	7.877	331.4E6	166.6E6	101.100	100.777
Target Compounds							
23)	Chlordane-1	4.596	3.687	160.6E6	63782053	1010.510	1017.103
24)	Chlordane-2	5.130	4.269	167.2E6	75314186	989.099	992.515
25)	Chlordane-3	5.845	4.905	740.3E6	239.0E6	1023.576	1028.245
26)	Chlordane-4	5.928	4.968	889.4E6	248.9E6	1016.137	1025.147
27)	Chlordane-5	6.780	5.642	143.4E6	68025954	1016.801	1018.412



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 00:19
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:56:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:55:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

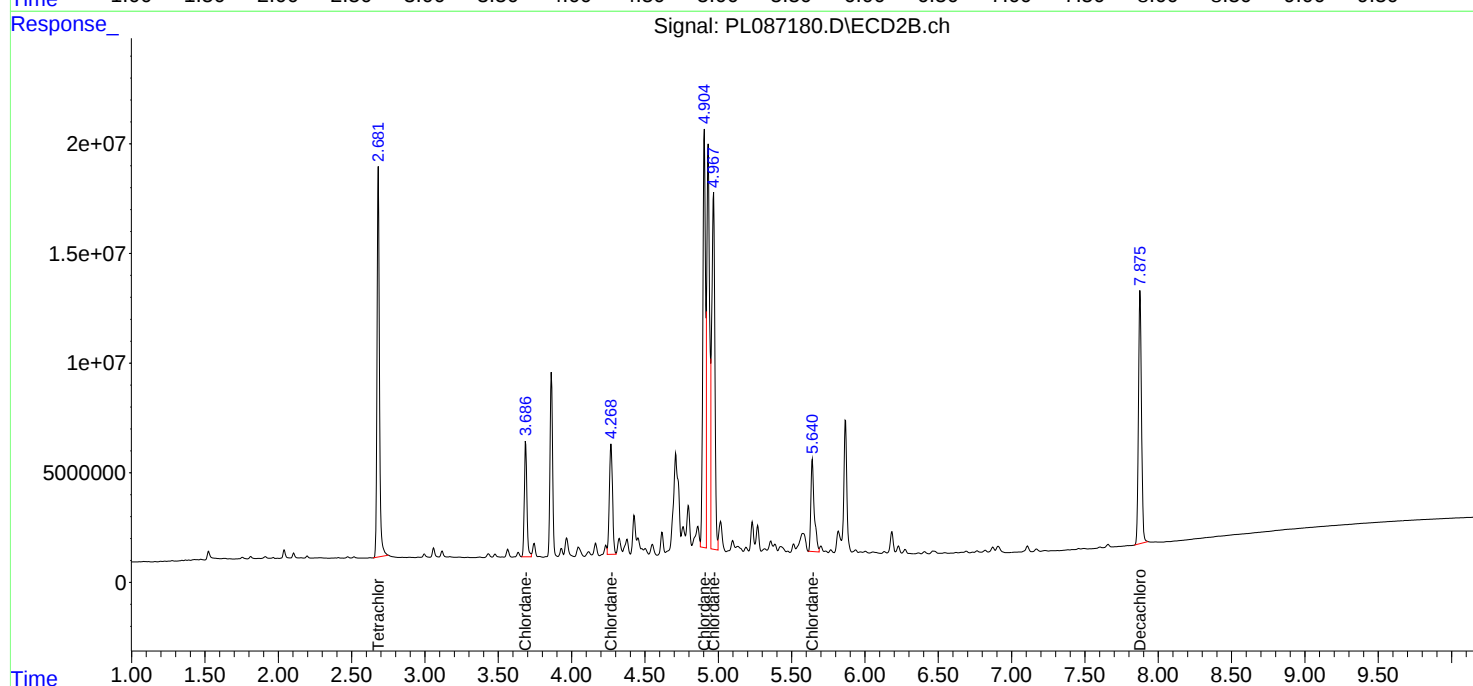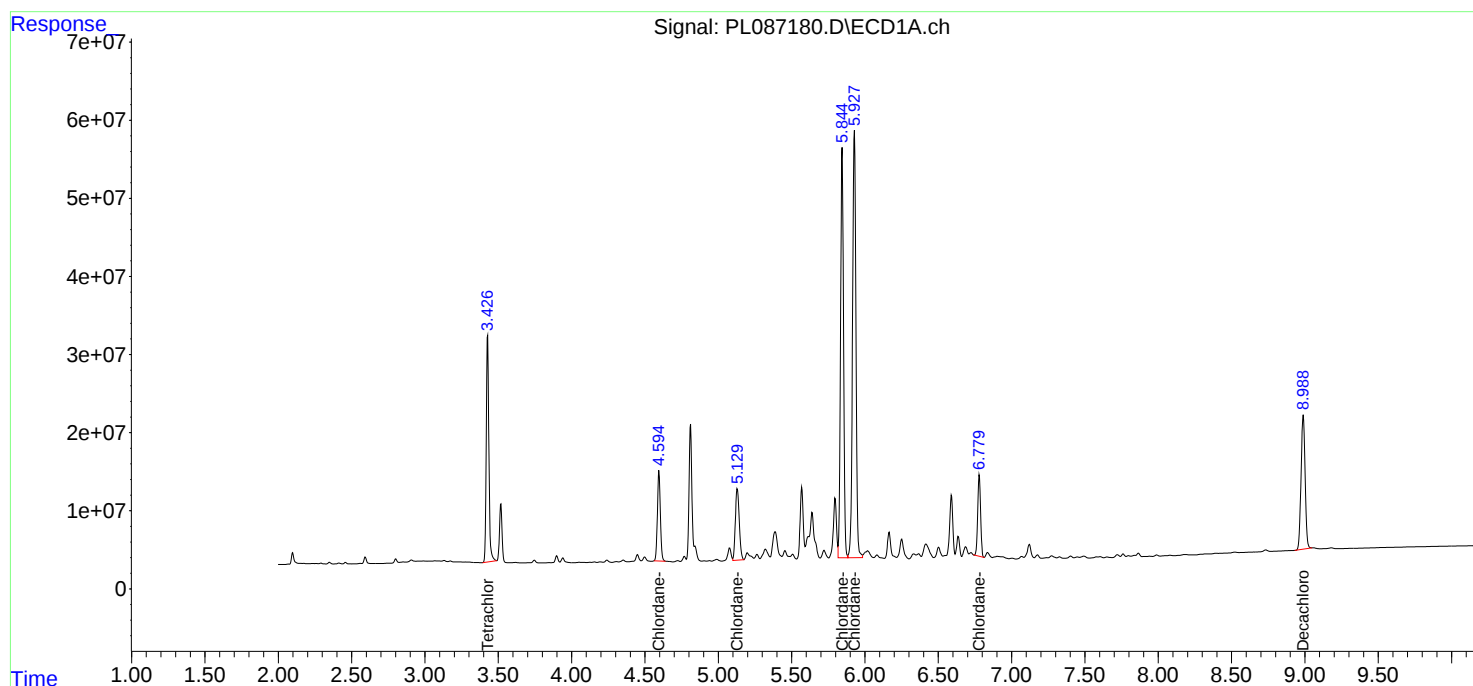


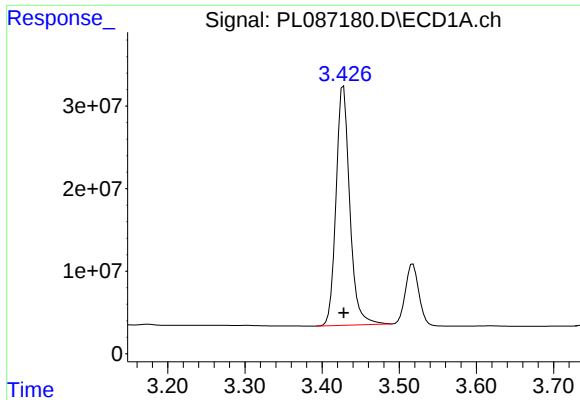

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 358819628
Conc: 100.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

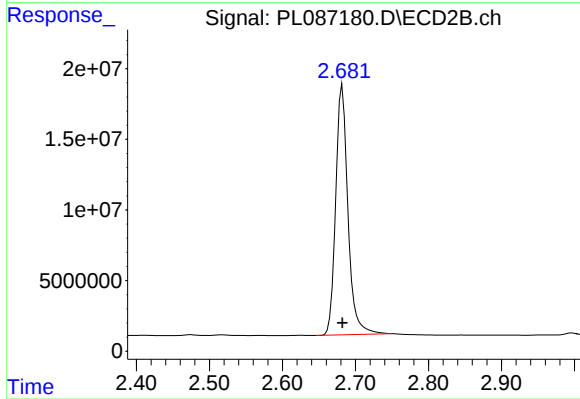


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 206262760
Conc: 101.45 ng/ml

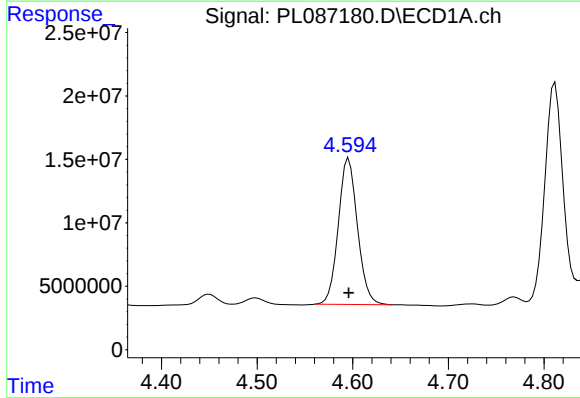


#23 Chlordane-1

R.T.: 4.596 min
Delta R.T.: 0.000 min
Response: 160602519
Conc: 1010.51 ng/ml

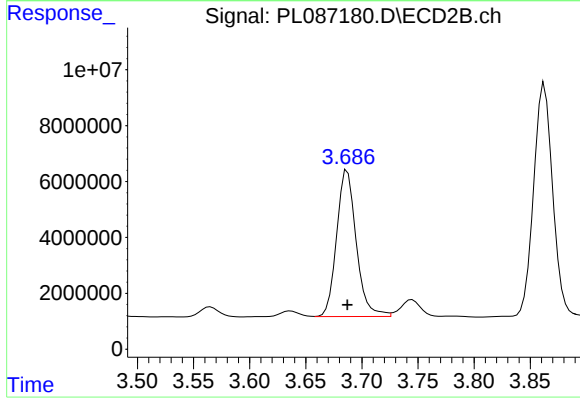

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 63782053
Conc: 1017.10 ng/ml

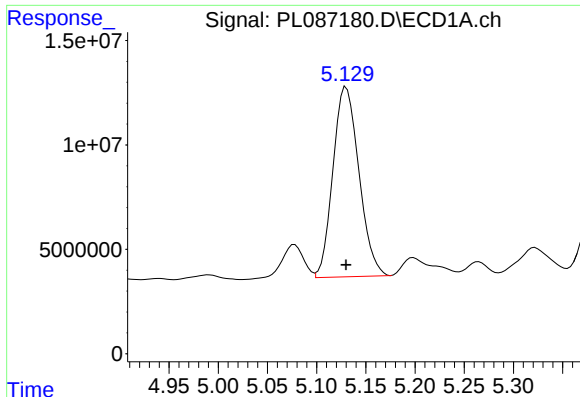

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 167206196
Conc: 989.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

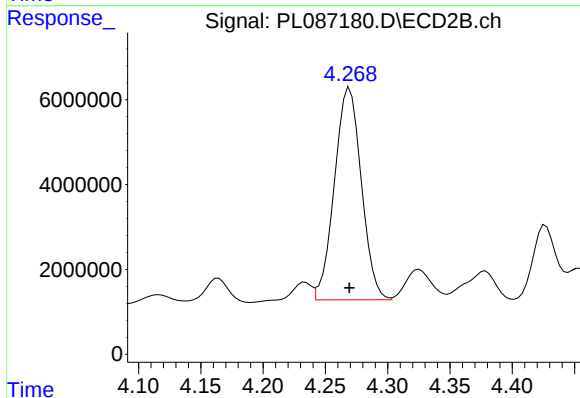


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 75314186
Conc: 992.51 ng/ml

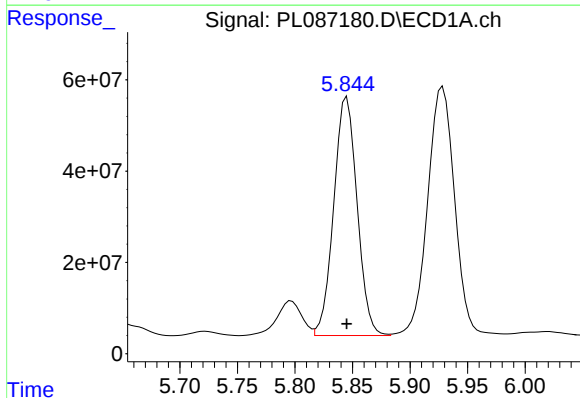


#25 Chlordane-3

R.T.: 5.845 min
Delta R.T.: 0.000 min
Response: 740257843
Conc: 1023.58 ng/ml

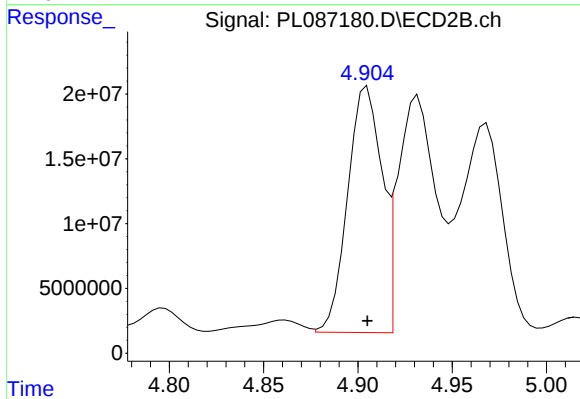

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 239048539
Conc: 1028.24 ng/ml

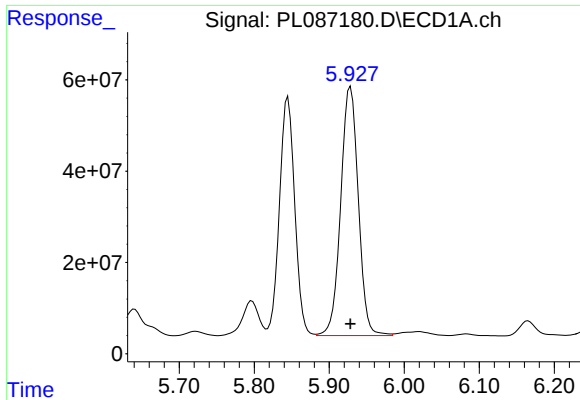

#26 Chlordane-4


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 889404137
Conc: 1016.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

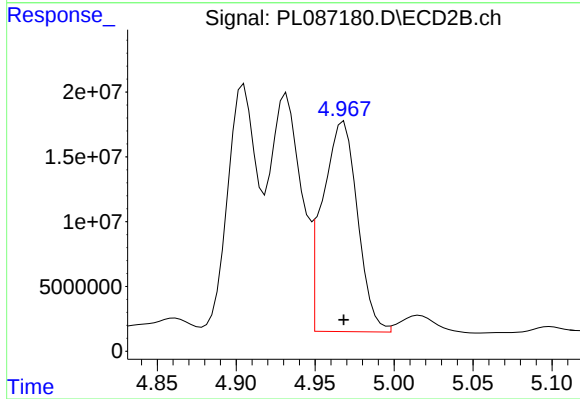


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 248937701
Conc: 1025.15 ng/ml

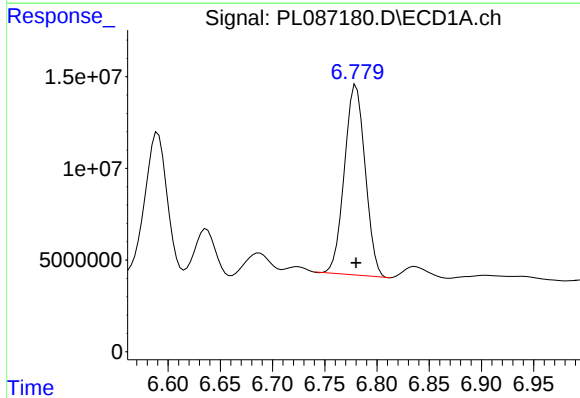


#27 Chlordane-5

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 143407391
Conc: 1016.80 ng/ml

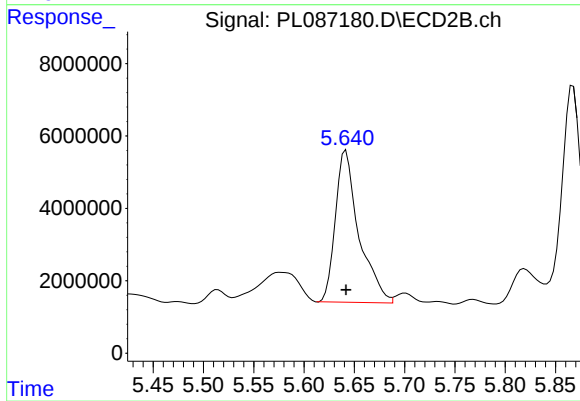

#27 Chlordane-5

R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 68025954
Conc: 1018.41 ng/ml

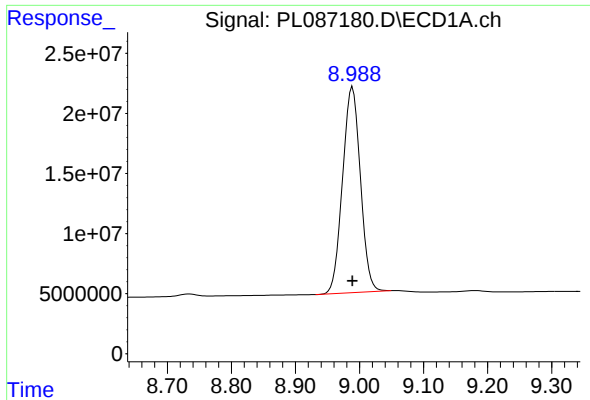

#28 Decachlorobiphenyl


R.T.: 8.989 min

Delta R.T.: 0.000 min

Response: 331403395

Conc: 101.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

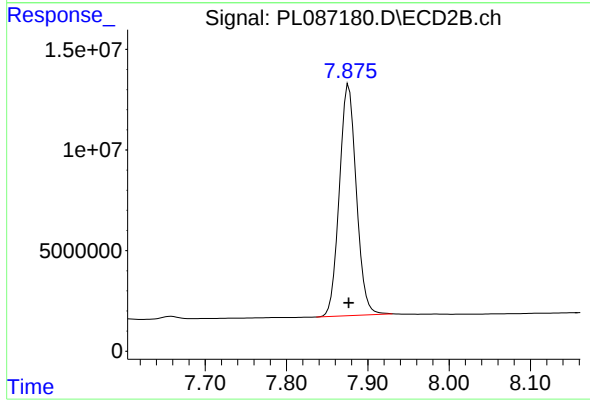

#28 Decachlorobiphenyl

R.T.: 7.877 min

Delta R.T.: 0.000 min

Response: 166574738

Conc: 100.78 ng/ml