

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 01:01
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:59:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:59:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	2.681	87165643	48614818	24.692	24.272
28)	SA Decachlor...	8.989	7.875	78742472	40419919	25.083	25.454
Target Compounds							
23)	Chlordane-1	4.594	3.686	38559683	14994818	246.337	243.746
24)	Chlordane-2	5.129	4.269	43515324	19377444	258.127	256.590
25)	Chlordane-3	5.844	4.905	166.8E6	52747162	238.151	235.048
26)	Chlordane-4	5.927	4.968	206.7E6	55541379	242.549	236.775
27)	Chlordane-5	6.780	5.641	33654783	15837627	245.472	244.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 01:01
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:59:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:59:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

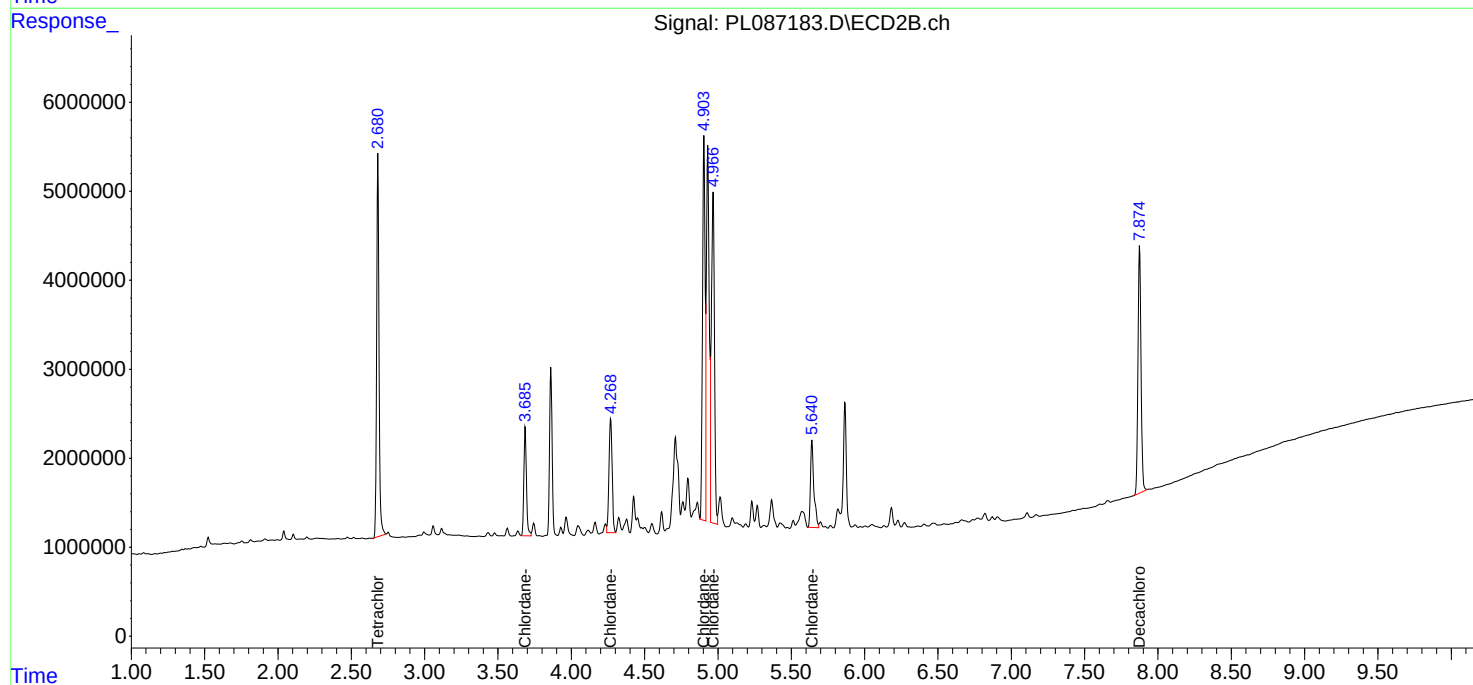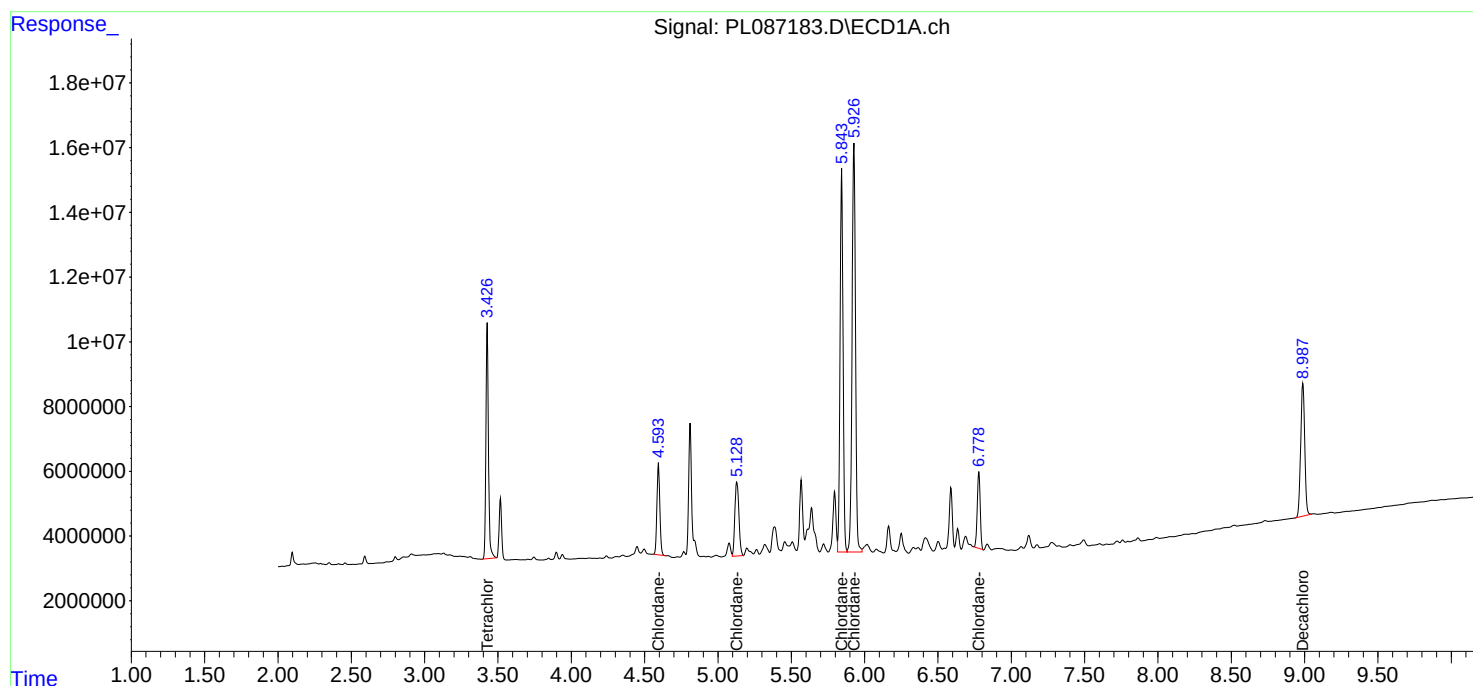


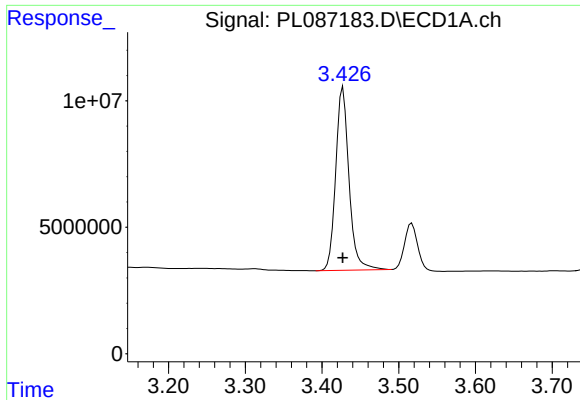

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: 0.000 min
Response: 87165643
Conc: 24.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

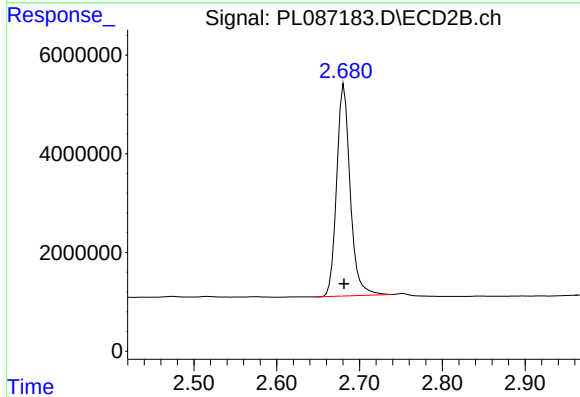


#1 Tetrachloro-m-xylene

R.T.: 2.681 min
Delta R.T.: 0.000 min
Response: 48614818
Conc: 24.27 ng/ml

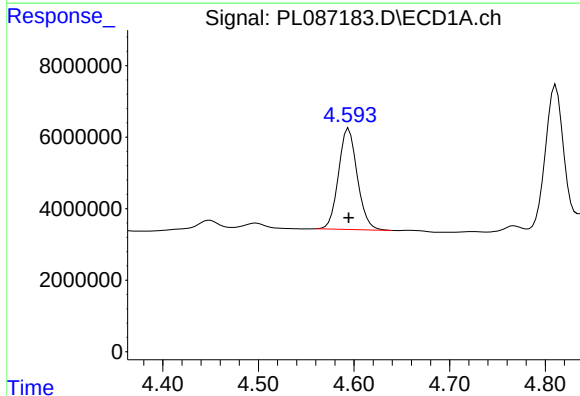


#23 Chlordane-1

R.T.: 4.594 min
Delta R.T.: 0.000 min
Response: 38559683
Conc: 246.34 ng/ml

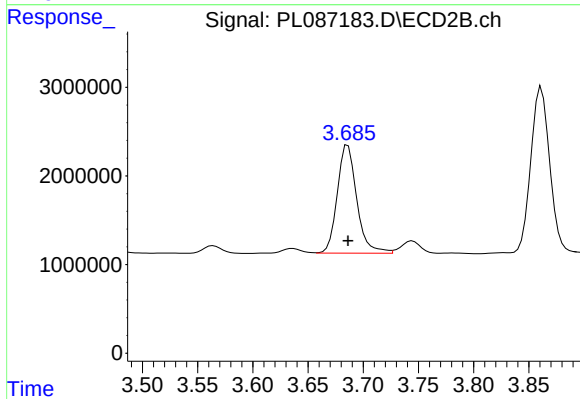

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 14994818
Conc: 243.75 ng/ml

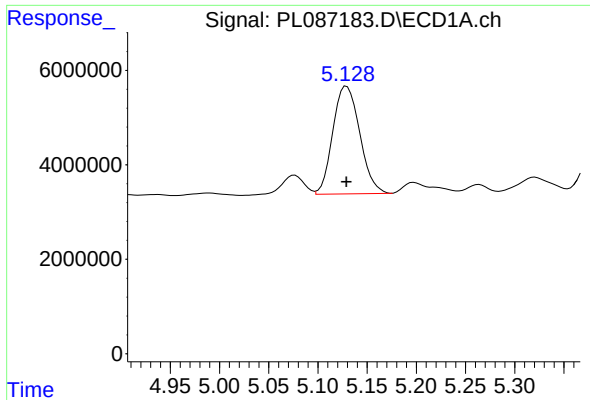

#24 Chlordane-2


R.T.: 5.129 min
Delta R.T.: 0.000 min
Response: 43515324
Conc: 258.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

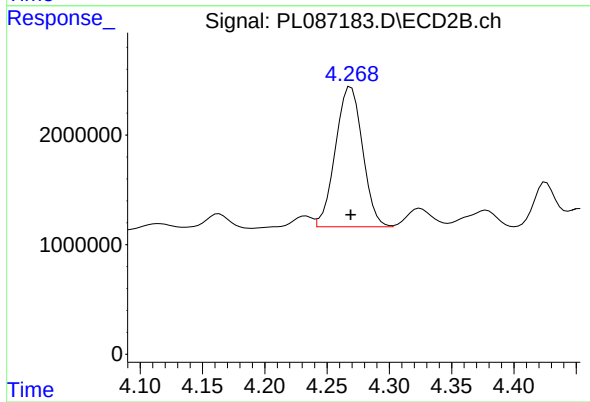


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 19377444
Conc: 256.59 ng/ml

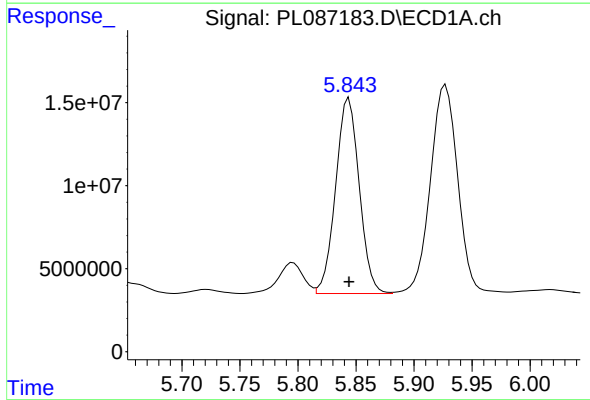


#25 Chlordane-3

R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 166818416
Conc: 238.15 ng/ml

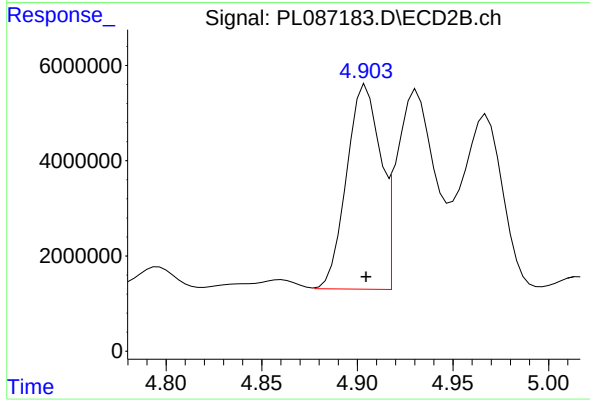

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 52747162
Conc: 235.05 ng/ml

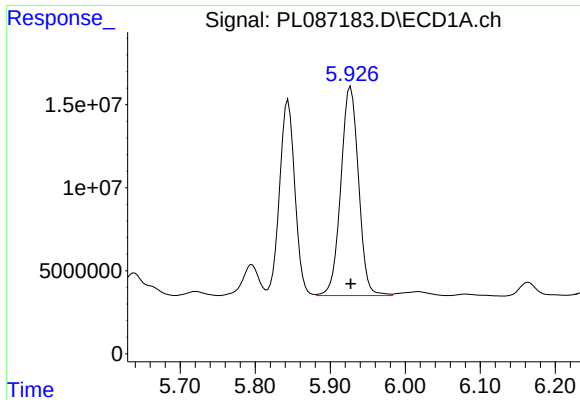

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 206666120
Conc: 242.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

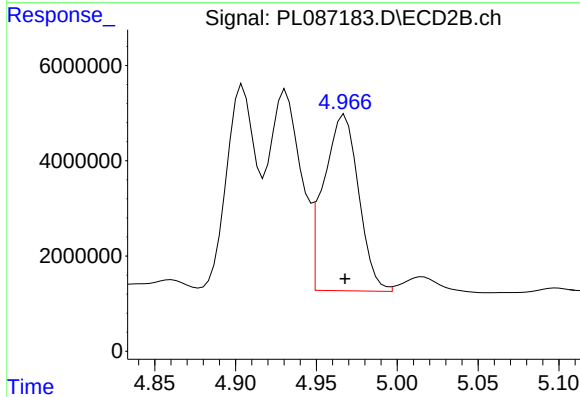


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 55541379
Conc: 236.77 ng/ml

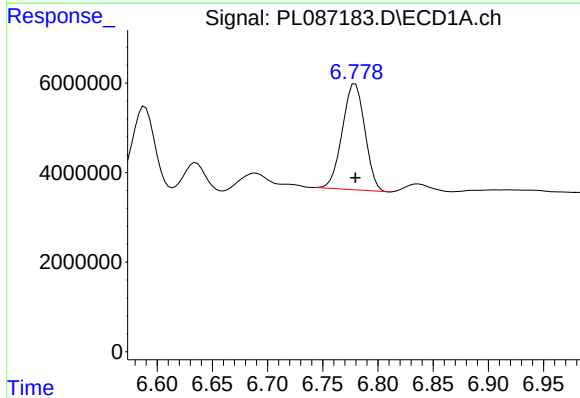


#27 Chlordane-5

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 33654783
Conc: 245.47 ng/ml

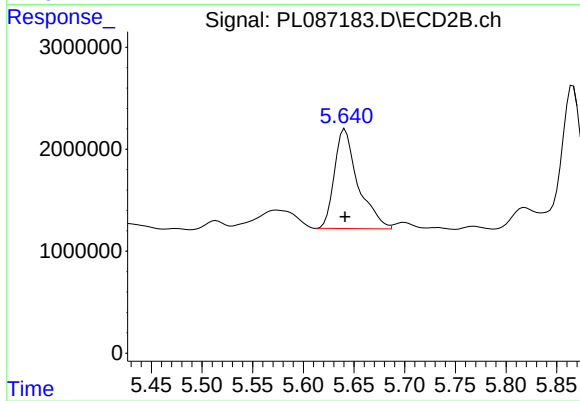

#27 Chlordane-5


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 15837627
Conc: 244.21 ng/ml

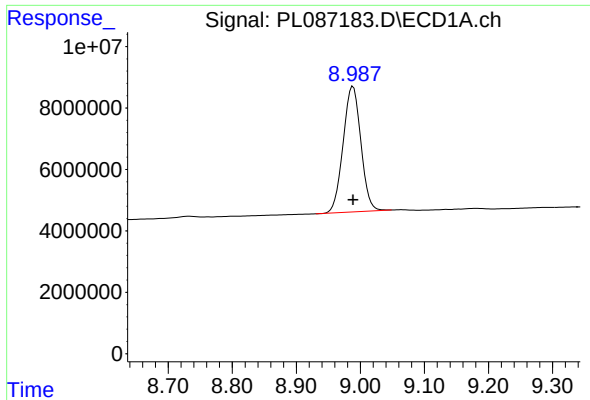

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 78742472
Conc: 25.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

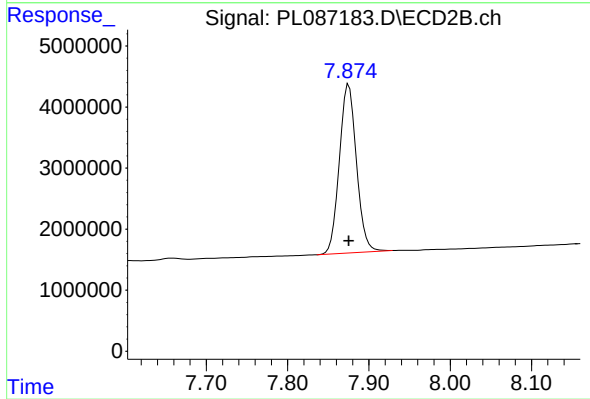

#28 Decachlorobiphenyl

R.T.: 7.875 min
Delta R.T.: 0.000 min
Response: 40419919
Conc: 25.45 ng/ml