

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 01:15
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:00:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:00:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	2.681	18592526	10133682	5.211	5.047
28)	SA Decachlor...	8.986	7.875	16977181	9183488	5.321	5.607
Target Compounds							
23)	Chlordane-1	4.594	3.686	8139443	3204973	51.586	51.664
24)	Chlordane-2	5.128	4.269	9831023	4089289	56.439	53.265
25)	Chlordane-3	5.843	4.904	34168582	10384729	49.019	46.975
26)	Chlordane-4	5.927	4.967	43355646	11289334	50.704	48.490
27)	Chlordane-5	6.779	5.641	7108241	3203913	51.466	49.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 01:15
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:00:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:00:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

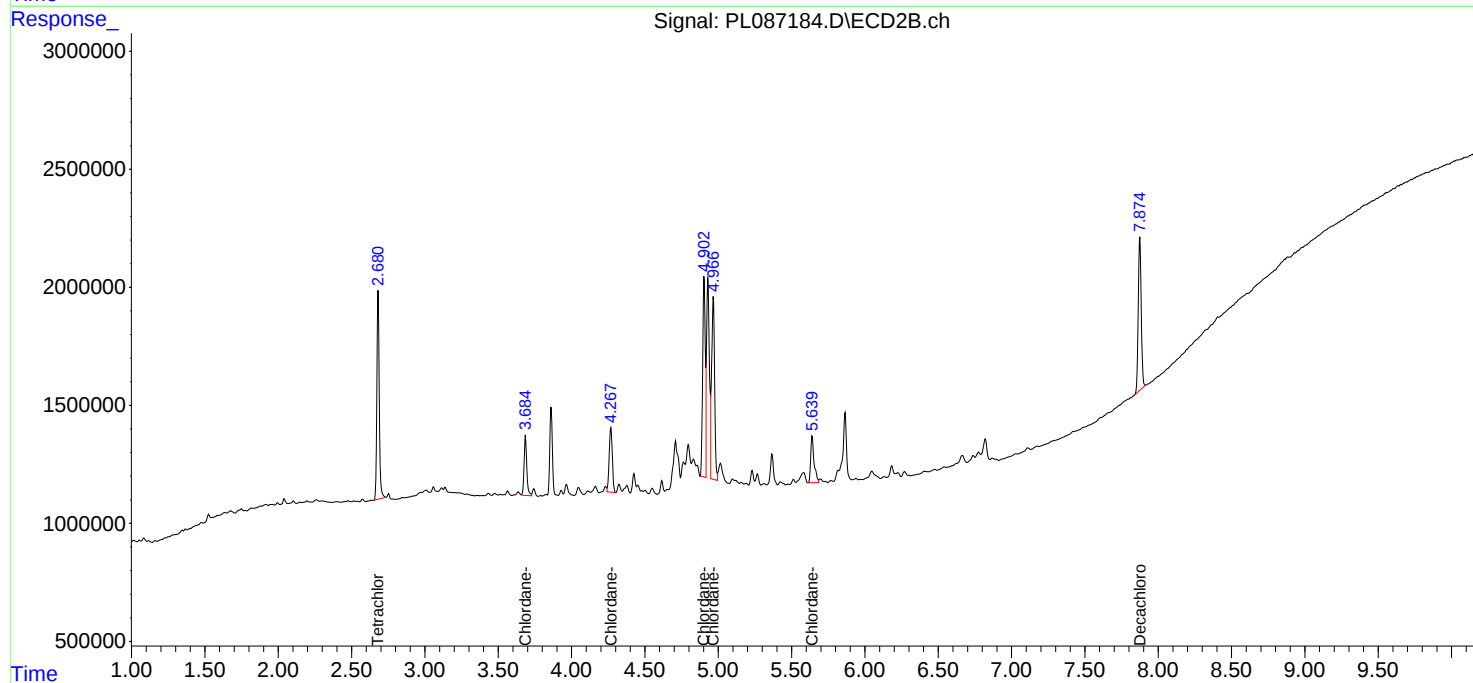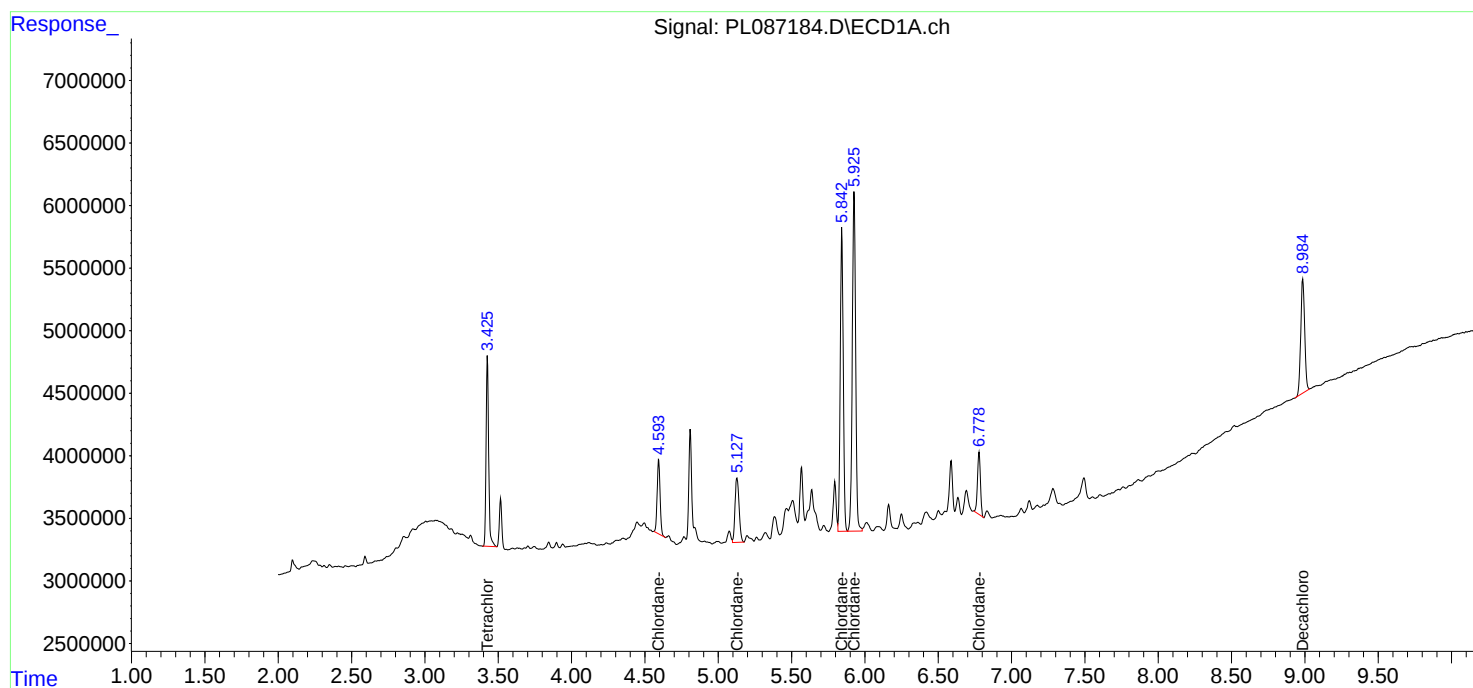


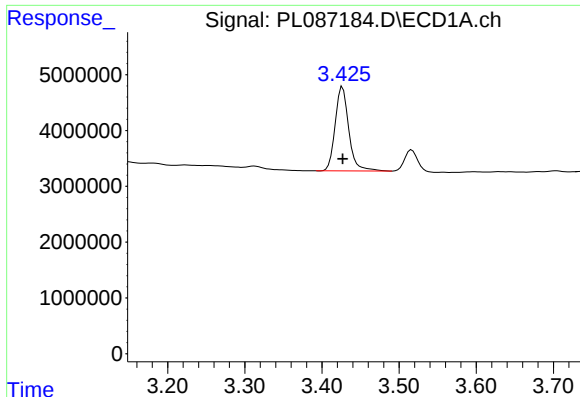

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: 0.000 min
Response: 18592526
Conc: 5.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

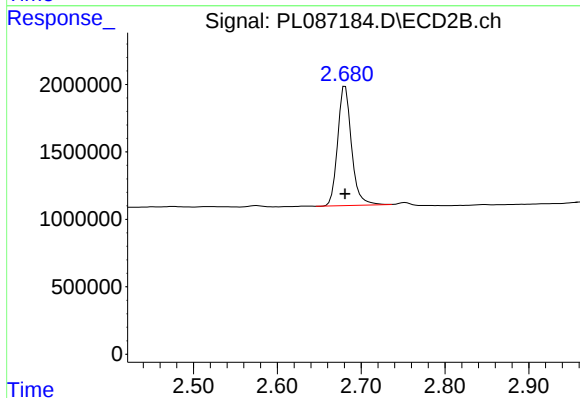


#1 Tetrachloro-m-xylene

R.T.: 2.681 min
Delta R.T.: 0.000 min
Response: 10133682
Conc: 5.05 ng/ml

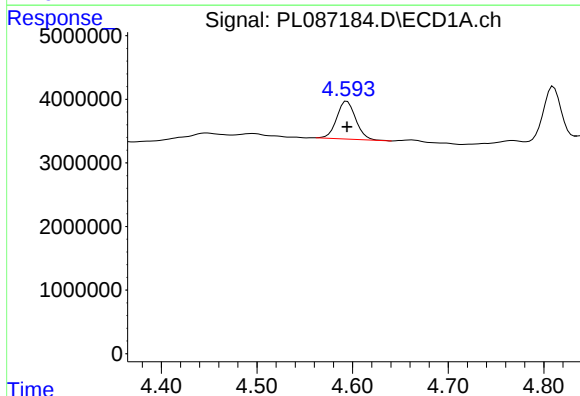


#23 Chlordane-1

R.T.: 4.594 min
Delta R.T.: 0.000 min
Response: 8139443
Conc: 51.59 ng/ml

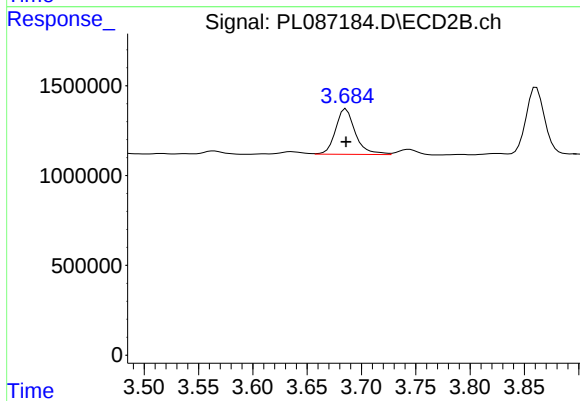

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 3204973
Conc: 51.66 ng/ml

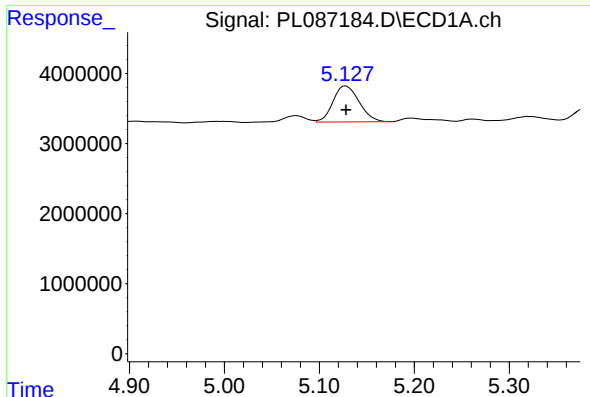

#24 Chlordane-2


R.T.: 5.128 min
Delta R.T.: 0.000 min
Response: 9831023
Conc: 56.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

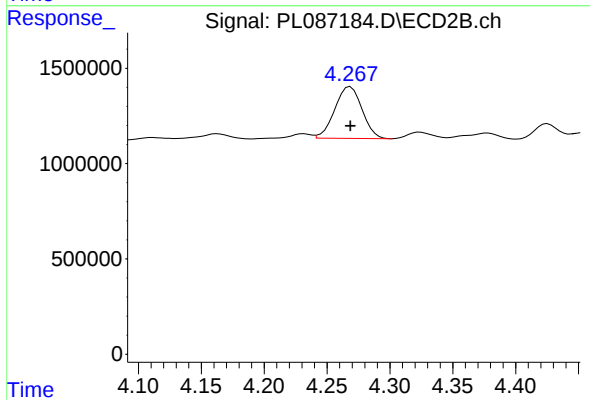


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 4089289
Conc: 53.27 ng/ml

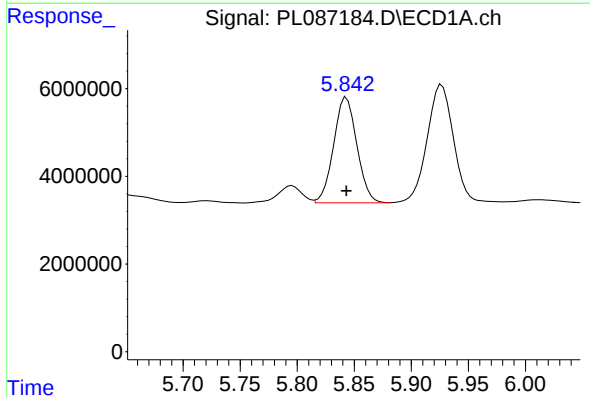


#25 Chlordane-3

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 34168582
Conc: 49.02 ng/ml

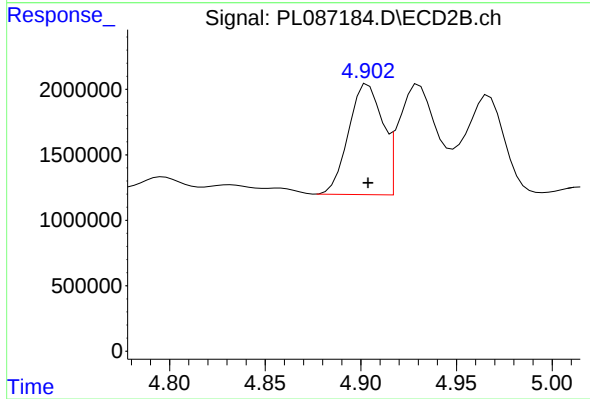

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 10384729
Conc: 46.98 ng/ml

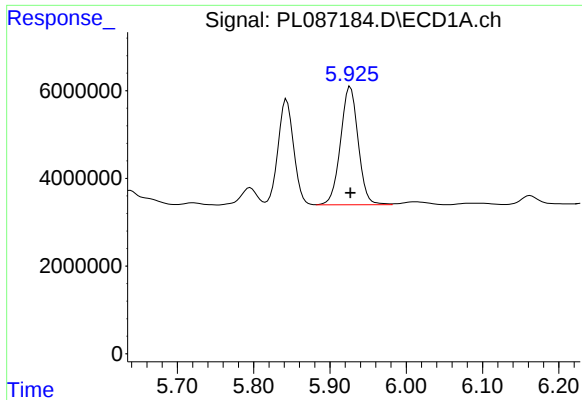

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 43355646
Conc: 50.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

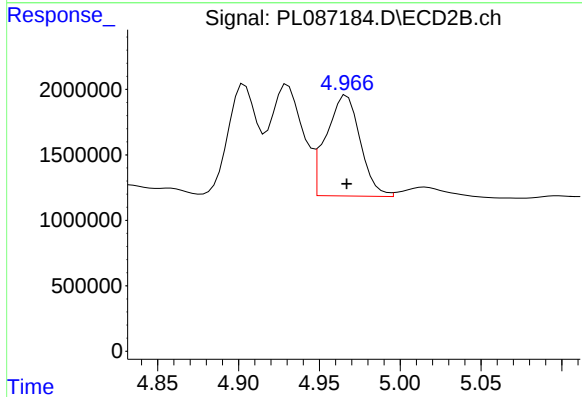


#26 Chlordane-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 11289334
Conc: 48.49 ng/ml

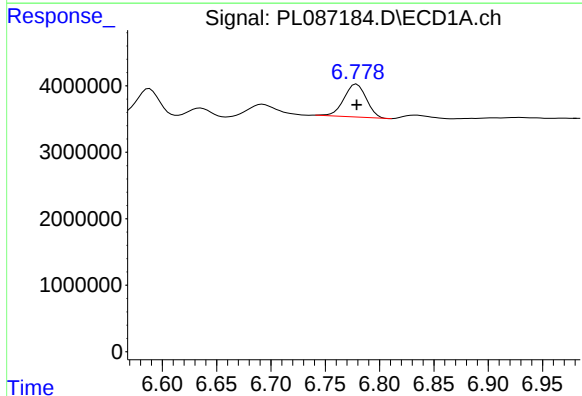


#27 Chlordane-5

R.T.: 6.779 min
Delta R.T.: 0.000 min
Response: 7108241
Conc: 51.47 ng/ml

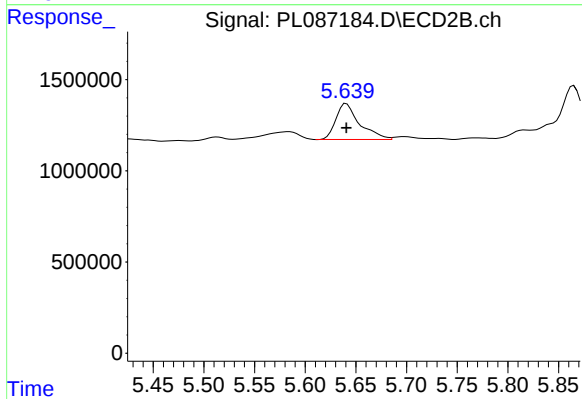

#27 Chlordane-5


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 3203913
Conc: 49.52 ng/ml

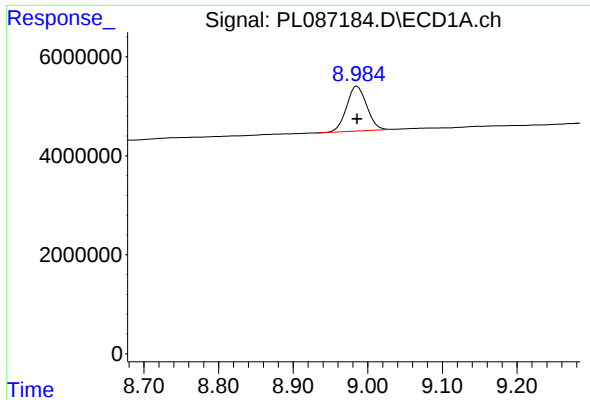

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 16977181
Conc: 5.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

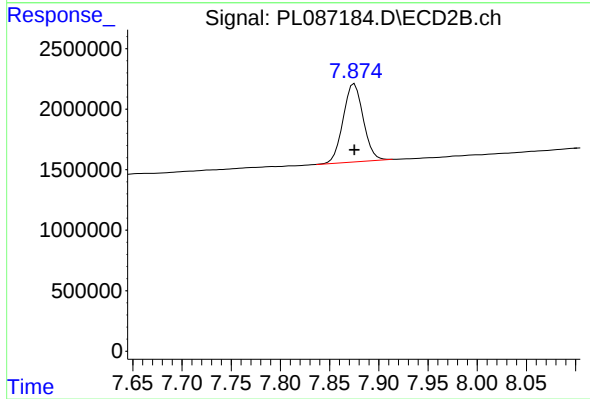

#28 Decachlorobiphenyl

R.T.: 7.875 min
Delta R.T.: 0.000 min
Response: 9183488
Conc: 5.61 ng/ml