

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
 Data File : PL087191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 02:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL121523CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:52:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:49:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	2.681	186.6E6	104.4E6	52.884	52.117
28)	SA Decachlor...	8.987	7.874	172.5E6	88294863	53.219	53.836
Target Compounds							
23)	Chlordane-1	4.594	3.686	83466103	32209325	530.746	522.564
24)	Chlordane-2	5.129	4.268	90966231	40220926	532.303	526.106
25)	Chlordane-3	5.844	4.904	377.4E6	119.4E6	534.502	528.664
26)	Chlordane-4	5.927	4.967	459.9E6	125.5E6	533.996	529.973
27)	Chlordane-5	6.780	5.641	74247545	34678249	535.433	528.903



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121523\
Data File : PL087191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 02:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL121523CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:52:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:49:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

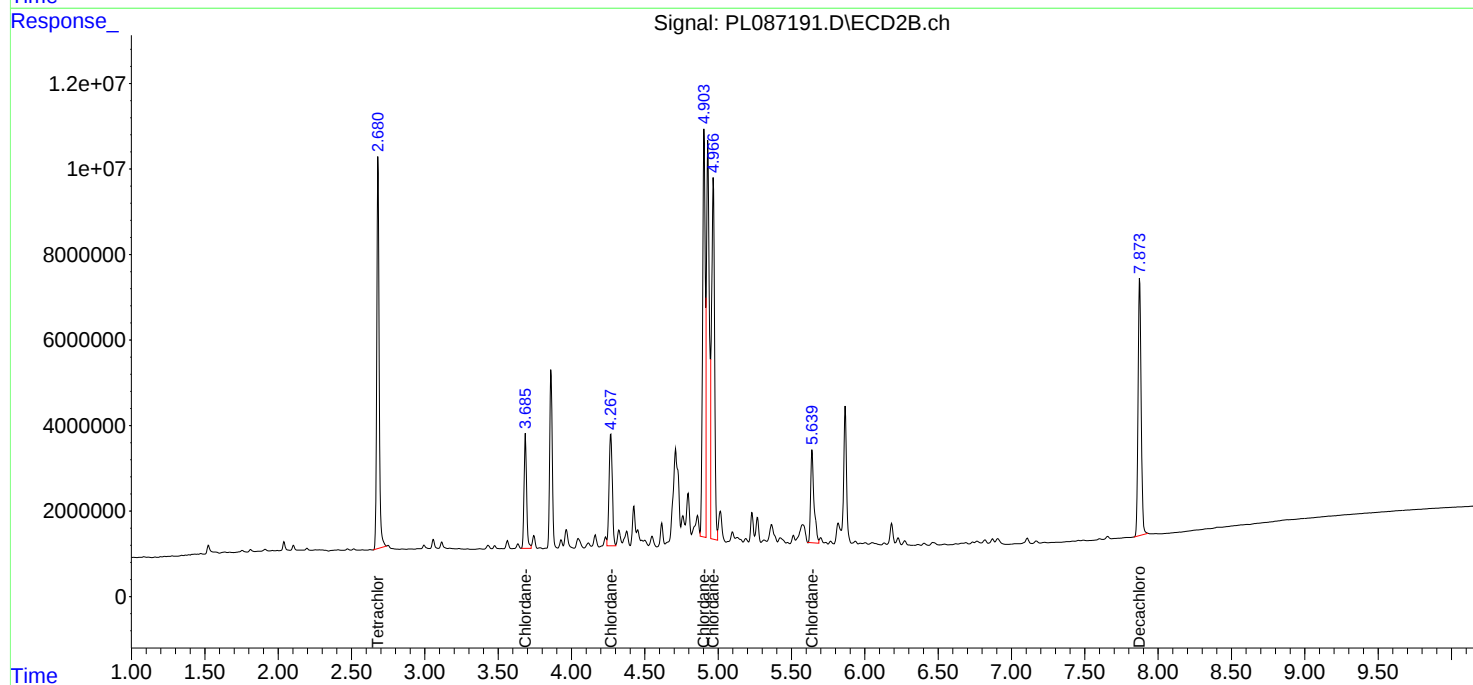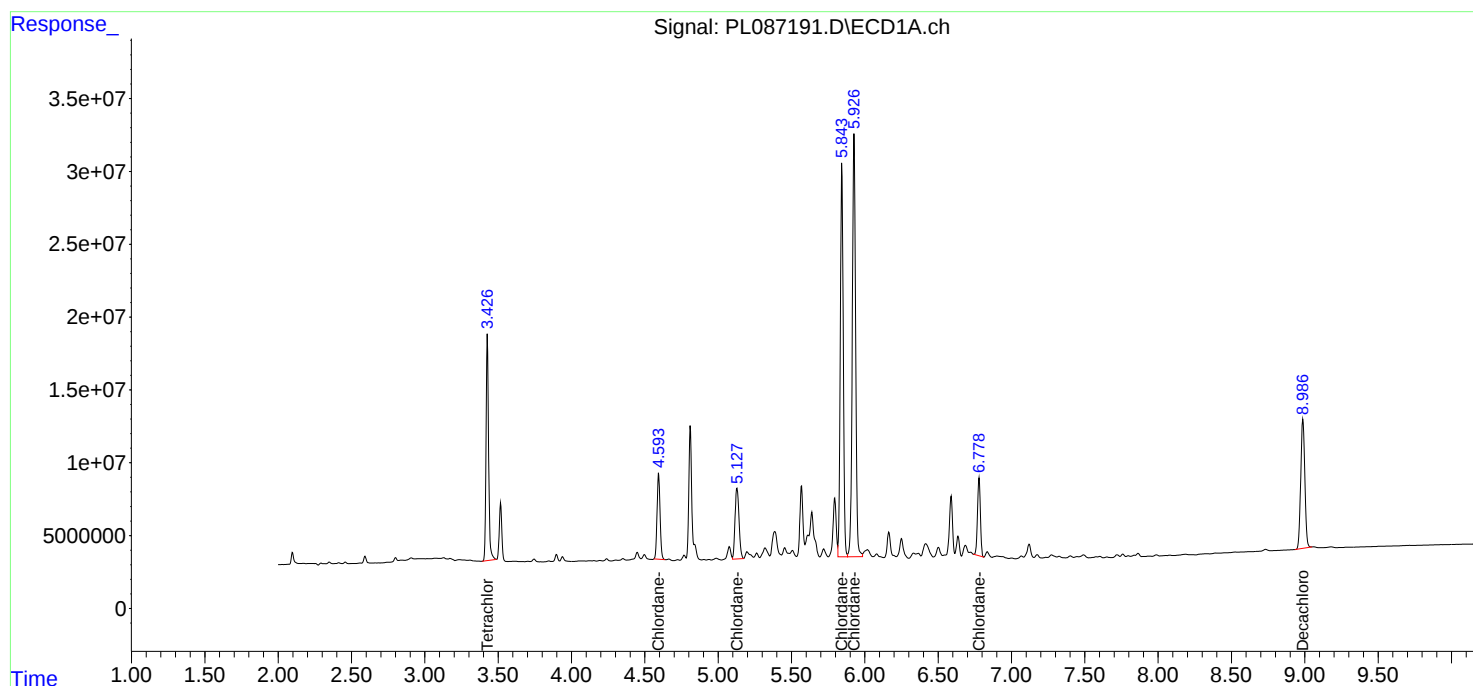


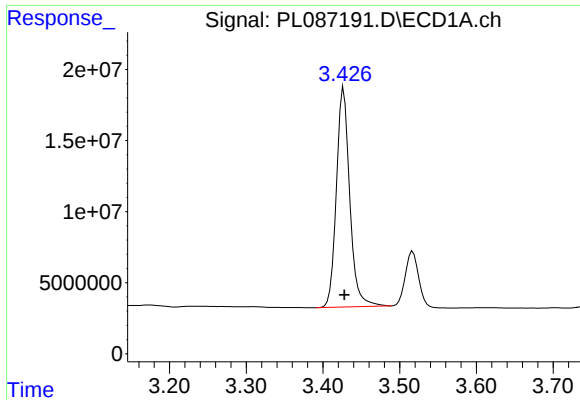

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: -0.001 min
Response: 186605436
Conc: 52.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121523CHLOR

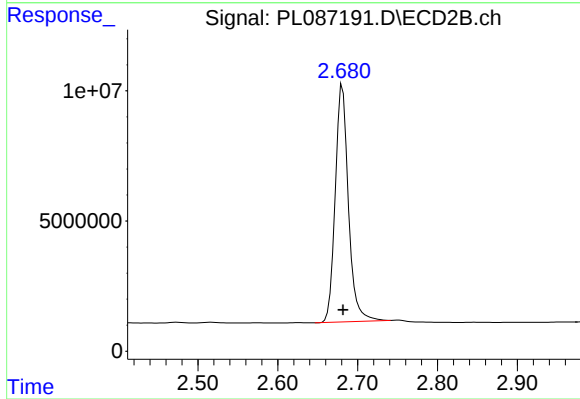


#1 Tetrachloro-m-xylene

R.T.: 2.681 min
Delta R.T.: 0.000 min
Response: 104435573
Conc: 52.12 ng/ml

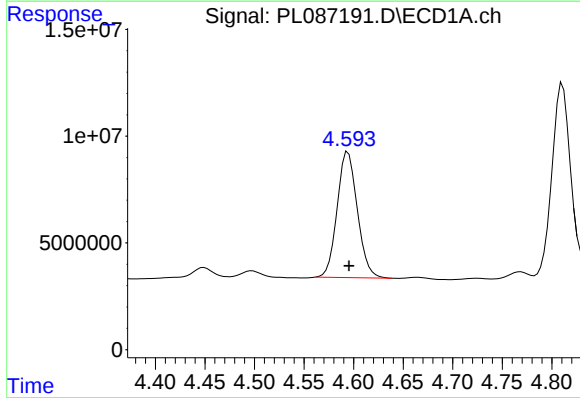


#23 Chlordane-1

R.T.: 4.594 min
Delta R.T.: -0.001 min
Response: 83466103
Conc: 530.75 ng/ml

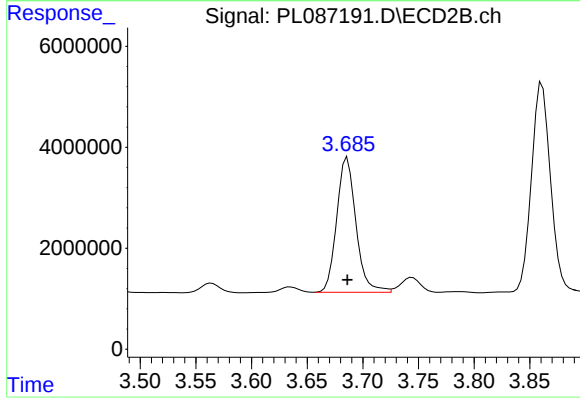

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 32209325
Conc: 522.56 ng/ml

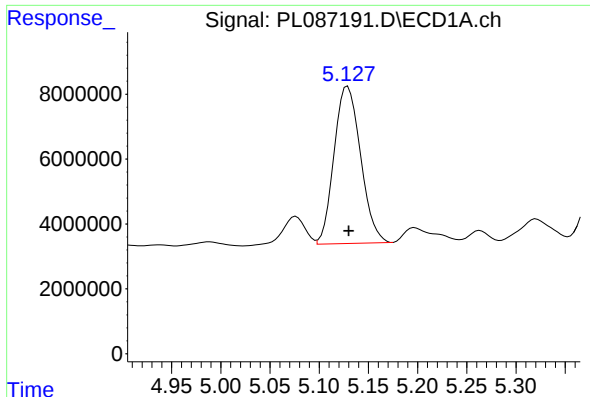

#24 Chlordane-2


R.T.: 5.129 min
Delta R.T.: -0.001 min
Response: 90966231
Conc: 532.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121523CHLOR

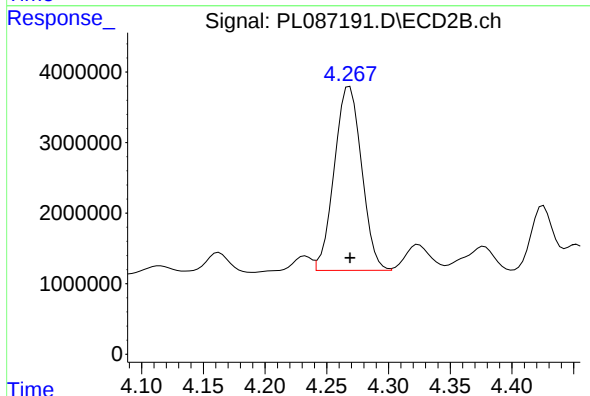


#24 Chlordane-2

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 40220926
Conc: 526.11 ng/ml

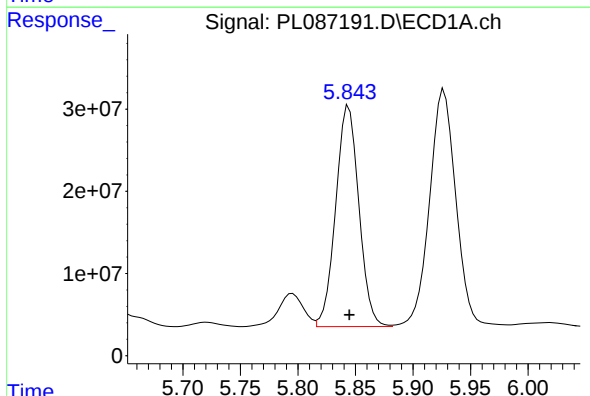


#25 Chlordane-3

R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 377442560
Conc: 534.50 ng/ml

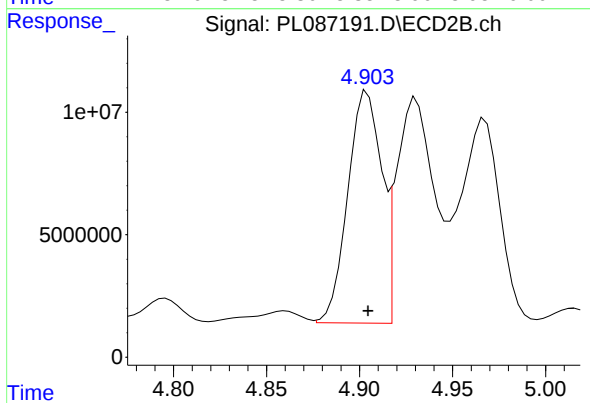

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 119433491
Conc: 528.66 ng/ml

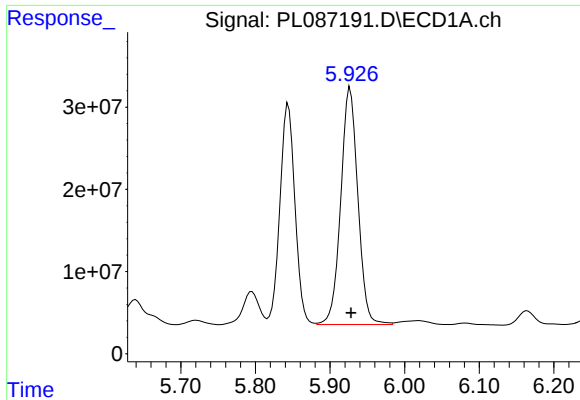

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: -0.001 min
Response: 459853854
Conc: 534.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121523CHLOR

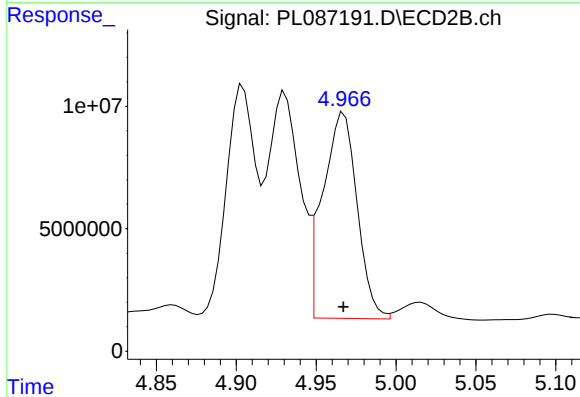


#26 Chlordane-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 125457600
Conc: 529.97 ng/ml

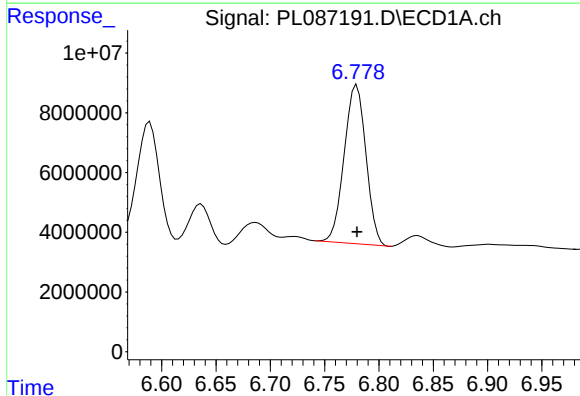


#27 Chlordane-5

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 74247545
Conc: 535.43 ng/ml

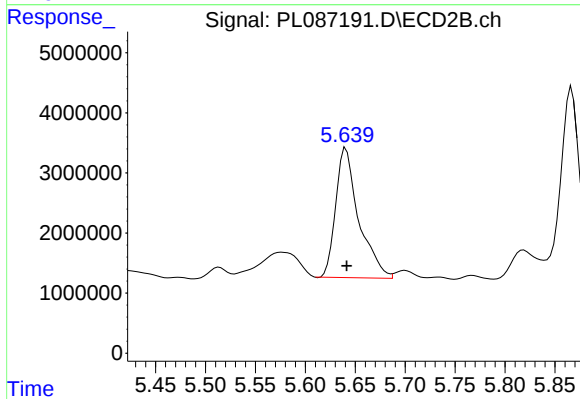

#27 Chlordane-5


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 34678249
Conc: 528.90 ng/ml

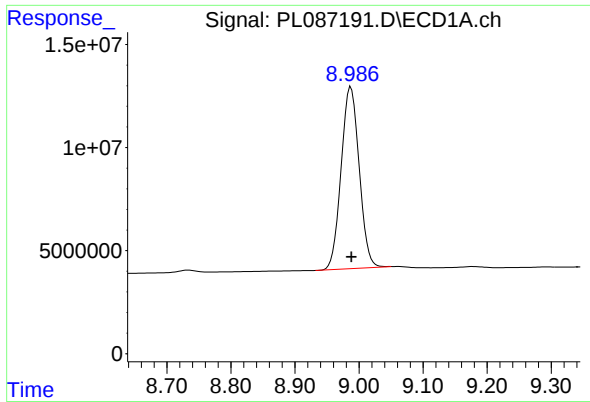

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: 0.000 min
Response: 172530070
Conc: 53.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121523CHLOR

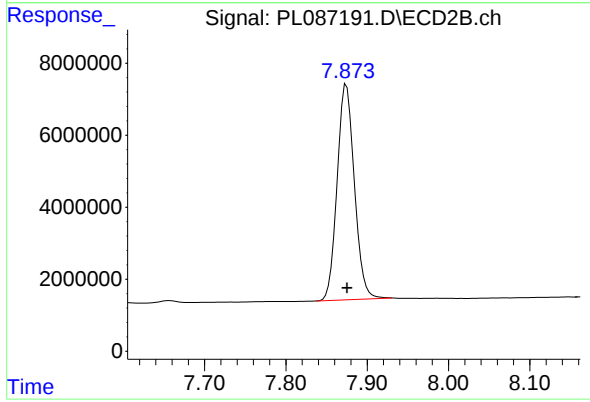

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: 0.000 min
Response: 88294863
Conc: 53.84 ng/ml