

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121525\
 Data File : PL097864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2025 19:36
 Operator : AR\AJ
 Sample : Q3859-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-121225

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:03:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	2.799	54619974	82833772	10.822	11.858
28)	SA Decachlor...	8.952	7.946	45737307	55895932	12.038	8.500 #
Target Compounds							
10)	B gamma-Chl...	5.871	0.000	6188755	0	0.953	N.D. #
11)	B alpha-Chl...	5.955	5.074	12972959	13953326	1.998	1.361 #
23)	Chlordane-1	0.000	3.801	0	5802076	N.D.	21.925 #
25)	Chlordane-3	5.871	0.000	6188755	0	7.014	N.D. #
26)	Chlordane-4	5.955	5.074	12972959	13953326	12.251	17.284 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121525\
Data File : PL097864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2025 19:36
Operator : AR\AJ
Sample : Q3859-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-02-121225

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:03:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

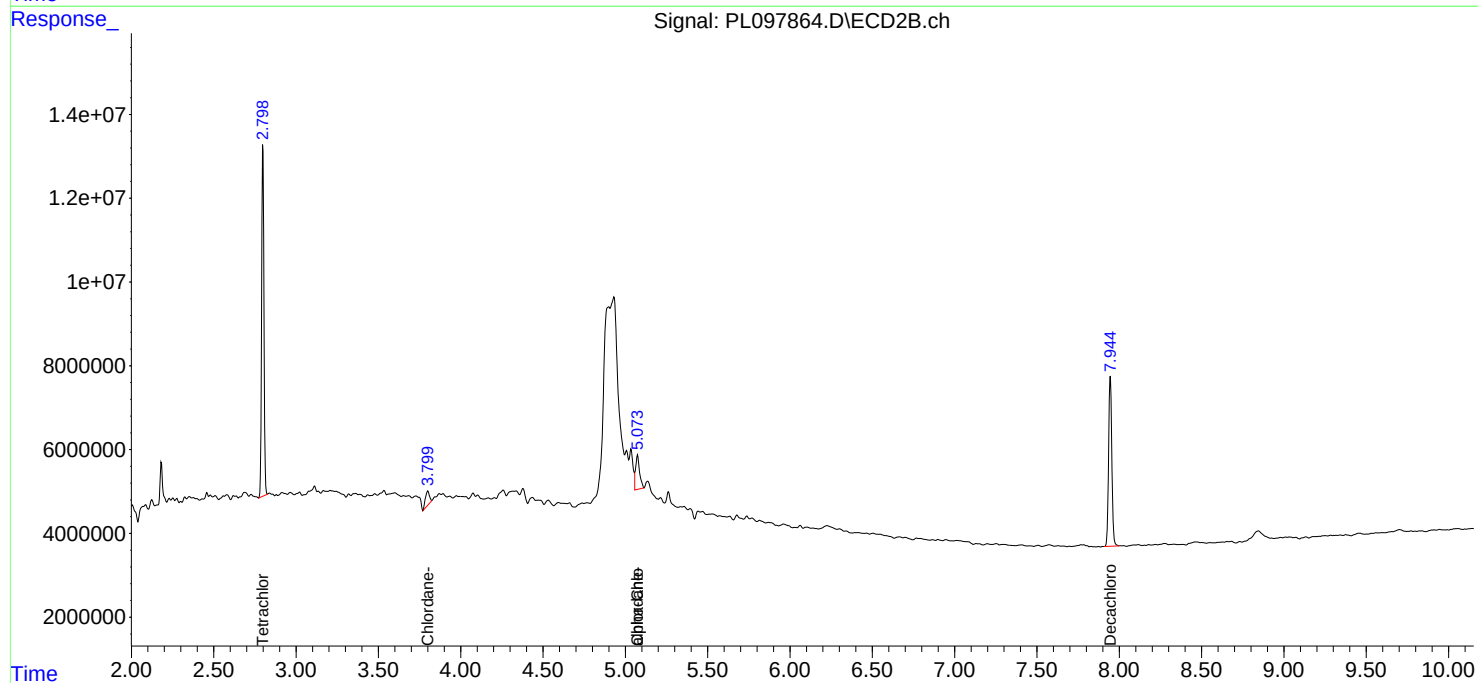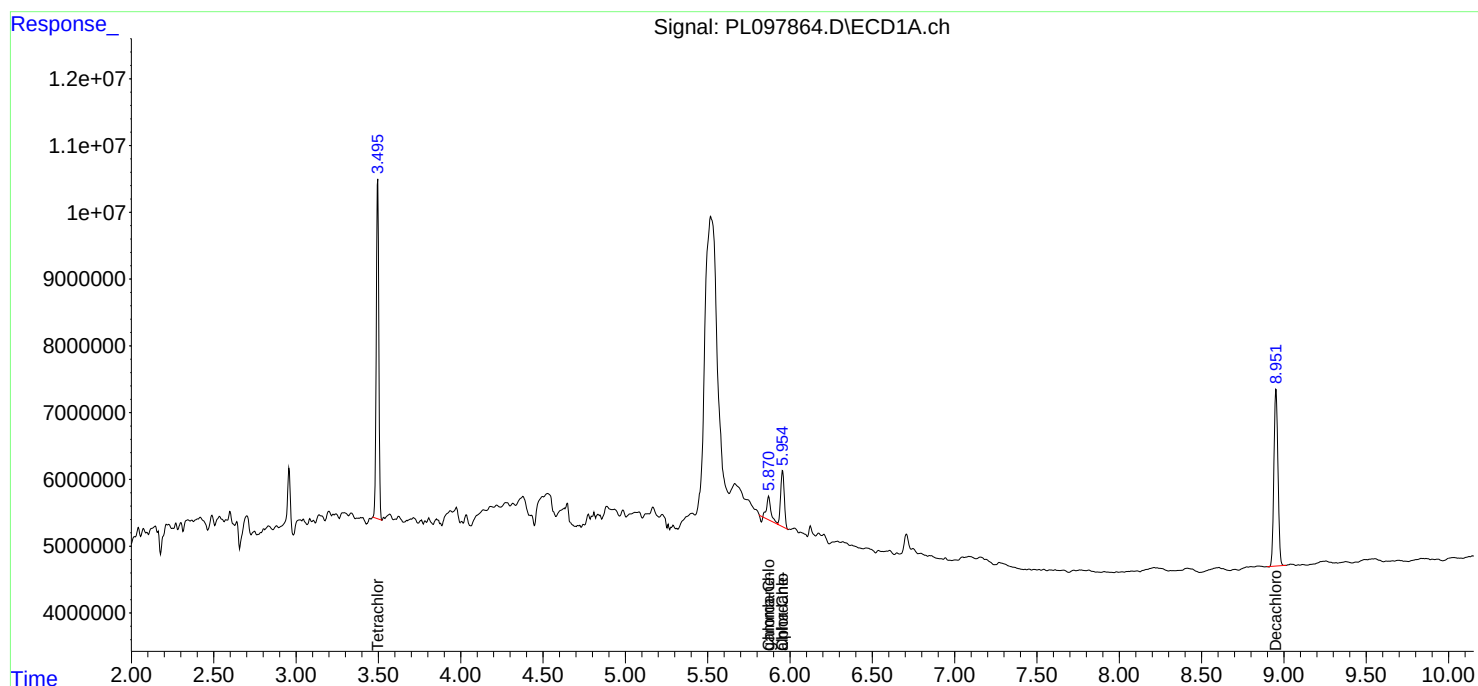


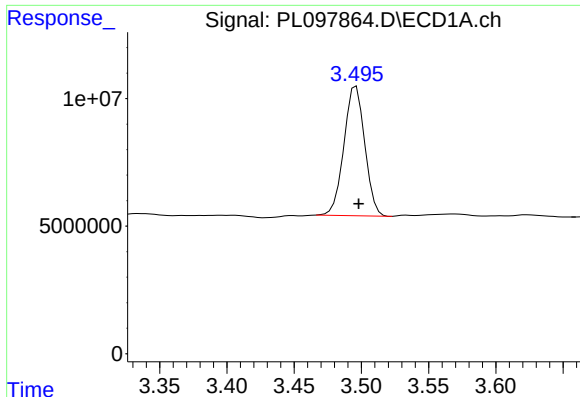

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: -0.002 min
Response: 54619974
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-121225

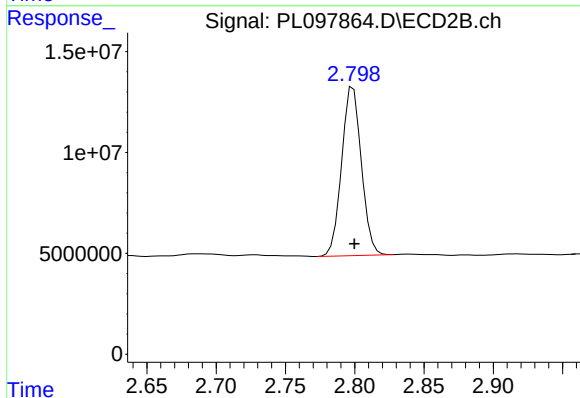


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: 0.000 min
Response: 82833772
Conc: 11.86 ng/ml

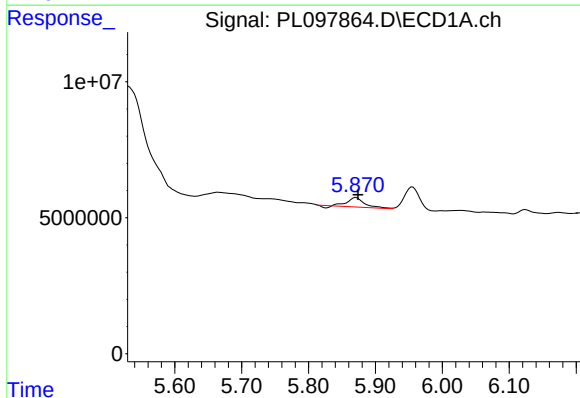


#10 gamma-Chlordane

R.T.: 5.871 min
Delta R.T.: -0.003 min
Response: 6188755
Conc: 0.95 ng/ml

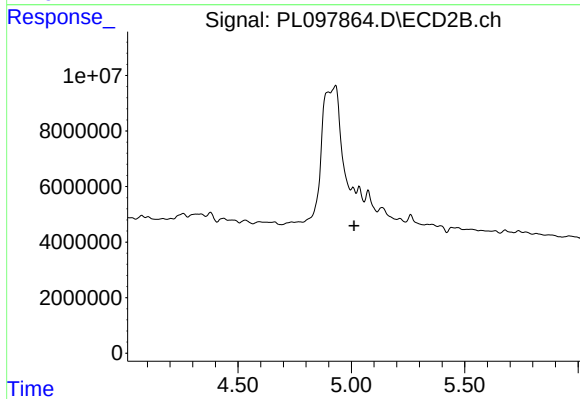

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

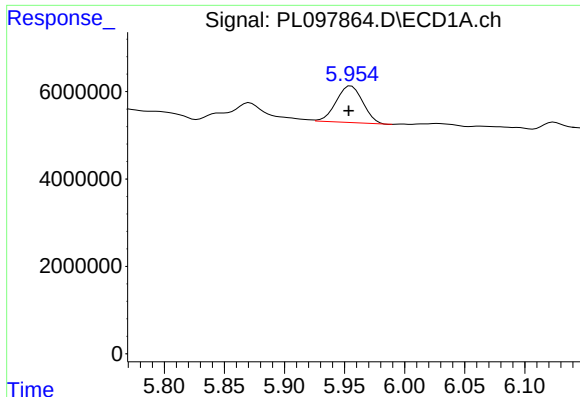

#11 alpha-Chlordane


R.T.: 5.955 min
Delta R.T.: 0.002 min
Response: 12972959
Conc: 2.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-121225

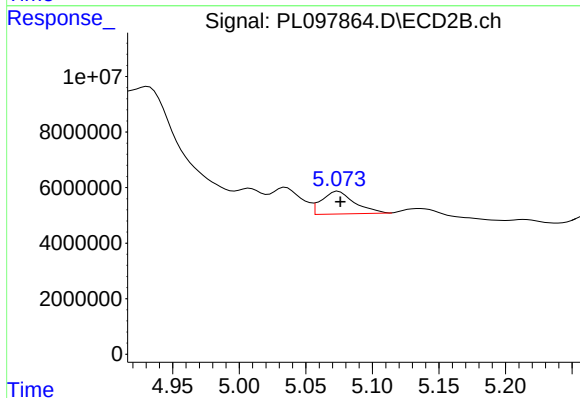


#11 alpha-Chlordane

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 13953326
Conc: 1.36 ng/ml

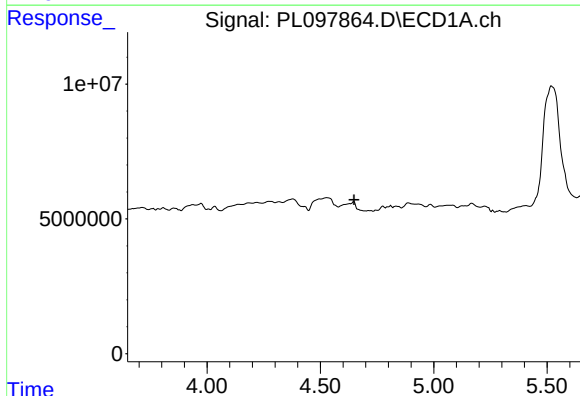


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

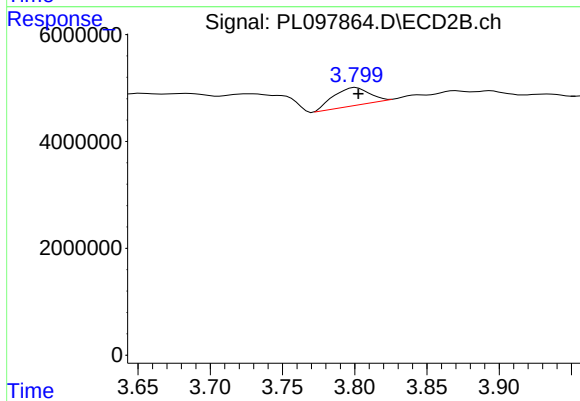

#23 Chlordane-1


R.T.: 3.801 min
Delta R.T.: -0.002 min
Response: 5802076
Conc: 21.93 ng/ml

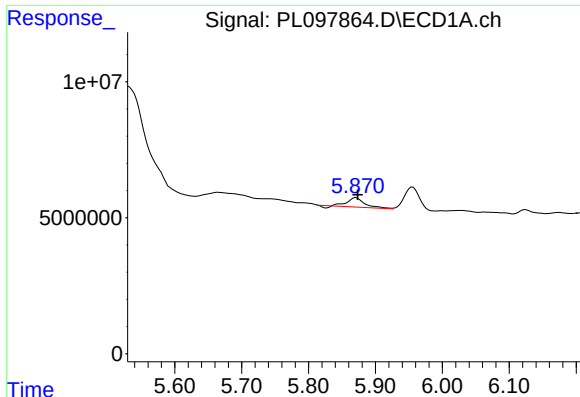

#25 Chlordane-3


R.T.: 5.871 min
Delta R.T.: -0.003 min
Response: 6188755
Conc: 7.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-121225

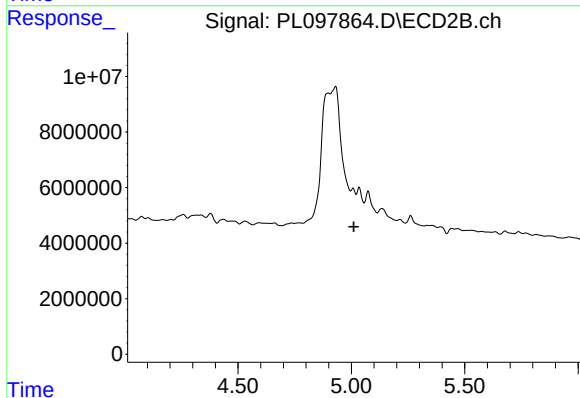


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.011 min
Response: 0
Conc: N.D.

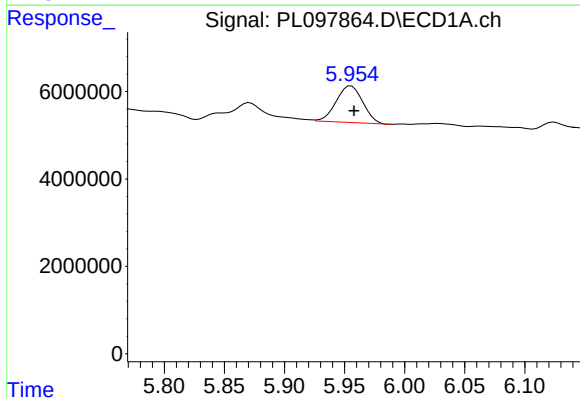


#26 Chlordane-4

R.T.: 5.955 min
Delta R.T.: -0.003 min
Response: 12972959
Conc: 12.25 ng/ml

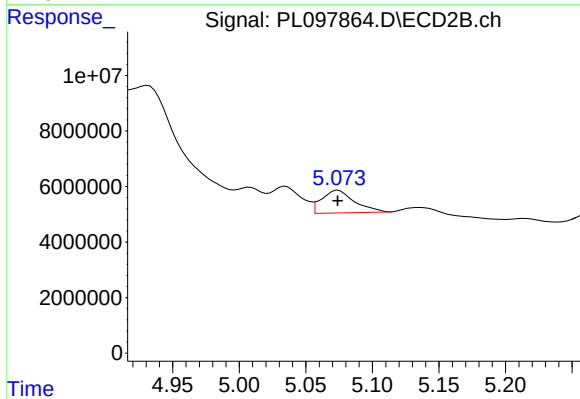

#26 Chlordane-4


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 13953326
Conc: 17.28 ng/ml

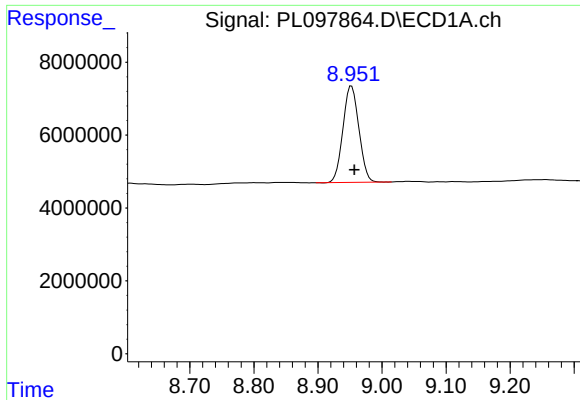

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.004 min
Response: 45737307
Conc: 12.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-121225

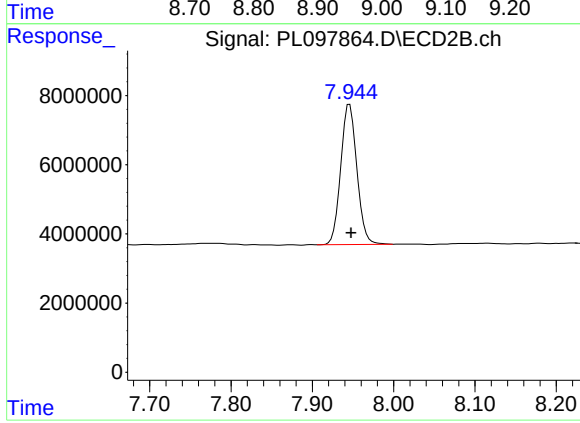

#28 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: -0.002 min
Response: 55895932
Conc: 8.50 ng/ml