

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121525\
 Data File : PL097852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2025 11:13
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:02:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	2.797	231.6E6	373.1E6	45.892	53.415
28)	SA Decachlor...	8.956	7.947	171.4E6	295.2E6	45.105	44.895
Target Compounds							
23)	Chlordane-1	4.648	3.802	112.8E6	128.7E6	480.044	486.452
24)	Chlordane-2	5.172	4.379	121.4E6	144.5E6	502.503	470.225
25)	Chlordane-3	5.875	5.010	433.9E6	422.6E6	491.698	483.989
26)	Chlordane-4	5.958	5.074	514.7E6	385.2E6	486.101	477.120
27)	Chlordane-5	6.795	5.966	88009154	155.5E6	483.924	472.706



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121525\
Data File : PL097852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2025 11:13
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:02:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

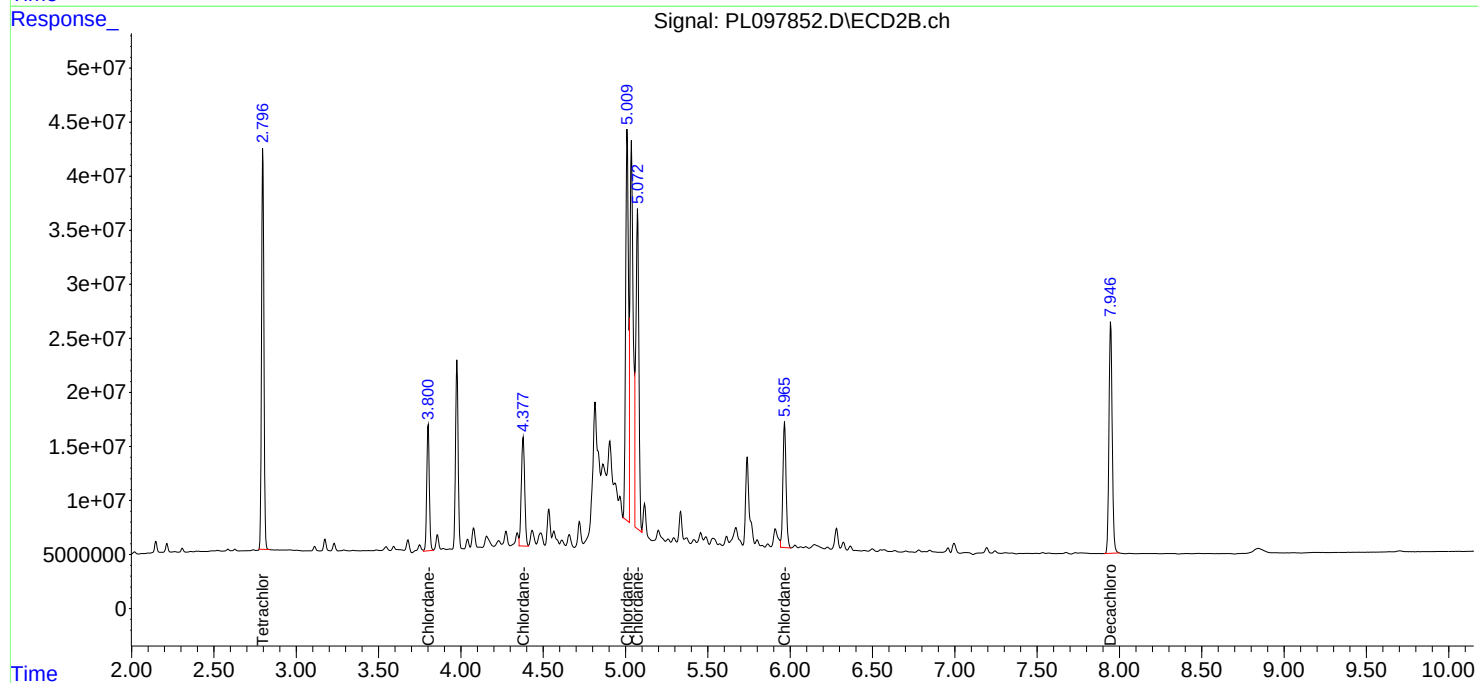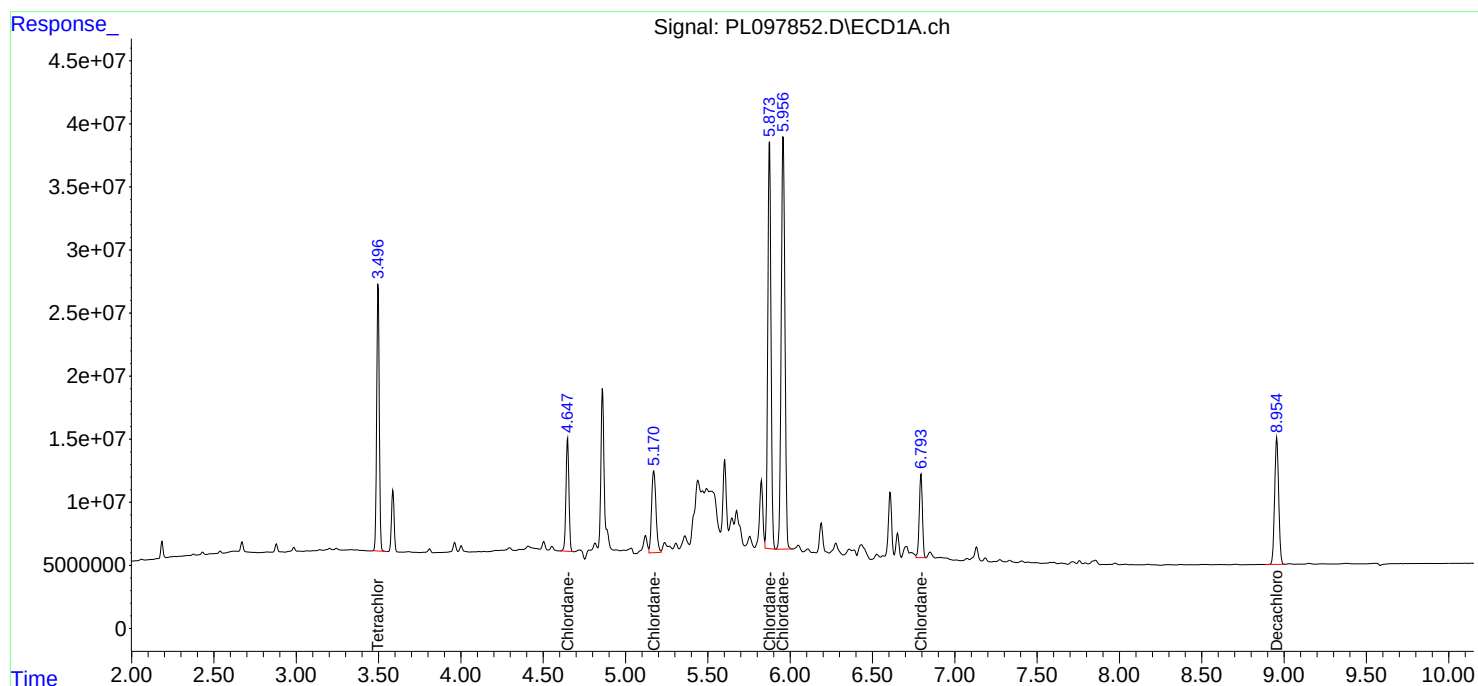


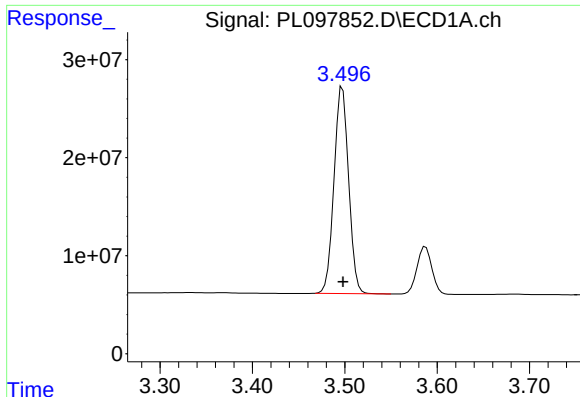

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 231614377
Conc: 45.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

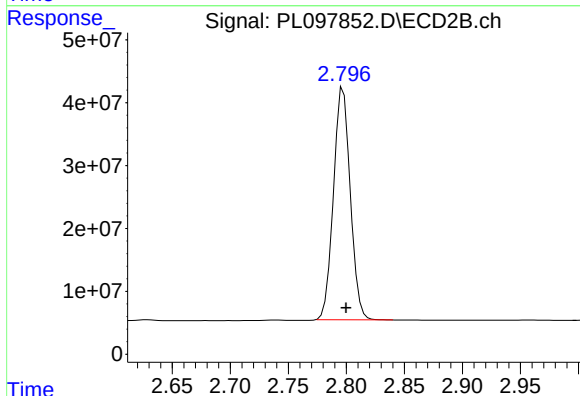


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: -0.002 min
Response: 373112993
Conc: 53.41 ng/ml

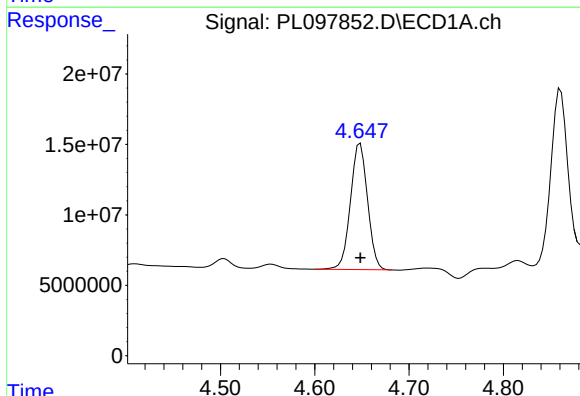


#23 Chlordane-1

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 112784008
Conc: 480.04 ng/ml

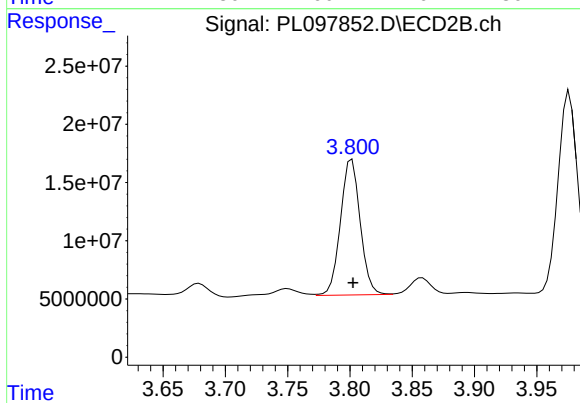

#23 Chlordane-1


R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 128729242
Conc: 486.45 ng/ml

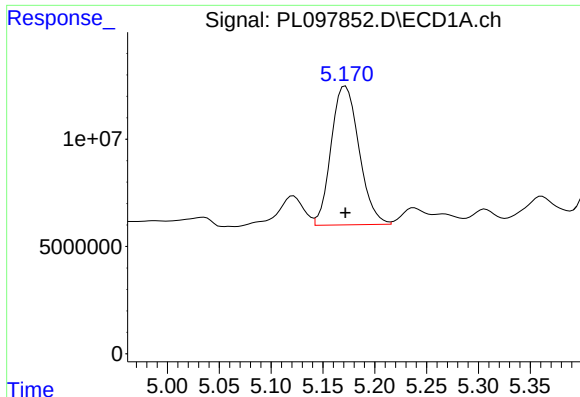

#24 Chlordane-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 121400533
Conc: 502.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

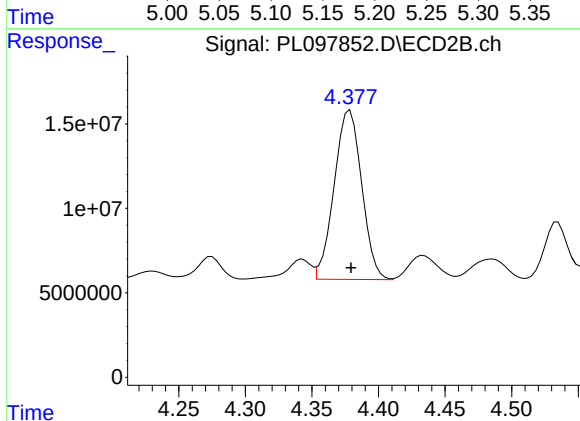


#24 Chlordane-2

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 144537119
Conc: 470.22 ng/ml

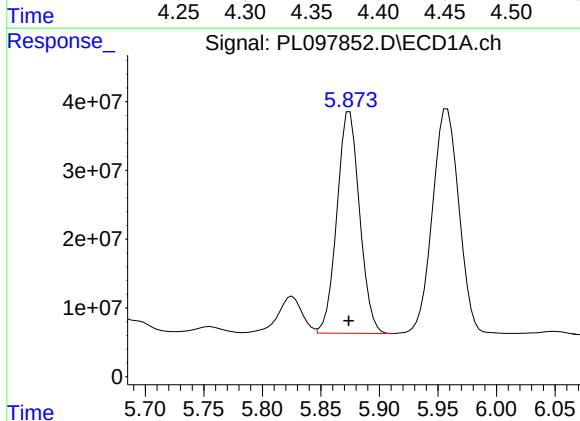


#25 Chlordane-3

R.T.: 5.875 min
Delta R.T.: 0.000 min
Response: 433852565
Conc: 491.70 ng/ml

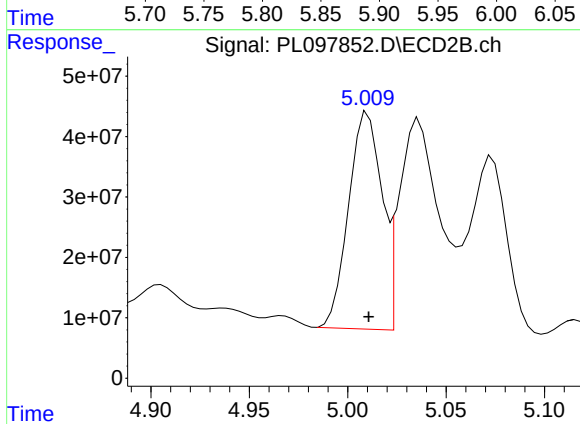

#25 Chlordane-3


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 422588625
Conc: 483.99 ng/ml

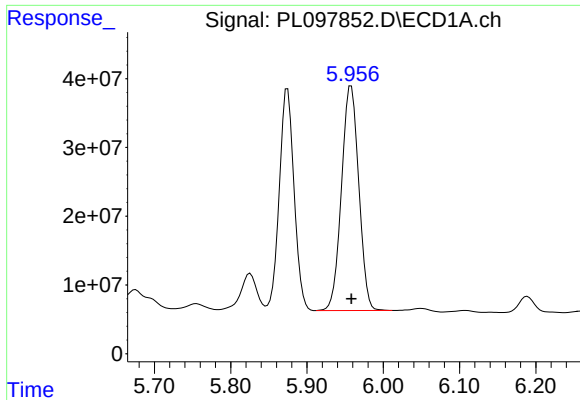

#26 Chlordane-4


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 514740168
Conc: 486.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

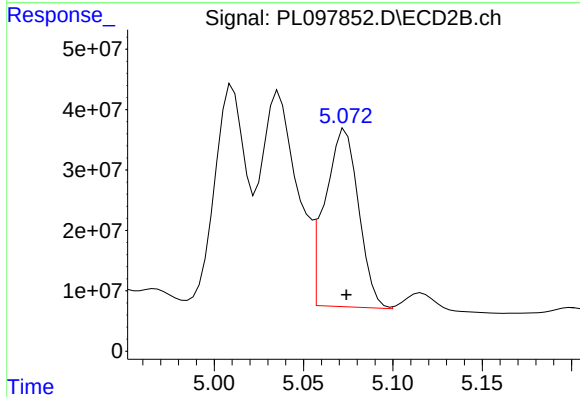


#26 Chlordane-4

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 385178160
Conc: 477.12 ng/ml

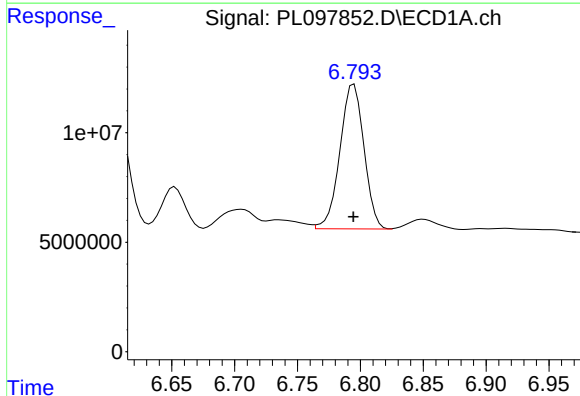


#27 Chlordane-5

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 88009154
Conc: 483.92 ng/ml

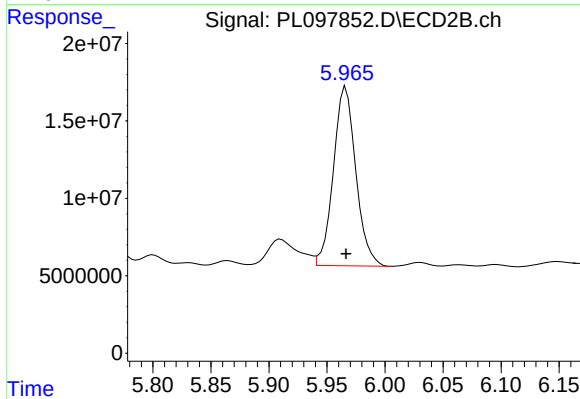

#27 Chlordane-5


R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 155505721
Conc: 472.71 ng/ml

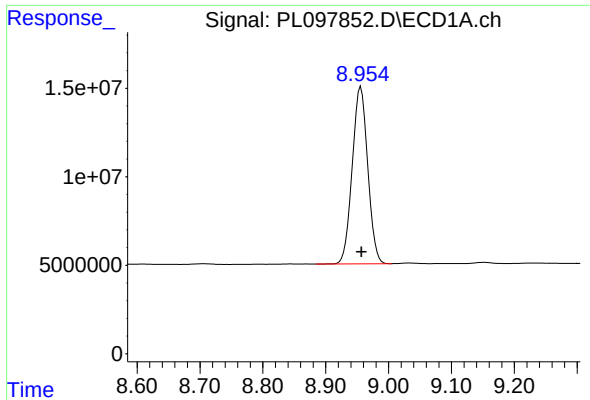

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 171374962
Conc: 45.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

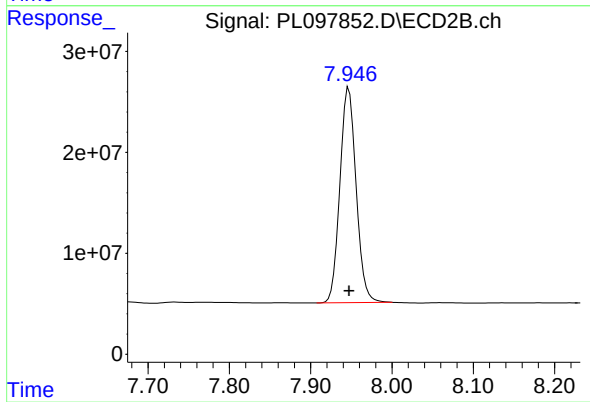

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 295236604
Conc: 44.90 ng/ml