

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2019 08:59
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 02:57:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7) B	delta-BHC	4.723	0.000	52790565	0	3.248	N.D. #
8) B	Heptachlo...	5.268	0.000	51279069	0	3.390	N.D. #
10) B	gamma-Chl...	5.481f	0.000	25245490	0	1.665	N.D. #
11) B	alpha-Chl...	5.542f	0.000	21044512	0	1.427	N.D. #
25)	Chlordane-3	5.481f	0.000	25245490	0	19.660	N.D. #
26)	Chlordane-4	5.542	0.000	21044512	0	19.923	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2019 08:59
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 02:57:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

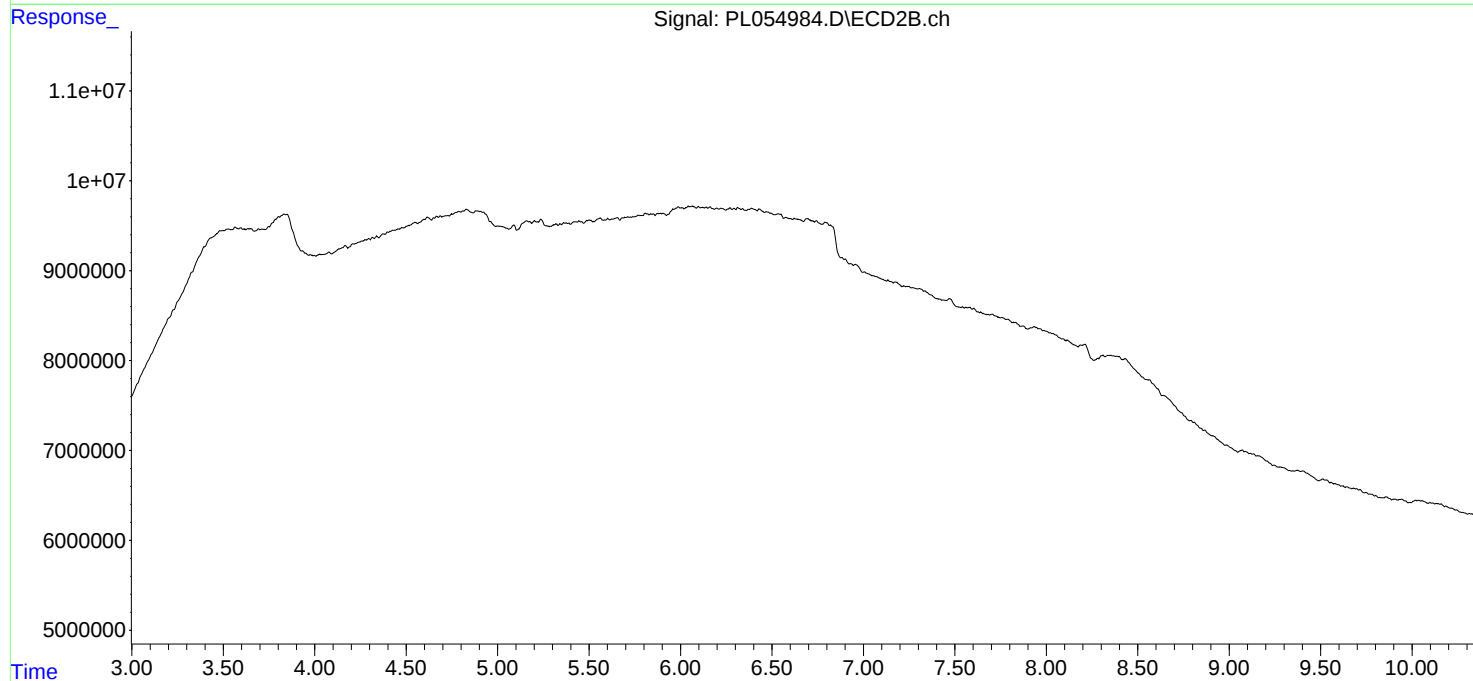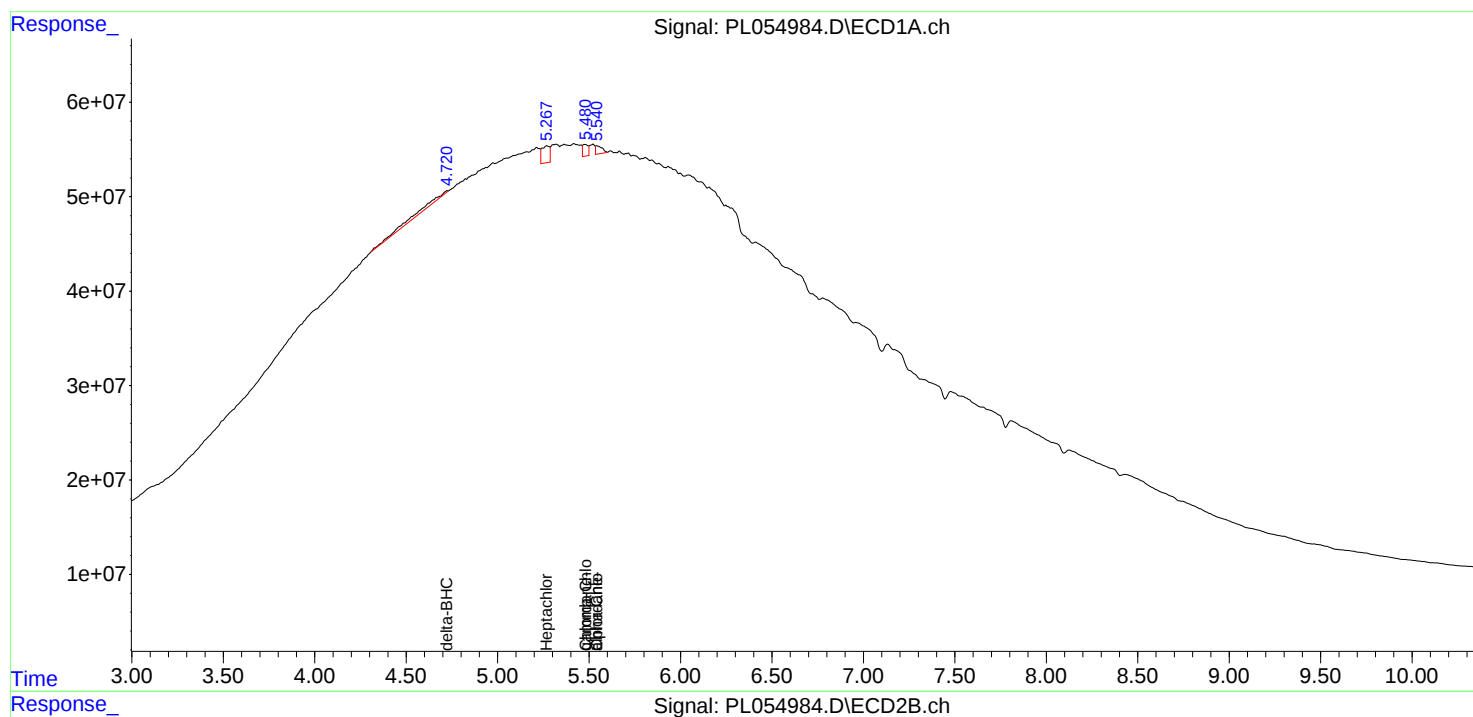


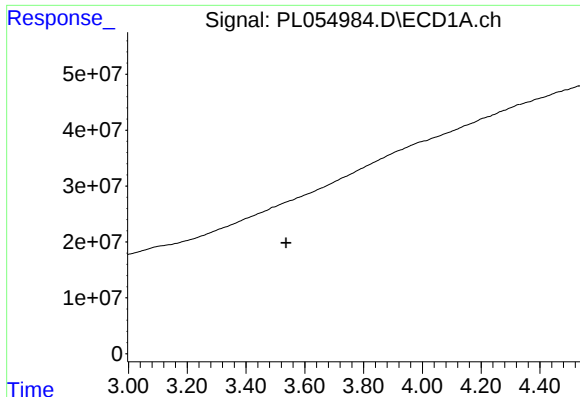

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

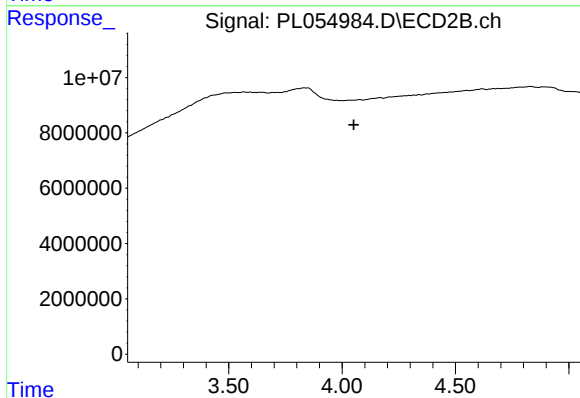


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.052 min
Response: 0
Conc: N.D.

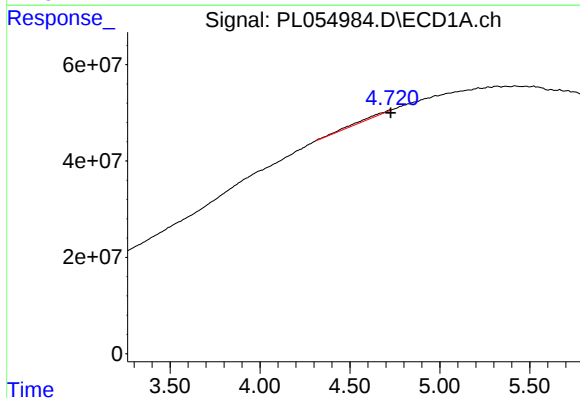


#7 delta-BHC

R.T.: 4.723 min
Delta R.T.: -0.003 min
Response: 52790565
Conc: 3.25 ng/ml

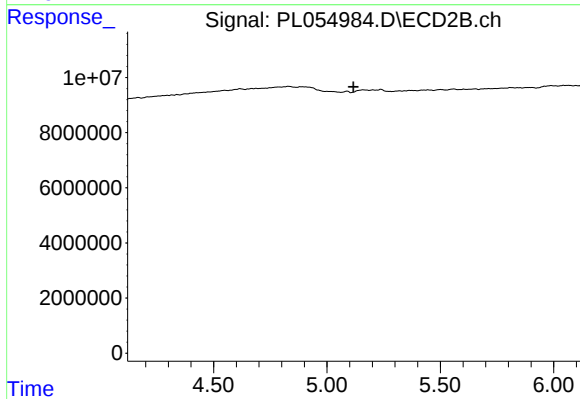

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

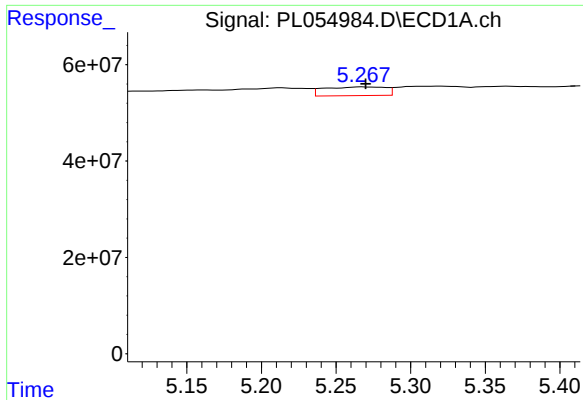

#8 Heptachlor epoxide


R.T.: 5.268 min
Delta R.T.: -0.002 min
Response: 51279069
Conc: 3.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

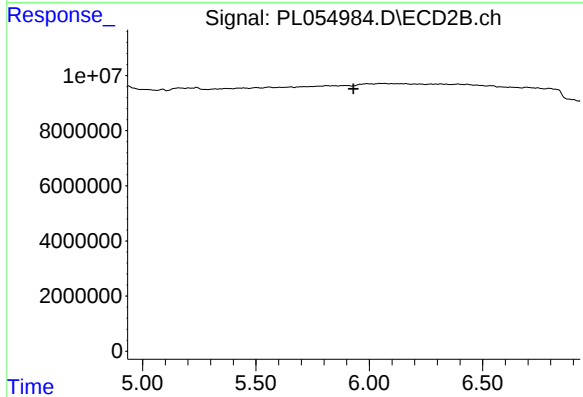


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.930 min
Response: 0
Conc: N.D.

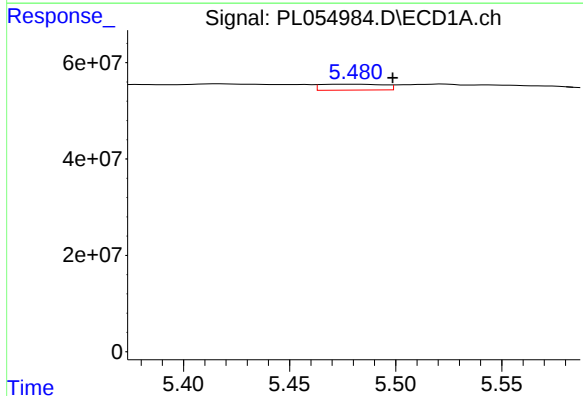


#10 gamma-Chlordane

R.T.: 5.481 min
Delta R.T.: -0.017 min
Response: 25245490
Conc: 1.66 ng/ml

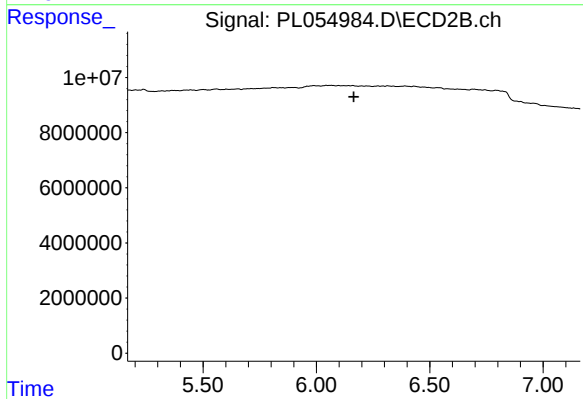

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

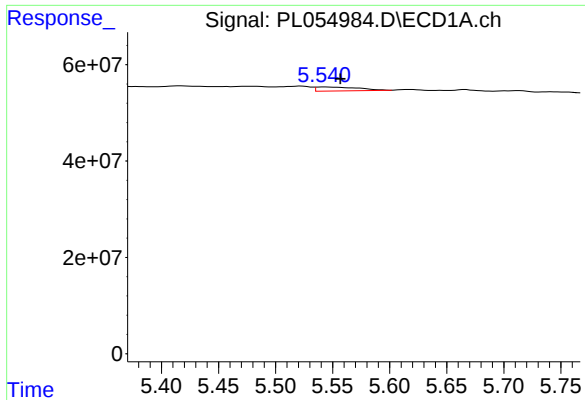

#11 alpha-Chlordane


R.T.: 5.542 min
Delta R.T.: -0.015 min
Response: 21044512
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

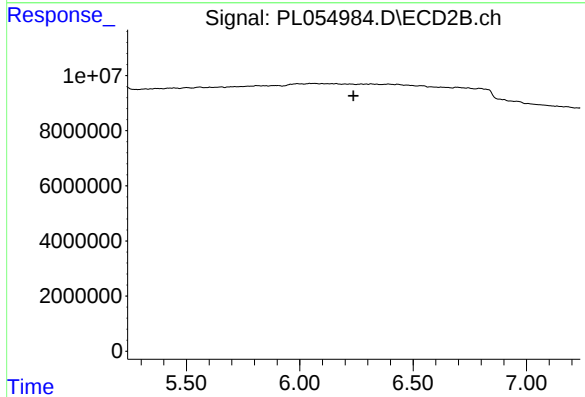


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

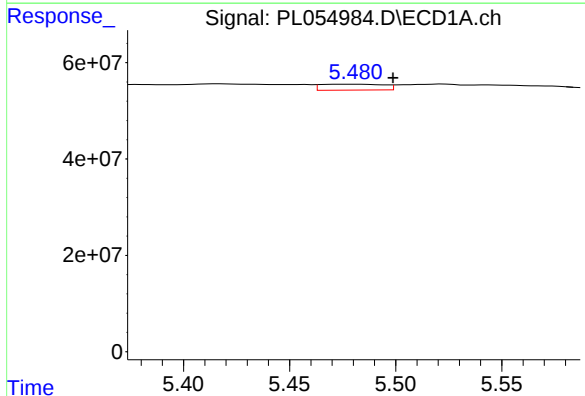


#25 Chlordane-3

R.T.: 5.481 min
Delta R.T.: -0.017 min
Response: 25245490
Conc: 19.66 ng/ml

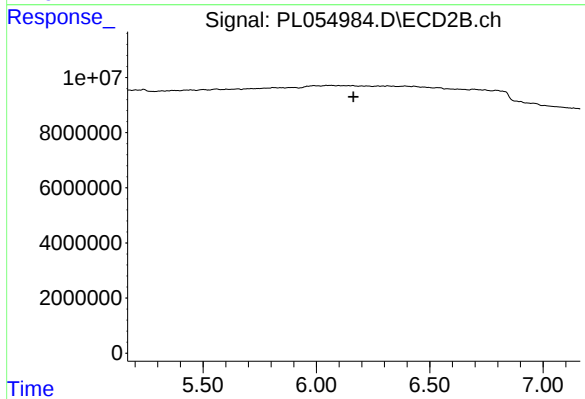

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

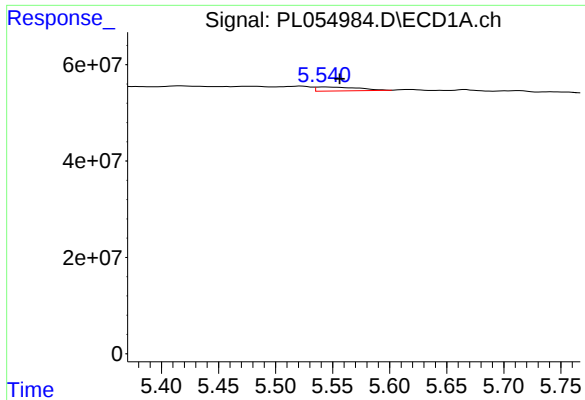

#26 Chlordane-4


R.T.: 5.542 min
Delta R.T.: -0.015 min
Response: 21044512
Conc: 19.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

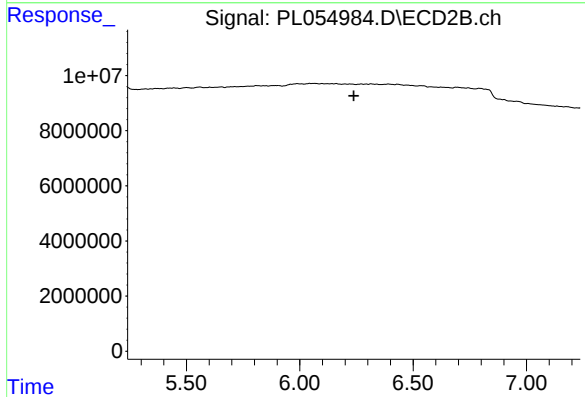


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

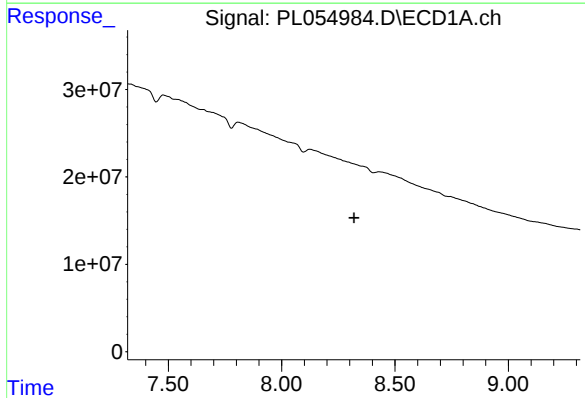

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.320 min
Response: 0
Conc: N.D.

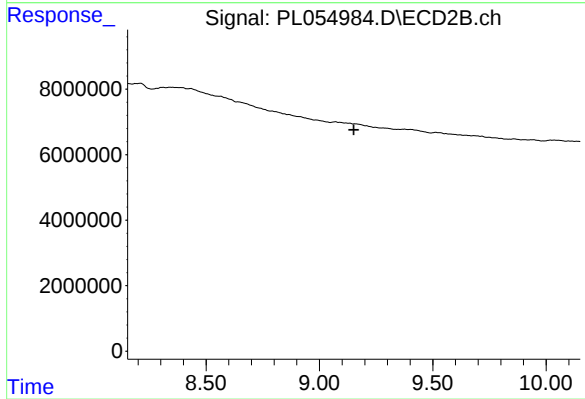

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.