

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121619\
 Data File : PL054995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2019 15:37
 Operator : SG\AJ
 Sample : K6113-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-121319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:00:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.048	128.9E6	32805851	11.080	12.856
28)	SA Decachlor...	8.314	9.145	106.8E6	27784039	11.157	11.589
Target Compounds							
4)	MA Heptachlor	4.573	0.000	8373060	0	0.475	N.D. #
10)	B gamma-Chl...	5.517f	6.161	21638119	1905381	1.427	0.723 #
11)	B alpha-Chl...	5.552	6.235	14117691	5773135	0.957	2.199 #
23)	Chlordane-1	4.417	0.000	8694056	0	22.031	N.D. #
24)	Chlordane-2	4.925	0.000	2253150	0	5.189	N.D. #
25)	Chlordane-3	5.517f	6.161	21638119	1905381	16.850	6.138 #
26)	Chlordane-4	5.552	6.235	14117691	5773135	13.365	15.342



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121619\
Data File : PL054995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2019 15:37
Operator : SG\AJ
Sample : K6113-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:00:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

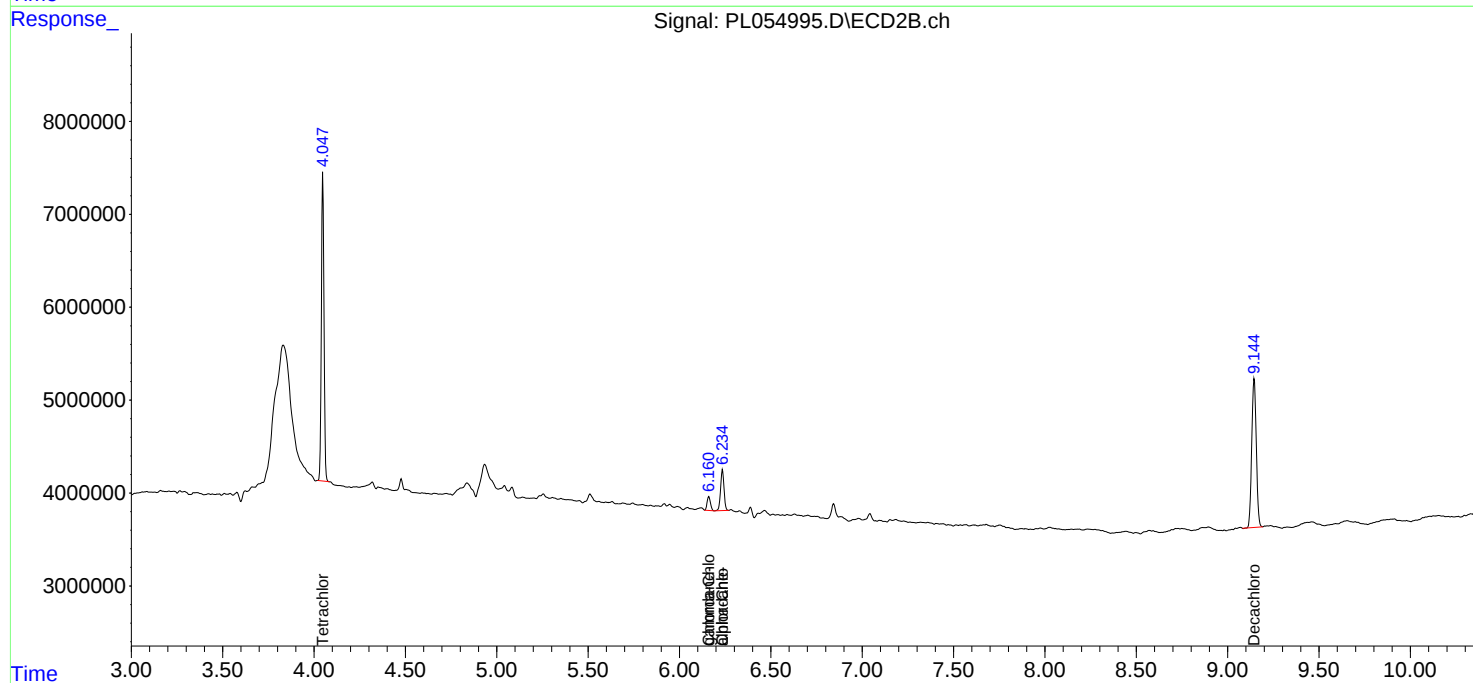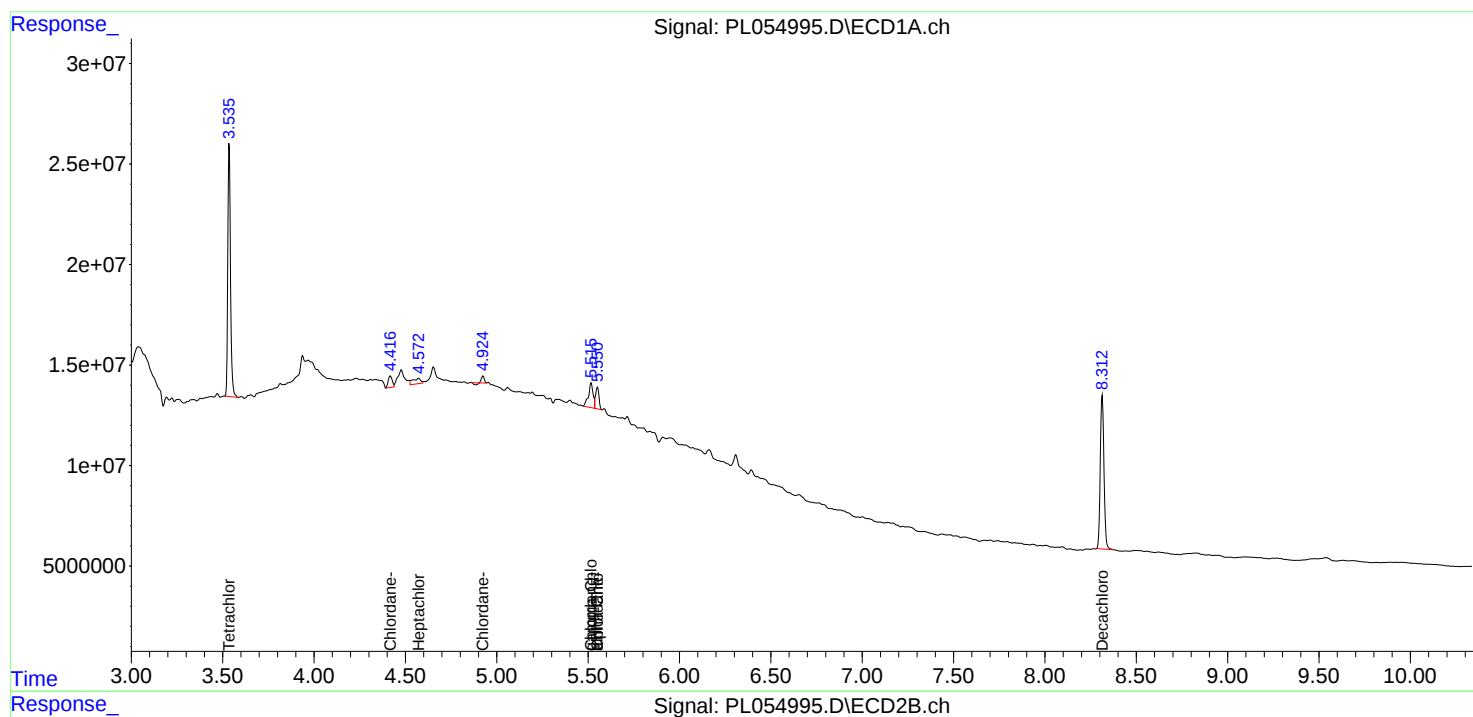


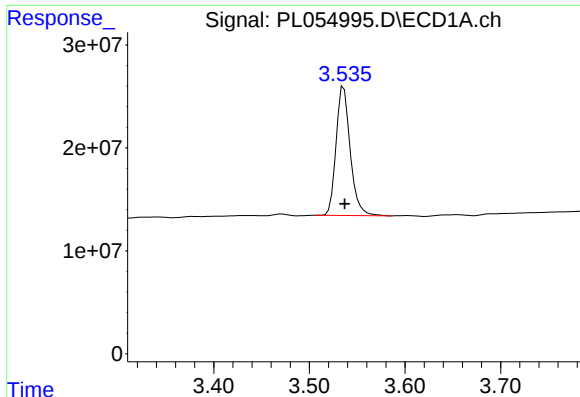

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 128901561
Conc: 11.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

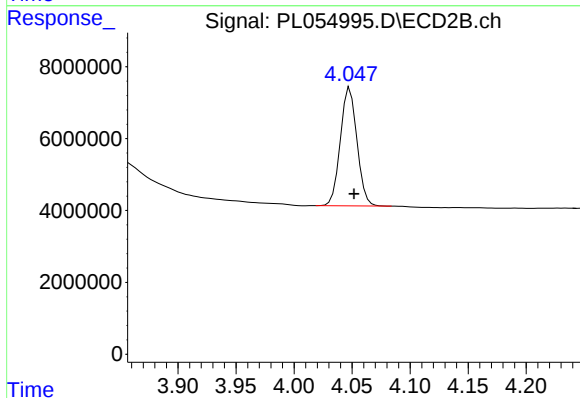


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 32805851
Conc: 12.86 ng/ml

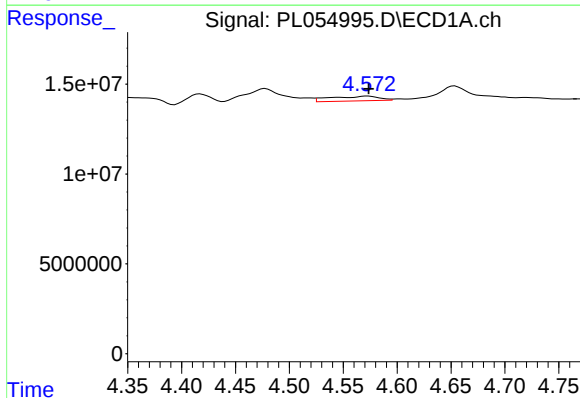


#4 Heptachlor

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 8373060
Conc: 0.47 ng/ml

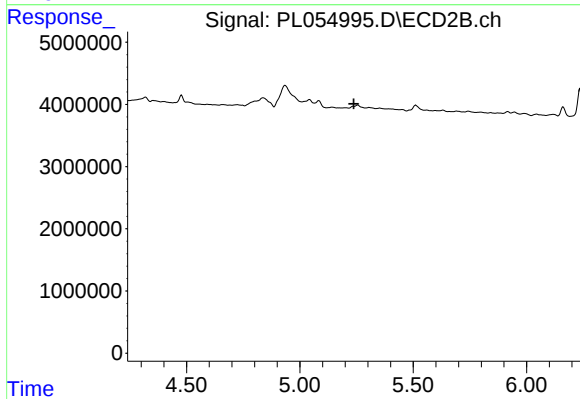

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.238 min
Response: 0
Conc: N.D.

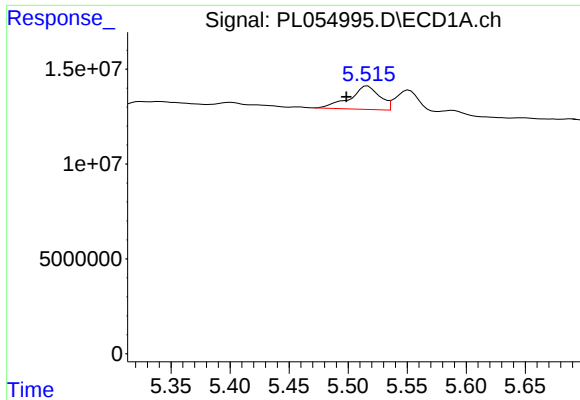

#10 gamma-Chlordane


R.T.: 5.517 min
Delta R.T.: 0.018 min
Response: 21638119
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

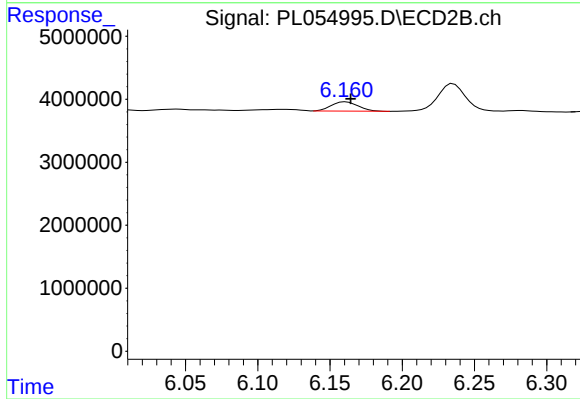


#10 gamma-Chlordane

R.T.: 6.161 min
Delta R.T.: -0.004 min
Response: 1905381
Conc: 0.72 ng/ml

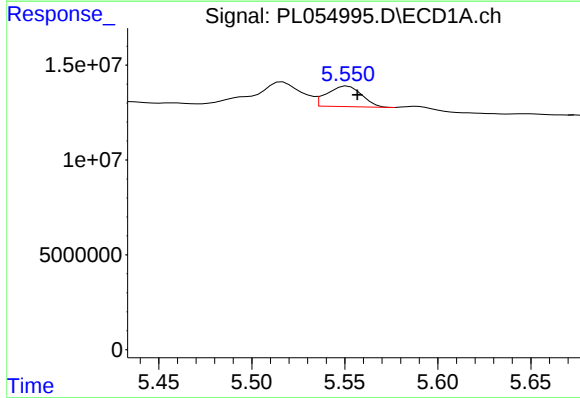


#11 alpha-Chlordane

R.T.: 5.552 min
Delta R.T.: -0.005 min
Response: 14117691
Conc: 0.96 ng/ml

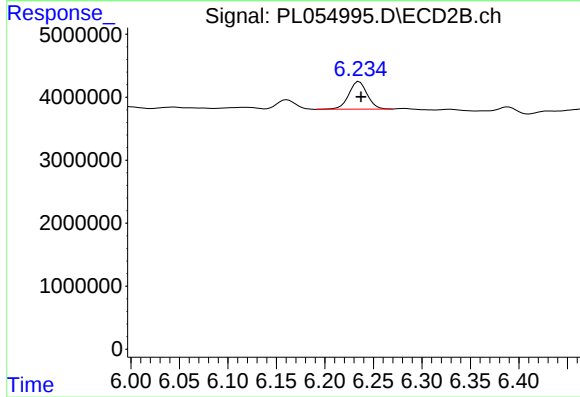

#11 alpha-Chlordane


R.T.: 6.235 min
Delta R.T.: -0.002 min
Response: 5773135
Conc: 2.20 ng/ml

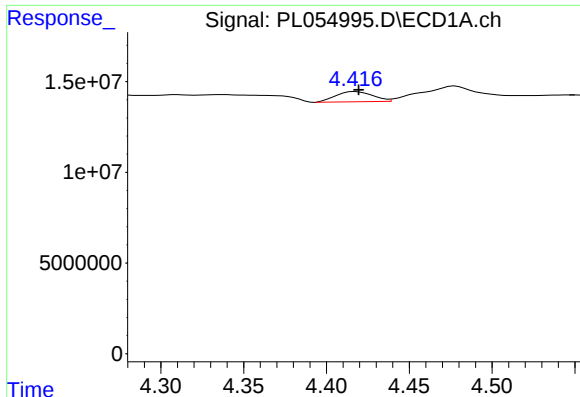

#23 Chlordane-1


R.T.: 4.417 min
Delta R.T.: -0.002 min
Response: 8694056
Conc: 22.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

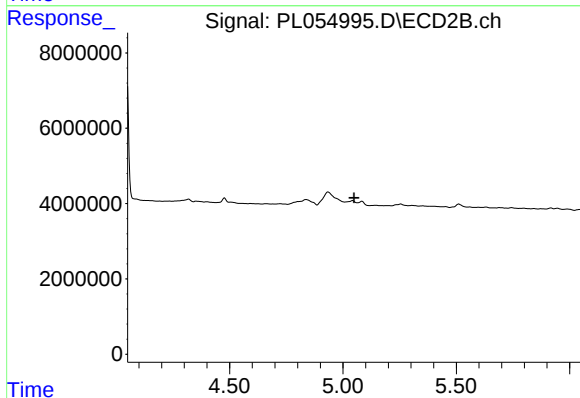


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

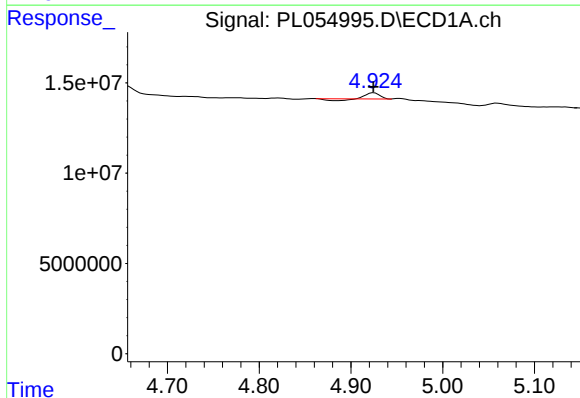


#24 Chlordane-2

R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 2253150
Conc: 5.19 ng/ml

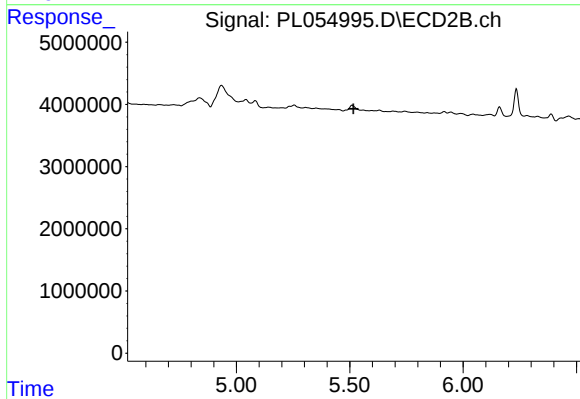

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.517 min
Response: 0
Conc: N.D.

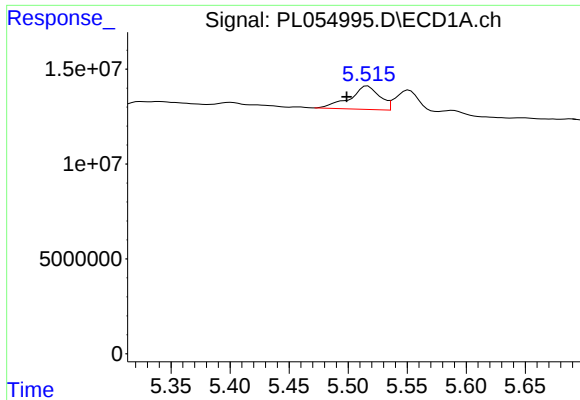

#25 Chlordane-3


R.T.: 5.517 min
Delta R.T.: 0.018 min
Response: 21638119
Conc: 16.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

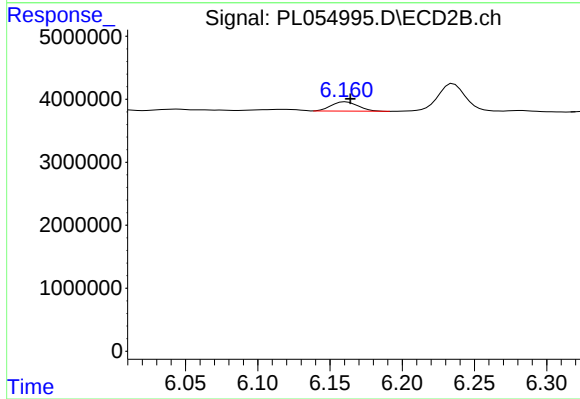


#25 Chlordane-3

R.T.: 6.161 min
Delta R.T.: -0.003 min
Response: 1905381
Conc: 6.14 ng/ml

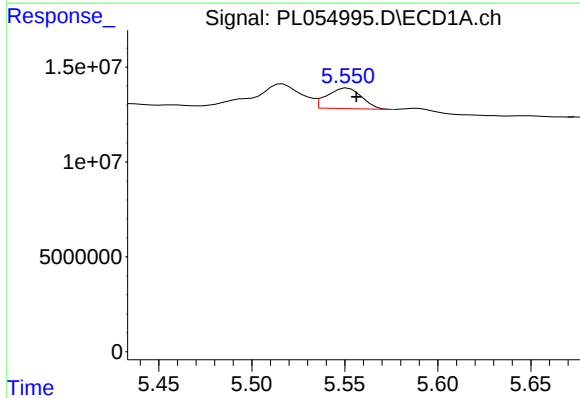


#26 Chlordane-4

R.T.: 5.552 min
Delta R.T.: -0.005 min
Response: 14117691
Conc: 13.37 ng/ml

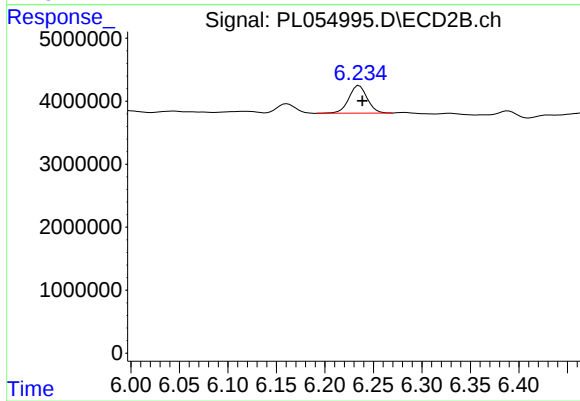

#26 Chlordane-4


R.T.: 6.235 min
Delta R.T.: -0.003 min
Response: 5773135
Conc: 15.34 ng/ml

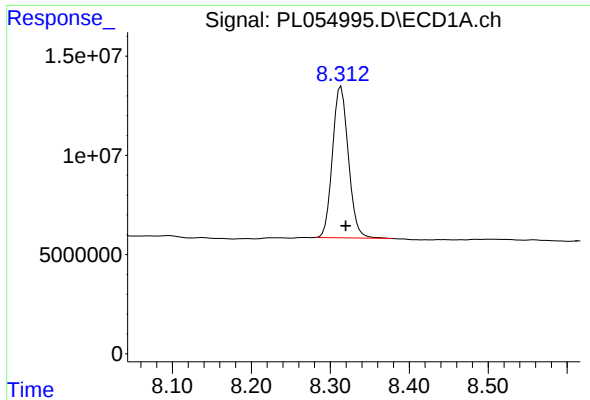

#28 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: -0.006 min
Response: 106842185
Conc: 11.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-121319

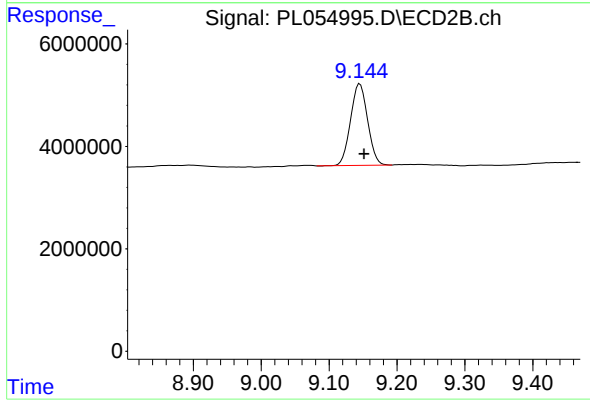

#28 Decachlorobiphenyl

R.T.: 9.145 min
Delta R.T.: -0.006 min
Response: 27784039
Conc: 11.59 ng/ml