

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
 Data File : PL063635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 03:51
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 07:59:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 07:58:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.149	58506751	83167503	24.331	25.516
28)	SA Decachlor...	8.229	9.338	56356998	66614425	26.469	25.277
Target Compounds							
23)	Chlordane-1	4.351	5.168	19141236	28970770	252.227	248.493
24)	Chlordane-2	4.852	5.645	22866601	31411785	259.448	247.085
25)	Chlordane-3	5.419	6.303	59502908	112.0E6	243.175	238.562
26)	Chlordane-4	5.478	6.377	50324542	134.0E6	246.489	240.769
27)	Chlordane-5	6.309	7.199	20511957	20507478	251.919	242.647



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
Data File : PL063635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 03:51
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 07:59:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 07:58:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

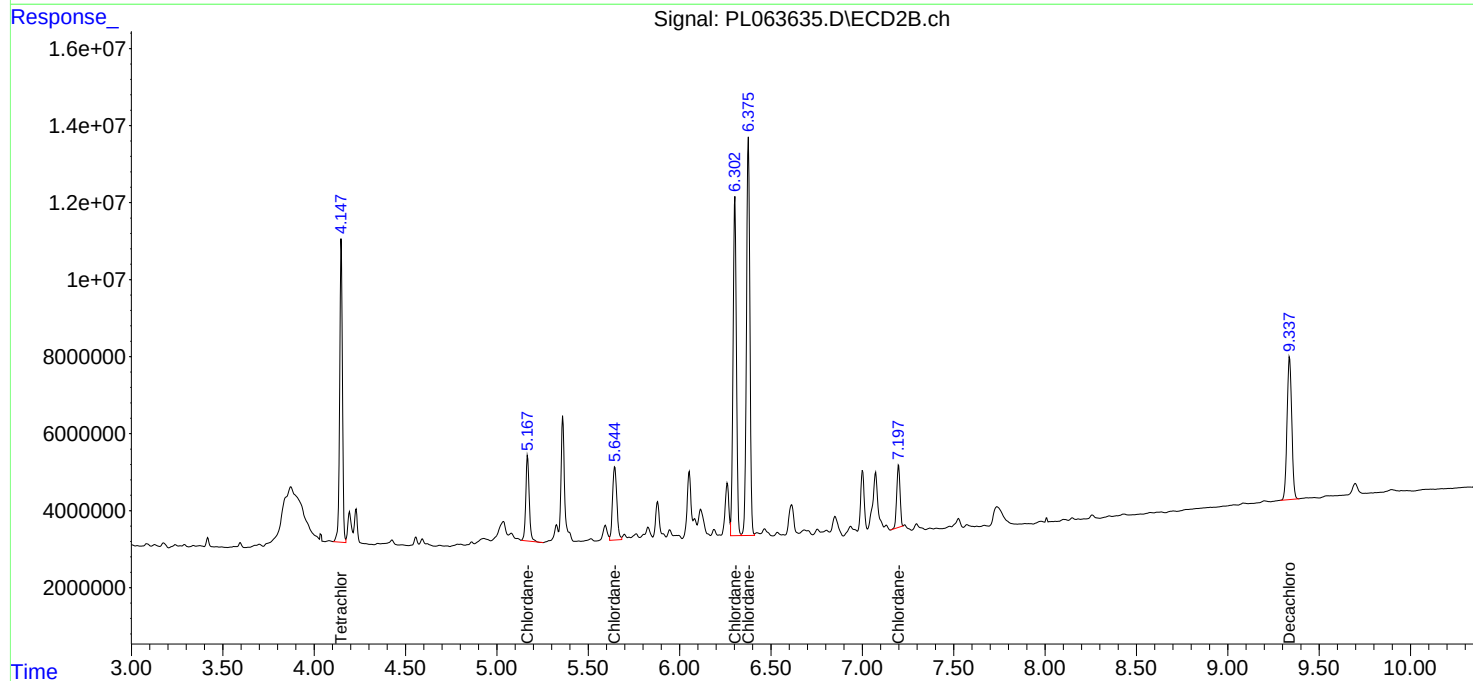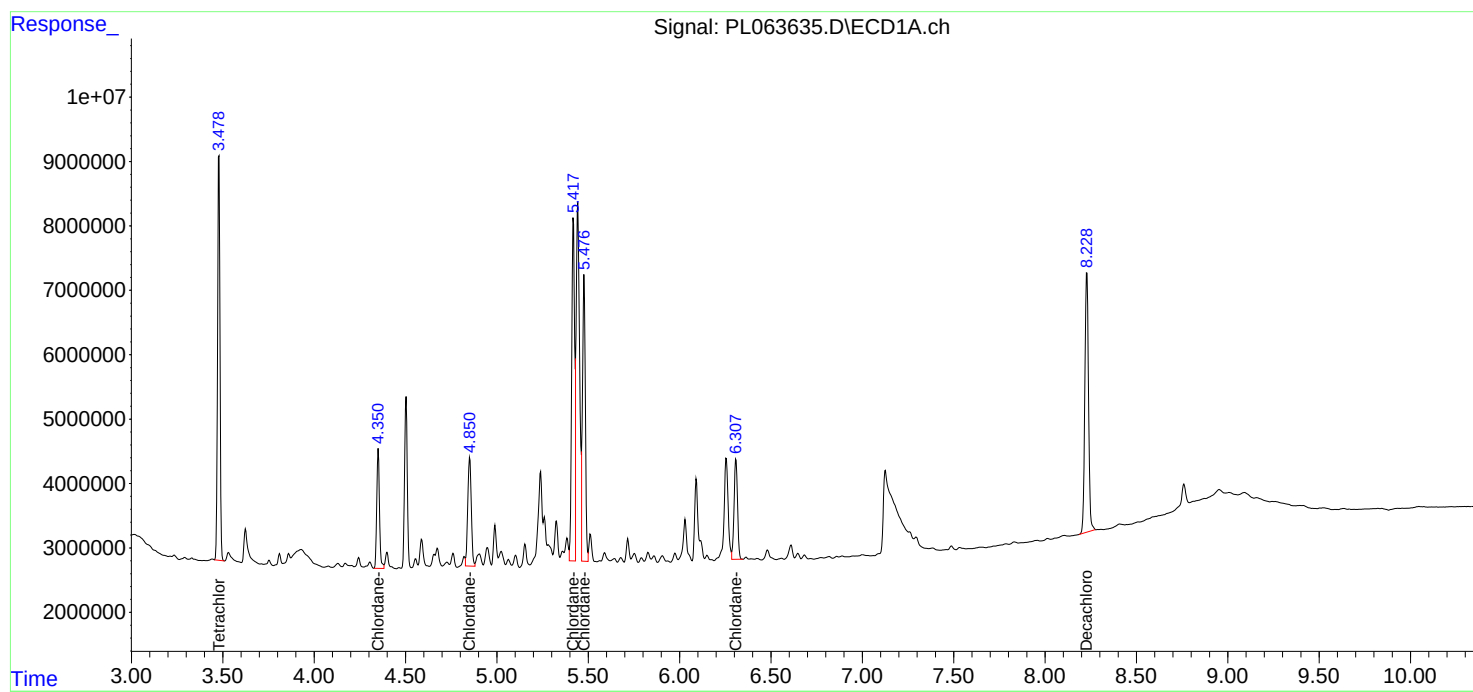


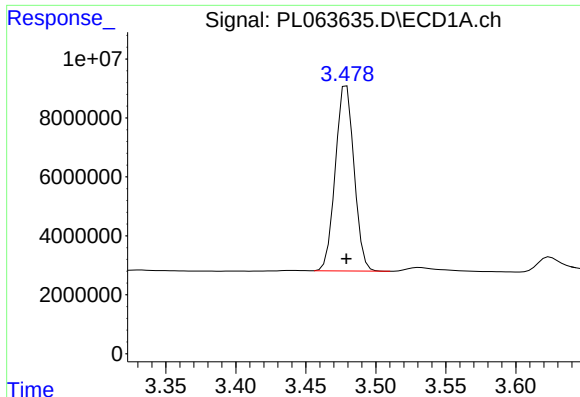

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 58506751
Conc: 24.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

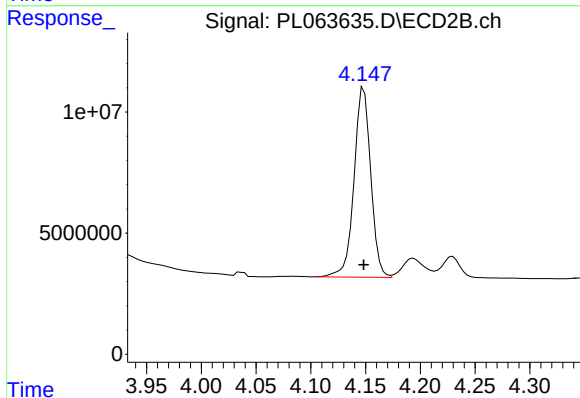


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 83167503
Conc: 25.52 ng/ml

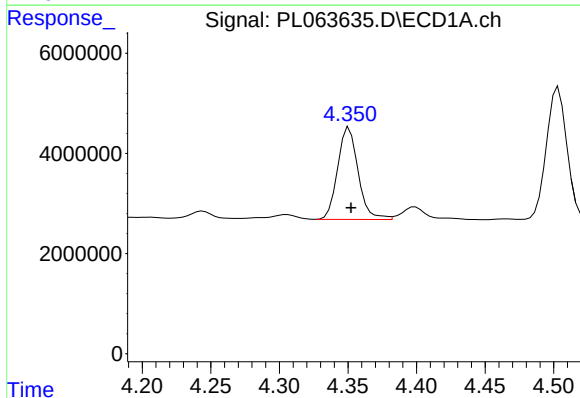


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: -0.001 min
Response: 19141236
Conc: 252.23 ng/ml

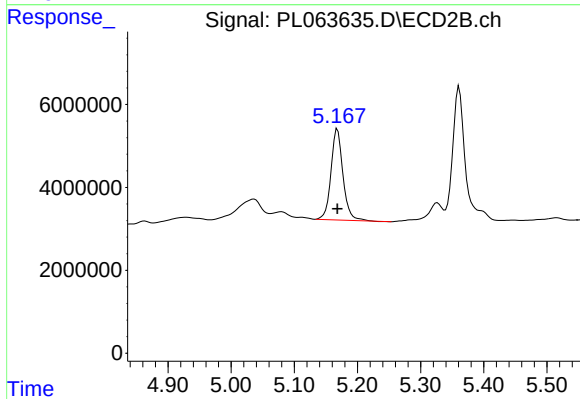

#23 Chlordane-1


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 28970770
Conc: 248.49 ng/ml

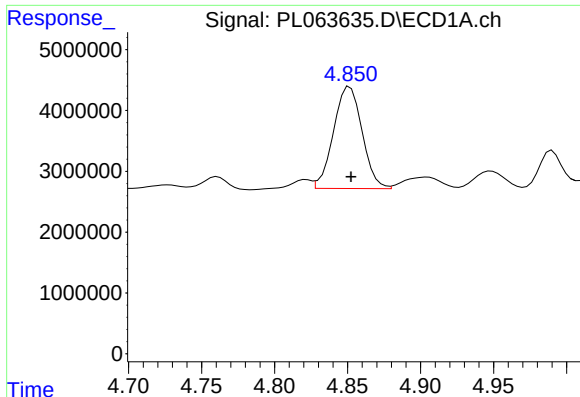

#24 Chlordane-2


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 22866601
Conc: 259.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

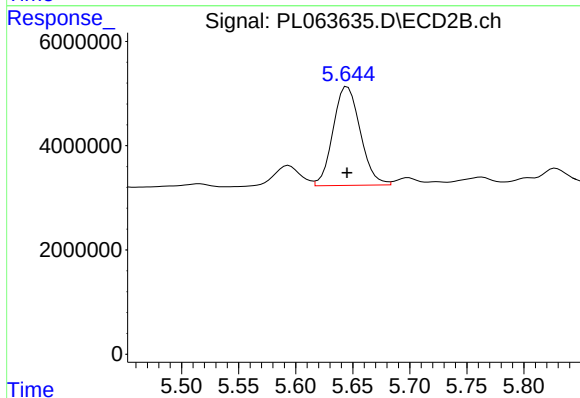


#24 Chlordane-2

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 31411785
Conc: 247.09 ng/ml

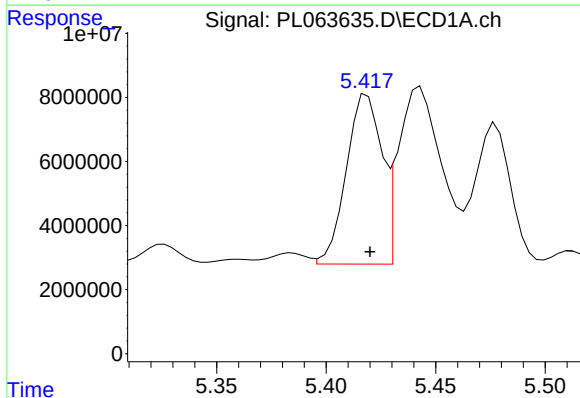


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: -0.001 min
Response: 59502908
Conc: 243.17 ng/ml

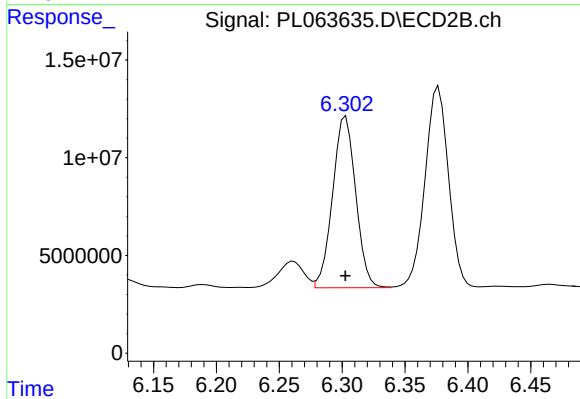

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 112048452
Conc: 238.56 ng/ml

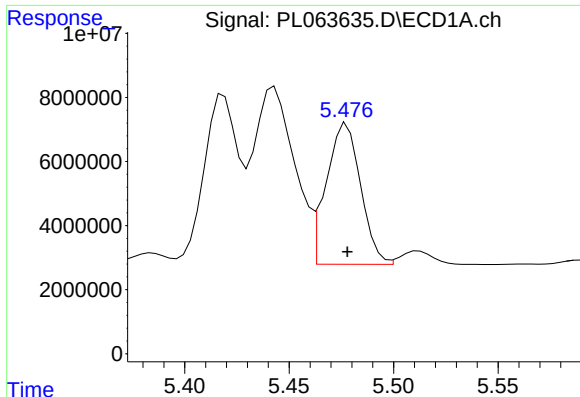

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 50324542
Conc: 246.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

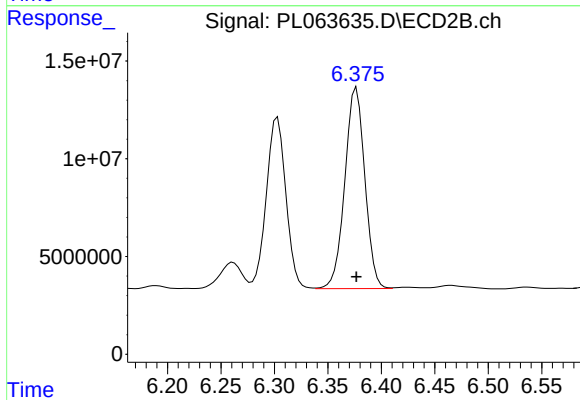


#26 Chlordane-4

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 134049071
Conc: 240.77 ng/ml

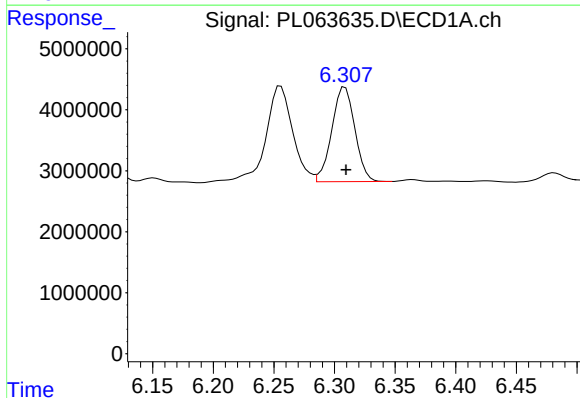


#27 Chlordane-5

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 20511957
Conc: 251.92 ng/ml

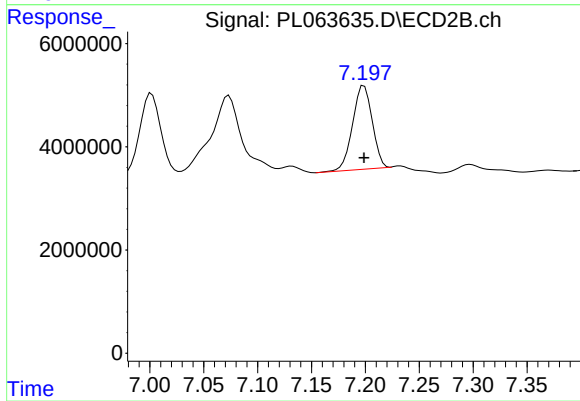

#27 Chlordane-5


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 20507478
Conc: 242.65 ng/ml

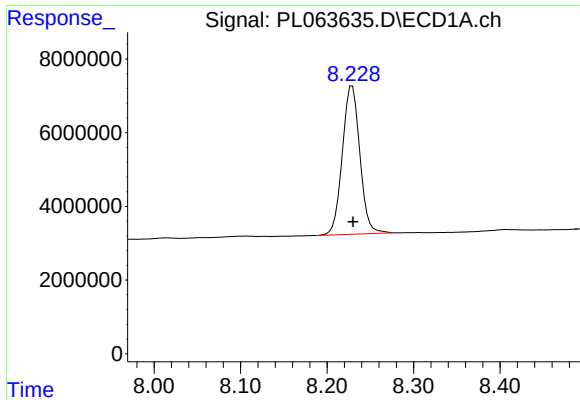

#28 Decachlorobiphenyl

R.T.: 8.229 min
Delta R.T.: -0.001 min
Response: 56356998
Conc: 26.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

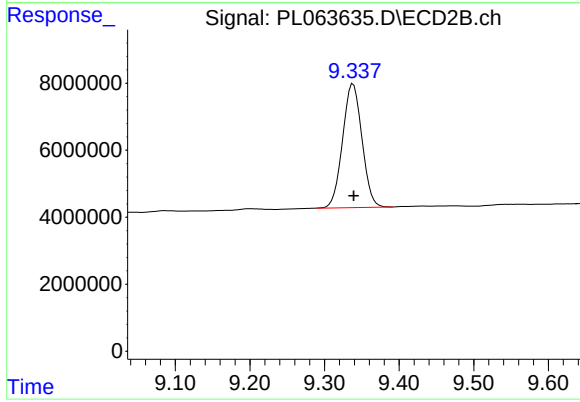

#28 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: 0.000 min
Response: 66614425
Conc: 25.28 ng/ml