

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
 Data File : PL063632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 03:07
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 07:58:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 07:58:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.478	4.148	238.7E6	319.6E6	99.265	98.044
28)	SA Decachlor...	8.227	9.339	196.5E6	249.7E6	92.267	94.764
Target Compounds							
23)	Chlordane-1	4.350	5.169	72584434	113.1E6	956.456	969.721
24)	Chlordane-2	4.850	5.645	81673124	120.7E6	926.677	949.220
25)	Chlordane-3	5.419	6.303	245.9E6	469.6E6	1004.900	999.823
26)	Chlordane-4	5.477	6.376	201.6E6	549.7E6	987.420	987.320
27)	Chlordane-5	6.308	7.199	79729334	89615226	979.203	1060.338



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
Data File : PL063632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 03:07
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 07:58:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 07:58:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

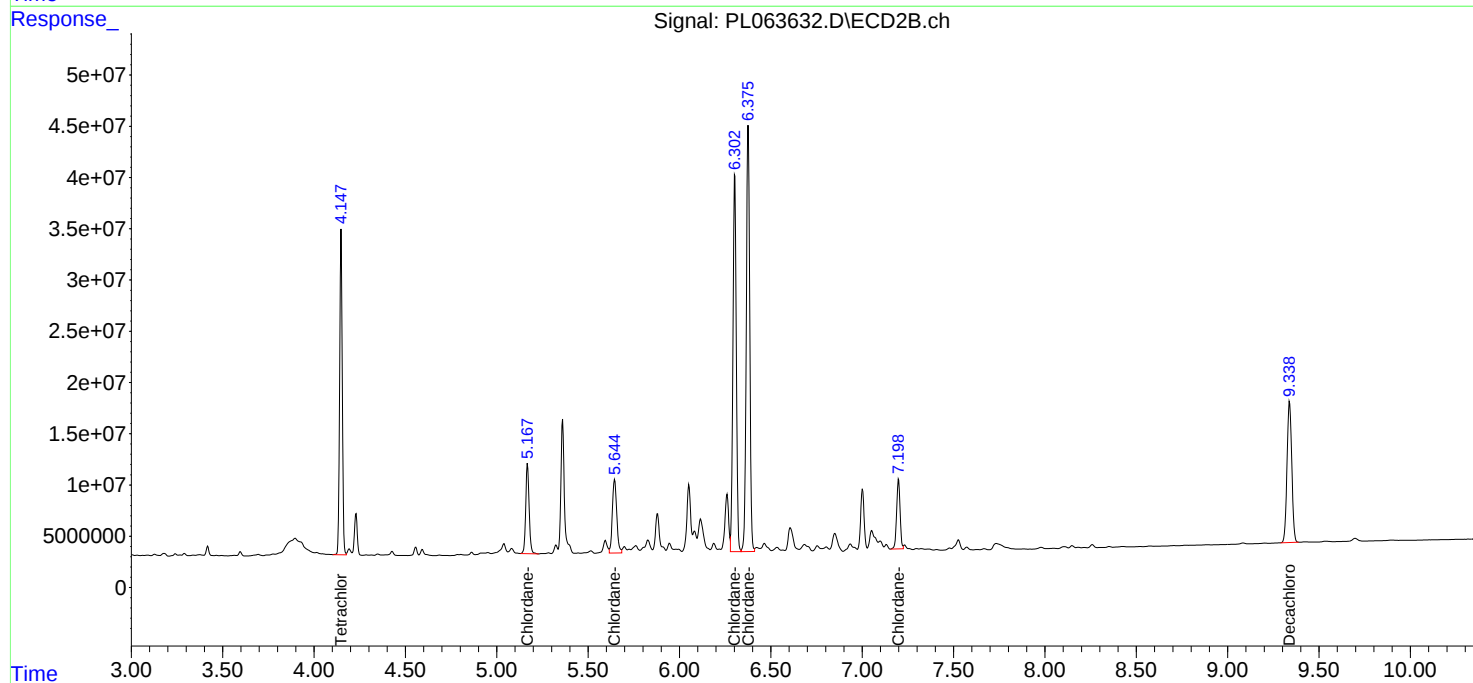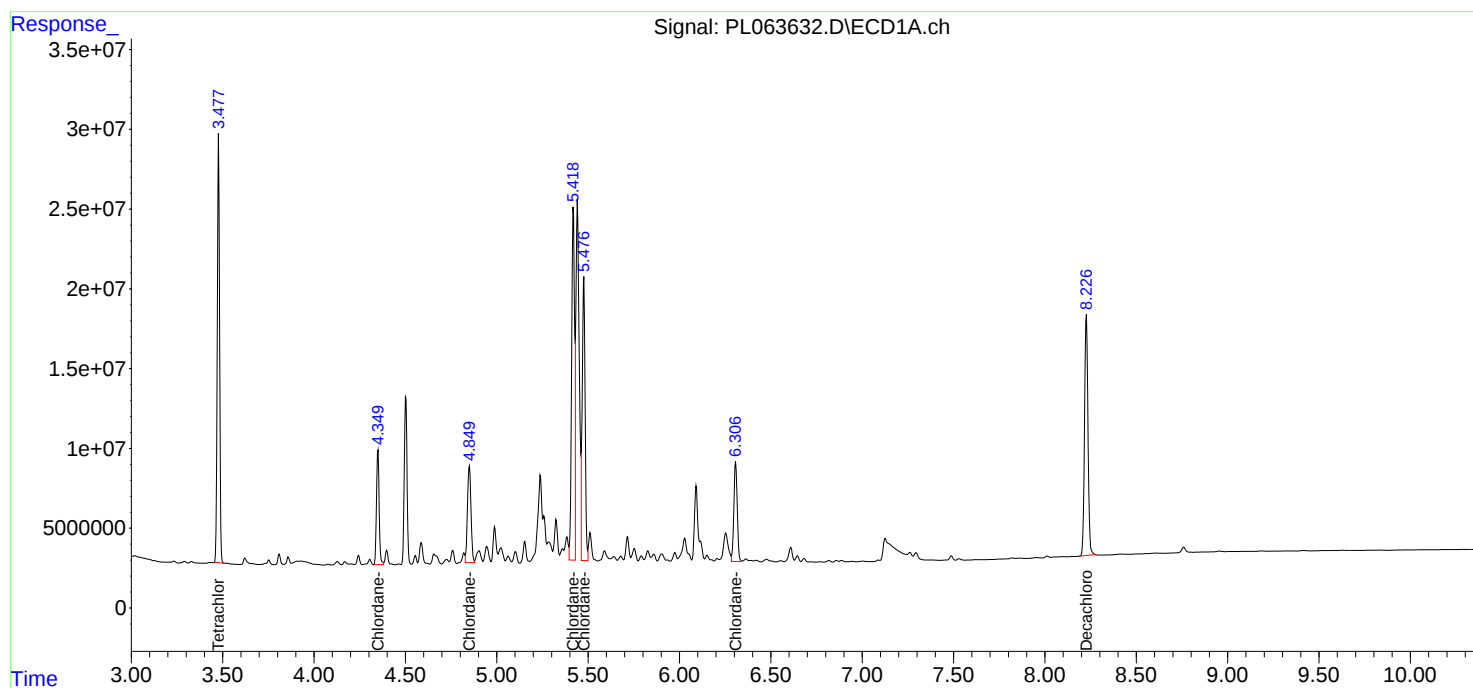


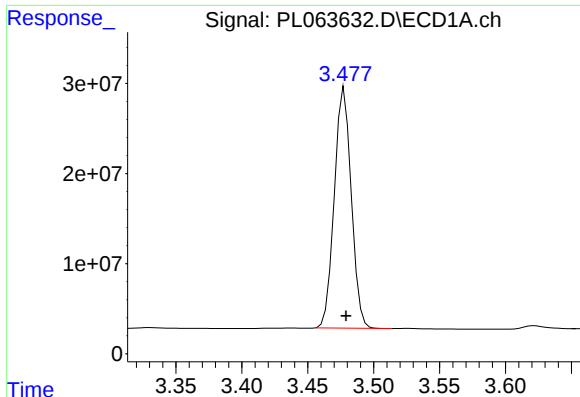

#1 Tetrachloro-m-xylene


R.T.: 3.478 min
Delta R.T.: -0.001 min
Response: 238693554
Conc: 99.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

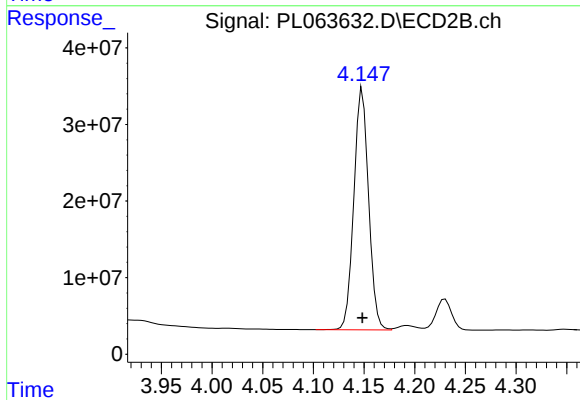


#1 Tetrachloro-m-xylene

R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 319564606
Conc: 98.04 ng/ml

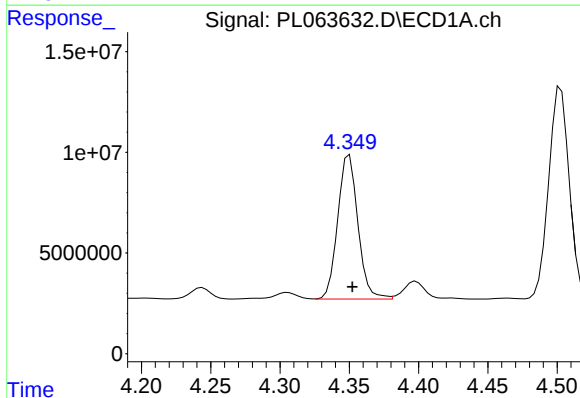


#23 Chlordane-1

R.T.: 4.350 min
Delta R.T.: -0.002 min
Response: 72584434
Conc: 956.46 ng/ml

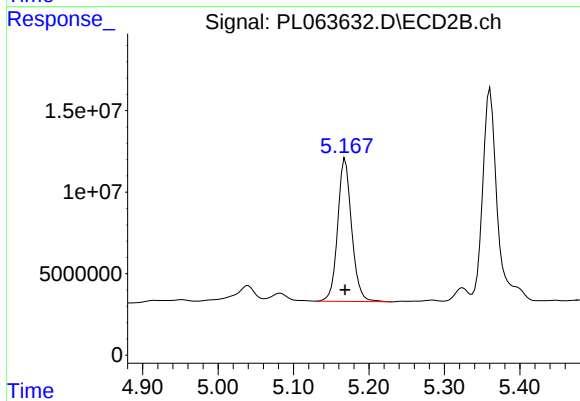

#23 Chlordane-1


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 113055870
Conc: 969.72 ng/ml

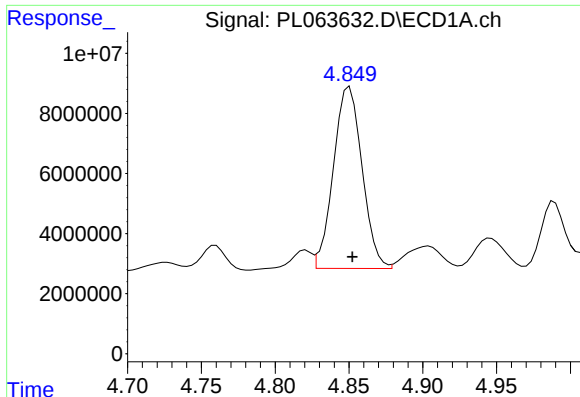

#24 Chlordane-2


R.T.: 4.850 min
Delta R.T.: -0.002 min
Response: 81673124
Conc: 926.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

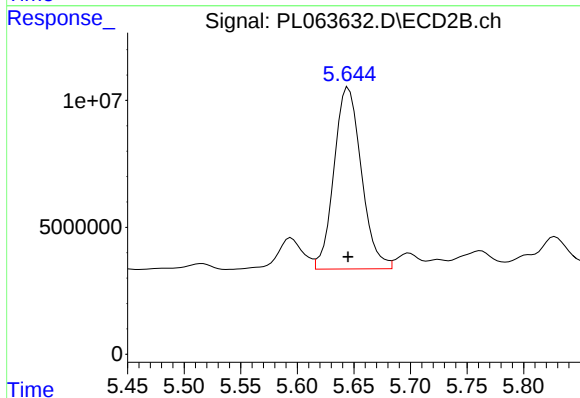


#24 Chlordane-2

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 120673634
Conc: 949.22 ng/ml

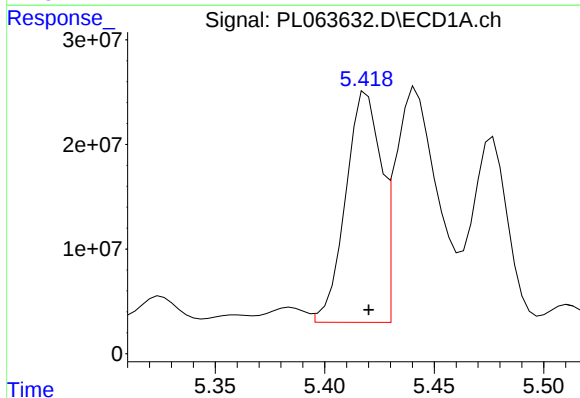


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.000 min
Response: 245890979
Conc: 1004.90 ng/ml

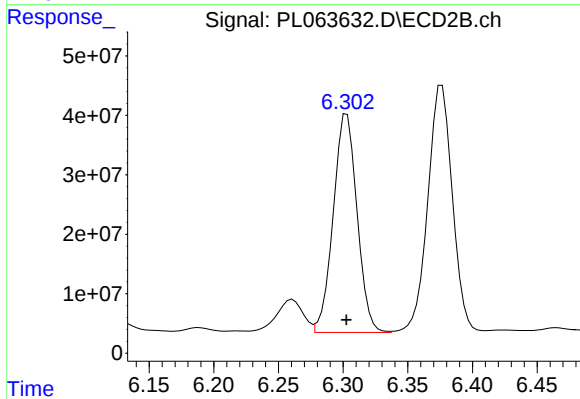

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 469600449
Conc: 999.82 ng/ml

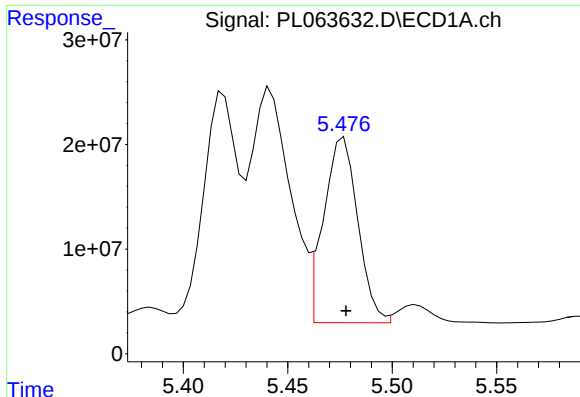

#26 Chlordane-4


R.T.: 5.477 min
Delta R.T.: -0.001 min
Response: 201597287
Conc: 987.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

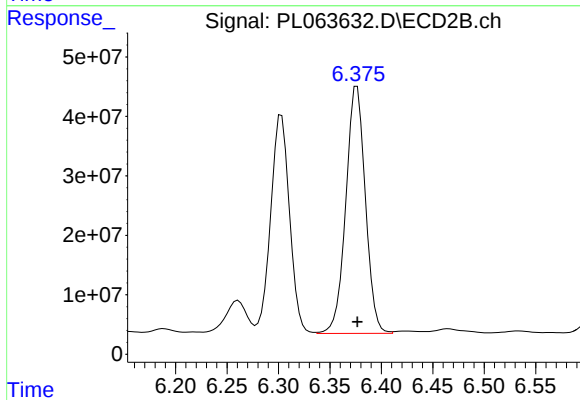


#26 Chlordane-4

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 549695062
Conc: 987.32 ng/ml

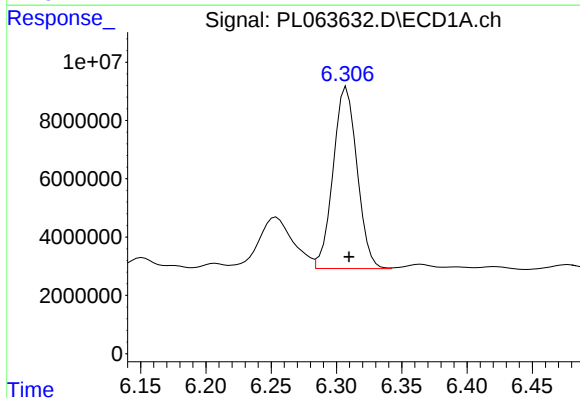


#27 Chlordane-5

R.T.: 6.308 min
Delta R.T.: -0.002 min
Response: 79729334
Conc: 979.20 ng/ml

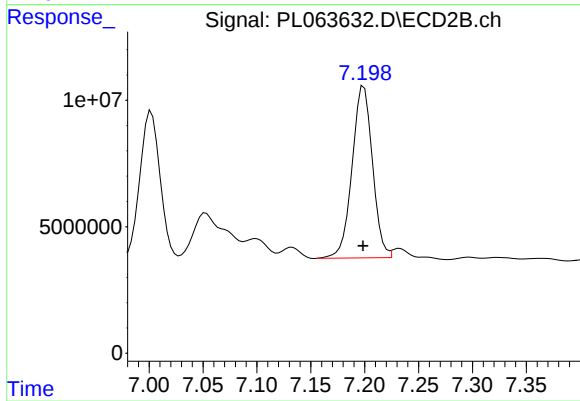

#27 Chlordane-5


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 89615226
Conc: 1060.34 ng/ml

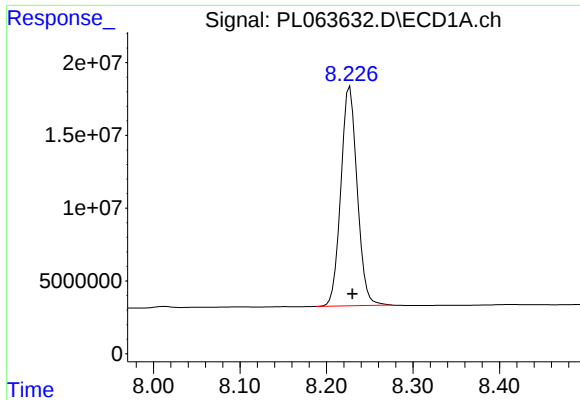

#28 Decachlorobiphenyl

R.T.: 8.227 min
Delta R.T.: -0.003 min
Response: 196450010
Conc: 92.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

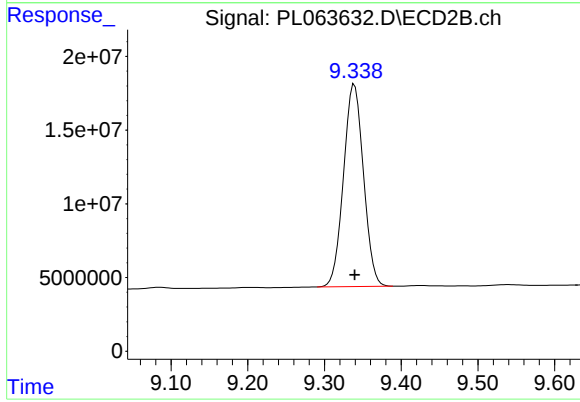

#28 Decachlorobiphenyl

R.T.: 9.339 min
Delta R.T.: 0.000 min
Response: 249737593
Conc: 94.76 ng/ml