

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
 Data File : PL063633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 03:21
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 07:58:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 07:58:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.149	187.8E6	249.7E6	78.115	76.614
28)	SA Decachlor...	8.229	9.339	158.1E6	199.4E6	74.244	75.681
Target Compounds							
23)	Chlordane-1	4.351	5.169	56985649	87867348	750.908	753.670
24)	Chlordane-2	4.852	5.645	65005506	95149694	737.563	748.449
25)	Chlordane-3	5.420	6.303	193.8E6	362.7E6	792.134	772.133
26)	Chlordane-4	5.478	6.376	155.8E6	425.8E6	763.017	764.858
27)	Chlordane-5	6.309	7.199	62695395	69637962	769.999	823.965



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
Data File : PL063633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 03:21
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 07:58:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 07:58:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

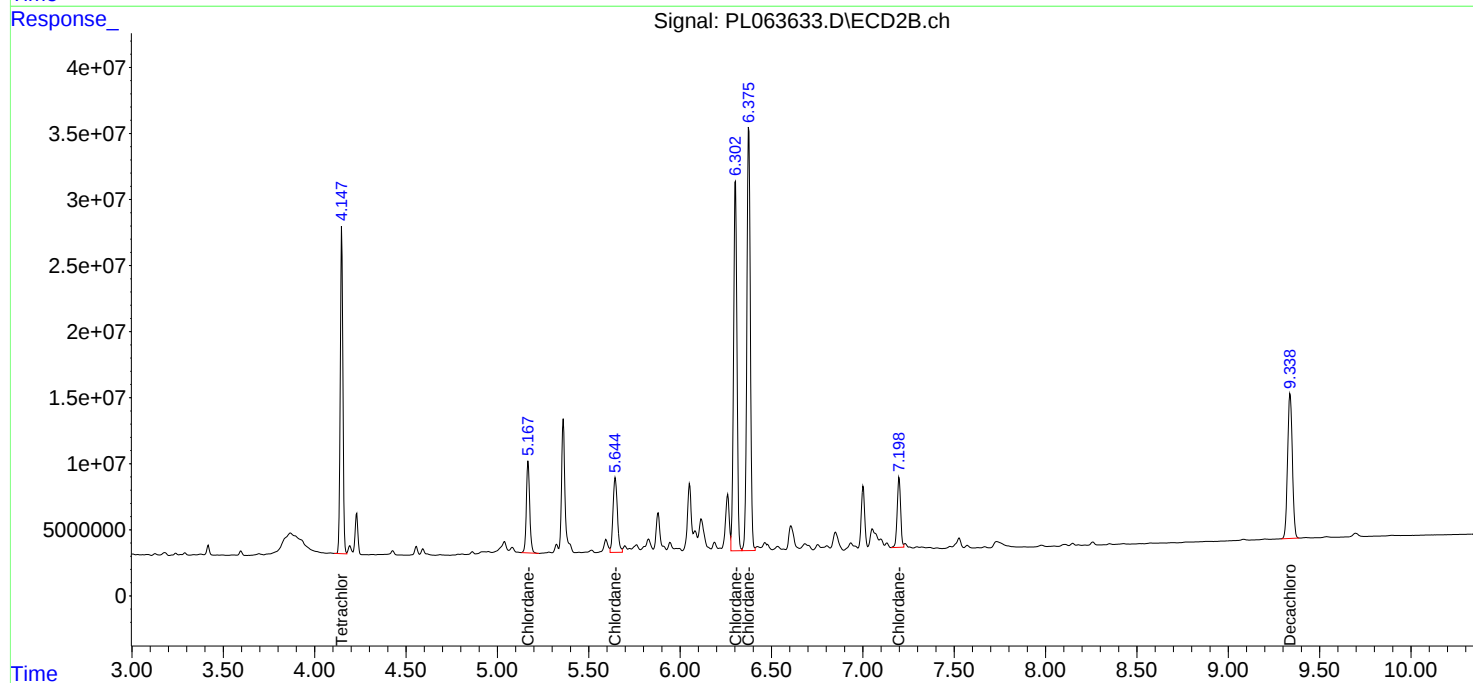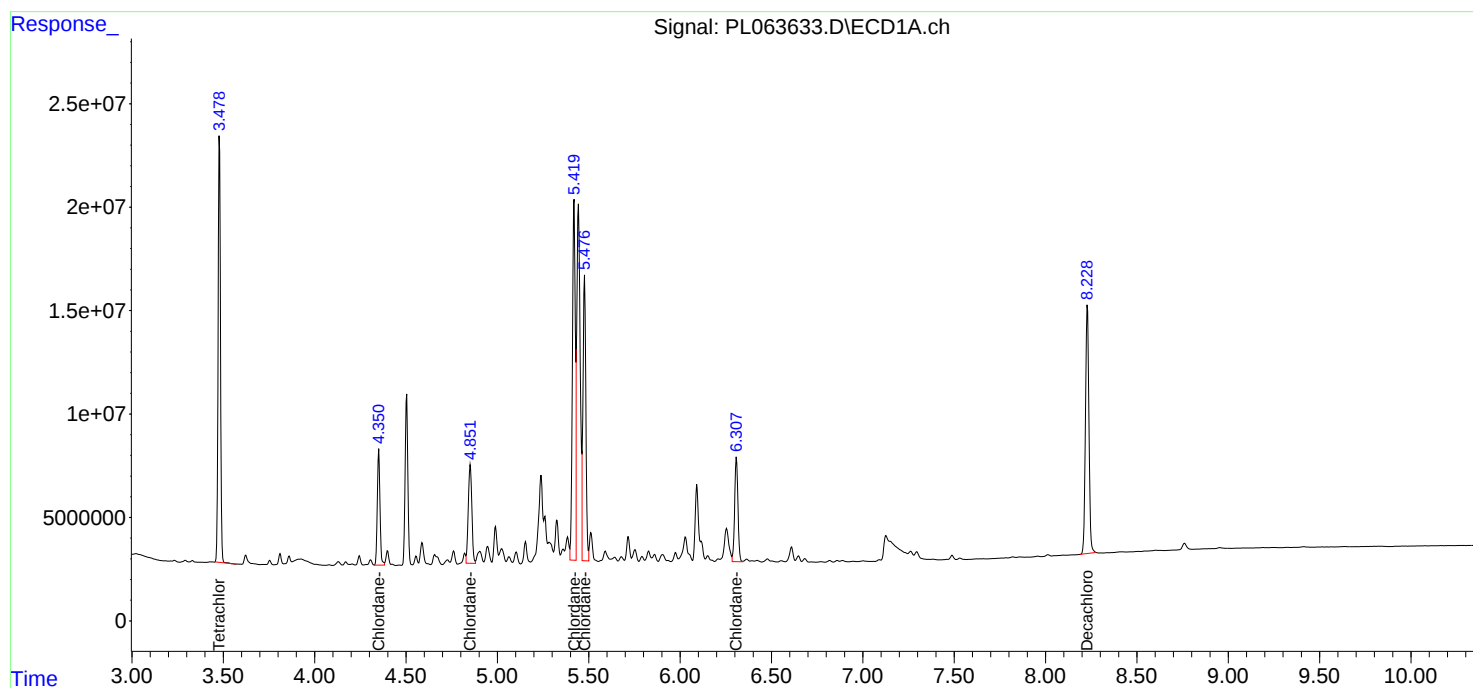


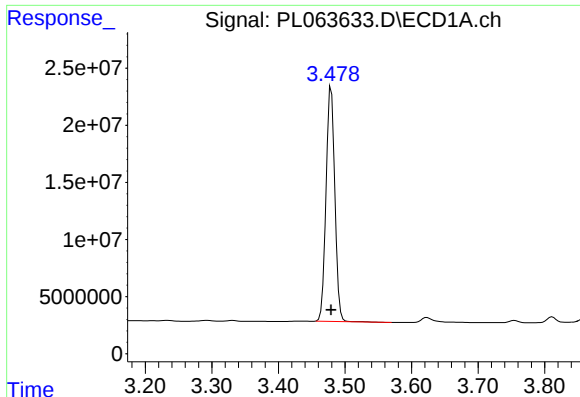

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 187835974
Conc: 78.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

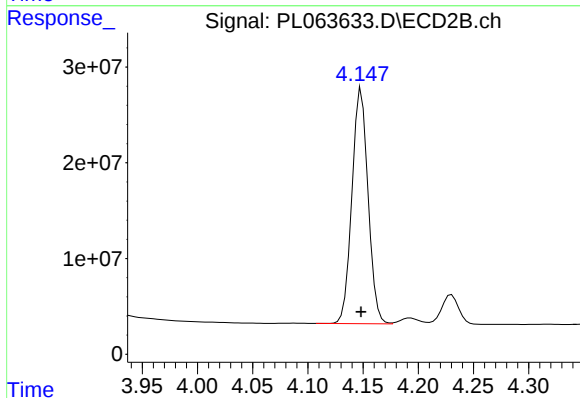


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 249716345
Conc: 76.61 ng/ml

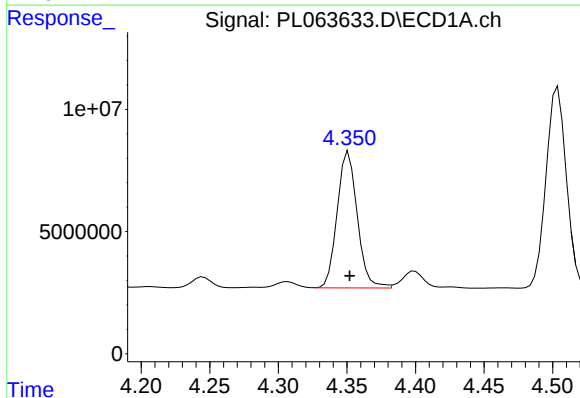


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 56985649
Conc: 750.91 ng/ml

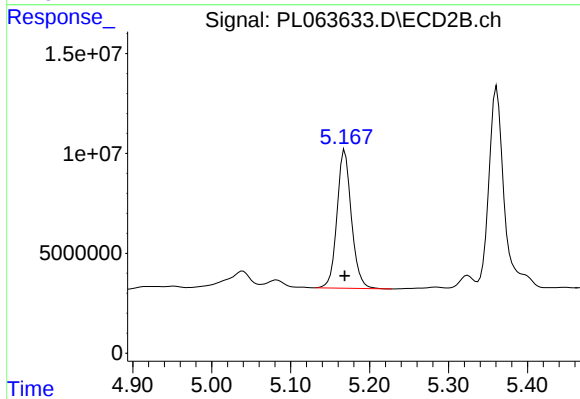

#23 Chlordane-1


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 87867348
Conc: 753.67 ng/ml

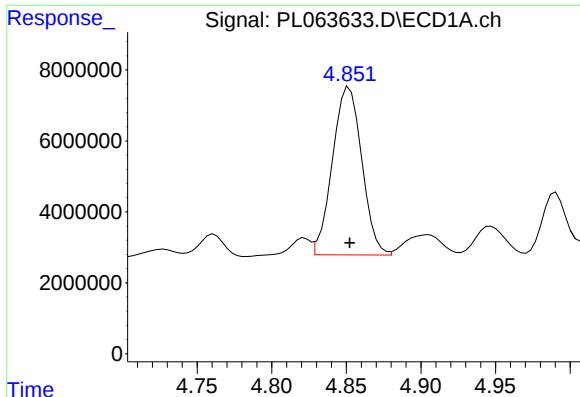

#24 Chlordane-2


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 65005506
Conc: 737.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

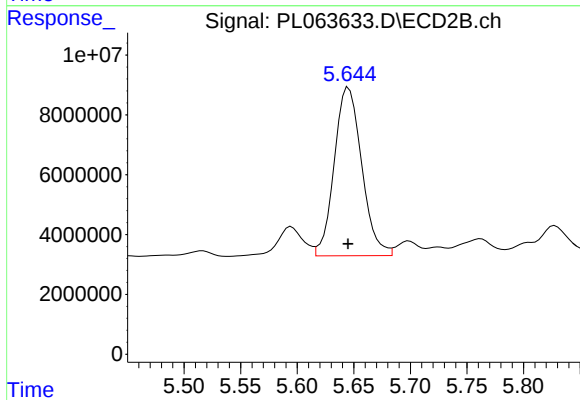


#24 Chlordane-2

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 95149694
Conc: 748.45 ng/ml

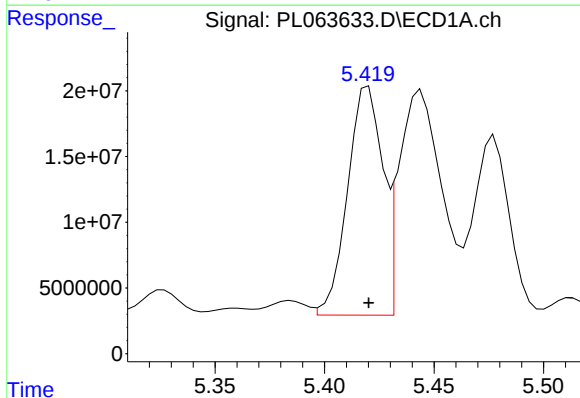


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 193828992
Conc: 792.13 ng/ml

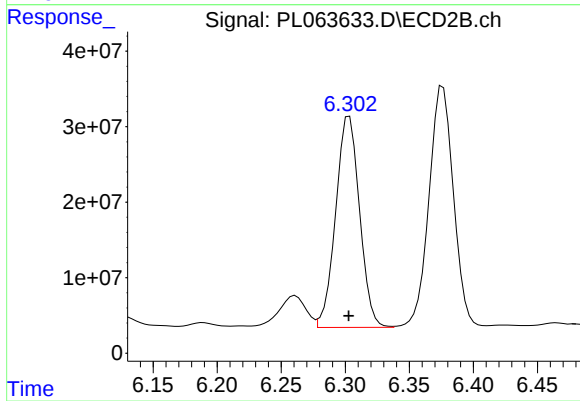

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 362658109
Conc: 772.13 ng/ml

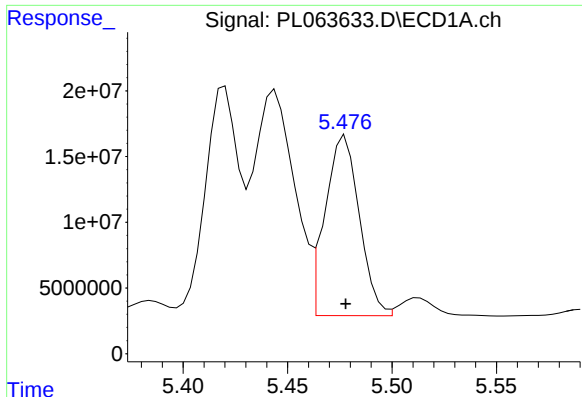

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 155781867
Conc: 763.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

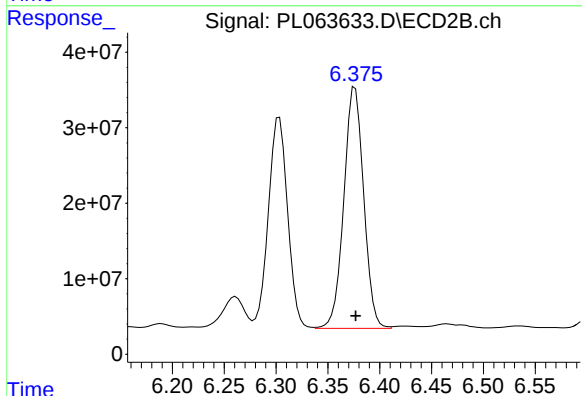


#26 Chlordane-4

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 425838611
Conc: 764.86 ng/ml

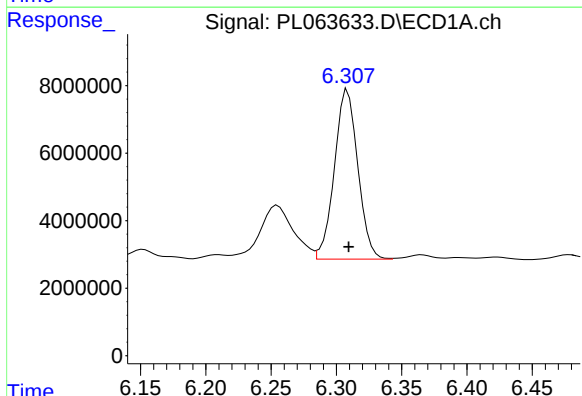


#27 Chlordane-5

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 62695395
Conc: 770.00 ng/ml

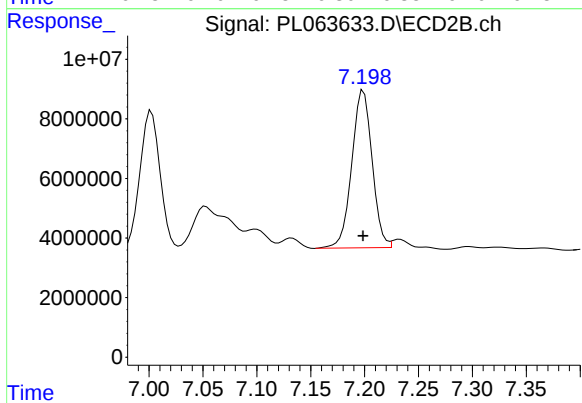

#27 Chlordane-5


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 69637962
Conc: 823.96 ng/ml

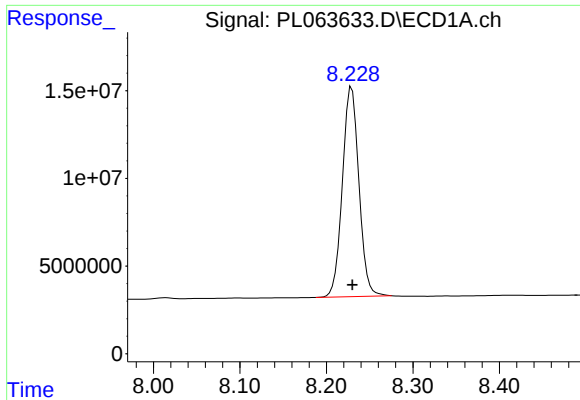

#28 Decachlorobiphenyl

R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 158075769
Conc: 74.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

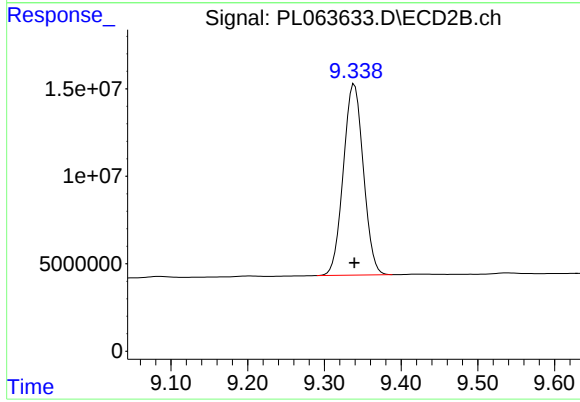

#28 Decachlorobiphenyl

R.T.: 9.339 min
Delta R.T.: 0.000 min
Response: 199447494
Conc: 75.68 ng/ml