

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
 Data File : PL063634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 03:36
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 07:58:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 07:58:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.148	120.2E6	163.0E6	50.000	50.000
28)	SA Decachlor...	8.230	9.339	106.5E6	131.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.352	5.168	37944487	58292986	500.000	500.000
24)	Chlordane-2	4.852	5.645	44067759	63564607	500.000	500.000
25)	Chlordane-3	5.420	6.303	122.3E6	234.8E6	500.000	500.000
26)	Chlordane-4	5.478	6.377	102.1E6	278.4E6	500.000	500.000
27)	Chlordane-5	6.310	7.199	40711349	42257842	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
Data File : PL063634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 03:36
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 07:58:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 07:58:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

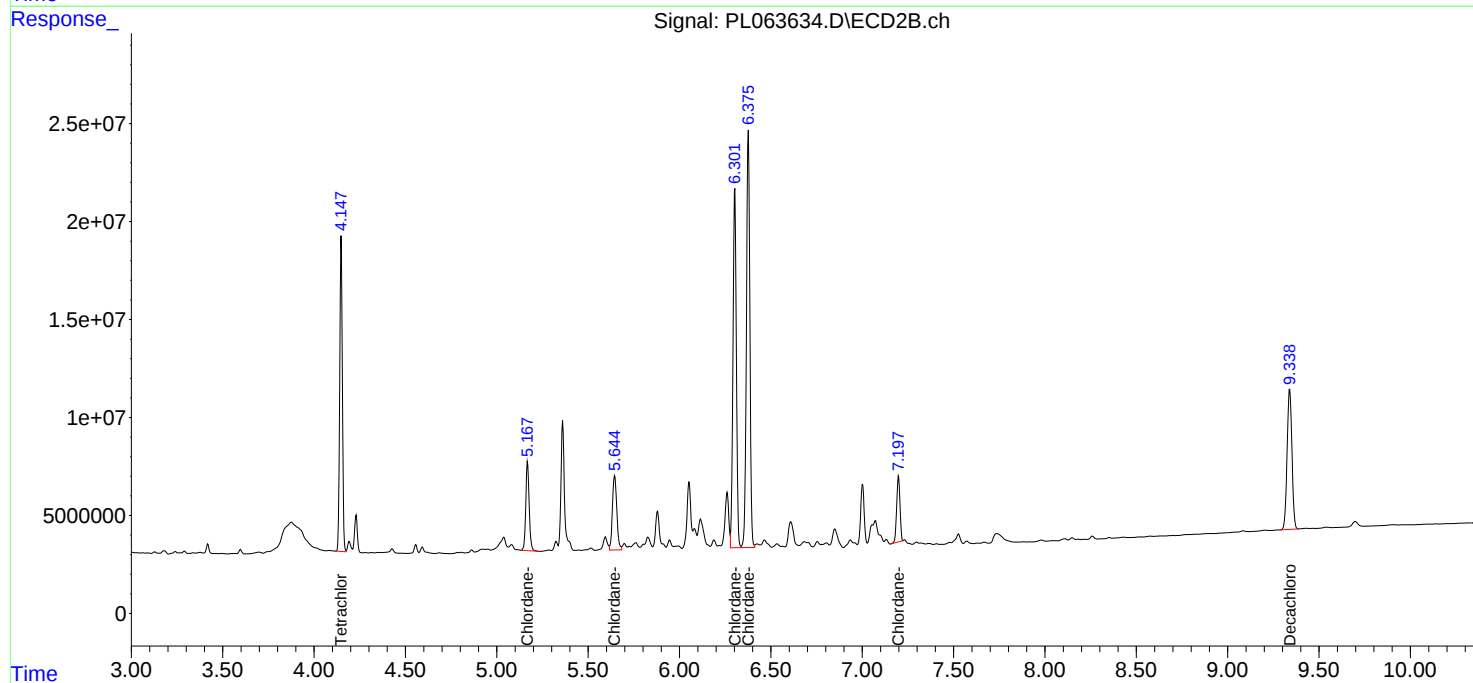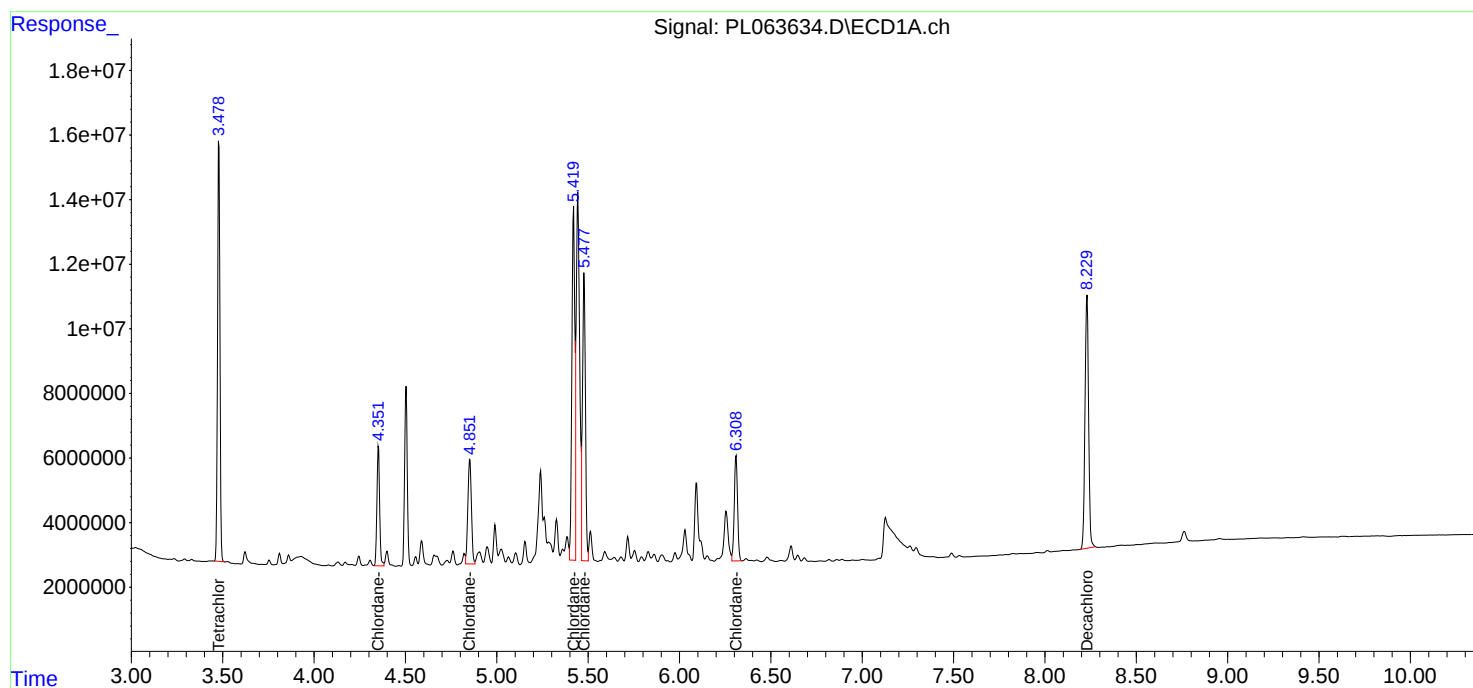


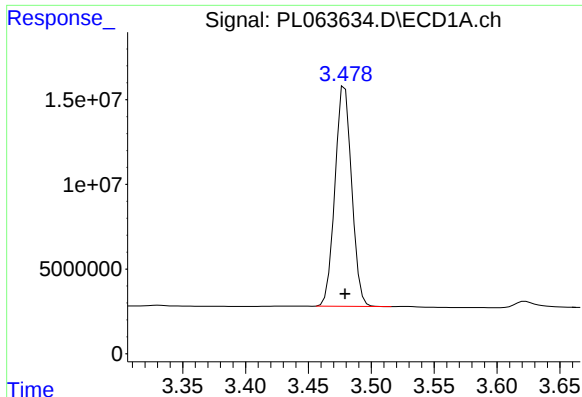

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 120230677
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

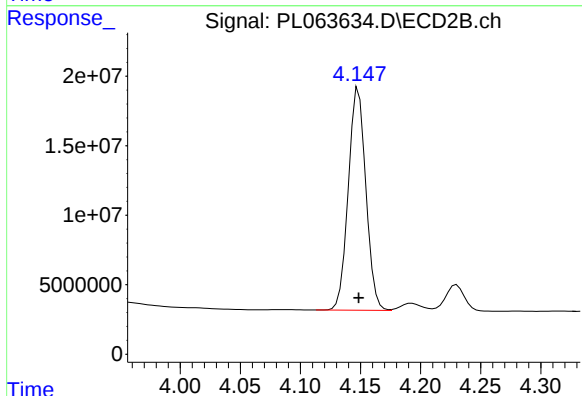


#1 Tetrachloro-m-xylene

R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 162970635
Conc: 50.00 ng/ml

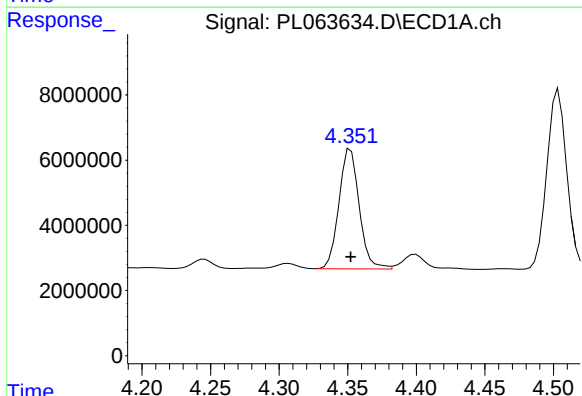


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 37944487
Conc: 500.00 ng/ml

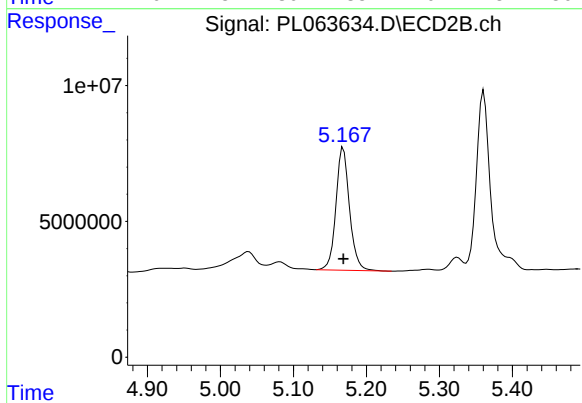

#23 Chlordane-1


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 58292986
Conc: 500.00 ng/ml

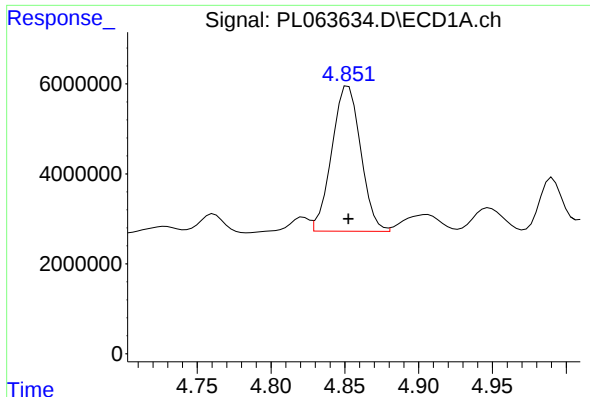

#24 Chlordane-2


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 44067759
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

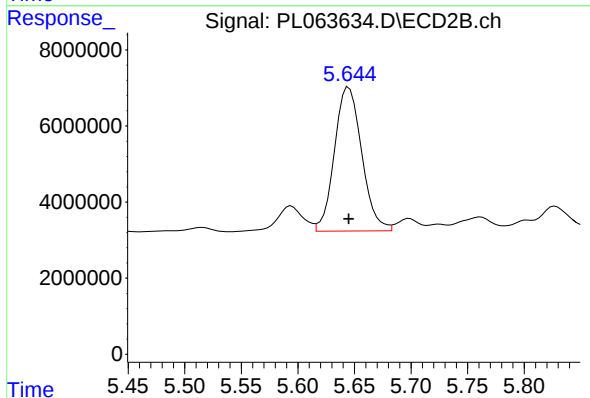


#24 Chlordane-2

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 63564607
Conc: 500.00 ng/ml

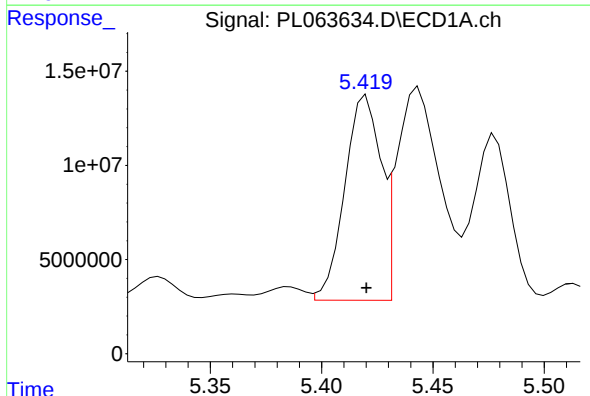


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 122346029
Conc: 500.00 ng/ml

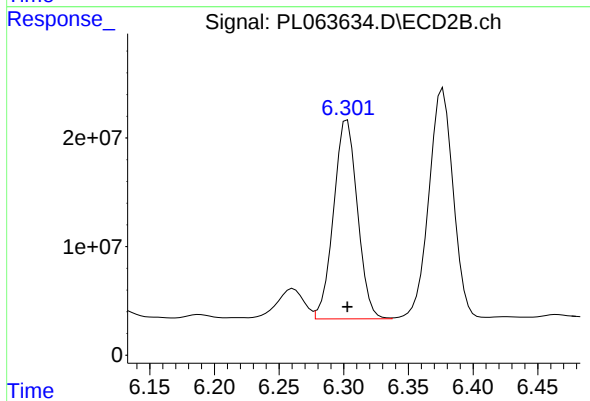

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 234841826
Conc: 500.00 ng/ml

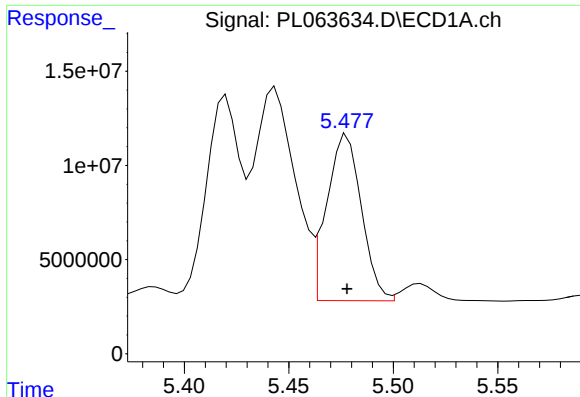

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 102082853
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

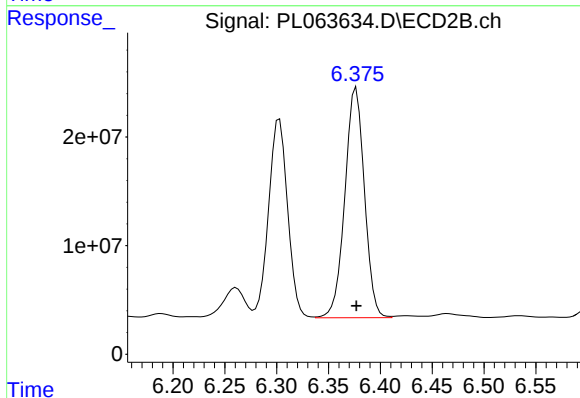


#26 Chlordane-4

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 278377436
Conc: 500.00 ng/ml

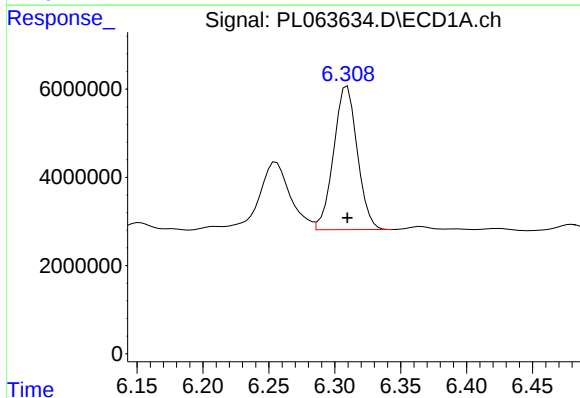


#27 Chlordane-5

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 40711349
Conc: 500.00 ng/ml

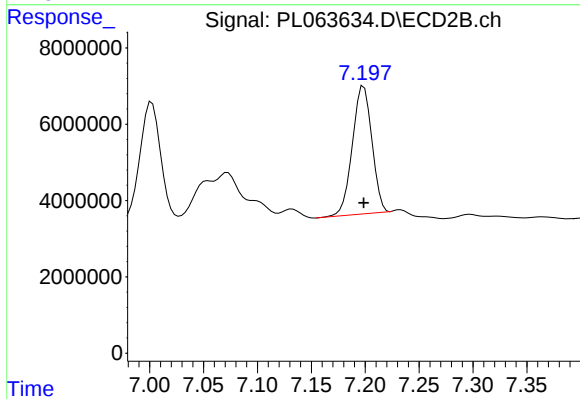

#27 Chlordane-5


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 42257842
Conc: 500.00 ng/ml

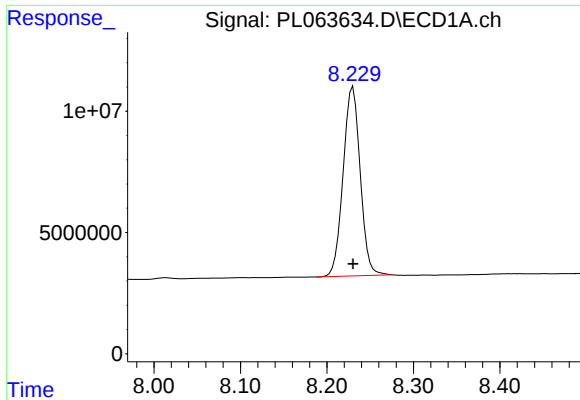

#28 Decachlorobiphenyl

R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 106457551
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

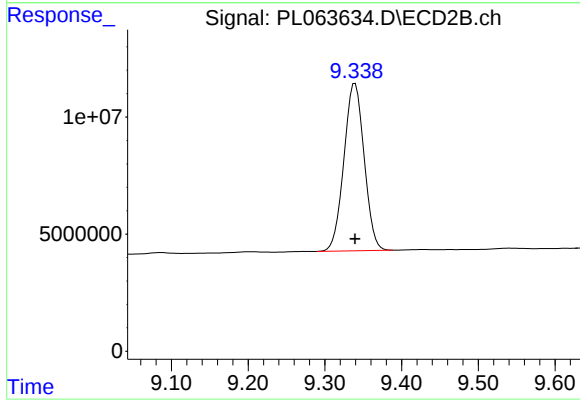

#28 Decachlorobiphenyl

R.T.: 9.339 min
Delta R.T.: 0.000 min
Response: 131768030
Conc: 50.00 ng/ml