

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
 Data File : PL063643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 05:50
 Operator : DD\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL121620CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 09:37:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 09:36:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.148	123.7E6	170.4E6	51.449	52.606
28)	SA Decachlor...	8.227	9.339	110.1E6	136.6E6	49.100	51.528
Target Compounds							
23)	Chlordane-1	4.351	5.168	38813968	61310882	516.262	527.715
24)	Chlordane-2	4.851	5.645	45234659	66844290	513.777	536.329
25)	Chlordane-3	5.419	6.303	126.5E6	245.4E6	514.230	530.686
26)	Chlordane-4	5.477	6.376	105.6E6	290.1E6	520.365	529.176
27)	Chlordane-5	6.309	7.199	42707082	44115385	508.410	506.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121620\
Data File : PL063643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 05:50
Operator : DD\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL121620CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 09:37:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 09:36:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

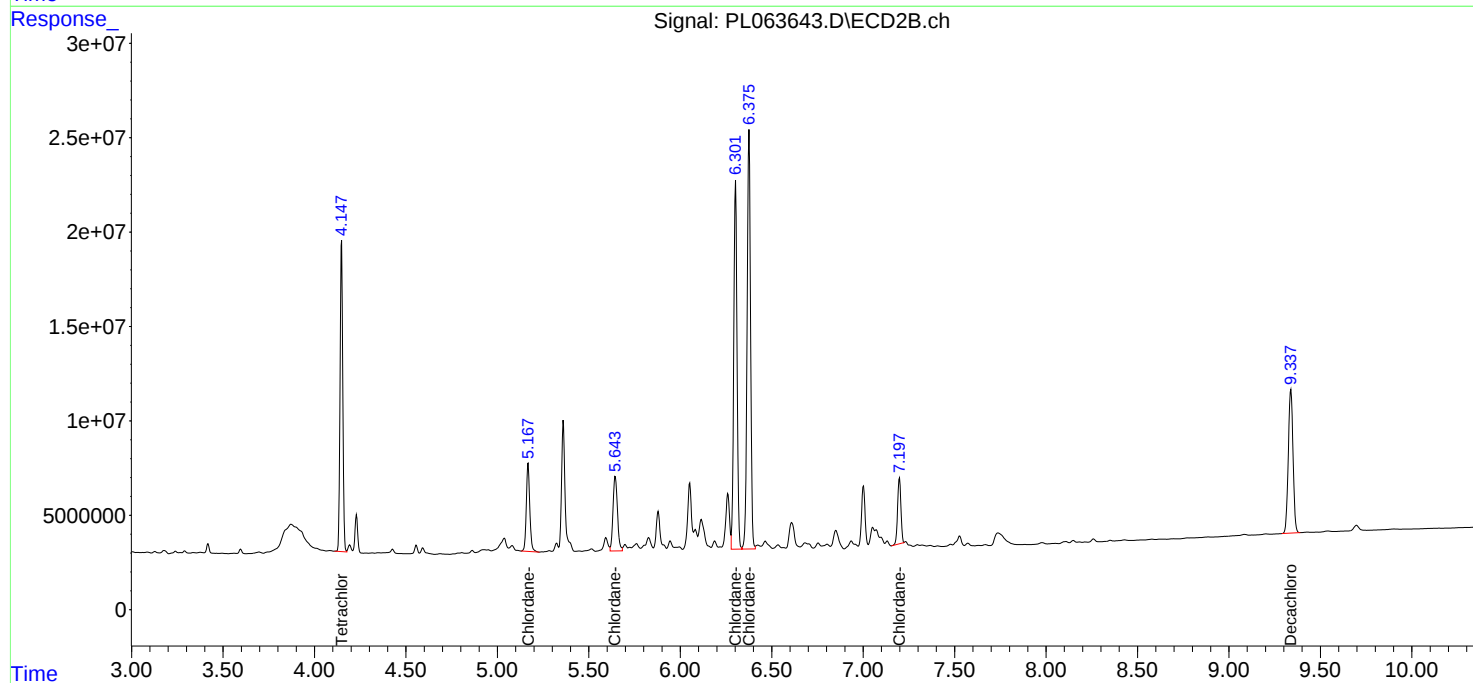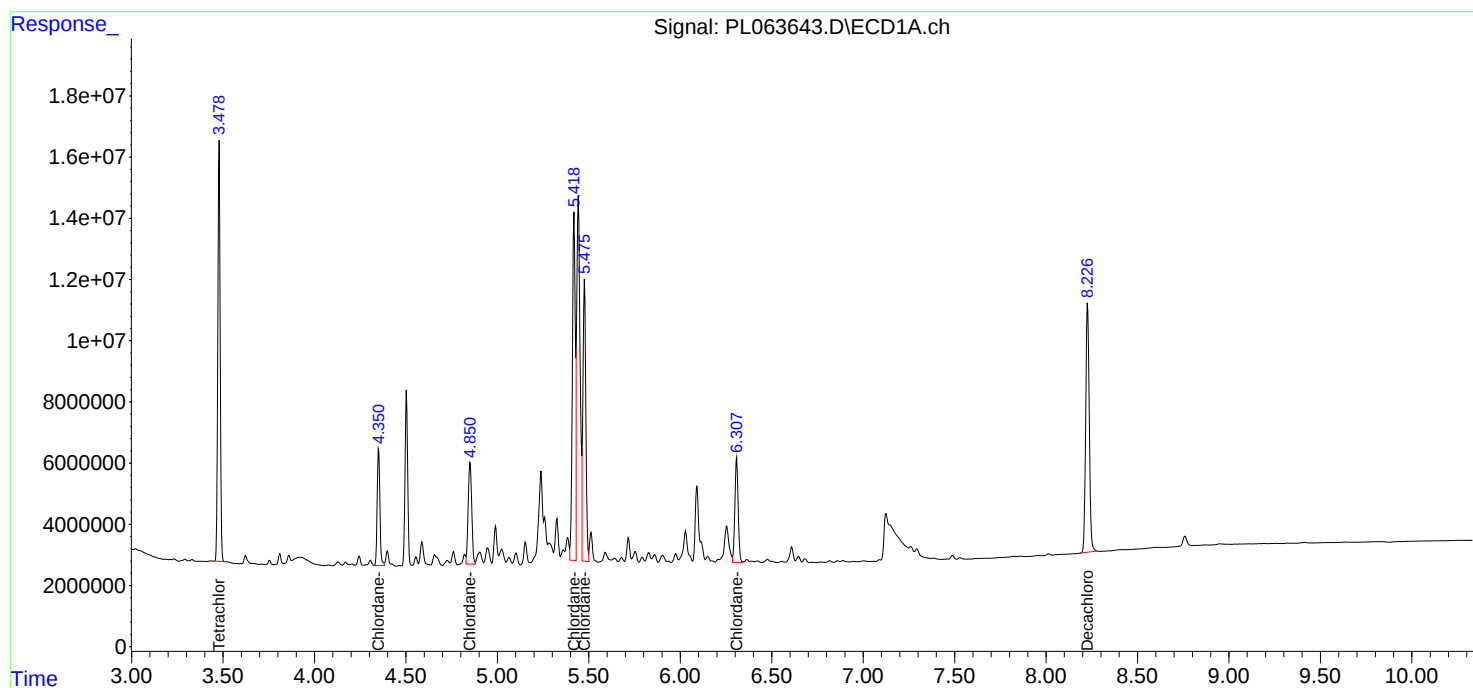


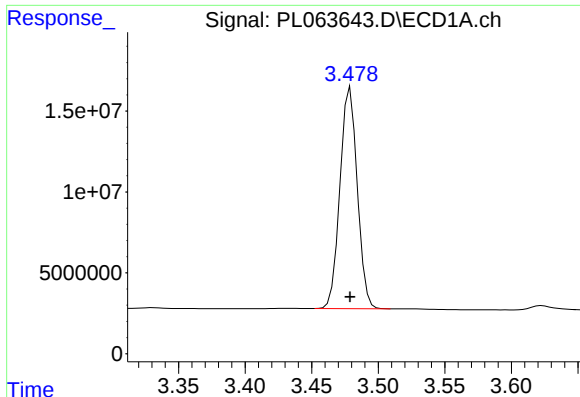

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 123661364
Conc: 51.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121620CHLOR

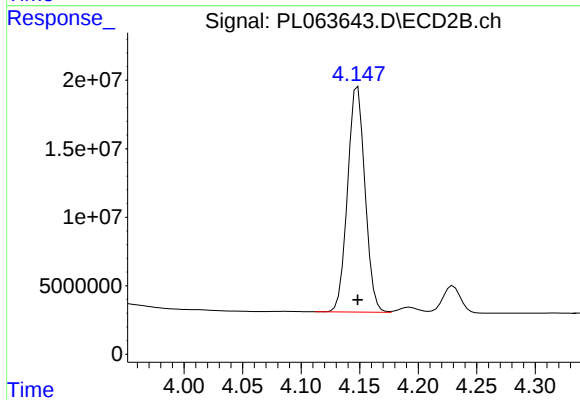


#1 Tetrachloro-m-xylene

R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 170412143
Conc: 52.61 ng/ml

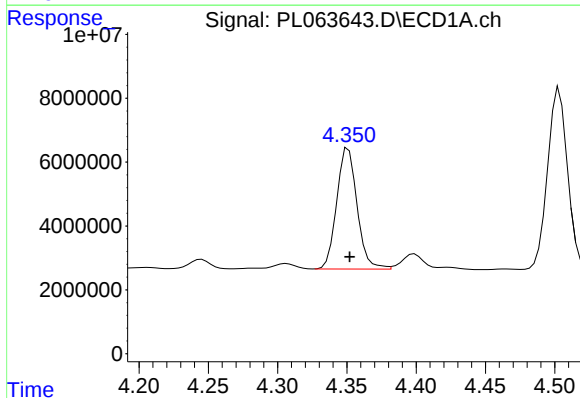


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: -0.001 min
Response: 38813968
Conc: 516.26 ng/ml

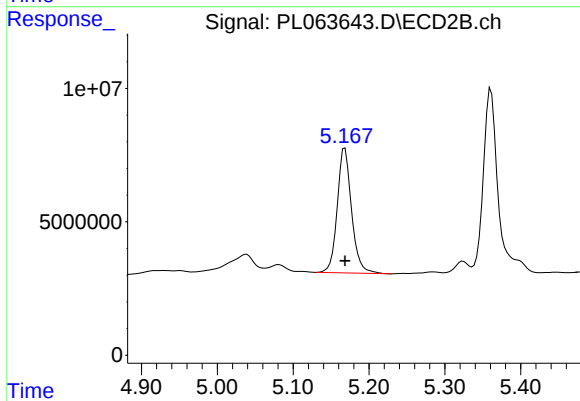

#23 Chlordane-1


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 61310882
Conc: 527.72 ng/ml

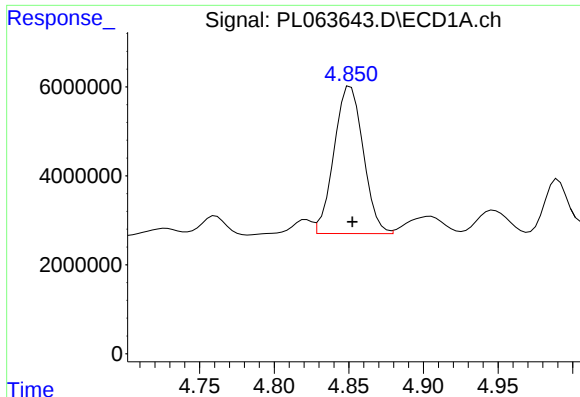

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: -0.001 min
Response: 45234659
Conc: 513.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121620CHLOR

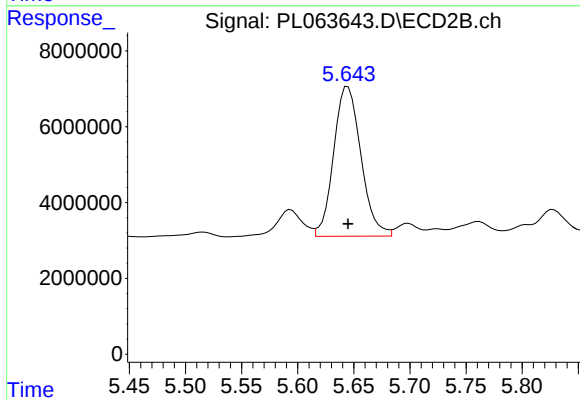


#24 Chlordane-2

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 66844290
Conc: 536.33 ng/ml

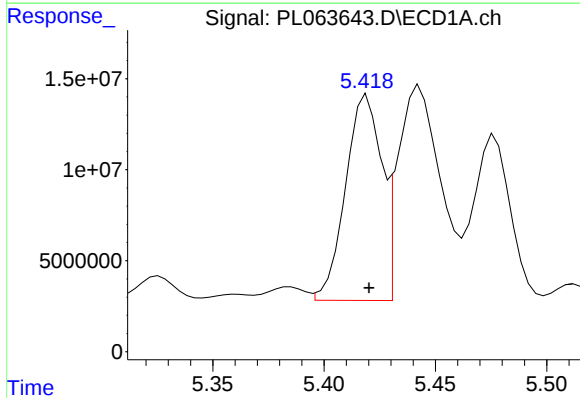


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.000 min
Response: 126498888
Conc: 514.23 ng/ml

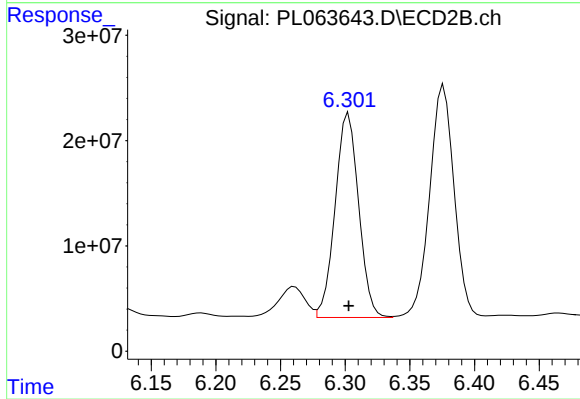

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 245353141
Conc: 530.69 ng/ml

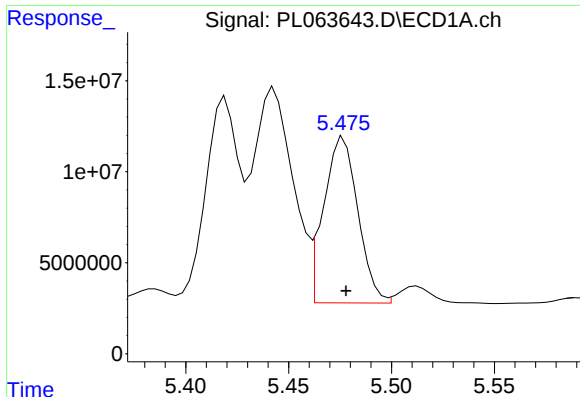

#26 Chlordane-4


R.T.: 5.477 min
Delta R.T.: -0.001 min
Response: 105565071
Conc: 520.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121620CHLOR

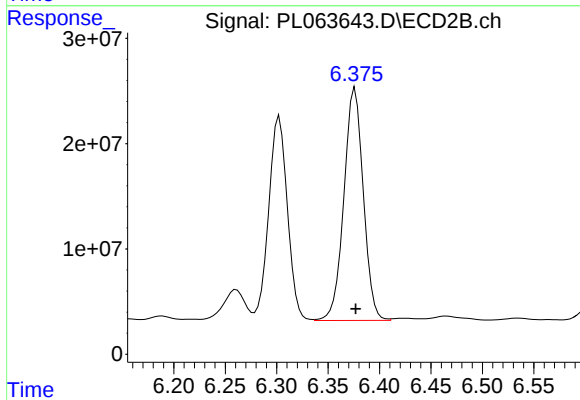


#26 Chlordane-4

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 290108380
Conc: 529.18 ng/ml

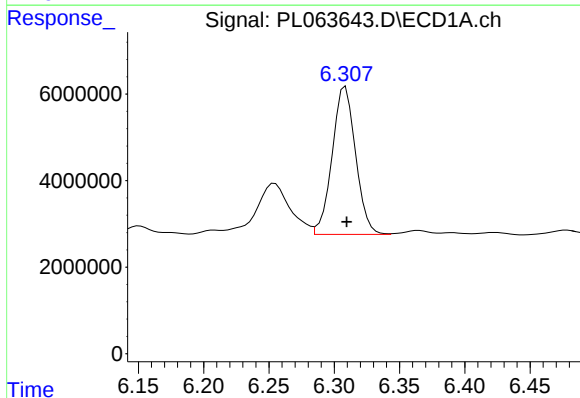


#27 Chlordane-5

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 42707082
Conc: 508.41 ng/ml

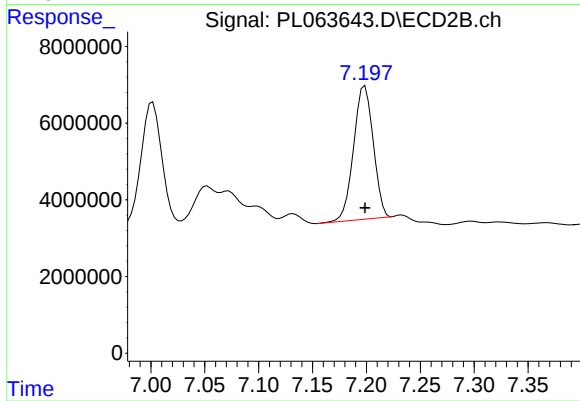

#27 Chlordane-5


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 44115385
Conc: 506.21 ng/ml

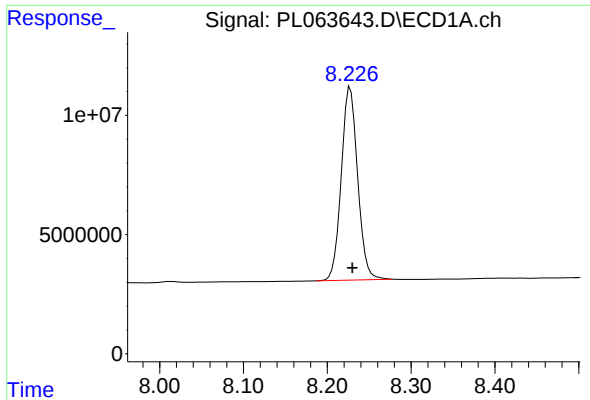

#28 Decachlorobiphenyl

R.T.: 8.227 min
Delta R.T.: -0.003 min
Response: 110072168
Conc: 49.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121620CHLOR

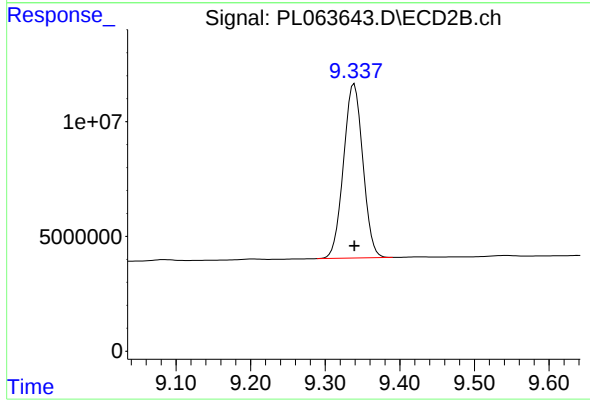

#28 Decachlorobiphenyl

R.T.: 9.339 min
Delta R.T.: 0.000 min
Response: 136638334
Conc: 51.53 ng/ml