

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121621\
 Data File : PL071475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2021 08:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 15:35:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	10.328	11.402f	241763	-60927	0.364	N.D. #
Target Compounds							
6)	B beta-BHC	6.051f	0.000	72205	0	0.253	N.D. #
7)	B delta-BHC	0.000	7.025f	0	579582	N.D.	0.379 #
9)	A Endosulfan I	0.000	8.341f	0	102415	N.D.	0.085 #
10)	B gamma-Chl...	0.000	8.235	0	73669	N.D.	0.057 #
11)	B alpha-Chl...	0.000	8.303	0	98188	N.D.	0.077 #
13)	MA Dieldrin	0.000	8.667f	0	969020	N.D.	0.797 #
14)	MA Endrin	0.000	8.895	0	861719	N.D.	0.851 #
16)	A 4,4'-DDD	0.000	9.016f	0	476038	N.D.	0.539 #
17)	MA 4,4'-DDT	0.000	9.376f	0	1209764	N.D.	1.223 #
18)	B Endrin al...	0.000	9.257	0	339031	N.D.	0.450 #
20)	A Methoxychlor	9.002	9.822f	475945	724124	1.469	1.443
22)	Mirex	0.000	10.459	0	1428557	N.D.	1.775 #
24)	Chlordane-2	0.000	7.456	0	58469	N.D.	1.240 #
25)	Chlordane-3	0.000	8.235	0	73669	N.D.	0.421 #
26)	Chlordane-4	0.000	8.303	0	98188	N.D.	0.468 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121621\
Data File : PL071475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2021 08:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 15:35:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

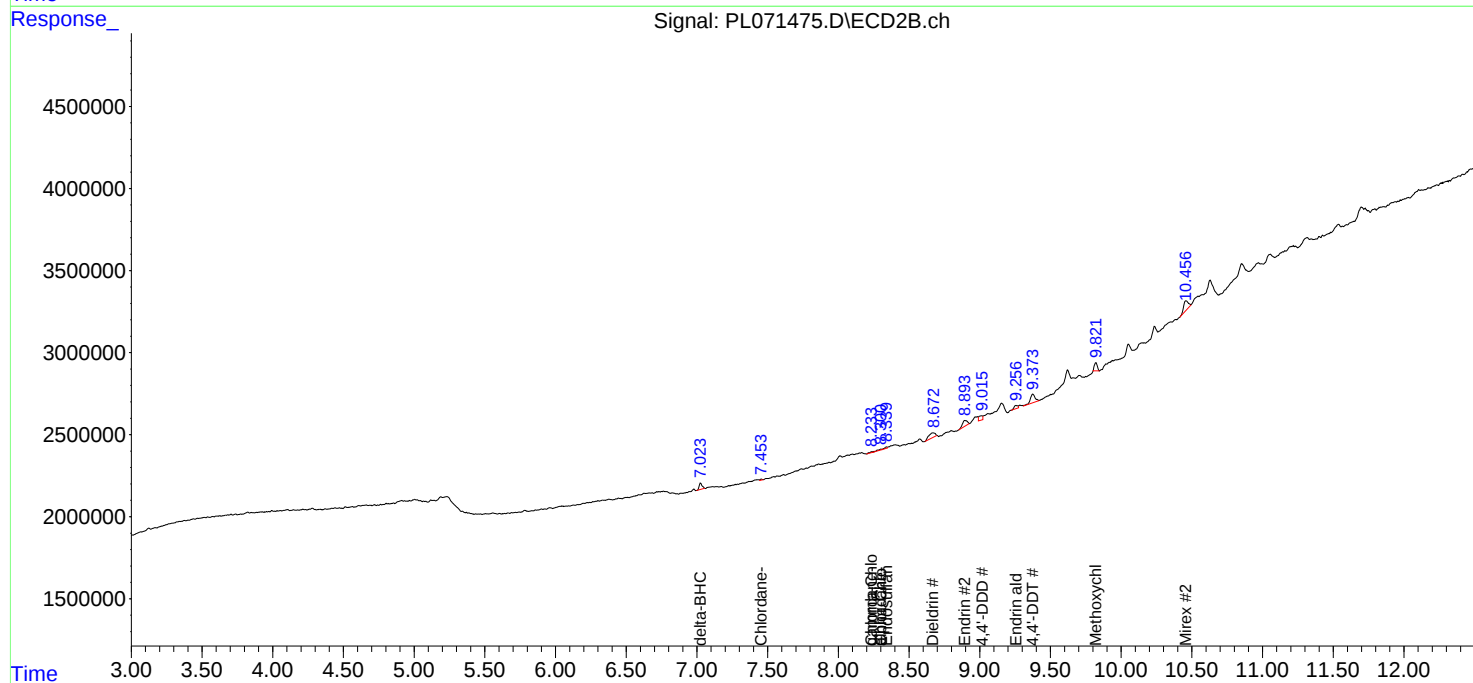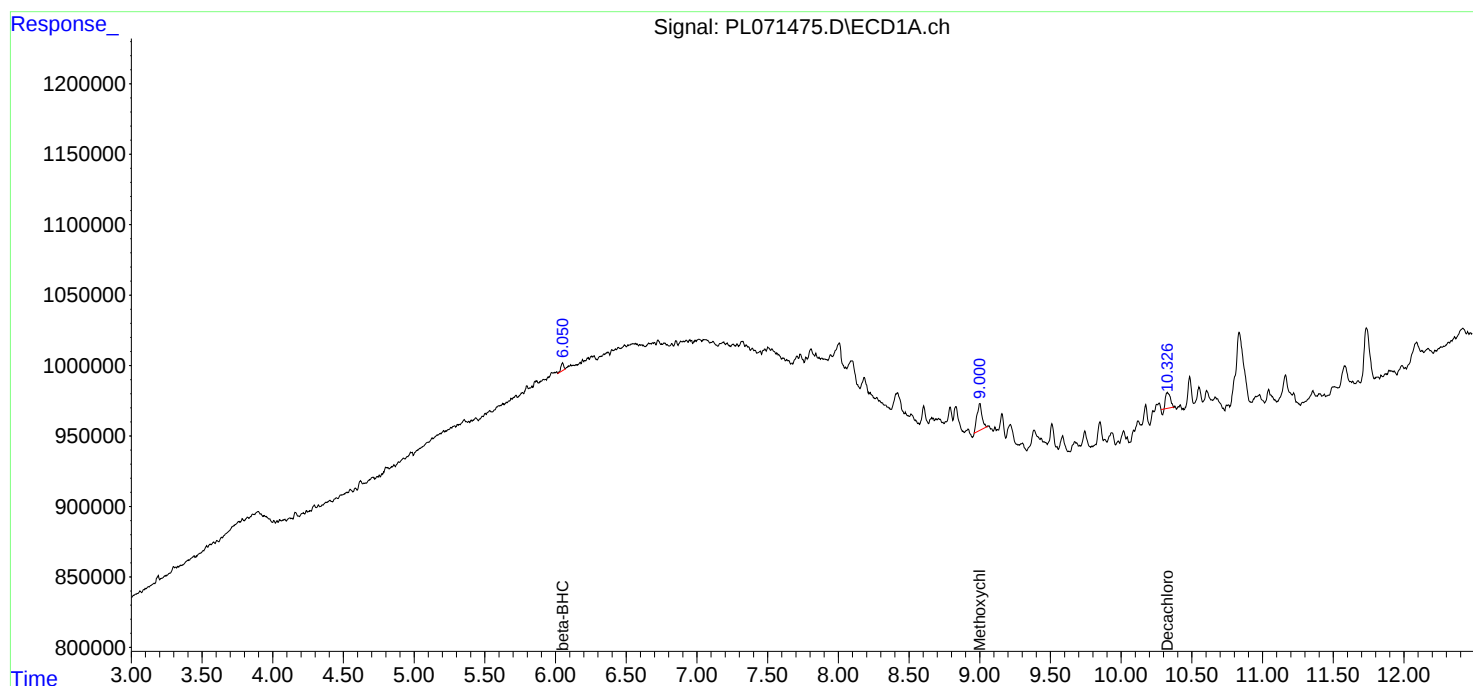


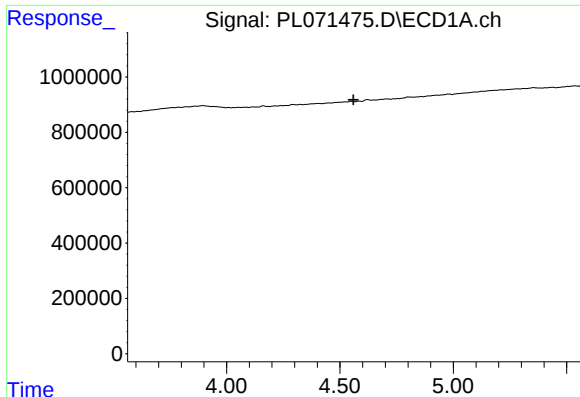

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

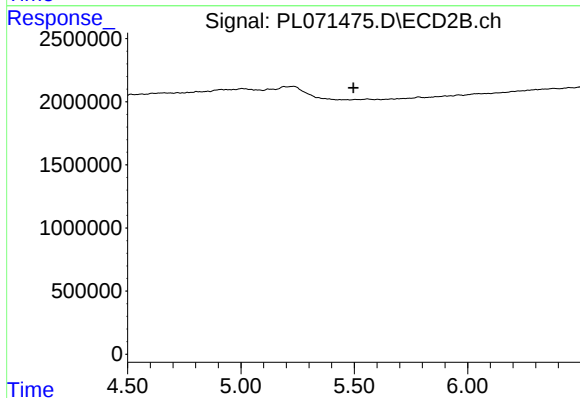


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

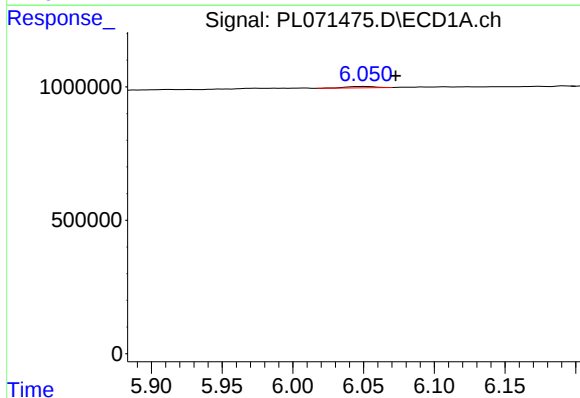


#6 beta-BHC

R.T.: 6.051 min
Delta R.T.: -0.022 min
Response: 72205
Conc: 0.25 ng/ml

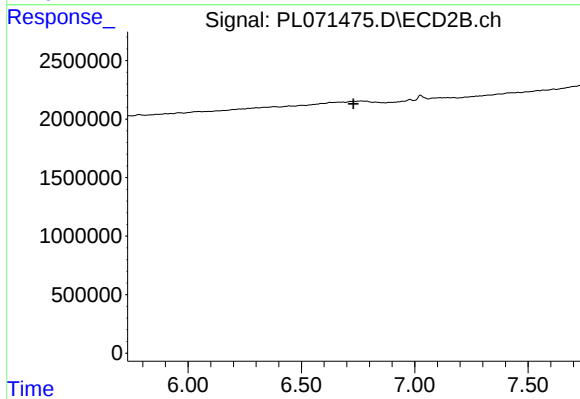

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.730 min
Response: 0
Conc: N.D.

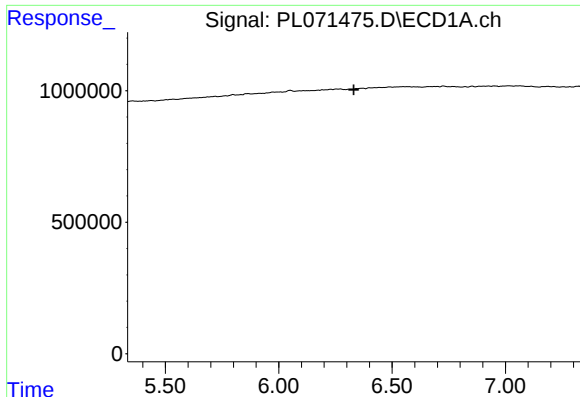

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

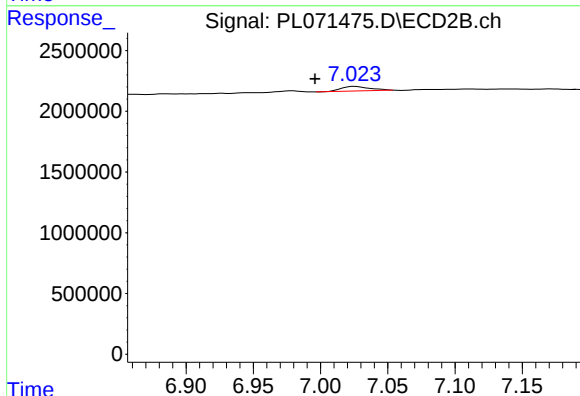


#7 delta-BHC

R.T.: 7.025 min
Delta R.T.: 0.029 min
Response: 579582
Conc: 0.38 ng/ml

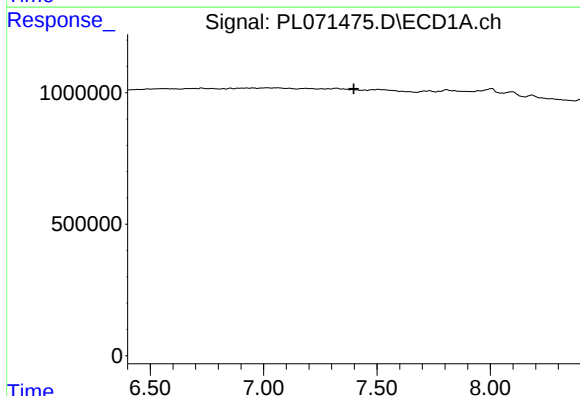


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

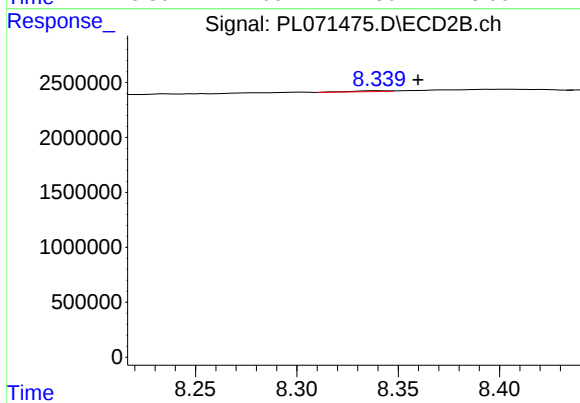

#9 Endosulfan I


R.T.: 8.341 min
Delta R.T.: -0.019 min
Response: 102415
Conc: 0.09 ng/ml

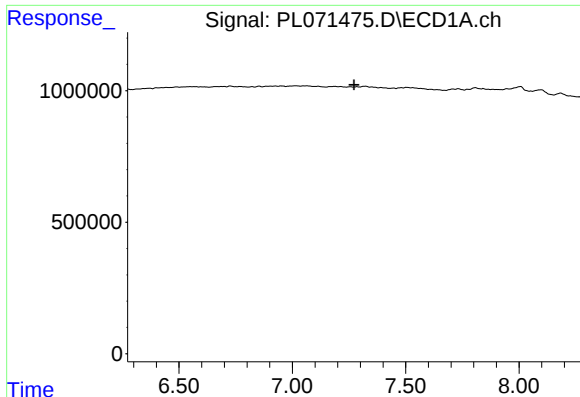

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

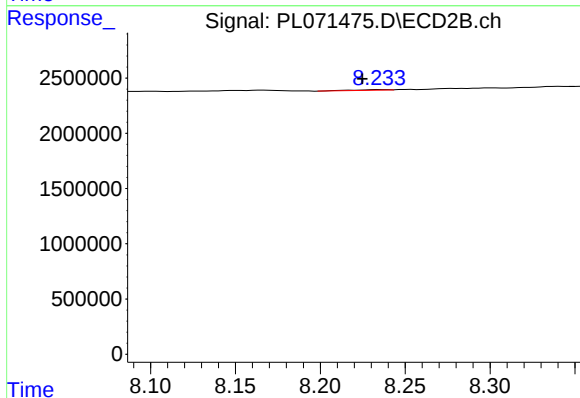


#10 gamma-Chlordane

R.T.: 8.235 min
Delta R.T.: 0.011 min
Response: 73669
Conc: 0.06 ng/ml

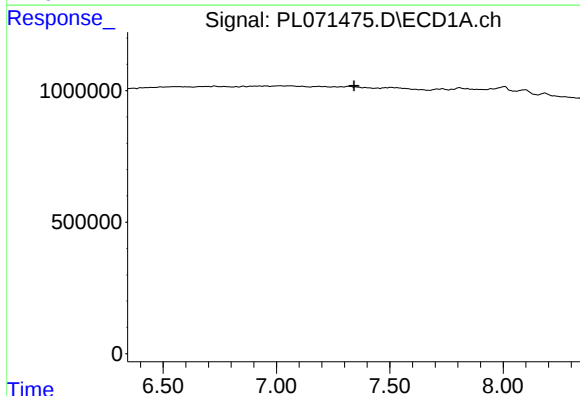


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

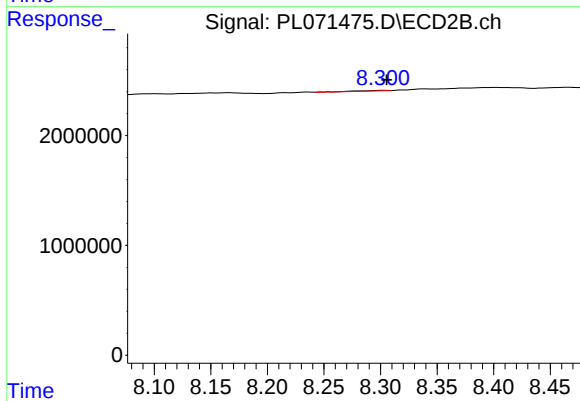

#11 alpha-Chlordane


R.T.: 8.303 min
Delta R.T.: -0.003 min
Response: 98188
Conc: 0.08 ng/ml

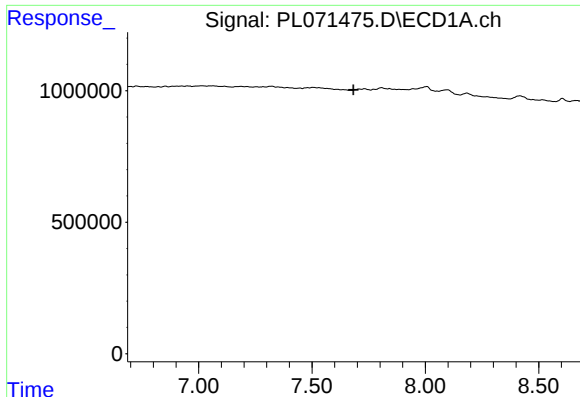

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

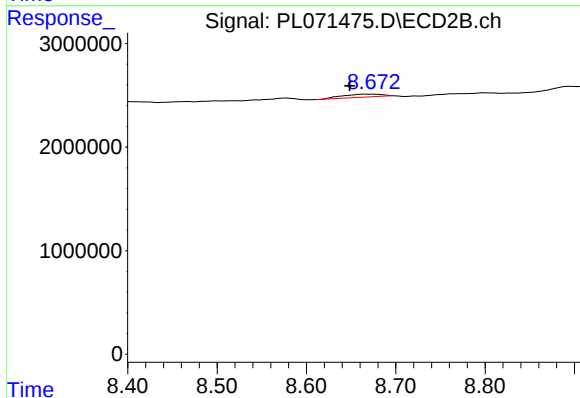


#13 Dieldrin

R.T.: 8.667 min
Delta R.T.: 0.019 min
Response: 969020
Conc: 0.80 ng/ml

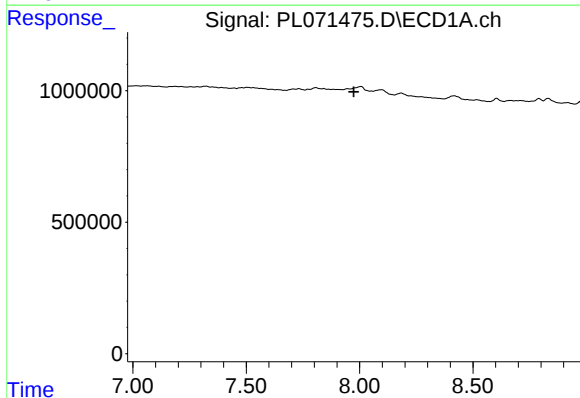


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

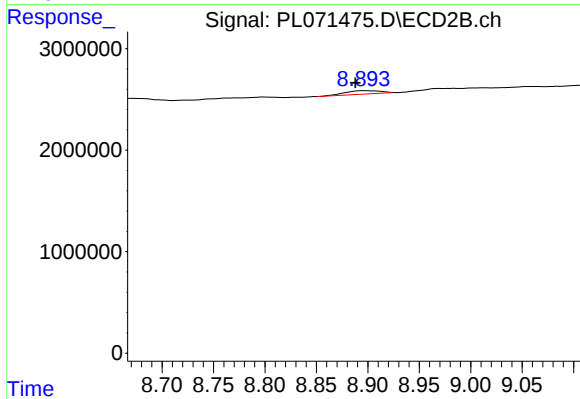

#14 Endrin


R.T.: 8.895 min
Delta R.T.: 0.007 min
Response: 861719
Conc: 0.85 ng/ml

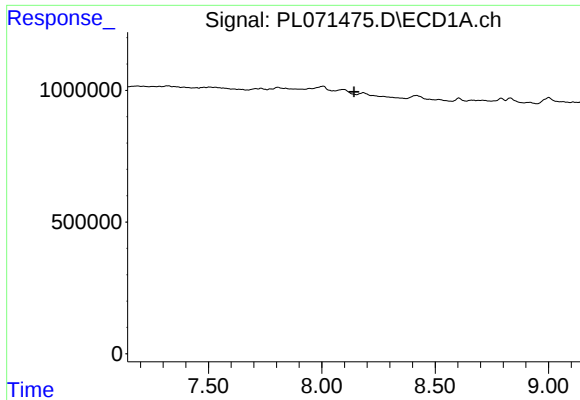

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

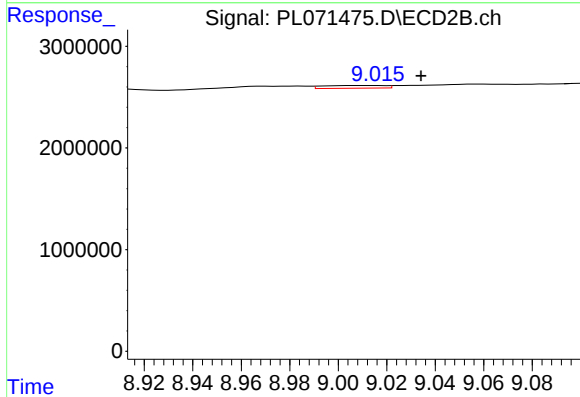


#16 4,4'-DDD

R.T.: 9.016 min
Delta R.T.: -0.018 min
Response: 476038
Conc: 0.54 ng/ml

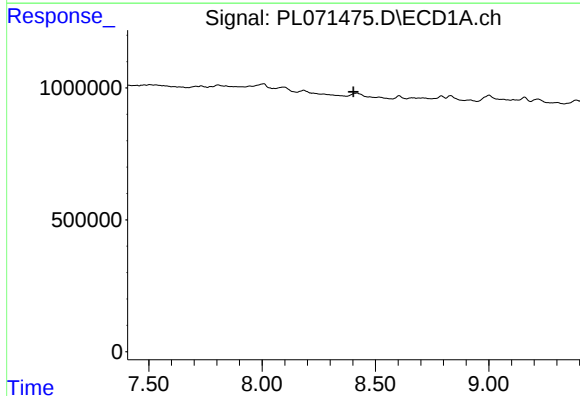


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.403 min
Response: 0
Conc: N.D.

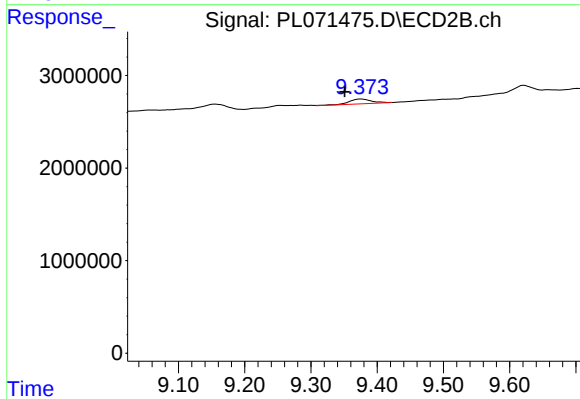

#17 4,4'-DDT


R.T.: 9.376 min
Delta R.T.: 0.025 min
Response: 1209764
Conc: 1.22 ng/ml

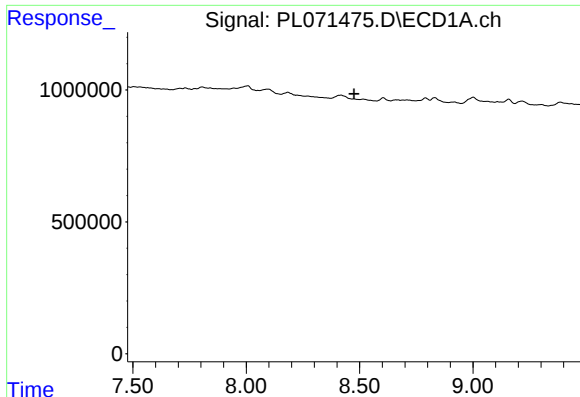

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

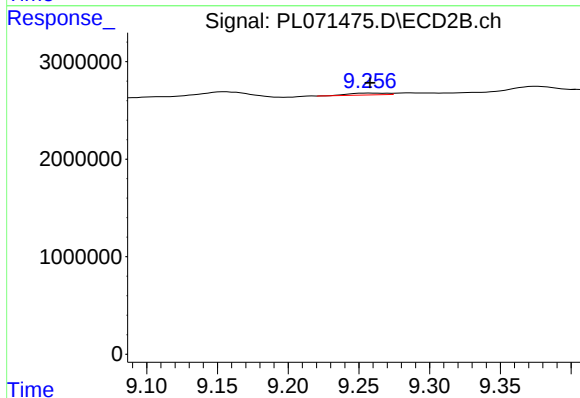


#18 Endrin aldehyde

R.T.: 9.257 min
Delta R.T.: -0.001 min
Response: 339031
Conc: 0.45 ng/ml

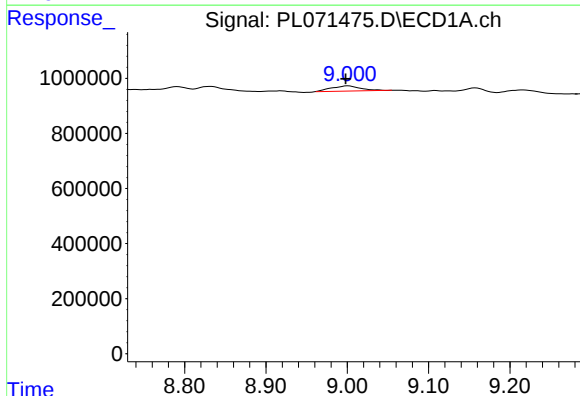


#20 Methoxychlor

R.T.: 9.002 min
Delta R.T.: 0.003 min
Response: 475945
Conc: 1.47 ng/ml

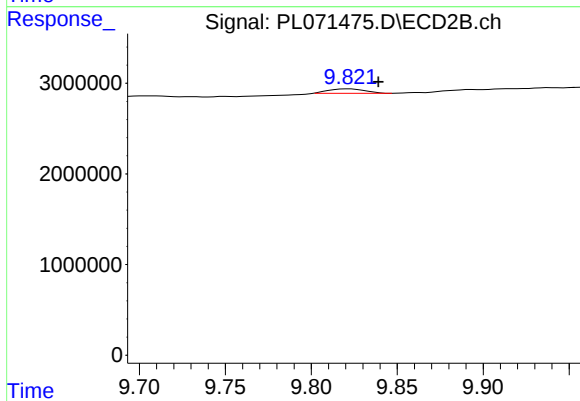

#20 Methoxychlor


R.T.: 9.822 min
Delta R.T.: -0.017 min
Response: 724124
Conc: 1.44 ng/ml

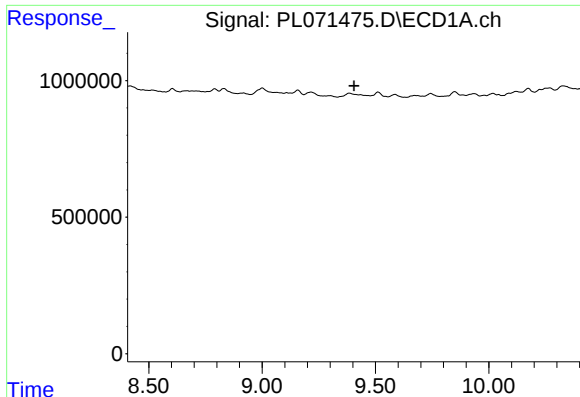

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

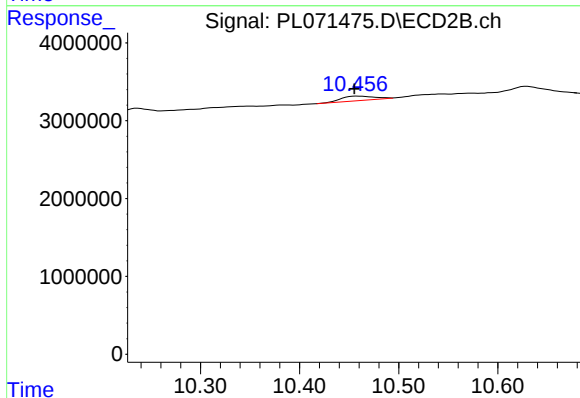


#22 Mirex

R.T.: 10.459 min
Delta R.T.: 0.003 min
Response: 1428557
Conc: 1.77 ng/ml

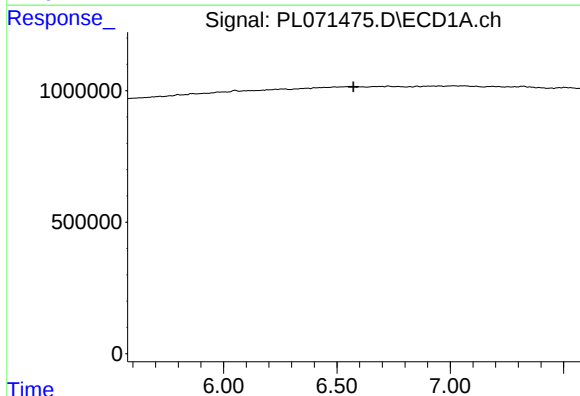


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

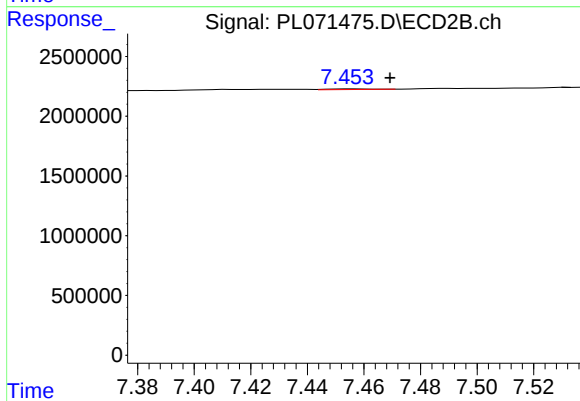

#24 Chlordane-2


R.T.: 7.456 min
Delta R.T.: -0.013 min
Response: 58469
Conc: 1.24 ng/ml

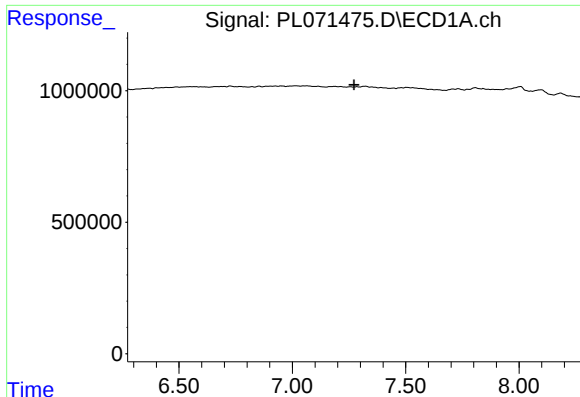

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

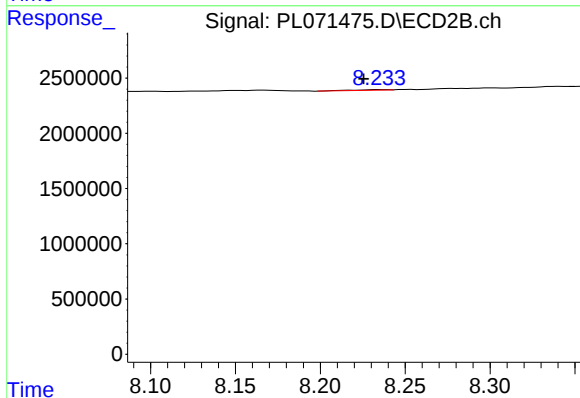


#25 Chlordane-3

R.T.: 8.235 min
Delta R.T.: 0.010 min
Response: 73669
Conc: 0.42 ng/ml

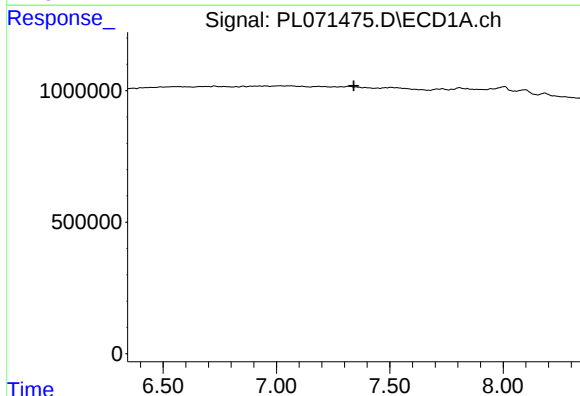


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

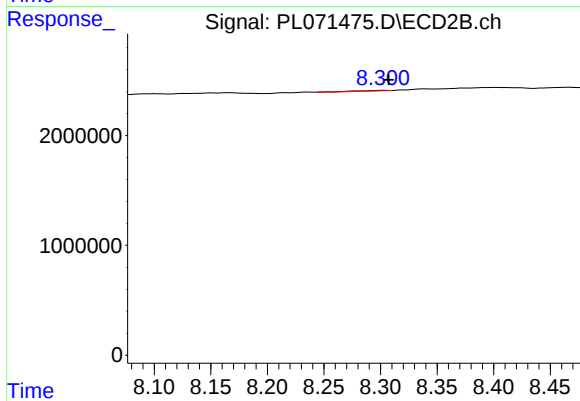

#26 Chlordane-4


R.T.: 8.303 min
Delta R.T.: -0.005 min
Response: 98188
Conc: 0.47 ng/ml

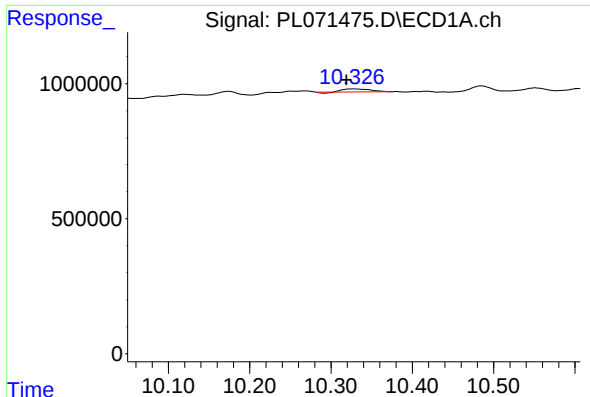

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.009 min
Response: 241763
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

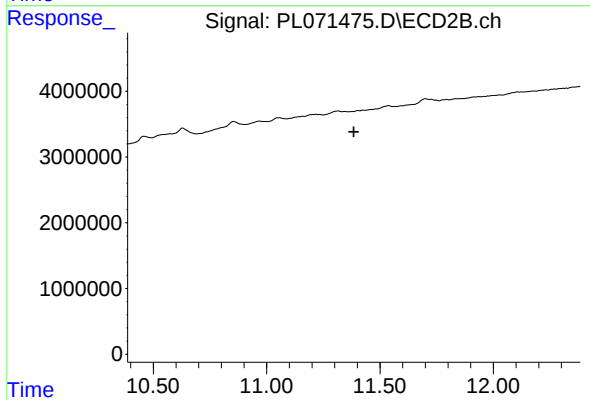

#28 Decachlorobiphenyl

R.T.: 11.402 min
Delta R.T.: 0.017 min
Response: -60927
Conc: N.D.