

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121621\
 Data File : PL071493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2021 16:20
 Operator : AR\AJ
 Sample : PB141480BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 16:58:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.500	9532159	25228751	20.110	21.177
28)	SA Decachlor...	10.326	11.393	14701159	25249726	22.127	23.240
Target Compounds							
7)	B delta-BHC	0.000	7.023f	0	2053571	N.D.	1.344 #
8)	B Heptachlo...	0.000	7.929f	0	279474	N.D.	0.208 #
10)	B gamma-Chl...	0.000	8.203f	0	36297	N.D.	0.028 #
11)	B alpha-Chl...	7.313f	0.000	561917	0	0.901	N.D. #
13)	MA Dieldrin	0.000	8.663	0	113449	N.D.	0.093 #
19)	B Endosulfa...	0.000	9.518f	0	101797	N.D.	0.104 #
20)	A Methoxychlor	0.000	9.844	0	98253	N.D.	0.196 #
21)	B Endrin ke...	0.000	10.007	0	41654	N.D.	0.040 #
24)	Chlordane-2	0.000	7.452f	0	287085	N.D.	6.088 #
25)	Chlordane-3	0.000	8.203f	0	36297	N.D.	0.207 #
26)	Chlordane-4	7.313f	0.000	561917	0	9.052	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121621\
Data File : PL071493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2021 16:20
Operator : AR\AJ
Sample : PB141480BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 16:58:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

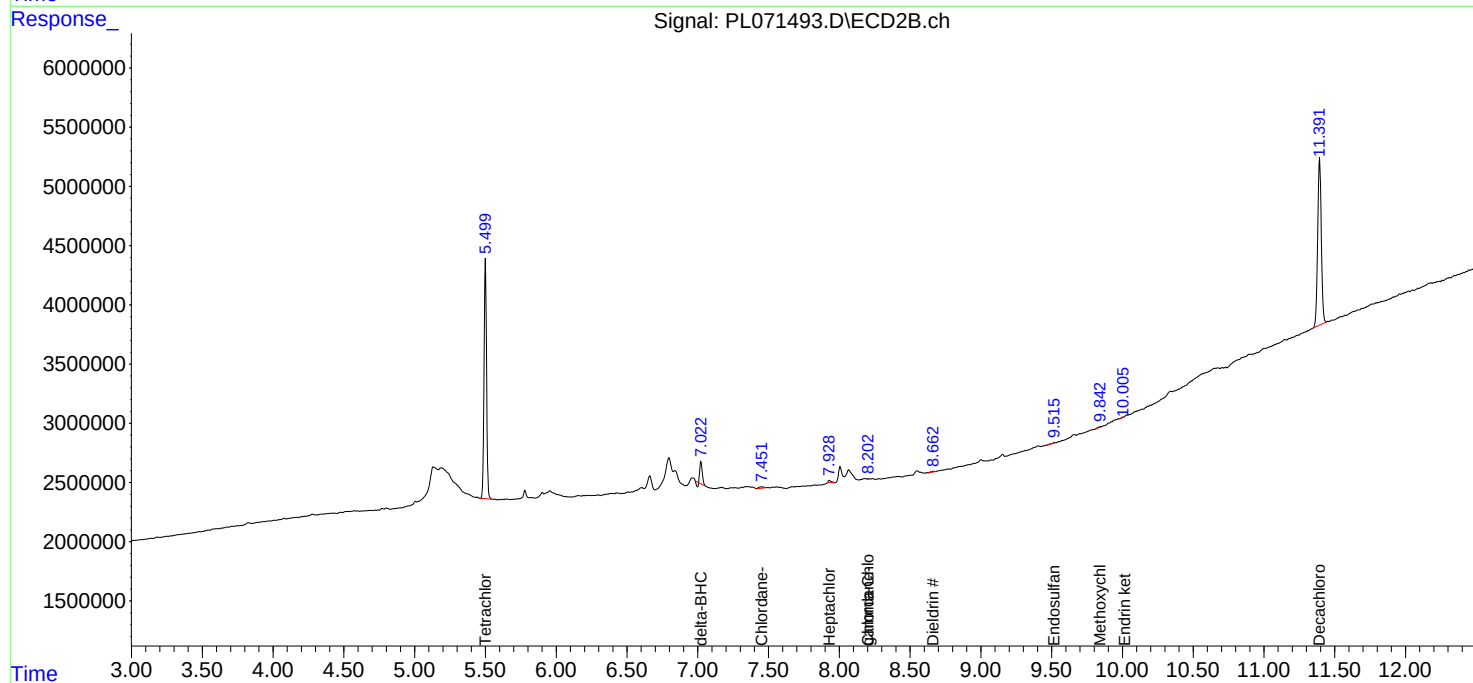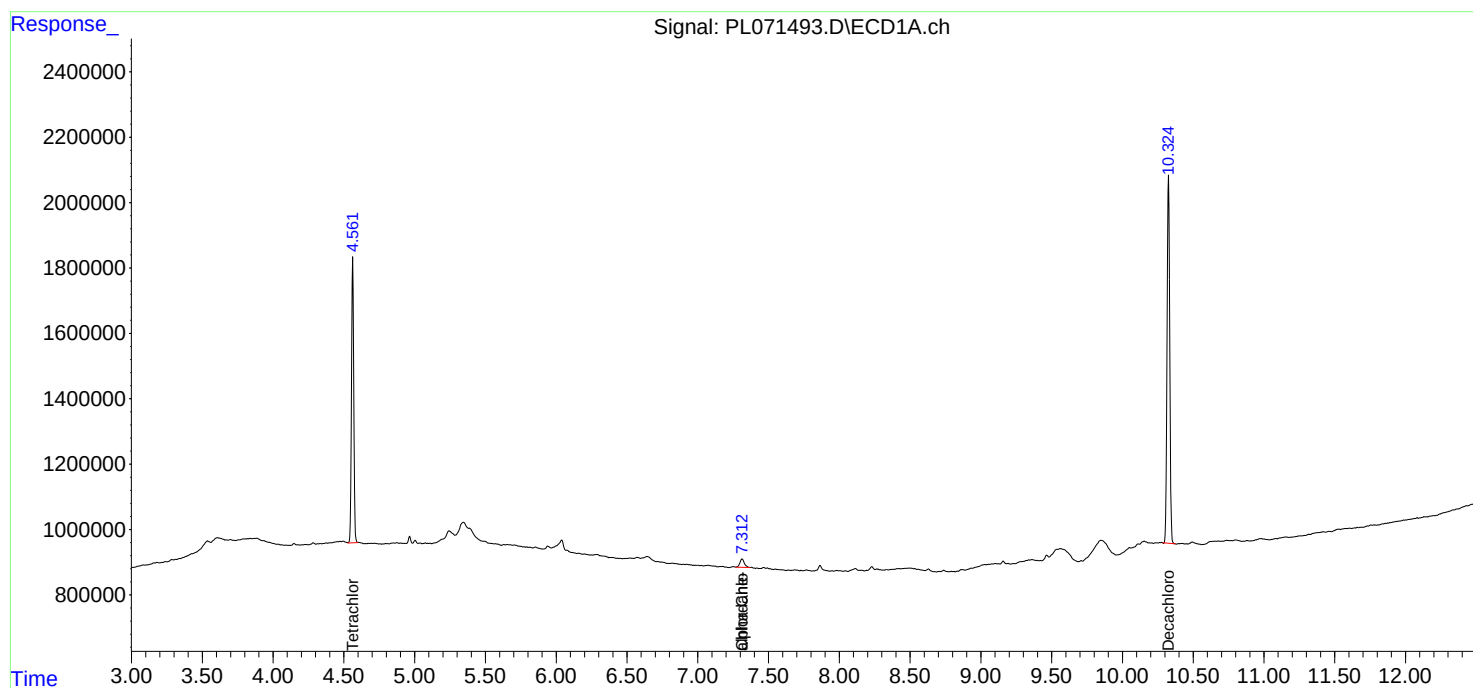


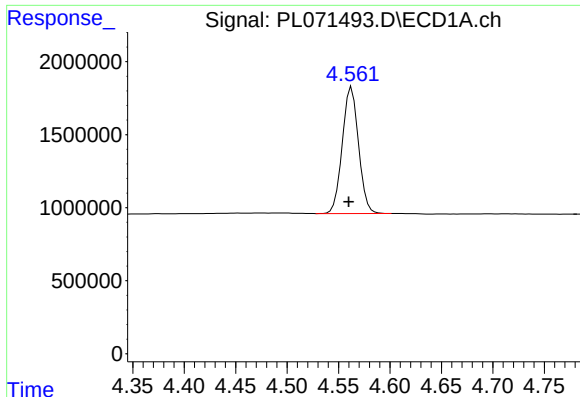

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.003 min
Response: 9532159
Conc: 20.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

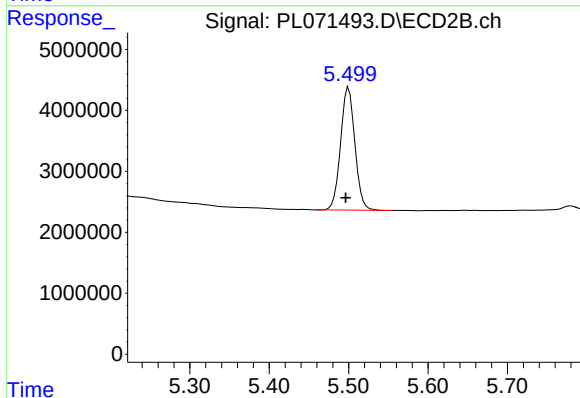


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.004 min
Response: 25228751
Conc: 21.18 ng/ml

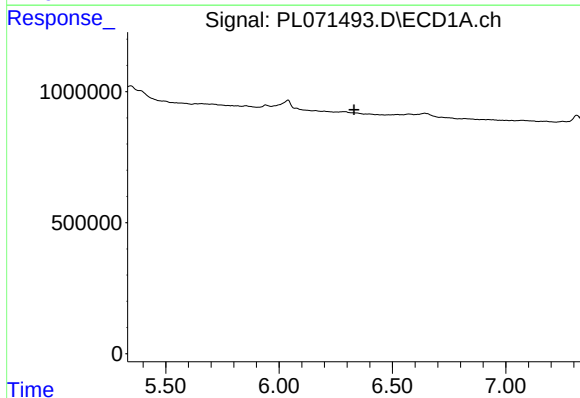


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

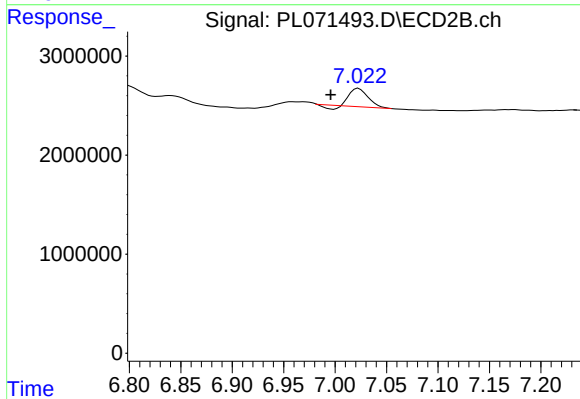

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.027 min
Response: 2053571
Conc: 1.34 ng/ml

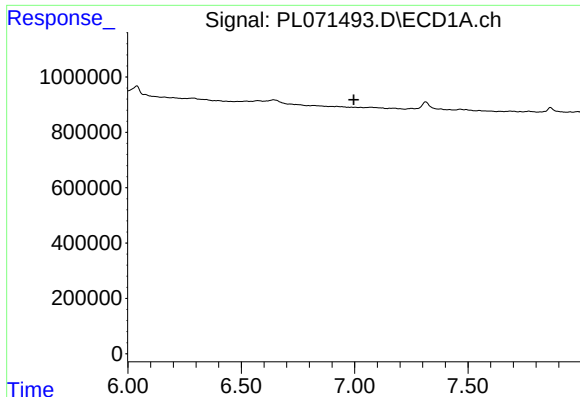

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

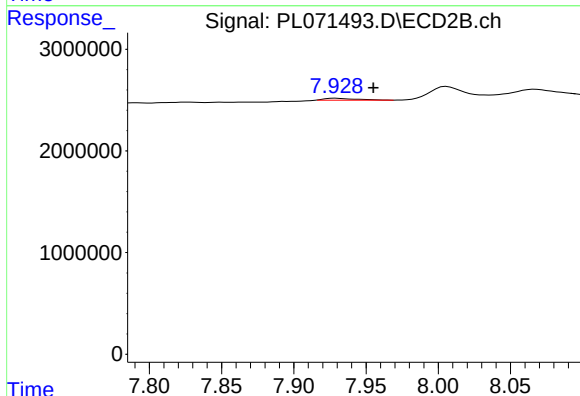


#8 Heptachlor epoxide

R.T.: 7.929 min
Delta R.T.: -0.026 min
Response: 279474
Conc: 0.21 ng/ml

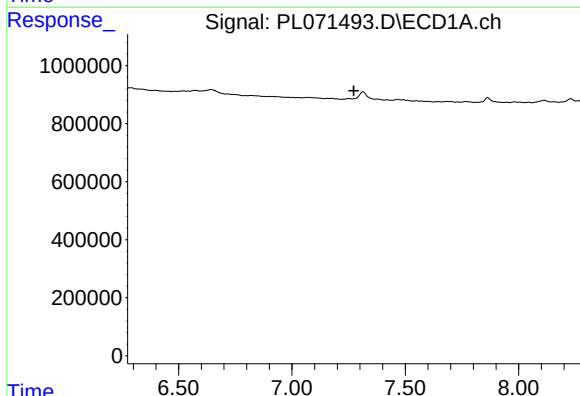


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

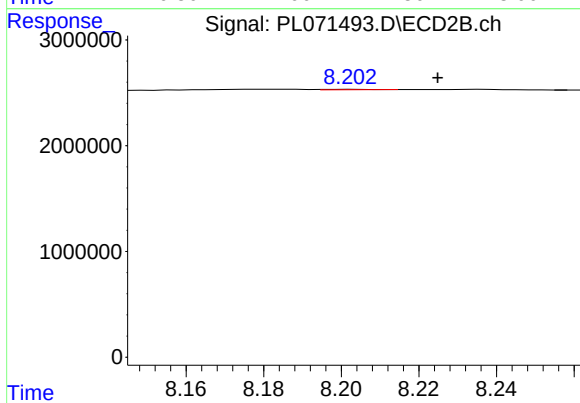

#10 gamma-Chlordane


R.T.: 8.203 min
Delta R.T.: -0.022 min
Response: 36297
Conc: 0.03 ng/ml

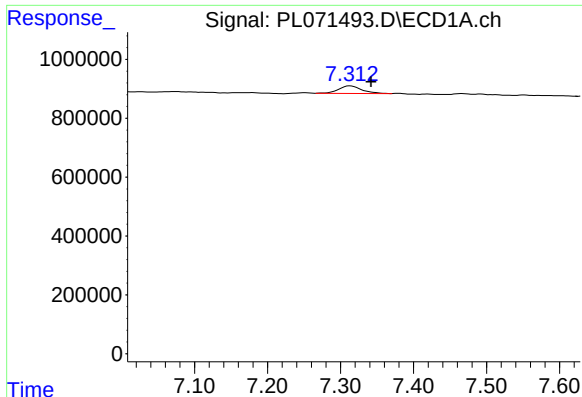

#11 alpha-Chlordane


R.T.: 7.313 min
Delta R.T.: -0.029 min
Response: 561917
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

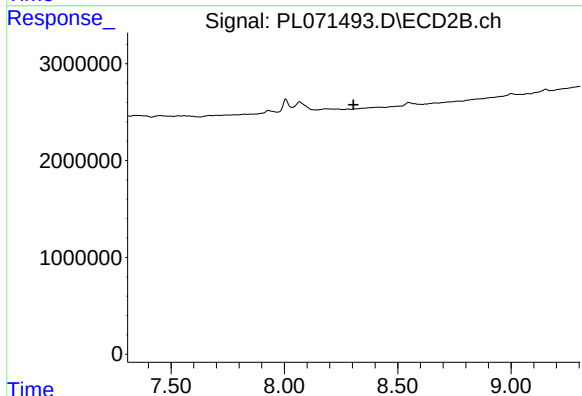


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.305 min
Response: 0
Conc: N.D.

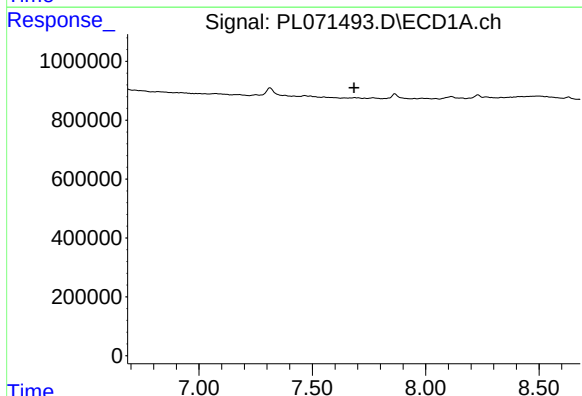


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.684 min
Response: 0
Conc: N.D.

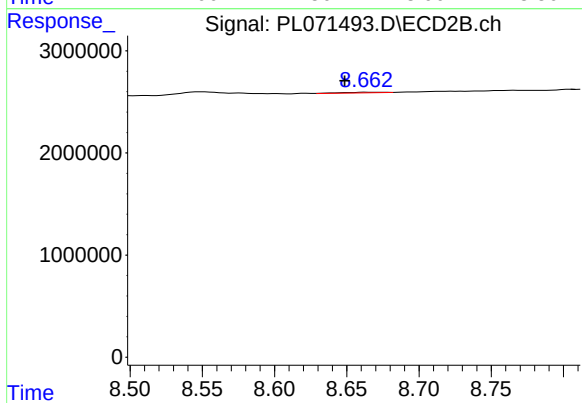

#13 Dieldrin


R.T.: 8.663 min
Delta R.T.: 0.014 min
Response: 113449
Conc: 0.09 ng/ml

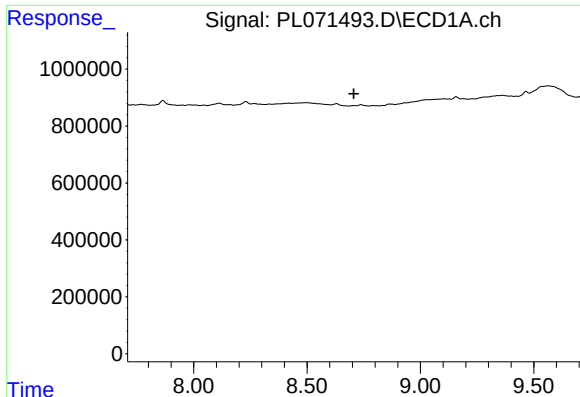

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

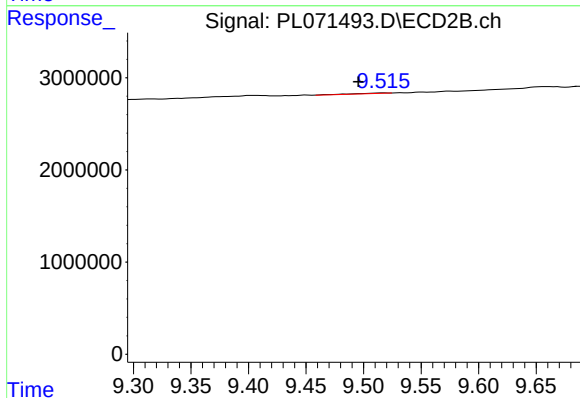


#19 Endosulfan Sulfate

R.T.: 9.518 min
Delta R.T.: 0.022 min
Response: 101797
Conc: 0.10 ng/ml

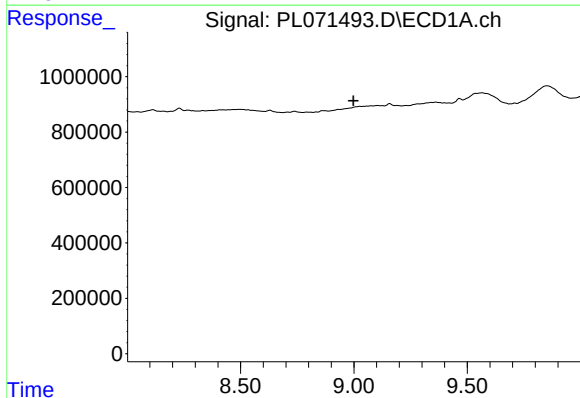


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 8.998 min
Response: 0
Conc: N.D.

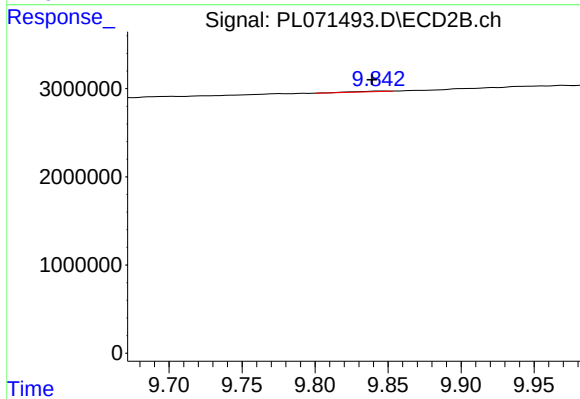

#20 Methoxychlor


R.T.: 9.844 min
Delta R.T.: 0.005 min
Response: 98253
Conc: 0.20 ng/ml

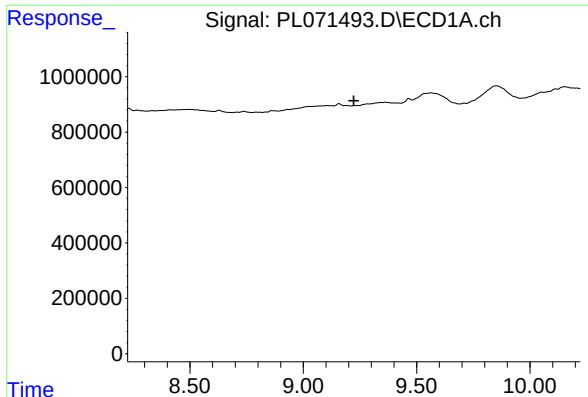

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

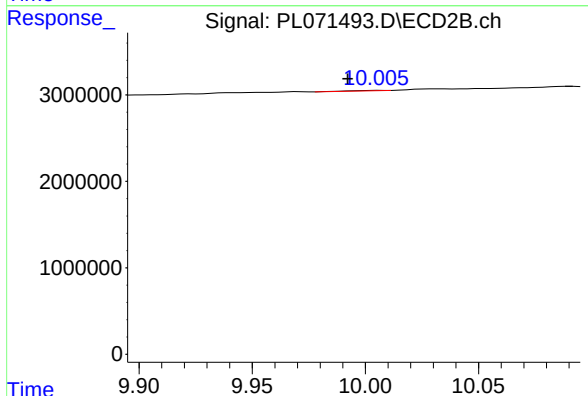


#21 Endrin ketone

R.T.: 10.007 min
Delta R.T.: 0.015 min
Response: 41654
Conc: 0.04 ng/ml

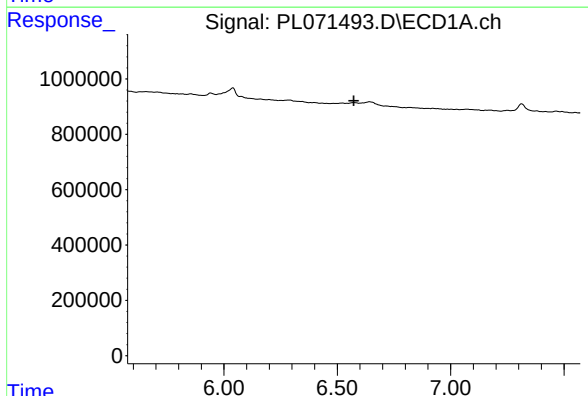


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

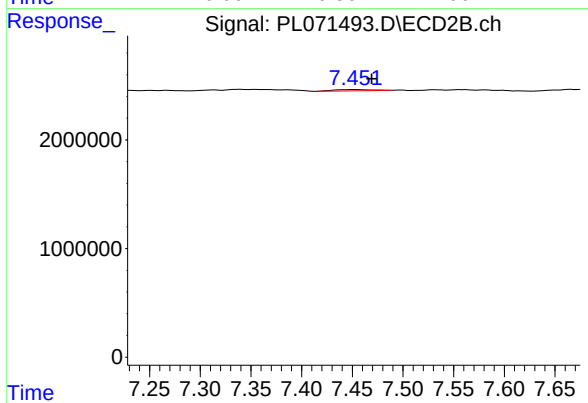

#24 Chlordane-2


R.T.: 7.452 min
Delta R.T.: -0.017 min
Response: 287085
Conc: 6.09 ng/ml

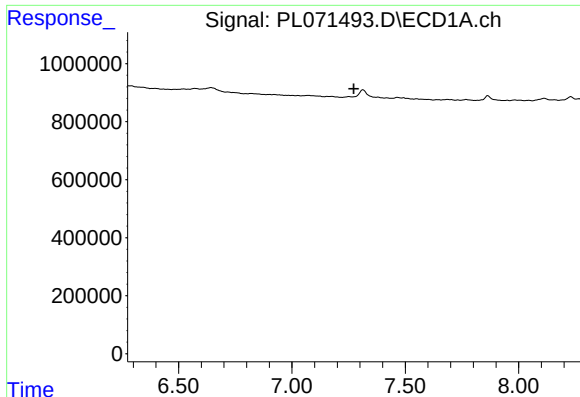

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

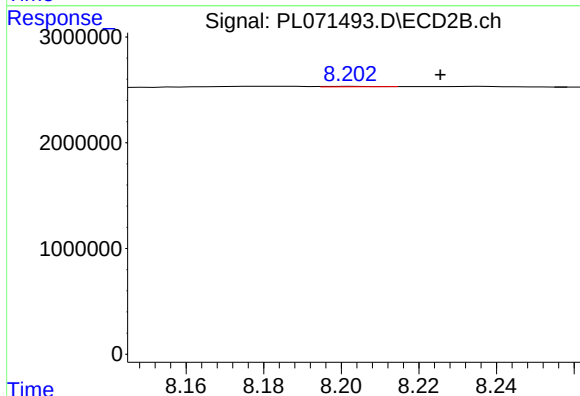


#25 Chlordane-3

R.T.: 8.203 min
Delta R.T.: -0.022 min
Response: 36297
Conc: 0.21 ng/ml

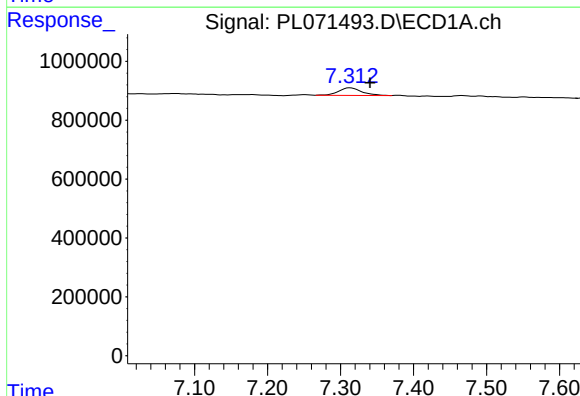


#26 Chlordane-4

R.T.: 7.313 min
Delta R.T.: -0.028 min
Response: 561917
Conc: 9.05 ng/ml

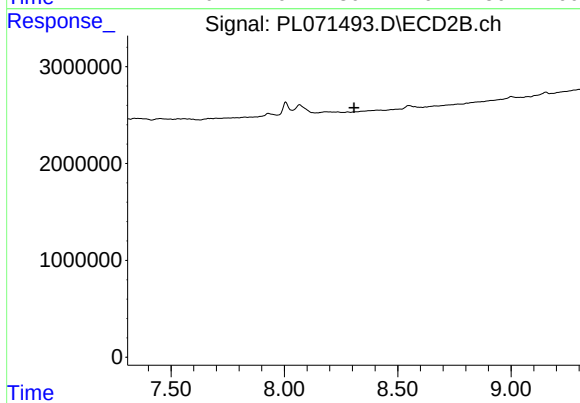

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.307 min
Response: 0
Conc: N.D.

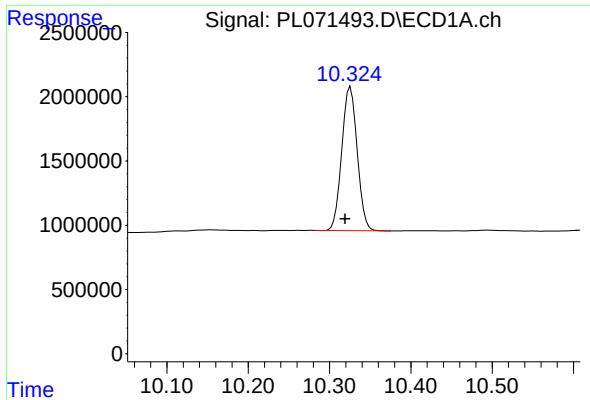

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.007 min
Response: 14701159
Conc: 22.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

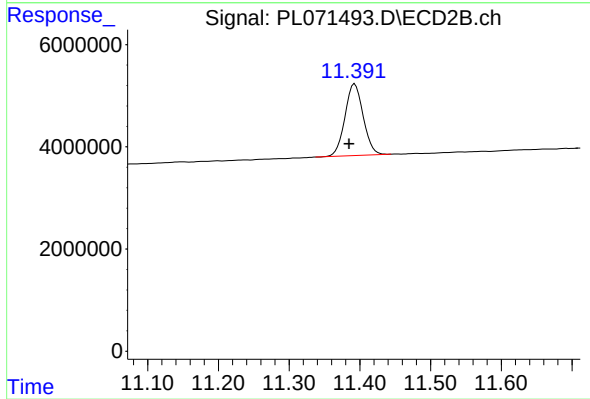

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.008 min
Response: 25249726
Conc: 23.24 ng/ml