

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121625\
 Data File : PL097880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2025 14:57
 Operator : AR\AJ
 Sample : Q3873-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:48:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	2.799	100.1E6	142.8E6	19.827	20.449
28)	SA Decachlor...	8.954	7.946	68104637	105.2E6	17.925	15.996
Target Compounds							
3)	MA gamma-BHC...	0.000	3.637	0	5223923	N.D.	0.486 #
8)	B Heptachlo...	5.639f	0.000	15262379	0	2.294	N.D. #
9)	A Endosulfan I	6.027f	5.151f	7982263	26248446	1.356	2.576 #
11)	B alpha-Chl...	0.000	5.088	0	21049571	N.D.	2.053 #
13)	MA Dieldrin	0.000	5.397	0	18693615	N.D.	1.995 #
20)	A Methoxychlor	0.000	6.666f	0	14211990	N.D.	3.401 #
23)	Chlordane-1	0.000	3.807	0	7534763	N.D.	28.473 #
26)	Chlordane-4	0.000	5.088	0	21049571	N.D.	26.074 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121625\
Data File : PL097880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2025 14:57
Operator : AR\AJ
Sample : Q3873-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:48:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

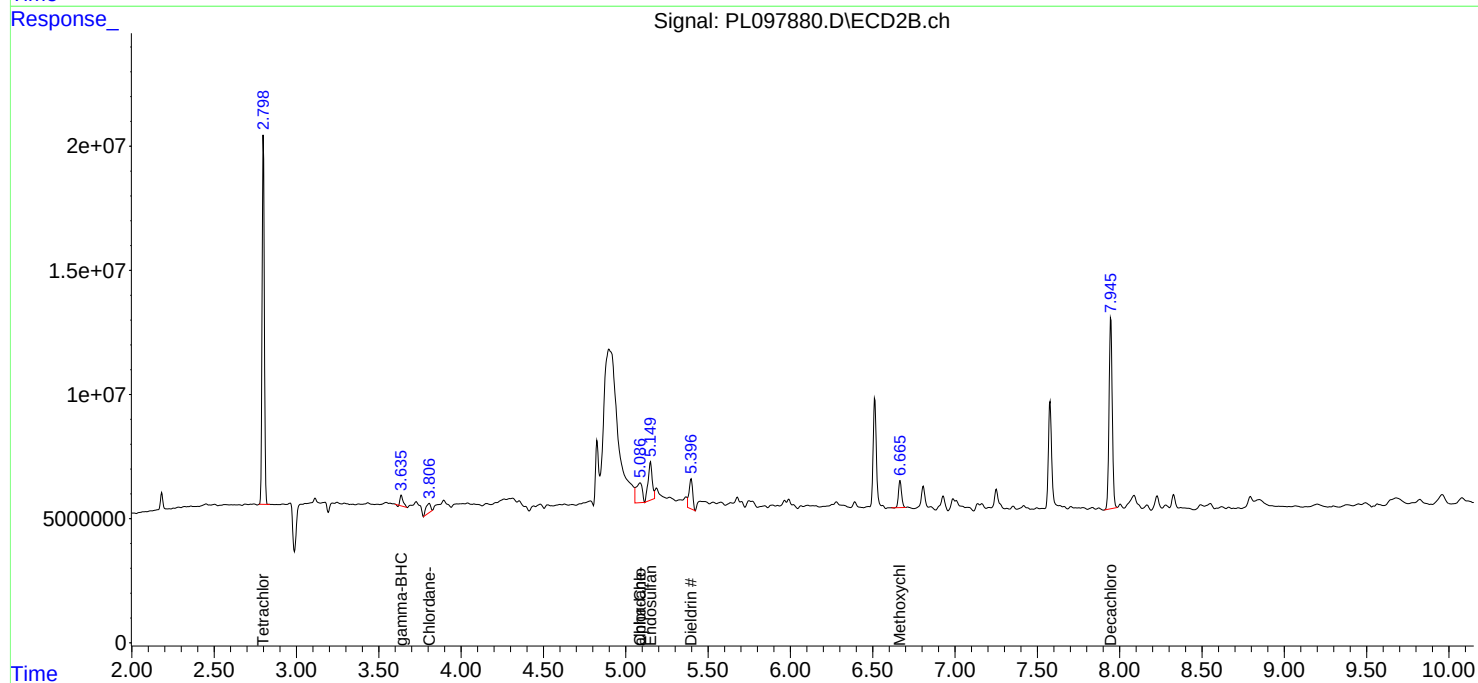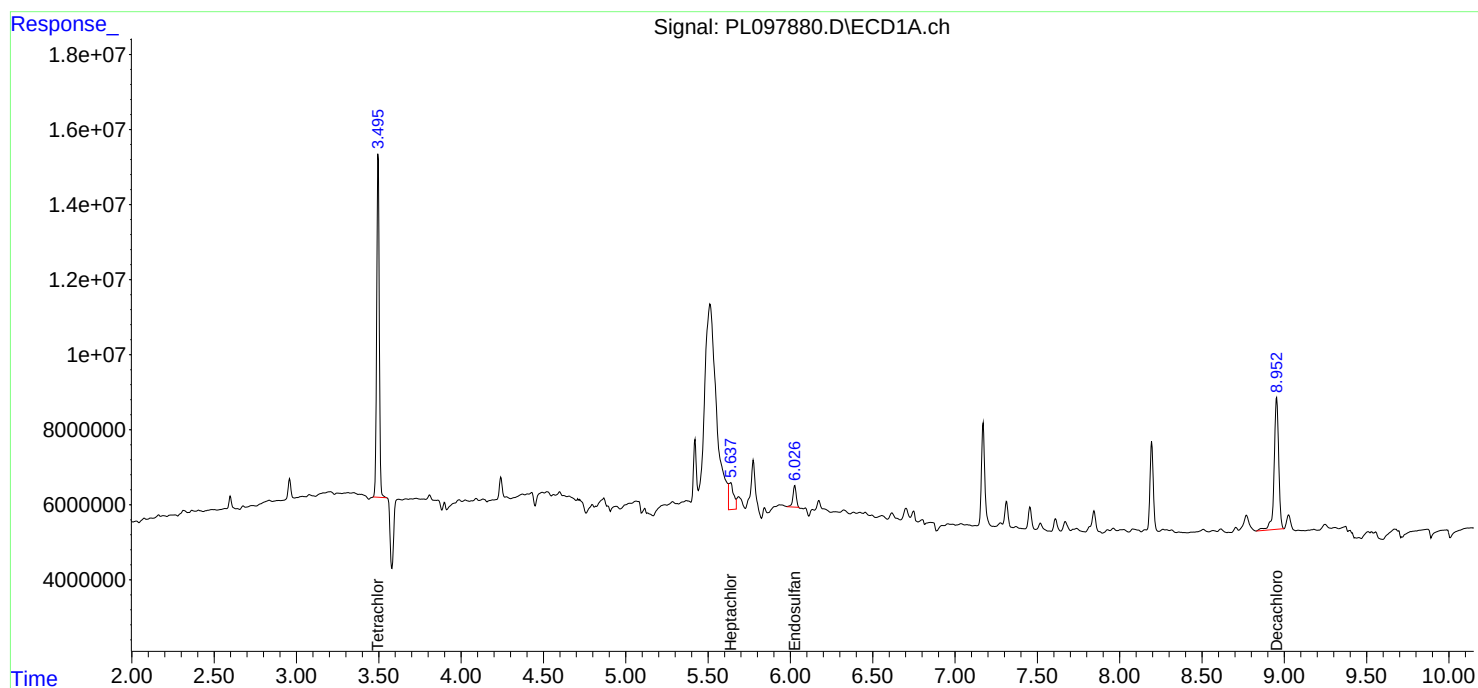


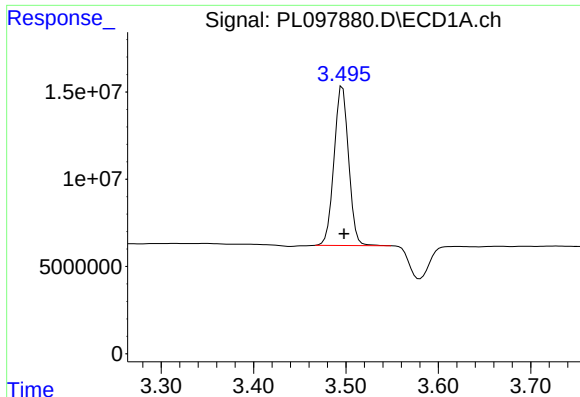

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: -0.002 min
Response: 100064626
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

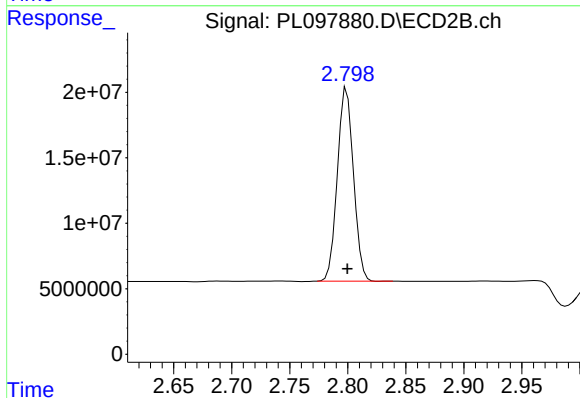


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: 0.000 min
Response: 142838074
Conc: 20.45 ng/ml

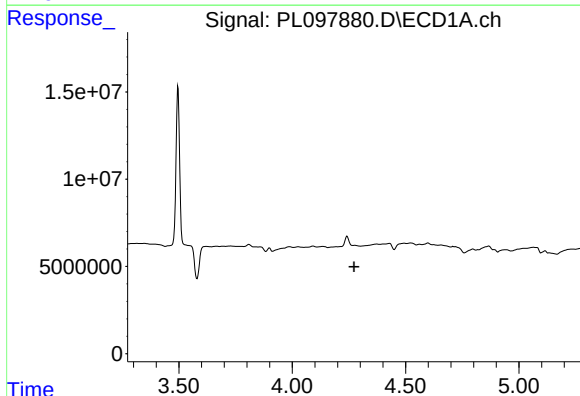


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

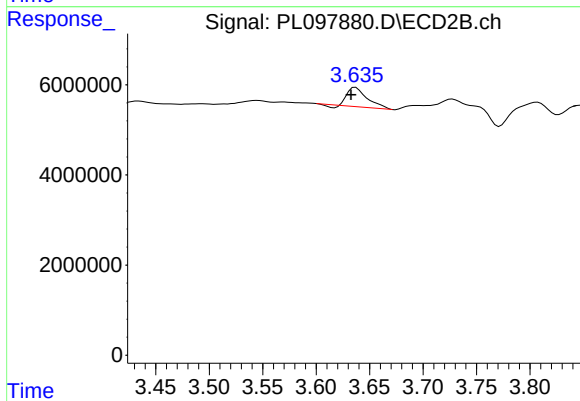

#3 gamma-BHC (Lindane)


R.T.: 3.637 min
Delta R.T.: 0.004 min
Response: 5223923
Conc: 0.49 ng/ml

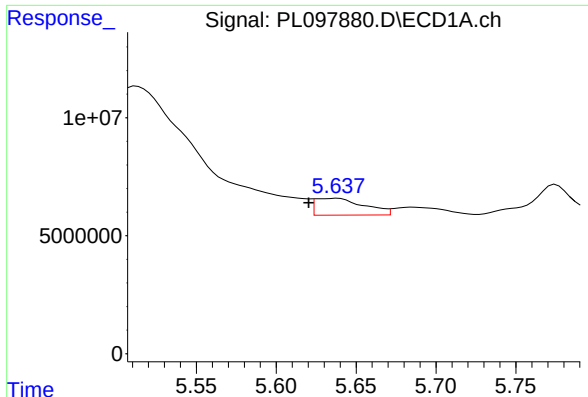

#8 Heptachlor epoxide


R.T.: 5.639 min
Delta R.T.: 0.018 min
Response: 15262379
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

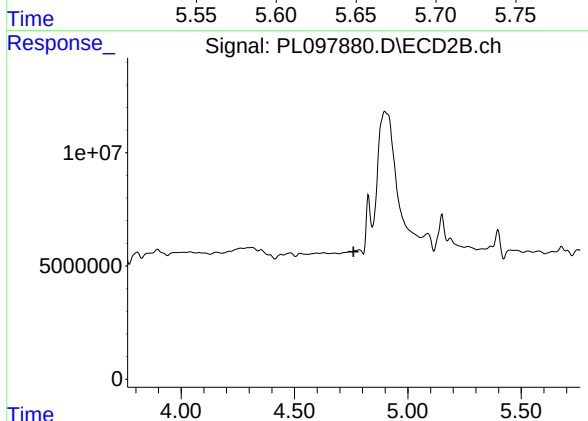


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.761 min
Response: 0
Conc: N.D.

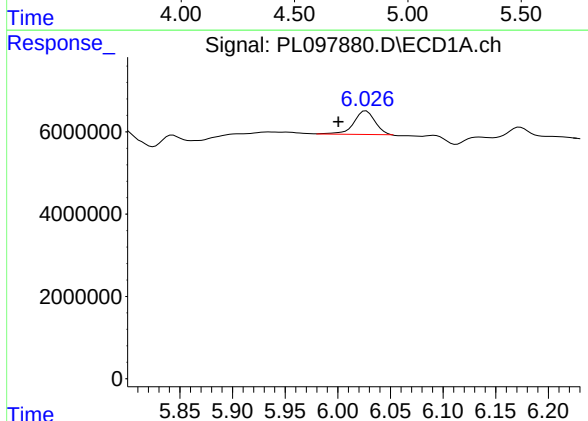


#9 Endosulfan I

R.T.: 6.027 min
Delta R.T.: 0.026 min
Response: 7982263
Conc: 1.36 ng/ml

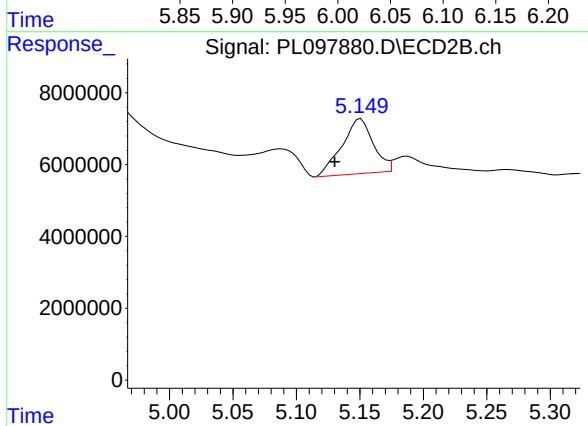

#9 Endosulfan I


R.T.: 5.151 min
Delta R.T.: 0.020 min
Response: 26248446
Conc: 2.58 ng/ml

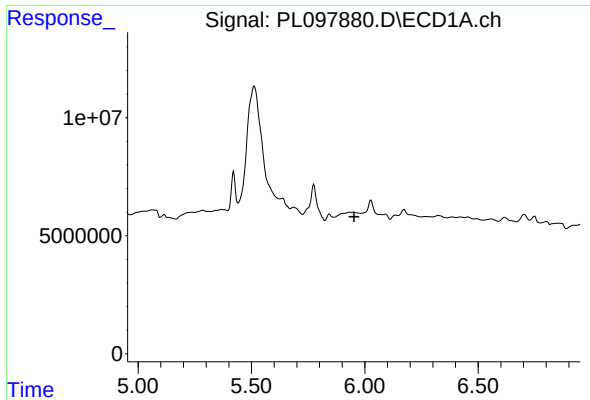

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

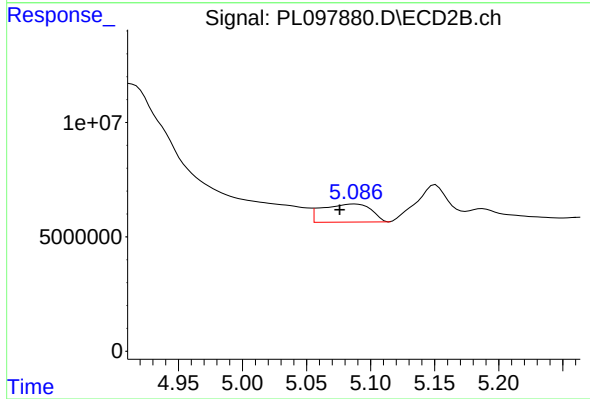


#11 alpha-Chlordane

R.T.: 5.088 min
Delta R.T.: 0.012 min
Response: 21049571
Conc: 2.05 ng/ml

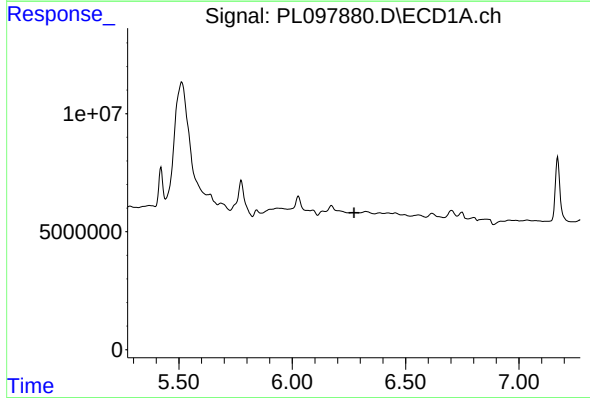


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.273 min
Response: 0
Conc: N.D.

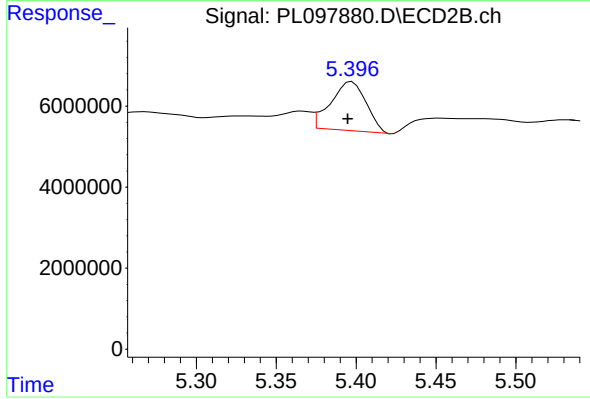

#13 Dieldrin


R.T.: 5.397 min
Delta R.T.: 0.003 min
Response: 18693615
Conc: 1.99 ng/ml

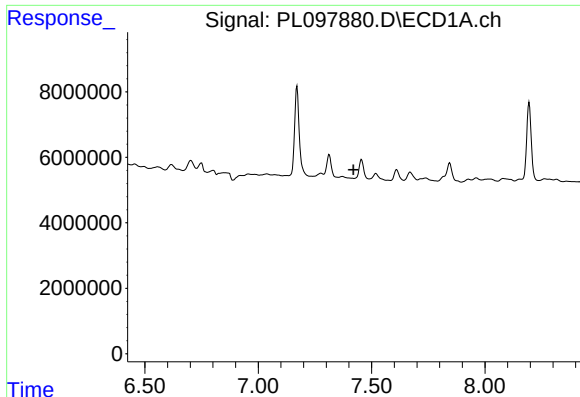

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

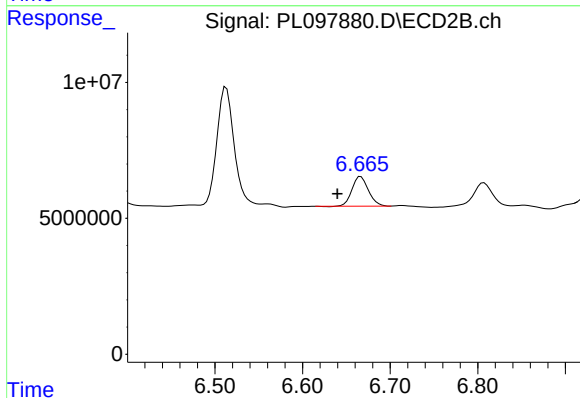


#20 Methoxychlor

R.T.: 6.666 min
Delta R.T.: 0.026 min
Response: 14211990
Conc: 3.40 ng/ml

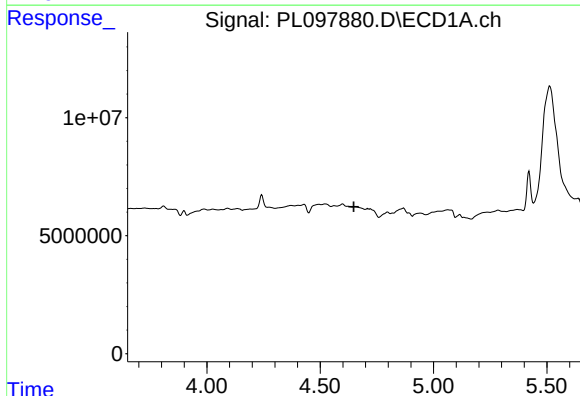


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

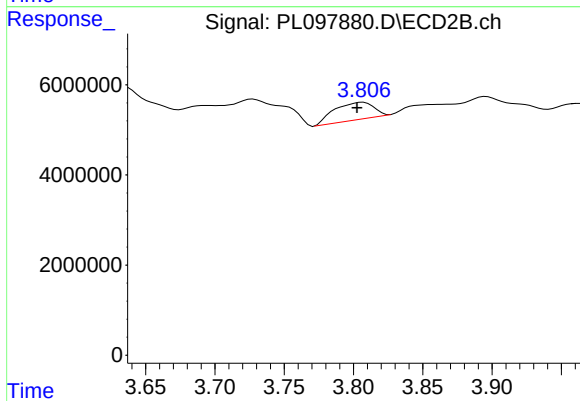

#23 Chlordane-1


R.T.: 3.807 min
Delta R.T.: 0.004 min
Response: 7534763
Conc: 28.47 ng/ml

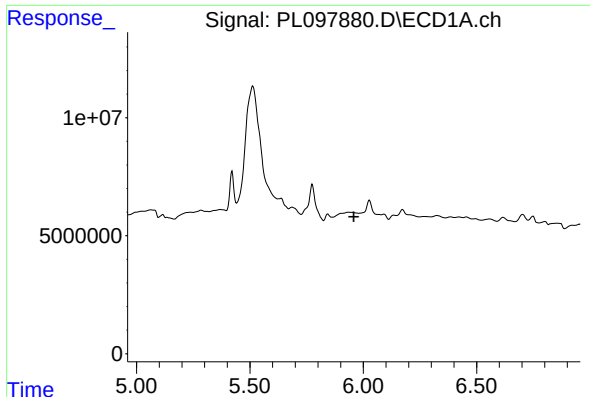

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

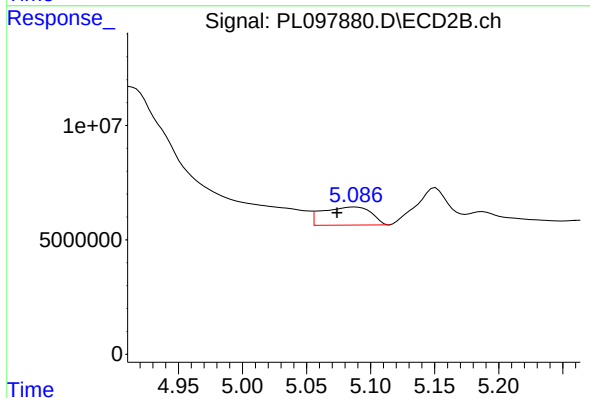


#26 Chlordane-4

R.T.: 5.088 min
Delta R.T.: 0.014 min
Response: 21049571
Conc: 26.07 ng/ml

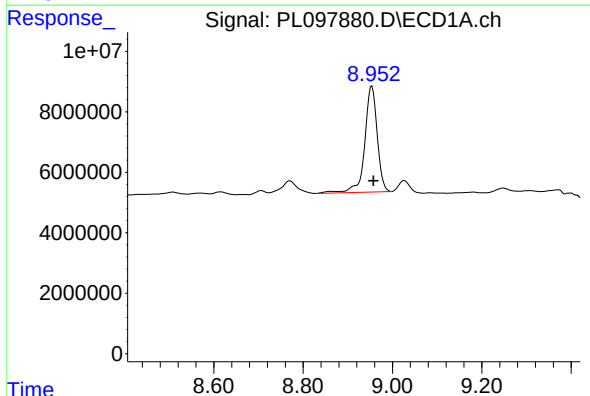

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.003 min
Response: 68104637
Conc: 17.92 ng/ml

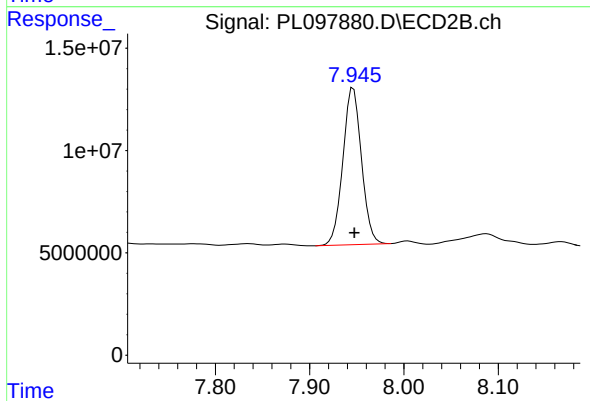

#28 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: -0.001 min
Response: 105189928
Conc: 16.00 ng/ml