

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 09:00
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:53:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	136.9E6	67589810	22.329	22.804
28)	SA Decachlor...	8.204	9.231	125.0E6	52242028	19.140	20.028
Target Compounds							
2)	A alpha-BHC	3.899	0.000	4421114	0	0.468	N.D. #
7)	B delta-BHC	0.000	5.173	0	1770092	N.D.	0.412 #
8)	B Heptachlo...	0.000	6.019	0	1216971	N.D.	0.321 #
9)	A Endosulfan I	0.000	6.311f	0	717878	N.D.	0.211 #
11)	B alpha-Chl...	0.000	6.311	0	717878	N.D.	0.200 #
20)	A Methoxychlor	6.886	0.000	2367491	0	0.706	N.D. #
21)	B Endrin ke...	0.000	7.862	0	3235548	N.D.	1.059 #
23)	Chlordane-1	4.363	5.173	-351011	1770092	N.D.	12.524
26)	Chlordane-4	0.000	6.311	0	717878	N.D.	1.258 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 09:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:53:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

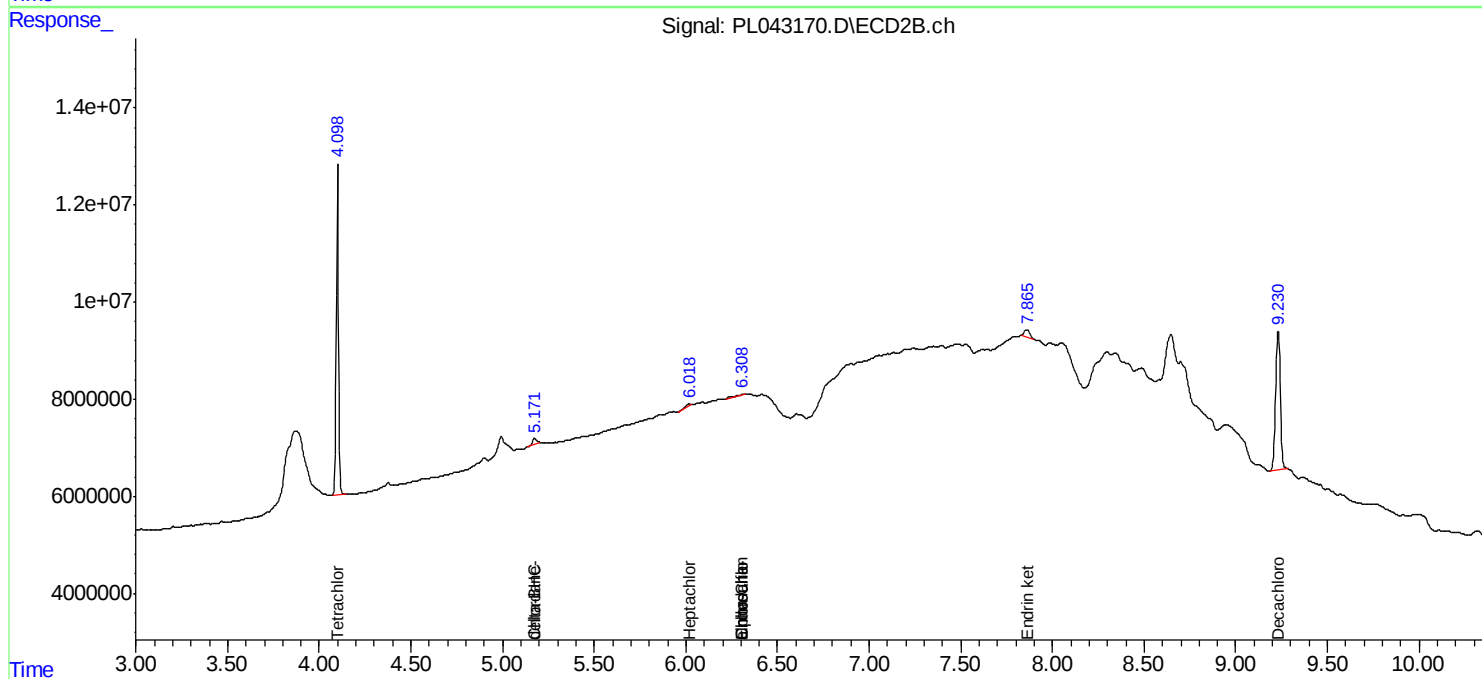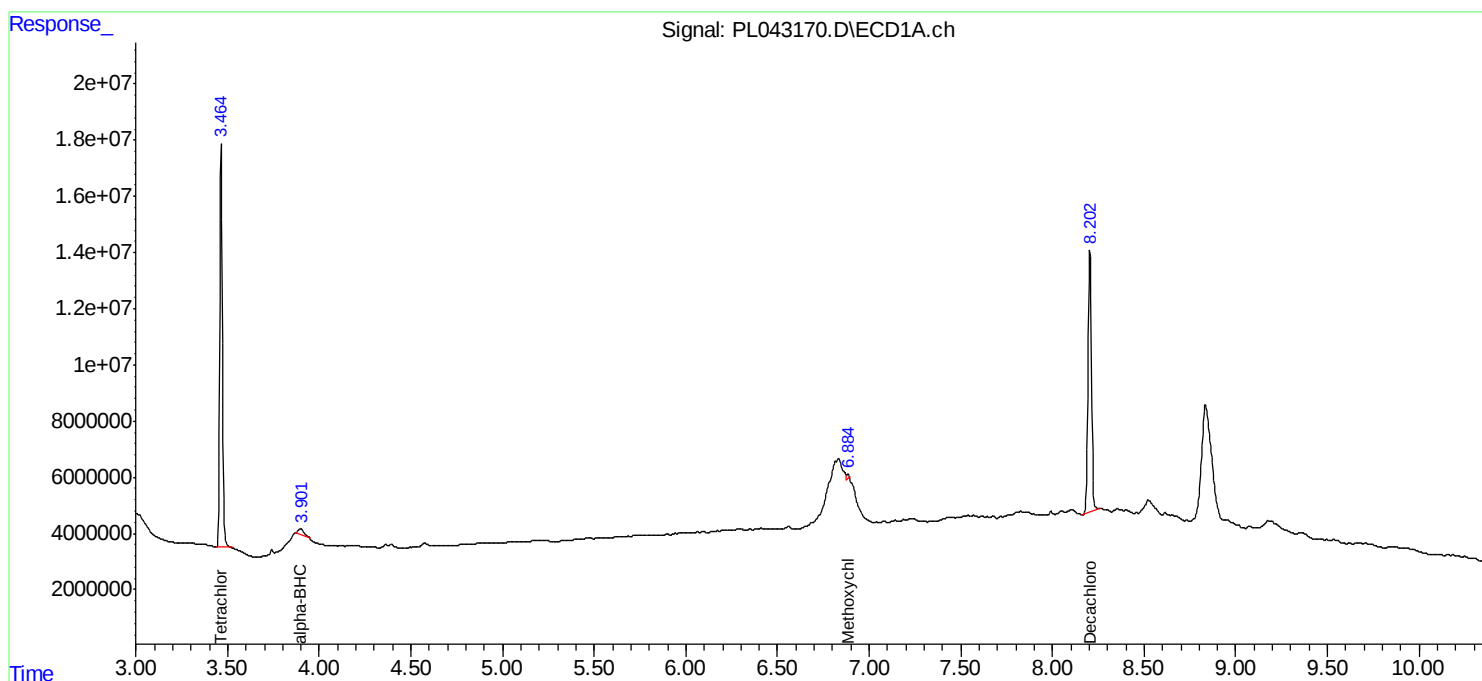


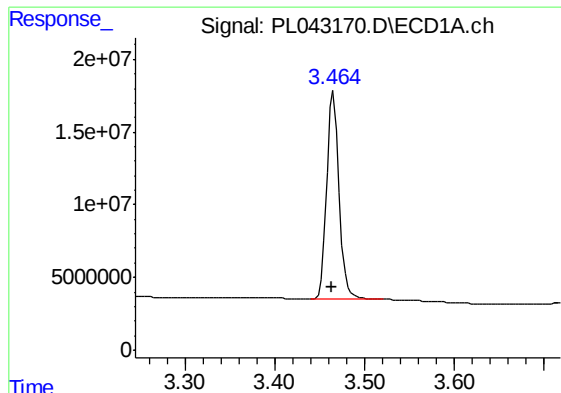

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 136942686
Conc: 22.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

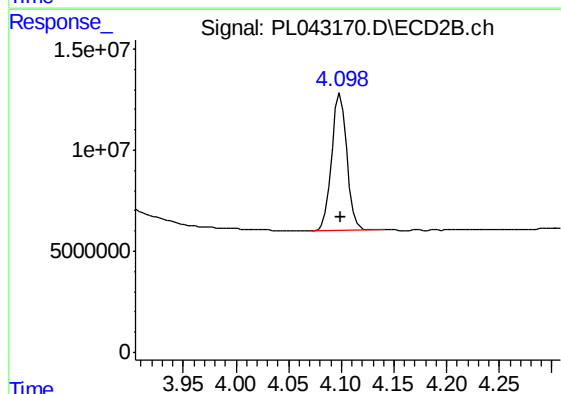


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 67589810
Conc: 22.80 ng/ml

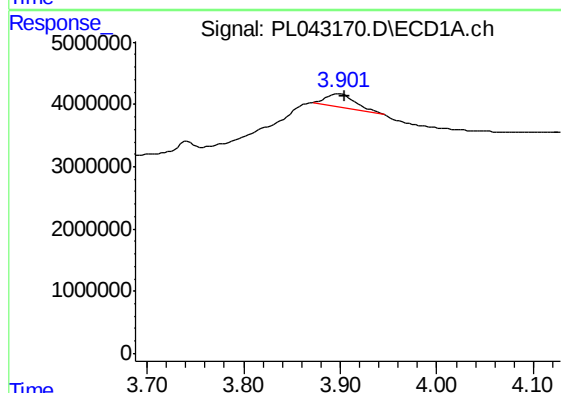


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: -0.005 min
Response: 4421114
Conc: 0.47 ng/ml

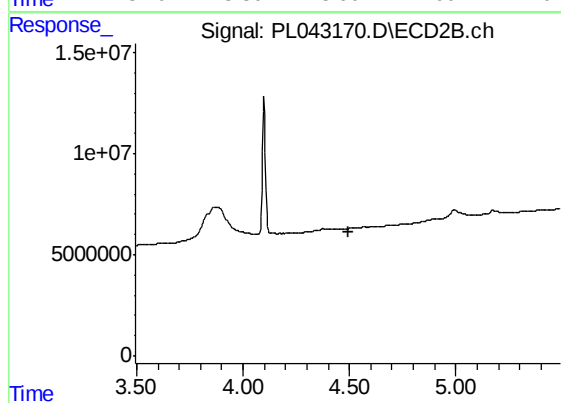

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

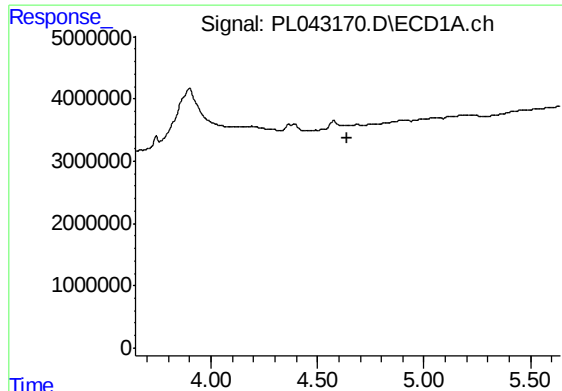

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

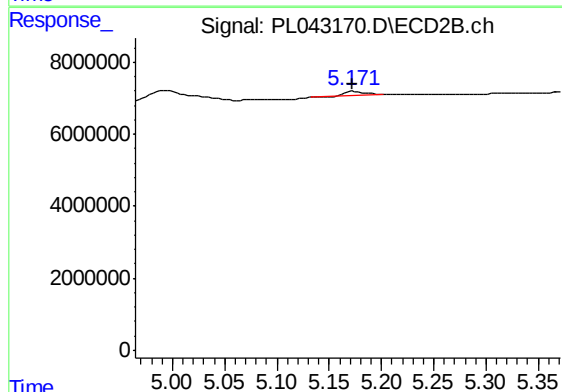


#7 delta-BHC

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 1770092
Conc: 0.41 ng/ml

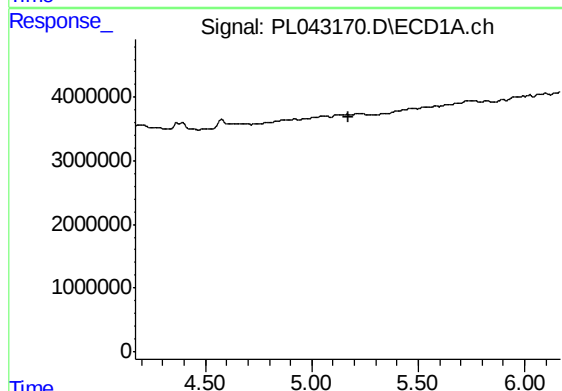


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

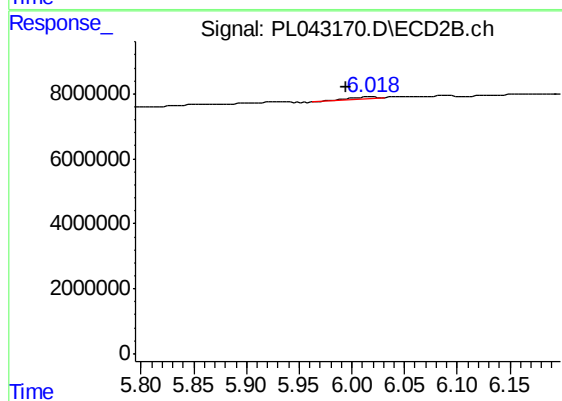

#8 Heptachlor epoxide


R.T.: 6.019 min
Delta R.T.: 0.024 min
Response: 1216971
Conc: 0.32 ng/ml

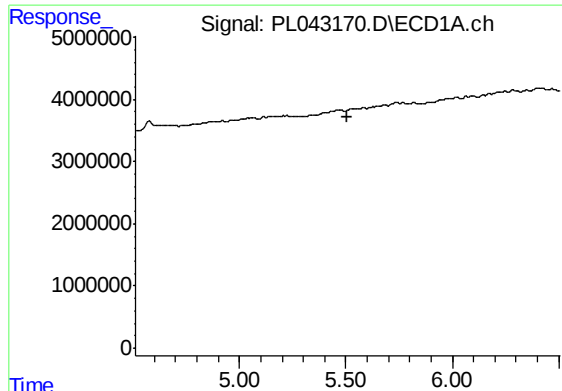

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

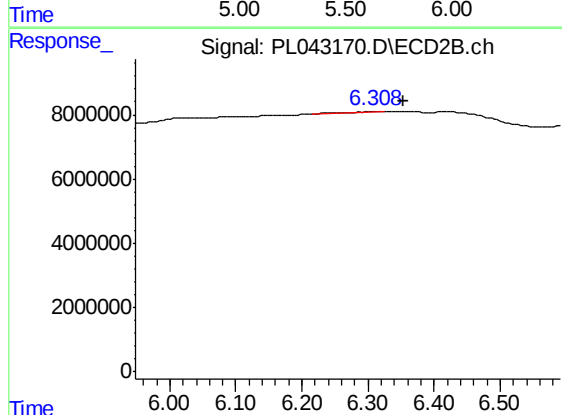


#9 Endosulfan I

R.T.: 6.311 min
Delta R.T.: -0.044 min
Response: 717878
Conc: 0.21 ng/ml

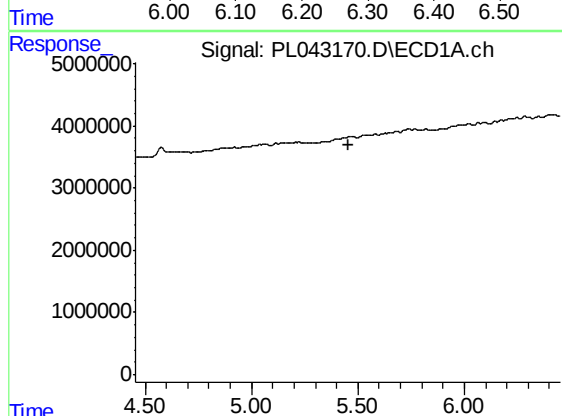


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.454 min
Response: 0
Conc: N.D.

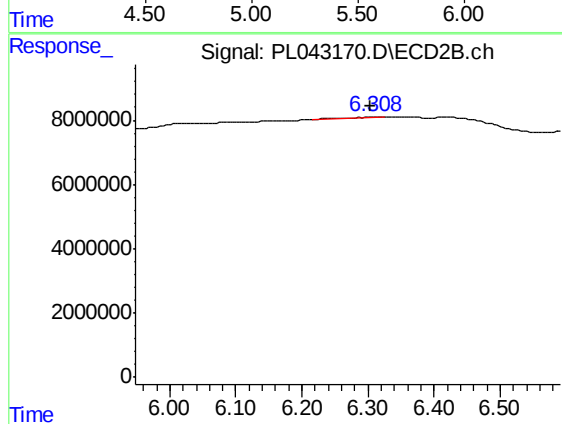

#11 alpha-Chlordane


R.T.: 6.311 min
Delta R.T.: 0.008 min
Response: 717878
Conc: 0.20 ng/ml

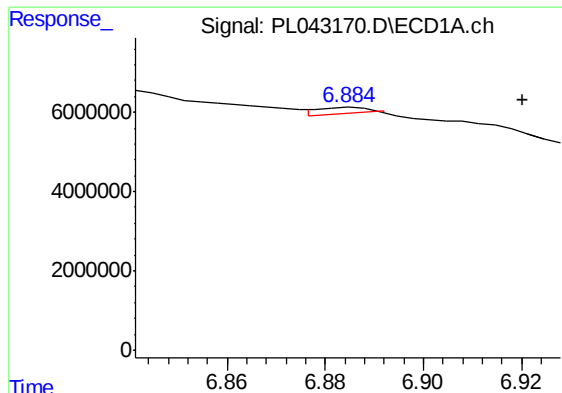

#20 Methoxychlor


R.T.: 6.886 min
Delta R.T.: -0.035 min
Response: 2367491
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

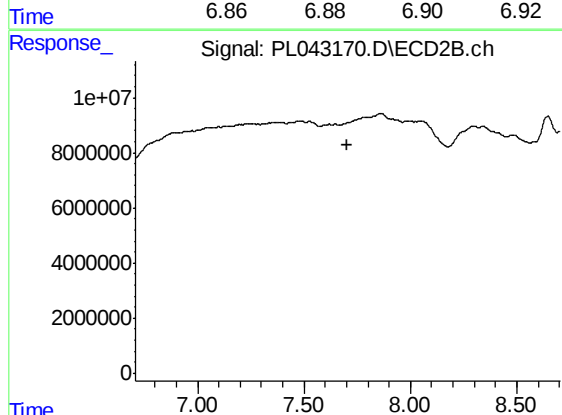


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.705 min
Response: 0
Conc: N.D.

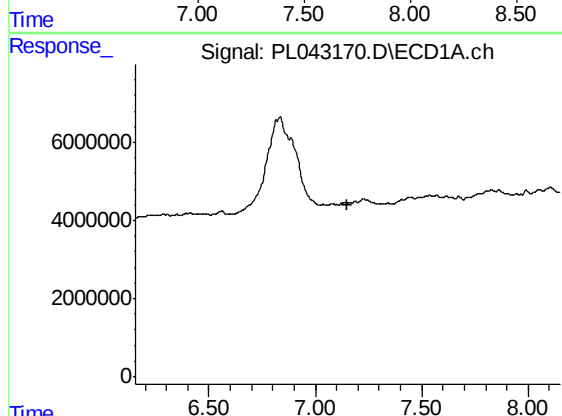


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

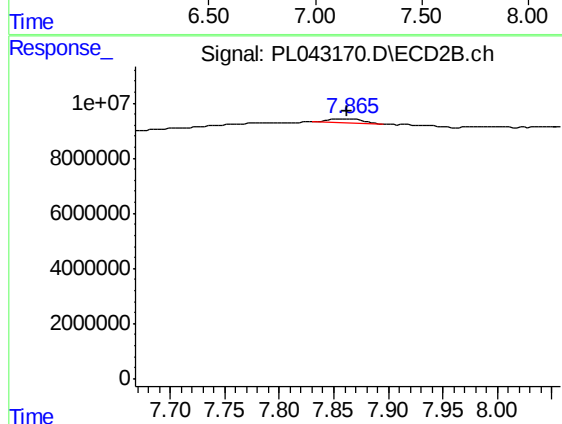

#21 Endrin ketone


R.T.: 7.862 min
Delta R.T.: 0.000 min
Response: 3235548
Conc: 1.06 ng/ml

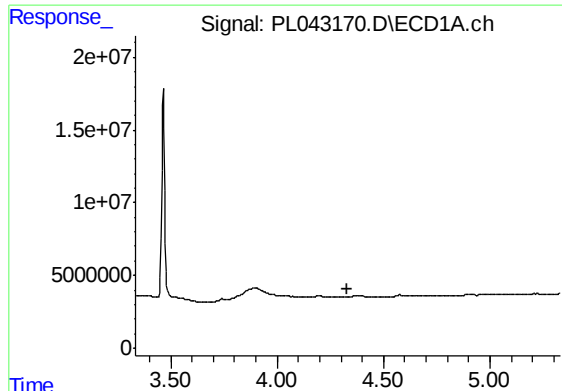

#23 Chlordane-1


R.T.: 4.363 min
Delta R.T.: 0.031 min
Response: -351011
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

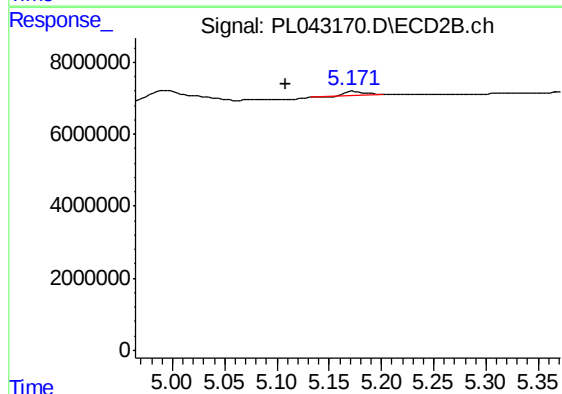


#23 Chlordane-1

R.T.: 5.173 min
Delta R.T.: 0.064 min
Response: 1770092
Conc: 12.52 ng/ml

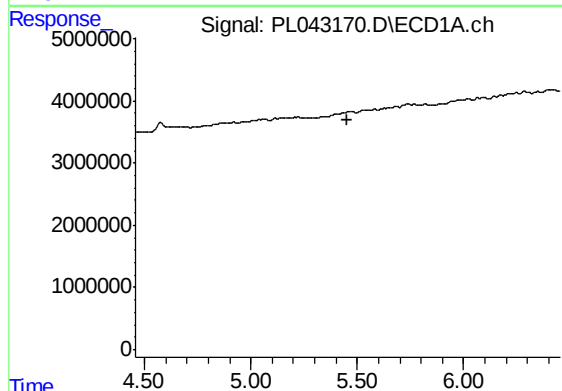


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

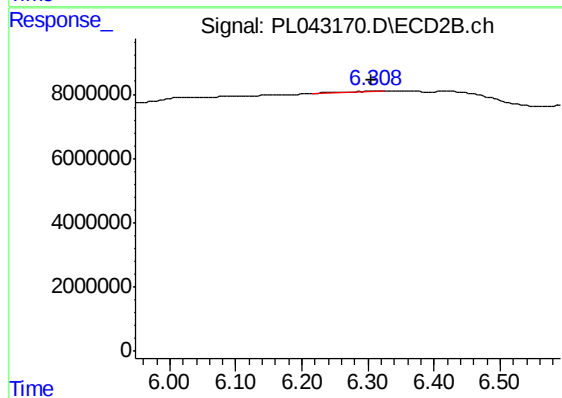

#26 Chlordane-4


R.T.: 6.311 min
Delta R.T.: 0.006 min
Response: 717878
Conc: 1.26 ng/ml

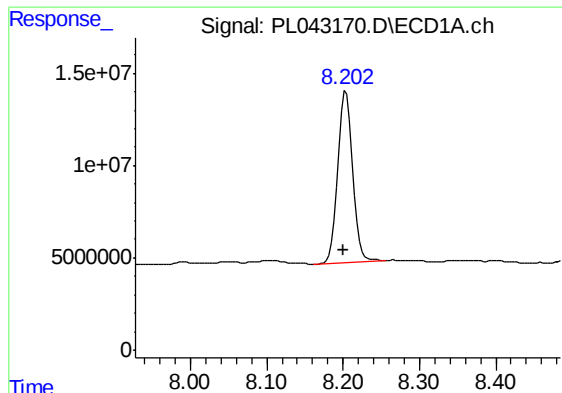

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.003 min
Response: 124981049
Conc: 19.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

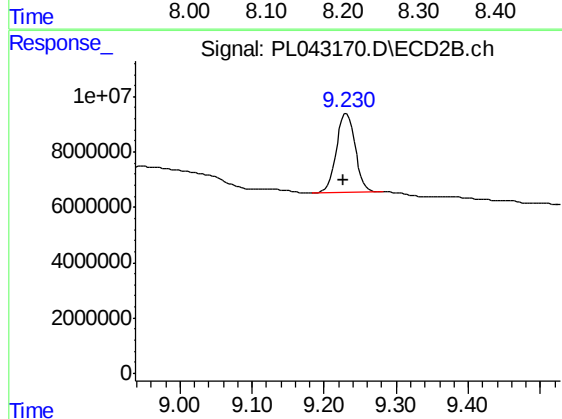

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 52242028
Conc: 20.03 ng/ml