

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 12:08
 Operator : AJ\SJ
 Sample : J6376-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:56:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	161.0E6	78311885	26.248	26.422
28)	SA Decachlor...	8.202	9.231	138.6E6	53845806	21.220	20.642
Target Compounds							
6)	B beta-BHC	4.398f	4.903f	2384351	2042601	0.646	1.207 #
7)	B delta-BHC	0.000	5.158	0	24253659	N.D.	5.644 #
8)	B Heptachlo...	0.000	5.995	0	19246949	N.D.	5.076 #
11)	B alpha-Chl...	0.000	6.261f	0	243332	N.D.	0.068 #
13)	MA Dieldrin	5.700f	0.000	1277896	0	0.164	N.D. #
15)	B Endosulfa...	6.228f	0.000	11488395	0	1.727	N.D. #
23)	Chlordane-1	4.364	5.158	1685947	24253659	6.274	171.606 #
26)	Chlordane-4	0.000	6.261	0	243332	N.D.	0.426 #
27)	Chlordane-5	6.228	0.000	11488395	0	47.897	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 12:08
Operator : AJ\SJ
Sample : J6376-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:56:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

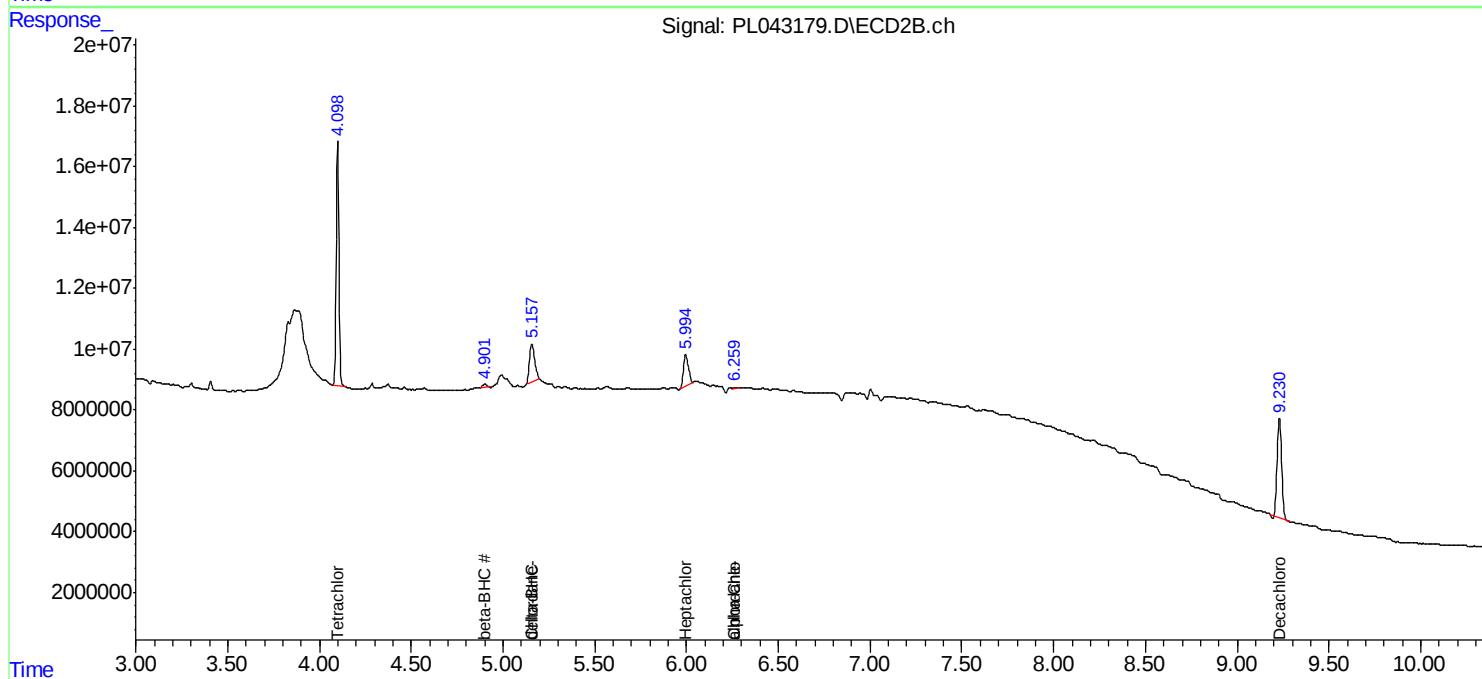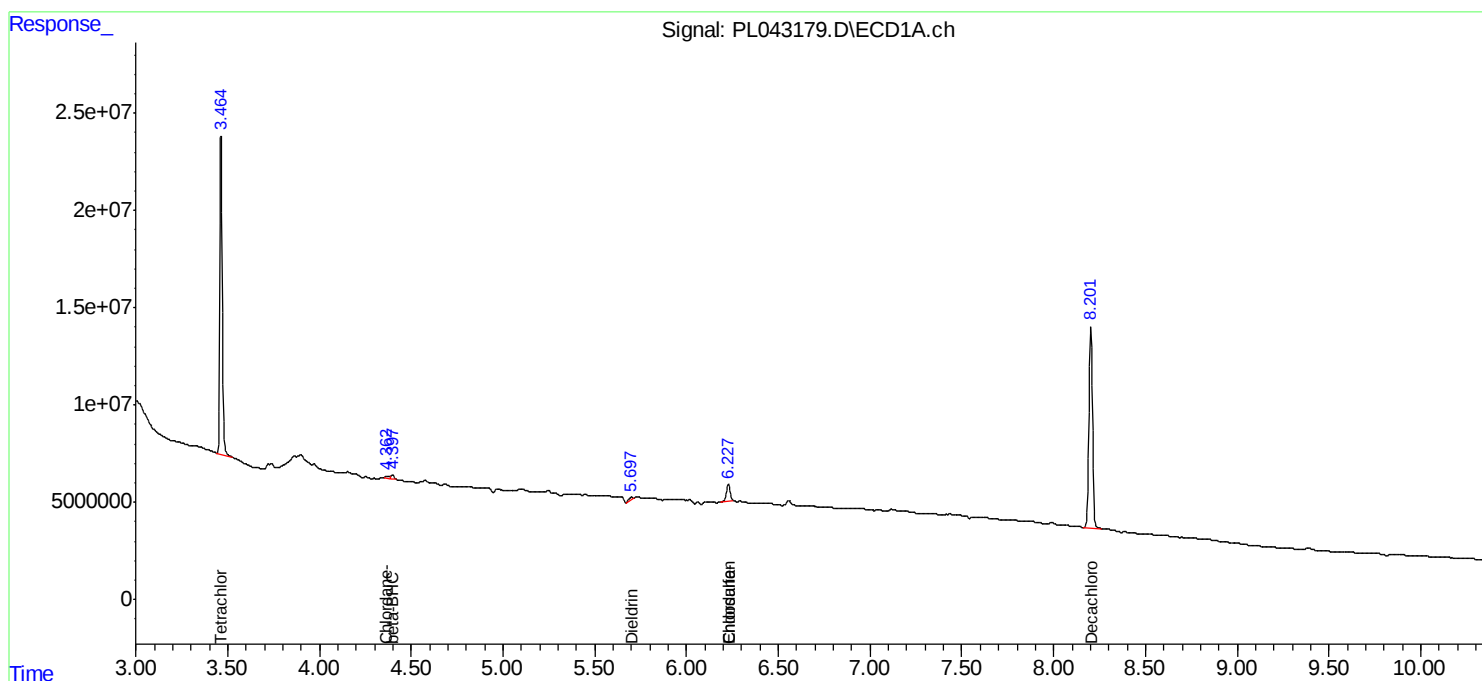


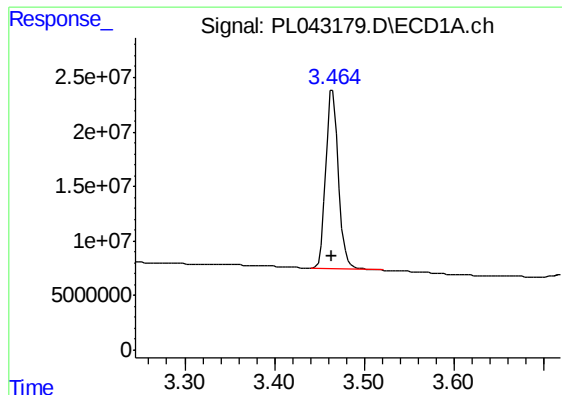

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 160975851
Conc: 26.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

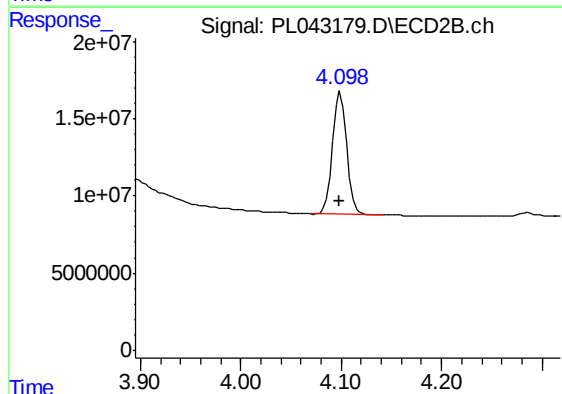


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 78311885
Conc: 26.42 ng/ml

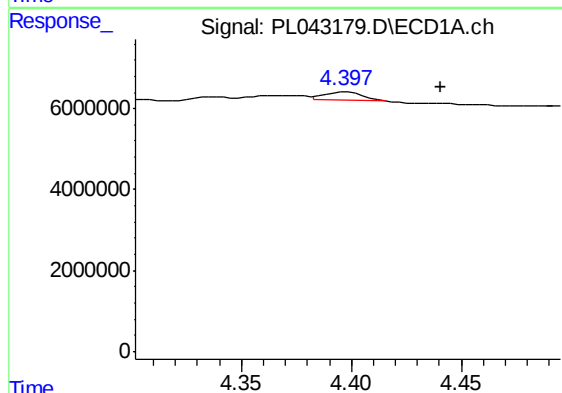


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 2384351
Conc: 0.65 ng/ml

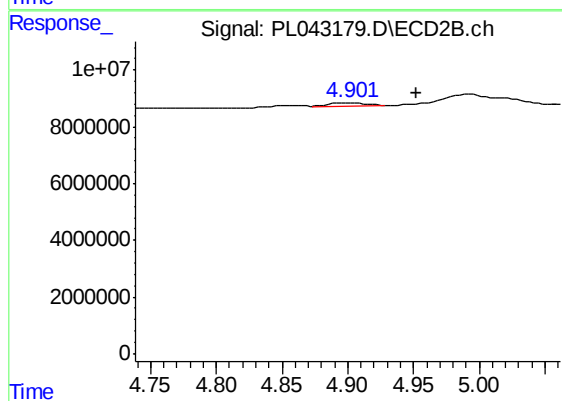

#6 beta-BHC


R.T.: 4.903 min
Delta R.T.: -0.049 min
Response: 2042601
Conc: 1.21 ng/ml

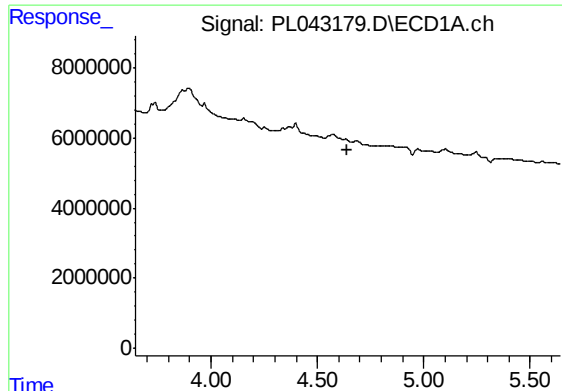

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

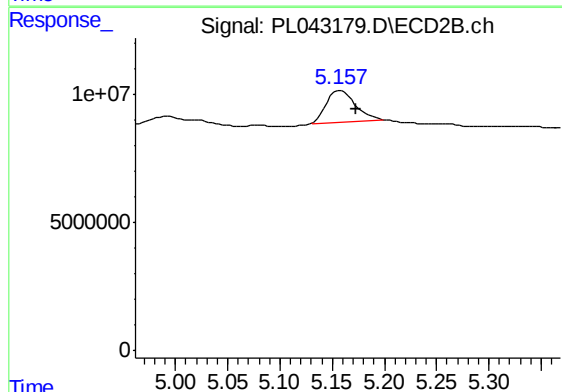


#7 delta-BHC

R.T.: 5.158 min
Delta R.T.: -0.015 min
Response: 24253659
Conc: 5.64 ng/ml

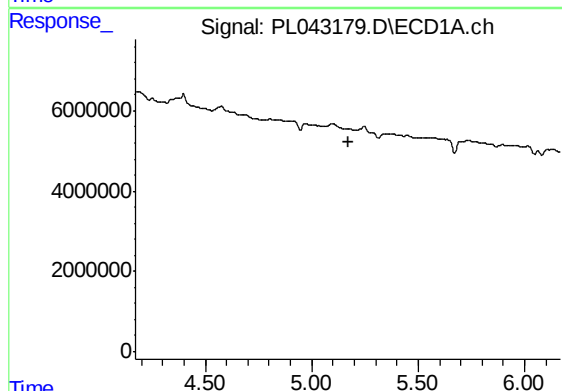


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

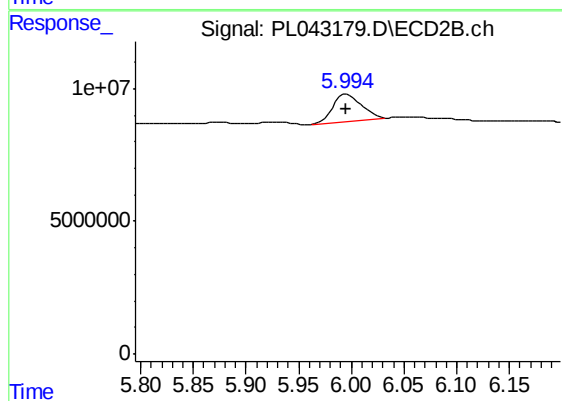

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 19246949
Conc: 5.08 ng/ml

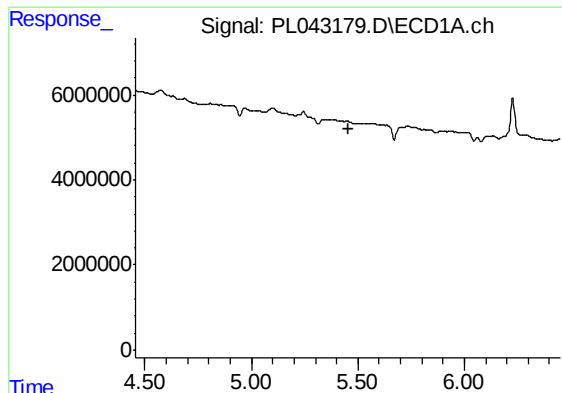

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

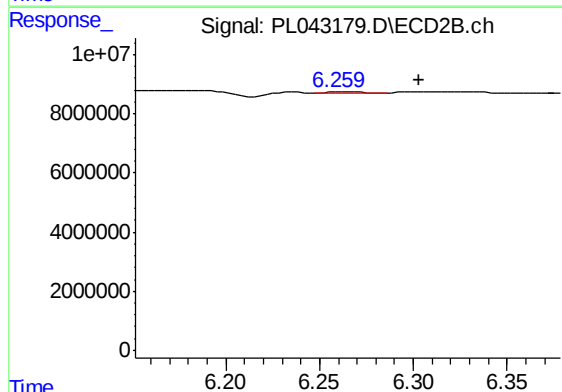


#11 alpha-Chlordane

R.T.: 6.261 min
Delta R.T.: -0.042 min
Response: 243332
Conc: 0.07 ng/ml

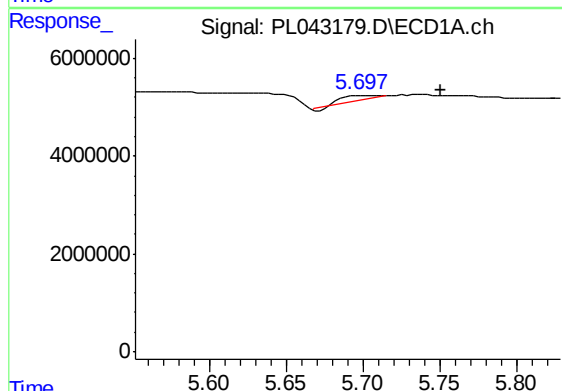


#13 Dieldrin

R.T.: 5.700 min
Delta R.T.: -0.051 min
Response: 1277896
Conc: 0.16 ng/ml

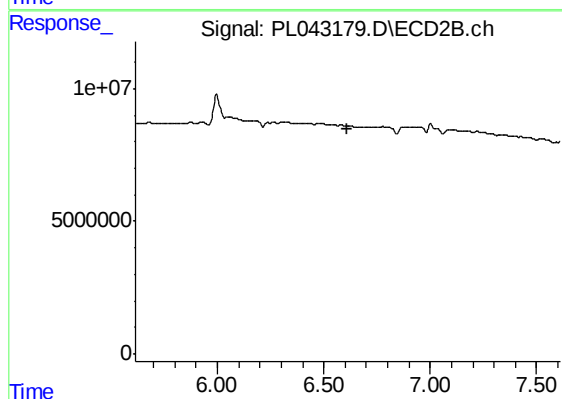

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

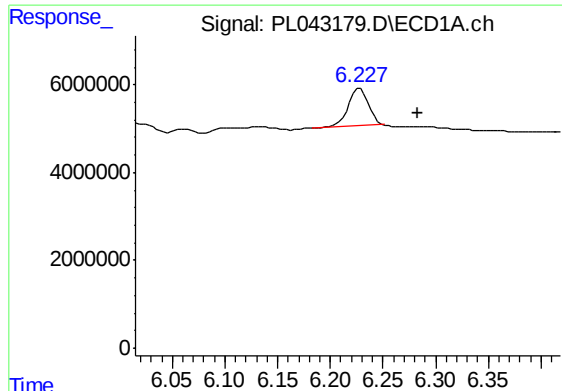

#15 Endosulfan II


R.T.: 6.228 min
Delta R.T.: -0.054 min
Response: 11488395
Conc: 1.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

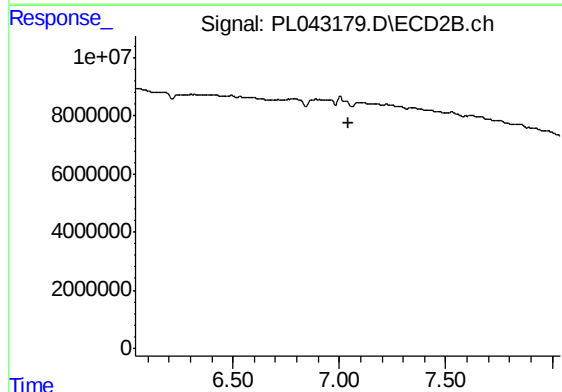


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

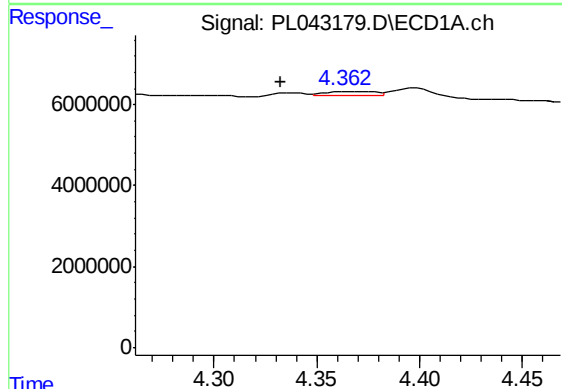


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.031 min
Response: 1685947
Conc: 6.27 ng/ml

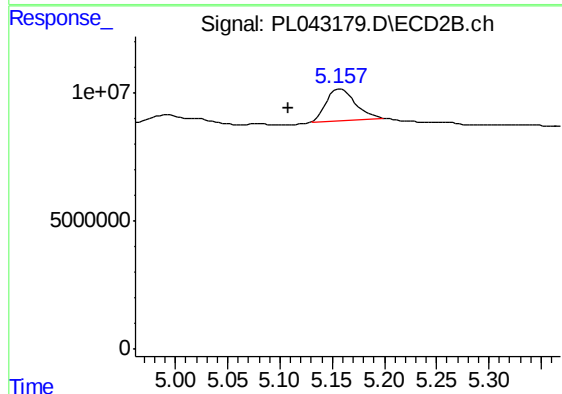

#23 Chlordane-1


R.T.: 5.158 min
Delta R.T.: 0.050 min
Response: 24253659
Conc: 171.61 ng/ml

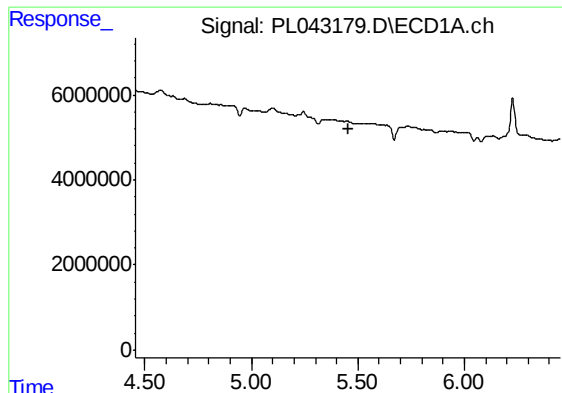

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

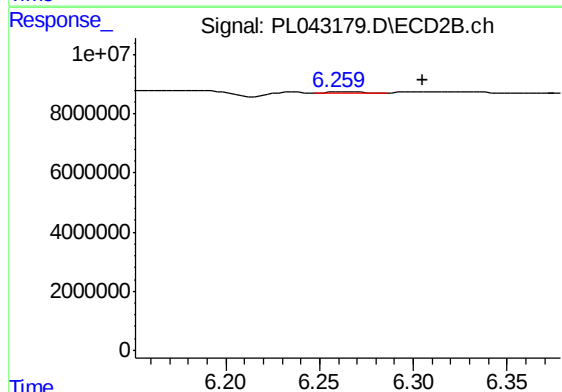


#26 Chlordane-4

R.T.: 6.261 min
Delta R.T.: -0.044 min
Response: 243332
Conc: 0.43 ng/ml

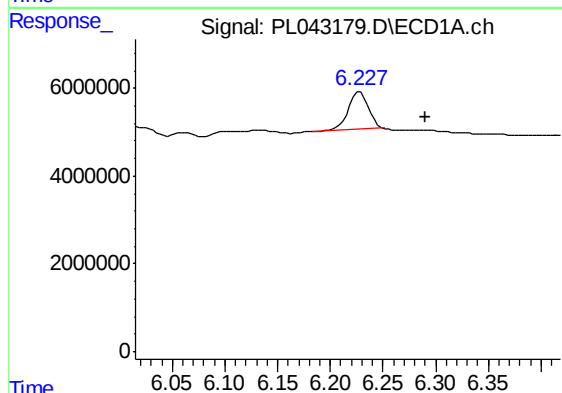


#27 Chlordane-5

R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 11488395
Conc: 47.90 ng/ml

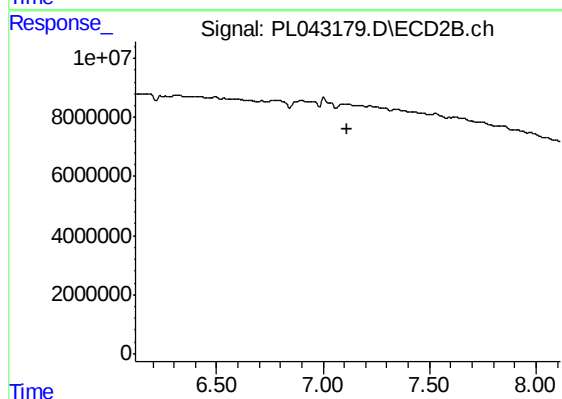

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

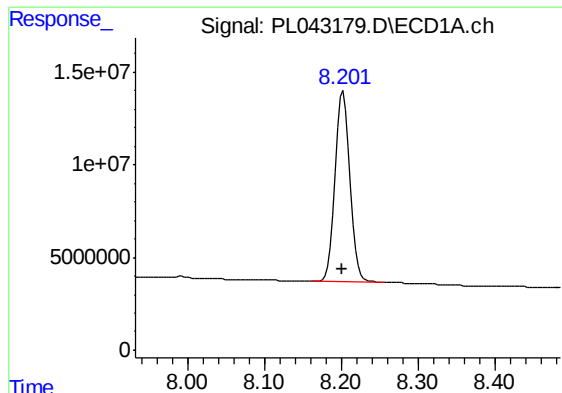

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.001 min
Response: 138569402
Conc: 21.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

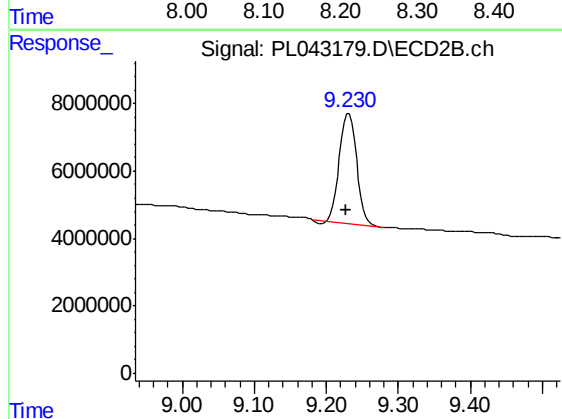

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 53845806
Conc: 20.64 ng/ml