

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 13:05
 Operator : AJ\SJ
 Sample : J6397-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EB10_12-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:57:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	114.5E6	56027328	18.668	18.903
28)	SA Decachlor...	8.202	9.231	117.3E6	47859184	17.961	18.347
Target Compounds							
2)	A alpha-BHC	3.897	0.000	4289462	0	0.454	N.D. #
6)	B beta-BHC	4.396f	0.000	2160259	0	0.586	N.D. #
7)	B delta-BHC	0.000	5.162	0	33350037	N.D.	7.760 #
8)	B Heptachlo...	0.000	5.995	0	23598421	N.D.	6.223 #
9)	A Endosulfan I	5.456f	6.371	2521991	127272	0.344	0.037 #
11)	B alpha-Chl...	5.456	6.336	2521991	739191	0.318	0.206 #
15)	B Endosulfa...	6.227f	0.000	8772686	0	1.319	N.D. #
20)	A Methoxychlor	6.962f	0.000	2089359	0	0.623	N.D. #
23)	Chlordane-1	4.357	5.162	2644990	33350037	9.843	235.968 #
26)	Chlordane-4	5.456	6.336	2521991	739191	3.336	1.295 #
27)	Chlordane-5	6.227	0.000	8772686	0	36.575	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 13:05
Operator : AJ\SJ
Sample : J6397-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
EB10_12-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:57:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

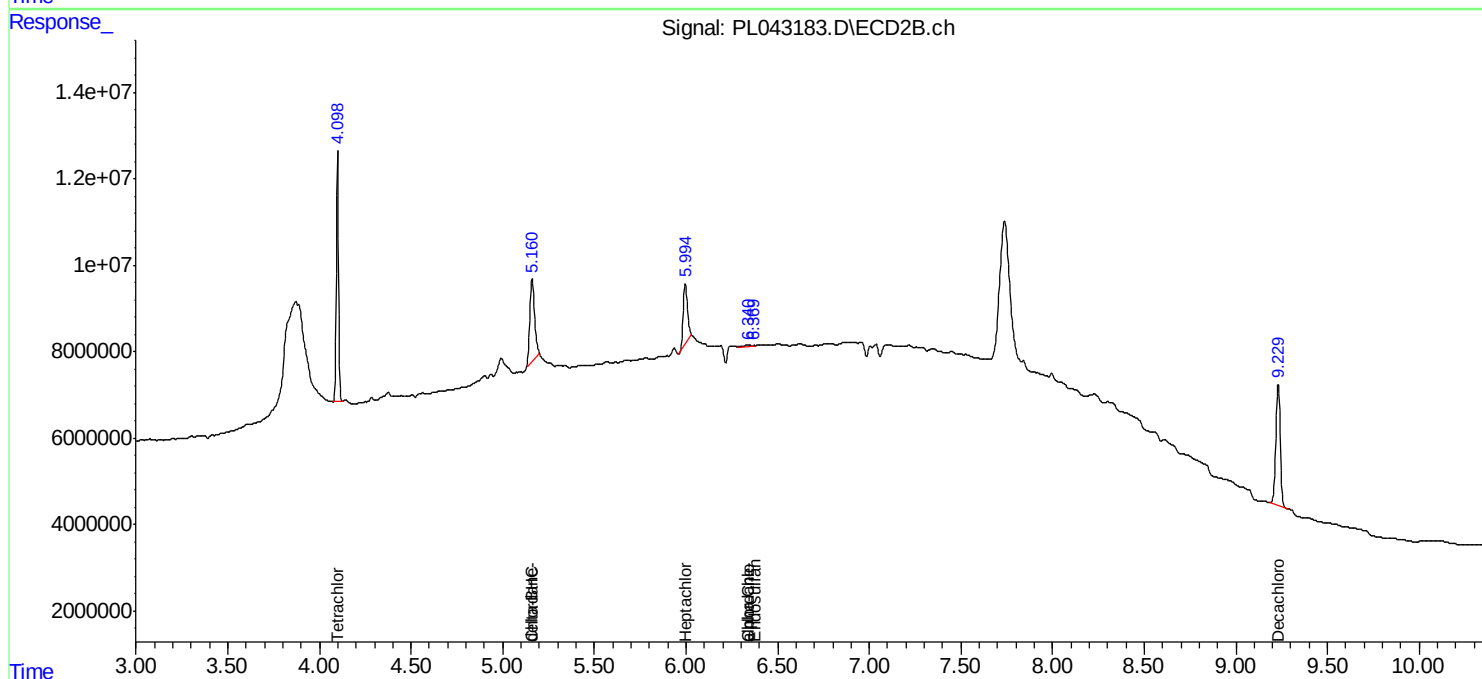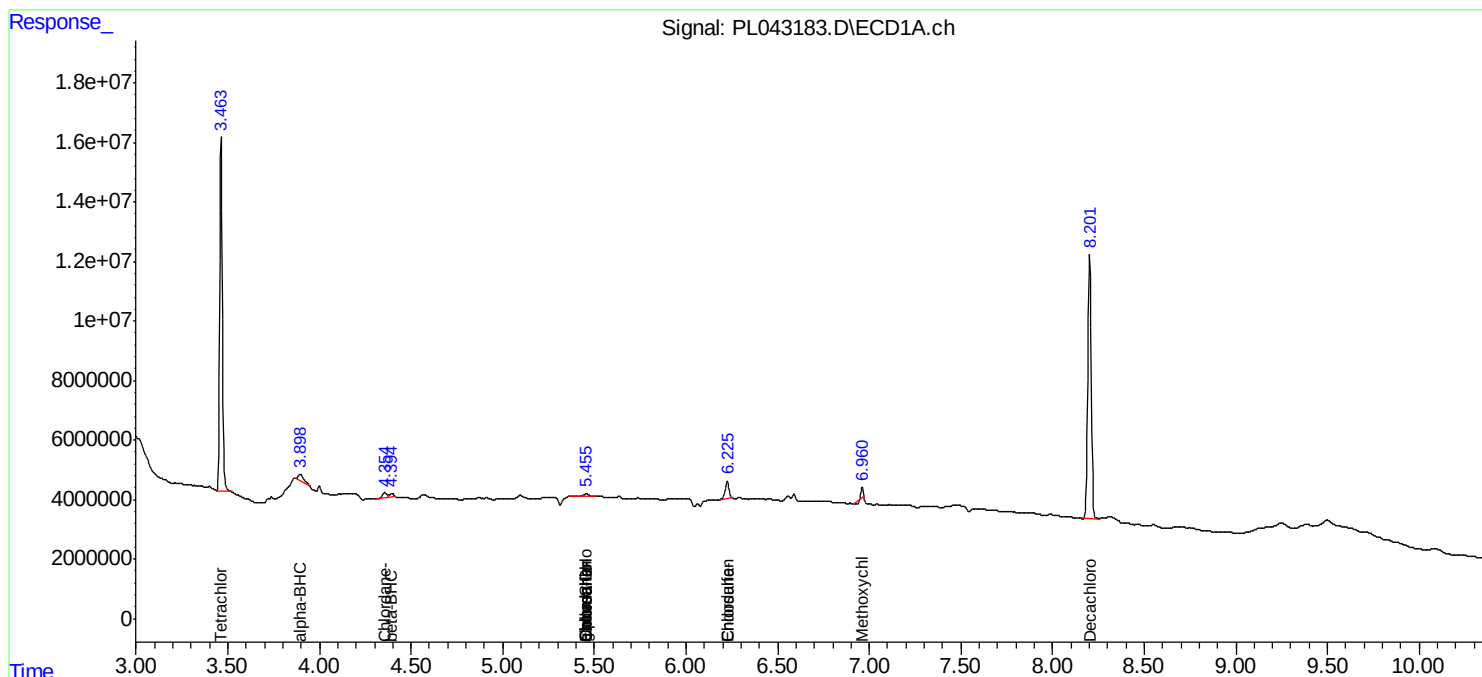


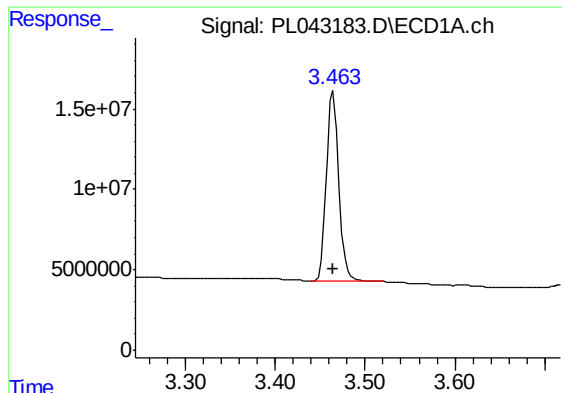

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 114487477
Conc: 18.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

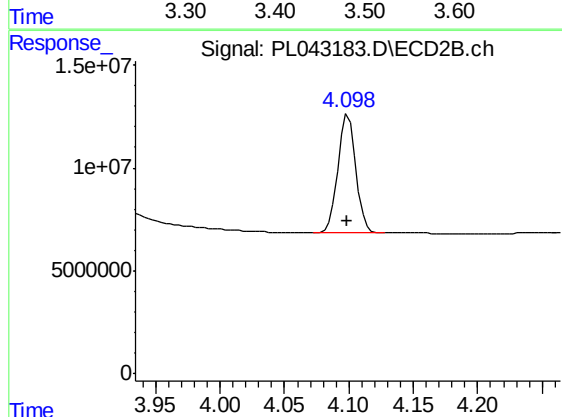


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 56027328
Conc: 18.90 ng/ml

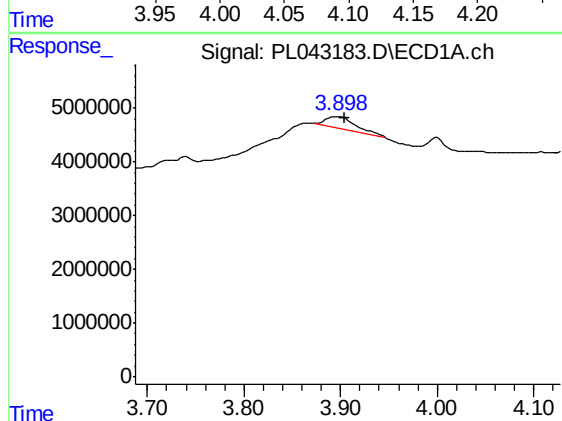


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: -0.007 min
Response: 4289462
Conc: 0.45 ng/ml

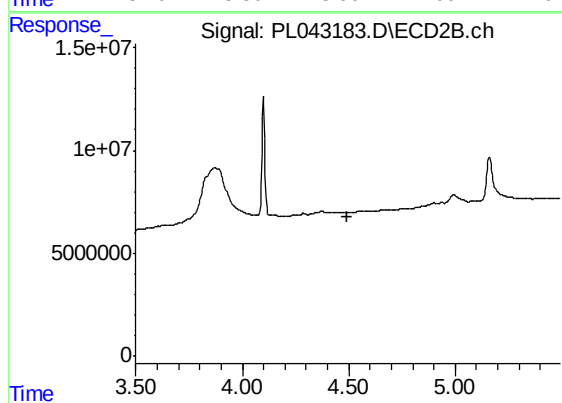

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

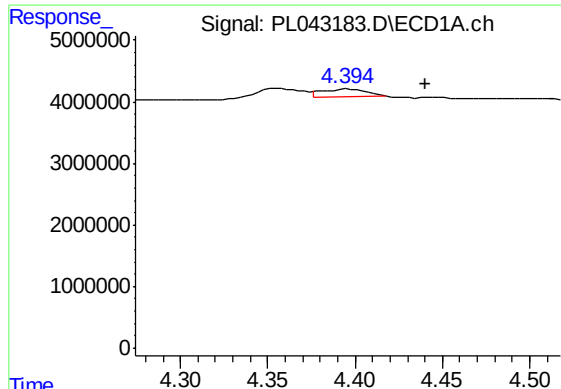

#6 beta-BHC


R.T.: 4.396 min
Delta R.T.: -0.045 min
Response: 2160259
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

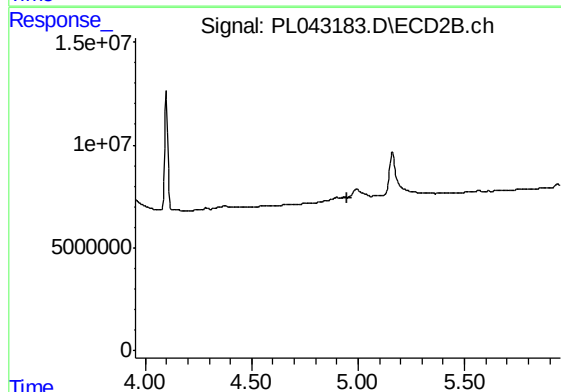


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

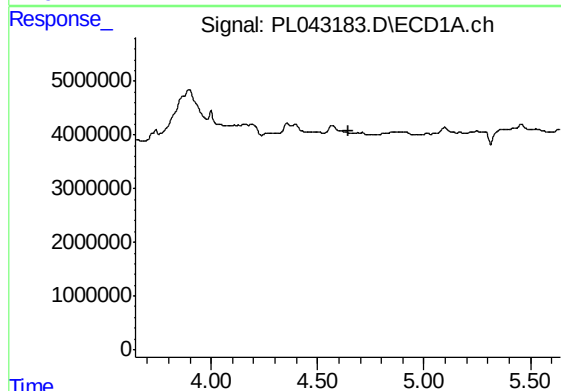


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

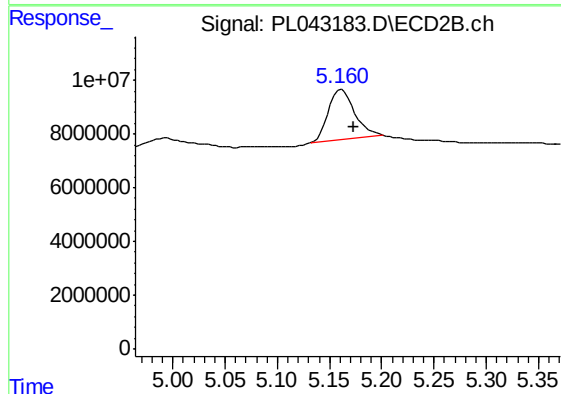

#7 delta-BHC


R.T.: 5.162 min
Delta R.T.: -0.011 min
Response: 33350037
Conc: 7.76 ng/ml

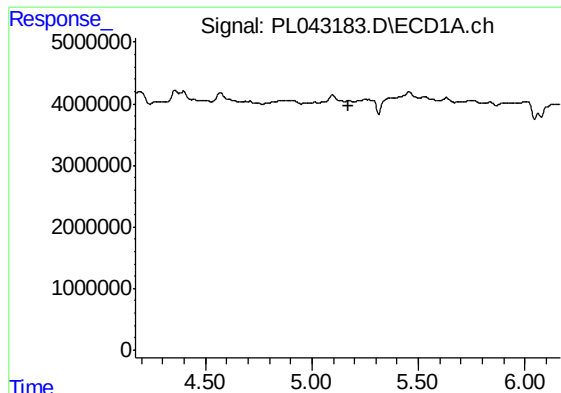

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

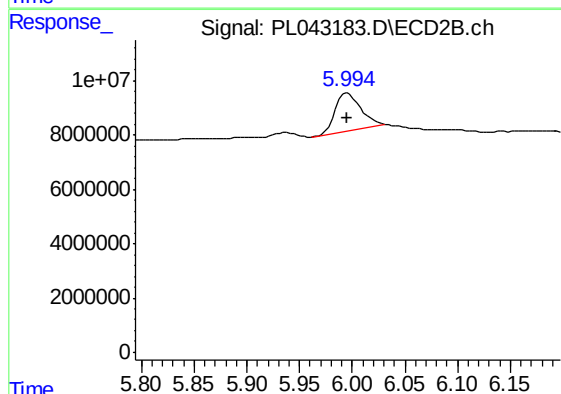


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 23598421
Conc: 6.22 ng/ml

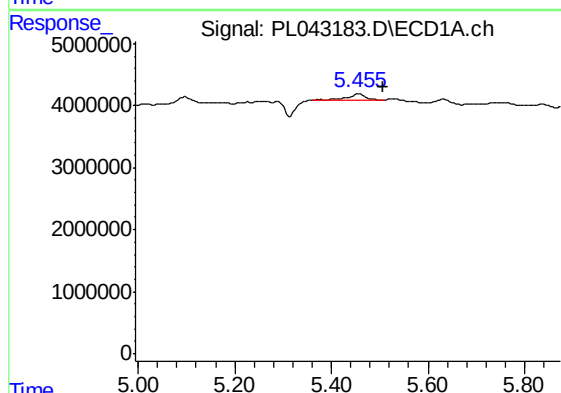


#9 Endosulfan I

R.T.: 5.456 min
Delta R.T.: -0.052 min
Response: 2521991
Conc: 0.34 ng/ml

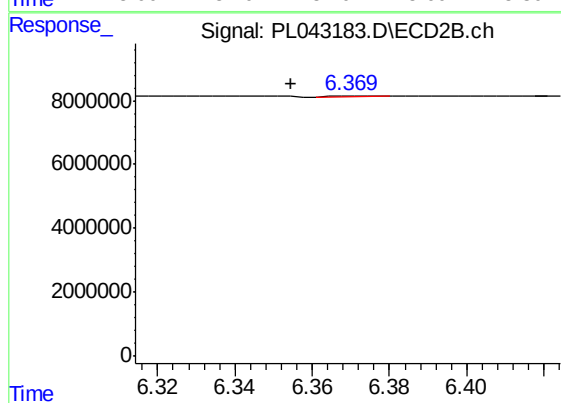

#9 Endosulfan I


R.T.: 6.371 min
Delta R.T.: 0.016 min
Response: 127272
Conc: 0.04 ng/ml

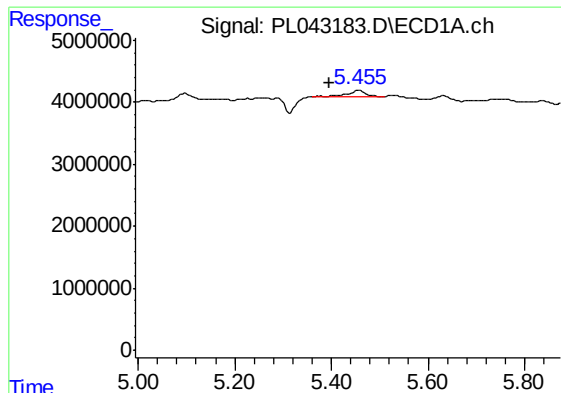

#10 gamma-Chlordane


R.T.: 5.456 min
Delta R.T.: 0.060 min
Response: 2521991
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

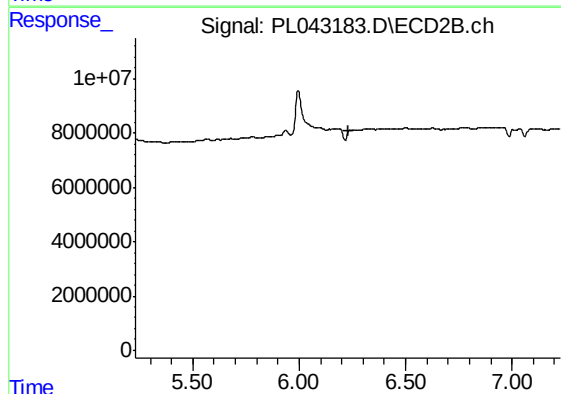


#10 gamma-Chlordane

R.T.: 6.248 min
Delta R.T.: 0.018 min
Response: -3881214
Conc: N.D.

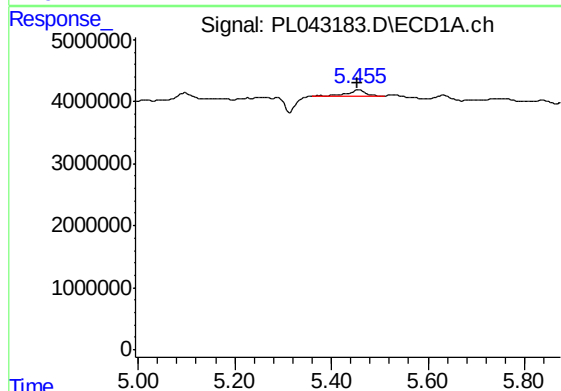


#11 alpha-Chlordane

R.T.: 5.456 min
Delta R.T.: 0.002 min
Response: 2521991
Conc: 0.32 ng/ml

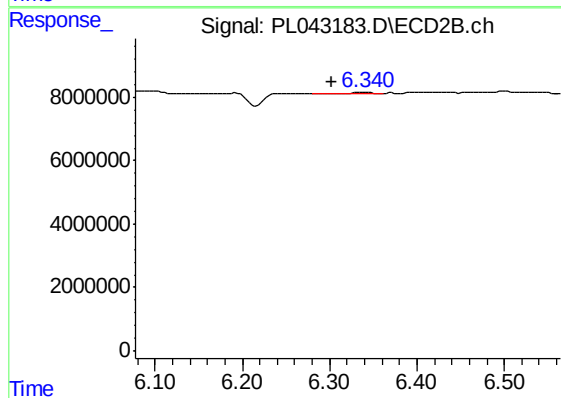

#11 alpha-Chlordane


R.T.: 6.336 min
Delta R.T.: 0.033 min
Response: 739191
Conc: 0.21 ng/ml

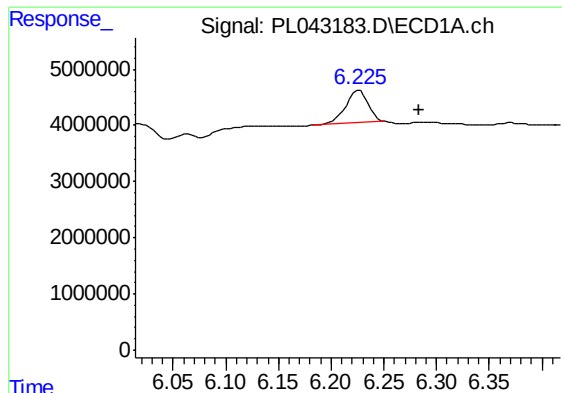

#15 Endosulfan II


R.T.: 6.227 min
Delta R.T.: -0.056 min
Response: 8772686
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

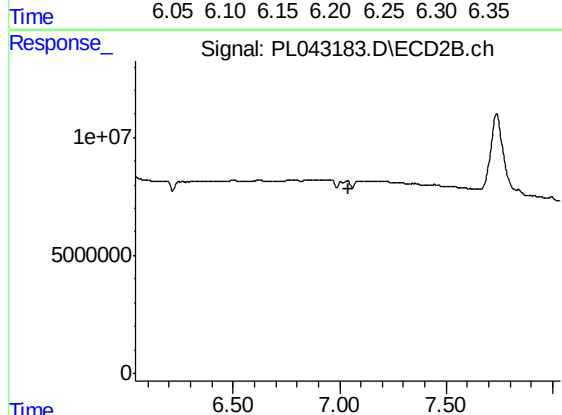


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

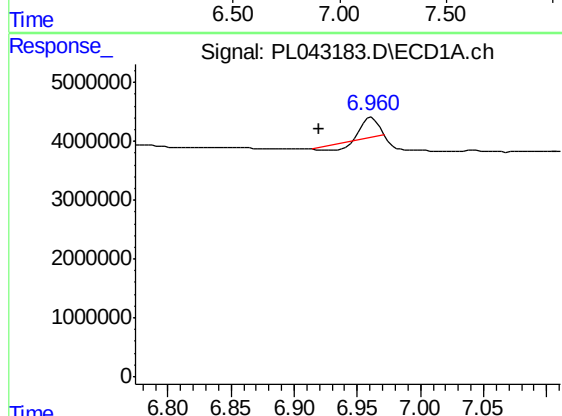


#20 Methoxychlor

R.T.: 6.962 min
Delta R.T.: 0.041 min
Response: 2089359
Conc: 0.62 ng/ml

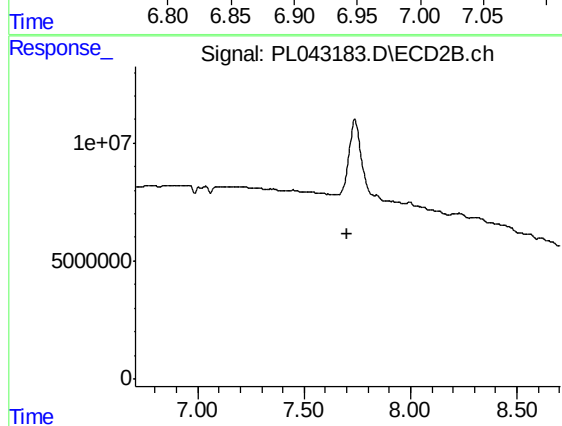

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.705 min
Response: 0
Conc: N.D.

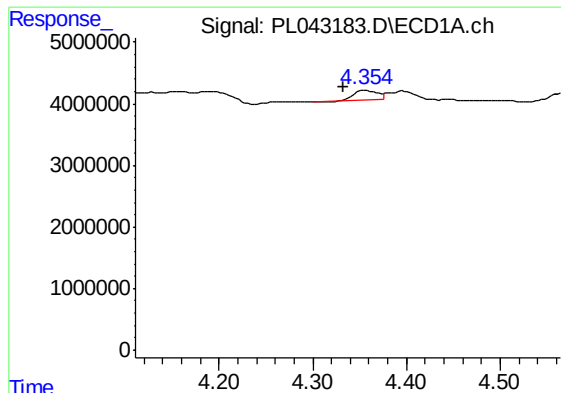

#23 Chlordane-1


R.T.: 4.357 min
Delta R.T.: 0.024 min
Response: 2644990
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

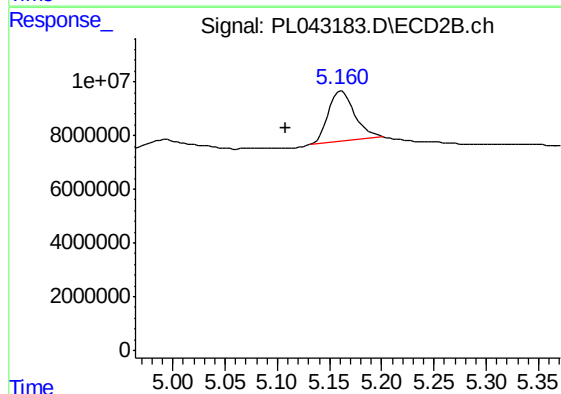


#23 Chlordane-1

R.T.: 5.162 min
Delta R.T.: 0.054 min
Response: 33350037
Conc: 235.97 ng/ml

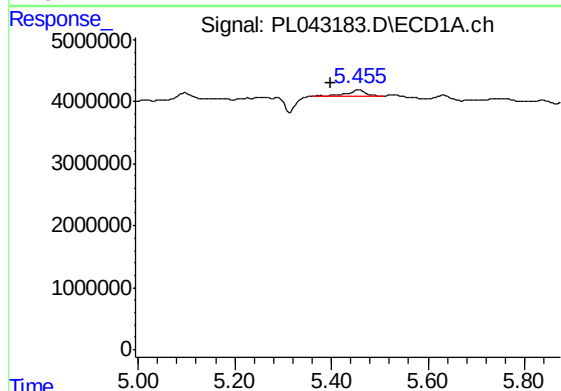


#25 Chlordane-3

R.T.: 5.456 min
Delta R.T.: 0.058 min
Response: 2521991
Conc: 3.03 ng/ml

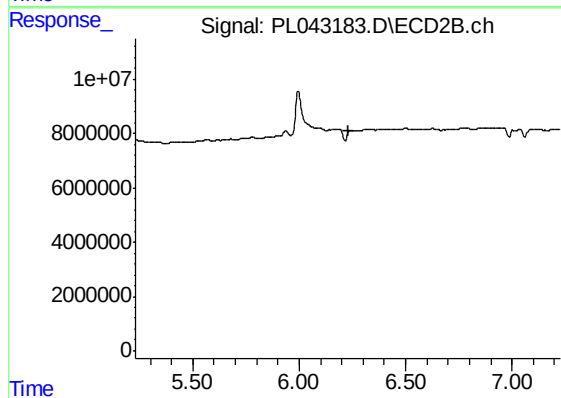

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.018 min
Response: -3881214
Conc: N.D.

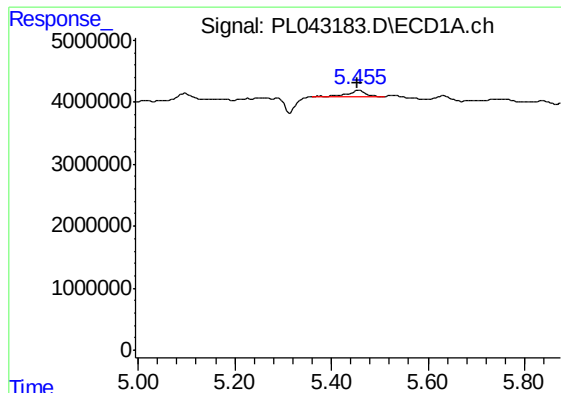

#26 Chlordane-4


R.T.: 5.456 min
Delta R.T.: 0.002 min
Response: 2521991
Conc: 3.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

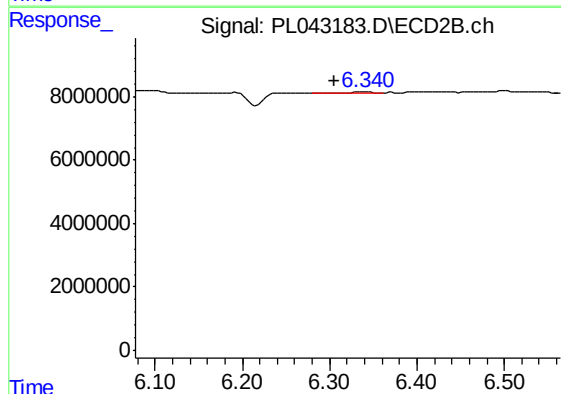


#26 Chlordane-4

R.T.: 6.336 min
Delta R.T.: 0.031 min
Response: 739191
Conc: 1.30 ng/ml

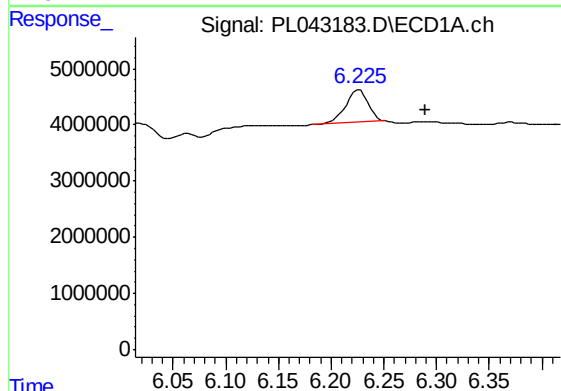


#27 Chlordane-5

R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 8772686
Conc: 36.57 ng/ml

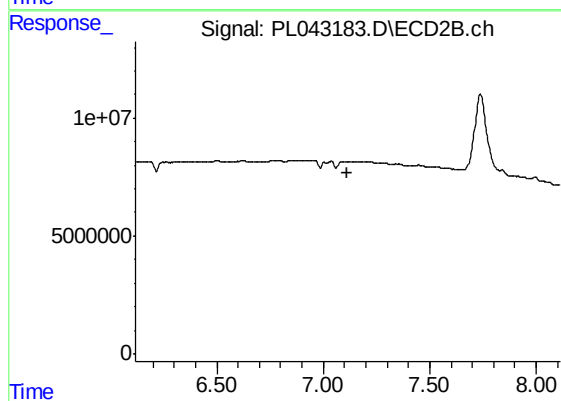

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

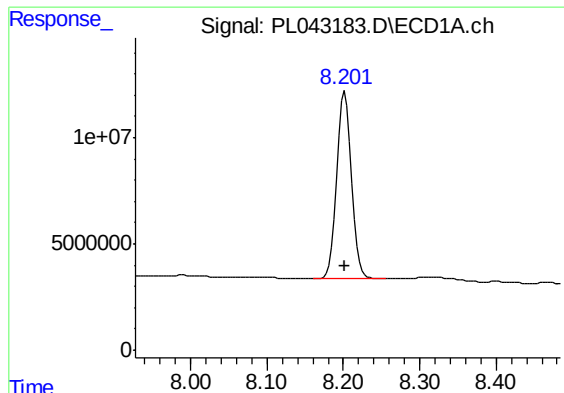

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 117287627
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB10_12-14

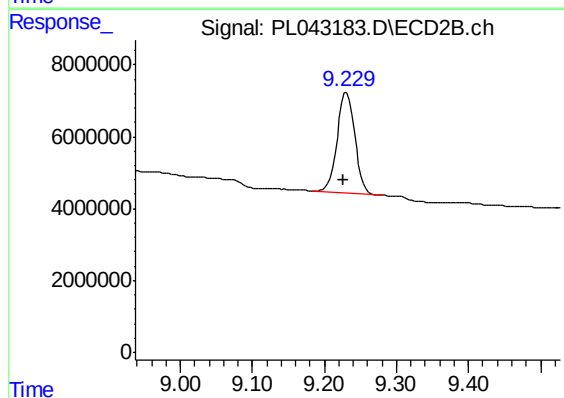

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 47859184
Conc: 18.35 ng/ml