

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 14:30
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:59:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	145.0E6	72102498	23.650	24.327
28)	SA Decachlor...	8.202	9.230	153.3E6	63204131	23.472	24.230
Target Compounds							
2)	A alpha-BHC	3.897	0.000	4156364	0	0.440	N.D. #
6)	B beta-BHC	4.393f	0.000	2123791	0	0.576	N.D. #
7)	B delta-BHC	0.000	5.163	0	20666165	N.D.	4.809 #
8)	B Heptachlo...	0.000	6.000	0	10048592	N.D.	2.650 #
15)	B Endosulfa...	6.228f	7.001f	5694244	457576	0.856	0.151 #
16)	A 4,4'-DDD	0.000	7.001f	0	457576	N.D.	0.156 #
23)	Chlordane-1	4.362	5.163	1549326	20666165	5.766	146.223 #
27)	Chlordane-5	6.228	0.000	5694244	0	23.740	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 14:30
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:59:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

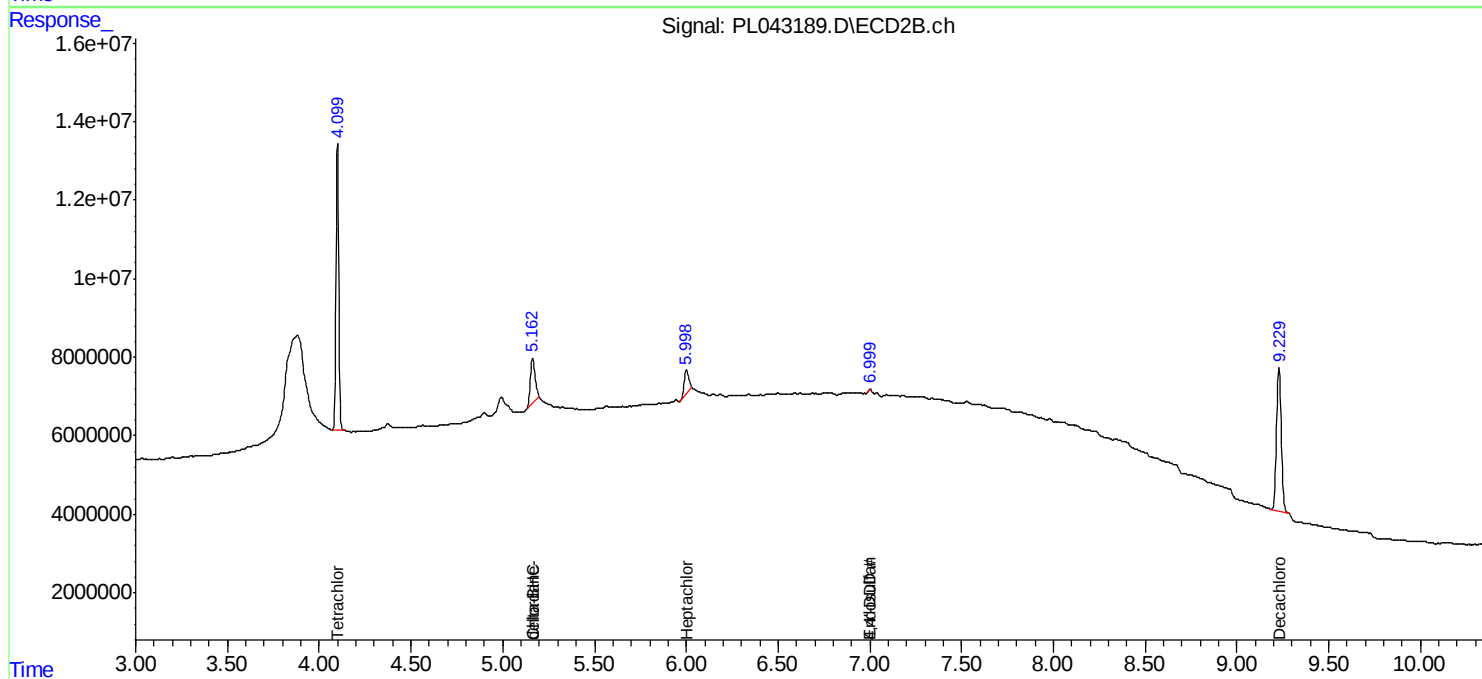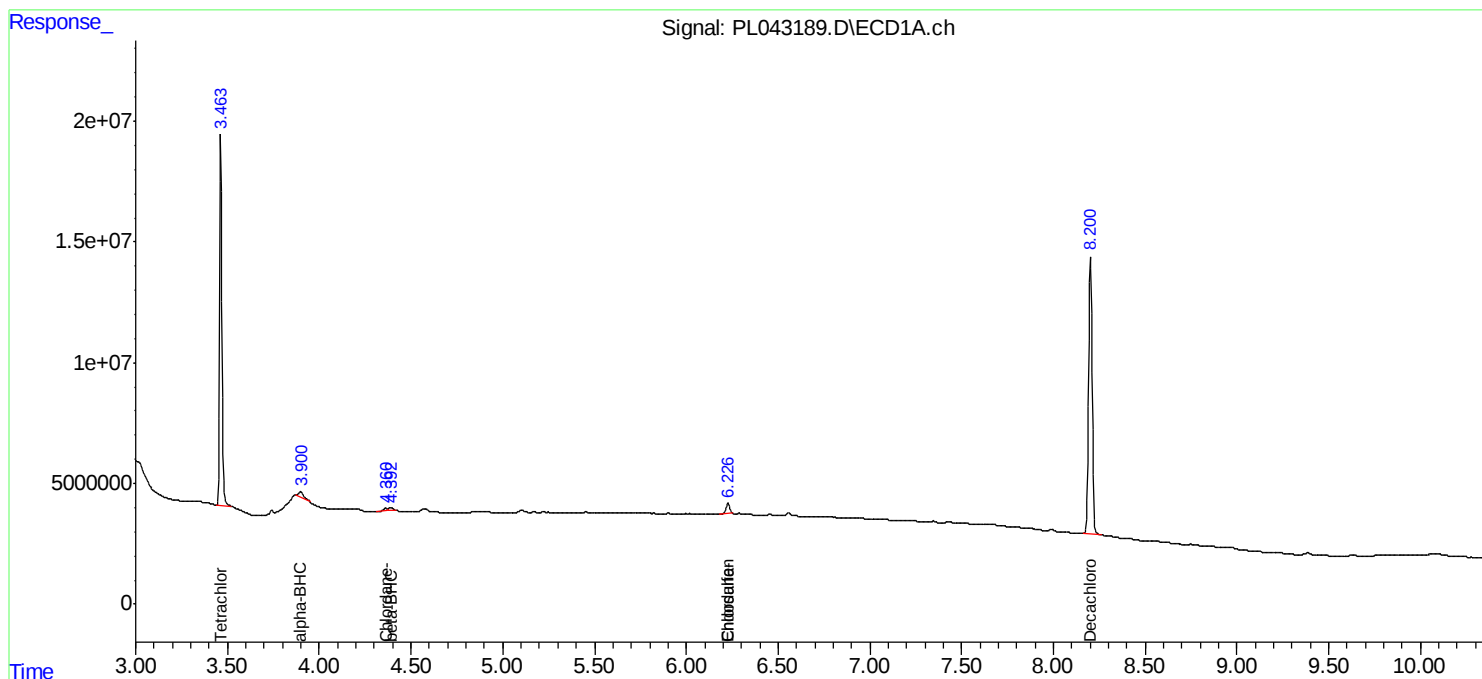


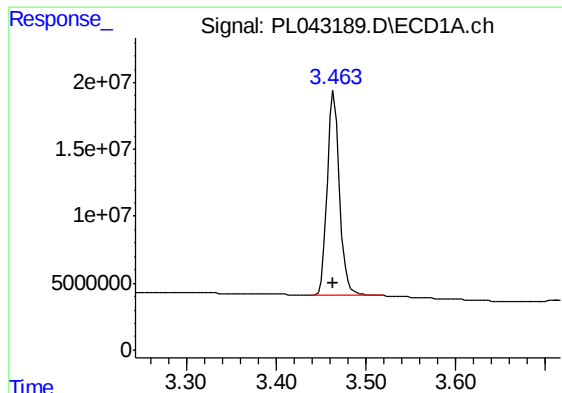

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 145041478
Conc: 23.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

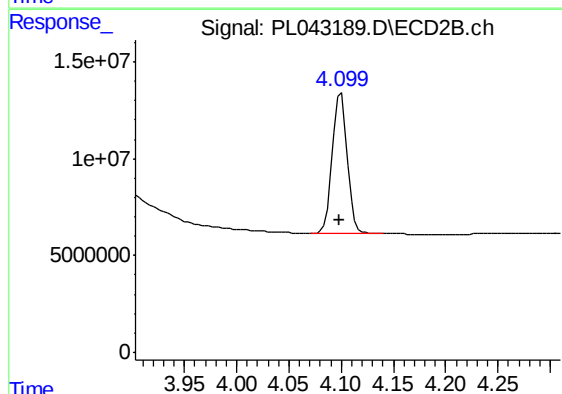


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 72102498
Conc: 24.33 ng/ml

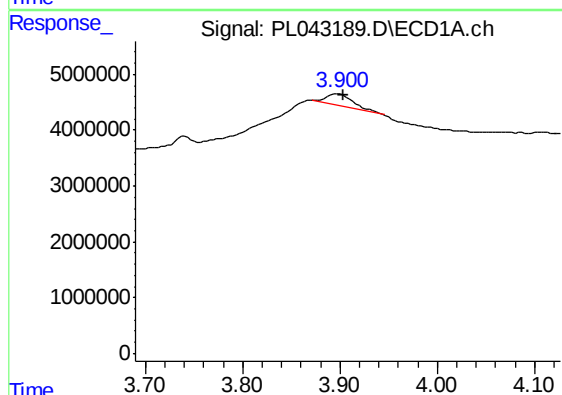


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: -0.007 min
Response: 4156364
Conc: 0.44 ng/ml

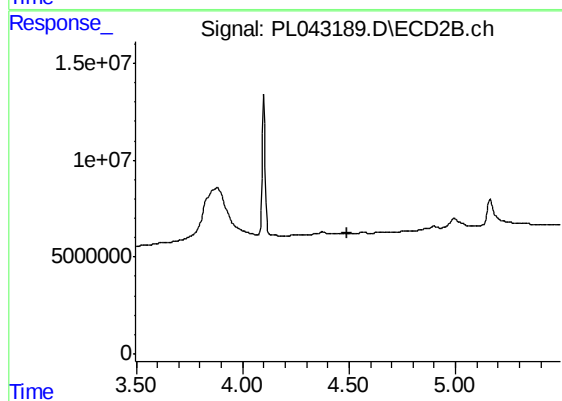

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

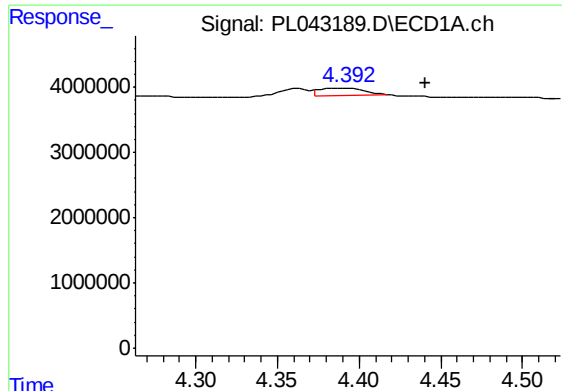

#6 beta-BHC


R.T.: 4.393 min
Delta R.T.: -0.047 min
Response: 2123791
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

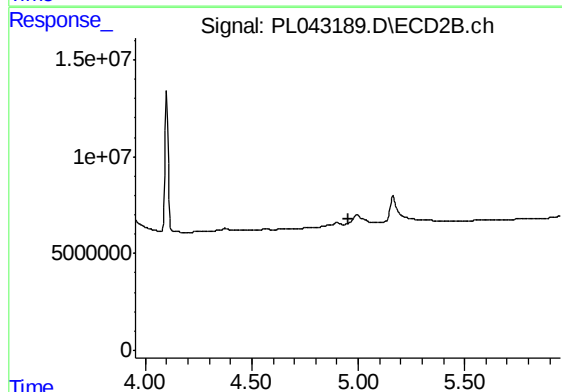


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

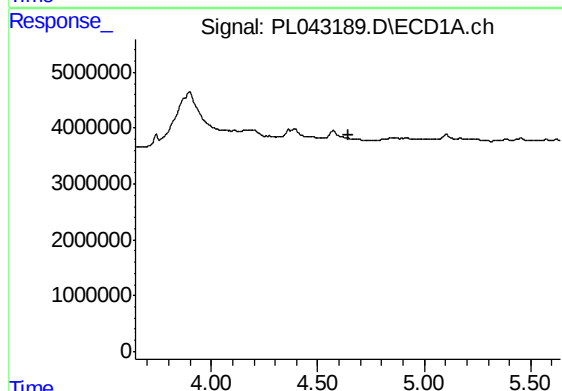


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

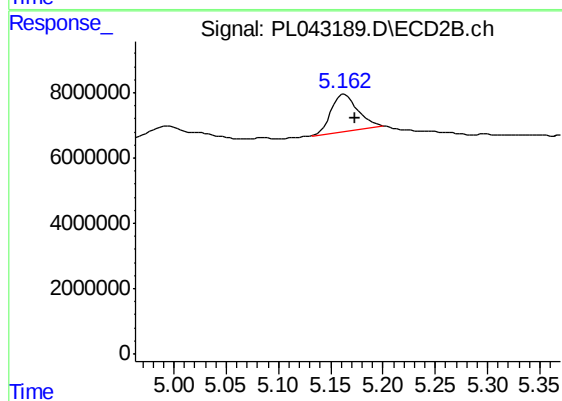

#7 delta-BHC


R.T.: 5.163 min
Delta R.T.: -0.010 min
Response: 20666165
Conc: 4.81 ng/ml

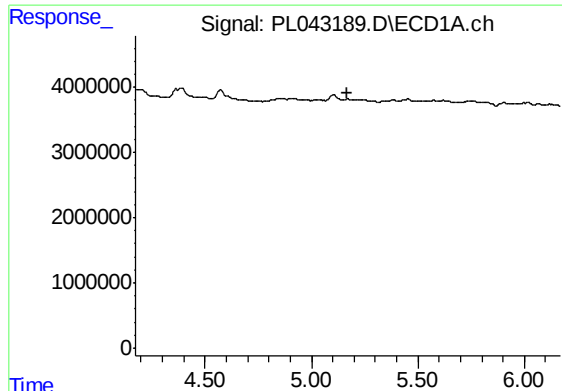

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

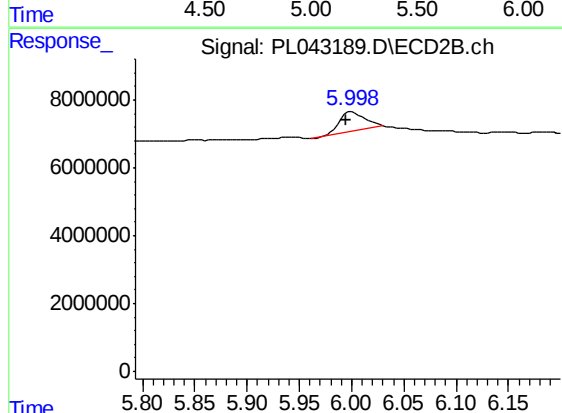


#8 Heptachlor epoxide

R.T.: 6.000 min
Delta R.T.: 0.005 min
Response: 10048592
Conc: 2.65 ng/ml

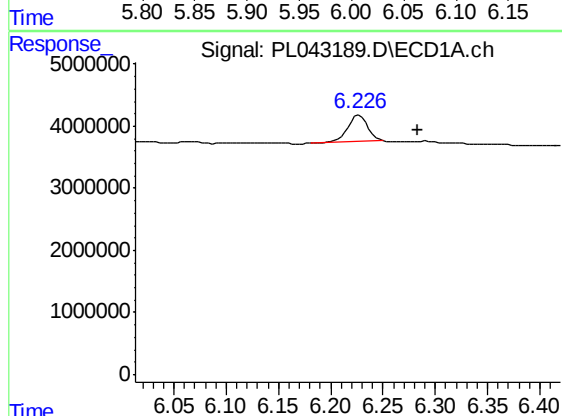


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.055 min
Response: 5694244
Conc: 0.86 ng/ml

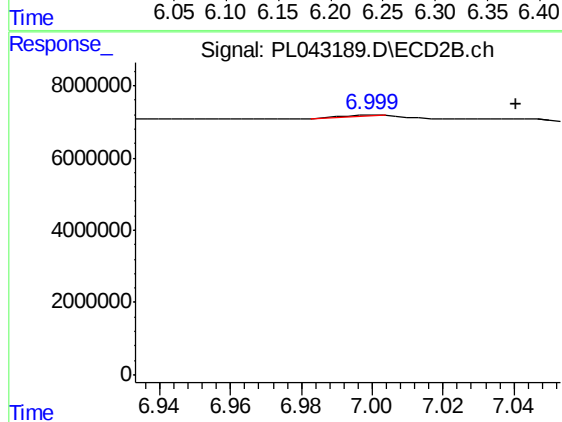

#15 Endosulfan II


R.T.: 7.001 min
Delta R.T.: -0.040 min
Response: 457576
Conc: 0.15 ng/ml

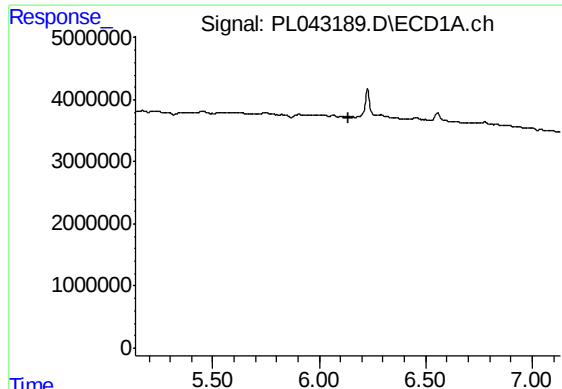

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

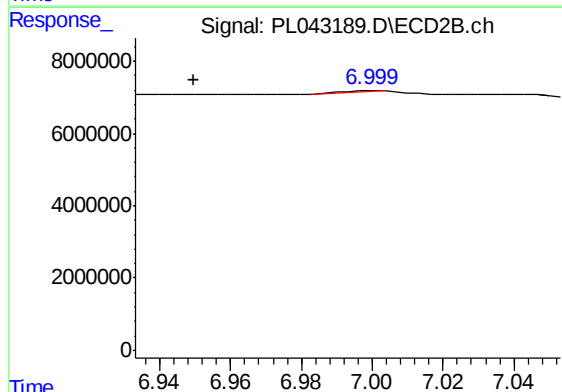


#16 4,4'-DDD

R.T.: 7.001 min
Delta R.T.: 0.051 min
Response: 457576
Conc: 0.16 ng/ml

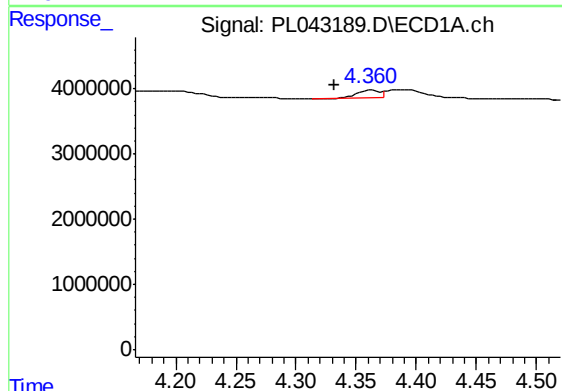


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 1549326
Conc: 5.77 ng/ml

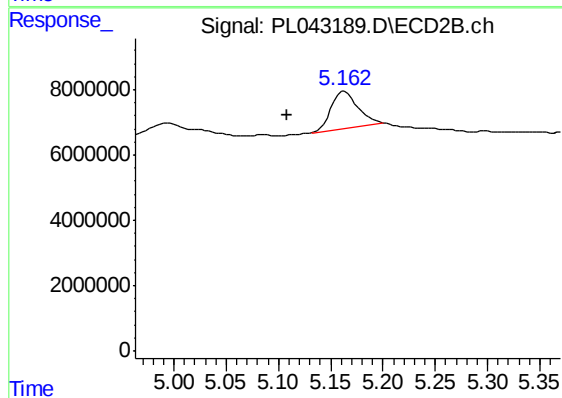

#23 Chlordane-1


R.T.: 5.163 min
Delta R.T.: 0.055 min
Response: 20666165
Conc: 146.22 ng/ml

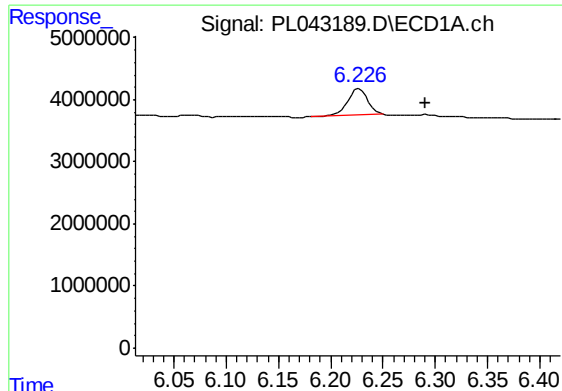

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 5694244
Conc: 23.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

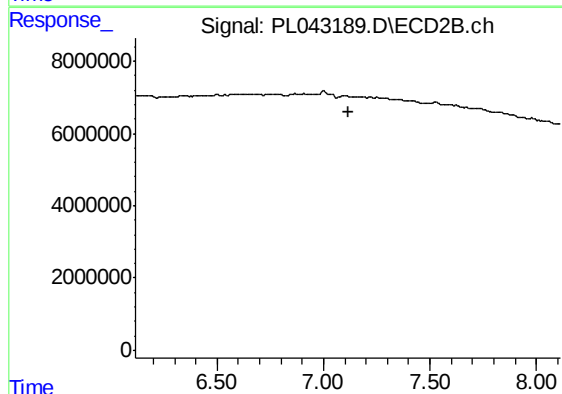


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

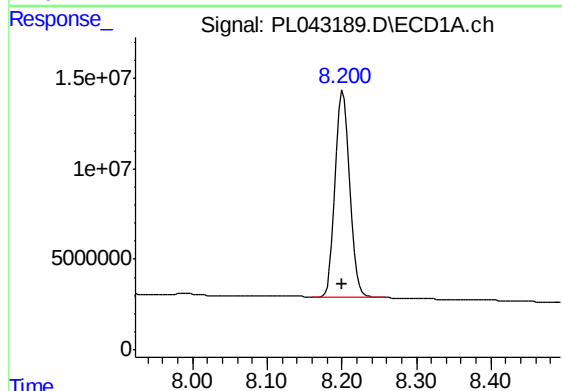

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 153272869
Conc: 23.47 ng/ml

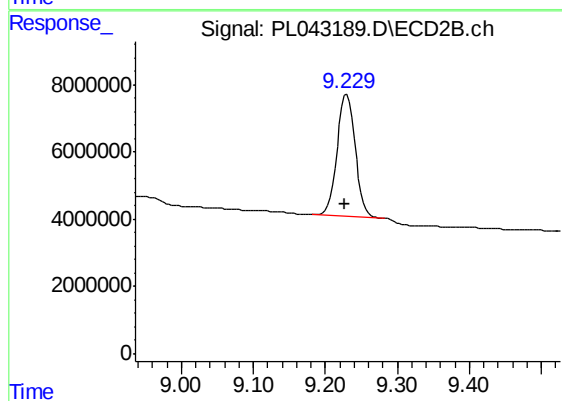

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.003 min
Response: 63204131
Conc: 24.23 ng/ml